

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP062573.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 00:54
 Operator : UA/AJ
 Sample : PB110339BS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110339BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 08:18:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 08:00:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.063	4.164	1798085	404102	19.747	1.780 #
2)	SA Decachlor...	8.315	9.058	16567293	3430572	110.870	21.552 #
Target Compounds							
3)	L1 Aroclor-1...	4.570	4.554	790835	950531	348.511	242.753 #
4)	L1 Aroclor-1...	4.995	4.997	674709	708466	257.467	244.162
5)	L1 Aroclor-1...	5.041	5.271	560677	1305251	312.067	222.801 #
6)	L1 Aroclor-1...	5.365	5.350	8467379	937157	7013.377	248.183 #
7)	L1 Aroclor-1...	5.365	5.616	8467379	1114713	5645.279	279.109 #
8)	L2 Aroclor-1...	0.000	4.314	0	1849228	N.D.	580.230 #
9)	L2 Aroclor-1...	4.321	4.405	1348975	360785	1114.892	179.004 #
10)	L2 Aroclor-1...	4.321	4.468	1348975	467367	286.852	64.720 #
11)	L3 Aroclor-1...	4.570	4.927	790835	782117	615.551	477.507
12)	L3 Aroclor-1...	4.995	5.171	674709	3004891	460.197	956.060 #
13)	L3 Aroclor-1...	5.041	5.271	560677	1305251	545.289	631.920
14)	L3 Aroclor-1...	5.365	5.474	8467379	701120	13273.816	333.078 #
15)	L3 Aroclor-1...	5.365	5.850	8467379	266240	9870.437	109.699 #
16)	L4 Aroclor-1...	4.570	4.782	790835	502954	385.294	82.414 #
17)	L4 Aroclor-1...	4.901	5.108	1456656	251706	316.849	33.241 #
18)	L4 Aroclor-1...	4.995	5.271	674709	1305251	314.543	433.534 #
19)	L4 Aroclor-1...	5.287	5.474	875839	701120	429.023	210.510 #
20)	L4 Aroclor-1...	5.610	5.616	626042	1114713	352.295	231.444 #
21)	L5 Aroclor-1...	5.287	5.474	875839	701120	256.930	113.991 #
22)	L5 Aroclor-1...	5.365	5.616	8467379	1114713	4397.504	153.158 #
23)	L5 Aroclor-1...	5.610	5.850	626042	266240	206.844	37.861 #
24)	L5 Aroclor-1...	5.610	5.850	626042	266240	202.953	33.616 #
25)	L5 Aroclor-1...	5.752	6.015	848085	183919	287.637	24.886 #
26)	L6 Aroclor-1...	5.752	5.850	848085	266240	183.885	36.545 #
27)	L6 Aroclor-1...	5.962	6.015	457033	183919	136.930	23.727 #
28)	L6 Aroclor-1...	6.056	6.340	525377	385321	86.587	29.699 #
29)	L6 Aroclor-1...	6.268	6.644	457815	215091	77.980	41.764 #
30)	L6 Aroclor-1...	6.629	6.993	2665999	1195294	350.819	110.732 #
31)	L7 Aroclor-1...	6.194	6.587	2077463	1997326	575.260	250.062 #
32)	L7 Aroclor-1...	6.629	6.739	2665999	2206967	287.458	243.371
33)	L7 Aroclor-1...	6.717	7.110	2074012	1260369	312.670	198.679 #
34)	L7 Aroclor-1...	6.916	7.361	1361652	2155460	260.724	293.935
35)	L7 Aroclor-1...	7.162	7.554	4851474	4045990	256.119	252.202
36)	L8 Aroclor-1...	6.194	6.644	2077463	215091	623.526	26.389 #
37)	L8 Aroclor-1...	6.405	6.847	2273389	8732123	338.896	1854.842 #
38)	L8 Aroclor-1...	6.717	7.023	2074012	1108426	179.253	100.542 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026573.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 00:54
 Operator : UA/AJ
 Sample : PB110339BS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110339BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 08:18:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 08:00:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39)	L8 Aroclor-1...	6.916	7.261	1361652	1023385	168.403	102.403 #
40)	L8 Aroclor-1...	7.162	7.471	4851474	1261272	183.444	59.863 #
41)	L9 Aroclor-1...	7.402	0.000	516.2E6	0	19018.650	N.D. #
42)	L9 Aroclor-1...	7.402	7.853	516.2E6	469.5E6	24986.608	24997.855
43)	L9 Aroclor-1...	7.632	0.000	723819	0	39.273	N.D. #
44)	L9 Aroclor-1...	7.931	8.246	4510187	706459	547.896	95.281 #
45)	L9 Aroclor-1...	8.154	0.000	478937	0	7.991	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026573.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 00:54
Operator : UA/AJ
Sample : PB110339BS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB110339BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 08:18:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 08:00:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

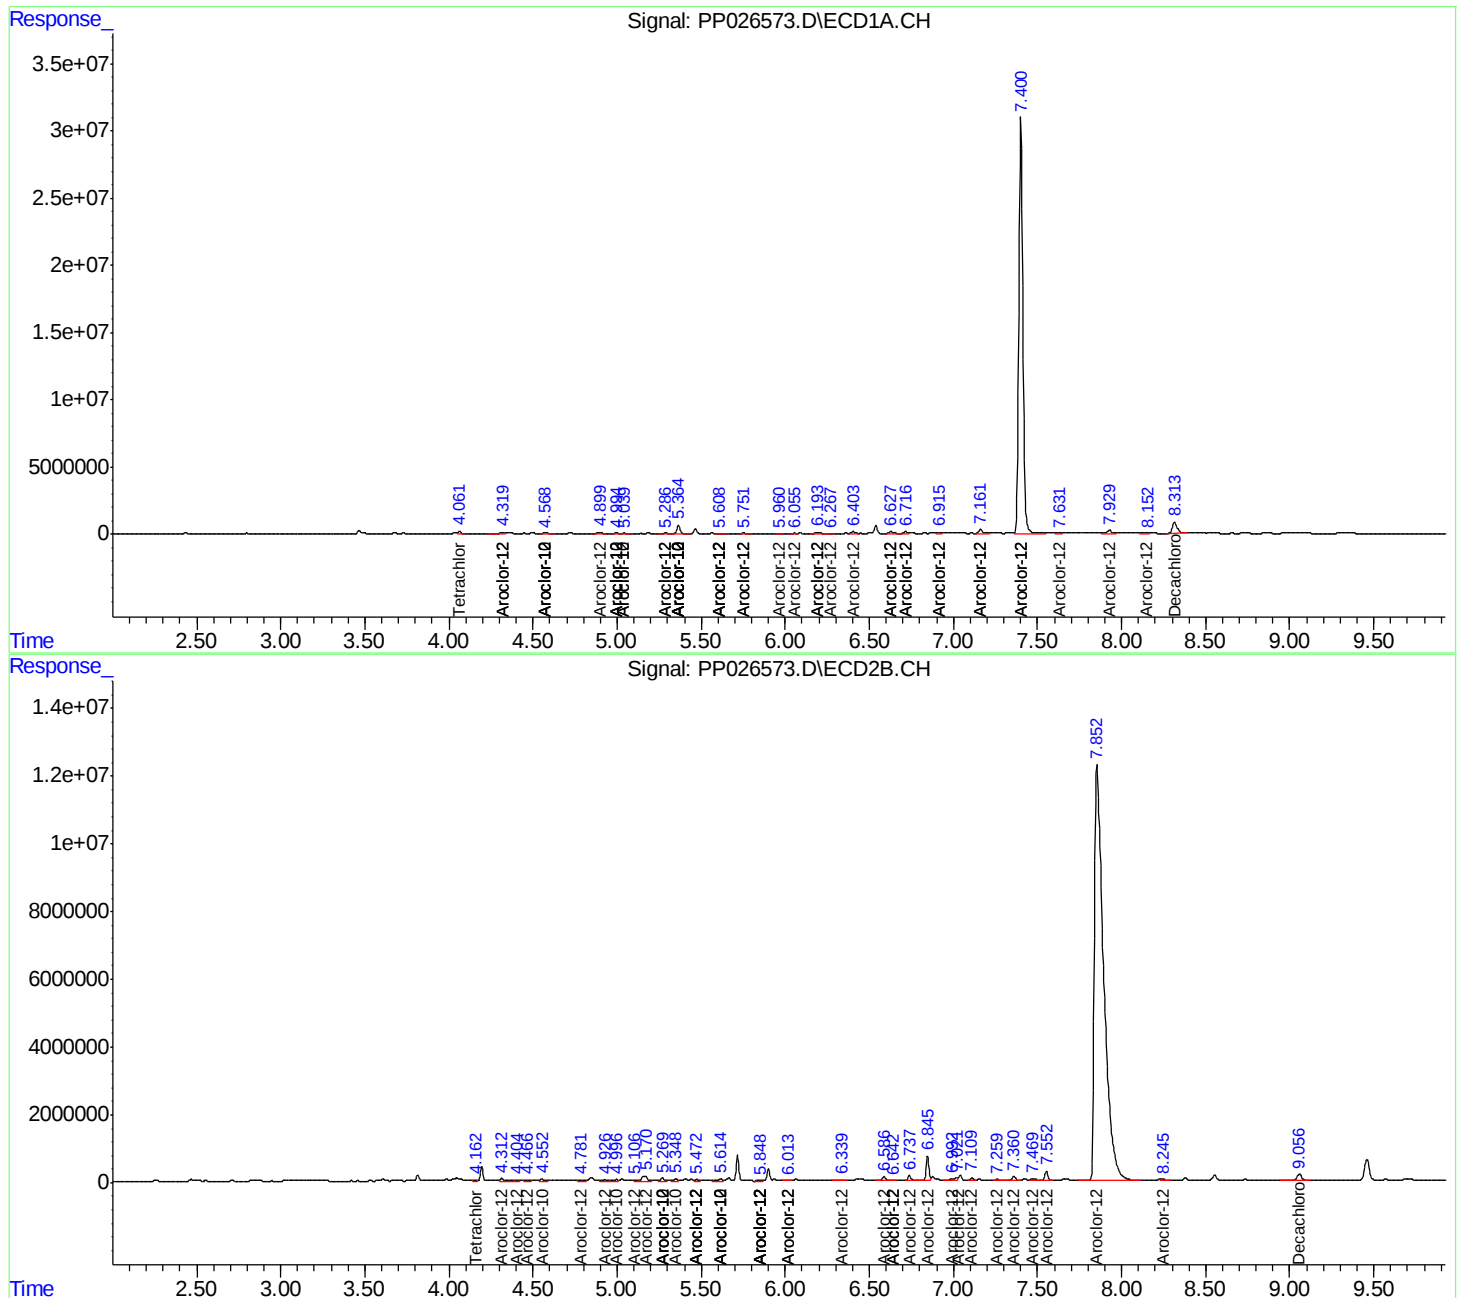


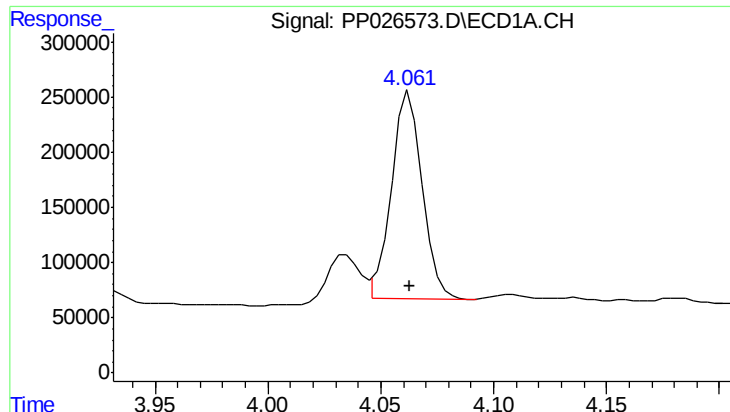

#1 Tetrachloro-m-xylene


R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1798085
Conc: 19.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

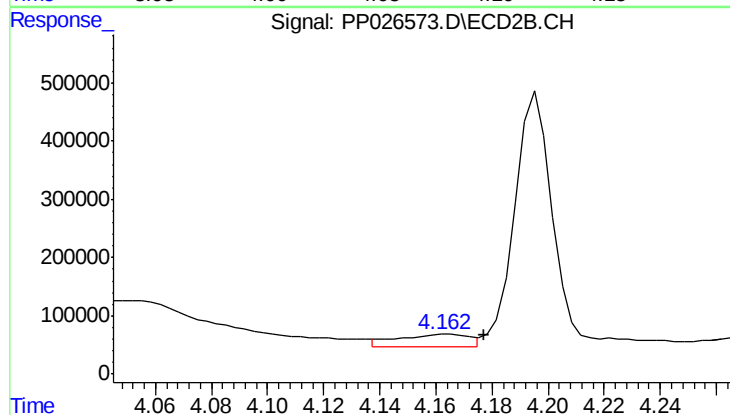


#1 Tetrachloro-m-xylene

R.T.: 4.164 min
Delta R.T.: -0.013 min
Response: 404102
Conc: 1.78 ng/ml

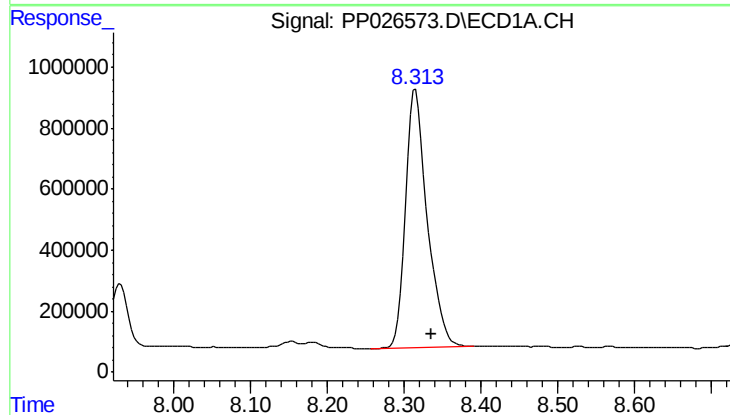


#2 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.020 min
Response: 16567293
Conc: 110.87 ng/ml

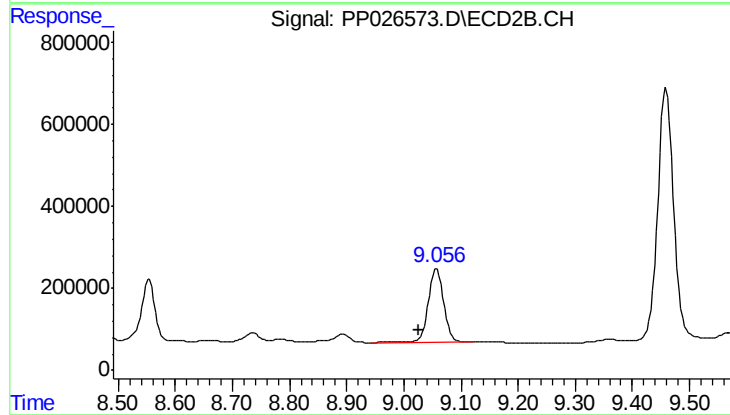

#2 Decachlorobiphenyl


R.T.: 9.058 min
Delta R.T.: 0.033 min
Response: 3430572
Conc: 21.55 ng/ml

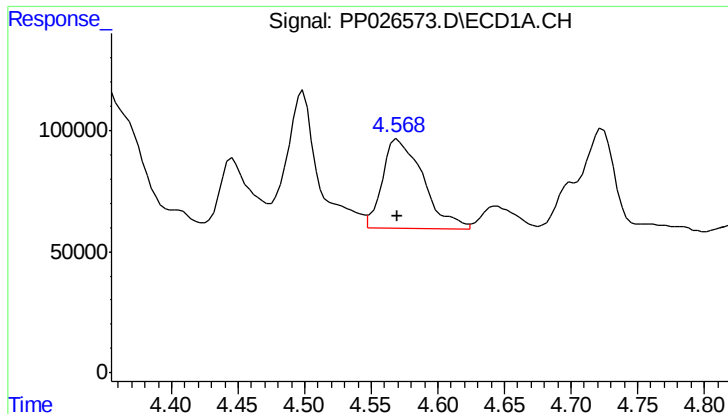

#3 Aroclor-1016-1


R.T.: 4.570 min
Delta R.T.: 0.000 min
Response: 790835
Conc: 348.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

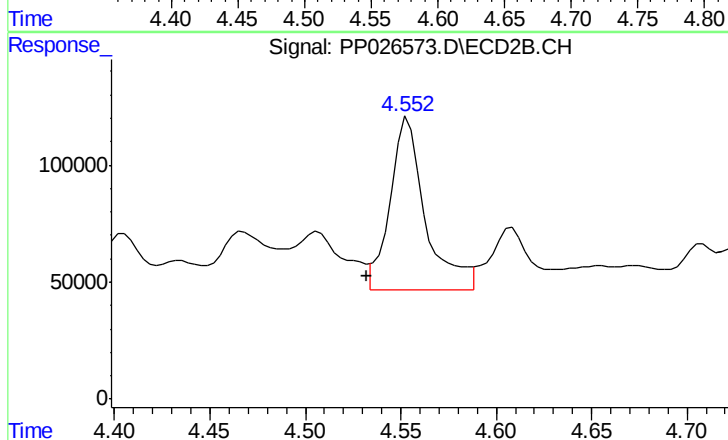


#3 Aroclor-1016-1

R.T.: 4.554 min
Delta R.T.: 0.021 min
Response: 950531
Conc: 242.75 ng/ml

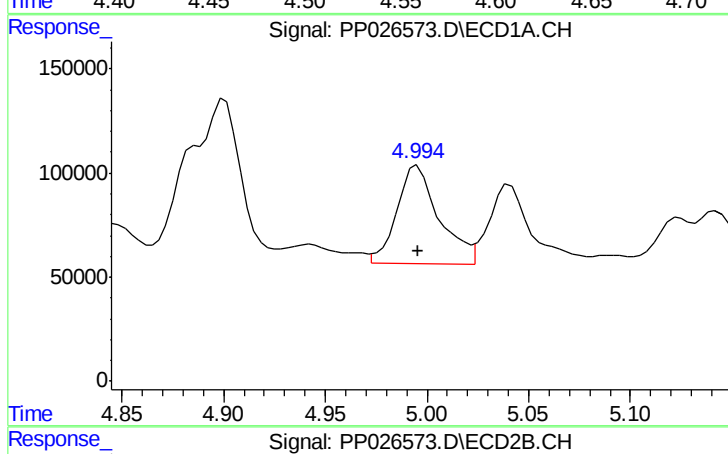


#4 Aroclor-1016-2

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 674709
Conc: 257.47 ng/ml

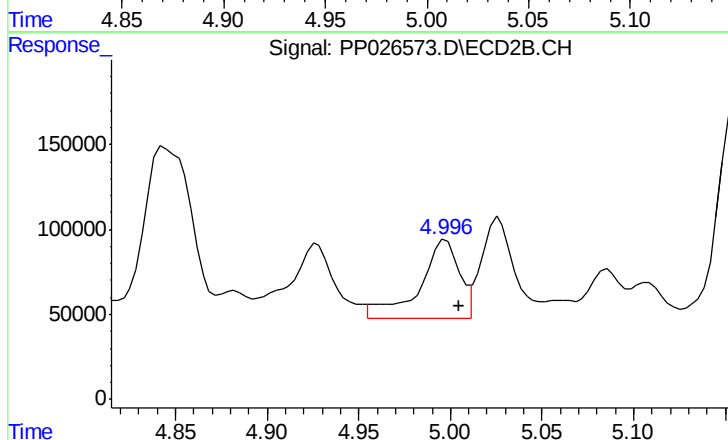

#4 Aroclor-1016-2


R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 708466
Conc: 244.16 ng/ml

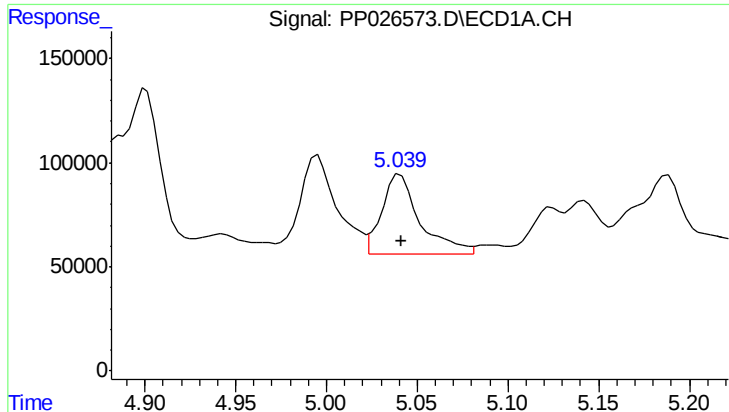

#5 Aroclor-1016-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 560677
Conc: 312.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

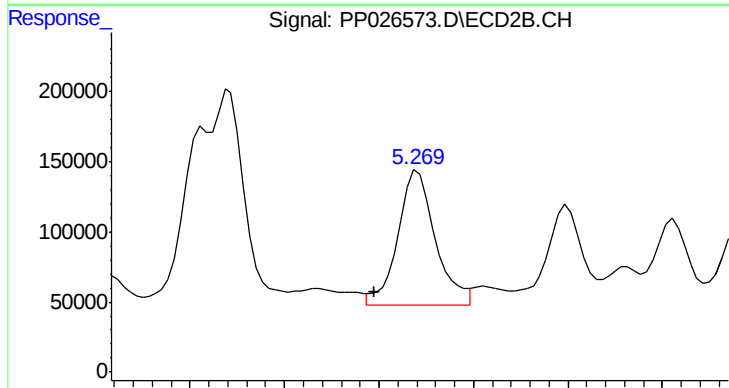


#5 Aroclor-1016-3

R.T.: 5.271 min
Delta R.T.: 0.023 min
Response: 1305251
Conc: 222.80 ng/ml

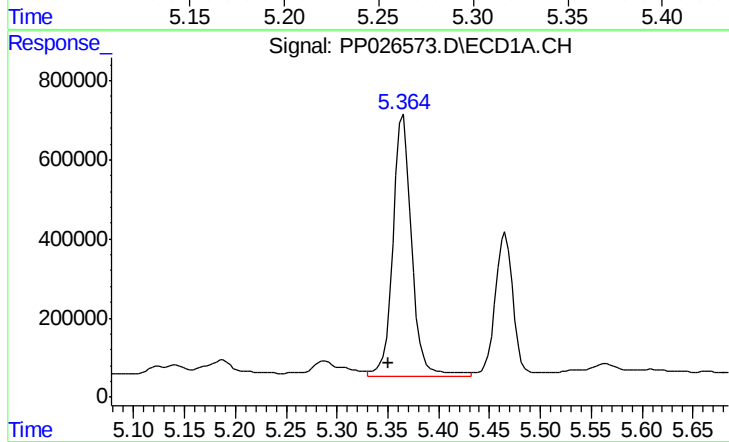


#6 Aroclor-1016-4

R.T.: 5.365 min
Delta R.T.: 0.015 min
Response: 8467379
Conc: 7013.38 ng/ml

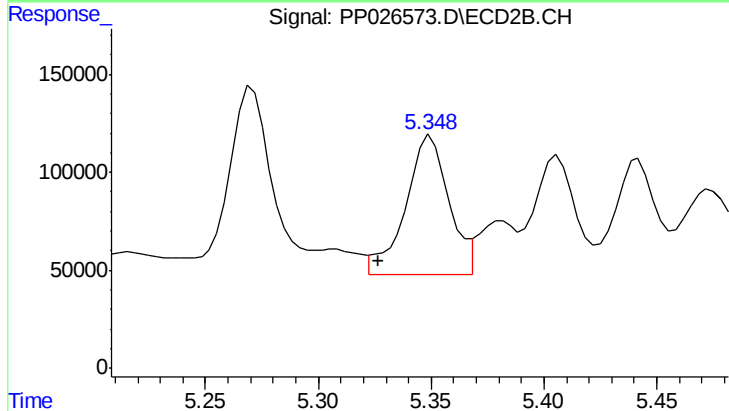

#6 Aroclor-1016-4


R.T.: 5.350 min
Delta R.T.: 0.023 min
Response: 937157
Conc: 248.18 ng/ml

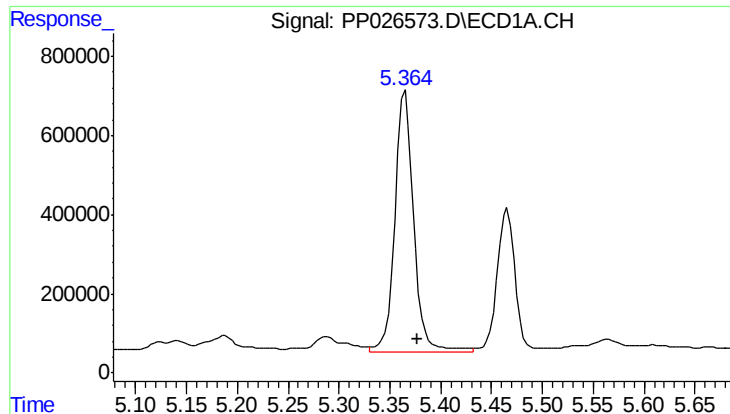

#7 Aroclor-1016-5


R.T.: 5.365 min
Delta R.T.: -0.012 min
Response: 8467379
Conc: 5645.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

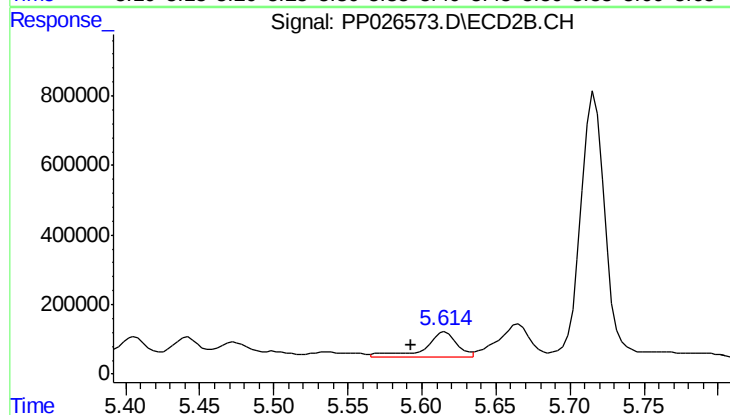


#7 Aroclor-1016-5

R.T.: 5.616 min
Delta R.T.: 0.023 min
Response: 1114713
Conc: 279.11 ng/ml

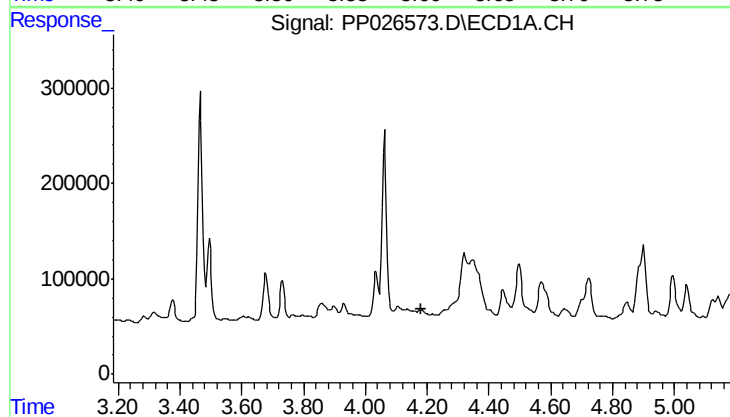


#8 Aroclor-1221-1

R.T.: 0.000 min
Exp R.T.: 4.182 min
Response: 0
Conc: N.D.

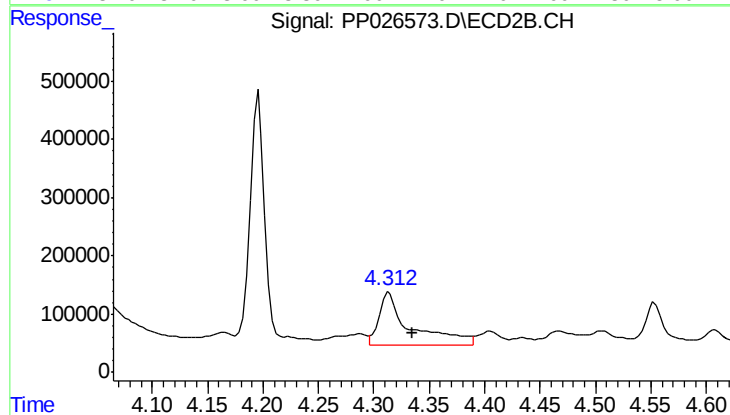

#8 Aroclor-1221-1


R.T.: 4.314 min
Delta R.T.: -0.021 min
Response: 1849228
Conc: 580.23 ng/ml

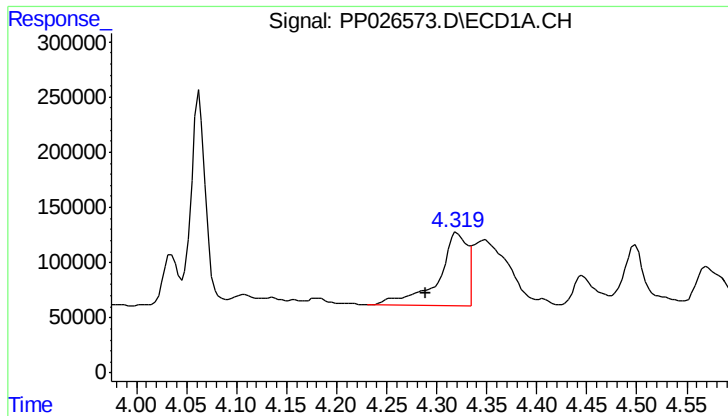

#9 Aroclor-1221-2


R.T.: 4.321 min
Delta R.T.: 0.032 min
Response: 1348975
Conc: 1114.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

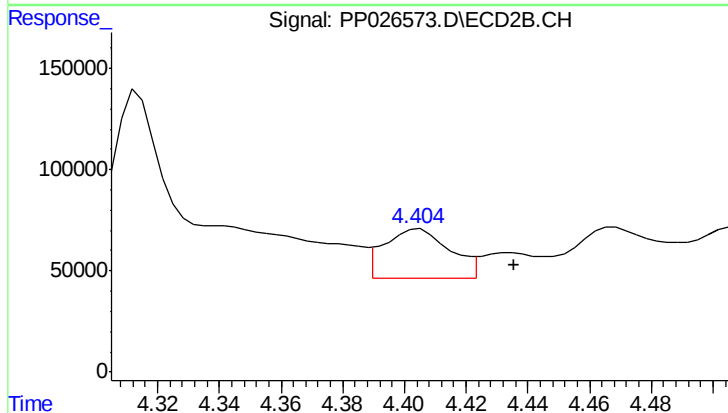


#9 Aroclor-1221-2

R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 360785
Conc: 179.00 ng/ml

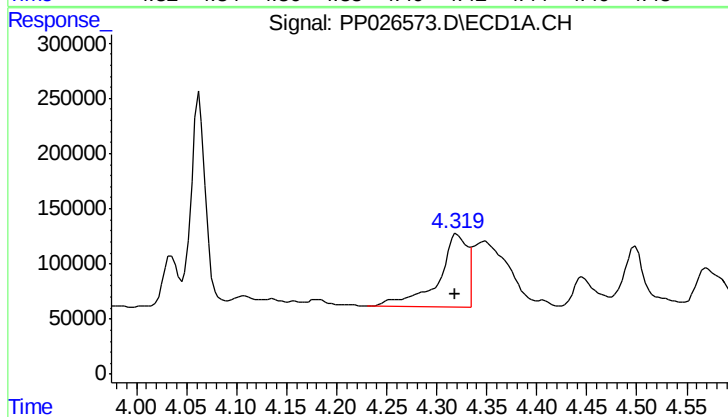


#10 Aroclor-1221-3

R.T.: 4.321 min
Delta R.T.: 0.002 min
Response: 1348975
Conc: 286.85 ng/ml

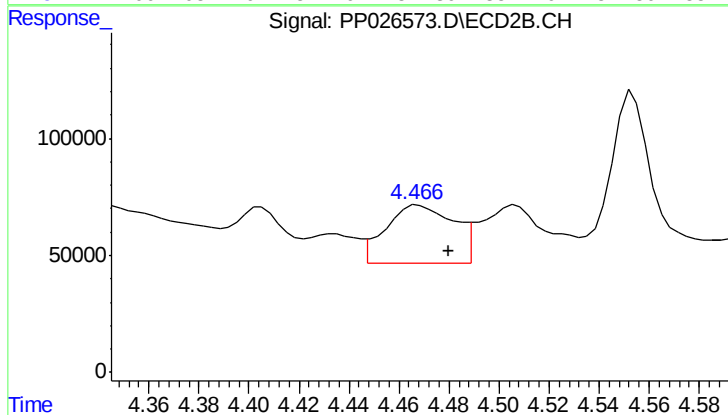

#10 Aroclor-1221-3


R.T.: 4.468 min
Delta R.T.: -0.012 min
Response: 467367
Conc: 64.72 ng/ml

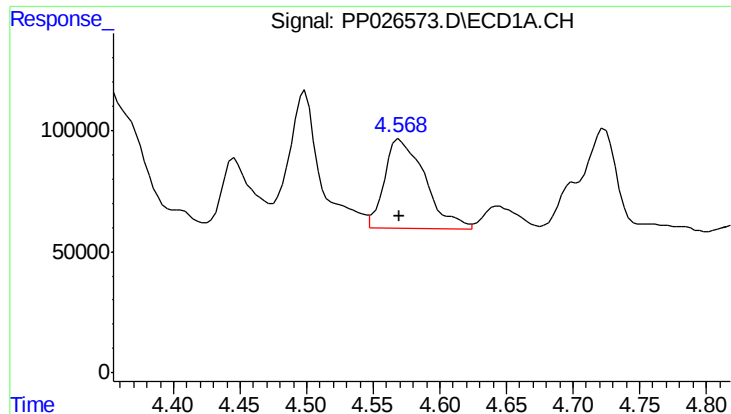

#11 Aroclor-1232-1


R.T.: 4.570 min
Delta R.T.: 0.000 min
Response: 790835
Conc: 615.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

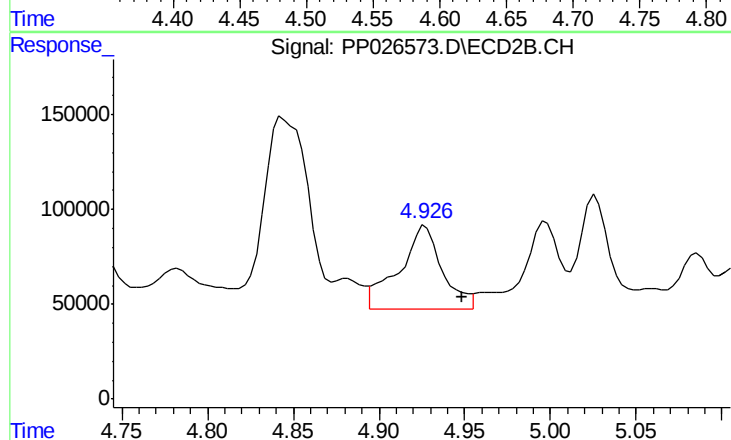


#11 Aroclor-1232-1

R.T.: 4.927 min
Delta R.T.: -0.022 min
Response: 782117
Conc: 477.51 ng/ml

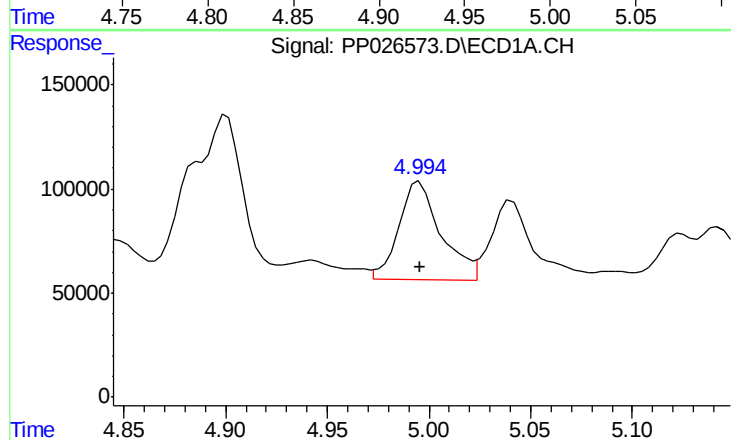


#12 Aroclor-1232-2

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 674709
Conc: 460.20 ng/ml

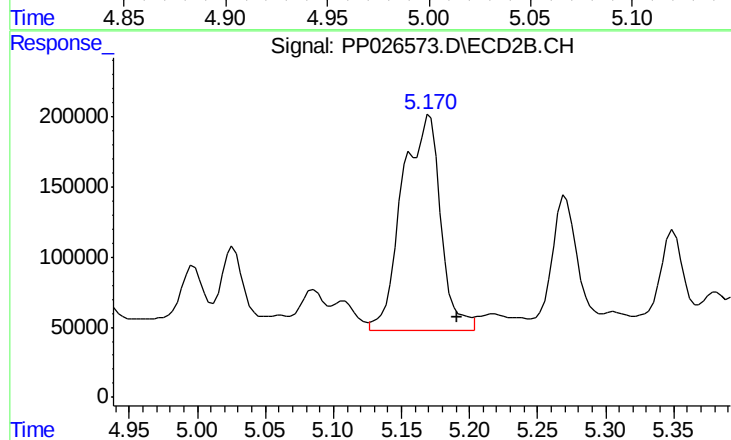

#12 Aroclor-1232-2


R.T.: 5.171 min
Delta R.T.: -0.020 min
Response: 3004891
Conc: 956.06 ng/ml

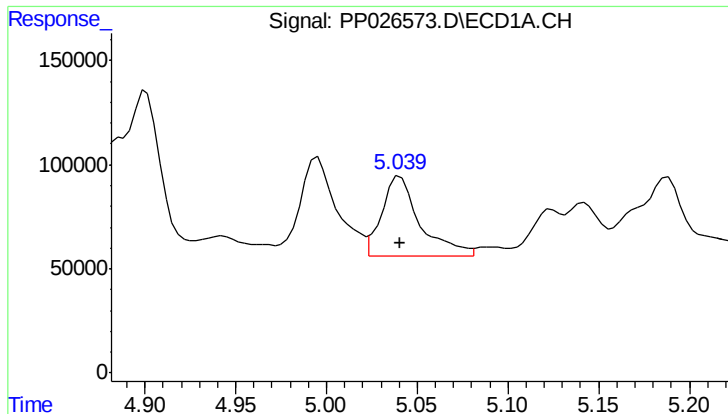

#13 Aroclor-1232-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 560677
Conc: 545.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

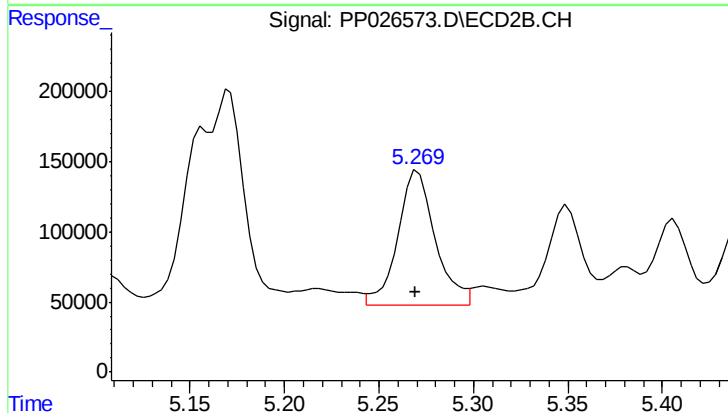


#13 Aroclor-1232-3

R.T.: 5.271 min
Delta R.T.: 0.002 min
Response: 1305251
Conc: 631.92 ng/ml

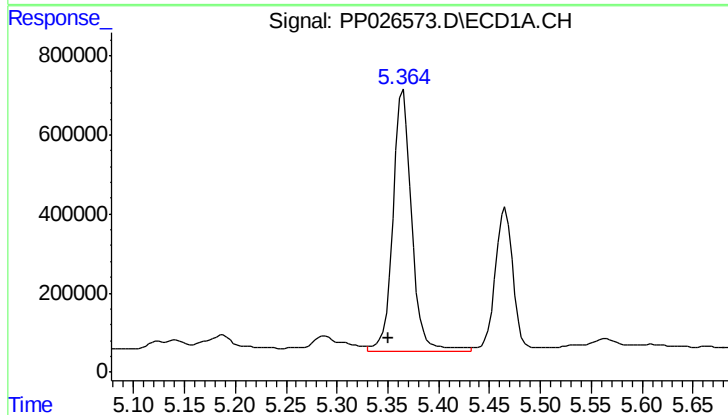


#14 Aroclor-1232-4

R.T.: 5.365 min
Delta R.T.: 0.015 min
Response: 8467379
Conc: 13273.82 ng/ml

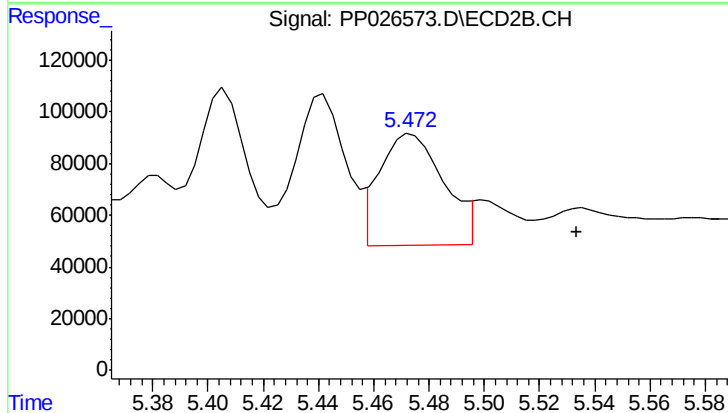

#14 Aroclor-1232-4


R.T.: 5.474 min
Delta R.T.: -0.060 min
Response: 701120
Conc: 333.08 ng/ml

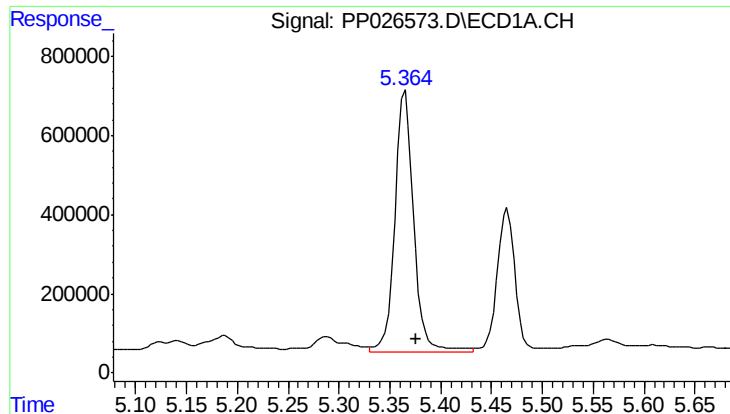

#15 Aroclor-1232-5


R.T.: 5.365 min
Delta R.T.: -0.011 min
Response: 8467379
Conc: 9870.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

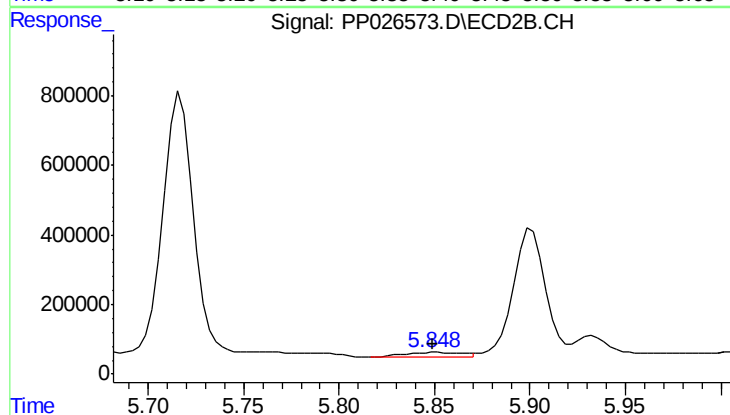


#15 Aroclor-1232-5

R.T.: 5.850 min
Delta R.T.: 0.002 min
Response: 266240
Conc: 109.70 ng/ml

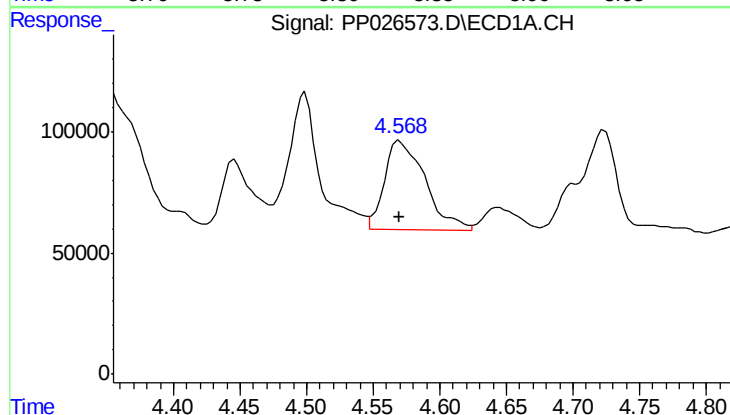


#16 Aroclor-1242-1

R.T.: 4.570 min
Delta R.T.: 0.000 min
Response: 790835
Conc: 385.29 ng/ml

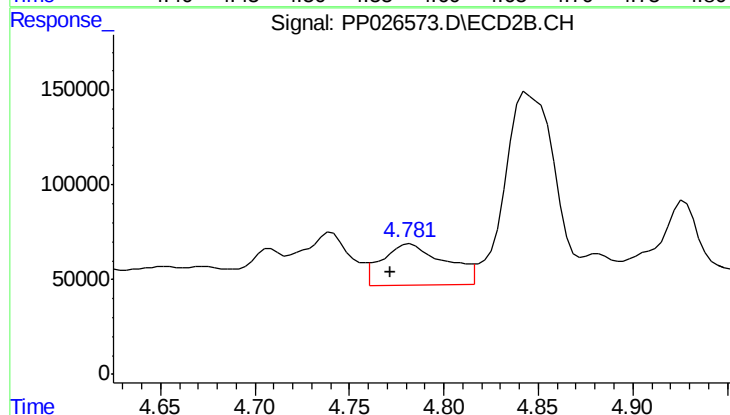

#16 Aroclor-1242-1


R.T.: 4.782 min
Delta R.T.: 0.010 min
Response: 502954
Conc: 82.41 ng/ml

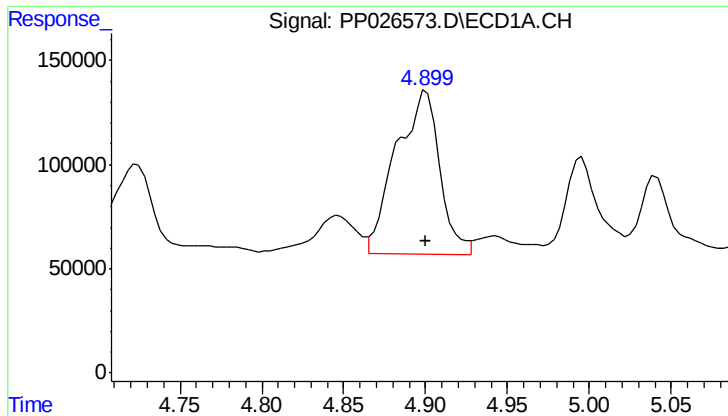

#17 Aroclor-1242-2


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 1456656
Conc: 316.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

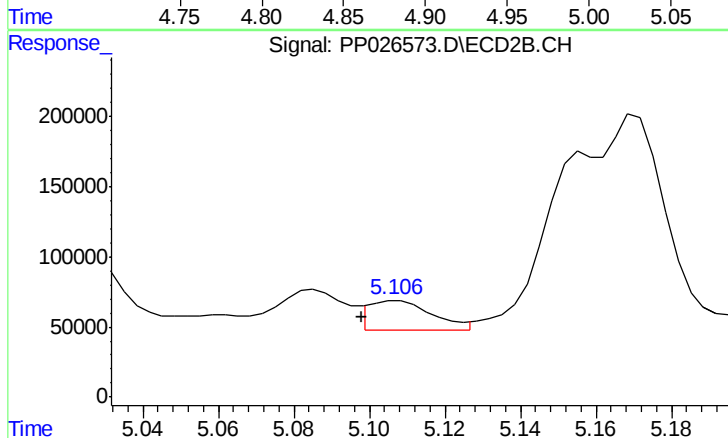


#17 Aroclor-1242-2

R.T.: 5.108 min
Delta R.T.: 0.010 min
Response: 251706
Conc: 33.24 ng/ml

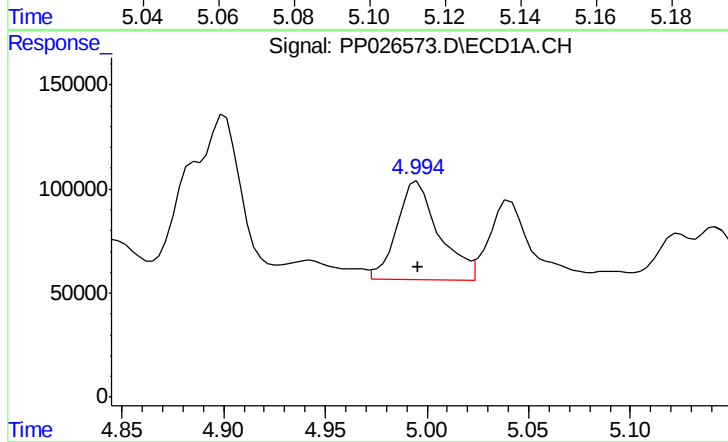


#18 Aroclor-1242-3

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 674709
Conc: 314.54 ng/ml

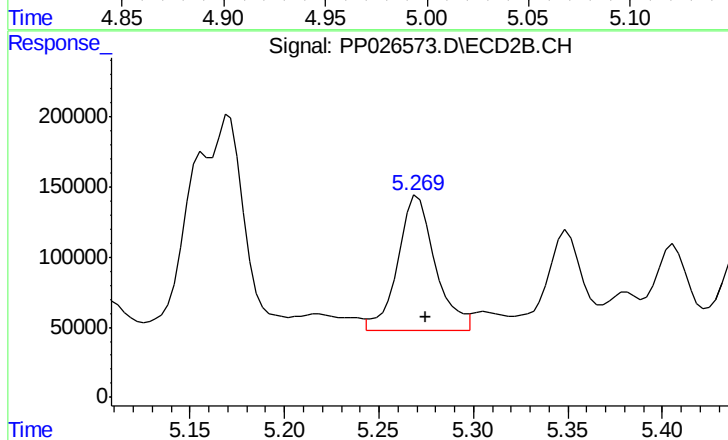

#18 Aroclor-1242-3


R.T.: 5.271 min
Delta R.T.: -0.004 min
Response: 1305251
Conc: 433.53 ng/ml

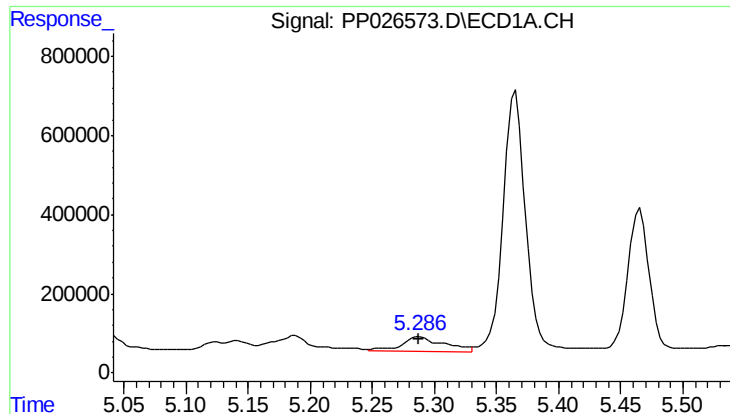

#19 Aroclor-1242-4


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 875839
Conc: 429.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

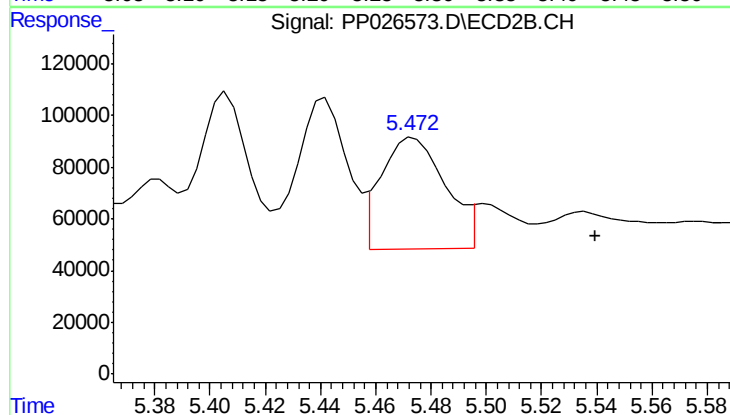


#19 Aroclor-1242-4

R.T.: 5.474 min
Delta R.T.: -0.066 min
Response: 701120
Conc: 210.51 ng/ml

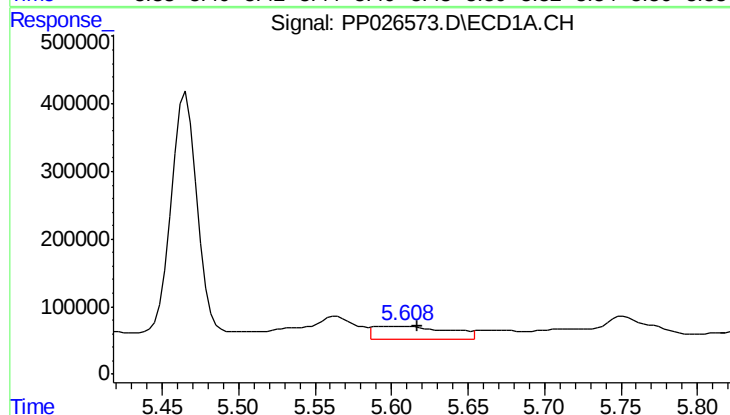


#20 Aroclor-1242-5

R.T.: 5.610 min
Delta R.T.: -0.007 min
Response: 626042
Conc: 352.29 ng/ml

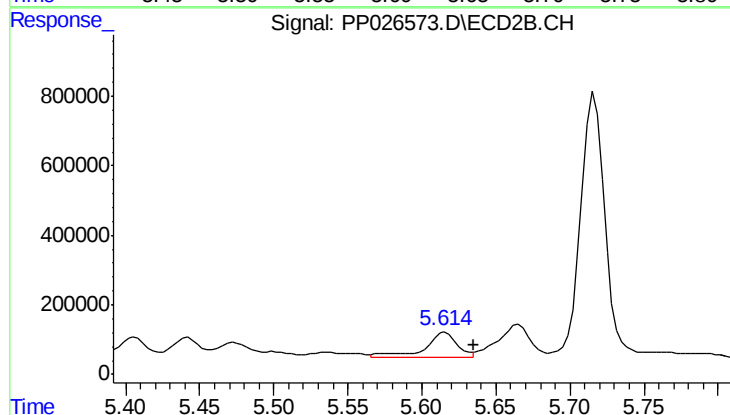

#20 Aroclor-1242-5


R.T.: 5.616 min
Delta R.T.: -0.019 min
Response: 1114713
Conc: 231.44 ng/ml

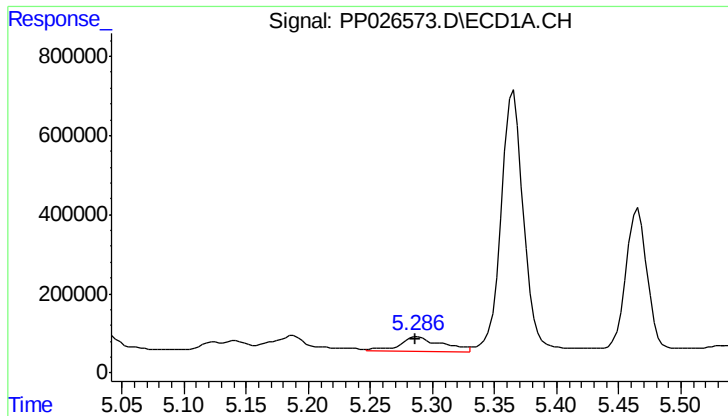

#21 Aroclor-1248-1


R.T.: 5.287 min
Delta R.T.: 0.001 min
Response: 875839
Conc: 256.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

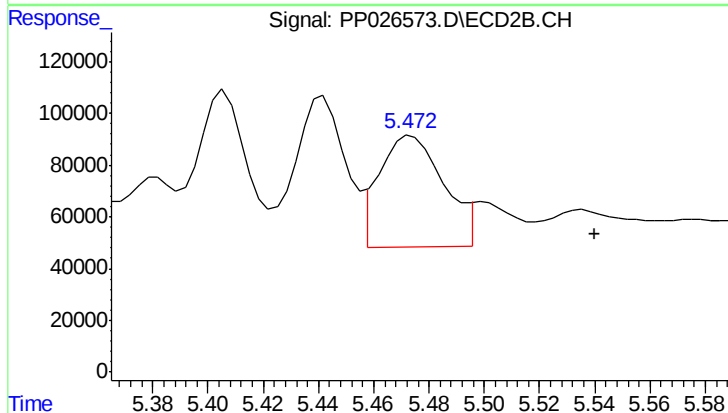


#21 Aroclor-1248-1

R.T.: 5.474 min
Delta R.T.: -0.066 min
Response: 701120
Conc: 113.99 ng/ml

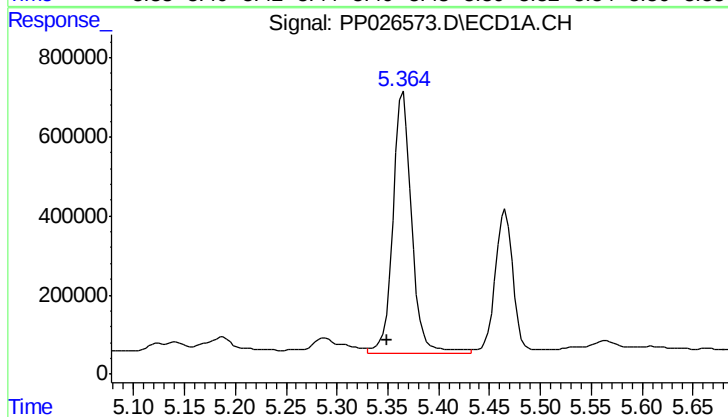


#22 Aroclor-1248-2

R.T.: 5.365 min
Delta R.T.: 0.016 min
Response: 8467379
Conc: 4397.50 ng/ml

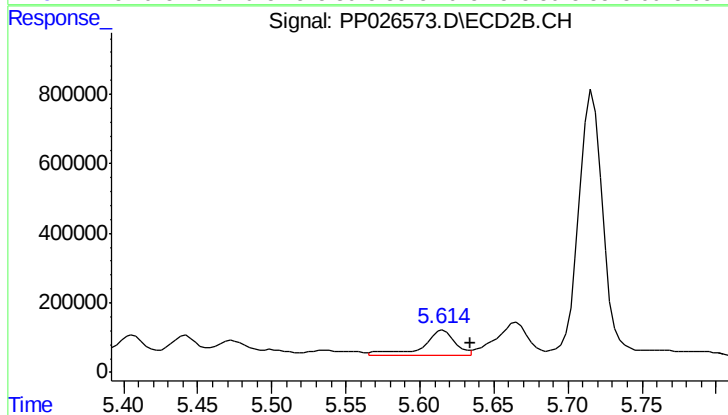

#22 Aroclor-1248-2


R.T.: 5.616 min
Delta R.T.: -0.019 min
Response: 1114713
Conc: 153.16 ng/ml

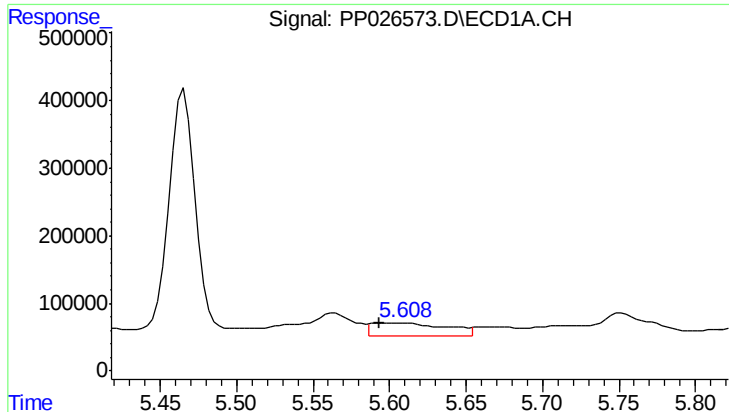

#23 Aroclor-1248-3


R.T.: 5.610 min
Delta R.T.: 0.016 min
Response: 626042
Conc: 206.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

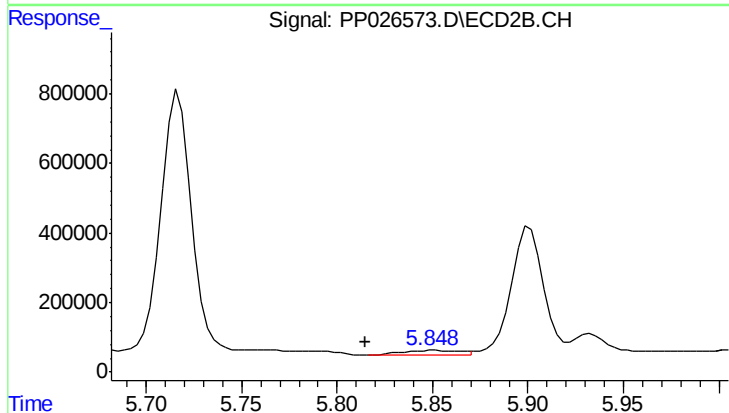


#23 Aroclor-1248-3

R.T.: 5.850 min
Delta R.T.: 0.036 min
Response: 266240
Conc: 37.86 ng/ml

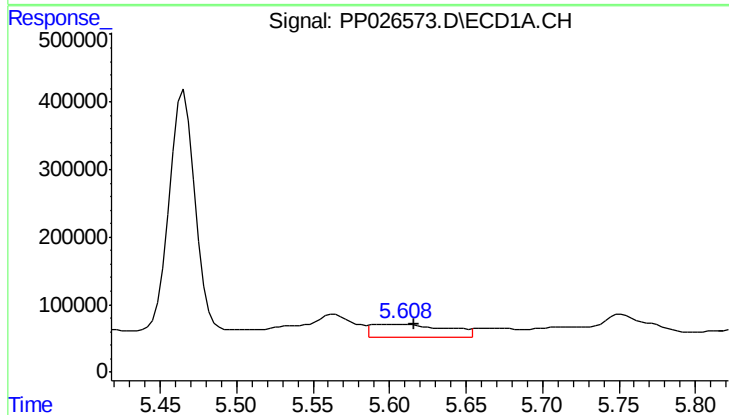


#24 Aroclor-1248-4

R.T.: 5.610 min
Delta R.T.: -0.006 min
Response: 626042
Conc: 202.95 ng/ml

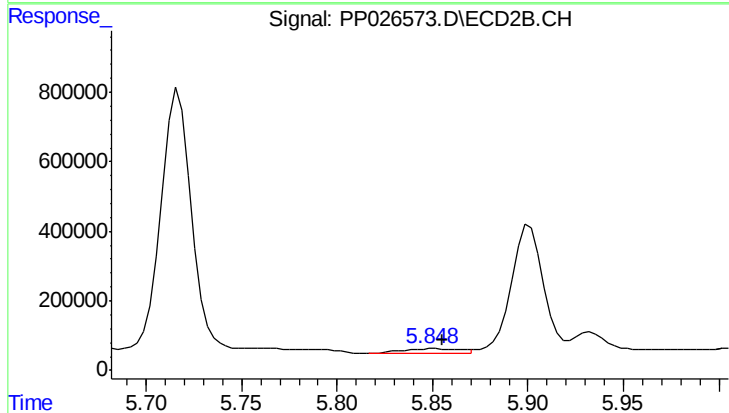

#24 Aroclor-1248-4


R.T.: 5.850 min
Delta R.T.: -0.005 min
Response: 266240
Conc: 33.62 ng/ml

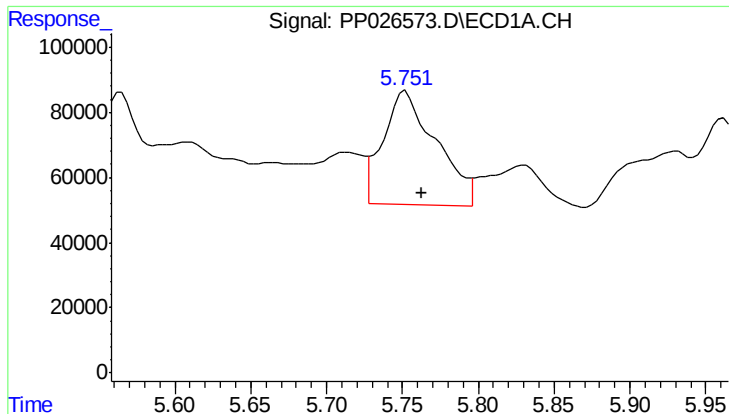

#25 Aroclor-1248-5


R.T.: 5.752 min
Delta R.T.: -0.011 min
Response: 848085
Conc: 287.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

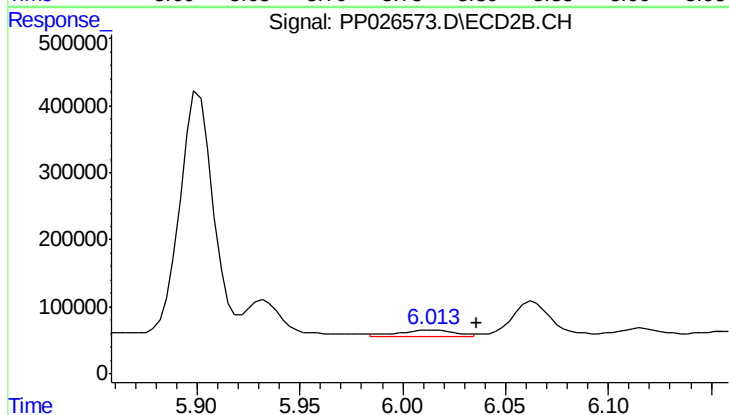


#25 Aroclor-1248-5

R.T.: 6.015 min
Delta R.T.: -0.021 min
Response: 183919
Conc: 24.89 ng/ml

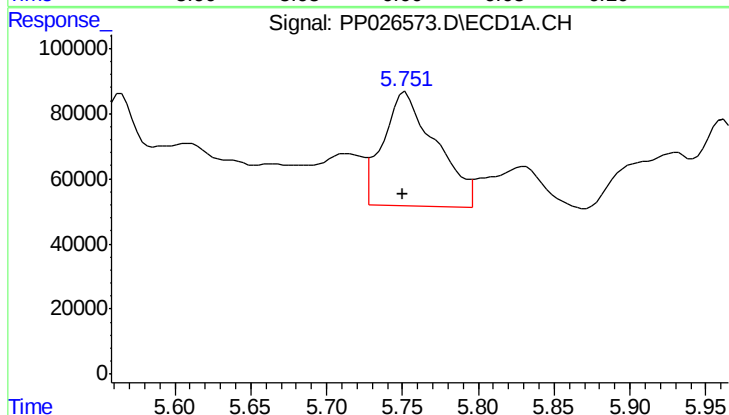


#26 Aroclor-1254-1

R.T.: 5.752 min
Delta R.T.: 0.002 min
Response: 848085
Conc: 183.88 ng/ml

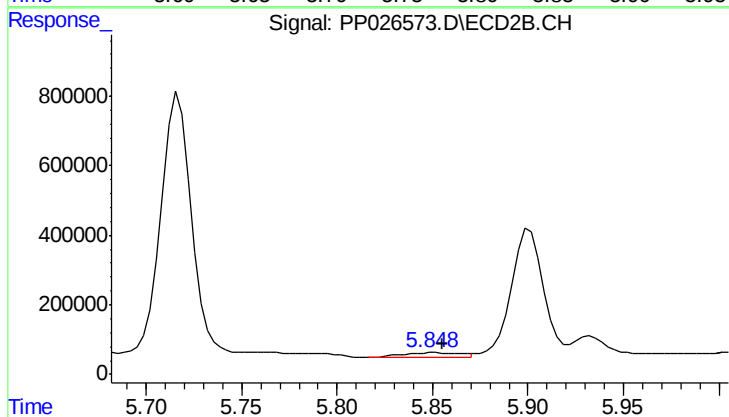

#26 Aroclor-1254-1


R.T.: 5.850 min
Delta R.T.: -0.005 min
Response: 266240
Conc: 36.54 ng/ml

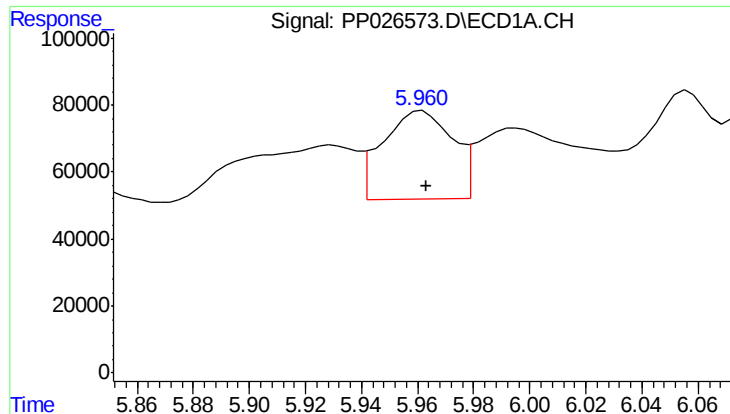

#27 Aroclor-1254-2


R.T.: 5.962 min
Delta R.T.: -0.002 min
Response: 457033
Conc: 136.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

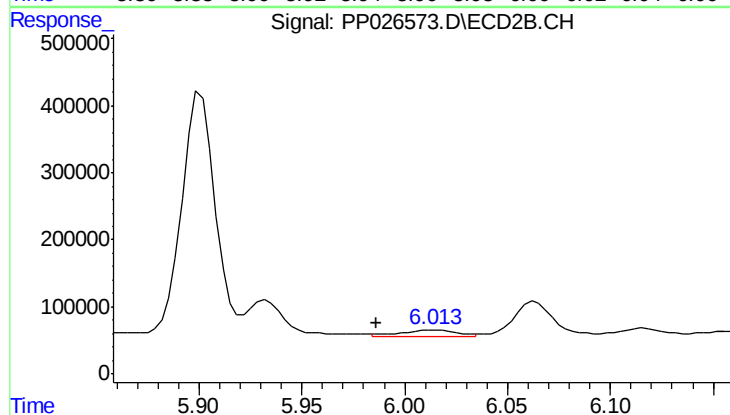


#27 Aroclor-1254-2

R.T.: 6.015 min
Delta R.T.: 0.029 min
Response: 183919
Conc: 23.73 ng/ml

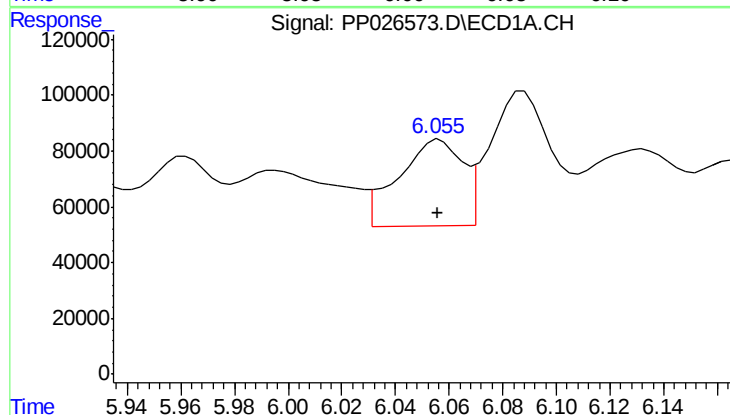


#28 Aroclor-1254-3

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 525377
Conc: 86.59 ng/ml

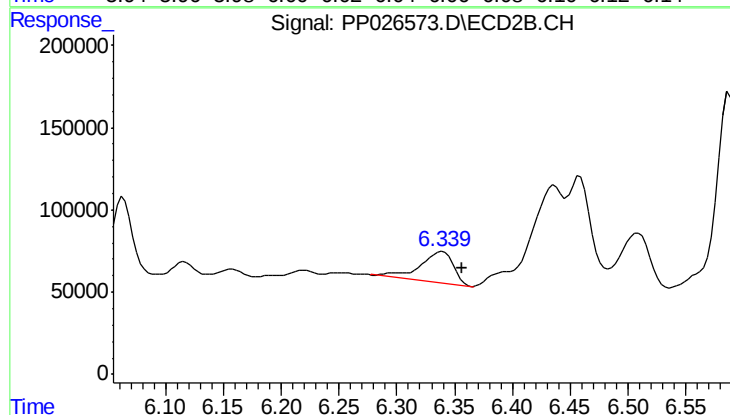

#28 Aroclor-1254-3


R.T.: 6.340 min
Delta R.T.: -0.017 min
Response: 385321
Conc: 29.70 ng/ml

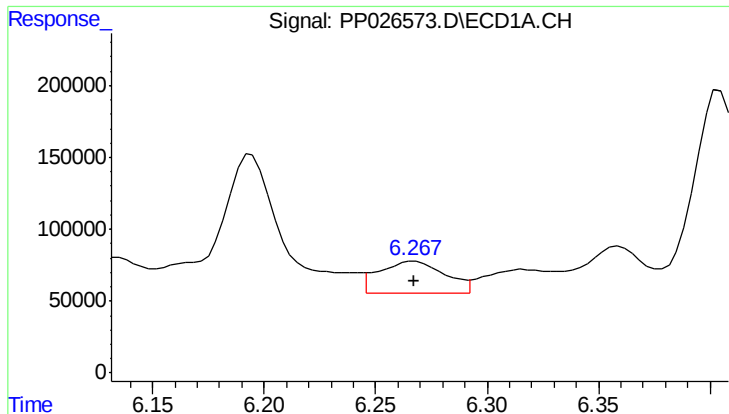

#29 Aroclor-1254-4


R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 457815
Conc: 77.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

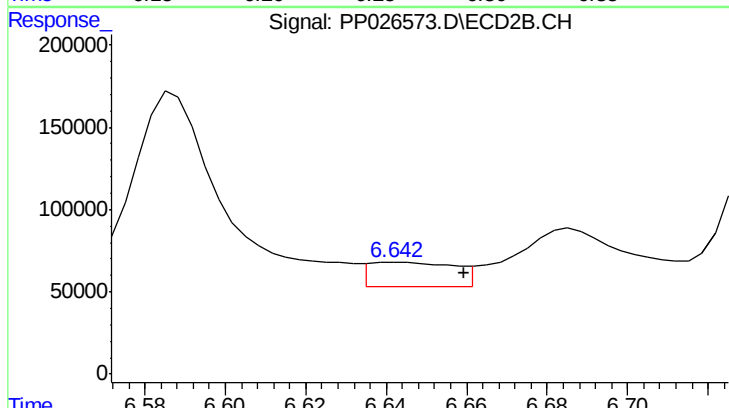


#29 Aroclor-1254-4

R.T.: 6.644 min
Delta R.T.: -0.016 min
Response: 215091
Conc: 41.76 ng/ml

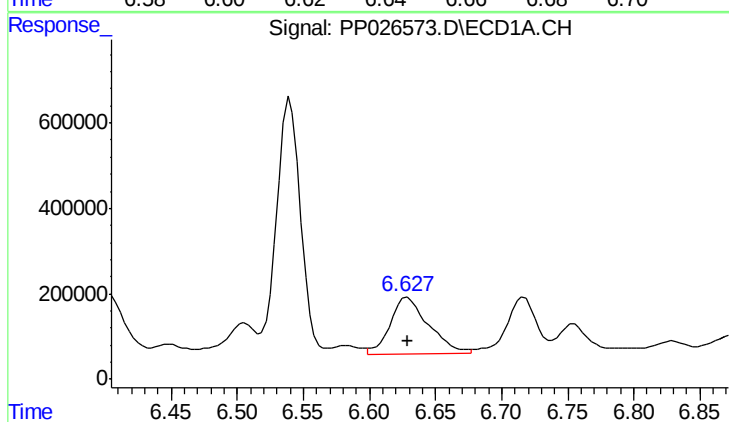


#30 Aroclor-1254-5

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 2665999
Conc: 350.82 ng/ml

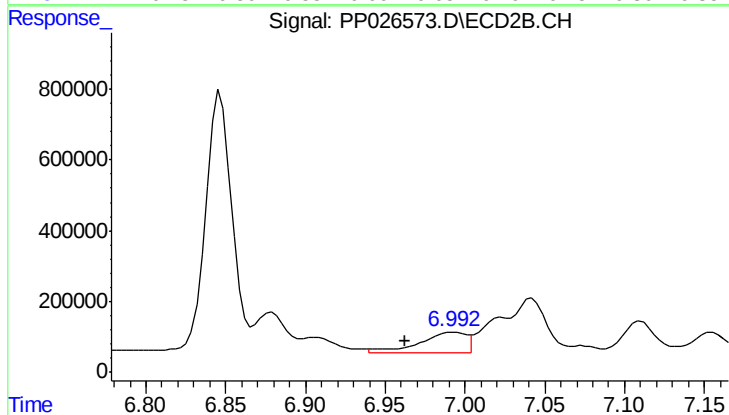

#30 Aroclor-1254-5


R.T.: 6.993 min
Delta R.T.: 0.031 min
Response: 1195294
Conc: 110.73 ng/ml

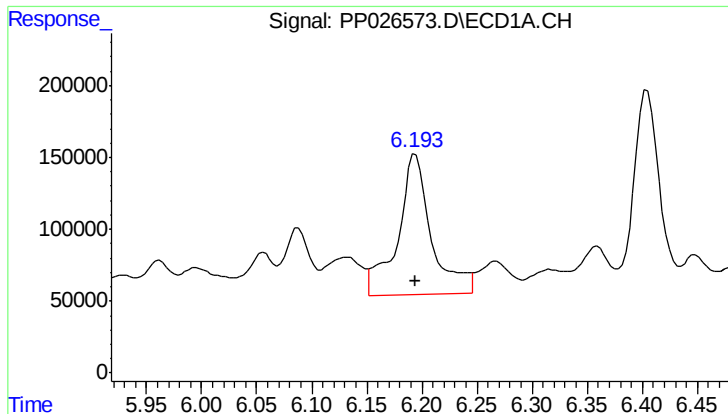

#31 Aroclor-1260-1


R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 2077463
Conc: 575.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

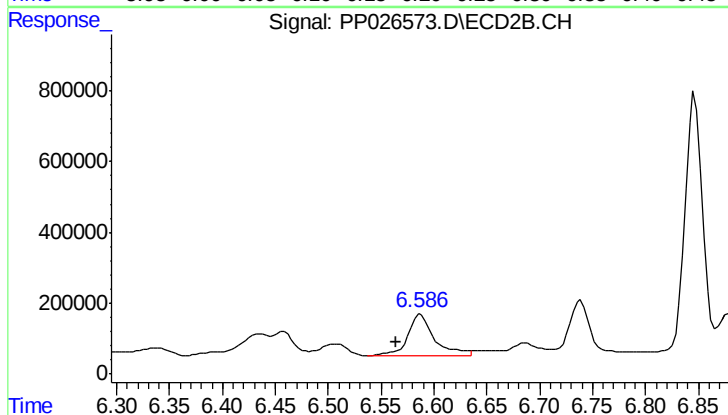


#31 Aroclor-1260-1

R.T.: 6.587 min
Delta R.T.: 0.023 min
Response: 1997326
Conc: 250.06 ng/ml

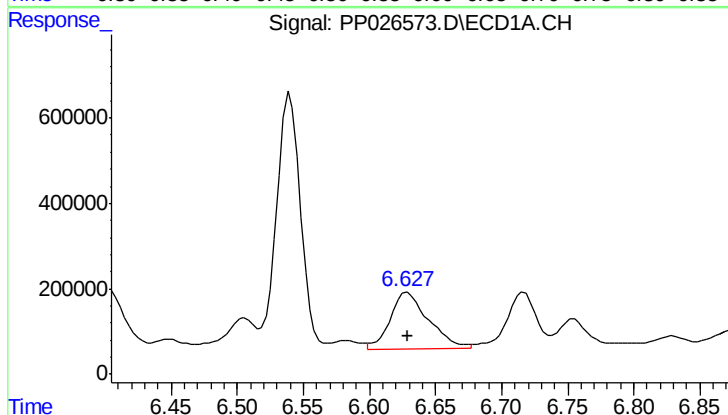


#32 Aroclor-1260-2

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 2665999
Conc: 287.46 ng/ml

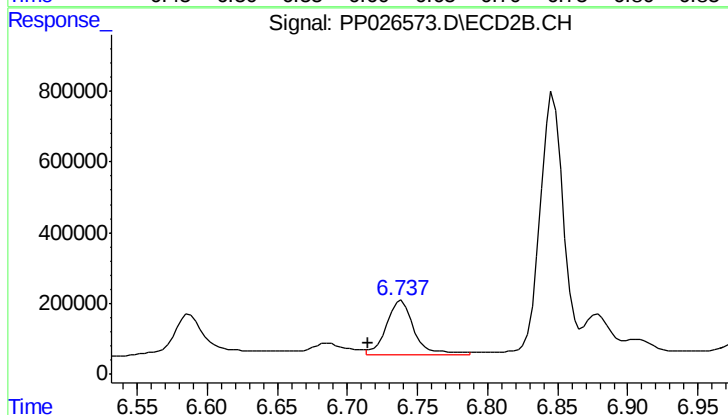

#32 Aroclor-1260-2


R.T.: 6.739 min
Delta R.T.: 0.024 min
Response: 2206967
Conc: 243.37 ng/ml

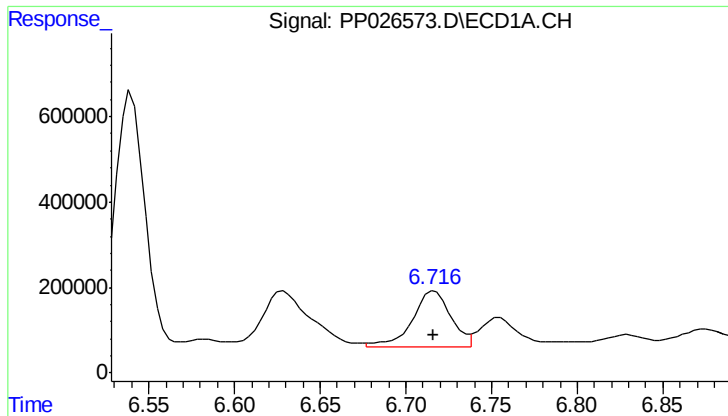

#33 Aroclor-1260-3


R.T.: 6.717 min
Delta R.T.: 0.001 min
Response: 2074012
Conc: 312.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

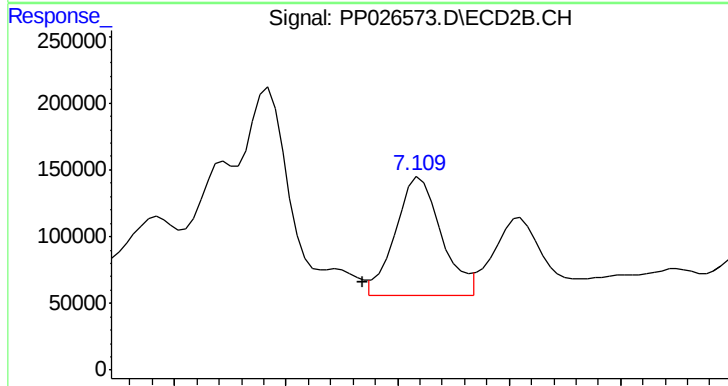


#33 Aroclor-1260-3

R.T.: 7.110 min
Delta R.T.: 0.026 min
Response: 1260369
Conc: 198.68 ng/ml

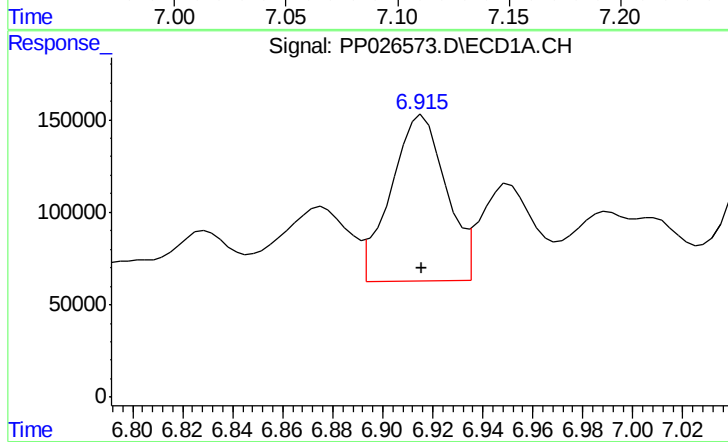


#34 Aroclor-1260-4

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 1361652
Conc: 260.72 ng/ml

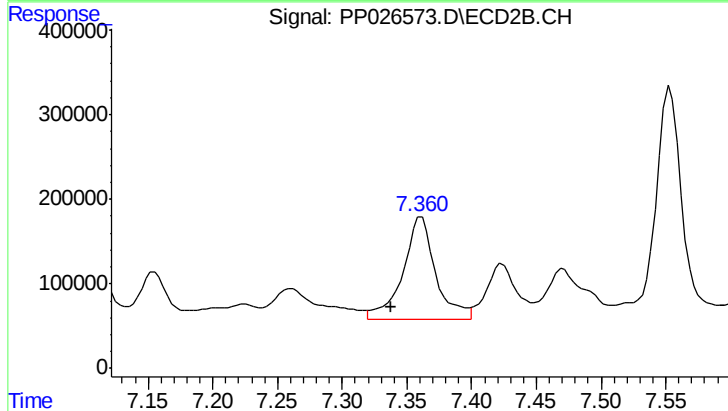

#34 Aroclor-1260-4


R.T.: 7.361 min
Delta R.T.: 0.023 min
Response: 2155460
Conc: 293.94 ng/ml

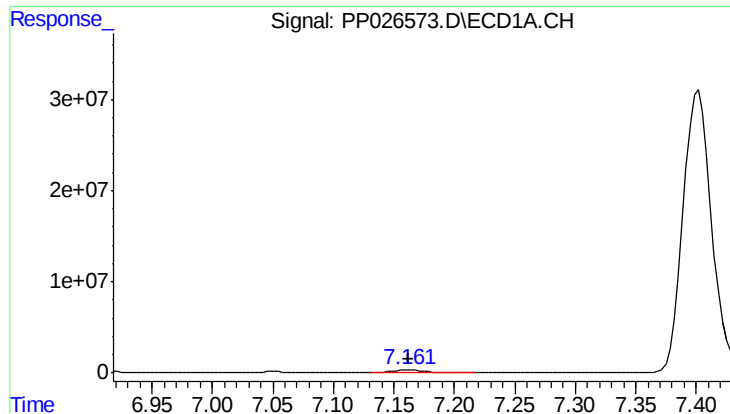

#35 Aroclor-1260-5


R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 4851474
Conc: 256.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

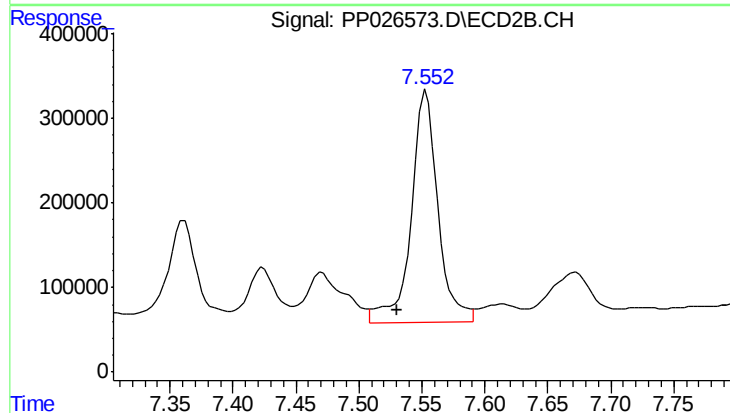


#35 Aroclor-1260-5

R.T.: 7.554 min
Delta R.T.: 0.023 min
Response: 4045990
Conc: 252.20 ng/ml

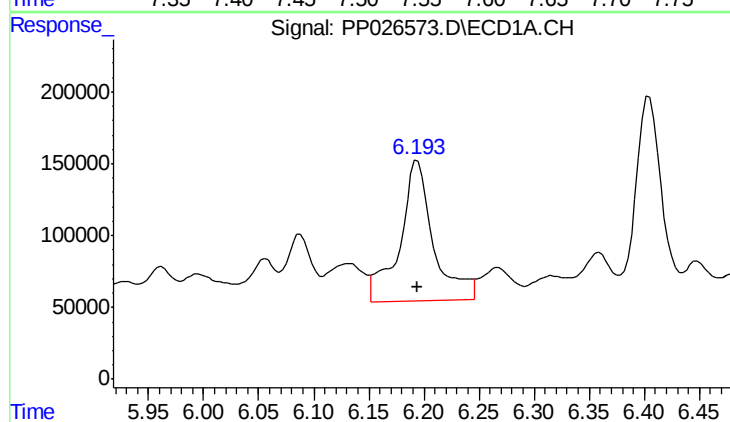


#36 Aroclor-1262-1

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 2077463
Conc: 623.53 ng/ml

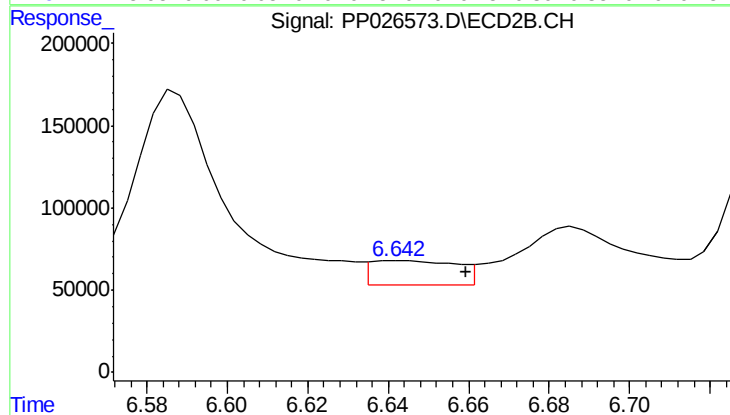

#36 Aroclor-1262-1


R.T.: 6.644 min
Delta R.T.: -0.016 min
Response: 215091
Conc: 26.39 ng/ml

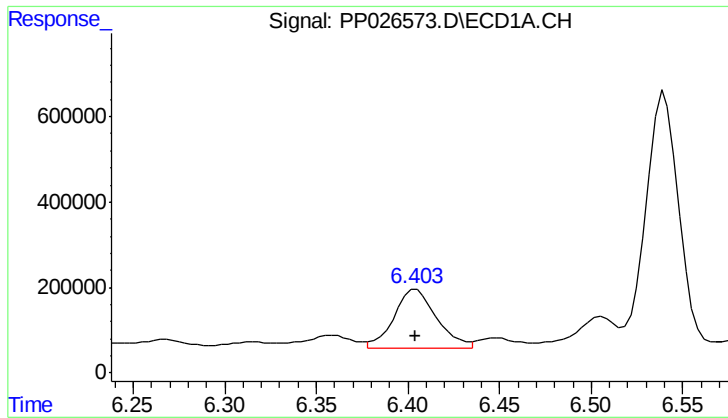

#37 Aroclor-1262-2


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 2273389
Conc: 338.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

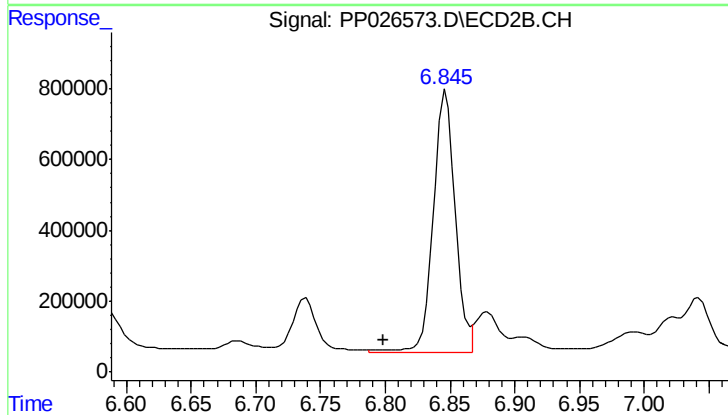


#37 Aroclor-1262-2

R.T.: 6.847 min
Delta R.T.: 0.048 min
Response: 8732123
Conc: 1854.84 ng/ml

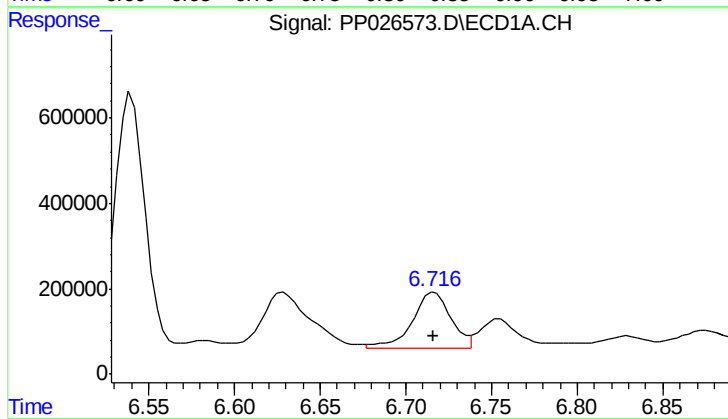


#38 Aroclor-1262-3

R.T.: 6.717 min
Delta R.T.: 0.001 min
Response: 2074012
Conc: 179.25 ng/ml

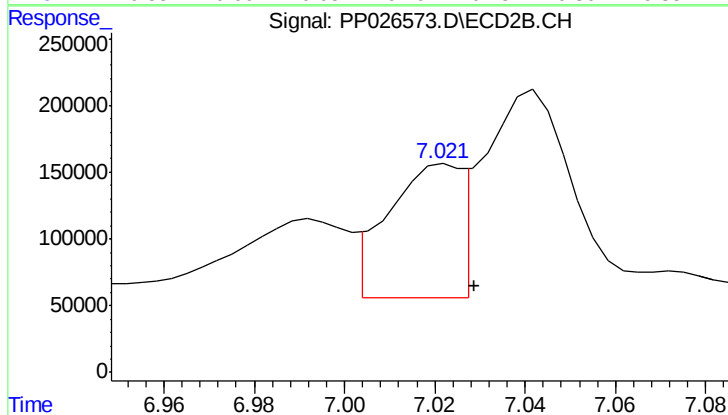

#38 Aroclor-1262-3


R.T.: 7.023 min
Delta R.T.: -0.006 min
Response: 1108426
Conc: 100.54 ng/ml

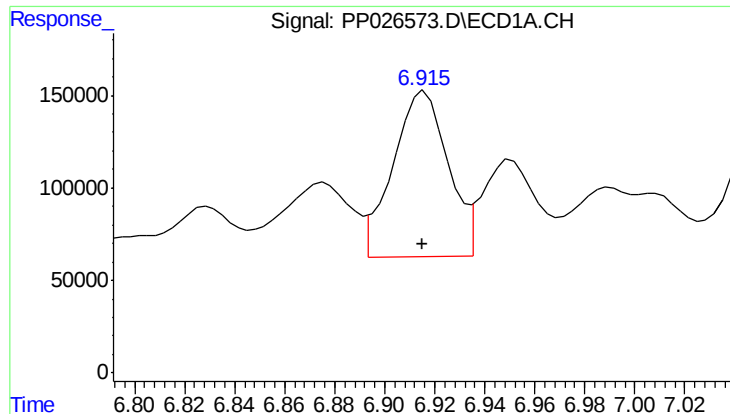

#39 Aroclor-1262-4


R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 1361652
Conc: 168.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

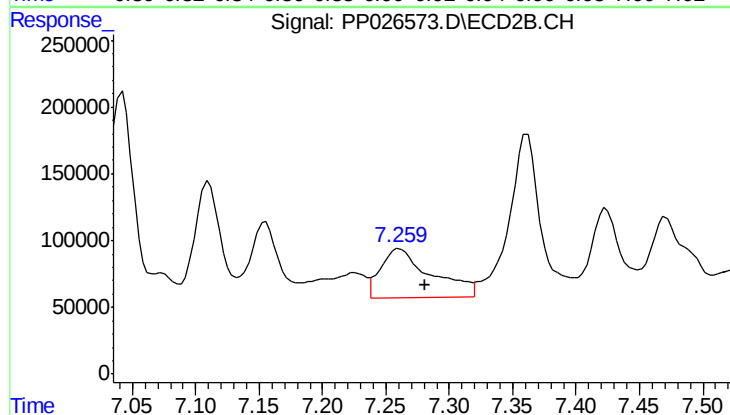


#39 Aroclor-1262-4

R.T.: 7.261 min
Delta R.T.: -0.021 min
Response: 1023385
Conc: 102.40 ng/ml

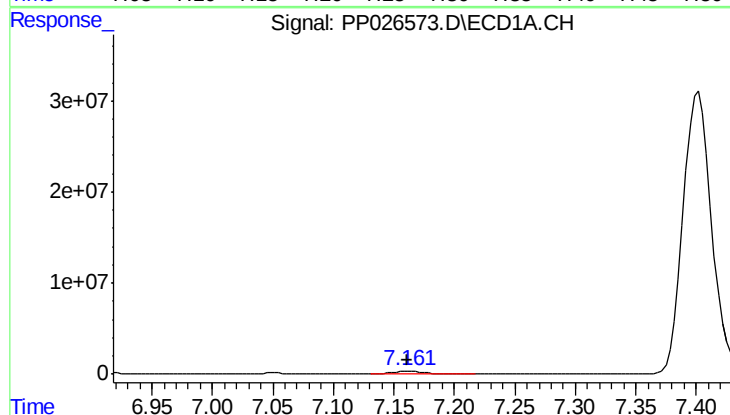


#40 Aroclor-1262-5

R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 4851474
Conc: 183.44 ng/ml

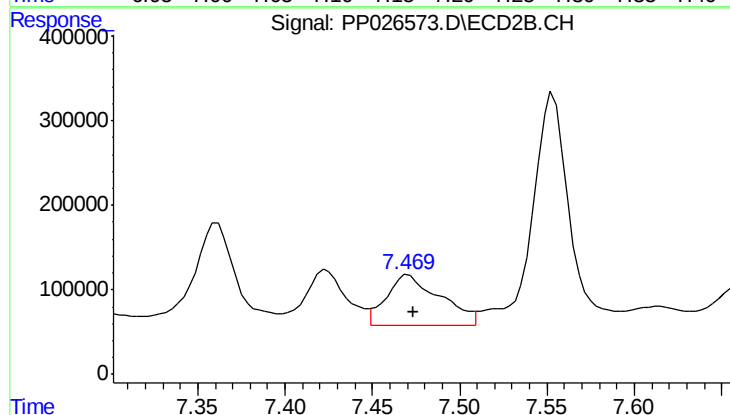

#40 Aroclor-1262-5


R.T.: 7.471 min
Delta R.T.: -0.003 min
Response: 1261272
Conc: 59.86 ng/ml

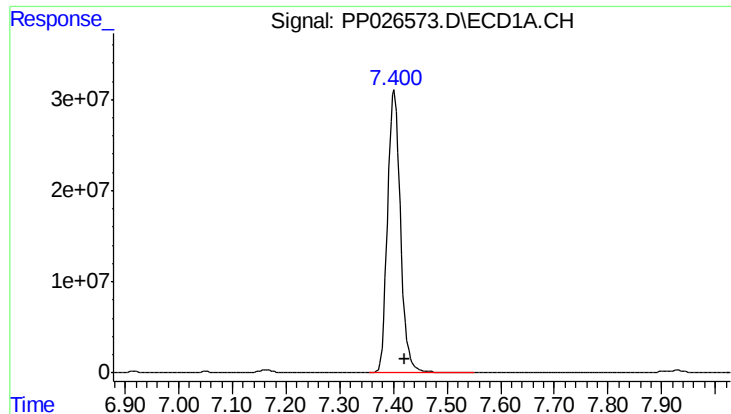

#41 Aroclor-1268-1


R.T.: 7.402 min
Delta R.T.: -0.018 min
Response: 516188191
Conc: 19018.65 ng/m

Instrument :
ECD_P
ClientSampleId :
PB110339BS

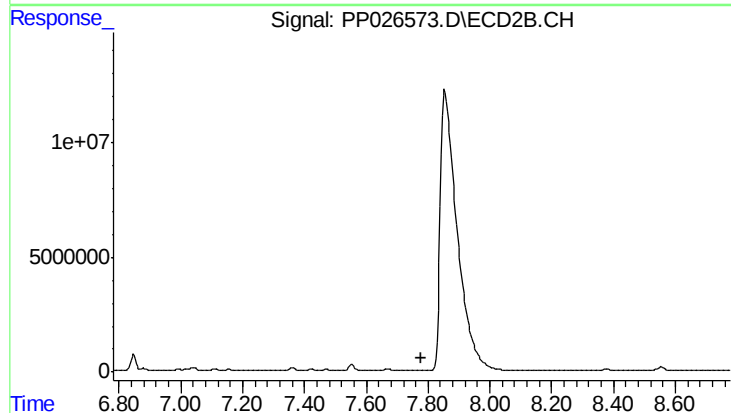


#41 Aroclor-1268-1

R.T.: 0.000 min
Exp R.T.: 7.779 min
Response: 0
Conc: N.D.

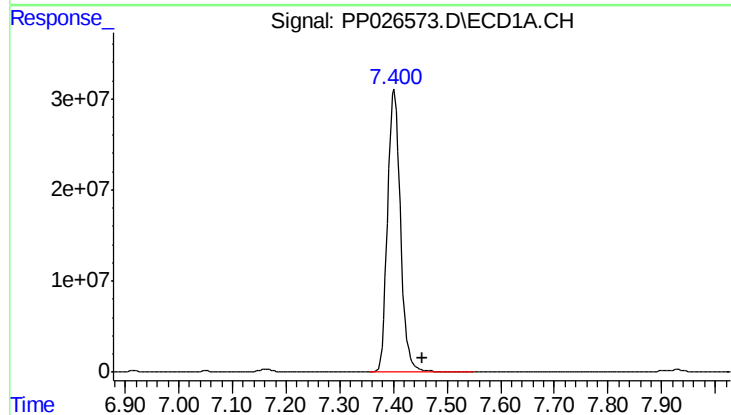


#42 Aroclor-1268-2

R.T.: 7.402 min
Delta R.T.: -0.053 min
Response: 516188191
Conc: 24986.61 ng/ml

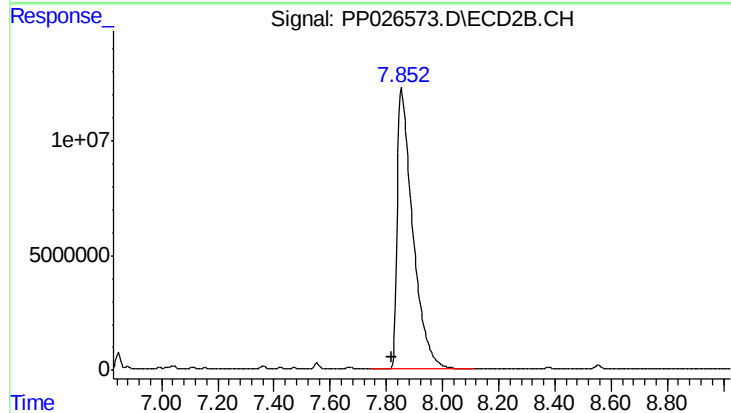

#42 Aroclor-1268-2


R.T.: 7.853 min
Delta R.T.: 0.034 min
Response: 469544009
Conc: 24997.85 ng/ml

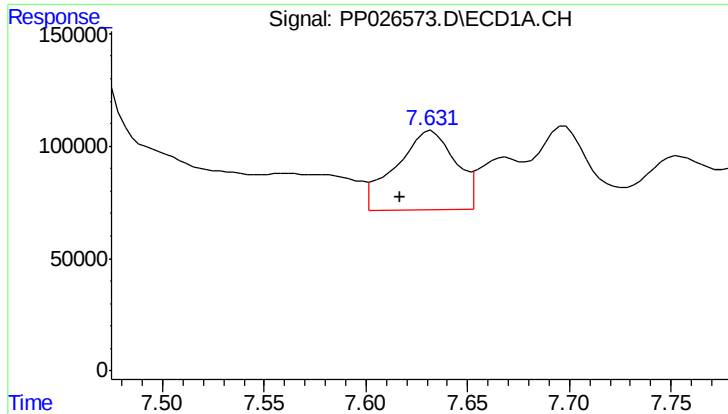

#43 Aroclor-1268-3


R.T.: 7.632 min
Delta R.T.: 0.016 min
Response: 723819
Conc: 39.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

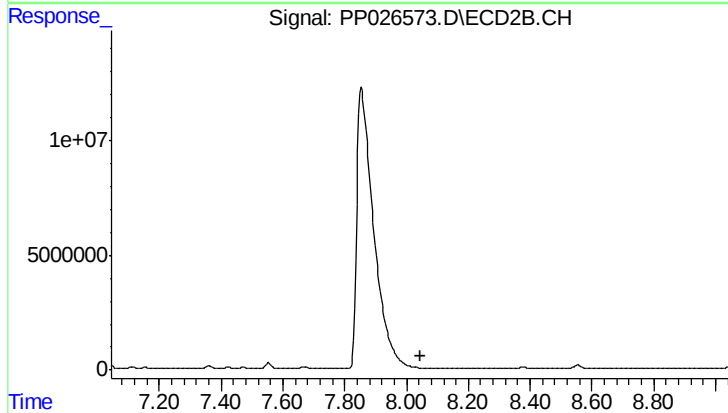


#43 Aroclor-1268-3

R.T.: 0.000 min
Exp R.T.: 8.044 min
Response: 0
Conc: N.D.

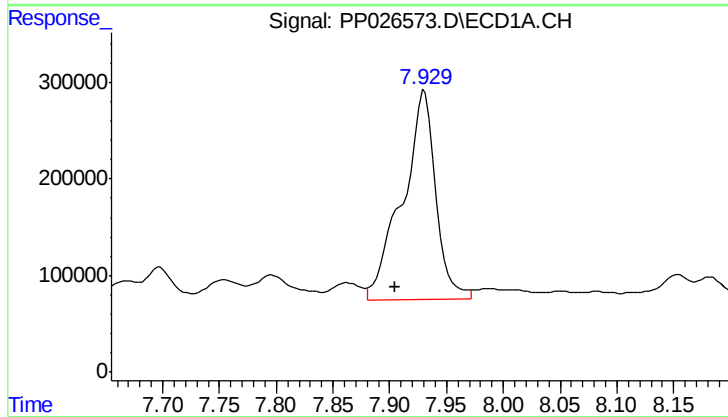


#44 Aroclor-1268-4

R.T.: 7.931 min
Delta R.T.: 0.026 min
Response: 4510187
Conc: 547.90 ng/ml

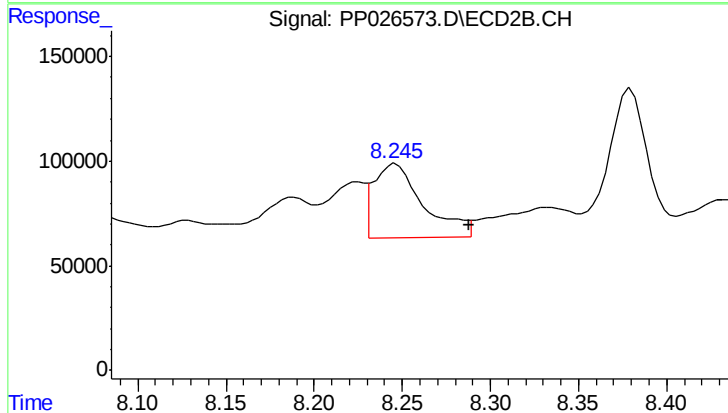

#44 Aroclor-1268-4


R.T.: 8.246 min
Delta R.T.: -0.041 min
Response: 706459
Conc: 95.28 ng/ml

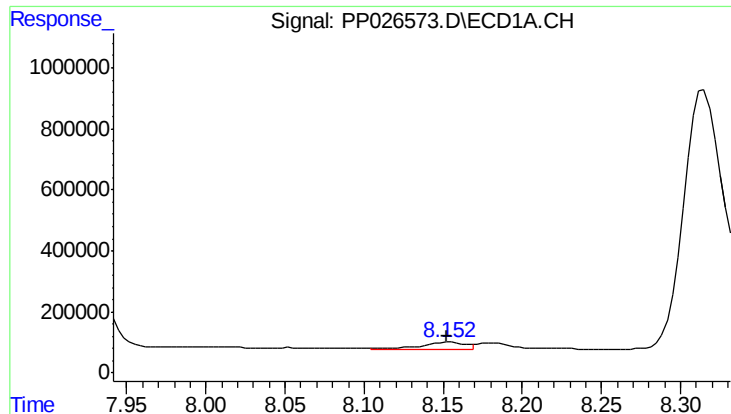

#45 Aroclor-1268-5

R.T.: 8.154 min
Delta R.T.: 0.001 min
Response: 478937
Conc: 7.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BS

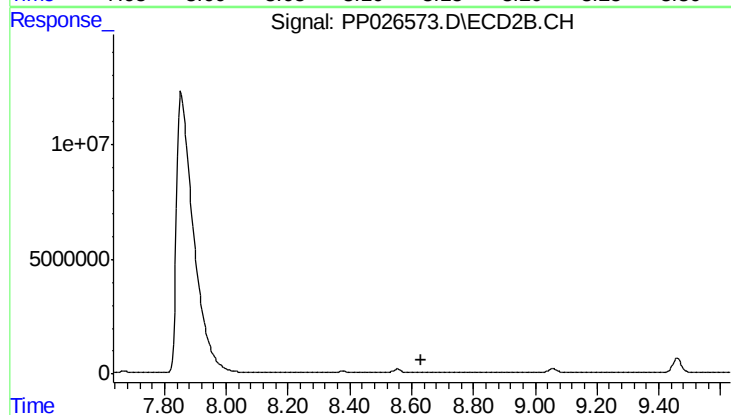

#45 Aroclor-1268-5

R.T.: 0.000 min
Exp R.T. : 8.633 min
Response: 0
Conc: N.D.