

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP062574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 1:08
 Operator : UA/AJ
 Sample : PB110339BSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110339BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 05:16:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 05:10:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	4.199	1802422	4050881	19.707	17.672
2) SA Decachlor...	8.316	9.063	9532528	3418720	63.117	21.295 #
Target Compounds						
3) L1 Aroclor-1...	4.569	4.557	689550	759014	301.395	194.195 #
4) L1 Aroclor-1...	4.995	5.030	595579	568909	224.835	196.237
5) L1 Aroclor-1...	5.041	5.275	443678	1029121	244.367	175.314 #
6) L1 Aroclor-1...	5.365	5.353	5329305	754238	4351.935	198.506 #
7) L1 Aroclor-1...	5.365	5.619	5329305	958821	3505.277	239.799 #
8) L2 Aroclor-1...	0.000	4.317	0	1284391	N.D.	1788.868 #
9) L2 Aroclor-1...	4.320	4.408	1159646	250371	1248.667	792.429 #
10) L2 Aroclor-1...	4.320	4.474	1159646	235629	332.606	291.376
11) L3 Aroclor-1...	4.569	4.931	689550	521438	280.736	247.762
12) L3 Aroclor-1...	4.995	5.174	595579	2609248	216.713	486.029 #
13) L3 Aroclor-1...	5.041	5.275	443678	1029121	229.981	4468.065 #
14) L3 Aroclor-1...	5.365	5.619	5329305	958821	4143.015	245.618 #
15) L3 Aroclor-1...	5.365	5.853	5329305	278948	3539.684	186.128 #
16) L4 Aroclor-1...	4.569	4.786	689550	254356	280.736	36.178 #
17) L4 Aroclor-1...	4.900	5.112	1396434	143986	233.281	10.261 #
18) L4 Aroclor-1...	4.995	5.275	595579	1029121	216.713	4468.065 #
19) L4 Aroclor-1...	5.287	5.619	538486	958821	222.028	245.618
20) L4 Aroclor-1...	5.592	5.668	16888	1069783	29.338	278.025 #
21) L5 Aroclor-1...	5.287	5.619	538486	958821	222.028	245.618
22) L5 Aroclor-1...	5.365	5.668	5329305	1069783	4143.015	278.025 #
23) L5 Aroclor-1...	5.592	5.853	16888	278948	24.036	186.128 #
24) L5 Aroclor-1...	5.592	5.853	16888	278948	29.338	186.128 #
25) L5 Aroclor-1...	5.752	6.067	560246	862800	378.125	2502.398 #
26) L6 Aroclor-1...	5.752	5.853	560246	278948	378.125	186.128 #
27) L6 Aroclor-1...	5.962	6.019	433768	352028	415.188	138.152 #
28) L6 Aroclor-1...	6.056	6.343	474505	658807	589.437	290.315 #
29) L6 Aroclor-1...	6.267	6.689	379476	662042	633.273	80.861 #
30) L6 Aroclor-1...	6.629	6.994	2117676	830498	232.997	72.768 #
31) L7 Aroclor-1...	6.194	6.591	1765651	2293955	481.588	286.937 #
32) L7 Aroclor-1...	6.629	6.742	2117676	2065167	225.257	228.391
33) L7 Aroclor-1...	6.716	7.113	1376547	1250770	204.326	195.704
34) L7 Aroclor-1...	6.916	7.365	1224434	2003351	230.288	270.395
35) L7 Aroclor-1...	7.162	7.557	4453739	3683514	233.664	229.035
36) L8 Aroclor-1...	6.194	6.689	1765651	662042	501.428	80.861 #
37) L8 Aroclor-1...	6.405	6.850	2186106	4589756	270.279	758.875 #
38) L8 Aroclor-1...	6.716	7.026	1376547	1015108	213.950	4710.444 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 1:08
 Operator : UA/AJ
 Sample : PB110339BSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110339BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 05:16:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 05:10:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39) L8	Aroclor-1...	6.916	7.265	1224434	950895	230.427	144.648 #
40) L8	Aroclor-1...	7.162	7.474	4453739	1186488	231.233	5235.997 #
41) L9	Aroclor-1...	7.401	0.000	345.4E6	0	27580.540	N.D. #
42) L9	Aroclor-1...	7.401	7.857	345.4E6	287.0E6	68853.070	25170.639 #
43) L9	Aroclor-1...	7.631	0.000	448625	0	1984.076	N.D. #
44) L9	Aroclor-1...	7.907	8.251	1118650	611211	217.169	127.322 #
45) L9	Aroclor-1...	8.154	0.000	328337	0	262.187	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 1:08
Operator : UA/AJ
Sample : PB110339BSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 05:16:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 05:10:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

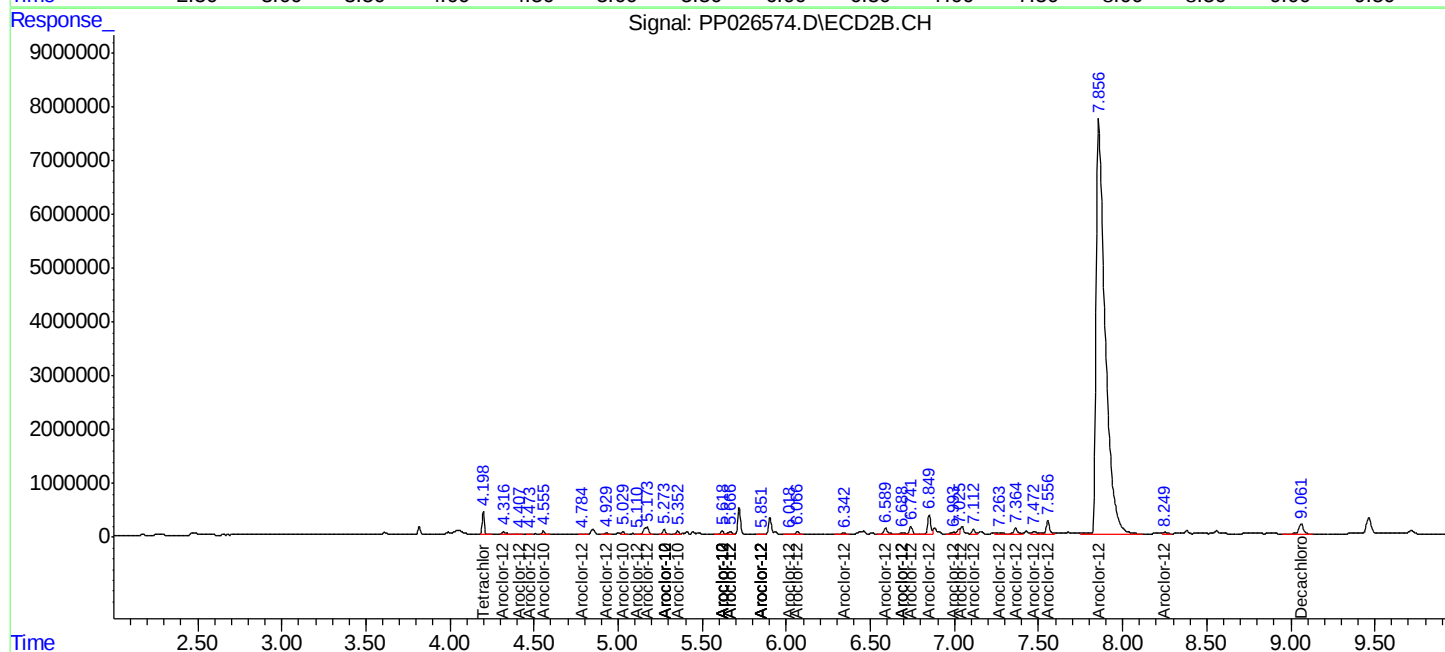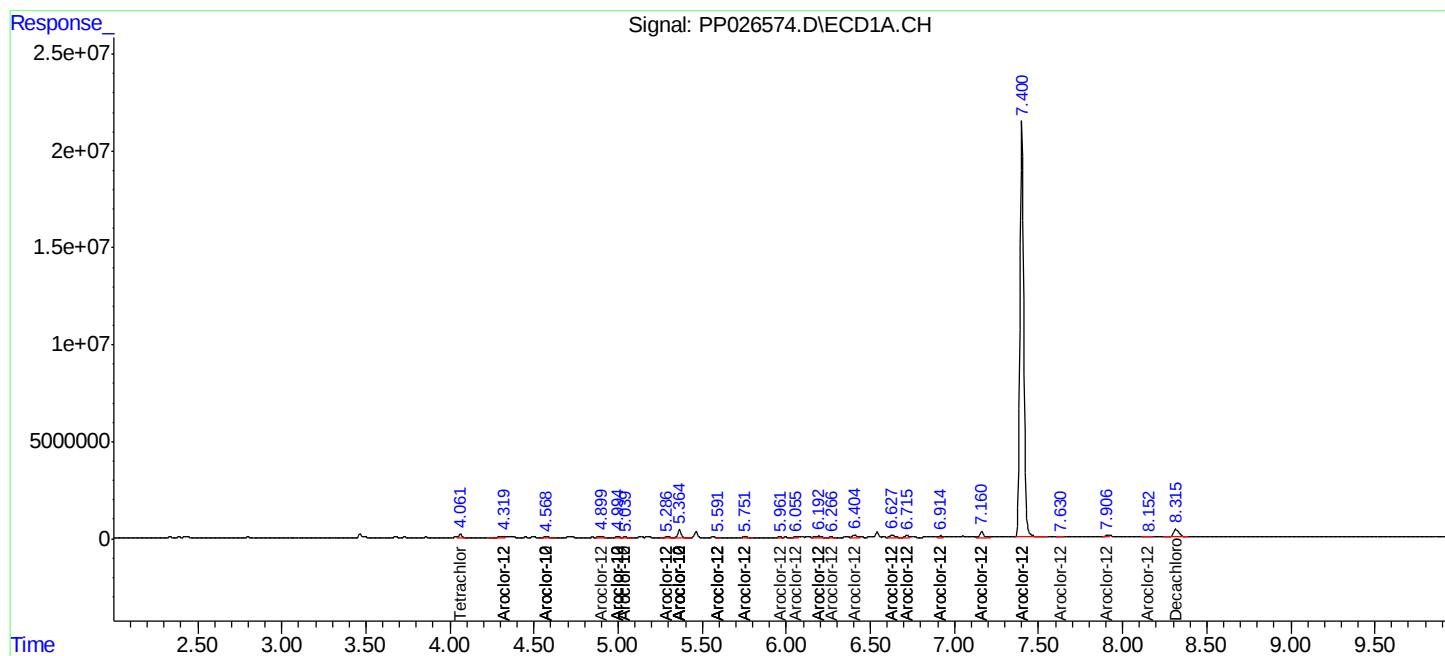


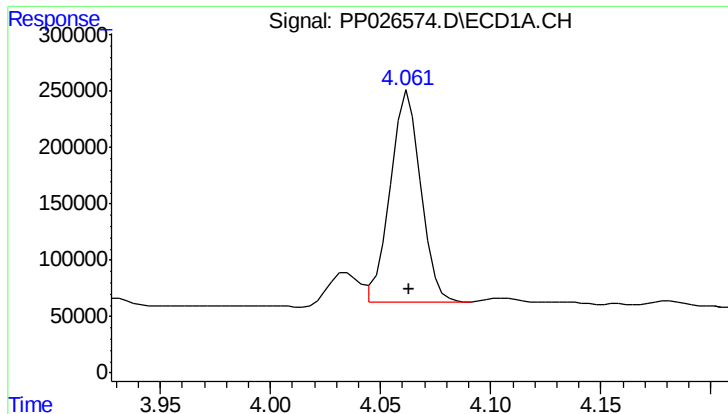

#1 Tetrachloro-m-xylene


R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1802422
Conc: 19.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

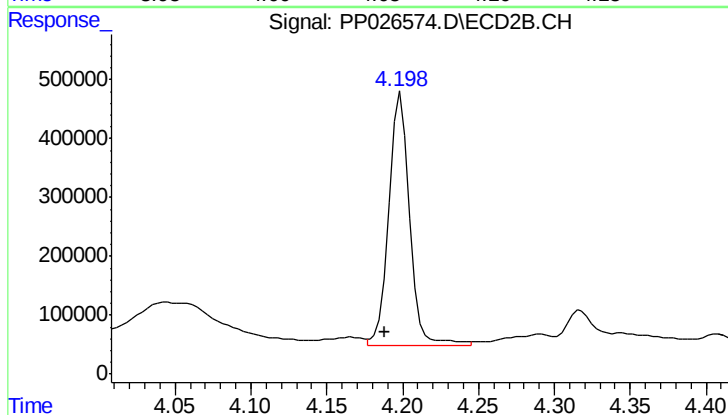


#1 Tetrachloro-m-xylene

R.T.: 4.199 min
Delta R.T.: 0.011 min
Response: 4050881
Conc: 17.67 ng/ml

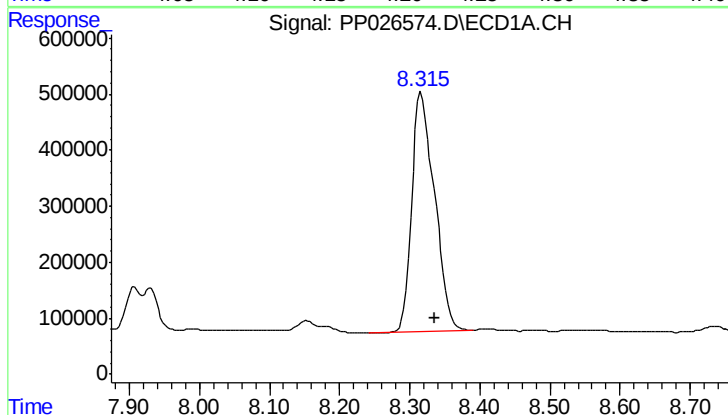


#2 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.019 min
Response: 9532528
Conc: 63.12 ng/ml

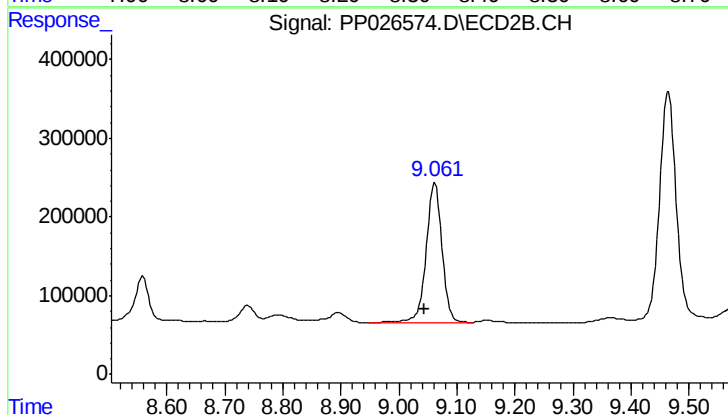

#2 Decachlorobiphenyl


R.T.: 9.063 min
Delta R.T.: 0.019 min
Response: 3418720
Conc: 21.29 ng/ml

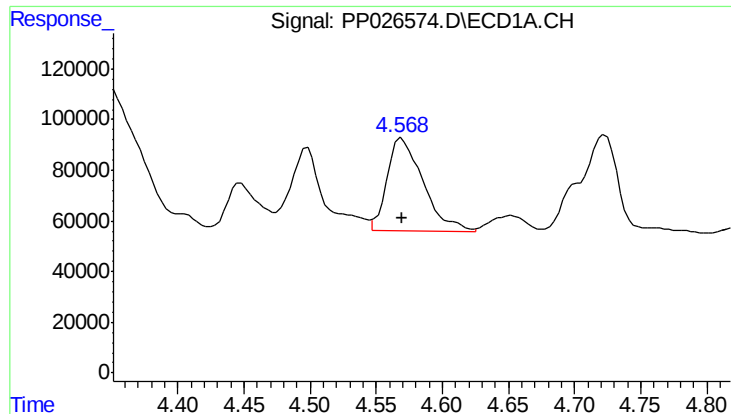

#3 Aroclor-1016-1


R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 689550
Conc: 301.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

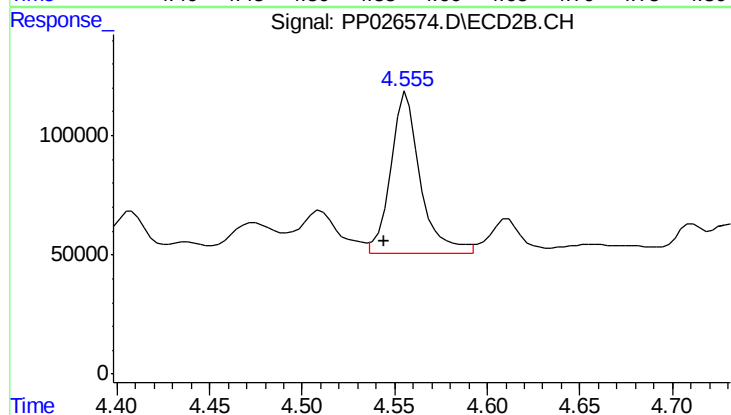


#3 Aroclor-1016-1

R.T.: 4.557 min
Delta R.T.: 0.012 min
Response: 759014
Conc: 194.20 ng/ml

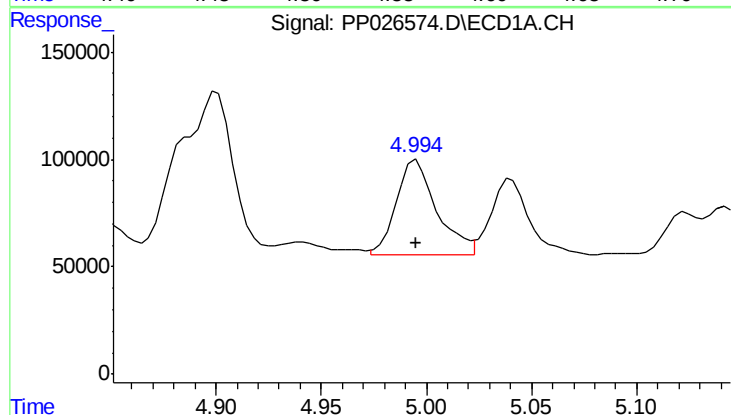


#4 Aroclor-1016-2

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 595579
Conc: 224.84 ng/ml

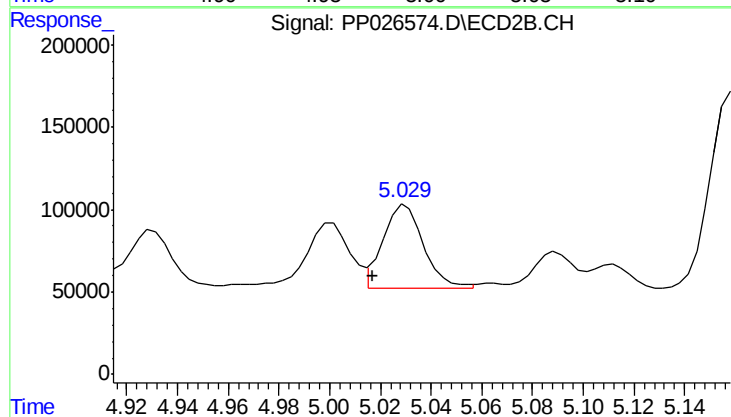

#4 Aroclor-1016-2


R.T.: 5.030 min
Delta R.T.: 0.013 min
Response: 568909
Conc: 196.24 ng/ml

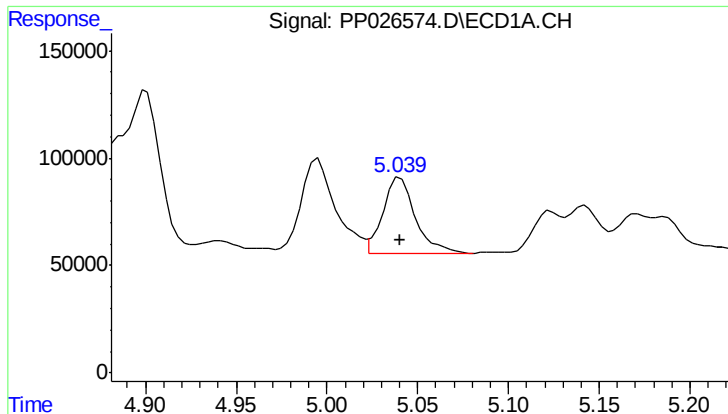

#5 Aroclor-1016-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 443678
Conc: 244.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

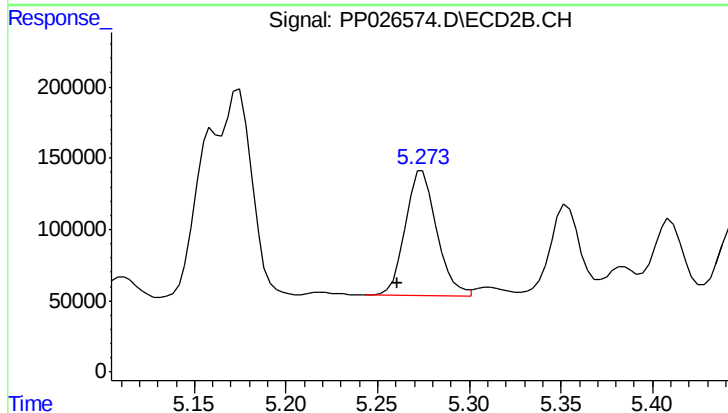


#5 Aroclor-1016-3

R.T.: 5.275 min
Delta R.T.: 0.014 min
Response: 1029121
Conc: 175.31 ng/ml

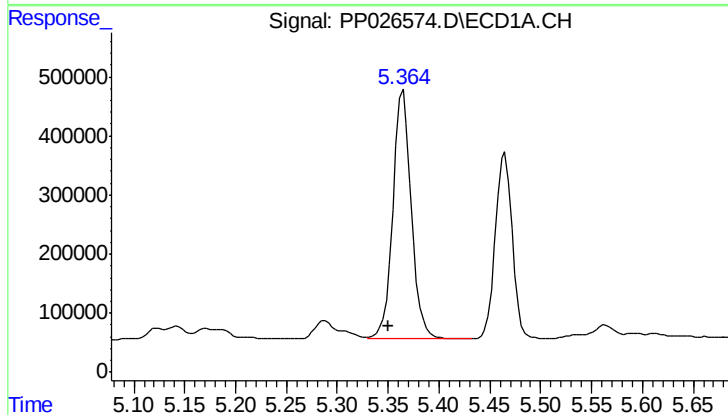


#6 Aroclor-1016-4

R.T.: 5.365 min
Delta R.T.: 0.015 min
Response: 5329305
Conc: 4351.93 ng/ml

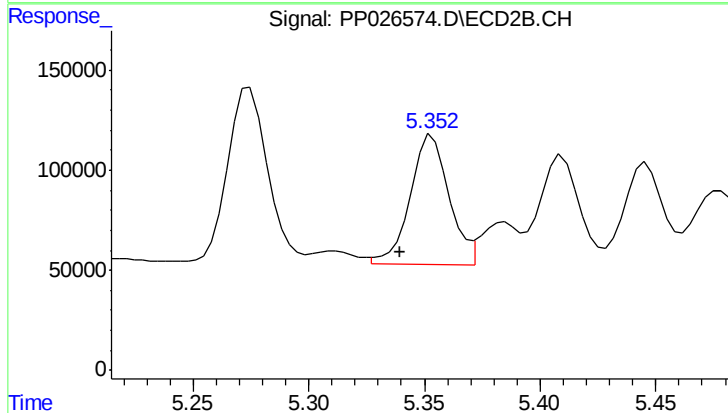

#6 Aroclor-1016-4


R.T.: 5.353 min
Delta R.T.: 0.014 min
Response: 754238
Conc: 198.51 ng/ml

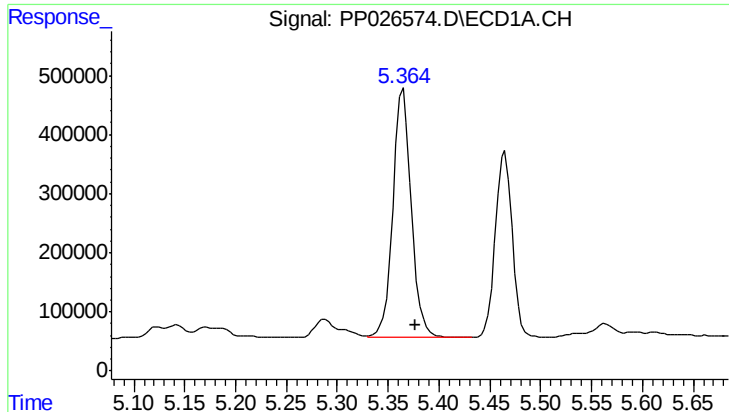

#7 Aroclor-1016-5


R.T.: 5.365 min
Delta R.T.: -0.012 min
Response: 5329305
Conc: 3505.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

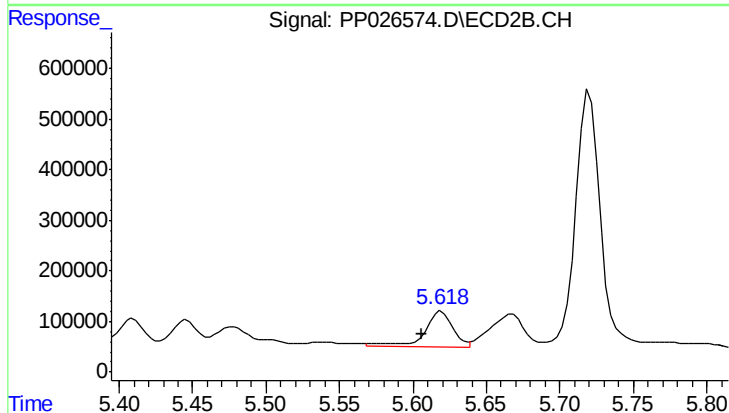


#7 Aroclor-1016-5

R.T.: 5.619 min
Delta R.T.: 0.014 min
Response: 958821
Conc: 239.80 ng/ml

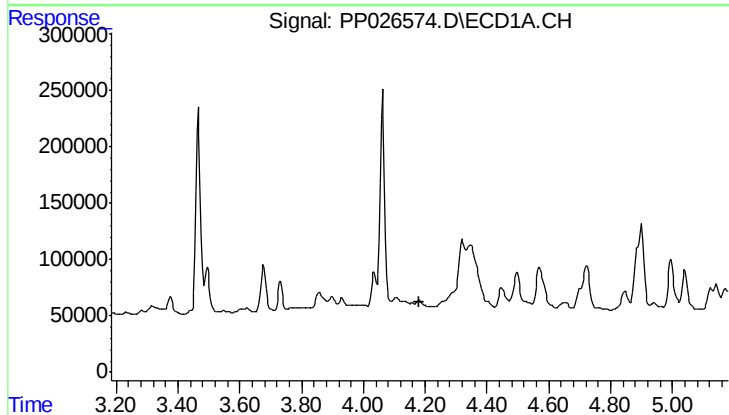


#8 Aroclor-1221-1

R.T.: 0.000 min
Exp R.T.: 4.182 min
Response: 0
Conc: N.D.

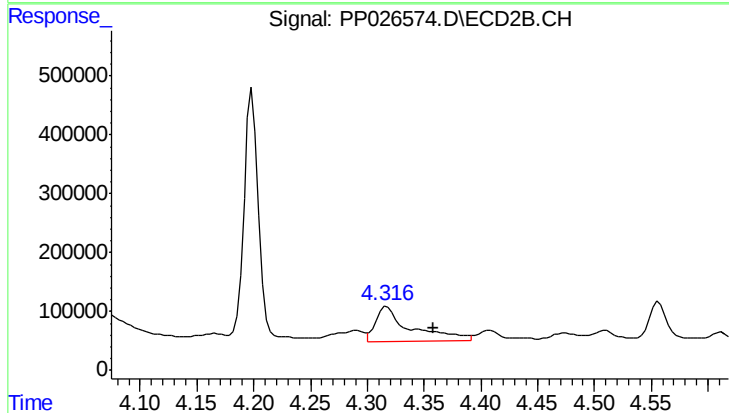

#8 Aroclor-1221-1


R.T.: 4.317 min
Delta R.T.: -0.041 min
Response: 1284391
Conc: 1788.87 ng/ml

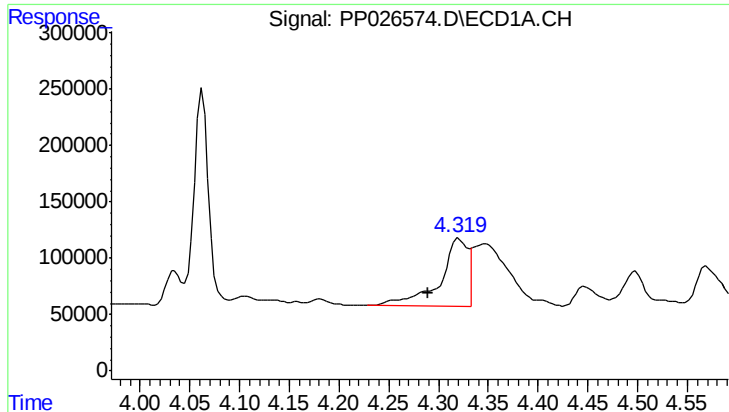

#9 Aroclor-1221-2


R.T.: 4.320 min
Delta R.T.: 0.030 min
Response: 1159646
Conc: 1248.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

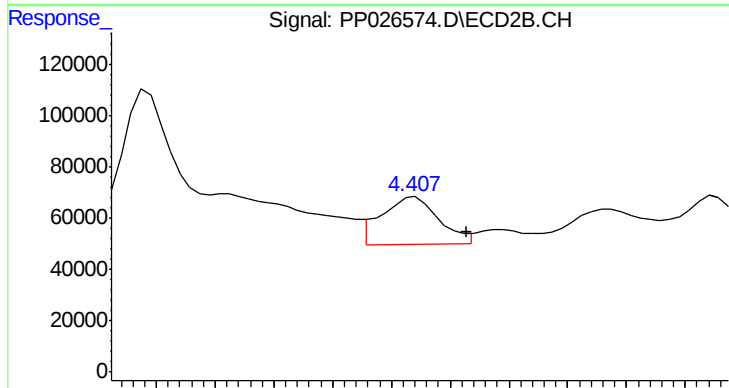


#9 Aroclor-1221-2

R.T.: 4.408 min
Delta R.T.: -0.018 min
Response: 250371
Conc: 792.43 ng/ml

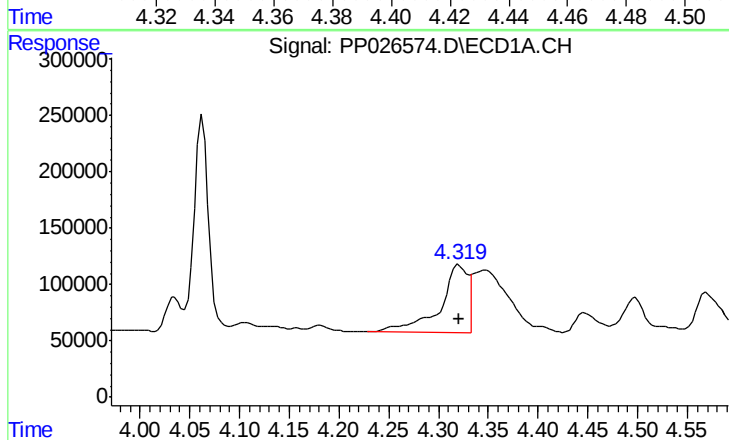


#10 Aroclor-1221-3

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 1159646
Conc: 332.61 ng/ml

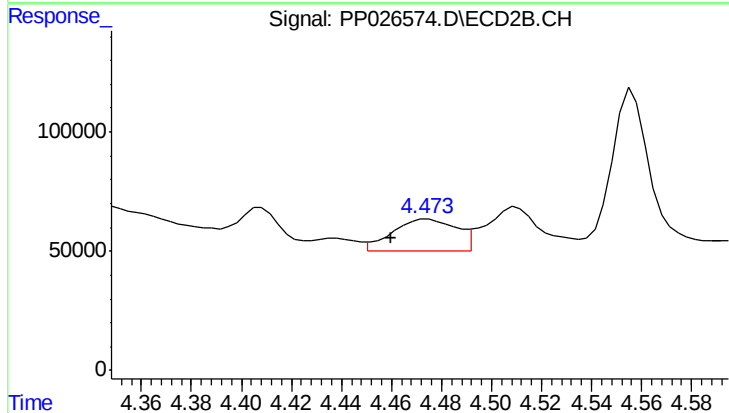

#10 Aroclor-1221-3


R.T.: 4.474 min
Delta R.T.: 0.014 min
Response: 235629
Conc: 291.38 ng/ml

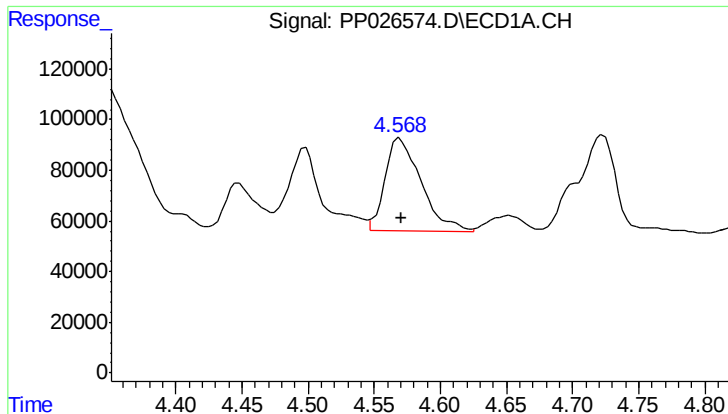

#11 Aroclor-1232-1


R.T.: 4.569 min
Delta R.T.: -0.001 min
Response: 689550
Conc: 280.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

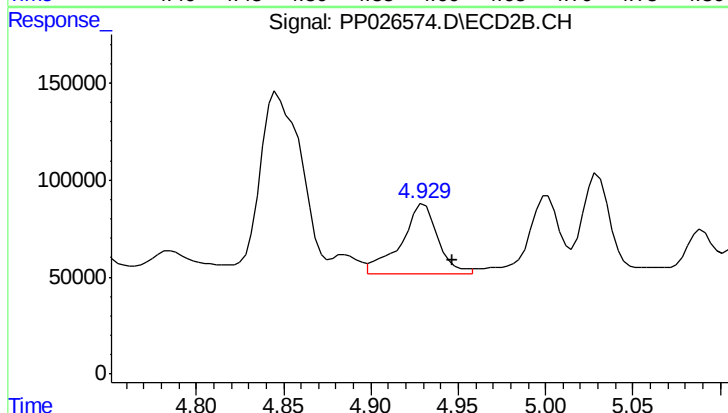


#11 Aroclor-1232-1

R.T.: 4.931 min
Delta R.T.: -0.016 min
Response: 521438
Conc: 247.76 ng/ml

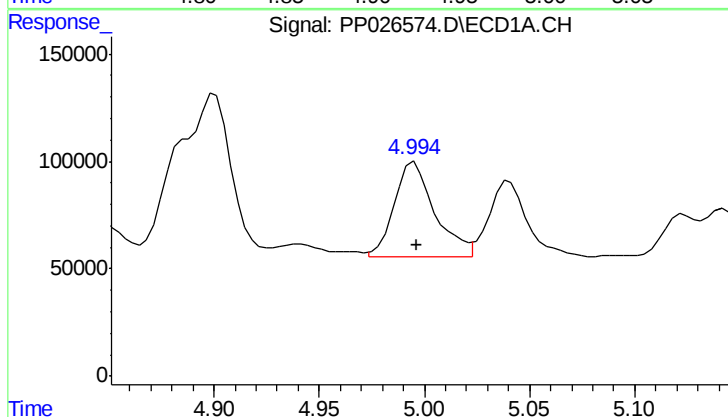


#12 Aroclor-1232-2

R.T.: 4.995 min
Delta R.T.: -0.001 min
Response: 595579
Conc: 216.71 ng/ml

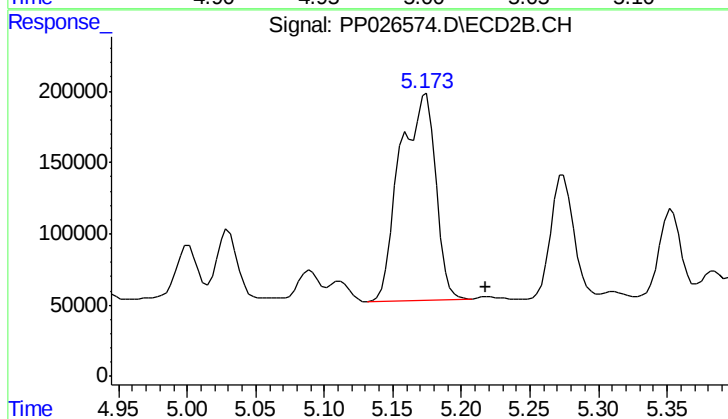

#12 Aroclor-1232-2


R.T.: 5.174 min
Delta R.T.: -0.044 min
Response: 2609248
Conc: 486.03 ng/ml

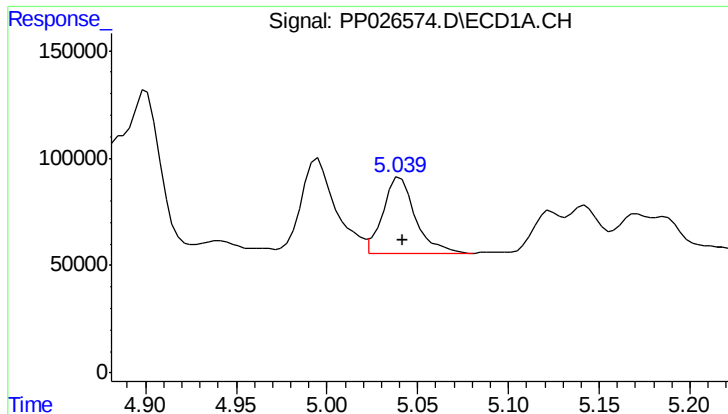

#13 Aroclor-1232-3


R.T.: 5.041 min
Delta R.T.: -0.001 min
Response: 443678
Conc: 229.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

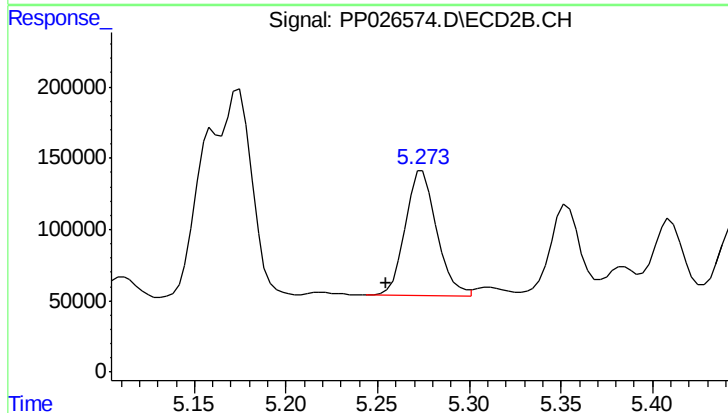


#13 Aroclor-1232-3

R.T.: 5.275 min
Delta R.T.: 0.020 min
Response: 1029121
Conc: 4468.07 ng/ml

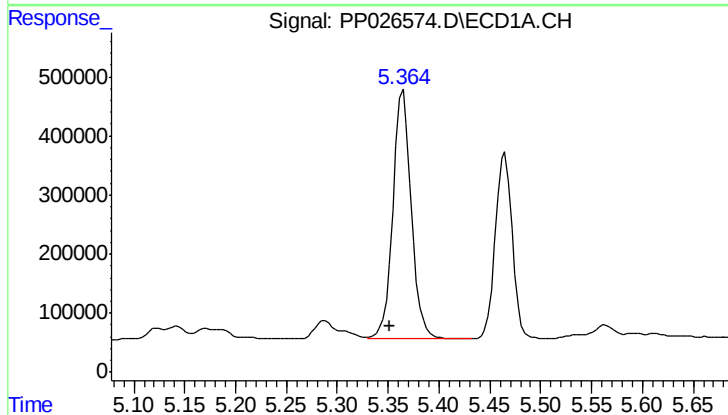


#14 Aroclor-1232-4

R.T.: 5.365 min
Delta R.T.: 0.014 min
Response: 5329305
Conc: 4143.02 ng/ml

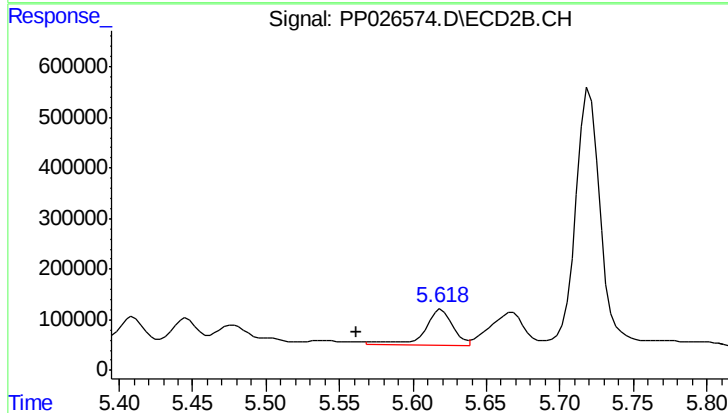

#14 Aroclor-1232-4


R.T.: 5.619 min
Delta R.T.: 0.057 min
Response: 958821
Conc: 245.62 ng/ml

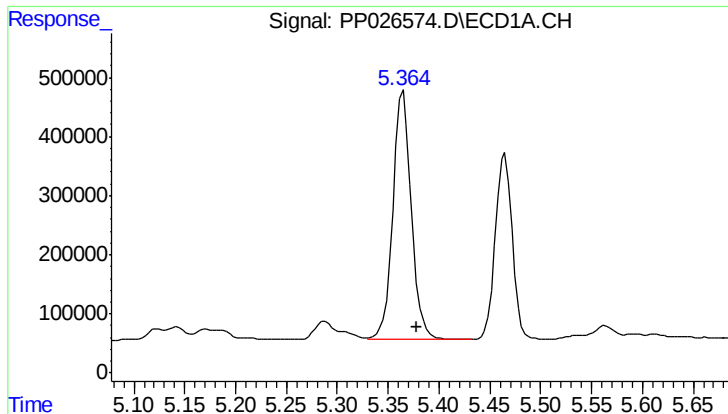

#15 Aroclor-1232-5


R.T.: 5.365 min
Delta R.T.: -0.013 min
Response: 5329305
Conc: 3539.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

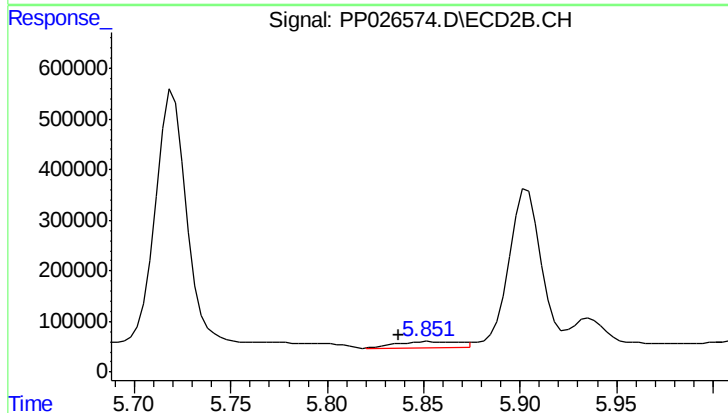


#15 Aroclor-1232-5

R.T.: 5.853 min
Delta R.T.: 0.016 min
Response: 278948
Conc: 186.13 ng/ml

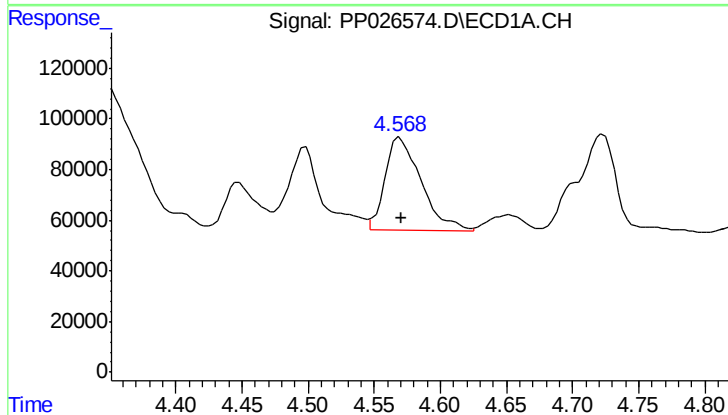


#16 Aroclor-1242-1

R.T.: 4.569 min
Delta R.T.: -0.001 min
Response: 689550
Conc: 280.74 ng/ml

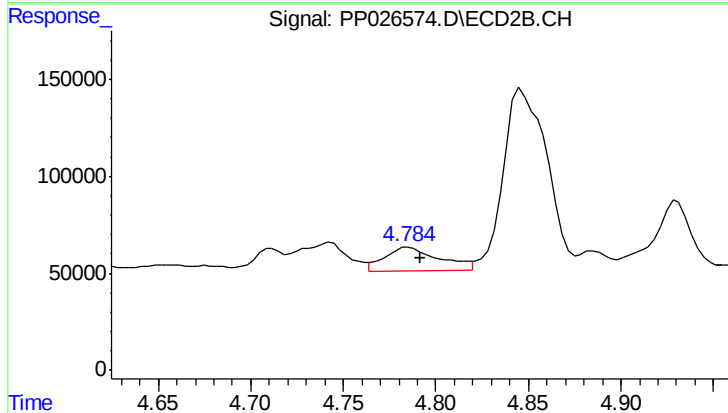

#16 Aroclor-1242-1


R.T.: 4.786 min
Delta R.T.: -0.006 min
Response: 254356
Conc: 36.18 ng/ml

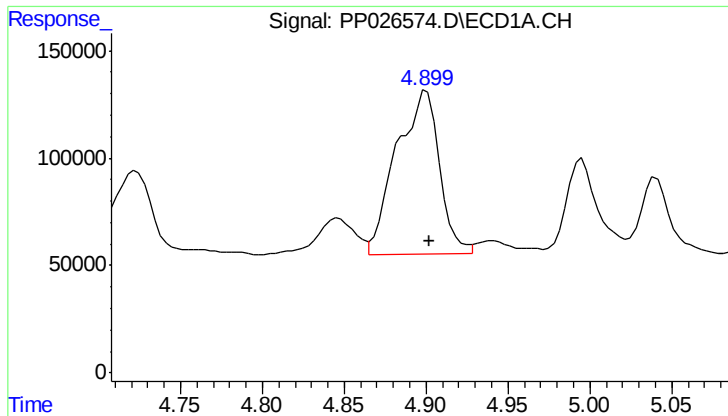

#17 Aroclor-1242-2


R.T.: 4.900 min
Delta R.T.: -0.001 min
Response: 1396434
Conc: 233.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

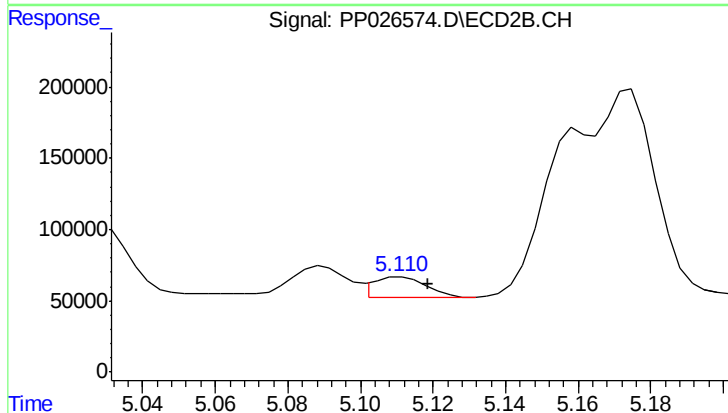


#17 Aroclor-1242-2

R.T.: 5.112 min
Delta R.T.: -0.007 min
Response: 143986
Conc: 10.26 ng/ml

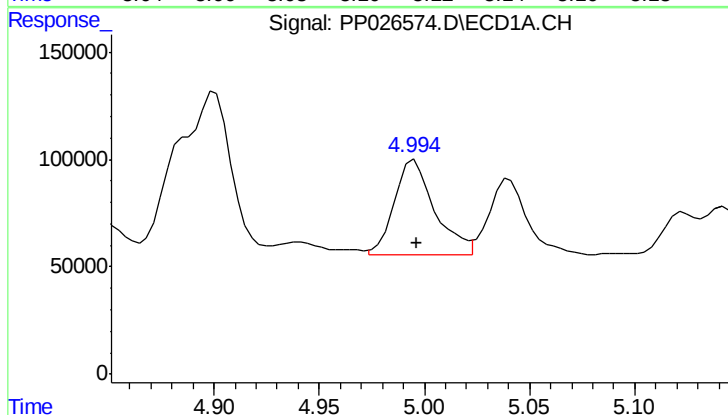


#18 Aroclor-1242-3

R.T.: 4.995 min
Delta R.T.: -0.001 min
Response: 595579
Conc: 216.71 ng/ml

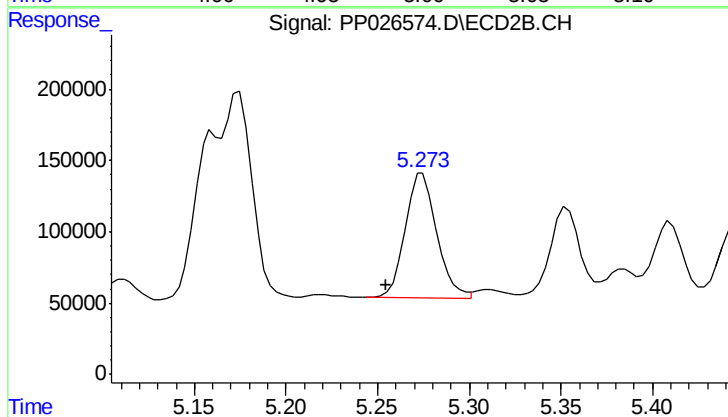

#18 Aroclor-1242-3


R.T.: 5.275 min
Delta R.T.: 0.020 min
Response: 1029121
Conc: 4468.07 ng/ml

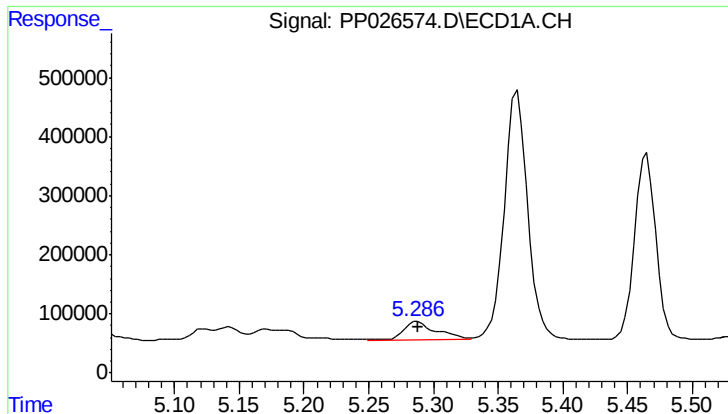

#19 Aroclor-1242-4


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 538486
Conc: 222.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

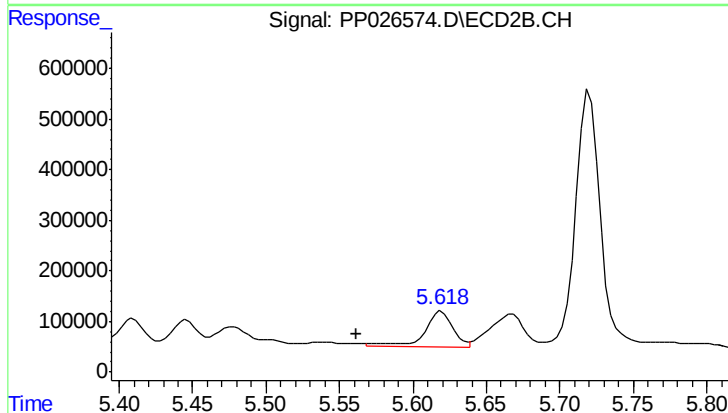


#19 Aroclor-1242-4

R.T.: 5.619 min
Delta R.T.: 0.057 min
Response: 958821
Conc: 245.62 ng/ml

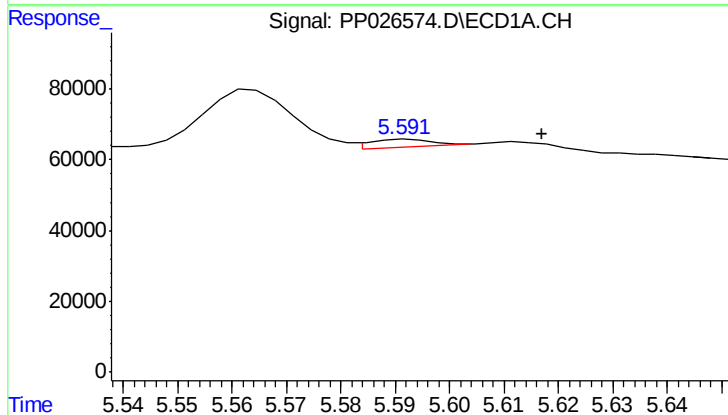


#20 Aroclor-1242-5

R.T.: 5.592 min
Delta R.T.: -0.025 min
Response: 16888
Conc: 29.34 ng/ml

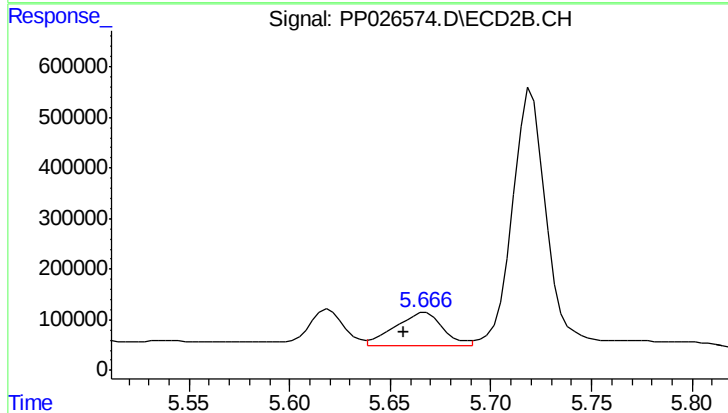

#20 Aroclor-1242-5


R.T.: 5.668 min
Delta R.T.: 0.011 min
Response: 1069783
Conc: 278.02 ng/ml

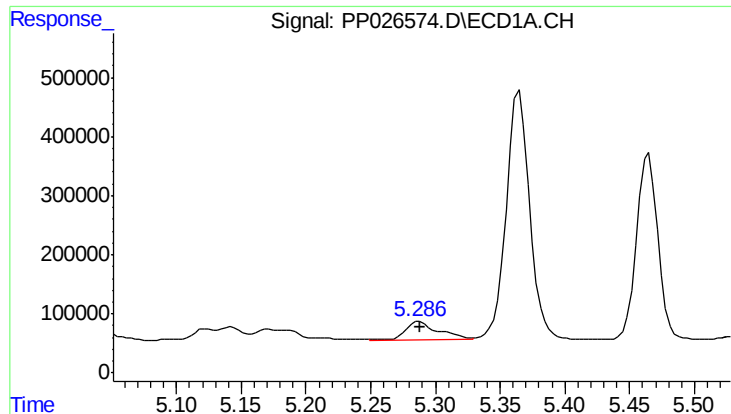

#21 Aroclor-1248-1


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 538486
Conc: 222.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

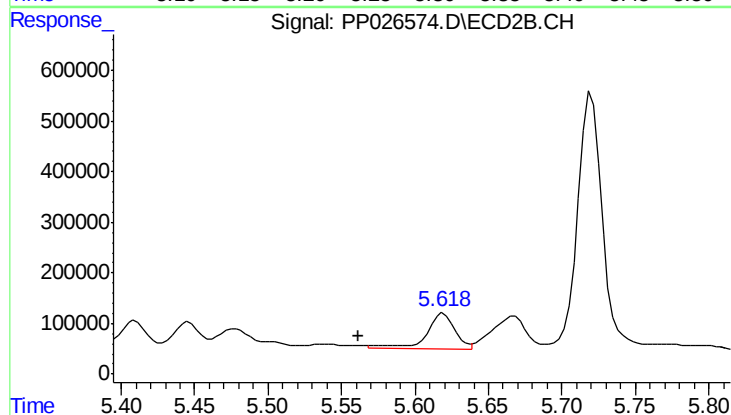


#21 Aroclor-1248-1

R.T.: 5.619 min
Delta R.T.: 0.057 min
Response: 958821
Conc: 245.62 ng/ml

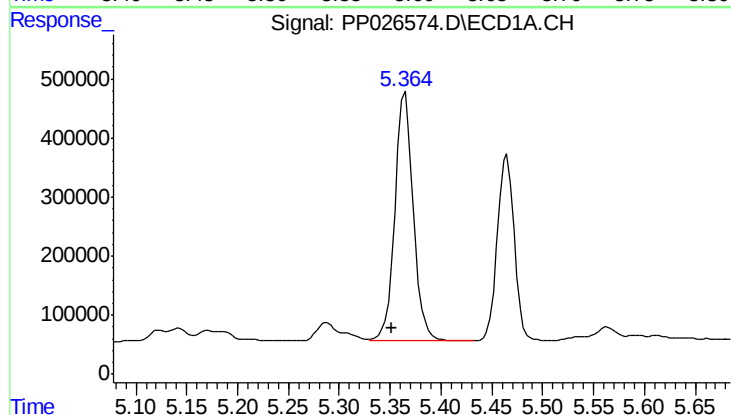


#22 Aroclor-1248-2

R.T.: 5.365 min
Delta R.T.: 0.014 min
Response: 5329305
Conc: 4143.02 ng/ml

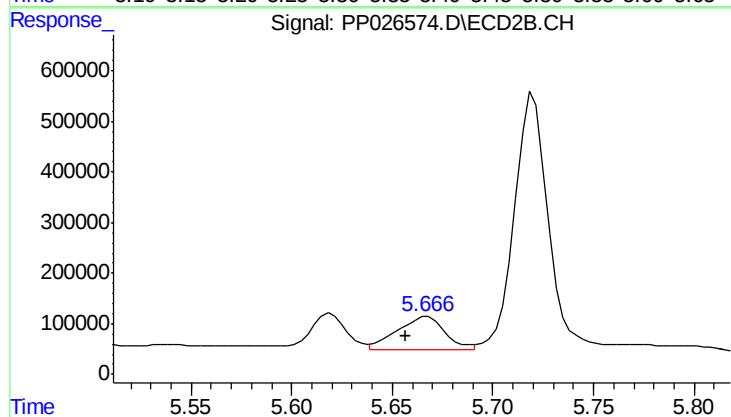

#22 Aroclor-1248-2


R.T.: 5.668 min
Delta R.T.: 0.011 min
Response: 1069783
Conc: 278.02 ng/ml

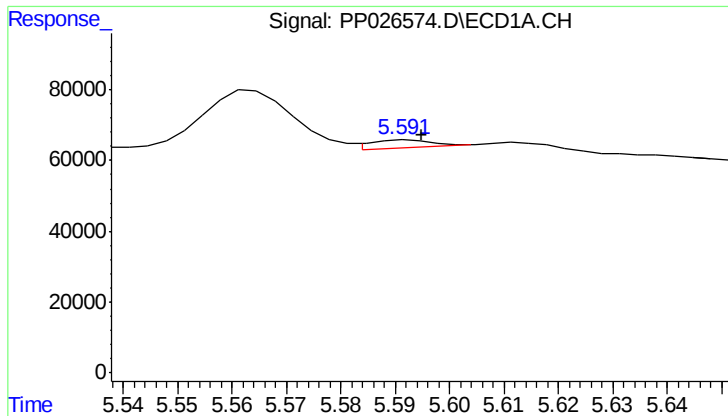

#23 Aroclor-1248-3


R.T.: 5.592 min
Delta R.T.: -0.003 min
Response: 16888
Conc: 24.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

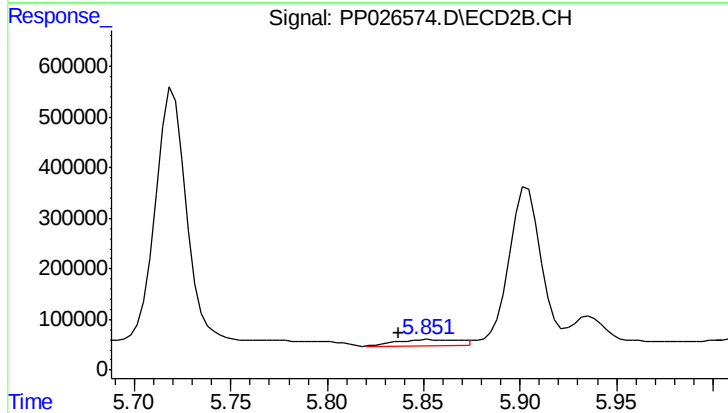


#23 Aroclor-1248-3

R.T.: 5.853 min
Delta R.T.: 0.016 min
Response: 278948
Conc: 186.13 ng/ml

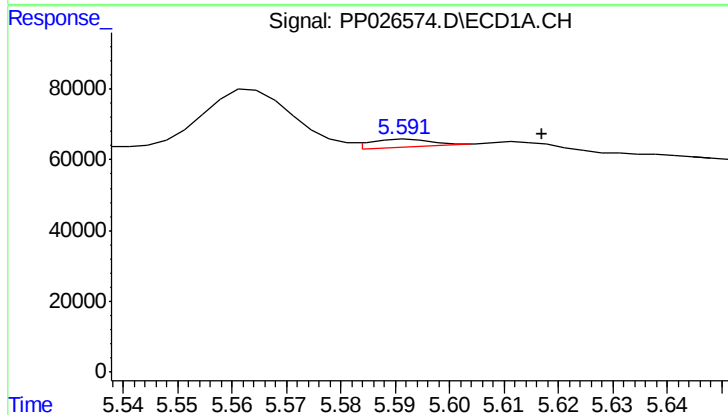


#24 Aroclor-1248-4

R.T.: 5.592 min
Delta R.T.: -0.025 min
Response: 16888
Conc: 29.34 ng/ml

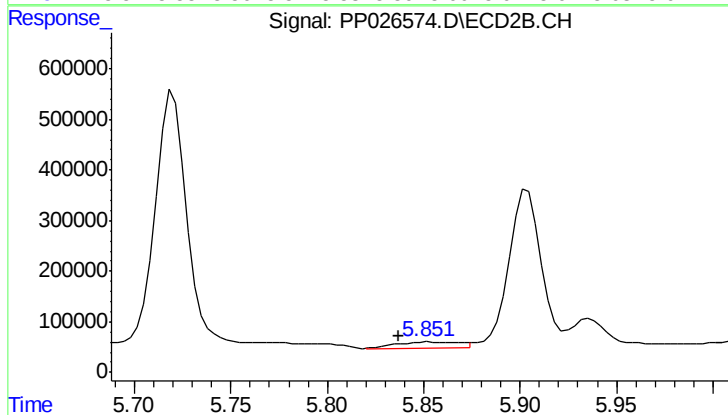

#24 Aroclor-1248-4


R.T.: 5.853 min
Delta R.T.: 0.016 min
Response: 278948
Conc: 186.13 ng/ml

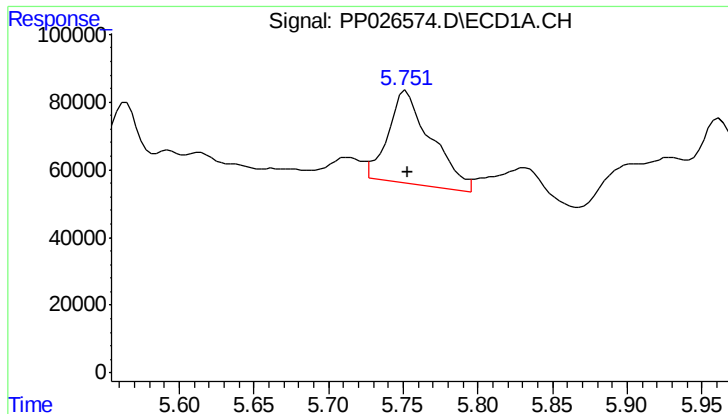

#25 Aroclor-1248-5


R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 560246
Conc: 378.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

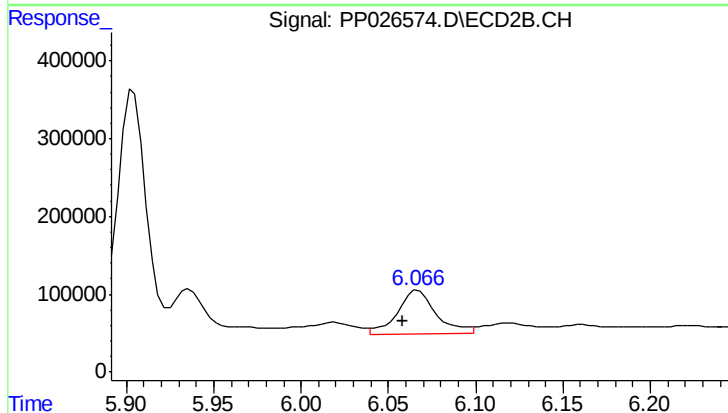


#25 Aroclor-1248-5

R.T.: 6.067 min
Delta R.T.: 0.009 min
Response: 862800
Conc: 2502.40 ng/ml

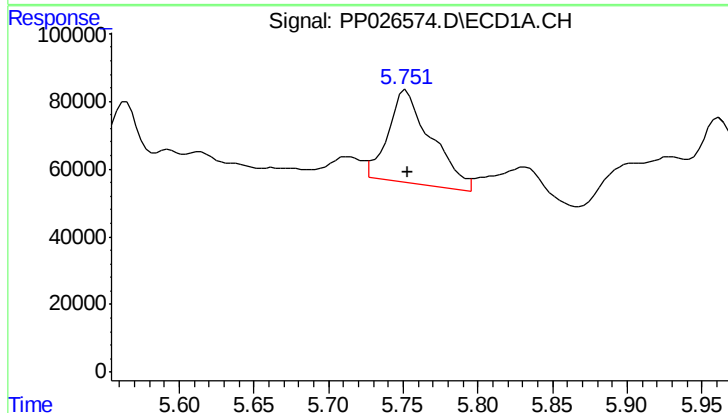


#26 Aroclor-1254-1

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 560246
Conc: 378.13 ng/ml

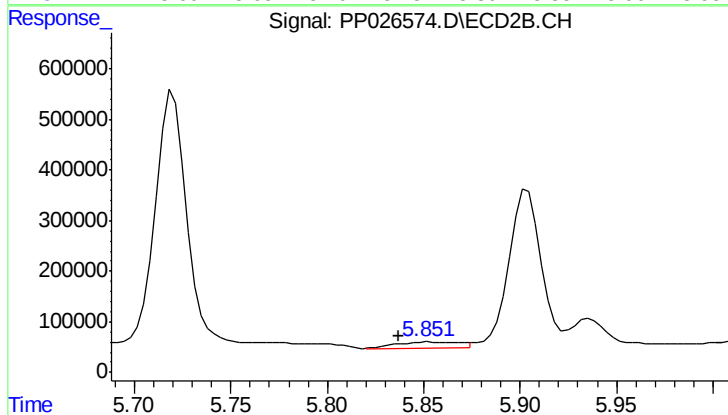

#26 Aroclor-1254-1


R.T.: 5.853 min
Delta R.T.: 0.016 min
Response: 278948
Conc: 186.13 ng/ml

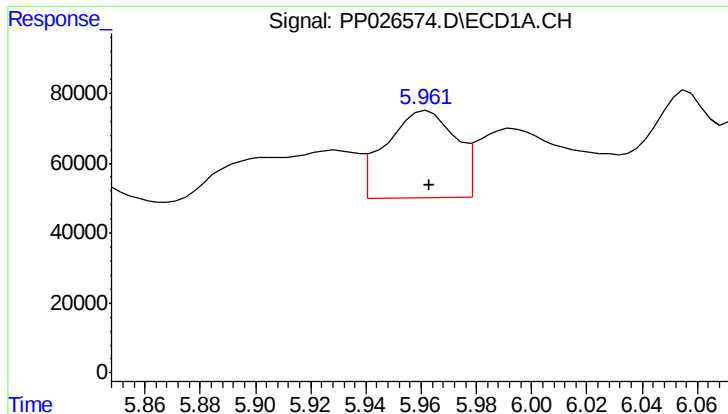

#27 Aroclor-1254-2


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 433768
Conc: 415.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

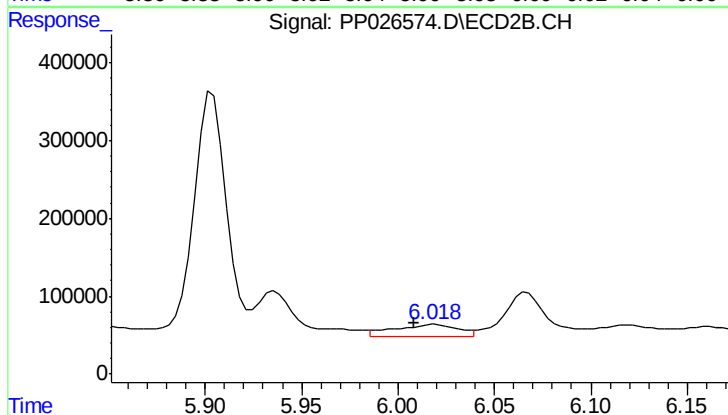


#27 Aroclor-1254-2

R.T.: 6.019 min
Delta R.T.: 0.011 min
Response: 352028
Conc: 138.15 ng/ml

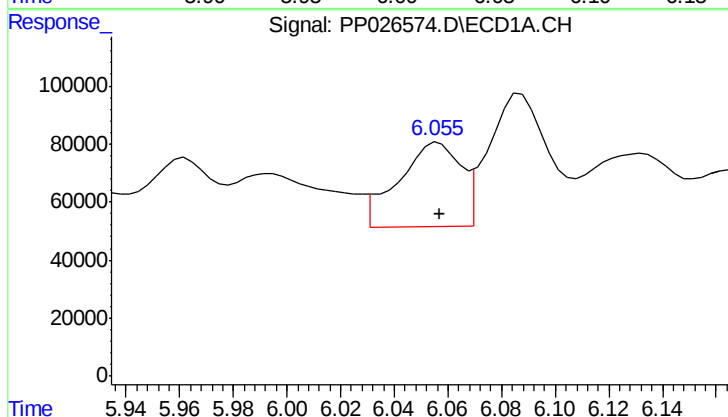


#28 Aroclor-1254-3

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 474505
Conc: 589.44 ng/ml

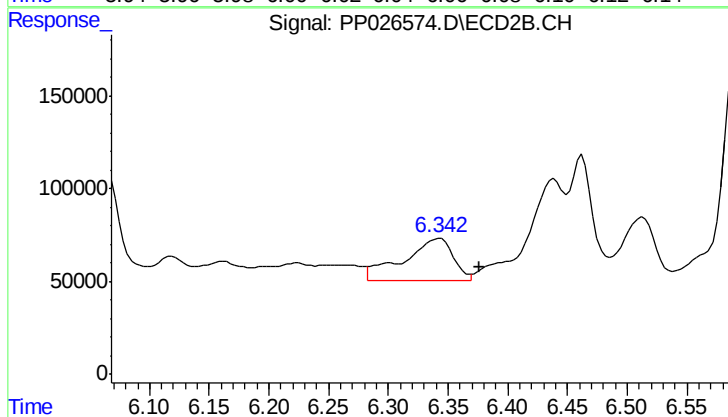

#28 Aroclor-1254-3


R.T.: 6.343 min
Delta R.T.: -0.033 min
Response: 658807
Conc: 290.31 ng/ml

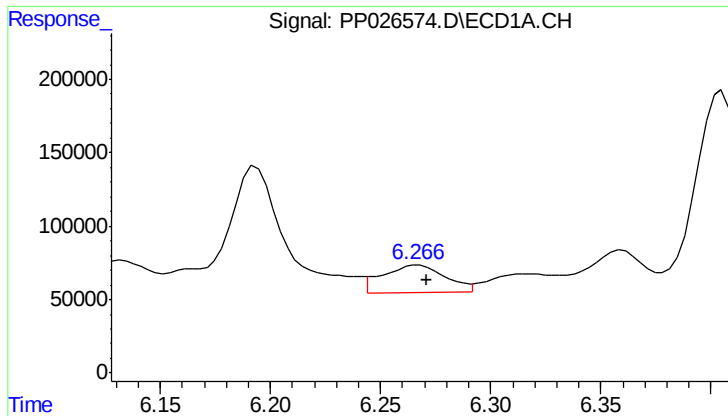

#29 Aroclor-1254-4


R.T.: 6.267 min
Delta R.T.: -0.004 min
Response: 379476
Conc: 633.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

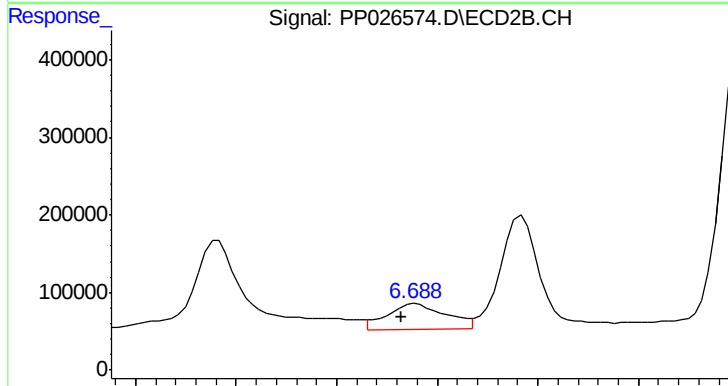


#29 Aroclor-1254-4

R.T.: 6.689 min
Delta R.T.: 0.007 min
Response: 662042
Conc: 80.86 ng/ml

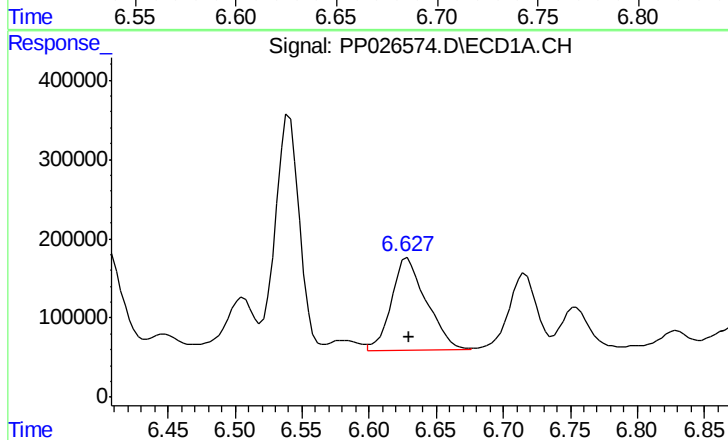


#30 Aroclor-1254-5

R.T.: 6.629 min
Delta R.T.: -0.001 min
Response: 2117676
Conc: 233.00 ng/ml

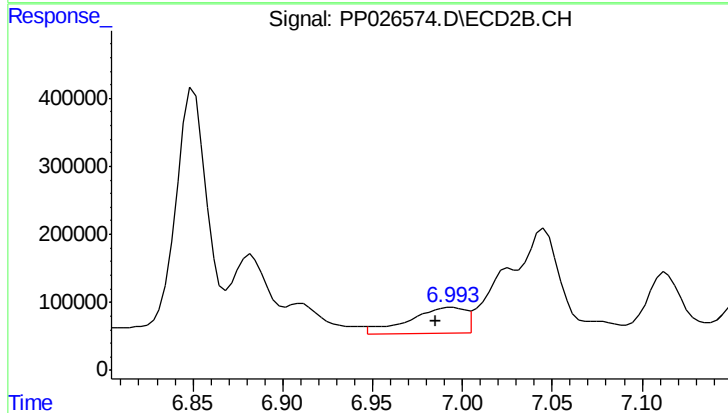

#30 Aroclor-1254-5


R.T.: 6.994 min
Delta R.T.: 0.009 min
Response: 830498
Conc: 72.77 ng/ml

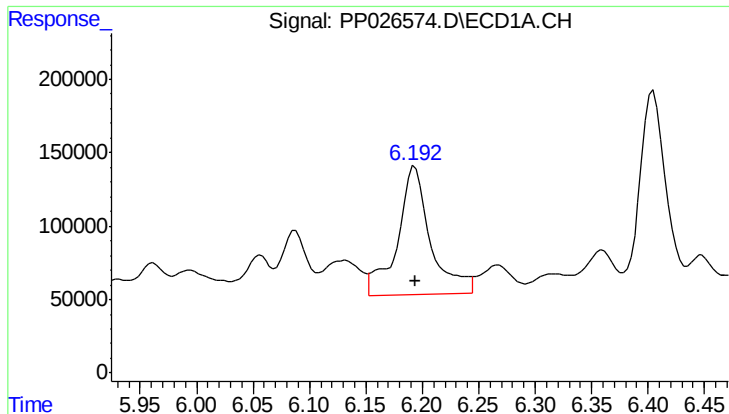

#31 Aroclor-1260-1


R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 1765651
Conc: 481.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

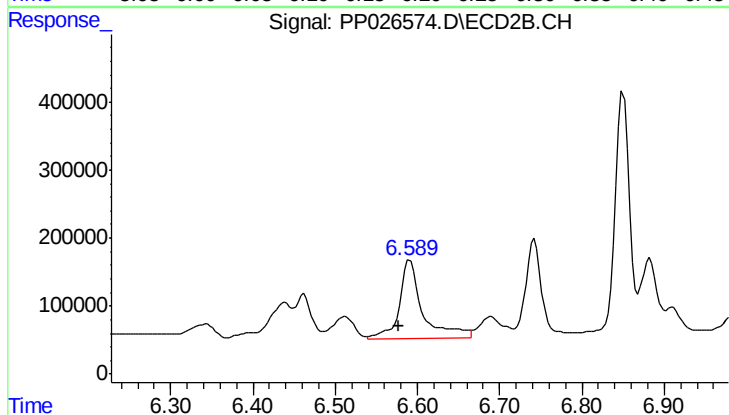


#31 Aroclor-1260-1

R.T.: 6.591 min
Delta R.T.: 0.014 min
Response: 2293955
Conc: 286.94 ng/ml

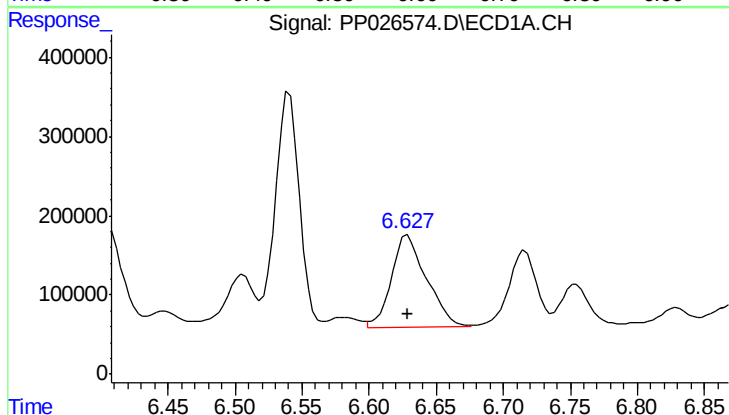


#32 Aroclor-1260-2

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 2117676
Conc: 225.26 ng/ml

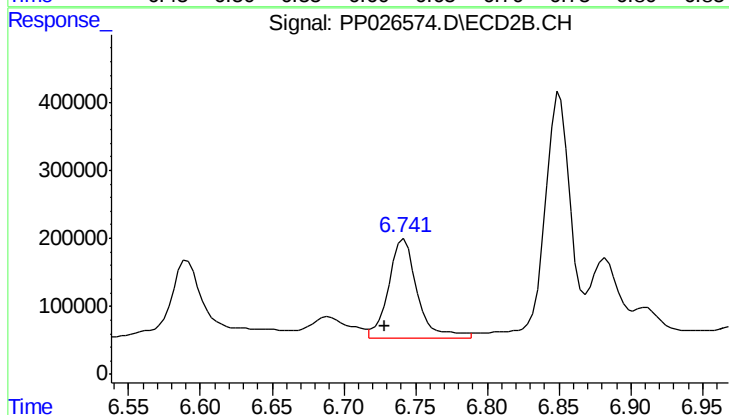

#32 Aroclor-1260-2


R.T.: 6.742 min
Delta R.T.: 0.014 min
Response: 2065167
Conc: 228.39 ng/ml

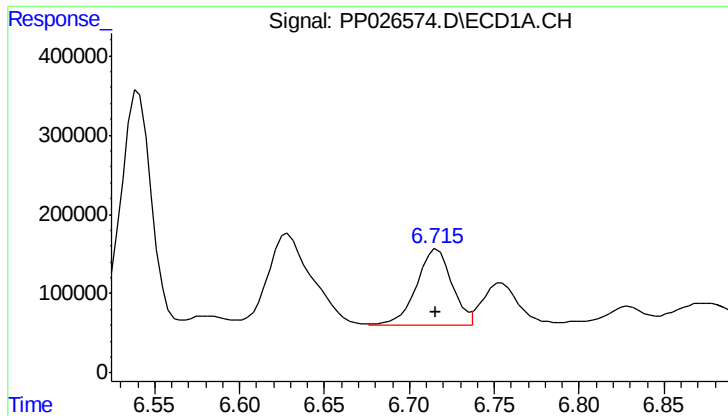

#33 Aroclor-1260-3


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 1376547
Conc: 204.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

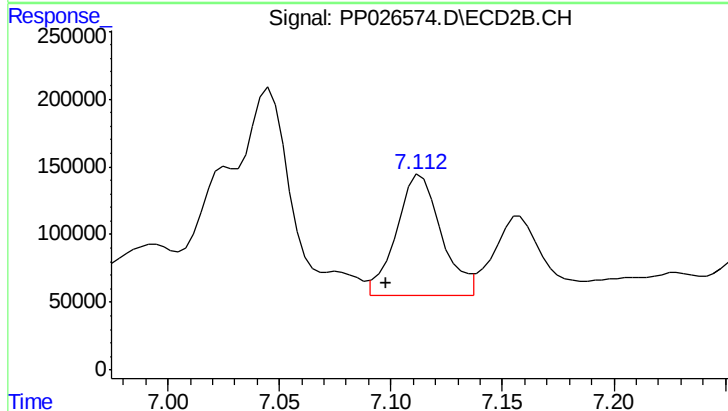


#33 Aroclor-1260-3

R.T.: 7.113 min
Delta R.T.: 0.016 min
Response: 1250770
Conc: 195.70 ng/ml

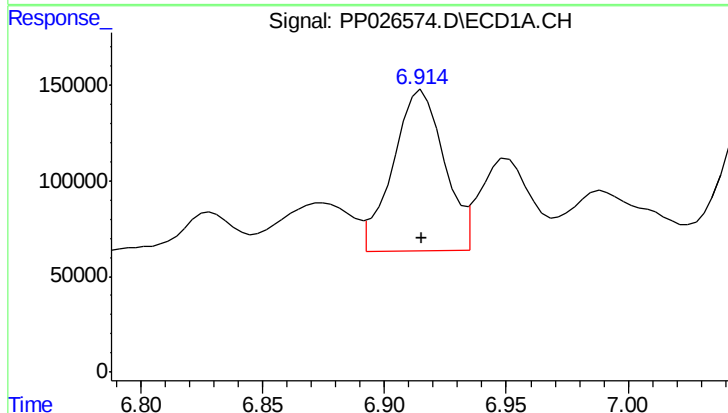


#34 Aroclor-1260-4

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 1224434
Conc: 230.29 ng/ml

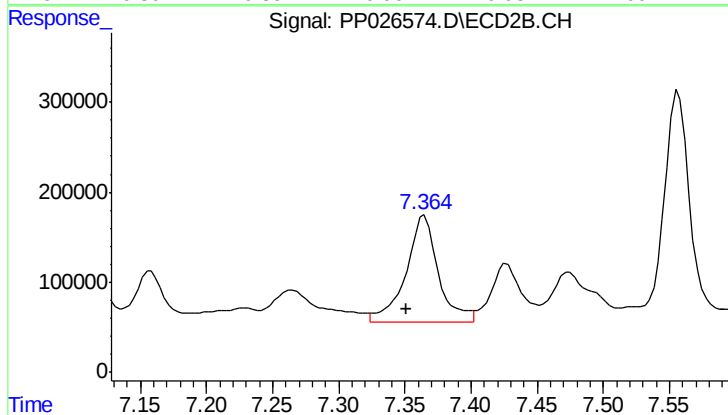

#34 Aroclor-1260-4


R.T.: 7.365 min
Delta R.T.: 0.014 min
Response: 2003351
Conc: 270.39 ng/ml

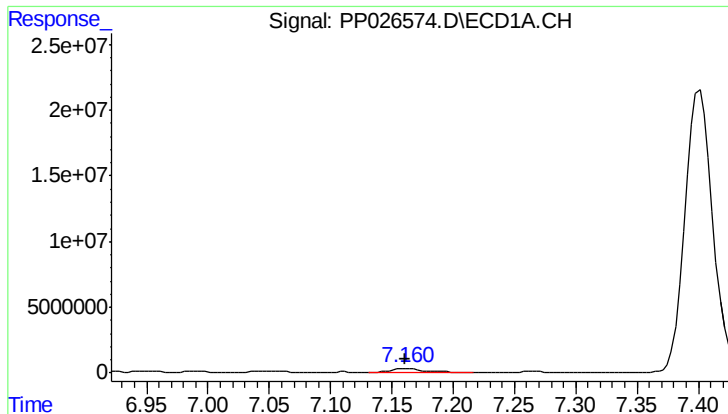

#35 Aroclor-1260-5


R.T.: 7.162 min
Delta R.T.: 0.001 min
Response: 4453739
Conc: 233.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

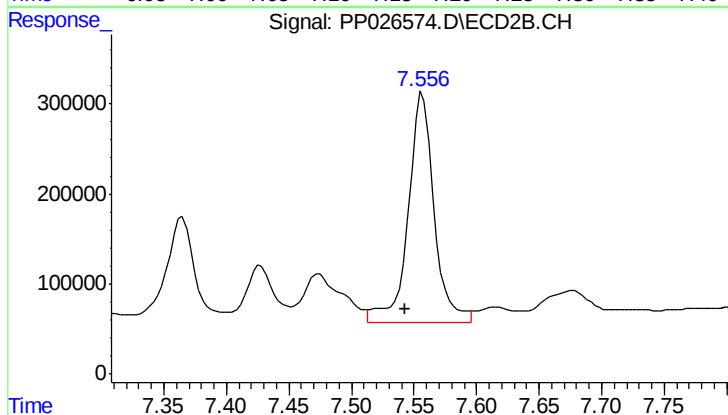


#35 Aroclor-1260-5

R.T.: 7.557 min
Delta R.T.: 0.014 min
Response: 3683514
Conc: 229.04 ng/ml

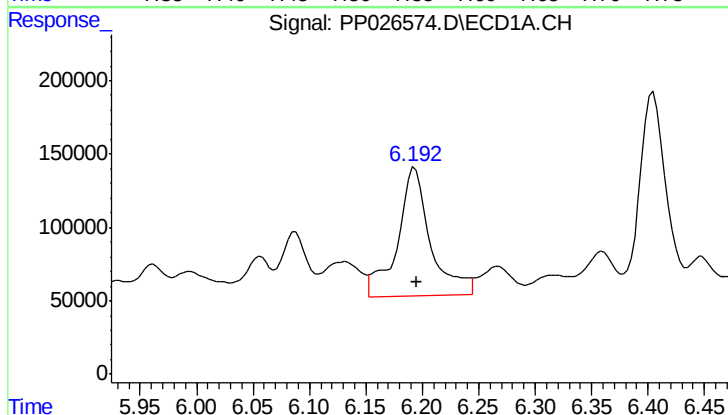


#36 Aroclor-1262-1

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 1765651
Conc: 501.43 ng/ml

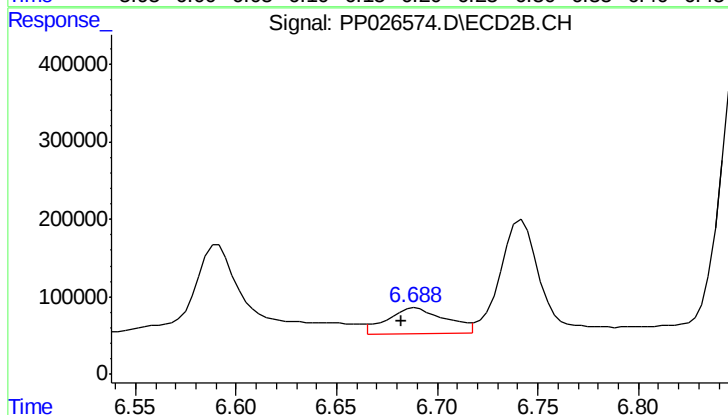

#36 Aroclor-1262-1


R.T.: 6.689 min
Delta R.T.: 0.007 min
Response: 662042
Conc: 80.86 ng/ml

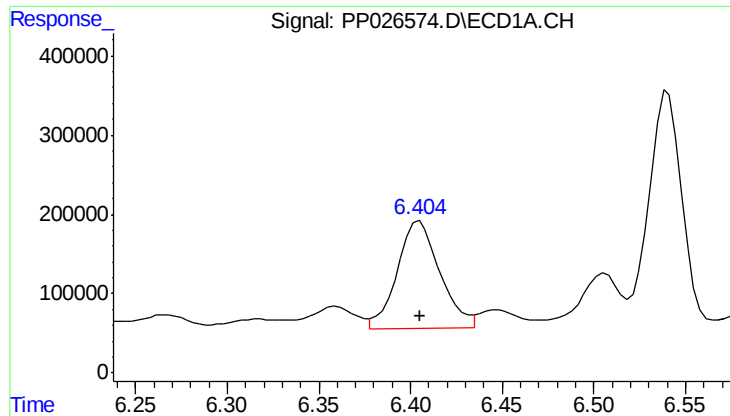

#37 Aroclor-1262-2


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 2186106
Conc: 270.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

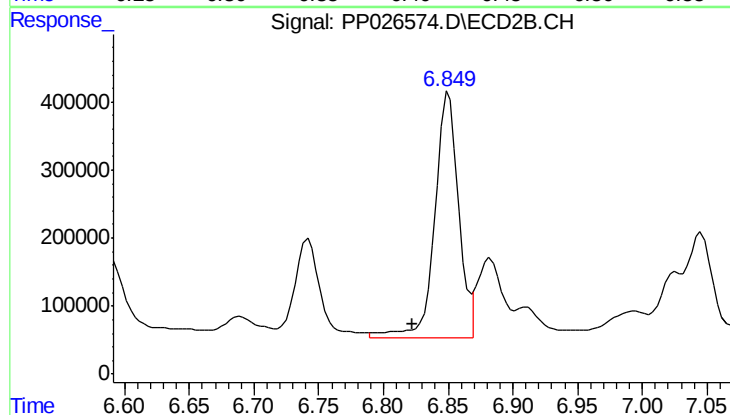


#37 Aroclor-1262-2

R.T.: 6.850 min
Delta R.T.: 0.028 min
Response: 4589756
Conc: 758.87 ng/ml

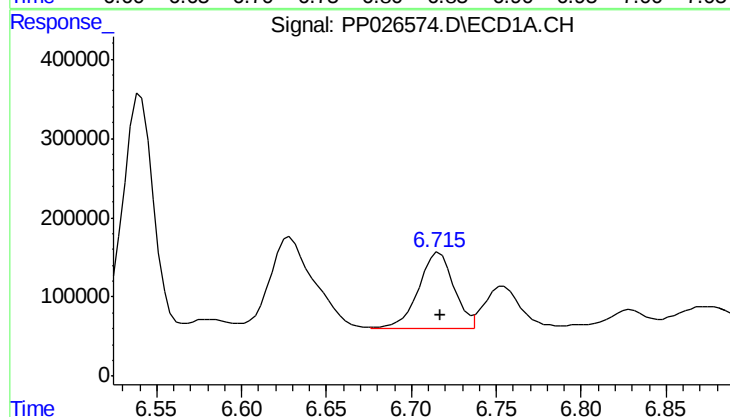


#38 Aroclor-1262-3

R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 1376547
Conc: 213.95 ng/ml

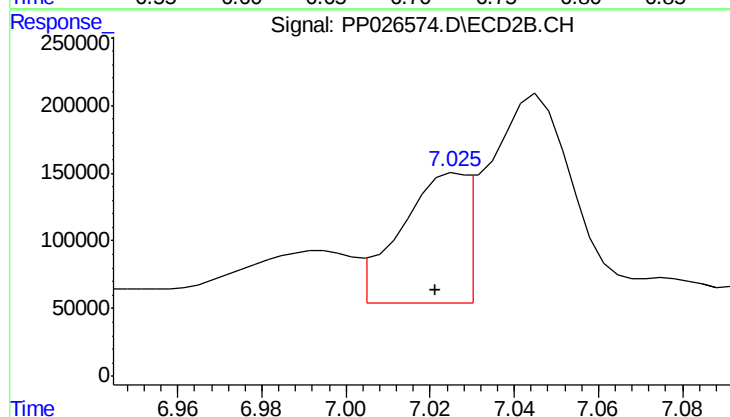

#38 Aroclor-1262-3


R.T.: 7.026 min
Delta R.T.: 0.005 min
Response: 1015108
Conc: 4710.44 ng/ml

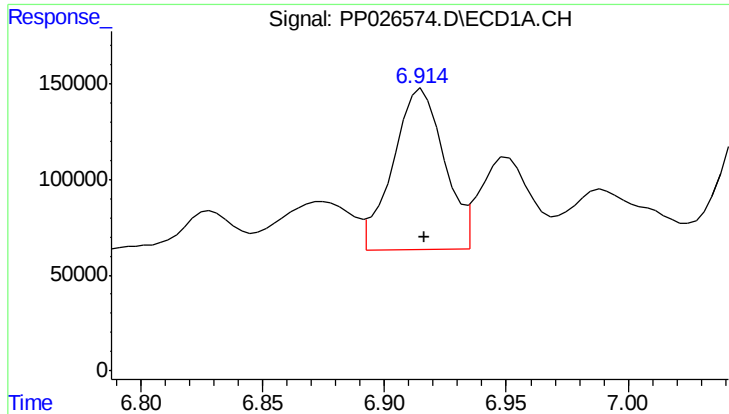

#39 Aroclor-1262-4


R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 1224434
Conc: 230.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

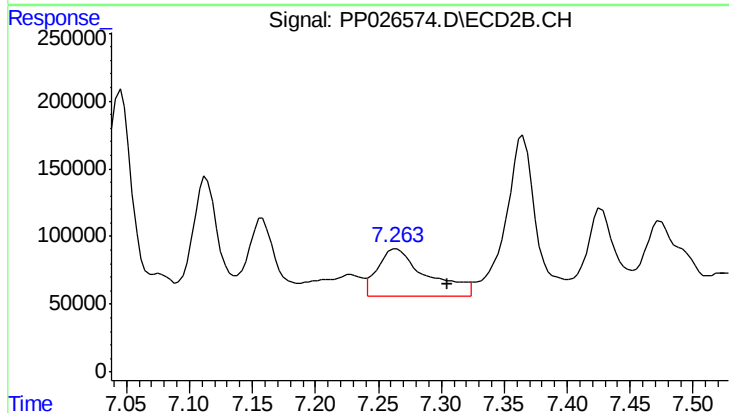


#39 Aroclor-1262-4

R.T.: 7.265 min
Delta R.T.: -0.040 min
Response: 950895
Conc: 144.65 ng/ml

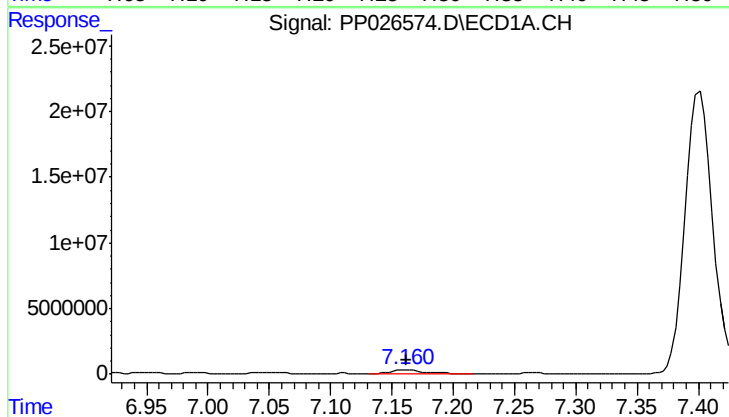


#40 Aroclor-1262-5

R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 4453739
Conc: 231.23 ng/ml

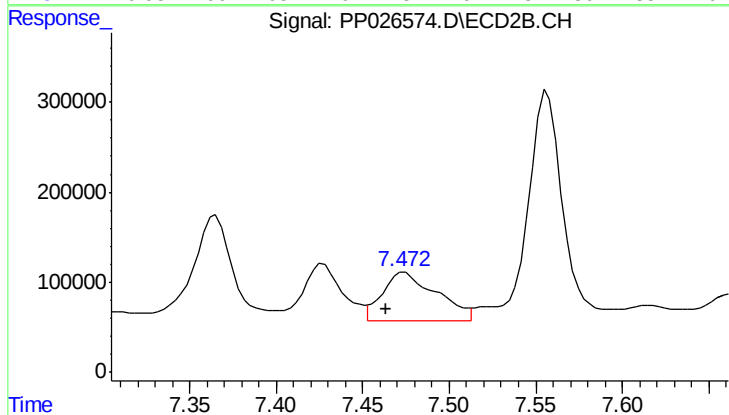

#40 Aroclor-1262-5


R.T.: 7.474 min
Delta R.T.: 0.011 min
Response: 1186488
Conc: 5236.00 ng/ml

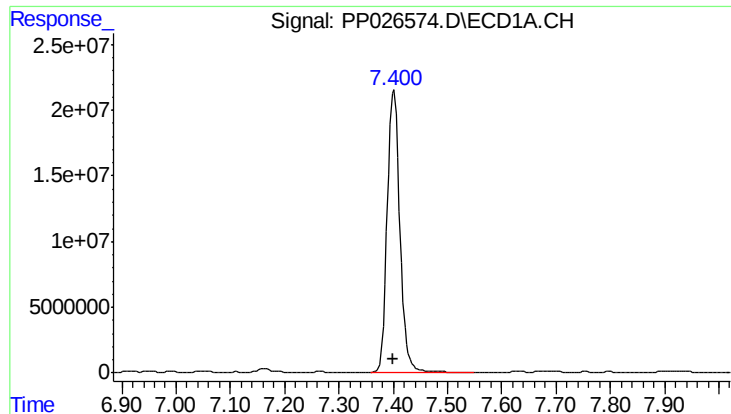

#41 Aroclor-1268-1


R.T.: 7.401 min
Delta R.T.: 0.002 min
Response: 345399268
Conc: 27580.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

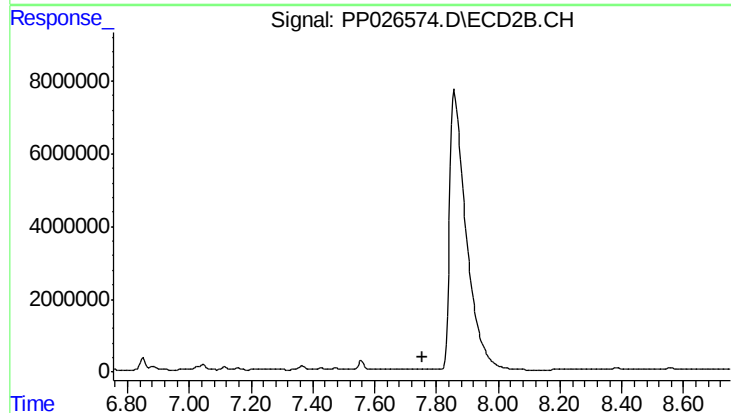


#41 Aroclor-1268-1

R.T.: 0.000 min
Exp R.T.: 7.754 min
Response: 0
Conc: N.D.

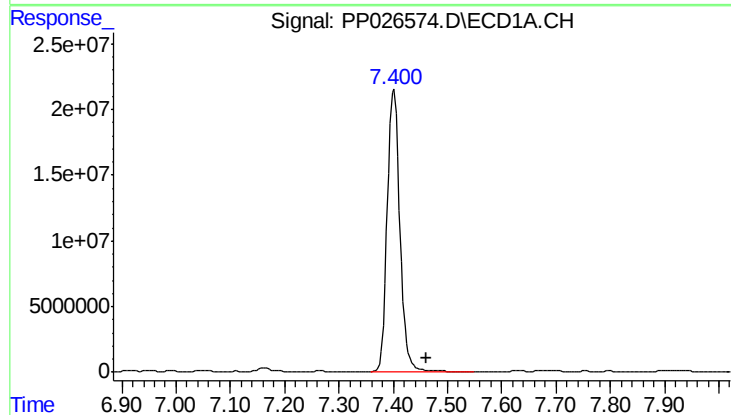


#42 Aroclor-1268-2

R.T.: 7.401 min
Delta R.T.: -0.059 min
Response: 345399268
Conc: 68853.07 ng/ml

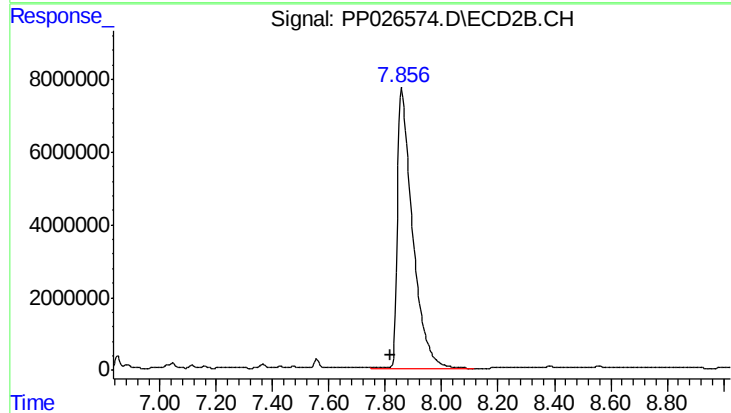

#42 Aroclor-1268-2


R.T.: 7.857 min
Delta R.T.: 0.040 min
Response: 286971665
Conc: 25170.64 ng/ml

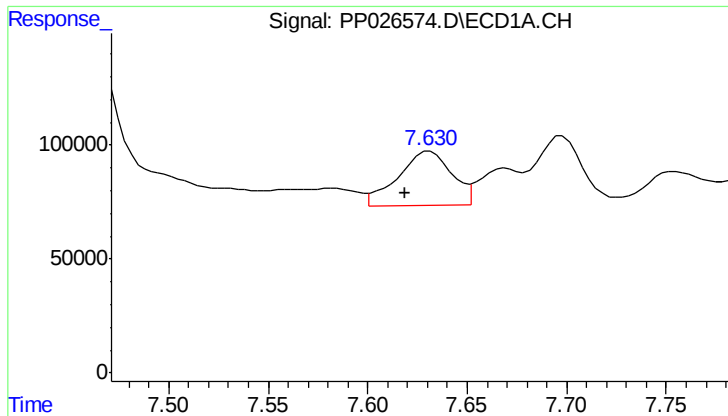

#43 Aroclor-1268-3


R.T.: 7.631 min
Delta R.T.: 0.013 min
Response: 448625
Conc: 1984.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

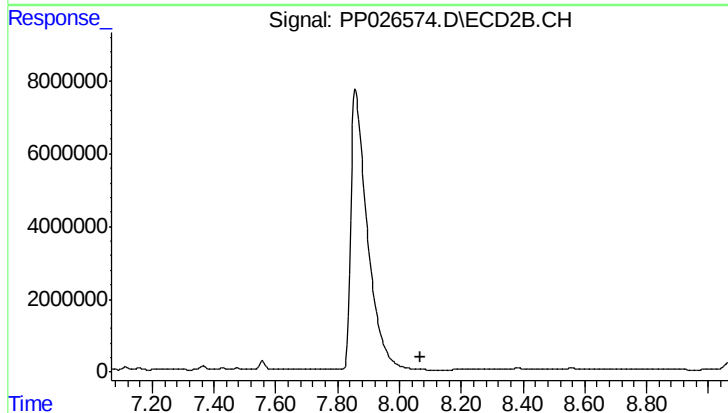


#43 Aroclor-1268-3

R.T.: 0.000 min
Exp R.T.: 8.068 min
Response: 0
Conc: N.D.

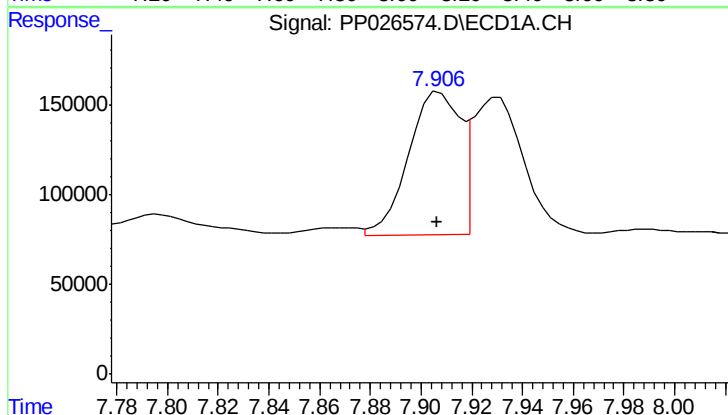


#44 Aroclor-1268-4

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 1118650
Conc: 217.17 ng/ml

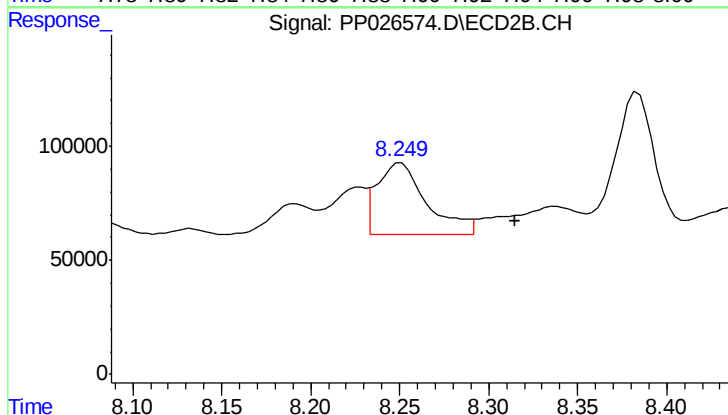

#44 Aroclor-1268-4


R.T.: 8.251 min
Delta R.T.: -0.064 min
Response: 611211
Conc: 127.32 ng/ml

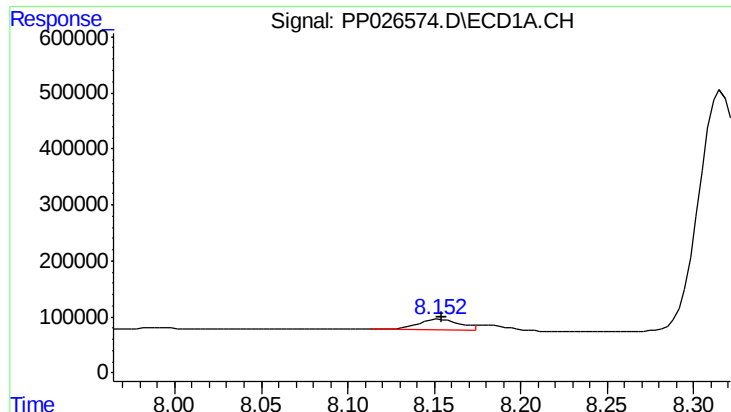

#45 Aroclor-1268-5

R.T.: 8.154 min
Delta R.T.: 0.000 min
Response: 328337
Conc: 262.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110339BSD

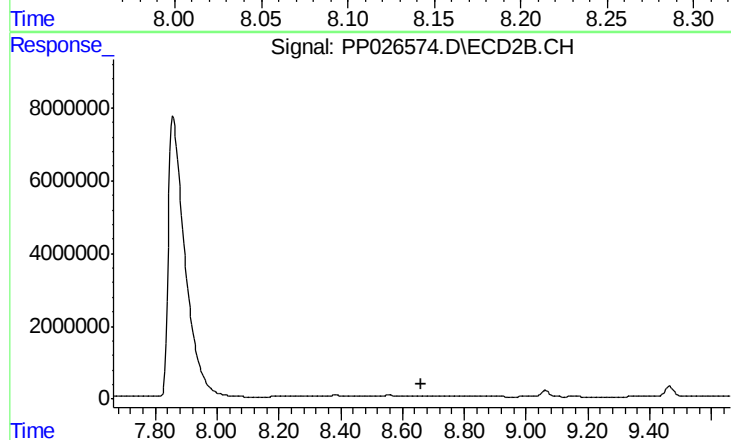

#45 Aroclor-1268-5

R.T.: 0.000 min
Exp R.T. : 8.662 min
Response: 0
Conc: N.D.