

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026577.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 1:50
 Operator : UA/AJ
 Sample : J3486-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DOCUMENTATION-4

Manual Integrations
 APPROVED

ugo
 6/22/2018 10:45:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 08:23:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 08:00:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	4.207	1554131	2981838	17.068	13.133
2) SA Decachlor...	8.334	9.076	3635404	4040355	24.329m	25.382m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026577.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 1:50
Operator : UA/AJ
Sample : J3486-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DOCUMENTATION-4


Manual Integrations
APPROVED

ugo
6/22/2018 10:45:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 08:23:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 08:00:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

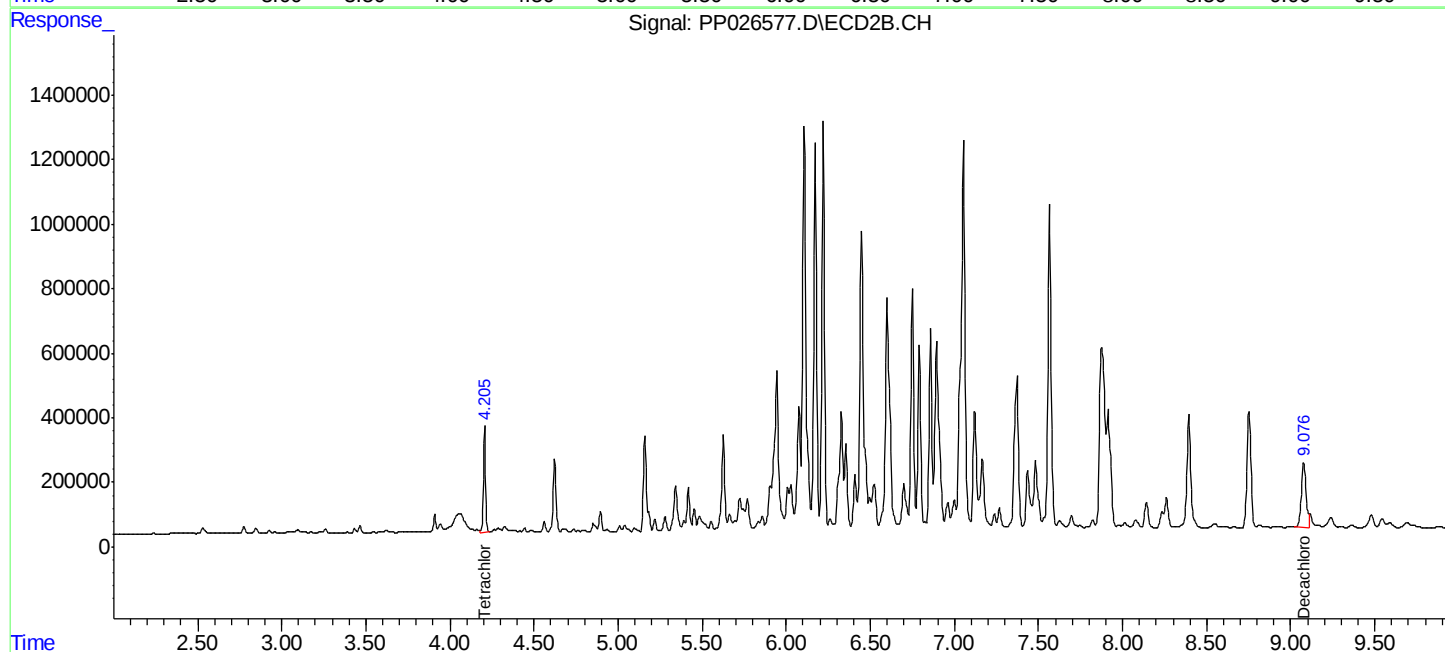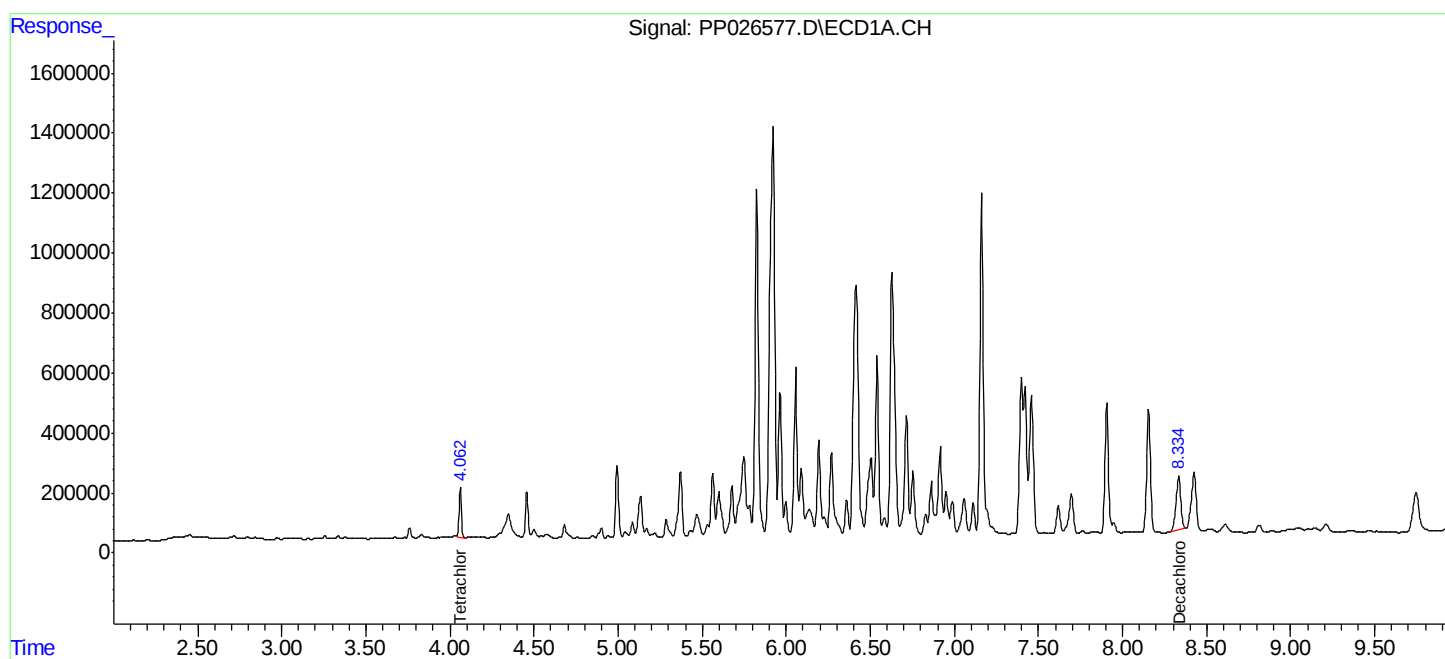

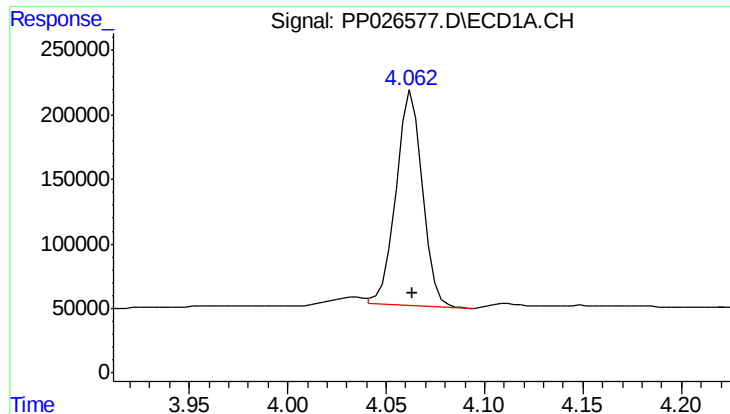


#1 Tetrachloro-m-xylene

R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1554131
Conc: 17.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
DOCUMENTATION-4


Manual Integrations
APPROVED

ugo
6/22/2018 10:45:01 AM

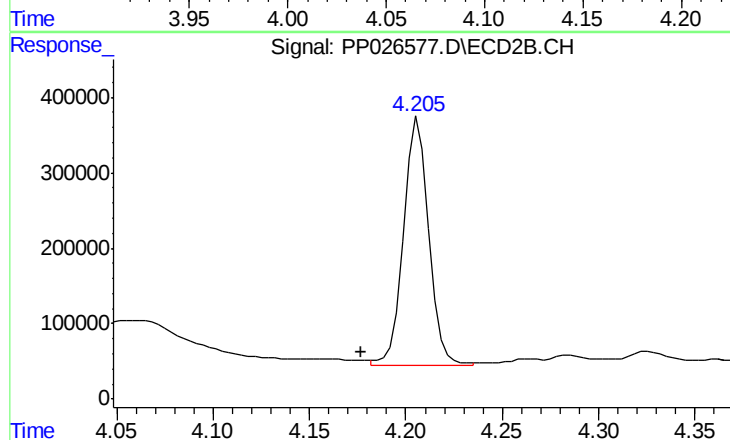


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: 0.030 min
Response: 2981838
Conc: 13.13 ng/ml

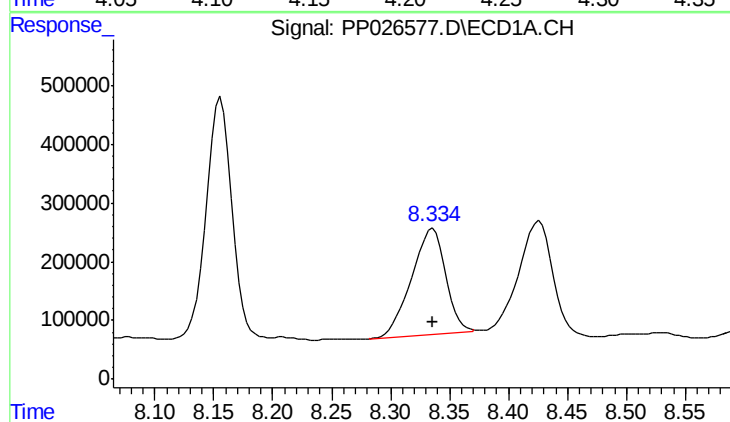

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.001 min
Response: 3635404
Conc: 24.33 ng/ml m

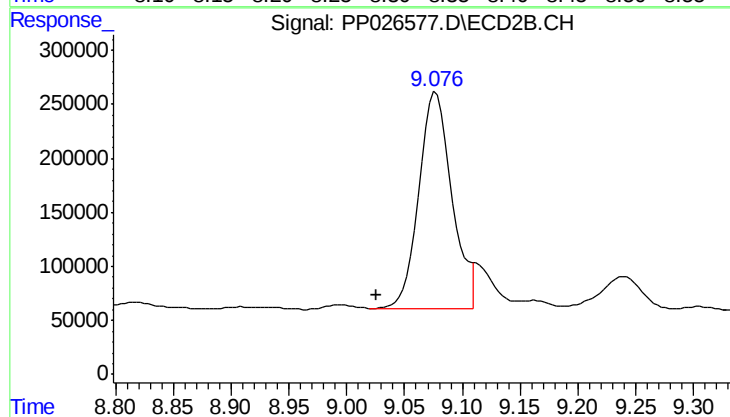

#2 Decachlorobiphenyl

R.T.: 9.076 min
Delta R.T.: 0.050 min
Response: 4040355
Conc: 25.38 ng/ml m