

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026583.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 3:15
Operator : UA/AJ
Sample : J3486-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DOCUMENTATION-10

Manual Integrations
APPROVED

ugo
6/22/2018 10:45:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 08:30:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 08:00:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.064	4.220	1661646	2711484	18.249	11.943m#
2) SA Decachlor...	8.325	9.101	5679175	3072947	38.006	19.305m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026583.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 3:15
Operator : UA/AJ
Sample : J3486-07
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DOCUMENTATION-10


Manual Integrations
APPROVED

ugo
6/22/2018 10:45:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 08:30:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 08:00:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

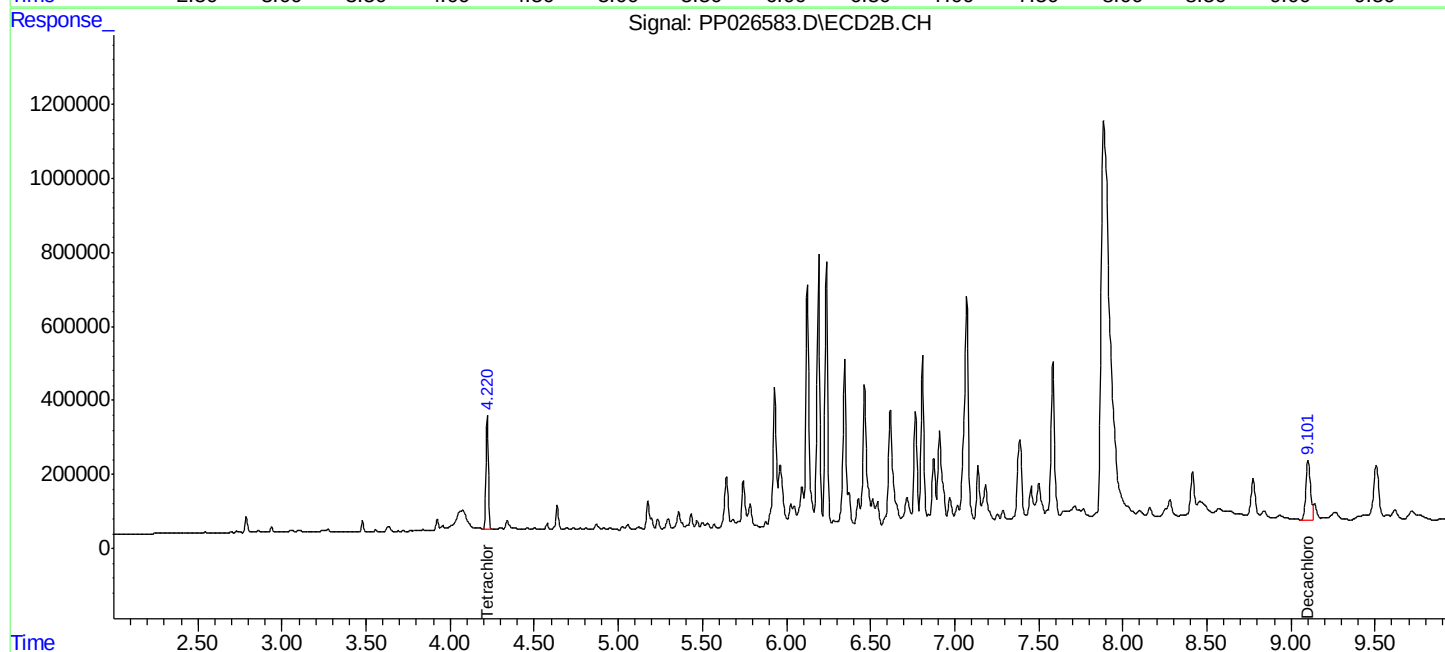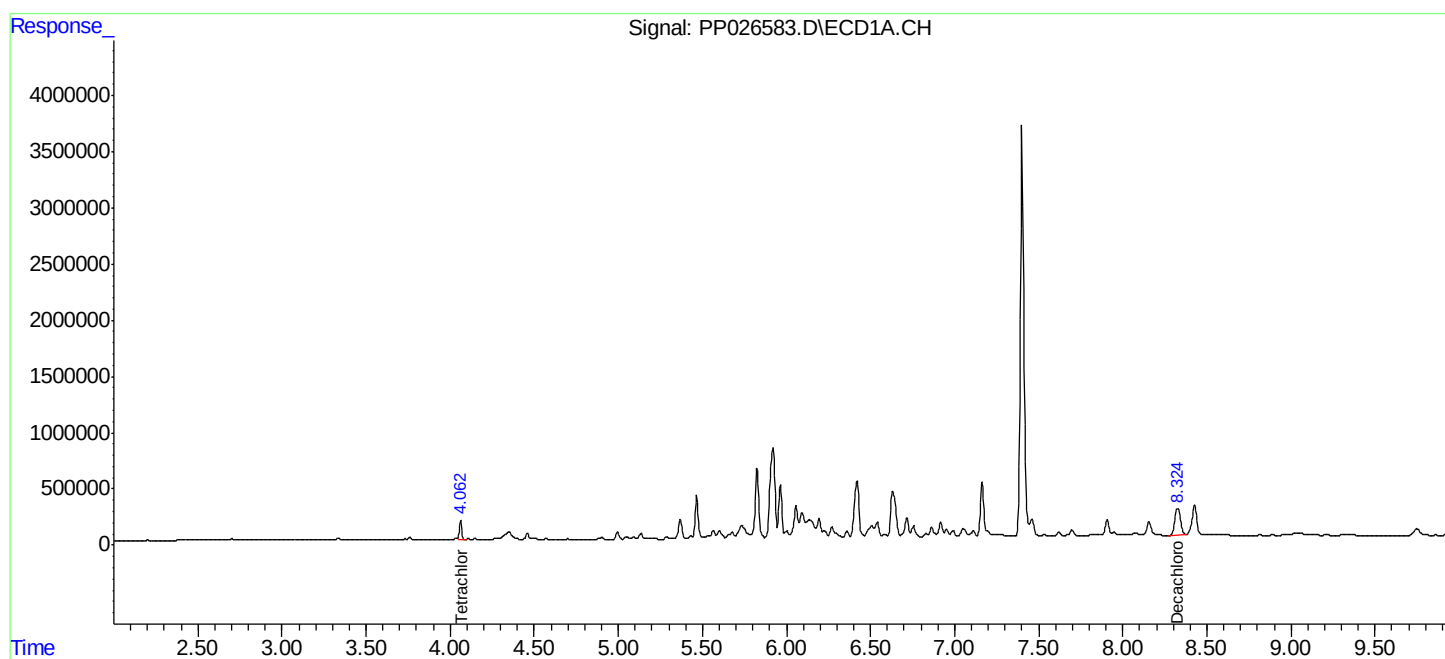

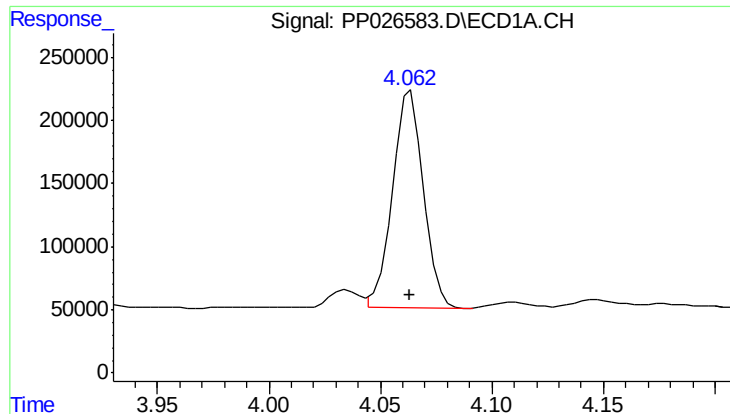


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.000 min
Response: 1661646
Conc: 18.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
DOCUMENTATION-10


Manual Integrations
APPROVED

ugo
6/22/2018 10:45:12 AM

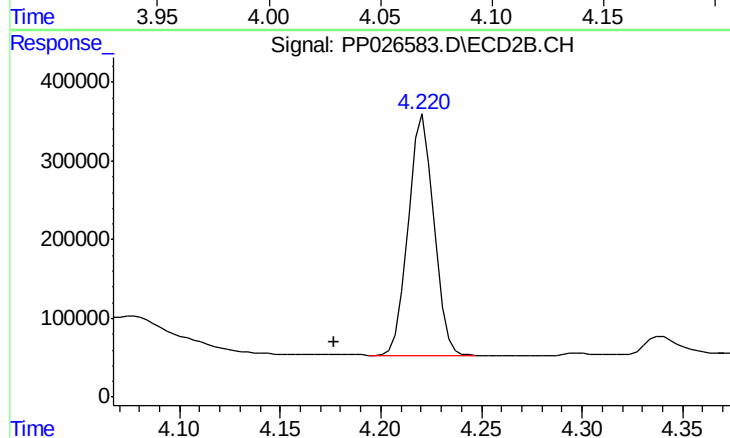


#1 Tetrachloro-m-xylene

R.T.: 4.220 min
Delta R.T.: 0.043 min
Response: 2711484
Conc: 11.94 ng/ml m

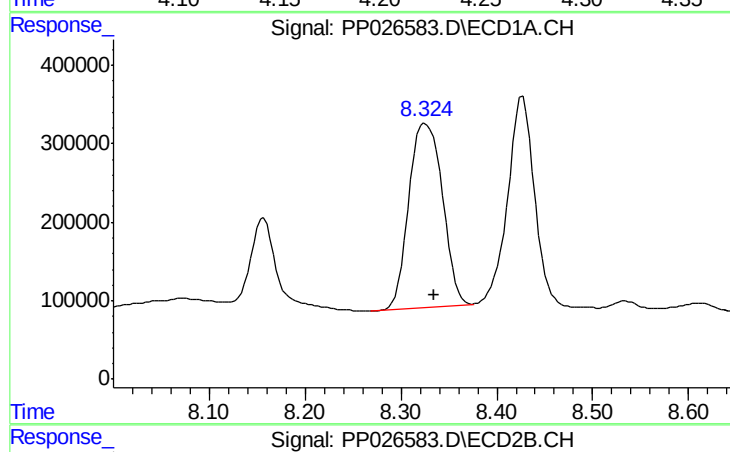

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.010 min
Response: 5679175
Conc: 38.01 ng/ml

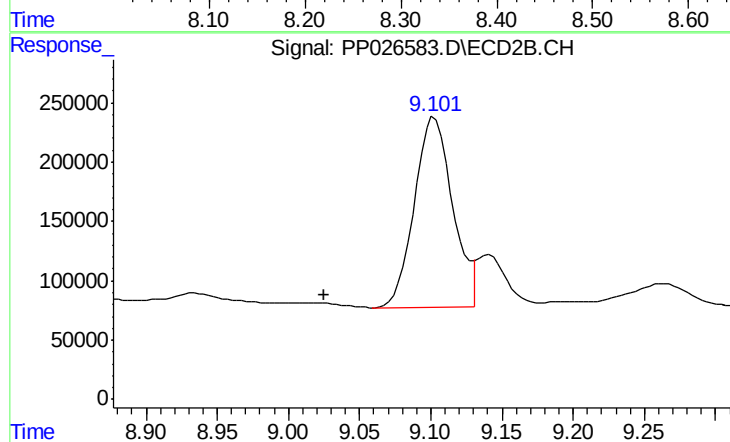

#2 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.076 min
Response: 3072947
Conc: 19.30 ng/ml m