

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP062121\  
 Data File : PP036644.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Jun 2021 10:20  
 Operator : DD\AJ  
 Sample : M2756-05  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 81644-N-1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 21 16:32:02 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP061721.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Jun 18 06:06:19 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

|                    |        |       |        |        |        |        |
|--------------------|--------|-------|--------|--------|--------|--------|
| 1) SA Tetrachlo... | 4.967  | 3.960 | 704607 | 464670 | 15.942 | 15.002 |
| 2) SA Decachlor... | 11.004 | 9.267 | 741441 | 419343 | 17.284 | 13.112 |

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP062121\  
Data File : PP036644.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Jun 2021 10:20  
Operator : DD\AJ  
Sample : M2756-05  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
81644-N-1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 21 16:32:02 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP061721.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Jun 18 06:06:19 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

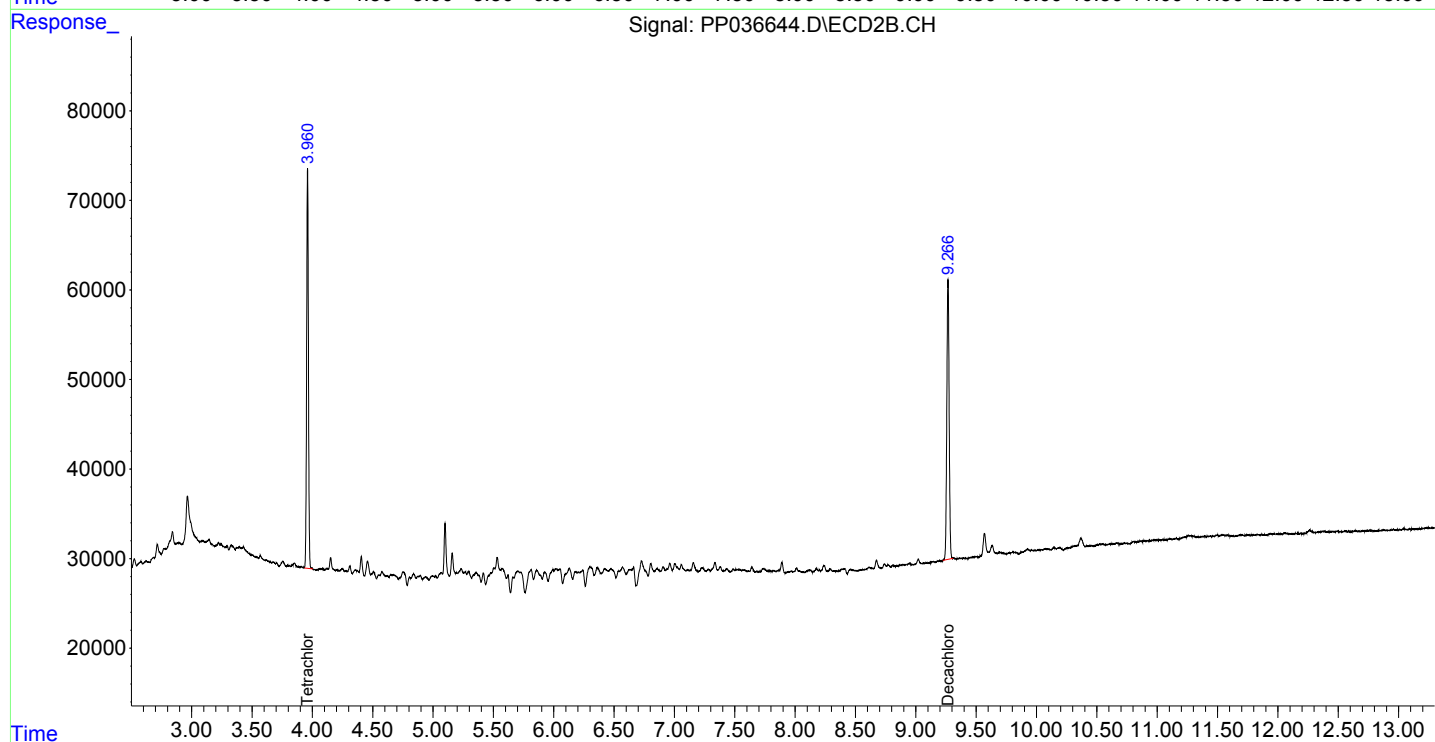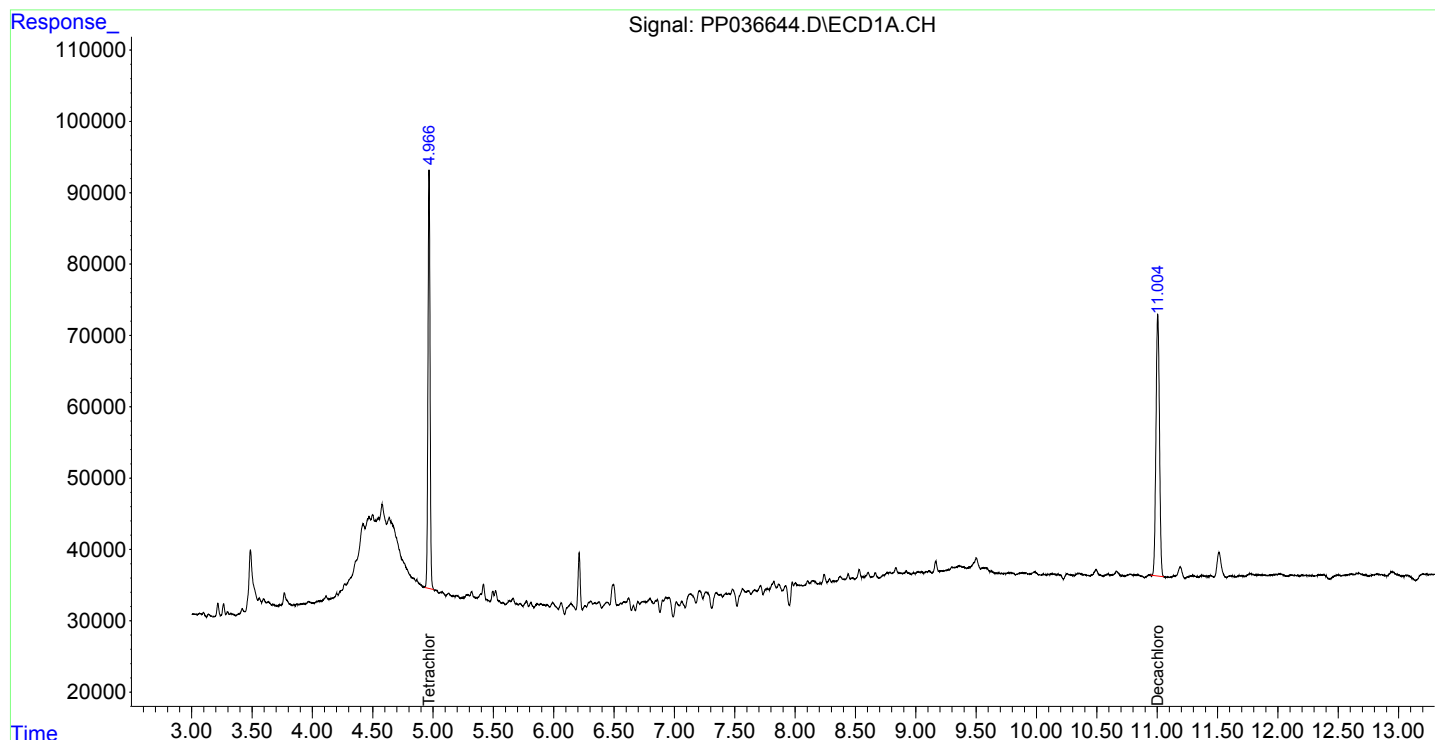


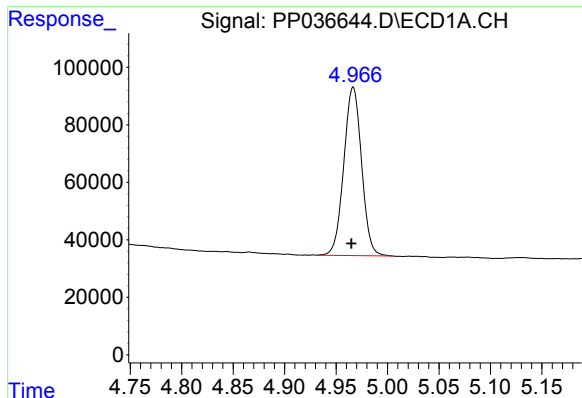

#1 Tetrachloro-m-xylene


R.T.: 4.967 min  
Delta R.T.: 0.002 min  
Response: 704607  
Conc: 15.94 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
81644-N-1

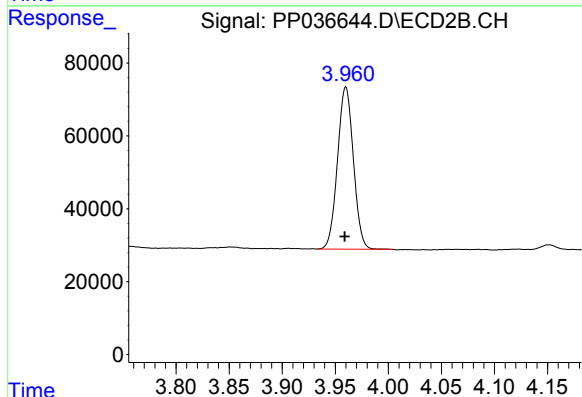


#1 Tetrachloro-m-xylene

R.T.: 3.960 min  
Delta R.T.: 0.001 min  
Response: 464670  
Conc: 15.00 ng/ml

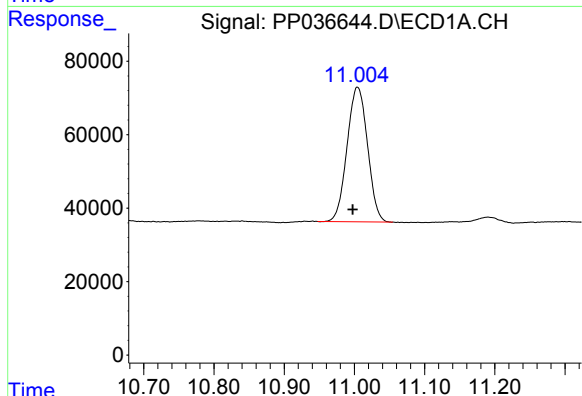

#2 Decachlorobiphenyl

R.T.: 11.004 min  
Delta R.T.: 0.007 min  
Response: 741441  
Conc: 17.28 ng/ml

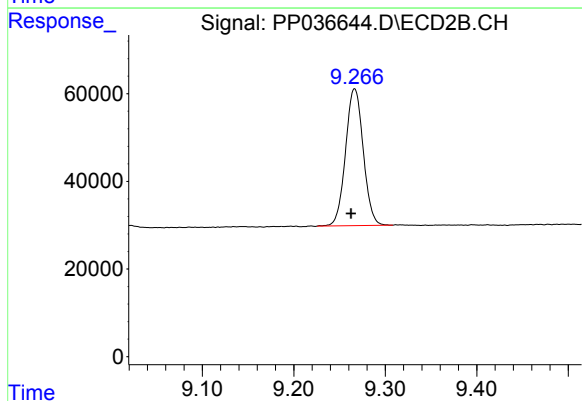

#2 Decachlorobiphenyl

R.T.: 9.267 min  
Delta R.T.: 0.004 min  
Response: 419343  
Conc: 13.11 ng/ml