

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062121\
 Data File : PP036645.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 10:37
 Operator : DD\AJ
 Sample : M2756-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 81644-N-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:32:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.967	3.960	635052	458726	14.368	14.810
2) SA Decachlor...	11.007	9.269	674274	399512	15.718	12.492

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062121\
Data File : PP036645.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 10:37
Operator : DD\AJ
Sample : M2756-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
81644-N-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:32:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

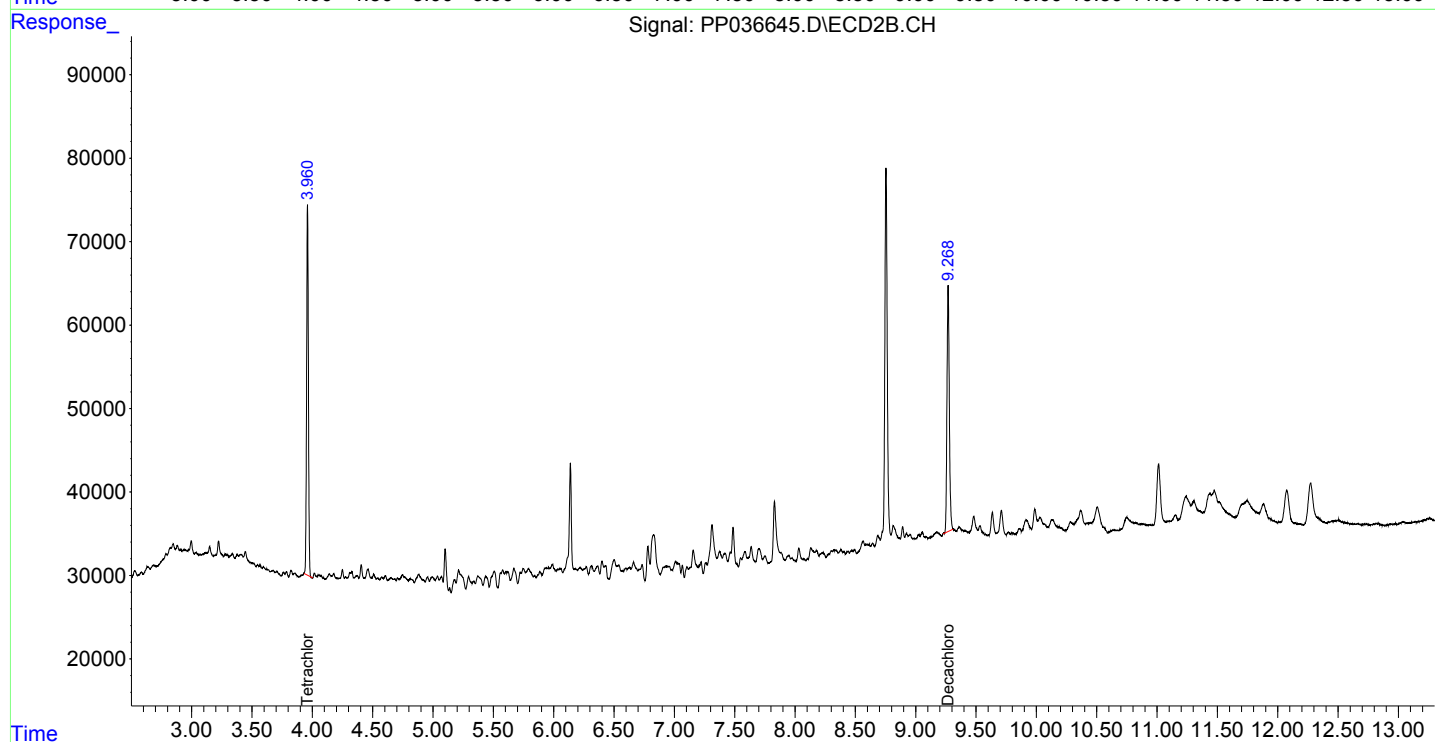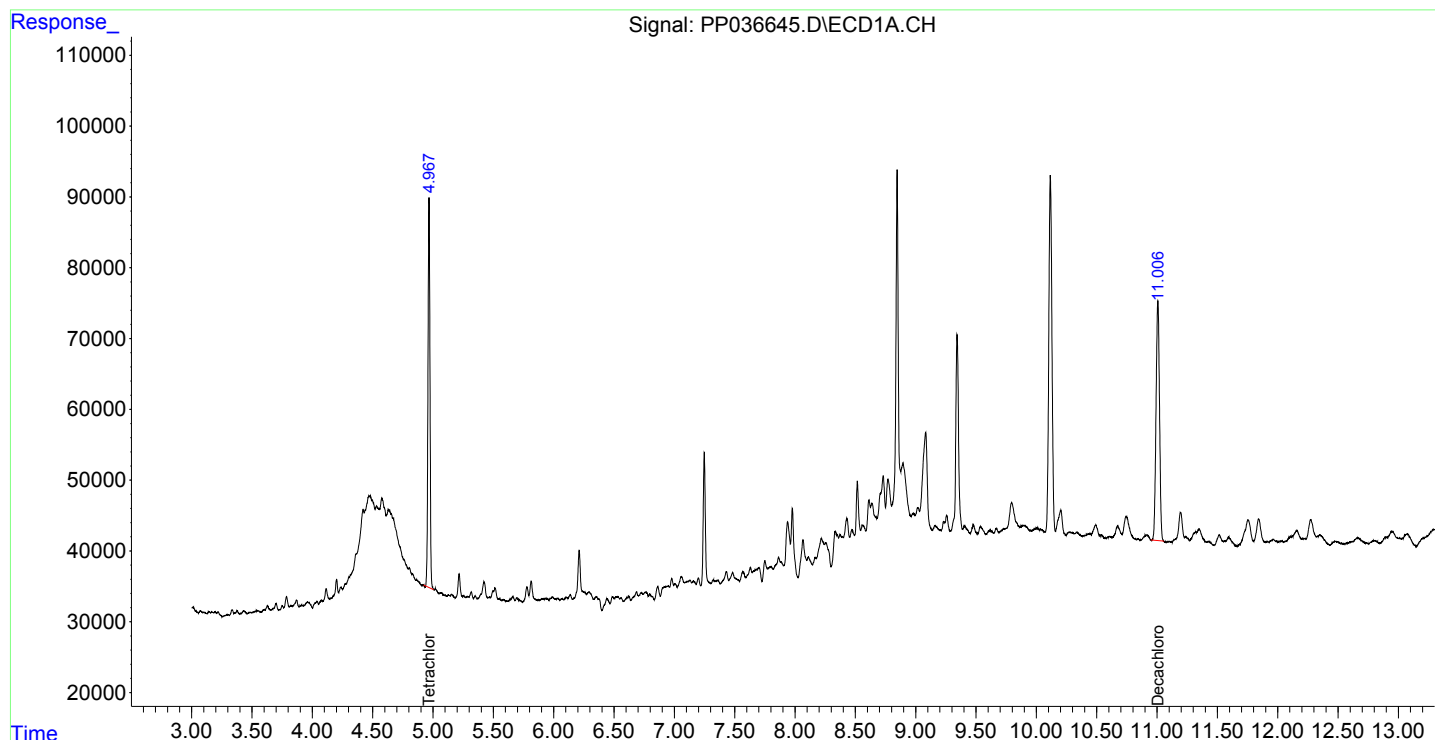


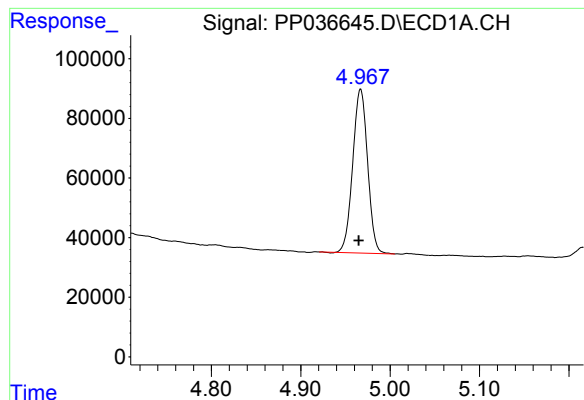

#1 Tetrachloro-m-xylene


R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 635052
Conc: 14.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
81644-N-2

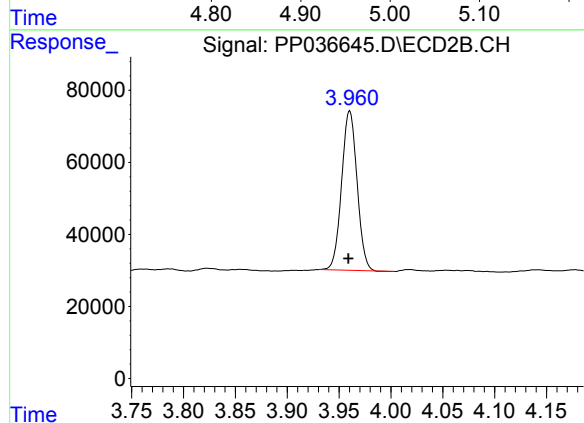


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.001 min
Response: 458726
Conc: 14.81 ng/ml

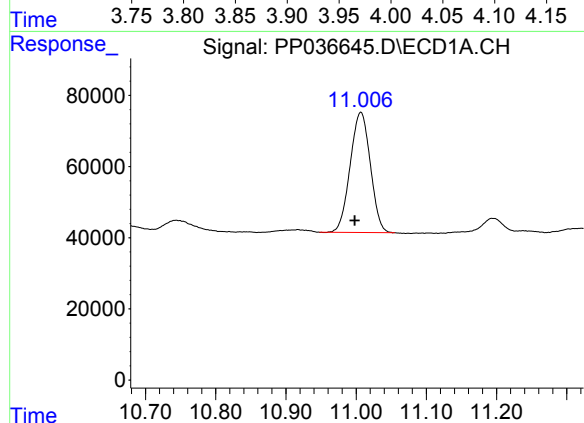

#2 Decachlorobiphenyl

R.T.: 11.007 min
Delta R.T.: 0.009 min
Response: 674274
Conc: 15.72 ng/ml

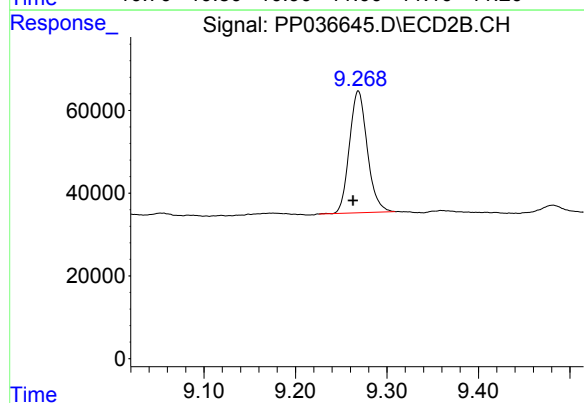

#2 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.006 min
Response: 399512
Conc: 12.49 ng/ml