

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062123\
 Data File : PP058605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 19:39
 Operator : YP\AJ
 Sample : 03329-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMPOSIT-SW01-8-15

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/22/2023
 Supervised By :Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 21:43:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 05:48:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.459	3.670	45602791	34431565	18.262m	21.110
2) SA Decachlor...	10.275	8.725	25888459	25845148	19.574	21.219

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062123\
Data File : PP058605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 19:39
Operator : YP\AJ
Sample : 03329-19
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMPOSIT-SW01-8-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/22/2023
Supervised By :Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 21:43:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 05:48:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

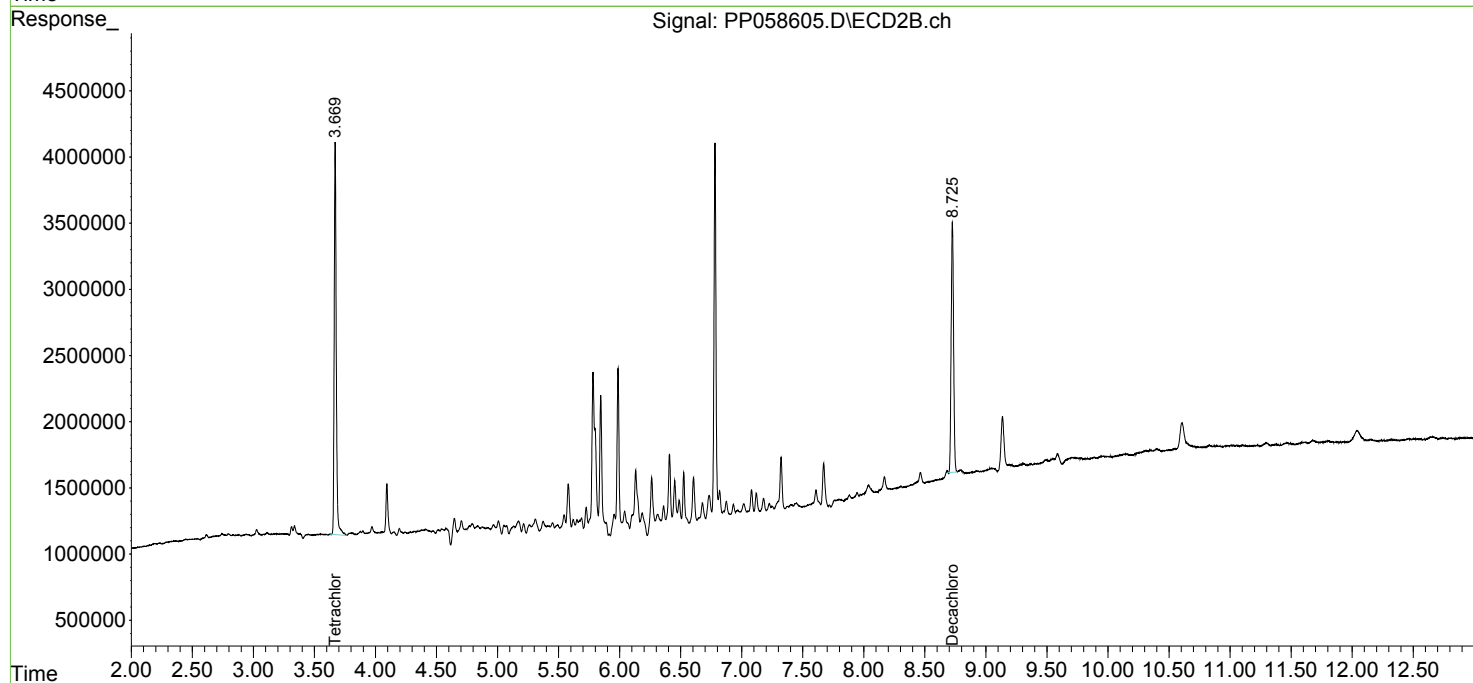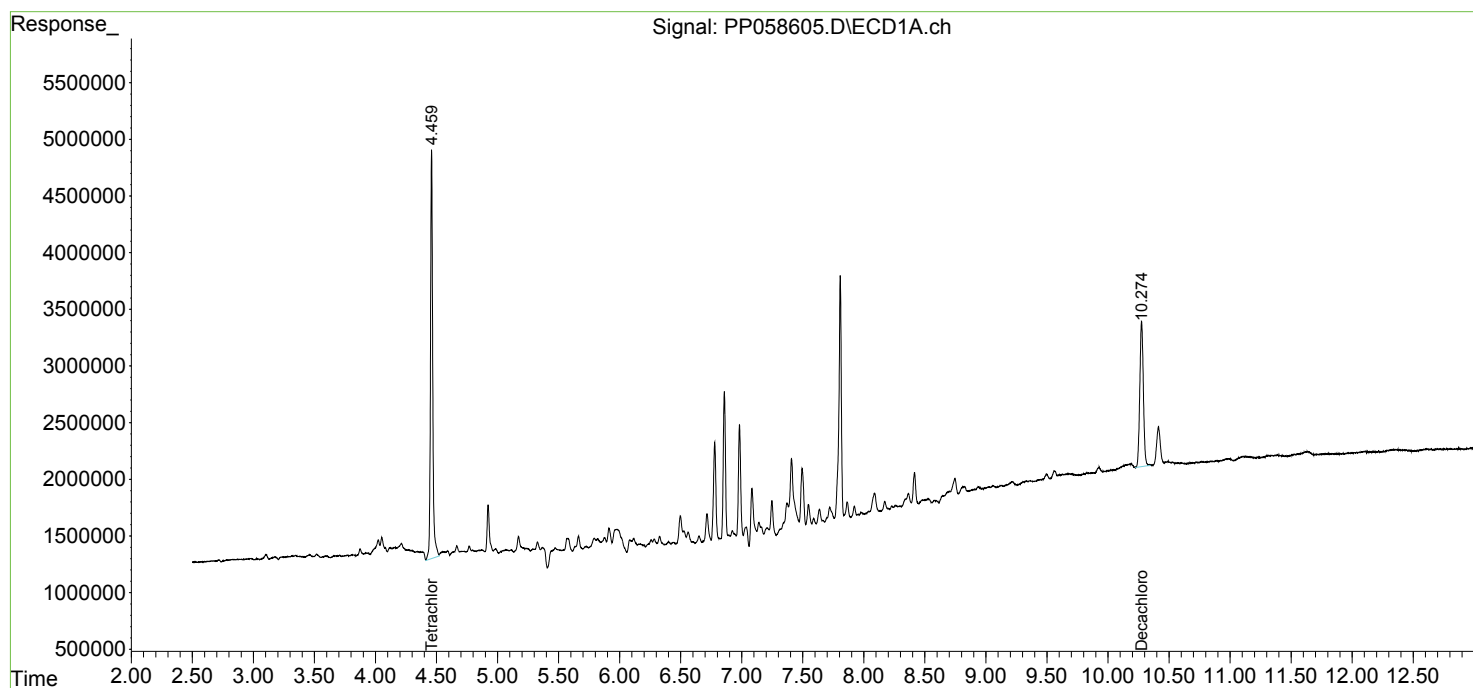

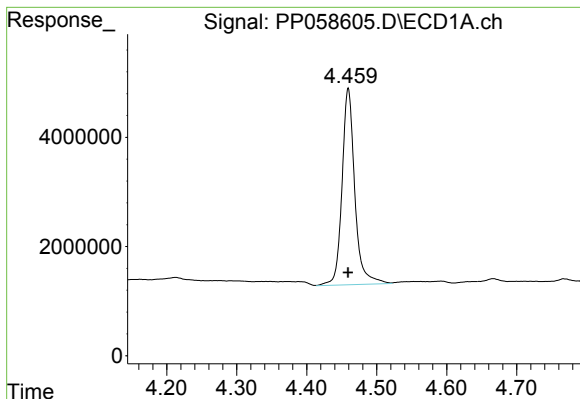


#1 Tetrachloro-m-xylene

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 45602791
Conc: 18.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMPOSIT-SW01-8-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/22/2023
Supervised By :Ankita Jodhani 06/22/2023

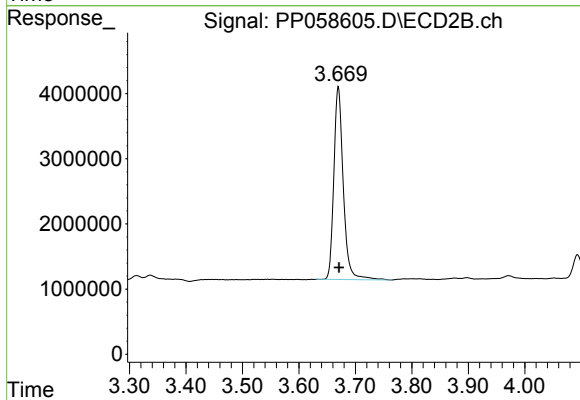


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.001 min
Response: 34431565
Conc: 21.11 ng/ml

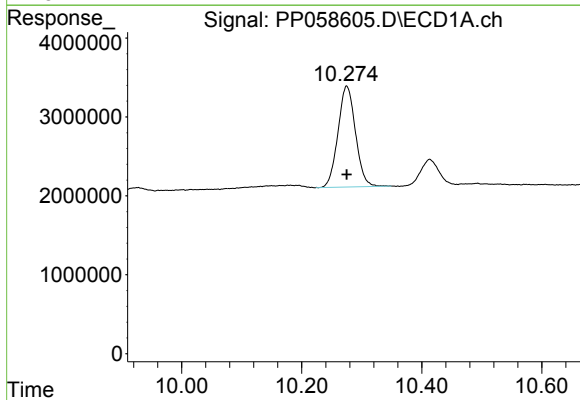

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: 0.000 min
Response: 25888459
Conc: 19.57 ng/ml

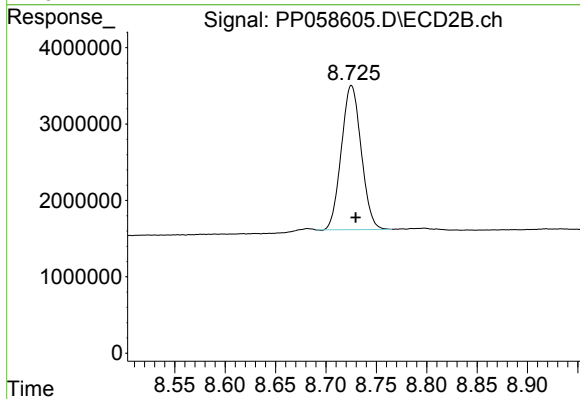

#2 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.004 min
Response: 25845148
Conc: 21.22 ng/ml