

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062123\
 Data File : PP058610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 21:00
 Operator : YP\AJ
 Sample : 03327-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMPOSIT-TW-02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/22/2023
 Supervised By :Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 05:03:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 05:48:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.459	3.670	55841434	44301226	22.362	27.161
2) SA Decachlor...	10.276	8.724	34540368	35874909	26.115	29.453

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062123\
Data File : PP058610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 21:00
Operator : YP\AJ
Sample : 03327-07
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMPOSIT-TW-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/22/2023
Supervised By :Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 05:03:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 05:48:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

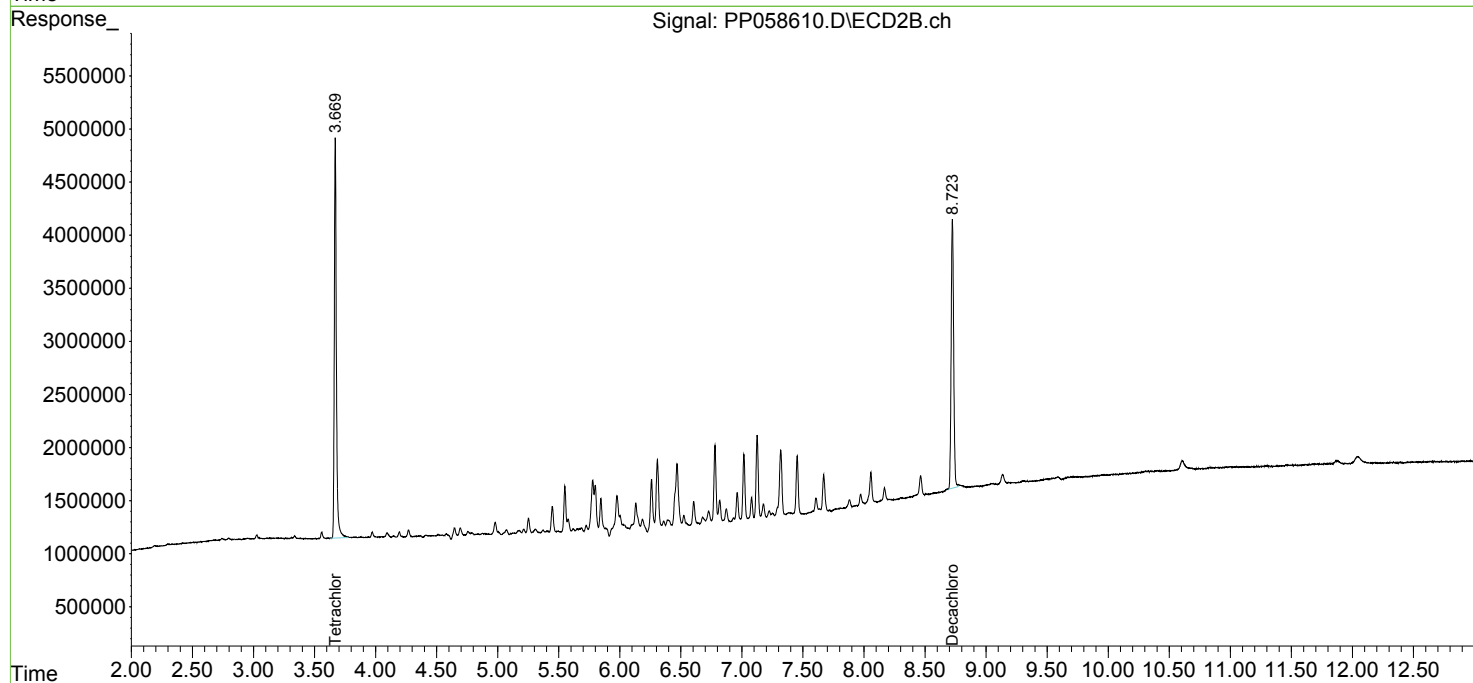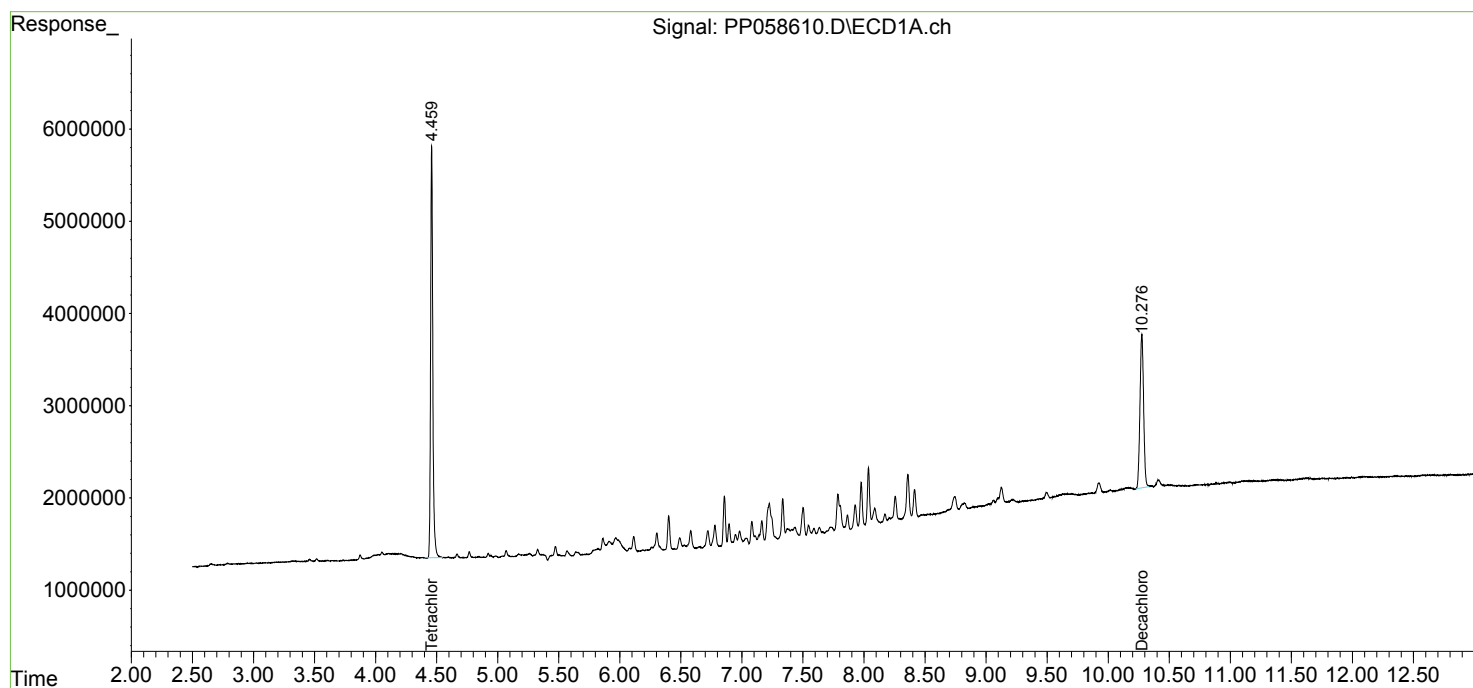

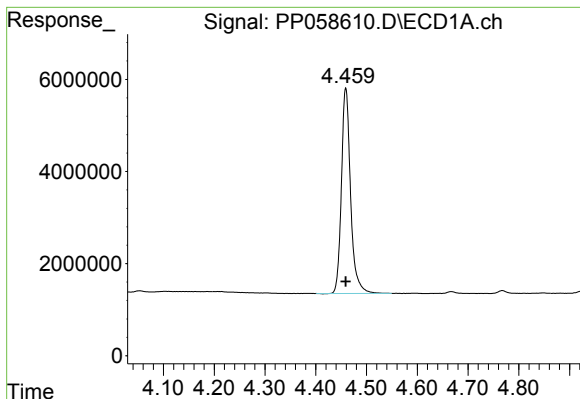

#1 Tetrachloro-m-xylene

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 55841434
Conc: 22.36 ng/ml

Instrument :

ECD_P


ClientSampleId :

COMPOSIT-TW-02

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/22/2023
Supervised By :Ankita Jodhani 06/22/2023

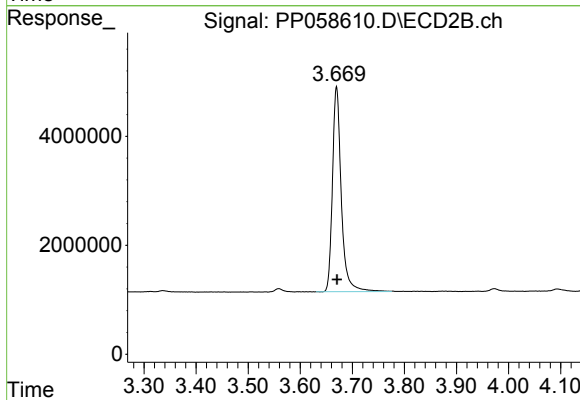


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.001 min
Response: 44301226
Conc: 27.16 ng/ml

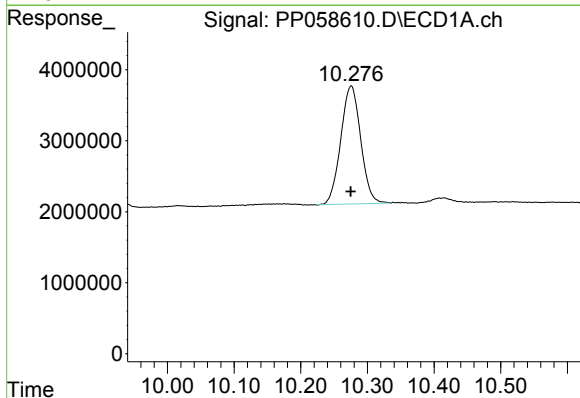

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: 0.000 min
Response: 34540368
Conc: 26.12 ng/ml

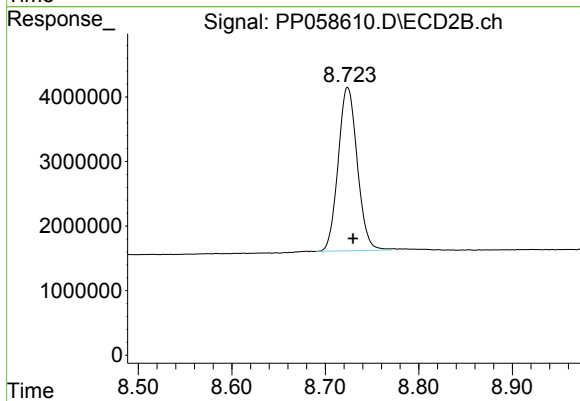

#2 Decachlorobiphenyl

R.T.: 8.724 min
Delta R.T.: -0.006 min
Response: 35874909
Conc: 29.45 ng/ml