

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
 Data File : PP036687.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 16:57
 Operator : DD\AJ
 Sample : M2786-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33265

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 17:52:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.965	3.958	389870	254805	8.821	8.227
2) SA Decachlor...	11.001	9.259	290185	201308	6.765	6.295

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
Data File : PP036687.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 16:57
Operator : DD\AJ
Sample : M2786-10
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
33265

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 17:52:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

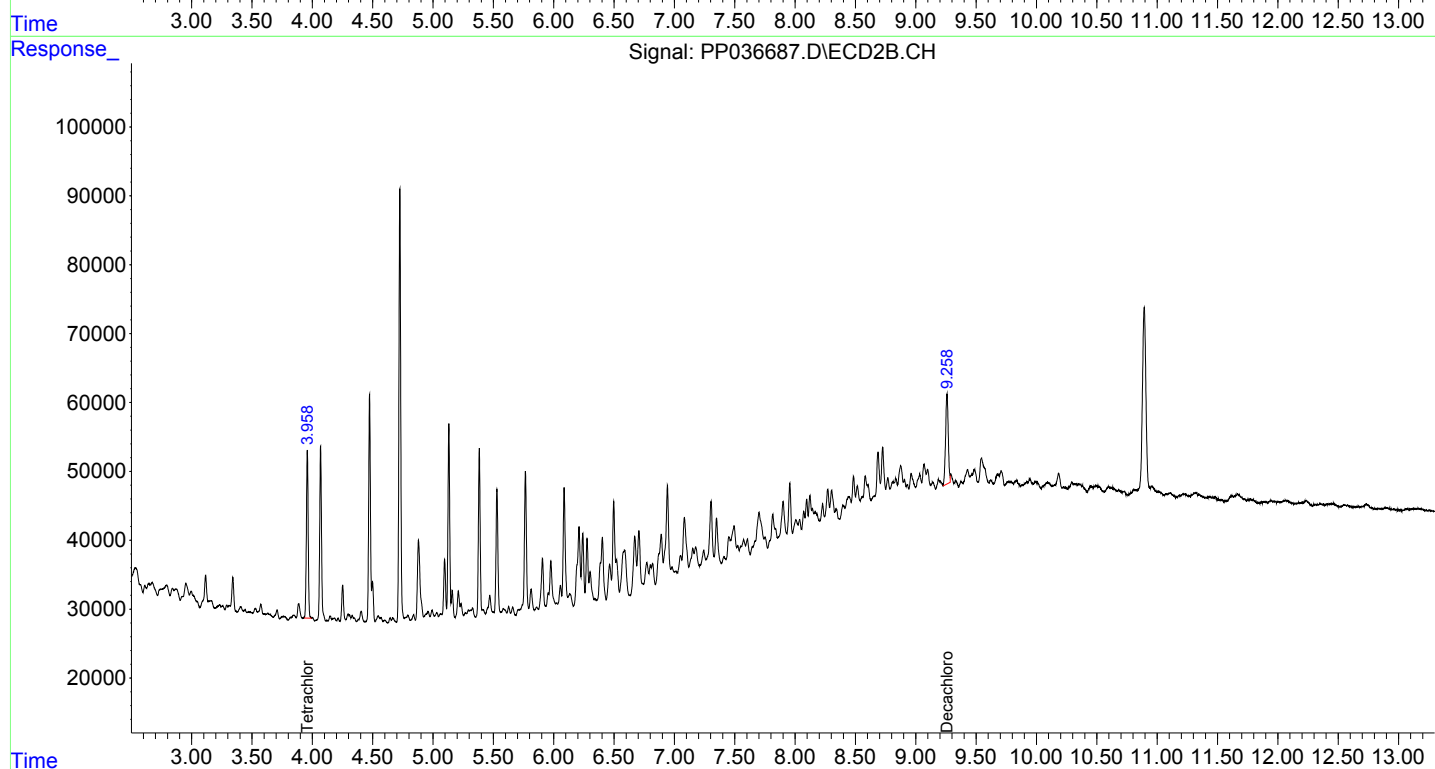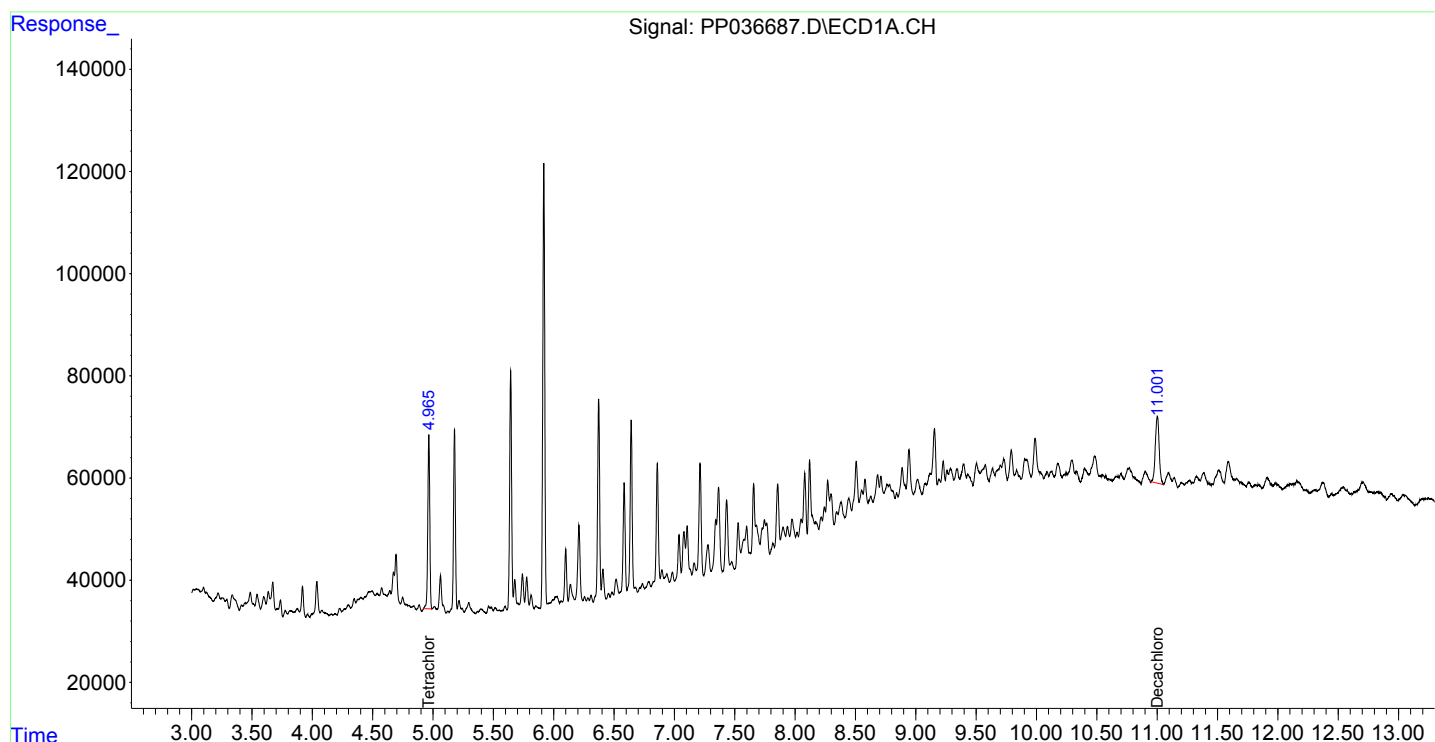


Time

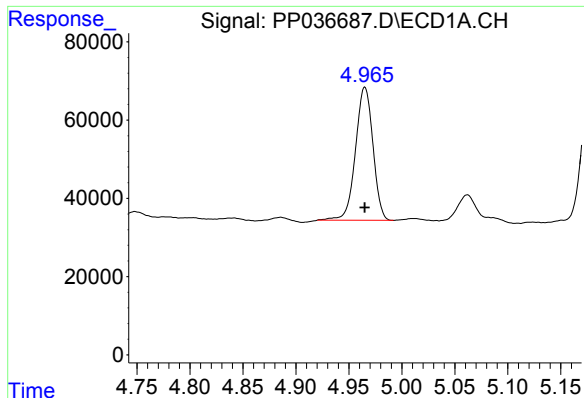

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 389870
Conc: 8.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
33265

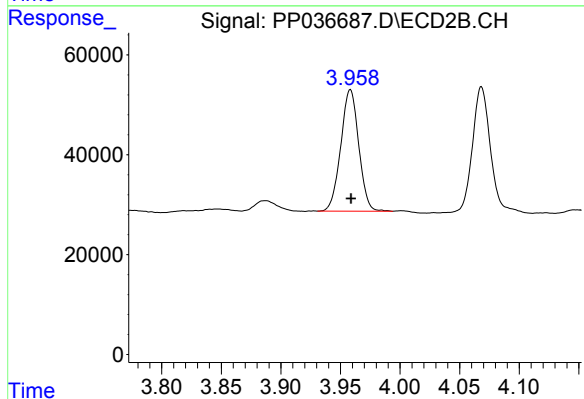


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 254805
Conc: 8.23 ng/ml

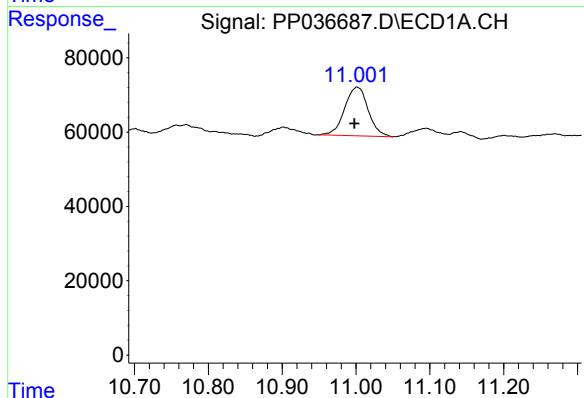

#2 Decachlorobiphenyl

R.T.: 11.001 min
Delta R.T.: 0.003 min
Response: 290185
Conc: 6.76 ng/ml

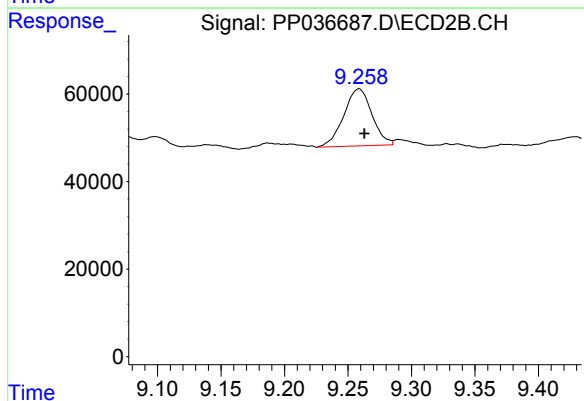

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.004 min
Response: 201308
Conc: 6.29 ng/ml