

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
 Data File : PP036700.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 21:08
 Operator : DD\AJ
 Sample : M2789-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONCRETE-SLAB-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 06:42:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.964	3.957	701879	490652	15.880	15.841
2) SA Decachlor...	10.999	9.256	743383	468710	17.329	14.656

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
Data File : PP036700.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 21:08
Operator : DD\AJ
Sample : M2789-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CONCRETE-SLAB-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 06:42:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

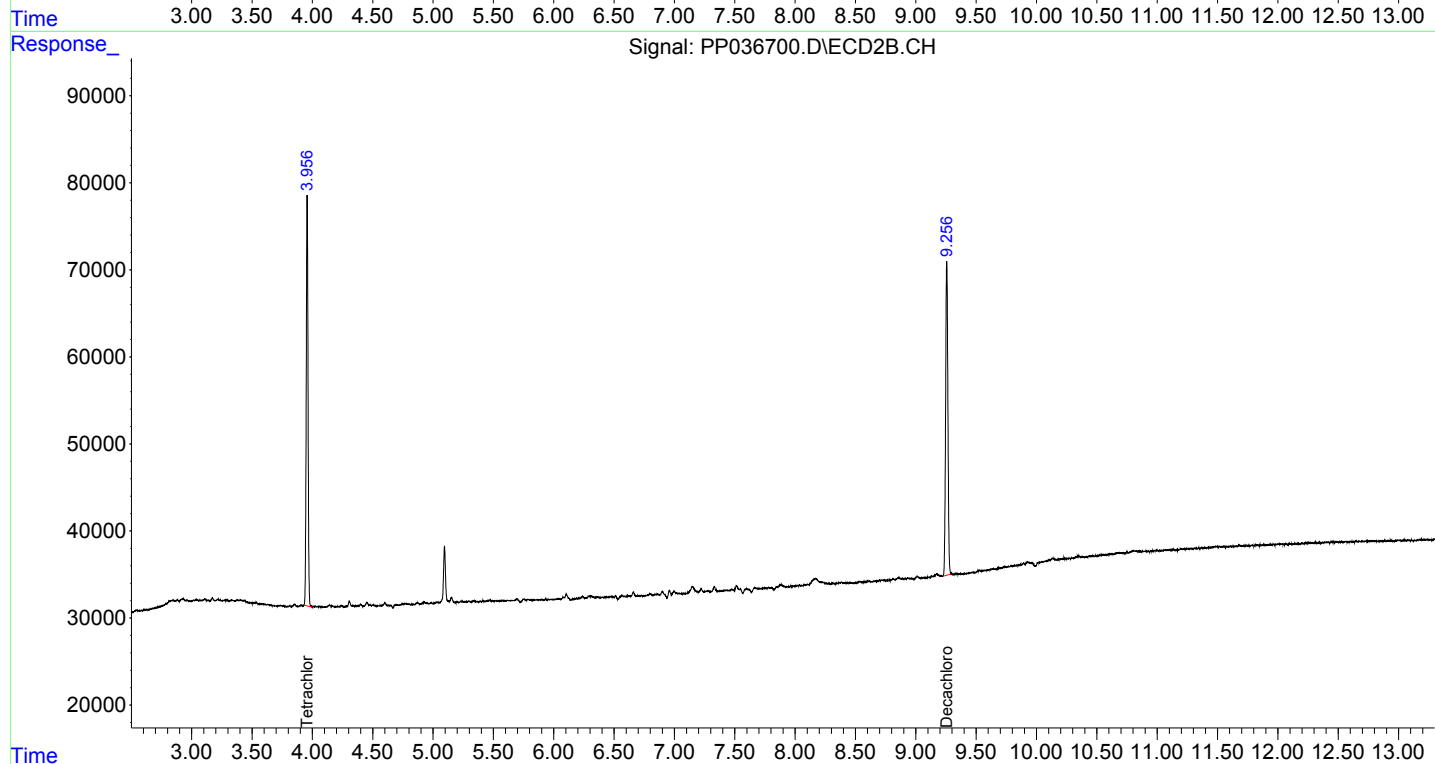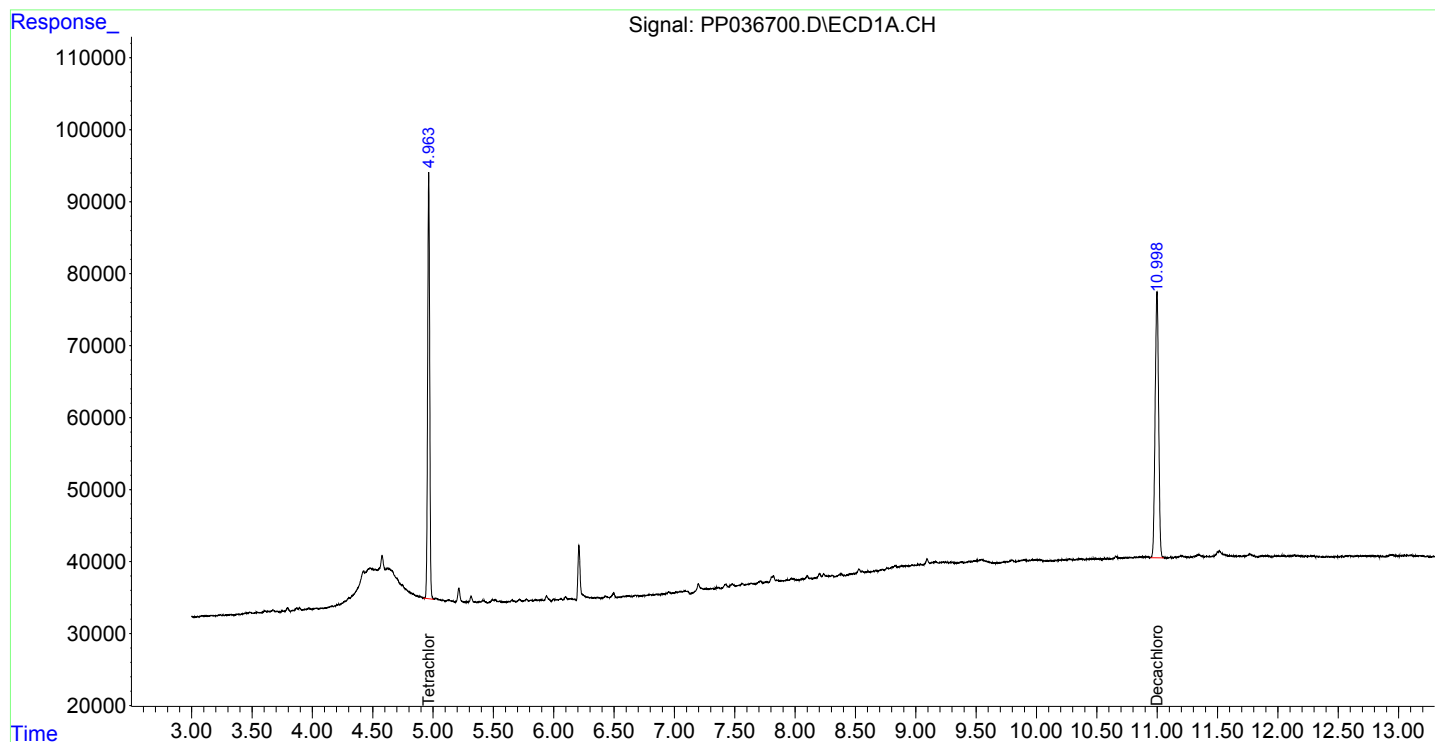


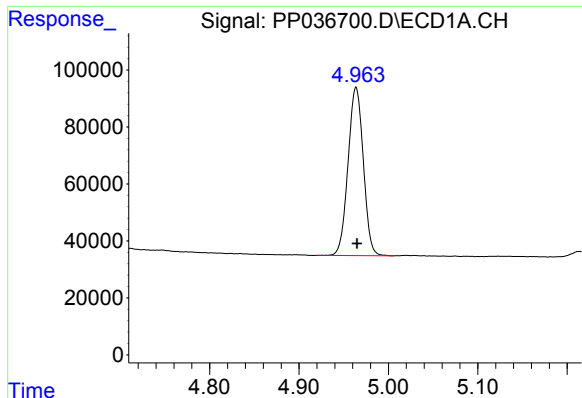

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 701879
Conc: 15.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-SLAB-1-2

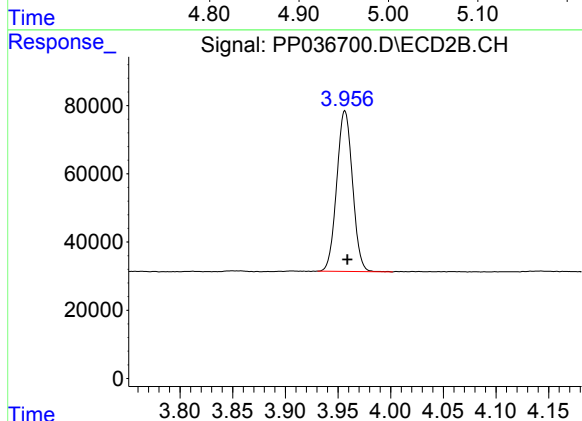


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.002 min
Response: 490652
Conc: 15.84 ng/ml

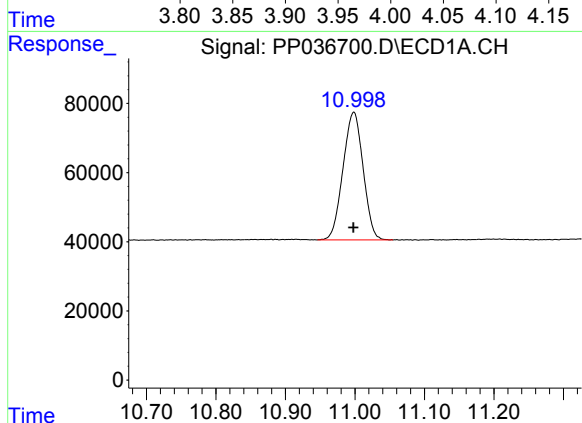

#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: 0.000 min
Response: 743383
Conc: 17.33 ng/ml

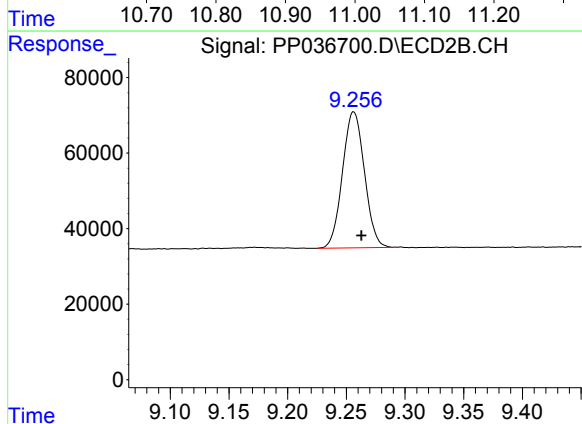

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.007 min
Response: 468710
Conc: 14.66 ng/ml