

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
 Data File : PP036705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 22:32
 Operator : DD\AJ
 Sample : M2789-23
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 06:45:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.957	801935	579231	18.144	18.701
2) SA Decachlor...	10.998	9.256	889375	567527	20.733	17.746
Target Compounds						
26) L6 AR-1254-1	7.195	6.081	35786	21201	20.348m	12.513 #
27) L6 AR-1254-2	7.424	6.240	46306	16303	17.114	10.961 #
28) L6 AR-1254-3	7.805	6.660	64237	38545	21.687	15.855 #
29) L6 AR-1254-4	8.101	6.900	47444	30723	21.582	19.854
30) L6 AR-1254-5	8.530	7.330	66944	96710	28.150	44.975 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sampled :
 1ST-WALLS

Manual Integrations
 APPROVED

Ankita
 6/23/2021 2:17:23 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
Data File : PP036705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 22:32
Operator : DD\AJ
Sample : M2789-23
Misc :
ALS Vial : 30 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 06:45:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
1ST-WALLS

Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:23 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

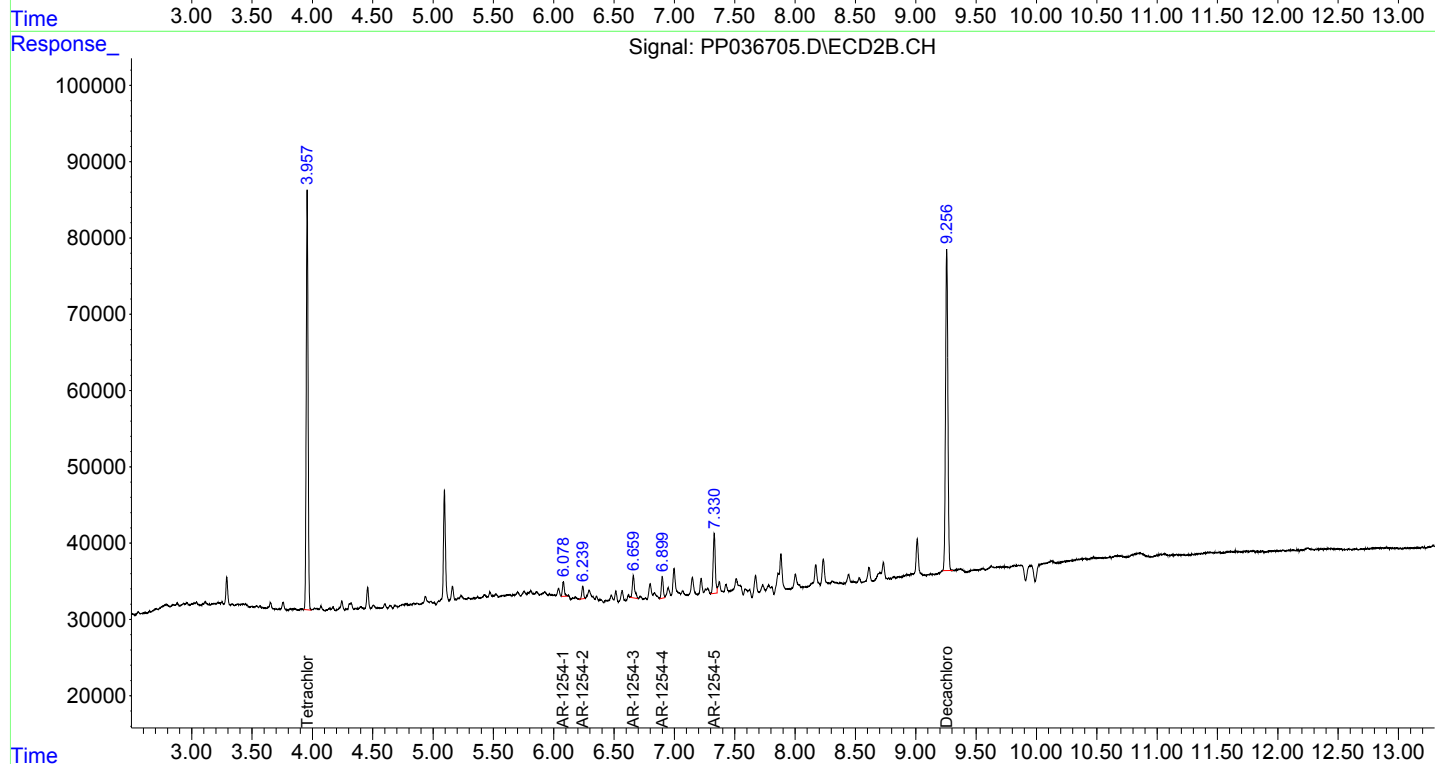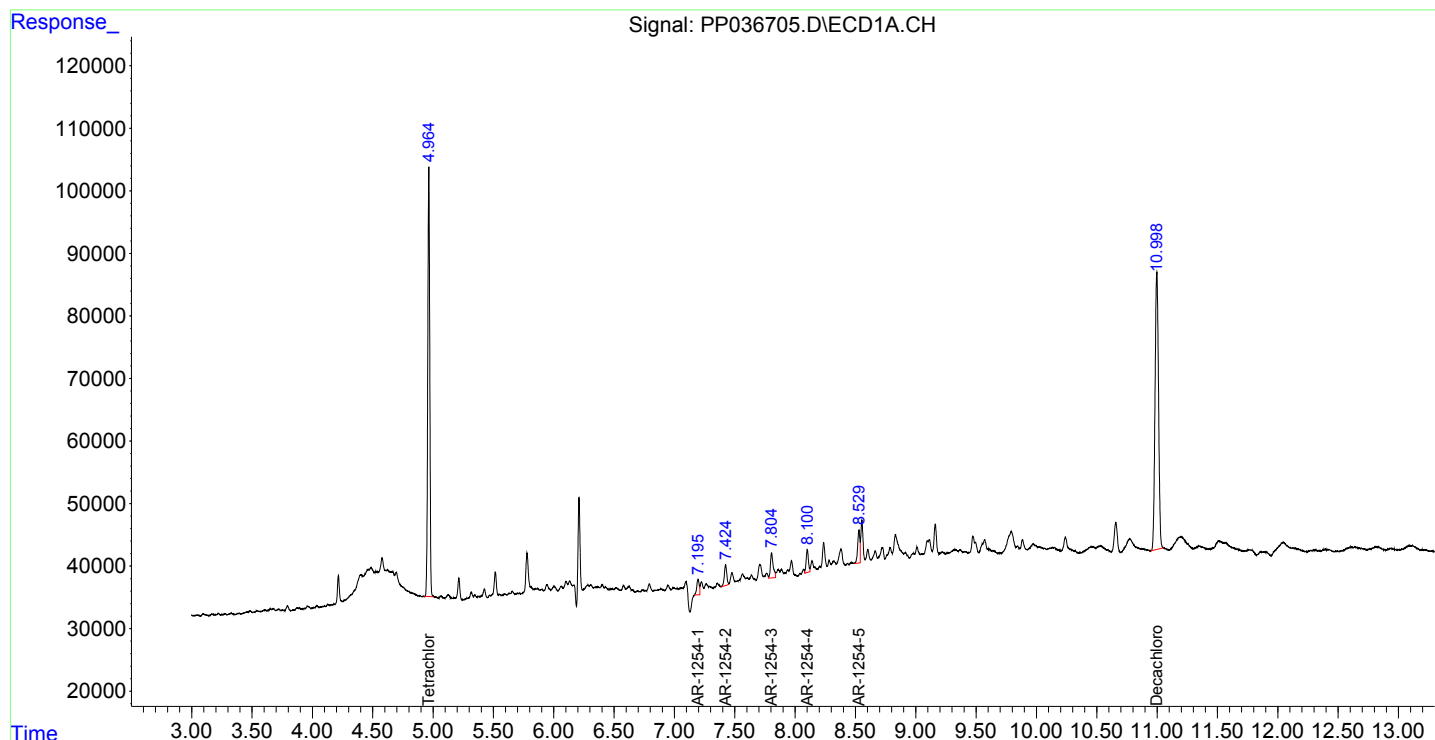

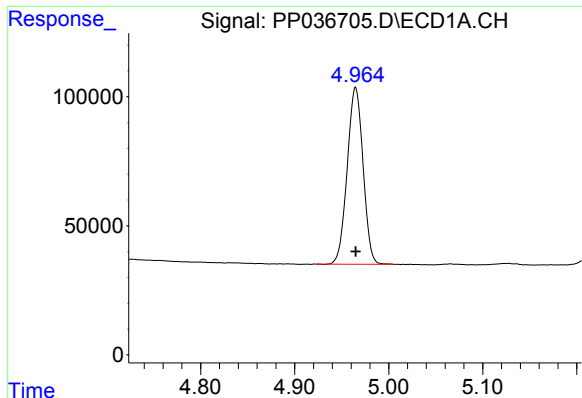


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 801935
Conc: 18.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:23 PM

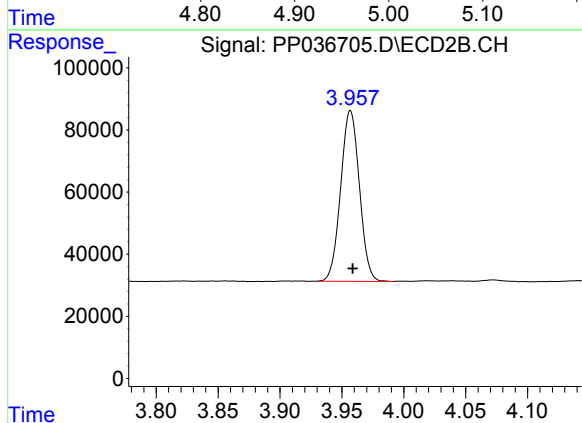


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.002 min
Response: 579231
Conc: 18.70 ng/ml

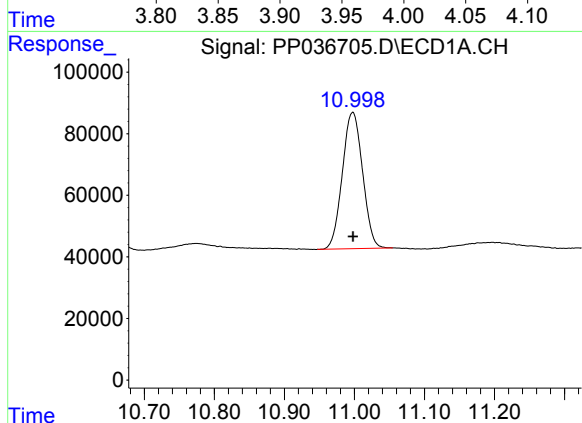


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 889375
Conc: 20.73 ng/ml

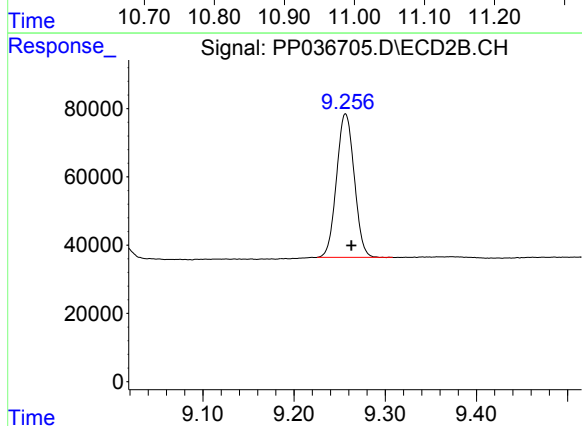

#2 Decachlorobiphenyl


R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 567527
Conc: 17.75 ng/ml

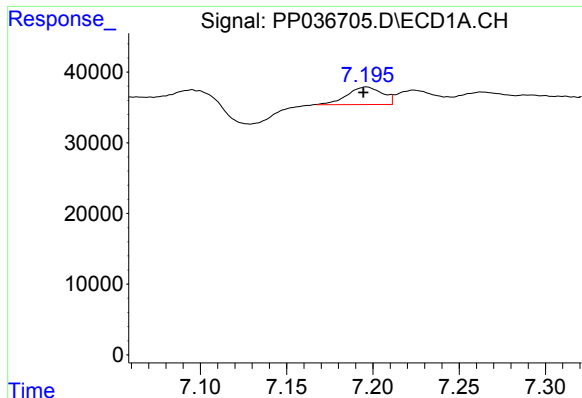

#26 AR-1254-1

R.T.: 7.195 min
Delta R.T.: 0.000 min
Response: 35786
Conc: 20.35 ng/ml m

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS

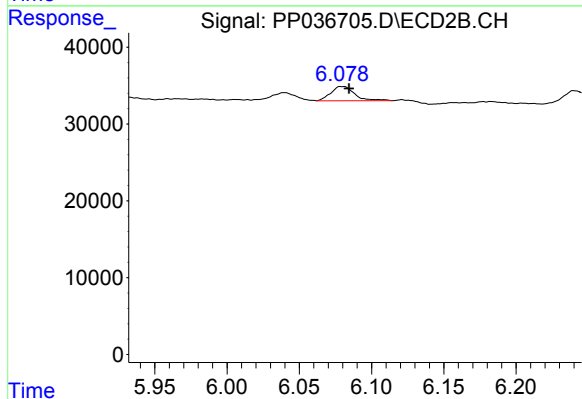


#26 AR-1254-1

R.T.: 6.081 min
Delta R.T.: -0.003 min
Response: 21201
Conc: 12.51 ng/ml


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:23 PM

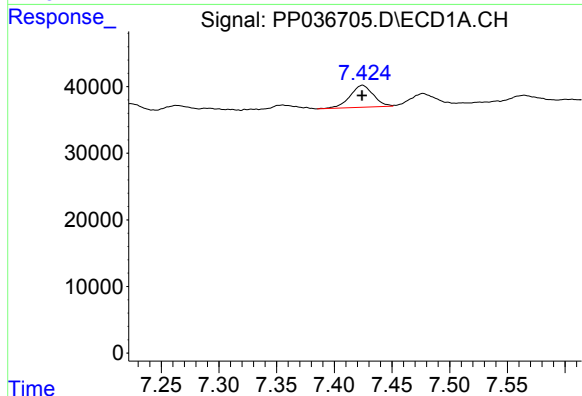


#27 AR-1254-2

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 46306
Conc: 17.11 ng/ml

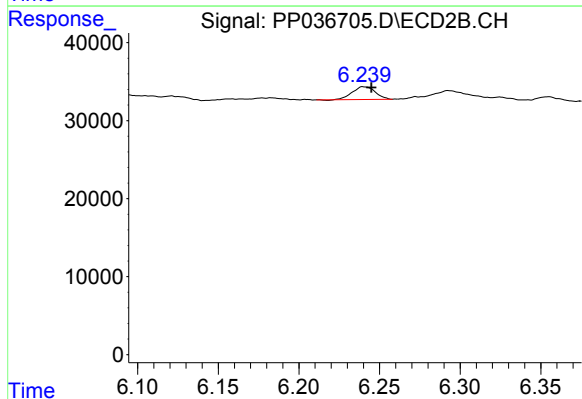

#27 AR-1254-2

R.T.: 6.240 min
Delta R.T.: -0.005 min
Response: 16303
Conc: 10.96 ng/ml

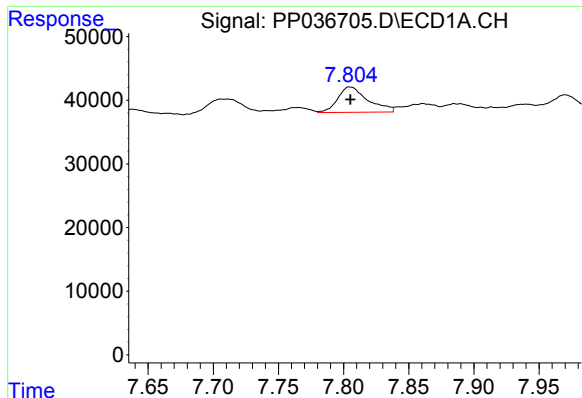


#28 AR-1254-3

R.T.: 7.805 min
Delta R.T.: 0.000 min
Response: 64237
Conc: 21.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:23 PM

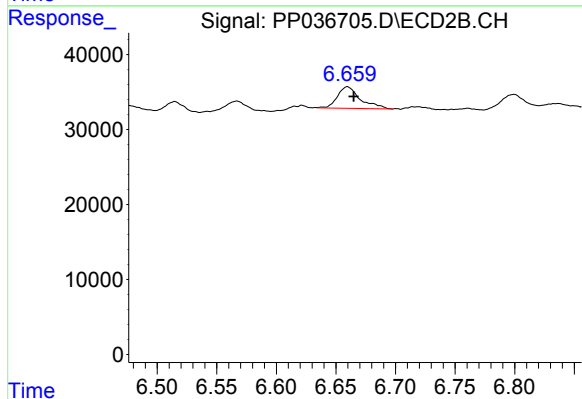


#28 AR-1254-3

R.T.: 6.660 min
Delta R.T.: -0.005 min
Response: 38545
Conc: 15.85 ng/ml

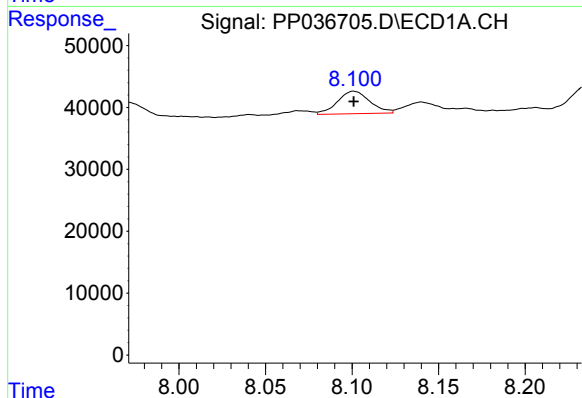


#29 AR-1254-4

R.T.: 8.101 min
Delta R.T.: 0.000 min
Response: 47444
Conc: 21.58 ng/ml

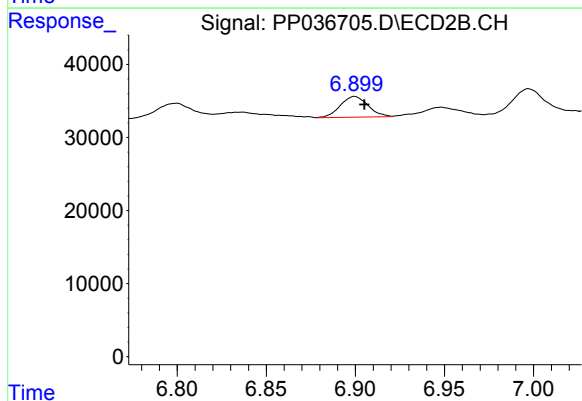


#29 AR-1254-4

R.T.: 6.900 min
Delta R.T.: -0.005 min
Response: 30723
Conc: 19.85 ng/ml

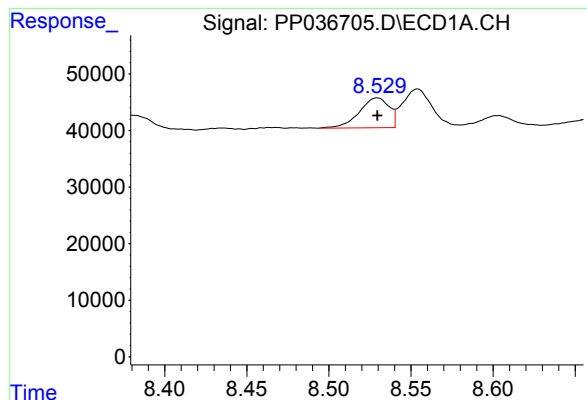

#30 AR-1254-5

R.T.: 8.530 min
Delta R.T.: 0.000 min
Response: 66944
Conc: 28.15 ng/ml

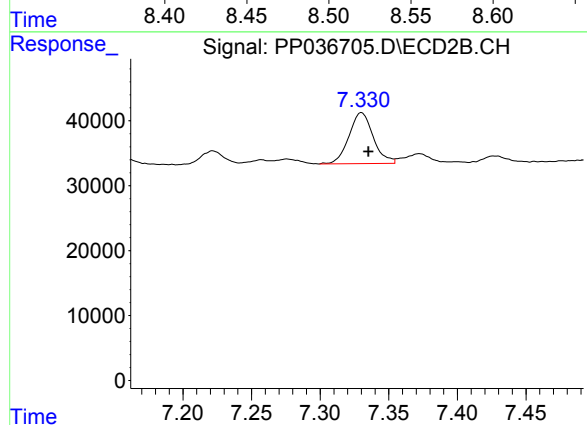

#30 AR-1254-5

R.T.: 7.330 min
Delta R.T.: -0.005 min
Response: 96710
Conc: 44.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS

Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:23 PM