

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
 Data File : PP036706.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 22:48
 Operator : DD\AJ
 Sample : M2789-25
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 06:45:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Instrument :
 ECD_P
 ClientSampleId :
 2ND-FLOORS

Manual Integrations
 APPROVED

Ankita
 6/23/2021 2:17:24 PM

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.957	313126	206889	7.085	6.680
2)	SA Decachlor...	10.998	9.256	799492	494182	18.637	15.453
Target Compounds							
21)	L5 AR-1248-1	6.282	5.209	82019	39035	81.302	56.023 #
22)	L5 AR-1248-2	6.578	5.473	72012	51718	53.026	54.602
23)	L5 AR-1248-3	6.797	5.517	86524	44151	53.178	44.622m
24)	L5 AR-1248-4	7.224	5.700	88591	41795	48.523	35.730 #
25)	L5 AR-1248-5	7.263	6.123	74034	38755	41.061m	32.672
26)	L6 AR-1254-1	7.193	6.080	226631	168086	128.866	99.203
27)	L6 AR-1254-2	7.422	6.240	333756	160978	123.352	108.228
28)	L6 AR-1254-3	7.804	6.660	230804	143546	77.921	59.044
29)	L6 AR-1254-4	8.099	6.900	177558	84402	80.769m	54.542 #
30)	L6 AR-1254-5	8.528	7.330	867663	534963	364.849	248.787 #
41)	L9 AR-1268-1	9.474	8.171	1953638	990754	325.633	212.764 #
42)	L9 AR-1268-2	9.570	8.235	1582470	1330246	277.609	308.386
43)	L9 AR-1268-3	9.798	8.444	699777	458709	145.553	125.636
44)	L9 AR-1268-4	10.241	8.732	1010943	641043	429.185	402.989
45)	L9 AR-1268-5	10.657	9.012	3103939	2083086	201.839	176.195

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
Data File : PP036706.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 22:48
Operator : DD\AJ
Sample : M2789-25
Misc :
ALS Vial : 31 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 06:45:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampled :
2ND-FLOORS

Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

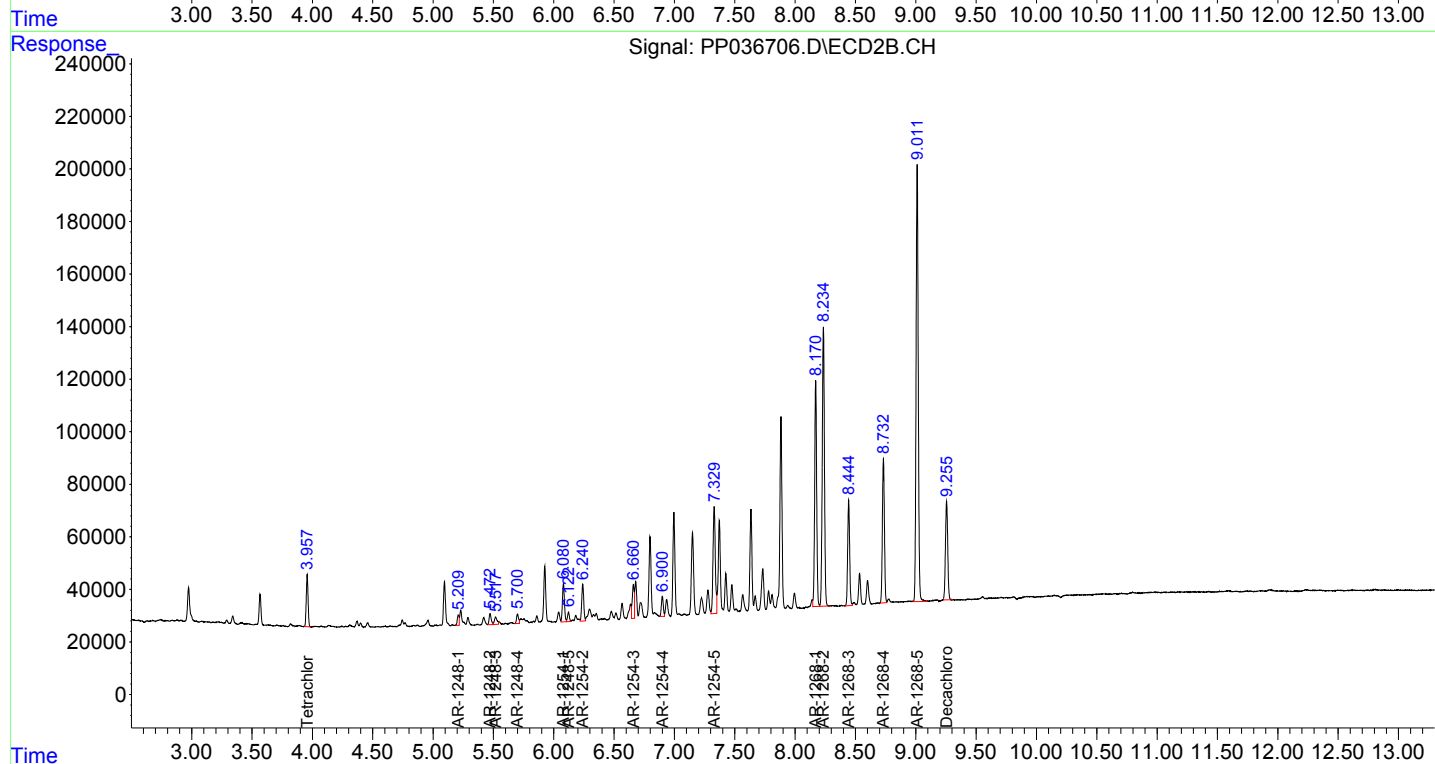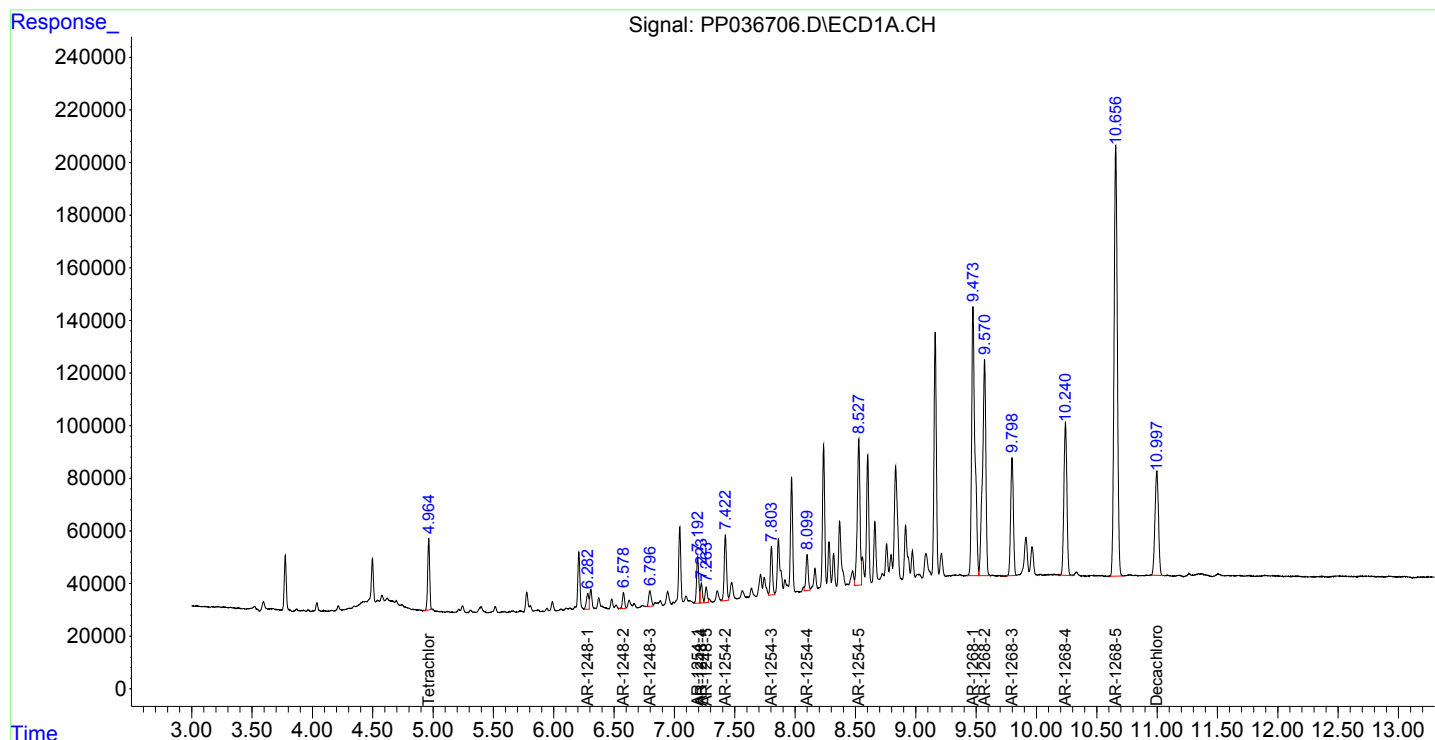

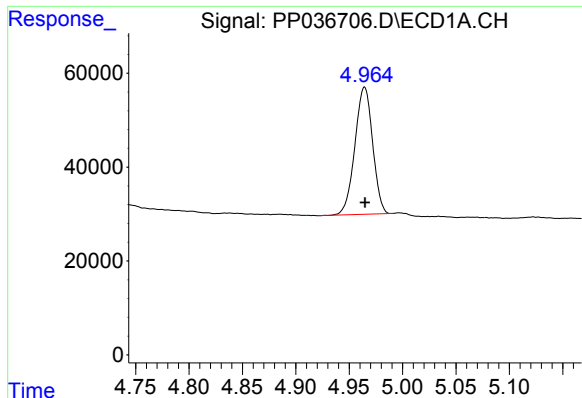


#1 Tetrachloro-m-xylene

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 313126
Conc: 7.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

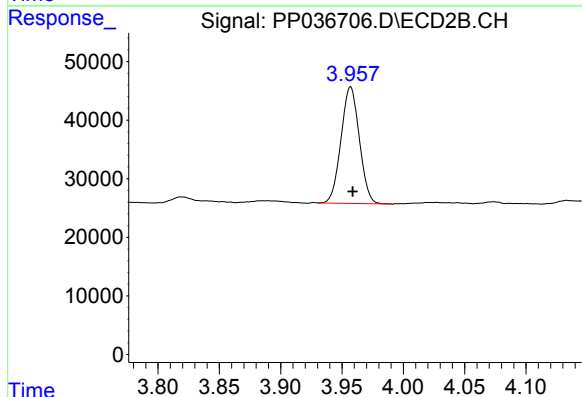


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.002 min
Response: 206889
Conc: 6.68 ng/ml

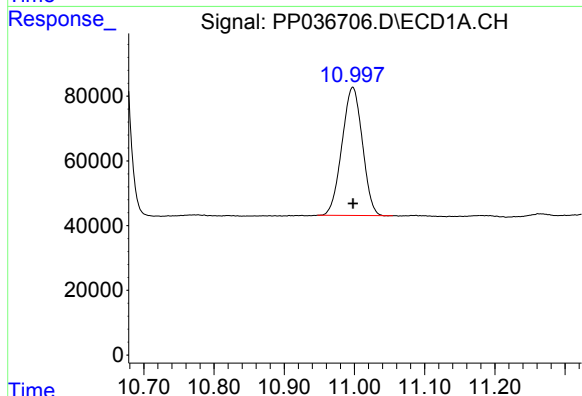


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 799492
Conc: 18.64 ng/ml

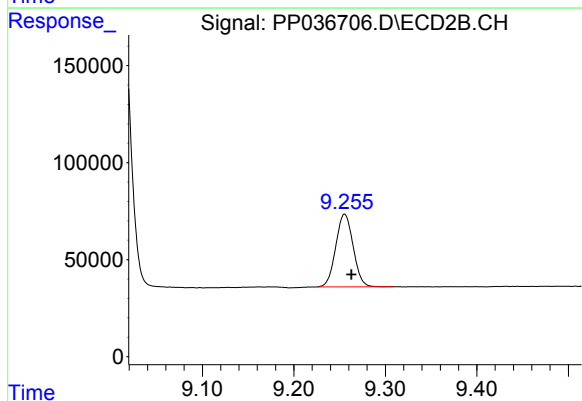

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.007 min
Response: 494182
Conc: 15.45 ng/ml

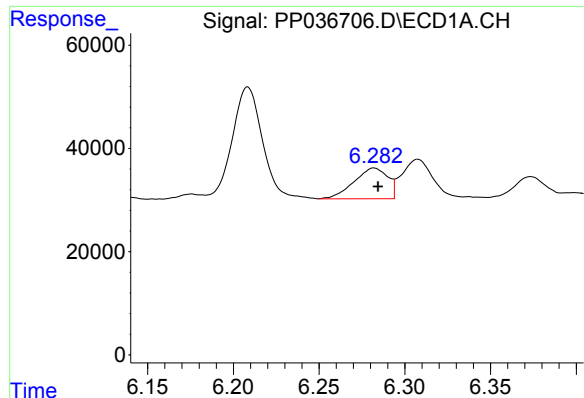


#21 AR-1248-1

R.T.: 6.282 min
Delta R.T.: -0.002 min
Response: 82019
Conc: 81.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

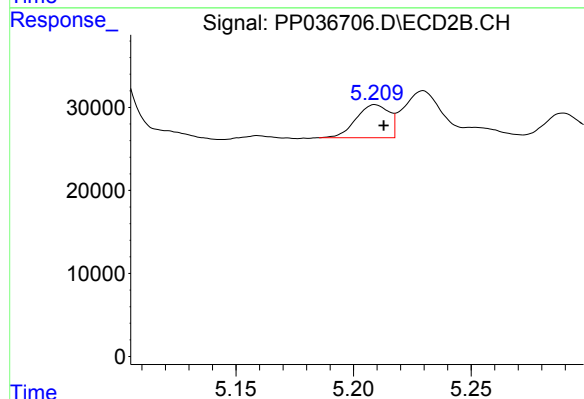


#21 AR-1248-1

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 39035
Conc: 56.02 ng/ml

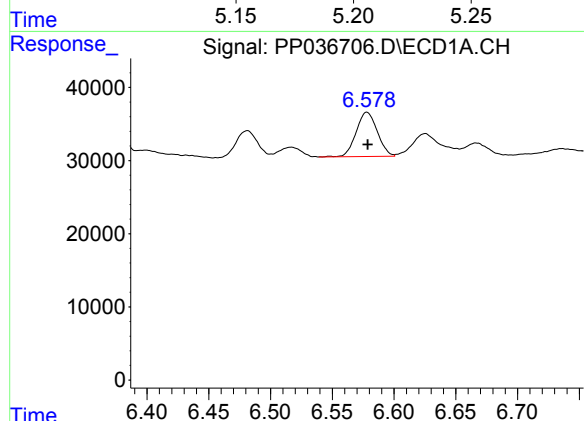


#22 AR-1248-2

R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 72012
Conc: 53.03 ng/ml

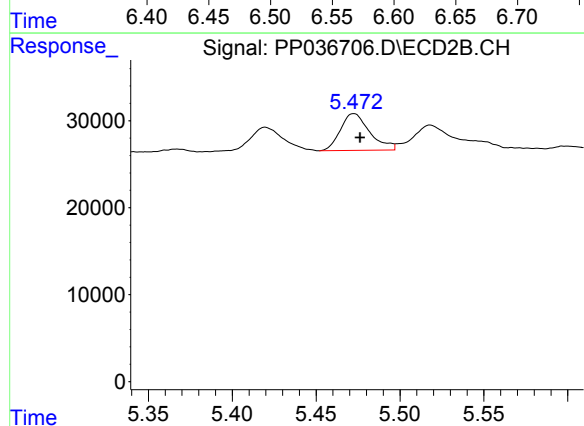

#22 AR-1248-2

R.T.: 5.473 min
Delta R.T.: -0.004 min
Response: 51718
Conc: 54.60 ng/ml

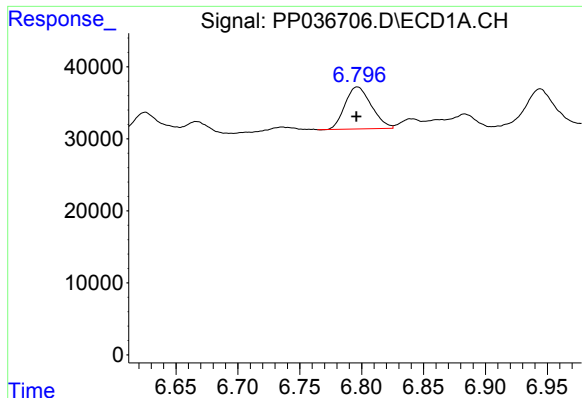

#23 AR-1248-3

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 86524
Conc: 53.18 ng/ml


Instrument :

ECD_P

ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

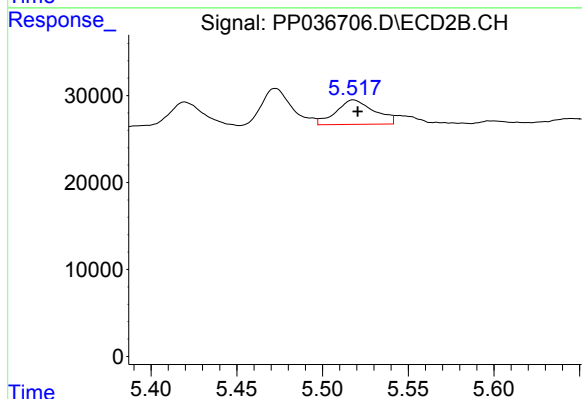


#23 AR-1248-3

R.T.: 5.517 min
Delta R.T.: -0.003 min
Response: 44151
Conc: 44.62 ng/ml m

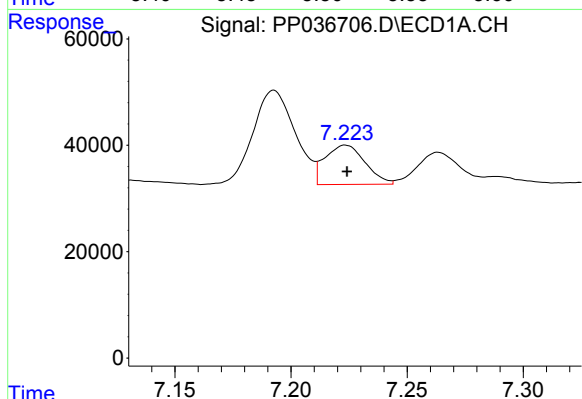


#24 AR-1248-4

R.T.: 7.224 min
Delta R.T.: 0.000 min
Response: 88591
Conc: 48.52 ng/ml

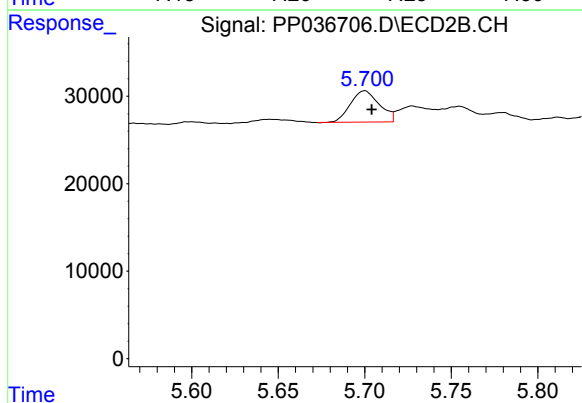

#24 AR-1248-4

R.T.: 5.700 min
Delta R.T.: -0.004 min
Response: 41795
Conc: 35.73 ng/ml

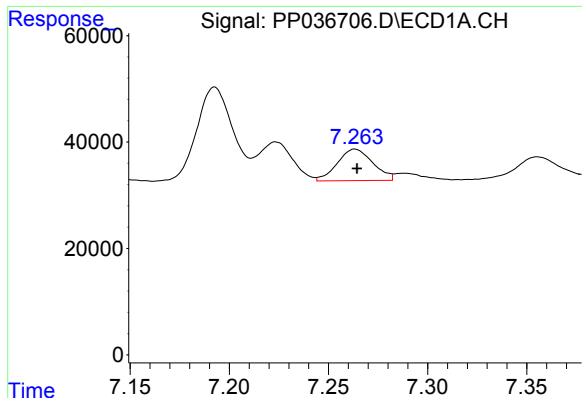


#25 AR-1248-5

R.T.: 7.263 min
Delta R.T.: -0.002 min
Response: 74034
Conc: 41.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

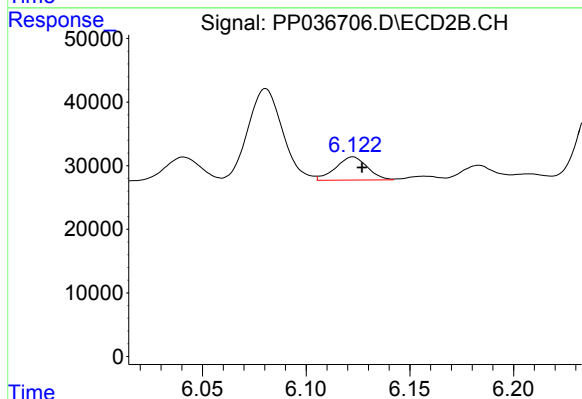


#25 AR-1248-5

R.T.: 6.123 min
Delta R.T.: -0.004 min
Response: 38755
Conc: 32.67 ng/ml

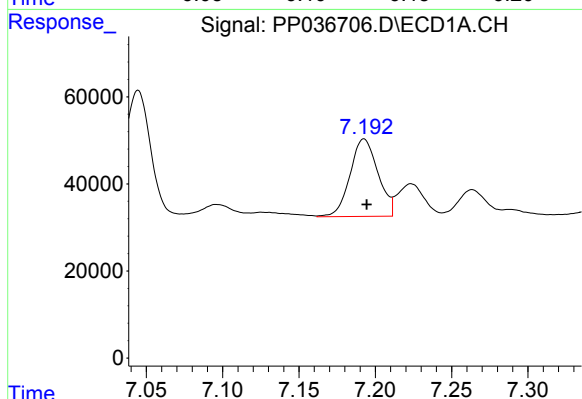


#26 AR-1254-1

R.T.: 7.193 min
Delta R.T.: -0.002 min
Response: 226631
Conc: 128.87 ng/ml

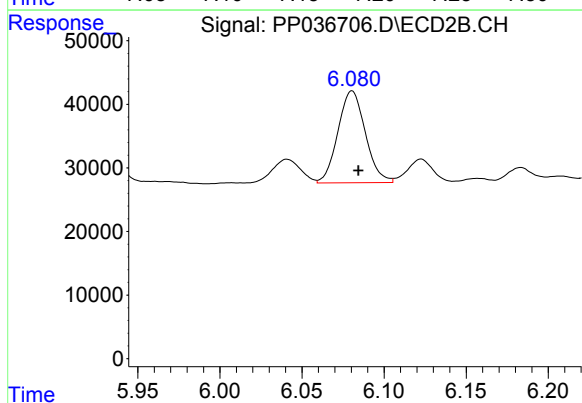

#26 AR-1254-1

R.T.: 6.080 min
Delta R.T.: -0.004 min
Response: 168086
Conc: 99.20 ng/ml

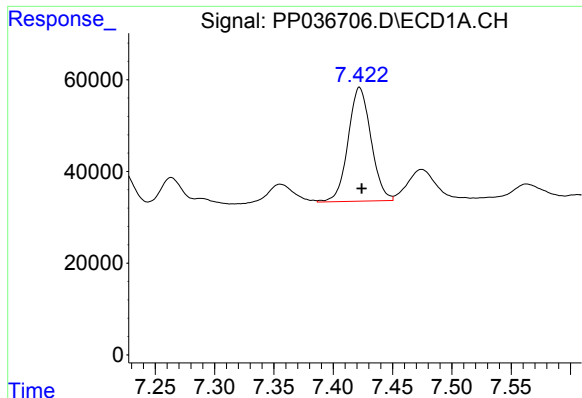


#27 AR-1254-2

R.T.: 7.422 min
Delta R.T.: -0.002 min
Response: 333756
Conc: 123.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

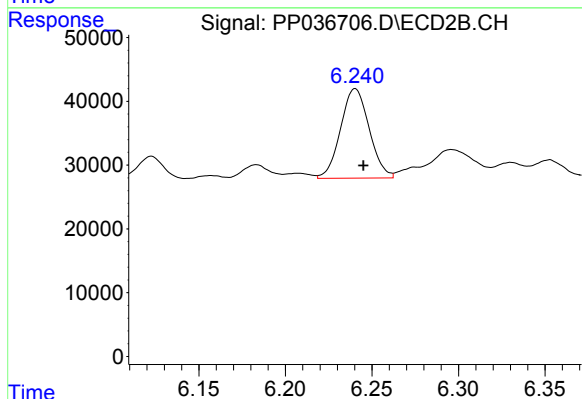


#27 AR-1254-2

R.T.: 6.240 min
Delta R.T.: -0.005 min
Response: 160978
Conc: 108.23 ng/ml

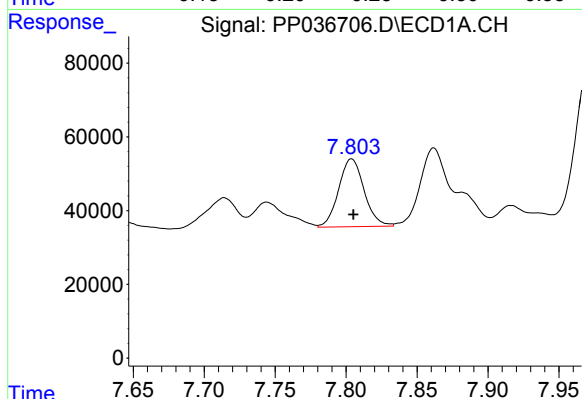


#28 AR-1254-3

R.T.: 7.804 min
Delta R.T.: -0.001 min
Response: 230804
Conc: 77.92 ng/ml

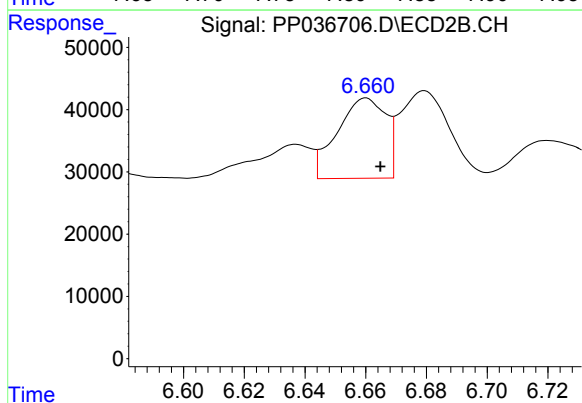

#28 AR-1254-3

R.T.: 6.660 min
Delta R.T.: -0.005 min
Response: 143546
Conc: 59.04 ng/ml

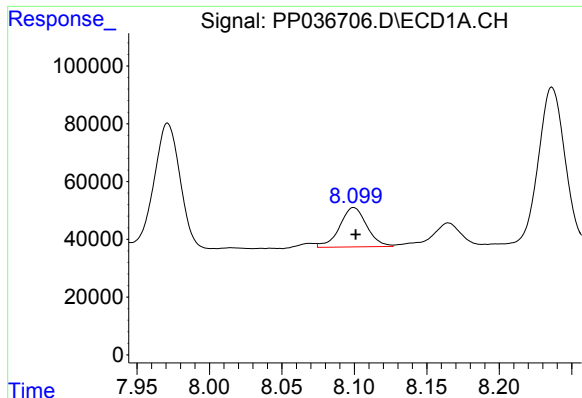


#29 AR-1254-4

R.T.: 8.099 min
Delta R.T.: -0.002 min
Response: 177558
Conc: 80.77 ng/ml m

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

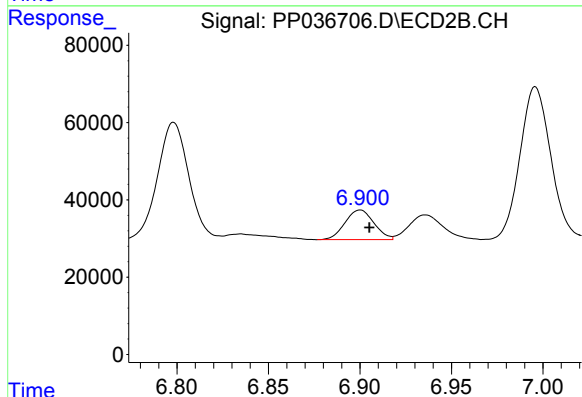


#29 AR-1254-4

R.T.: 6.900 min
Delta R.T.: -0.005 min
Response: 84402
Conc: 54.54 ng/ml

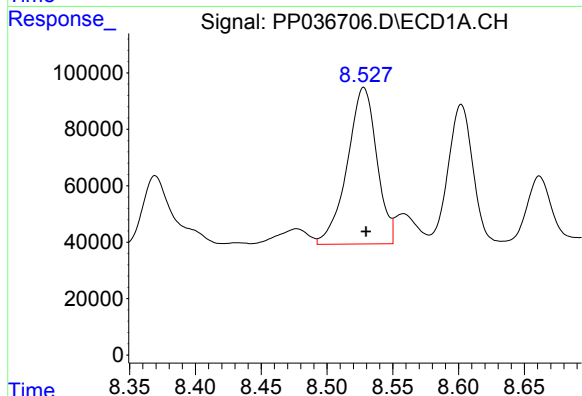


#30 AR-1254-5

R.T.: 8.528 min
Delta R.T.: -0.002 min
Response: 867663
Conc: 364.85 ng/ml

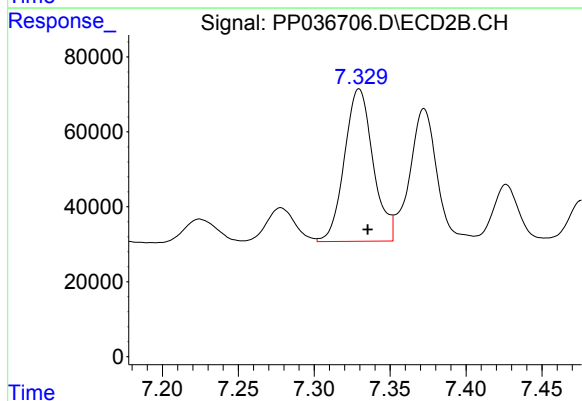

#30 AR-1254-5

R.T.: 7.330 min
Delta R.T.: -0.006 min
Response: 534963
Conc: 248.79 ng/ml

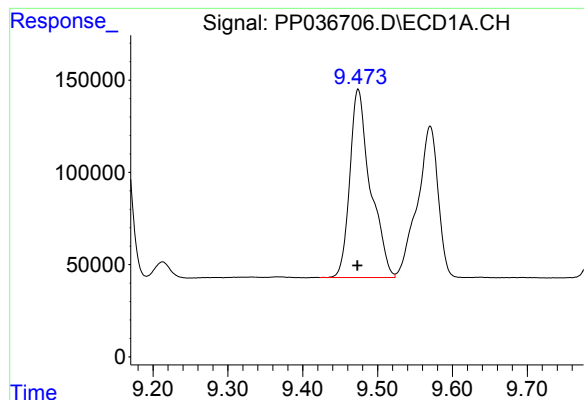


#41 AR-1268-1

R.T.: 9.474 min
Delta R.T.: 0.000 min
Response: 1953638
Conc: 325.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

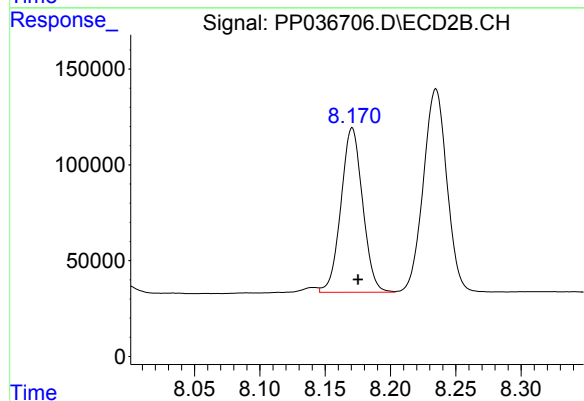


#41 AR-1268-1

R.T.: 8.171 min
Delta R.T.: -0.005 min
Response: 990754
Conc: 212.76 ng/ml

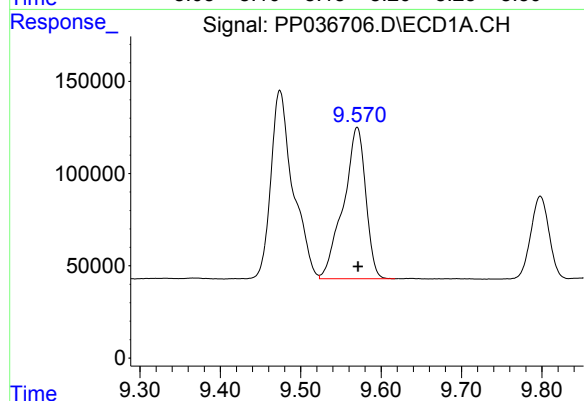


#42 AR-1268-2

R.T.: 9.570 min
Delta R.T.: -0.001 min
Response: 1582470
Conc: 277.61 ng/ml

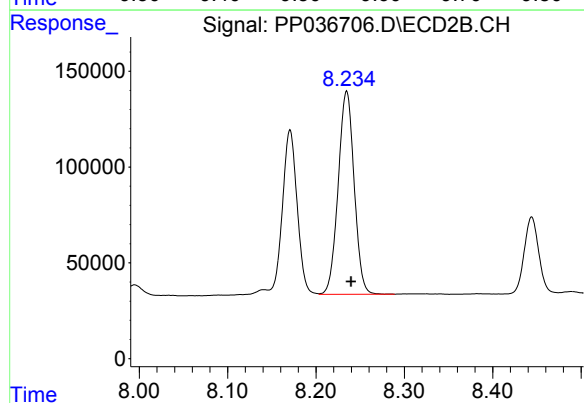

#42 AR-1268-2

R.T.: 8.235 min
Delta R.T.: -0.005 min
Response: 1330246
Conc: 308.39 ng/ml

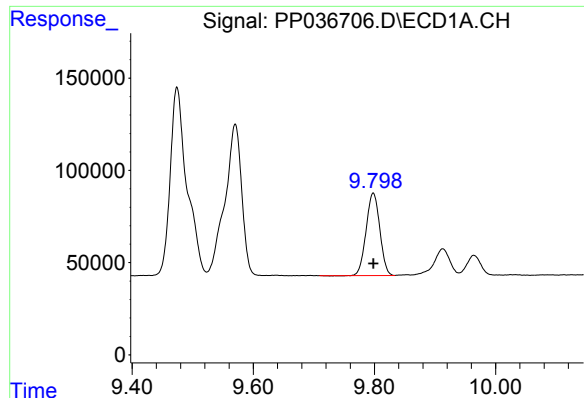


#43 AR-1268-3

R.T.: 9.798 min
Delta R.T.: 0.000 min
Response: 699777
Conc: 145.55 ng/ml

Instrument :
ECD_P
ClientSampled :
2ND-FLOORS


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM

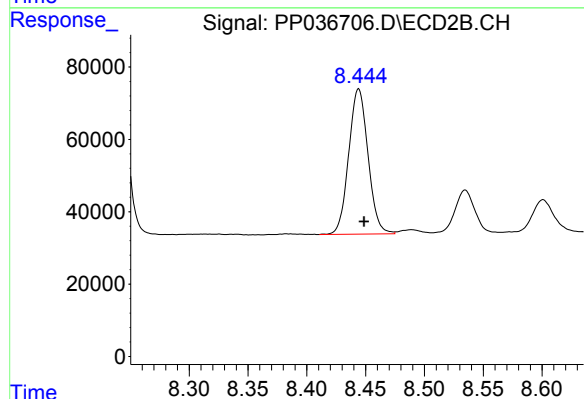


#43 AR-1268-3

R.T.: 8.444 min
Delta R.T.: -0.005 min
Response: 458709
Conc: 125.64 ng/ml

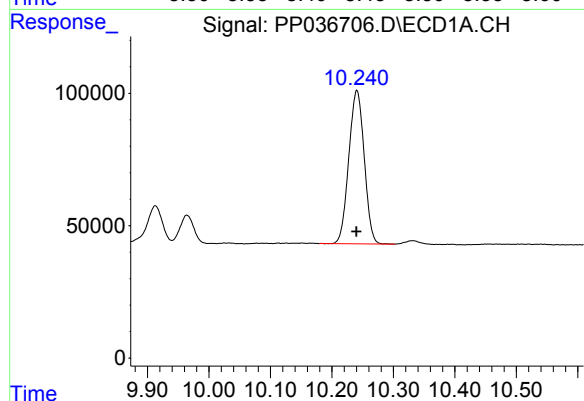


#44 AR-1268-4

R.T.: 10.241 min
Delta R.T.: 0.000 min
Response: 1010943
Conc: 429.18 ng/ml

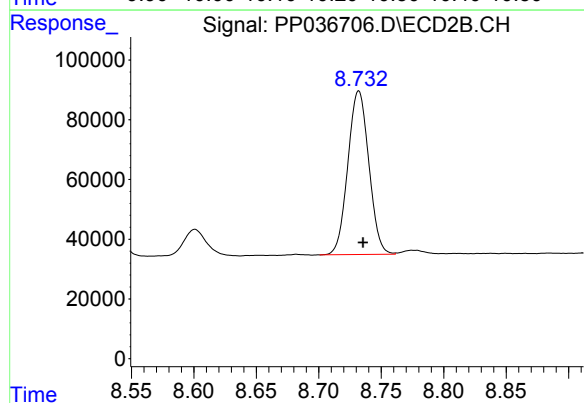

#44 AR-1268-4


R.T.: 8.732 min
Delta R.T.: -0.004 min
Response: 641043
Conc: 402.99 ng/ml

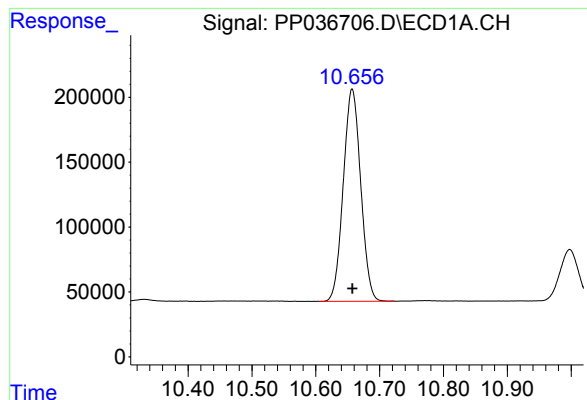

#45 AR-1268-5

R.T.: 10.657 min
Delta R.T.: 0.000 min
Response: 3103939
Conc: 201.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
2ND-FLOORS

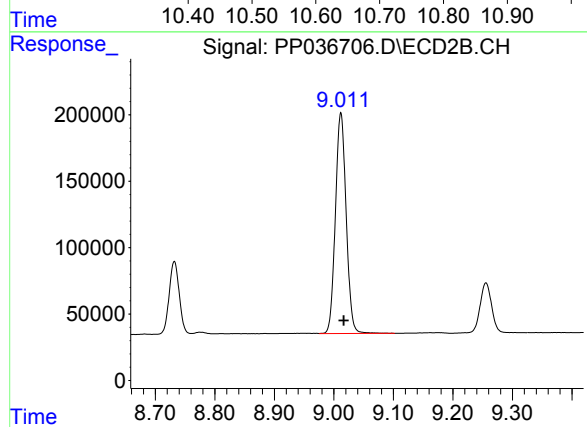

#45 AR-1268-5

R.T.: 9.012 min
Delta R.T.: -0.005 min
Response: 2083086
Conc: 176.19 ng/ml

Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:24 PM