

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
 Data File : PP036710.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 00:30
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 06:48:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.957	2412944	1727371	54.593	55.770
2)	SA Decachlor...	10.997	9.256	2424353	1629376	56.515	50.949
Target Compounds							
26)	L6 AR-1254-1	7.193	6.079	1109200	974031	630.707	574.865m
27)	L6 AR-1254-2	7.422	6.239	1367309	746593	505.341m	501.944m
28)	L6 AR-1254-3	7.804	6.659	1534844	1226064	518.170	504.311m
29)	L6 AR-1254-4	8.100	6.900	1132822	780211	515.306	504.183
30)	L6 AR-1254-5	8.529	7.329	1228508	1099115	516.583	511.148

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sample ID :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 6/23/2021 2:17:29 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062221\
Data File : PP036710.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 00:30
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 06:48:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:29 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

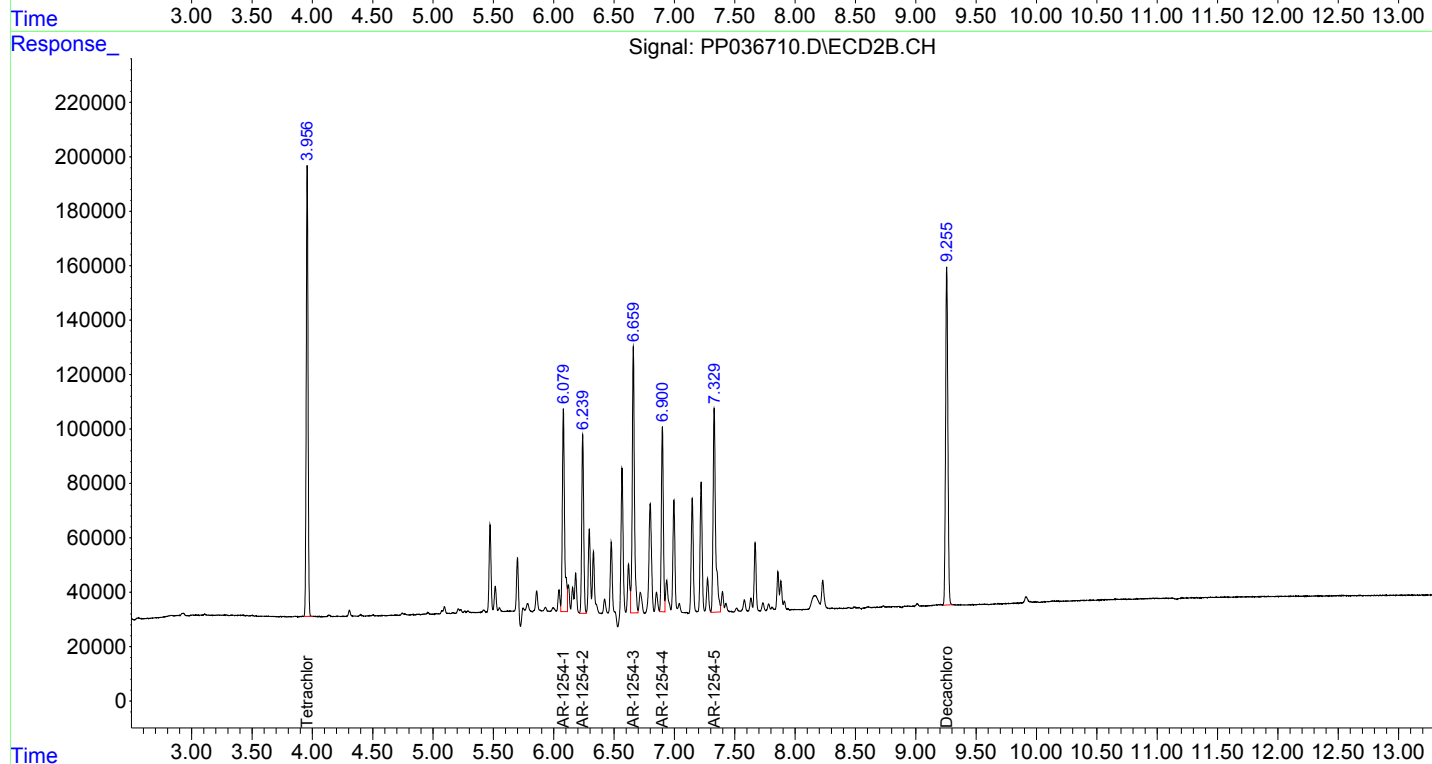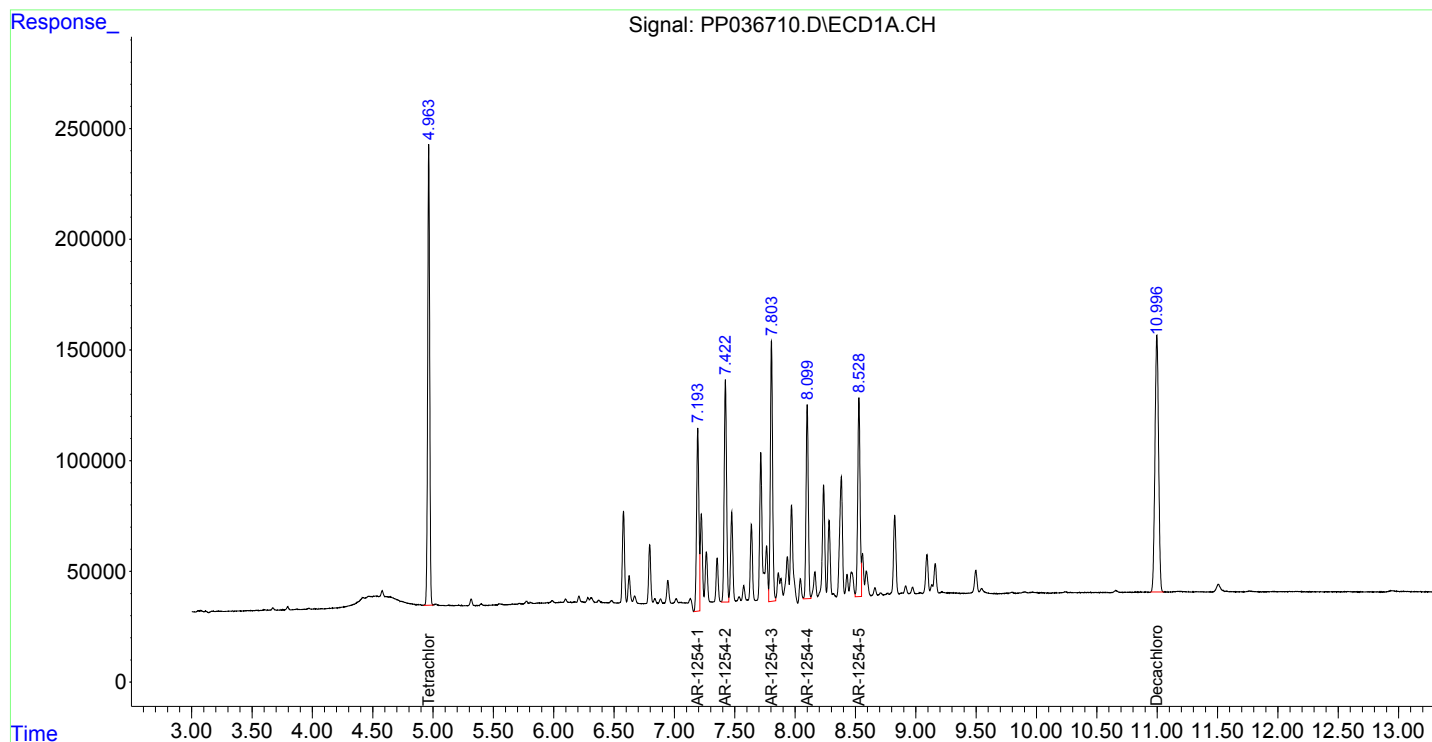

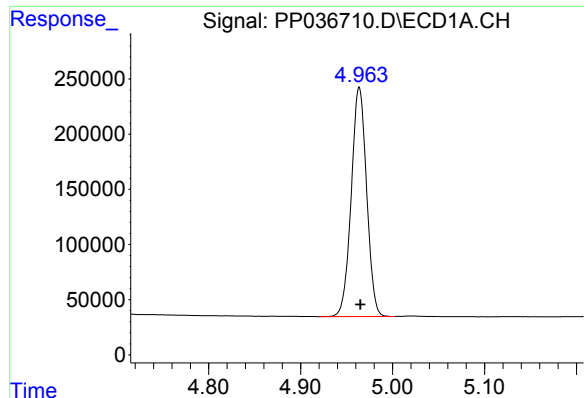


#1 Tetrachloro-m-xylene

R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 2412944
Conc: 54.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:29 PM

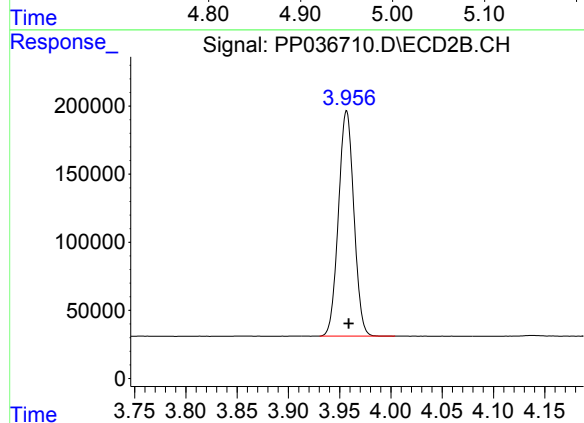


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.002 min
Response: 1727371
Conc: 55.77 ng/ml

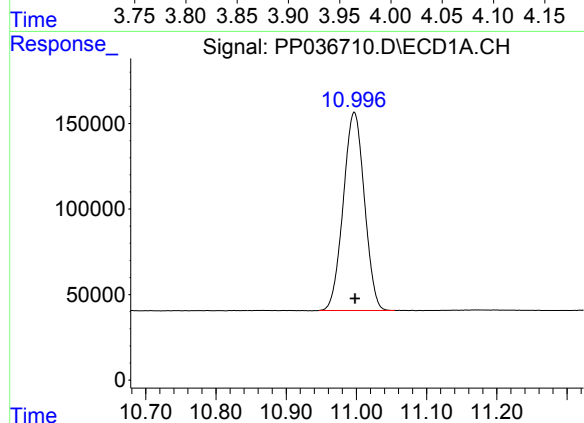


#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 2424353
Conc: 56.52 ng/ml

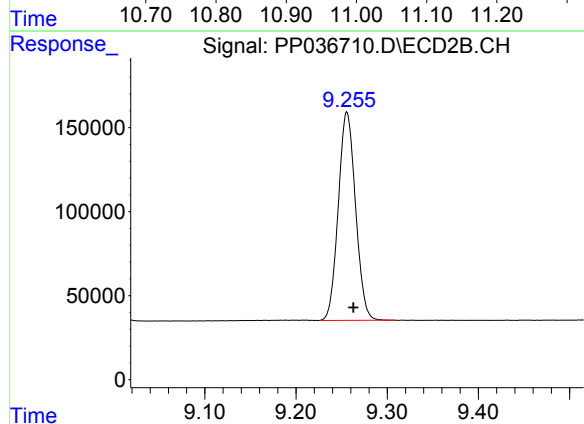

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.007 min
Response: 1629376
Conc: 50.95 ng/ml

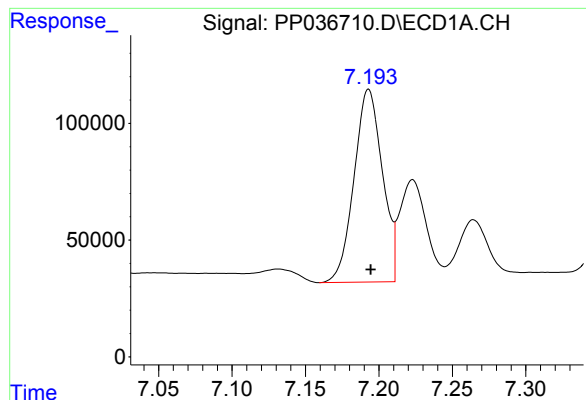


#26 AR-1254-1

R.T.: 7.193 min
Delta R.T.: -0.001 min
Response: 1109200
Conc: 630.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:29 PM

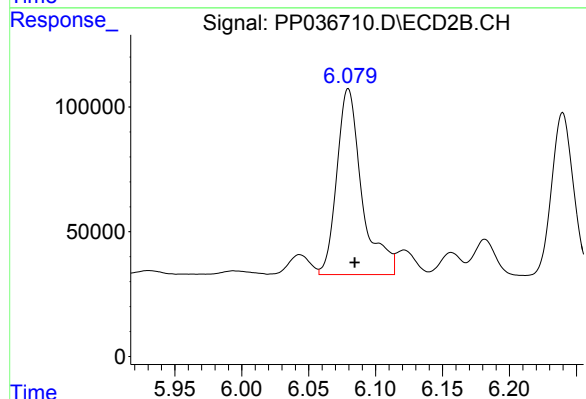


#26 AR-1254-1

R.T.: 6.079 min
Delta R.T.: -0.005 min
Response: 974031
Conc: 574.86 ng/ml m

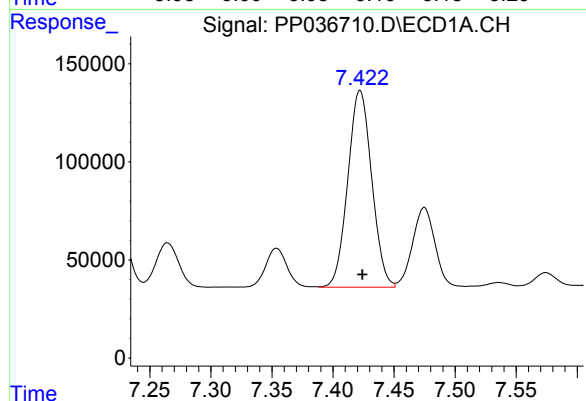


#27 AR-1254-2

R.T.: 7.422 min
Delta R.T.: -0.002 min
Response: 1367309
Conc: 505.34 ng/ml m

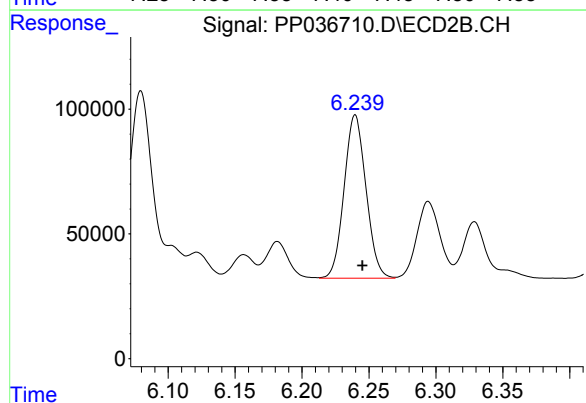

#27 AR-1254-2

R.T.: 6.239 min
Delta R.T.: -0.006 min
Response: 746593
Conc: 501.94 ng/ml m

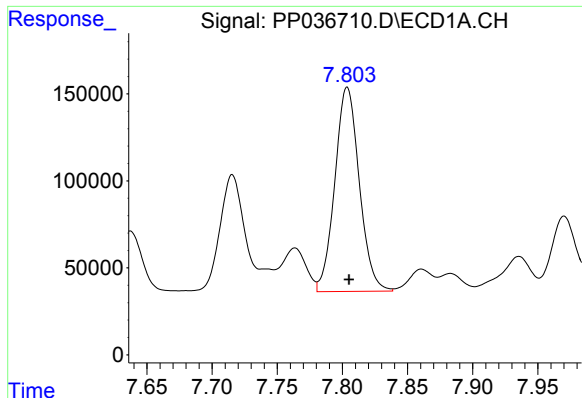


#28 AR-1254-3

R.T.: 7.804 min
Delta R.T.: -0.001 min
Response: 1534844
Conc: 518.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:29 PM

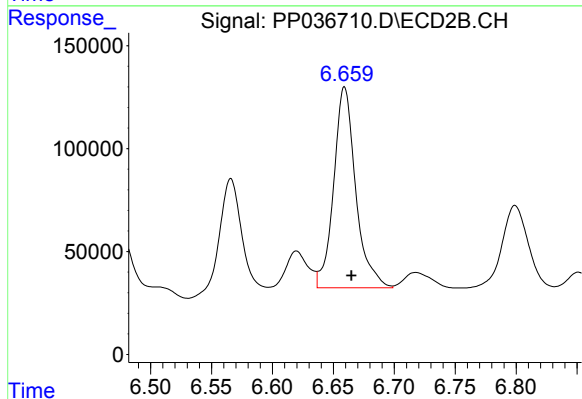


#28 AR-1254-3

R.T.: 6.659 min
Delta R.T.: -0.006 min
Response: 1226064
Conc: 504.31 ng/ml m

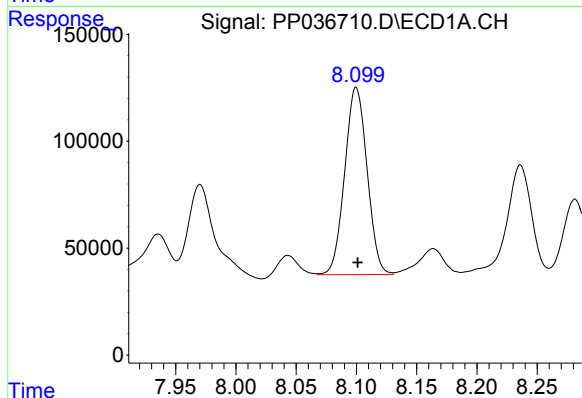


#29 AR-1254-4

R.T.: 8.100 min
Delta R.T.: -0.001 min
Response: 1132822
Conc: 515.31 ng/ml

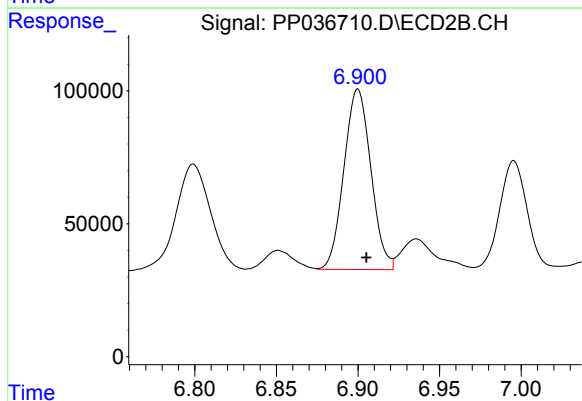


#29 AR-1254-4

R.T.: 6.900 min
Delta R.T.: -0.005 min
Response: 780211
Conc: 504.18 ng/ml

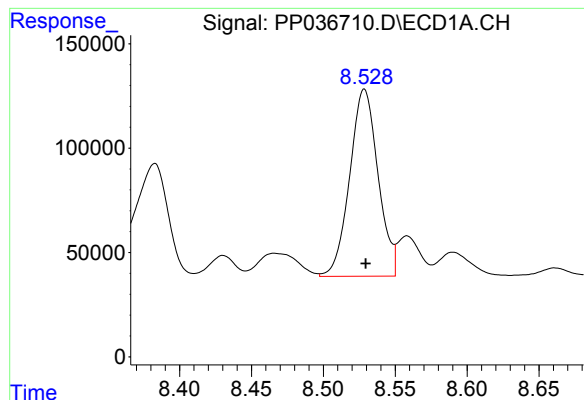

#30 AR-1254-5

R.T.: 8.529 min
Delta R.T.: -0.001 min
Response: 1228508
Conc: 516.58 ng/ml

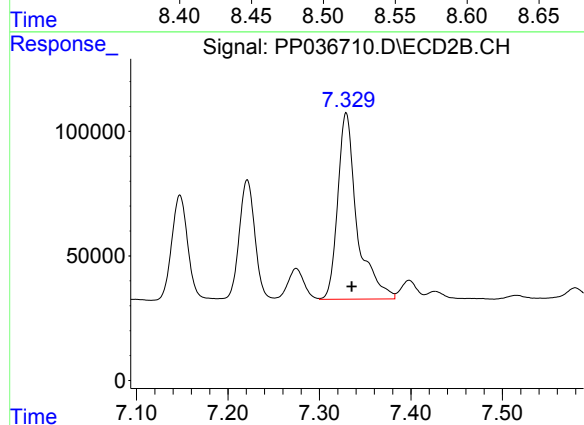

#30 AR-1254-5

R.T.: 7.329 min
Delta R.T.: -0.006 min
Response: 1099115
Conc: 511.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
6/23/2021 2:17:29 PM