

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036719.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 9:12
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:16:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.956	21300	11368	0.482	0.367
Target Compounds							
3)	L1 AR-1016-1	6.287	0.000	9463	0	5.587	N.D. #
4)	L1 AR-1016-2	6.287f	0.000	9463	0	3.924	N.D. #
12)	L3 AR-1232-2	6.013f	0.000	1628	0	2.961	N.D. #
13)	L3 AR-1232-3	6.287f	0.000	9463	0	9.263	N.D. #
16)	L4 AR-1242-1	6.287	0.000	9463	0	7.379	N.D. #
17)	L4 AR-1242-2	6.287f	0.000	9463	0	5.186	N.D. #
21)	L5 AR-1248-1	6.287	0.000	9463	0	9.380	N.D. #
24)	L5 AR-1248-4	7.229	0.000	13401	0	7.340	N.D. #
26)	L6 AR-1254-1	7.202	0.000	22793	0	12.960	N.D. #
28)	L6 AR-1254-3	7.820f	0.000	17115	0	5.778	N.D. #
30)	L6 AR-1254-5	8.550f	0.000	32927	0	13.846	N.D. #
32)	L7 AR-1260-2	8.238	0.000	16627	0	6.487	N.D. #
33)	L7 AR-1260-3	0.000	7.148	0	15791	N.D.	8.683 #
35)	L7 AR-1260-5	9.161	0.000	4272	0	0.957	N.D. #
37)	L8 AR-1262-2	9.161	0.000	4272	0	0.841	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036719.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 9:12
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:16:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

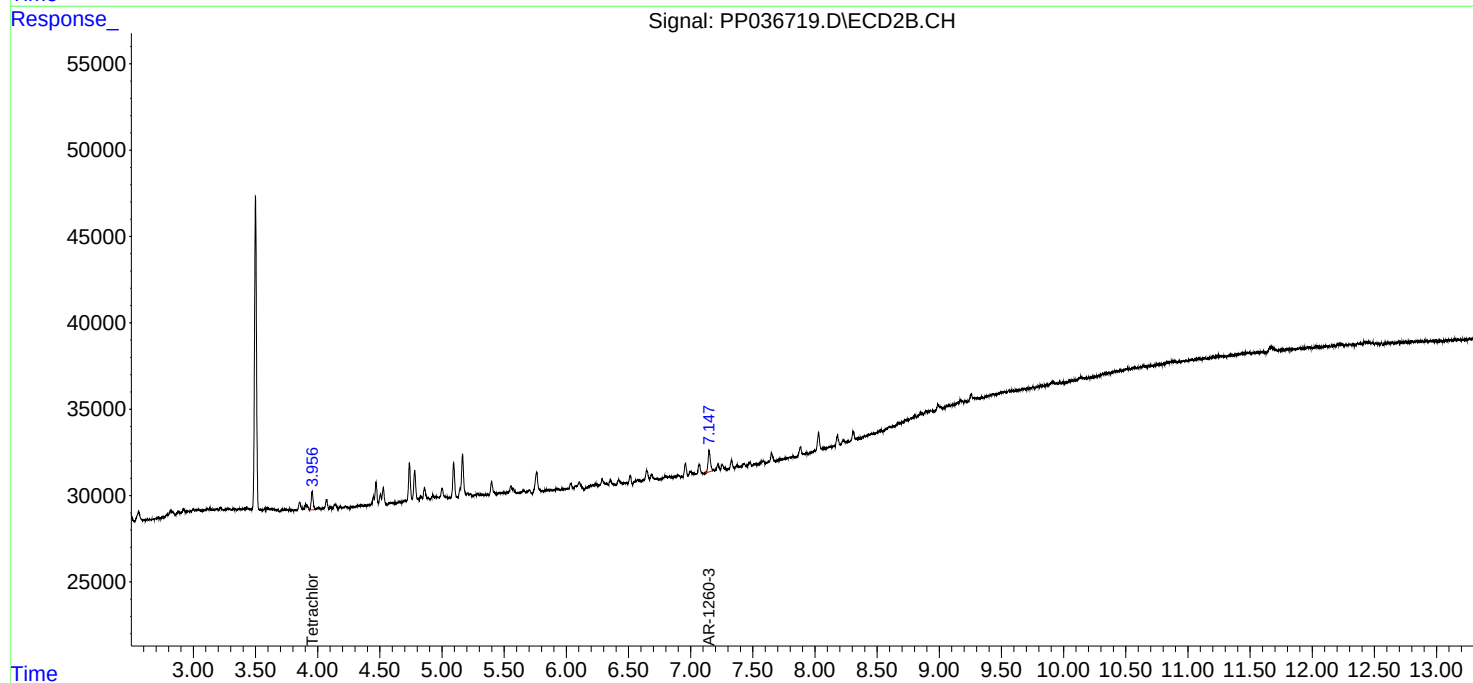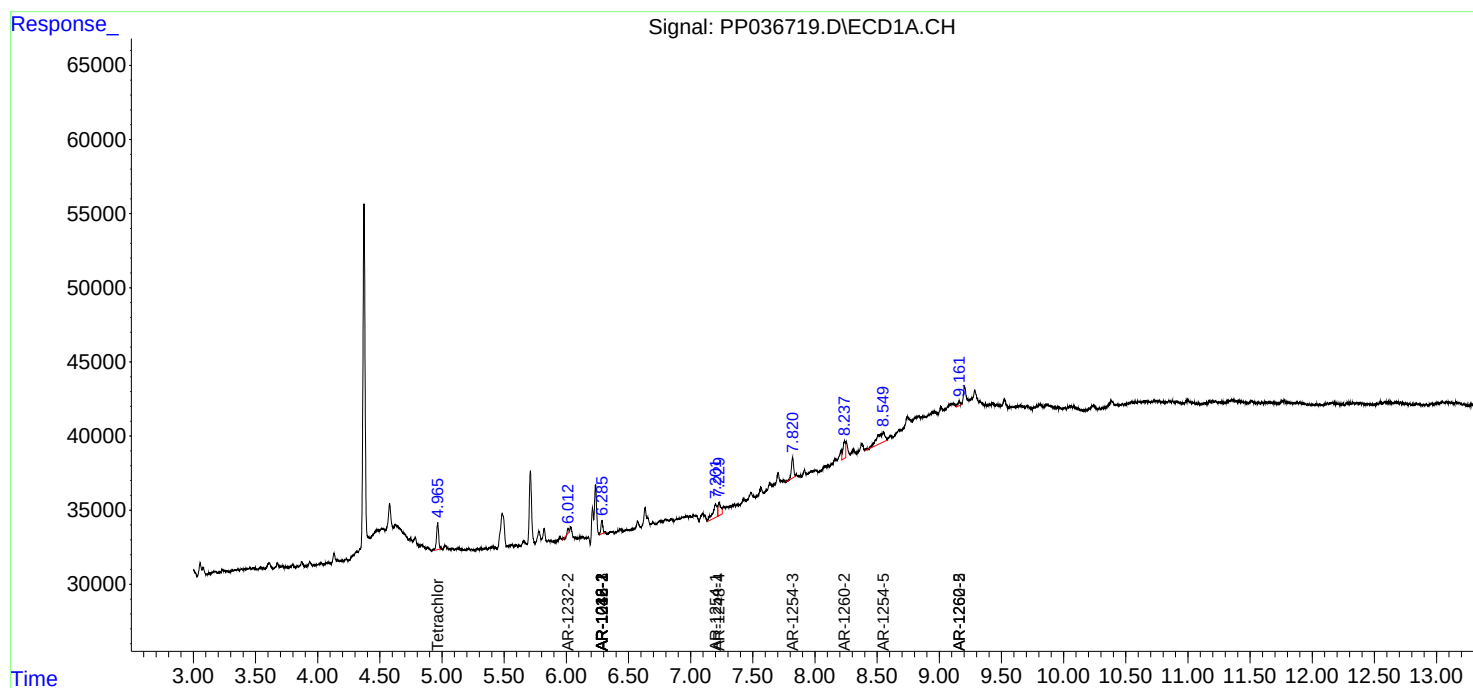


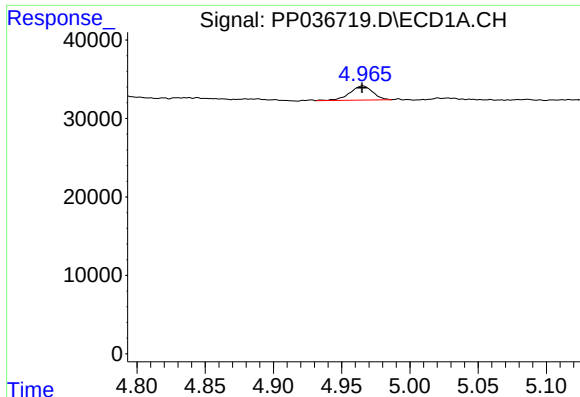

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 21300
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

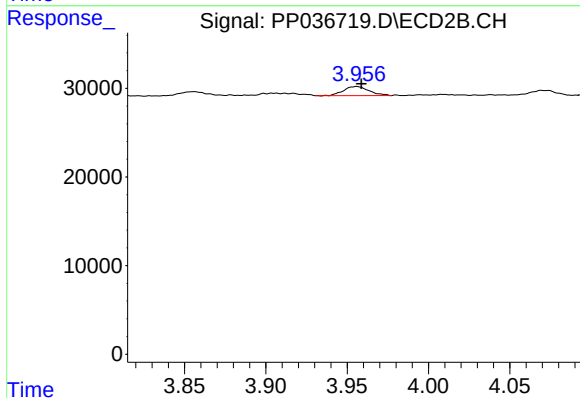


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.003 min
Response: 11368
Conc: 0.37 ng/ml

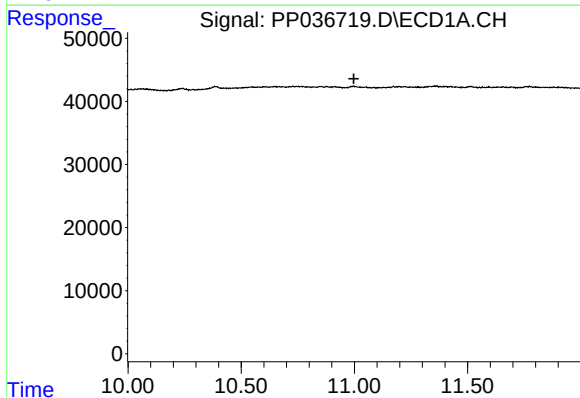


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.998 min
Response: 0
Conc: N.D.

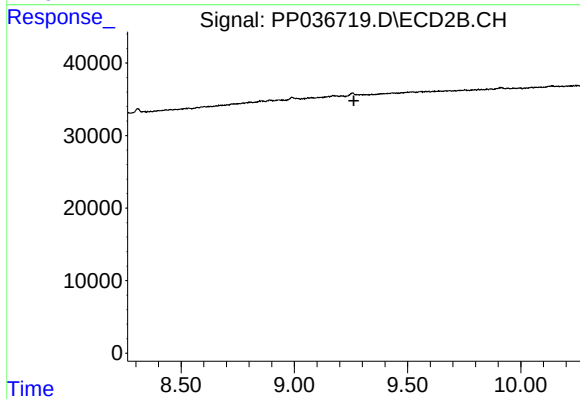

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.263 min
Response: 0
Conc: N.D.

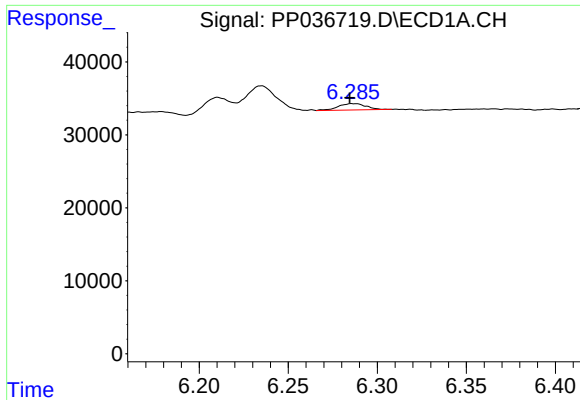

#3 AR-1016-1


R.T.: 6.287 min
Delta R.T.: 0.002 min
Response: 9463
Conc: 5.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

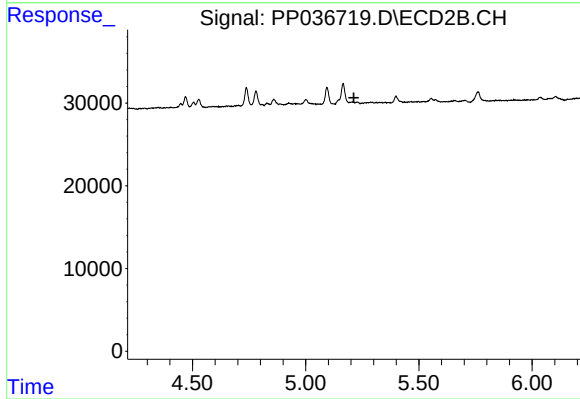


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

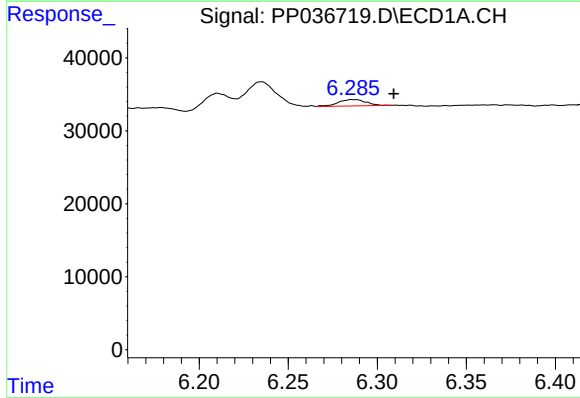


#4 AR-1016-2

R.T.: 6.287 min
Delta R.T.: -0.023 min
Response: 9463
Conc: 3.92 ng/ml

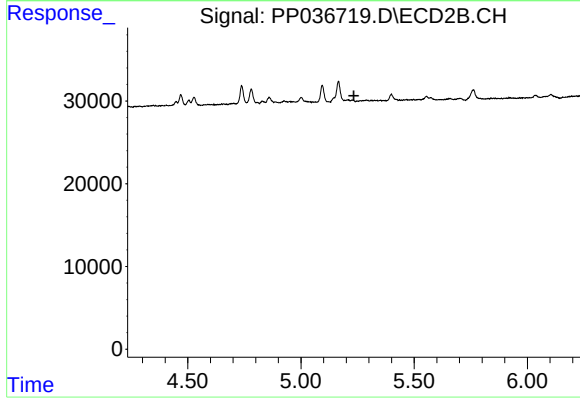

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 5.234 min
Response: 0
Conc: N.D.

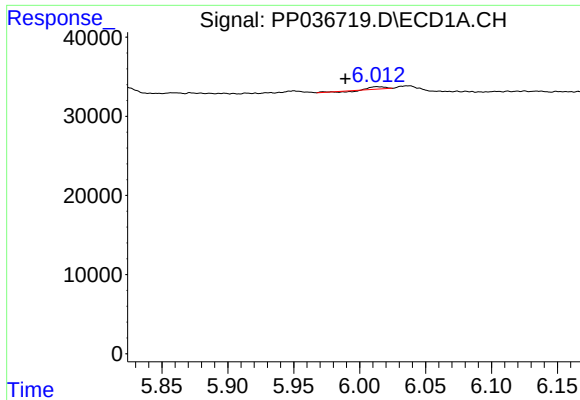

#12 AR-1232-2


R.T.: 6.013 min
Delta R.T.: 0.024 min
Response: 1628
Conc: 2.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

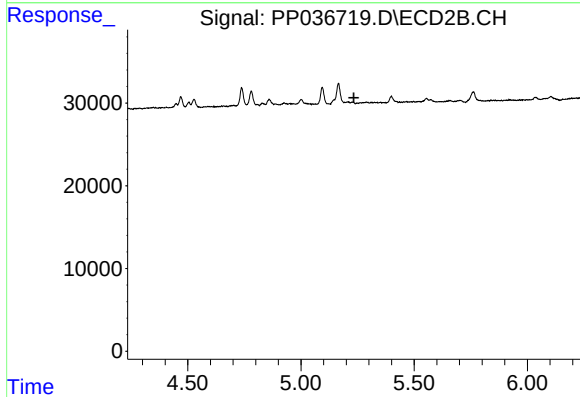


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.234 min
Response: 0
Conc: N.D.

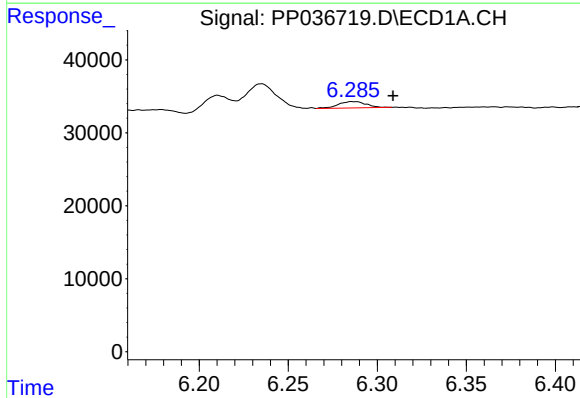


#13 AR-1232-3

R.T.: 6.287 min
Delta R.T.: -0.022 min
Response: 9463
Conc: 9.26 ng/ml

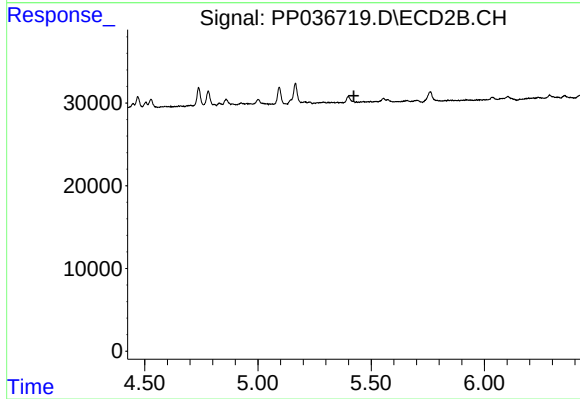

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.424 min
Response: 0
Conc: N.D.

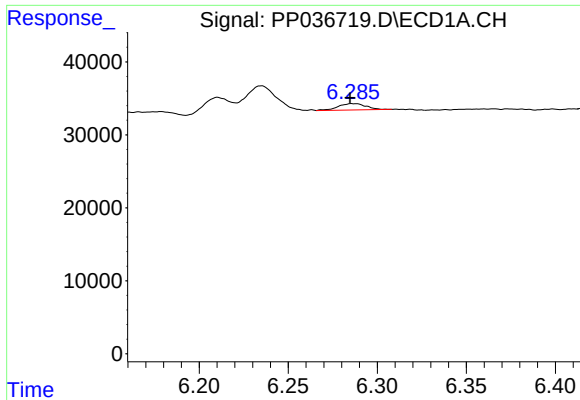

#16 AR-1242-1


R.T.: 6.287 min
Delta R.T.: 0.002 min
Response: 9463
Conc: 7.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

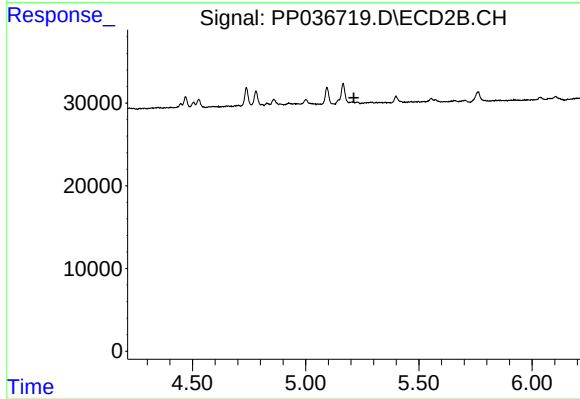


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

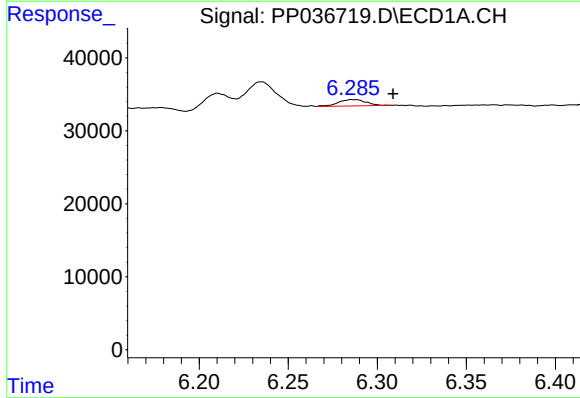


#17 AR-1242-2

R.T.: 6.287 min
Delta R.T.: -0.022 min
Response: 9463
Conc: 5.19 ng/ml

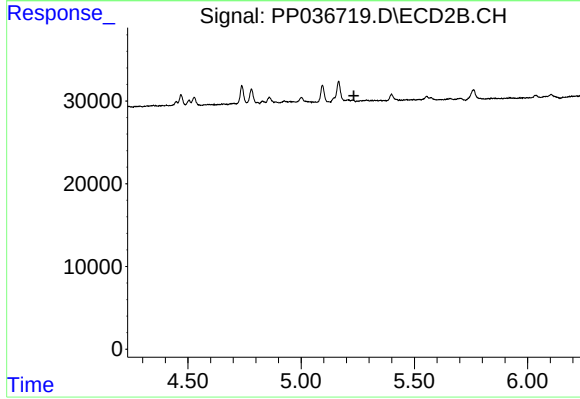

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

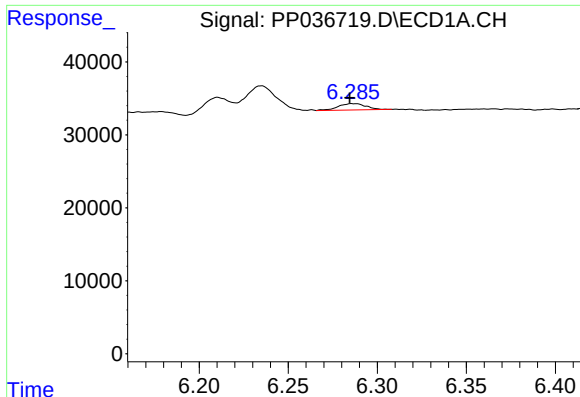

#21 AR-1248-1


R.T.: 6.287 min
Delta R.T.: 0.002 min
Response: 9463
Conc: 9.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

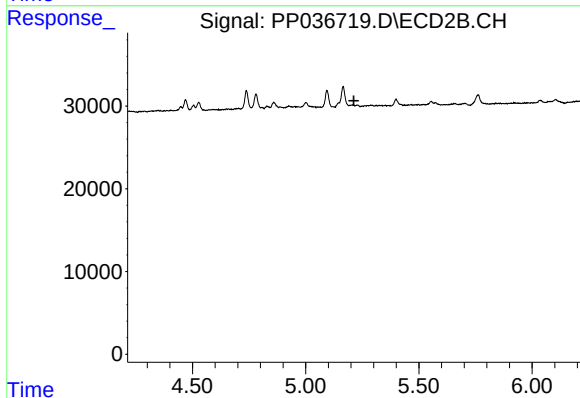


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

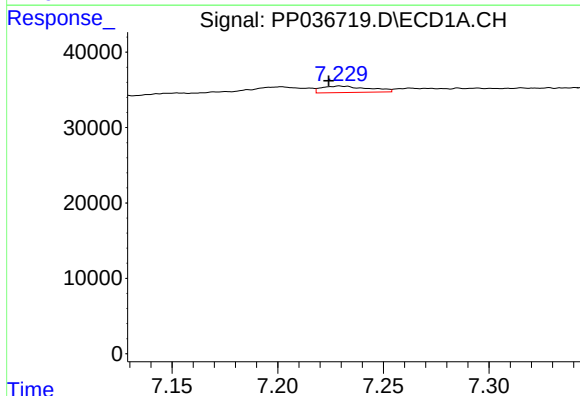


#24 AR-1248-4

R.T.: 7.229 min
Delta R.T.: 0.005 min
Response: 13401
Conc: 7.34 ng/ml

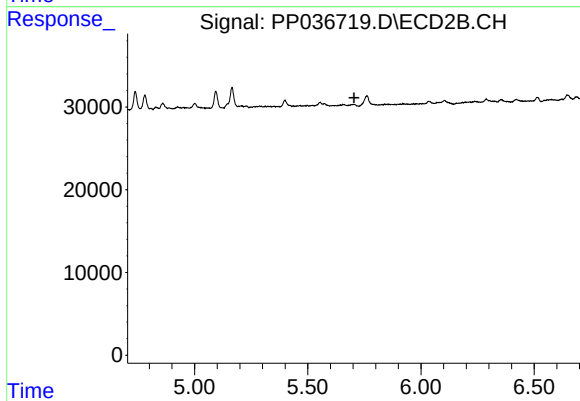

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

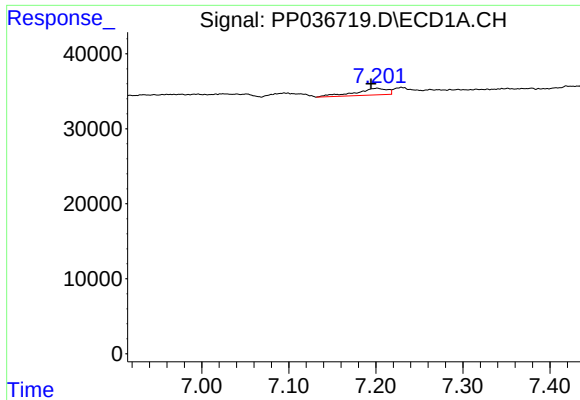

#26 AR-1254-1


R.T.: 7.202 min
Delta R.T.: 0.007 min
Response: 22793
Conc: 12.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

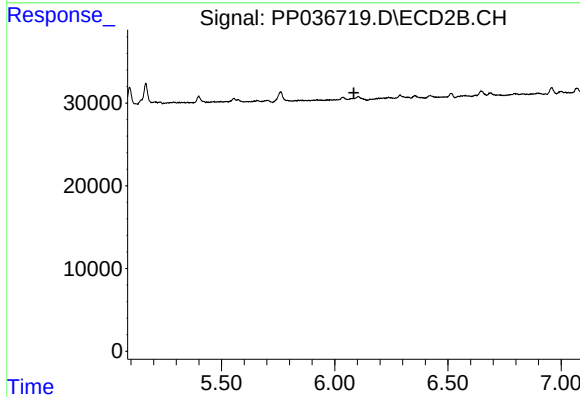


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

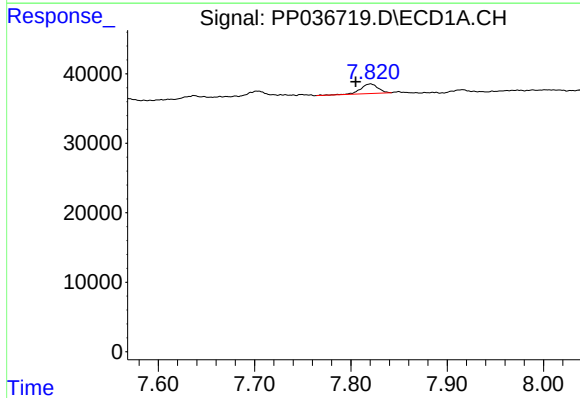


#28 AR-1254-3

R.T.: 7.820 min
Delta R.T.: 0.015 min
Response: 17115
Conc: 5.78 ng/ml

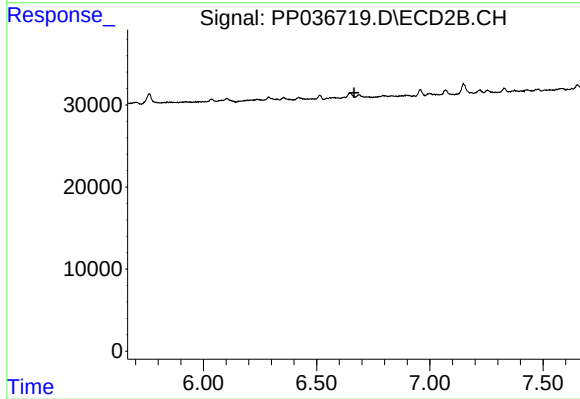

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

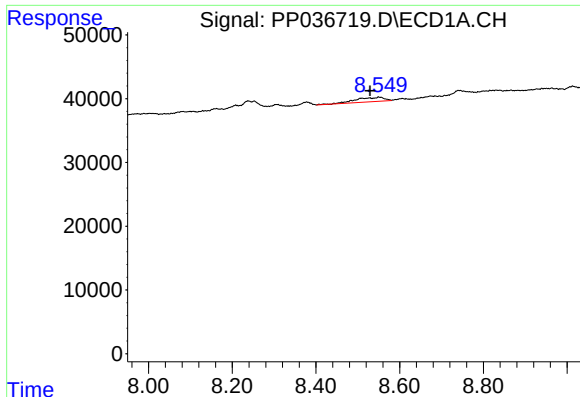

#30 AR-1254-5


R.T.: 8.550 min
Delta R.T.: 0.020 min
Response: 32927
Conc: 13.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

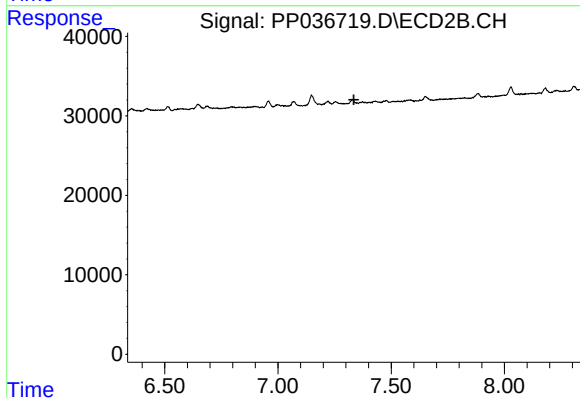


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.335 min
Response: 0
Conc: N.D.

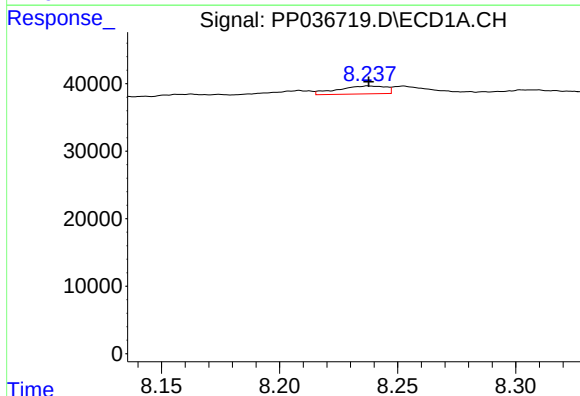


#32 AR-1260-2

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 16627
Conc: 6.49 ng/ml

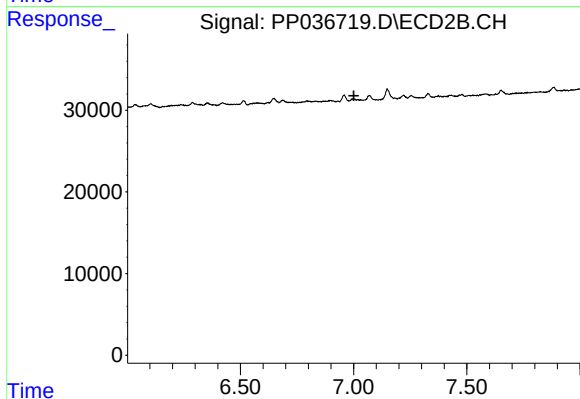

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.001 min
Response: 0
Conc: N.D.

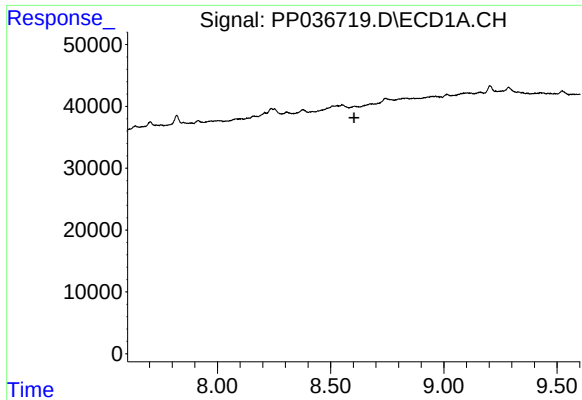

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

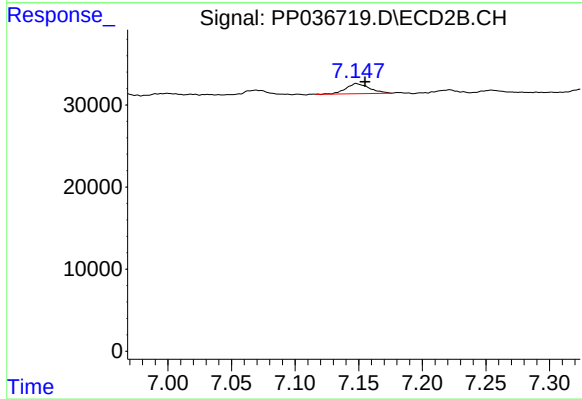


#33 AR-1260-3

R.T.: 7.148 min
Delta R.T.: -0.007 min
Response: 15791
Conc: 8.68 ng/ml

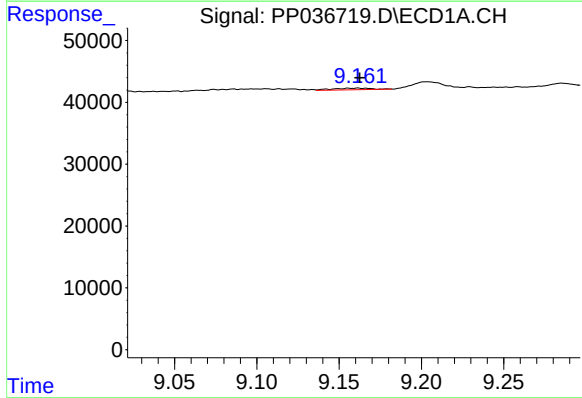


#35 AR-1260-5

R.T.: 9.161 min
Delta R.T.: -0.001 min
Response: 4272
Conc: 0.96 ng/ml

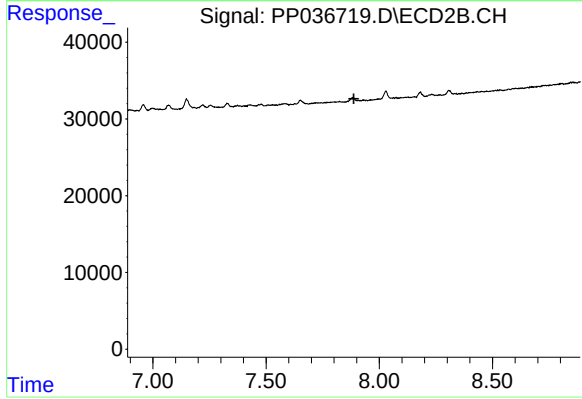

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.888 min
Response: 0
Conc: N.D.

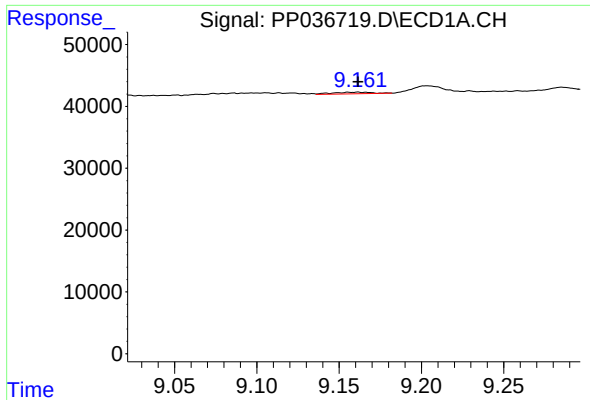

#37 AR-1262-2

R.T.: 9.161 min
Delta R.T.: 0.000 min
Response: 4272
Conc: 0.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

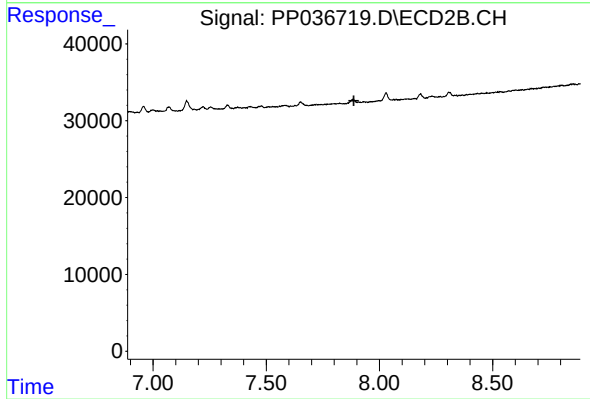

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.887 min
Response: 0
Conc: N.D.