

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036739.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 15:13
 Operator : DD\AJ
 Sample : M2795-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B3-6-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:22:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.963	3.955	914318	630000	20.687	20.340
2)	SA Decachlor...	10.993	9.252	771370	464423	17.982	14.522
Target Compounds							
8)	L2 AR-1221-1	5.213	0.000	105759	0	188.380	N.D. #
9)	L2 AR-1221-2	5.313	4.304	12452	8291	28.895	27.777
24)	L5 AR-1248-4	7.200f	0.000	2778	0	1.522	N.D. #
26)	L6 AR-1254-1	7.200	0.000	2778	0	1.580	N.D. #
28)	L6 AR-1254-3	7.816	6.657	14710	11427	4.966	4.700
30)	L6 AR-1254-5	8.533	0.000	37972	0	15.967	N.D. #
45)	L9 AR-1268-5	10.651	0.000	16311	0	1.061	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036739.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 15:13
Operator : DD\AJ
Sample : M2795-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
B3-6-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:22:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

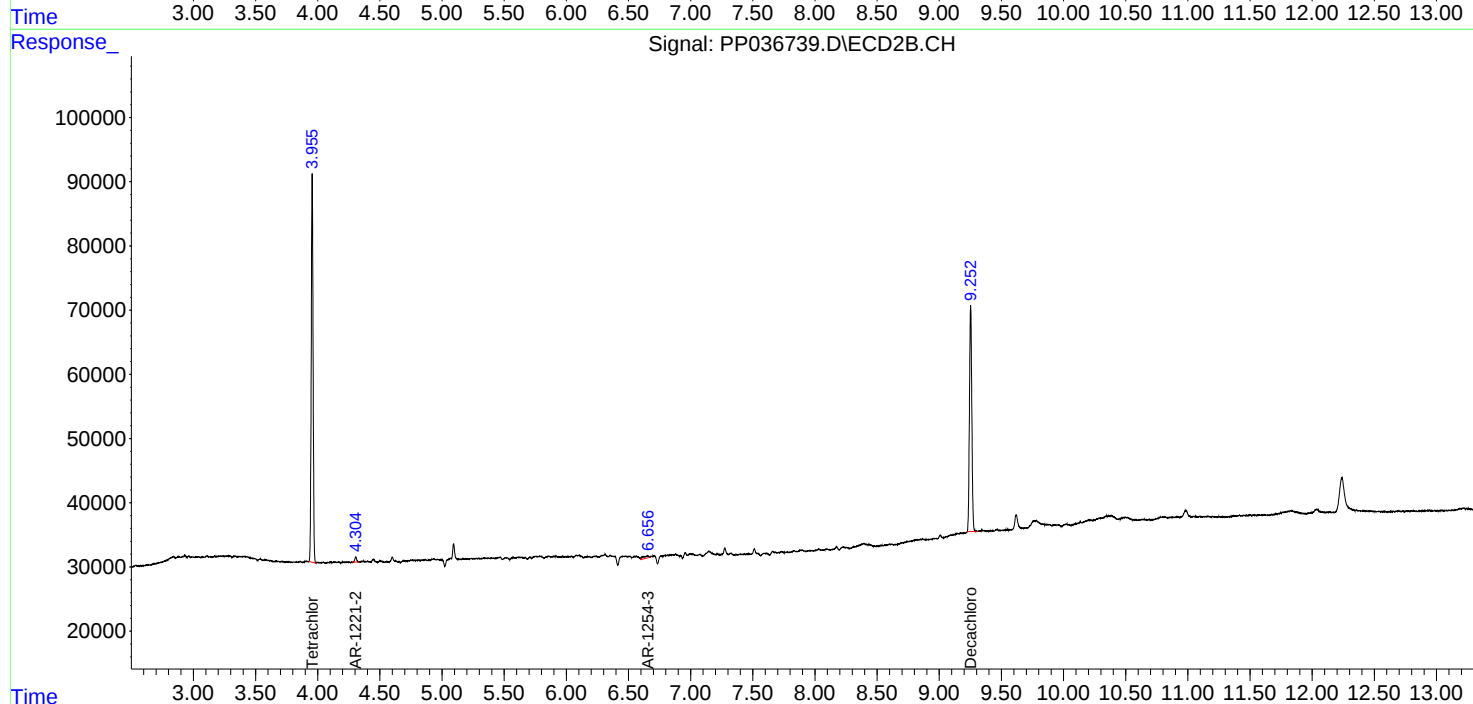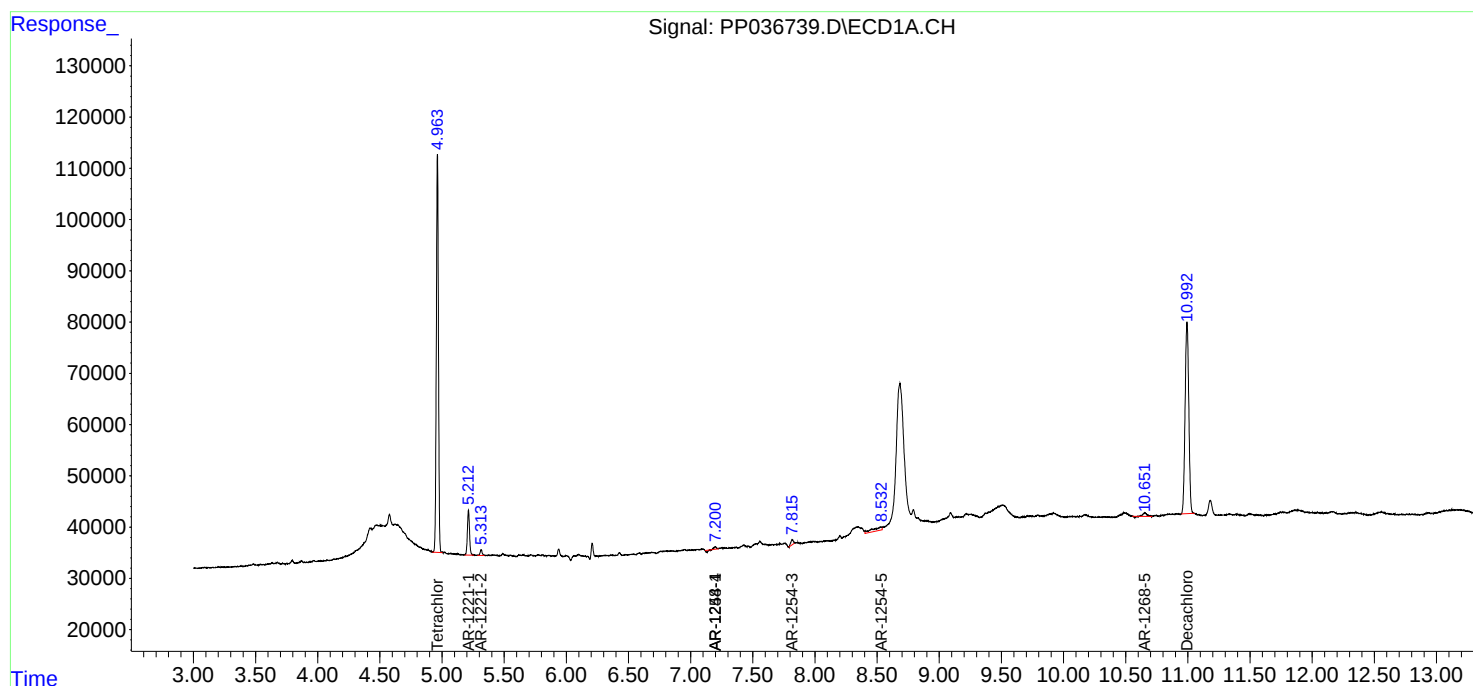


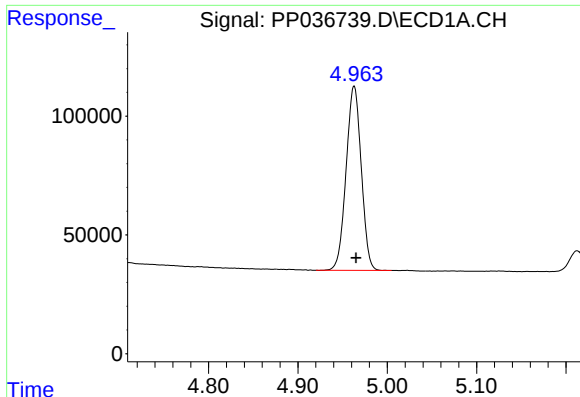

#1 Tetrachloro-m-xylene


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 914318
Conc: 20.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
B3-6-8

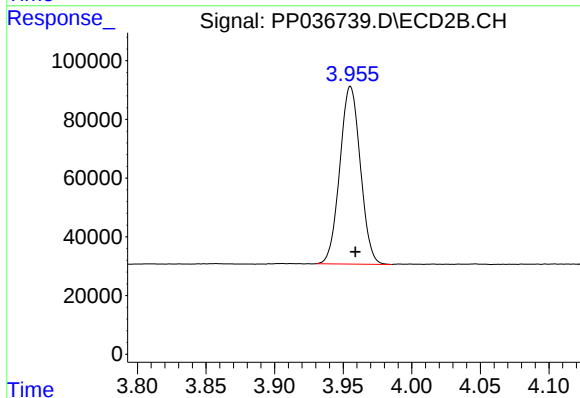


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.003 min
Response: 630000
Conc: 20.34 ng/ml

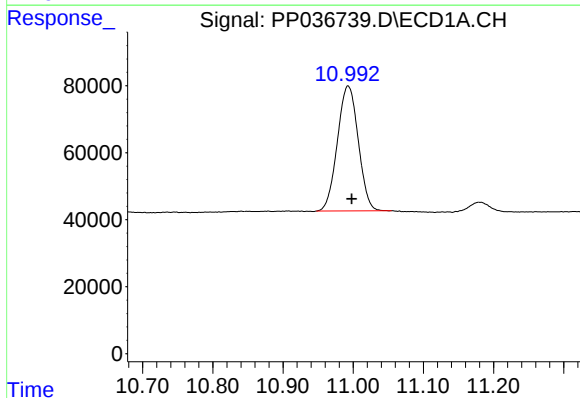


#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 771370
Conc: 17.98 ng/ml

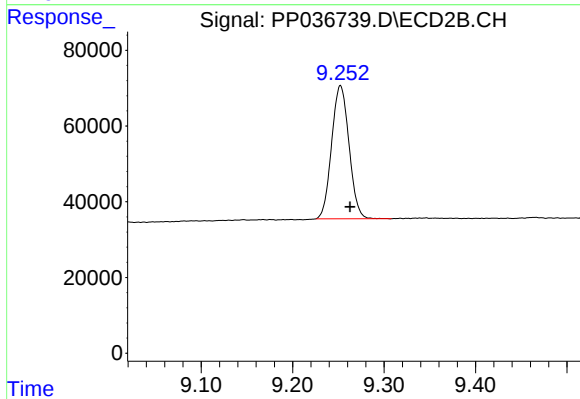

#2 Decachlorobiphenyl


R.T.: 9.252 min
Delta R.T.: -0.011 min
Response: 464423
Conc: 14.52 ng/ml

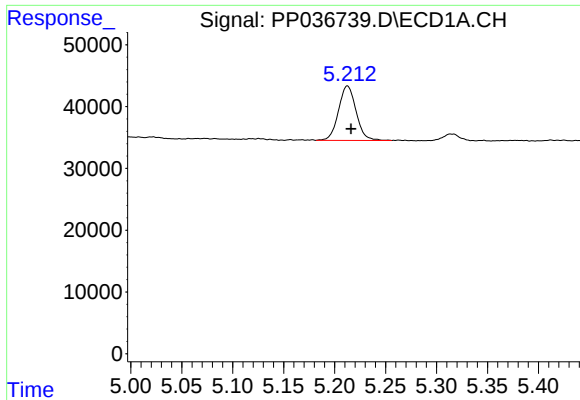

#8 AR-1221-1


R.T.: 5.213 min
Delta R.T.: -0.004 min
Response: 105759
Conc: 188.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
B3-6-8

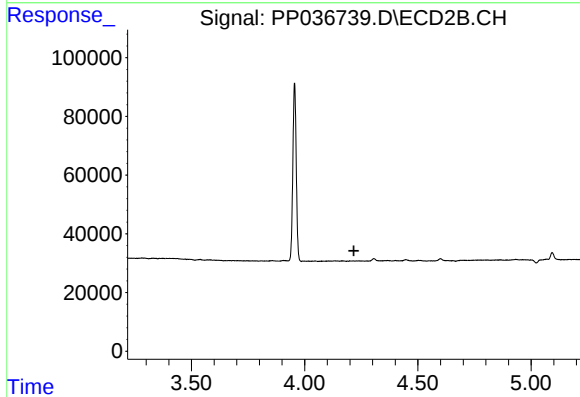


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

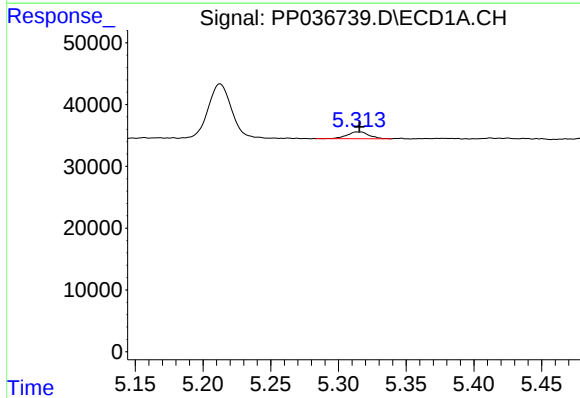


#9 AR-1221-2

R.T.: 5.313 min
Delta R.T.: -0.002 min
Response: 12452
Conc: 28.89 ng/ml

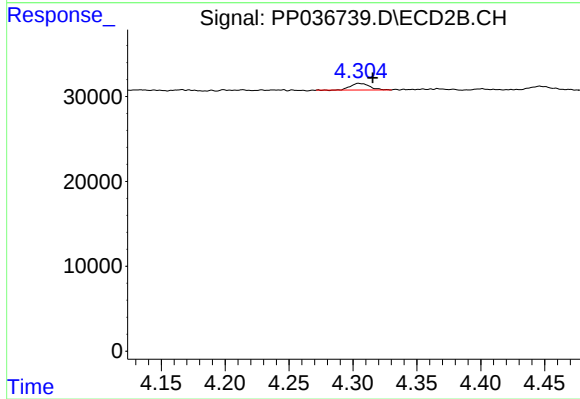

#9 AR-1221-2


R.T.: 4.304 min
Delta R.T.: -0.011 min
Response: 8291
Conc: 27.78 ng/ml

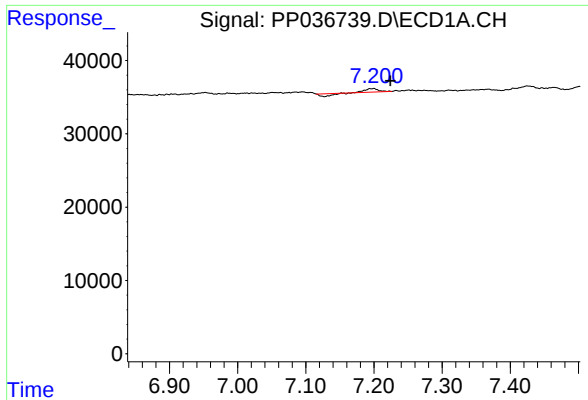

#24 AR-1248-4


R.T.: 7.200 min
Delta R.T.: -0.024 min
Response: 2778
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
B3-6-8

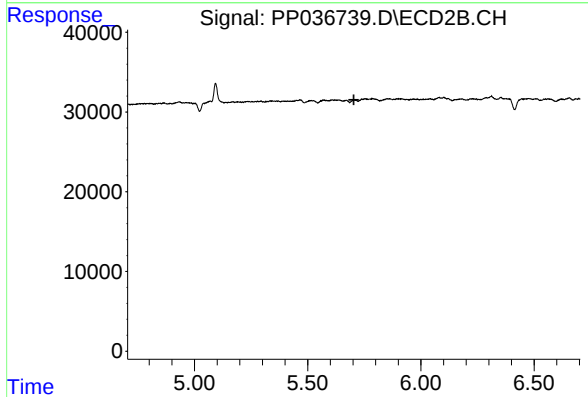


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

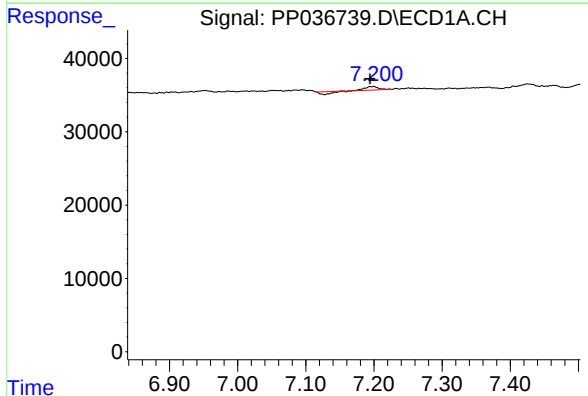


#26 AR-1254-1

R.T.: 7.200 min
Delta R.T.: 0.005 min
Response: 2778
Conc: 1.58 ng/ml

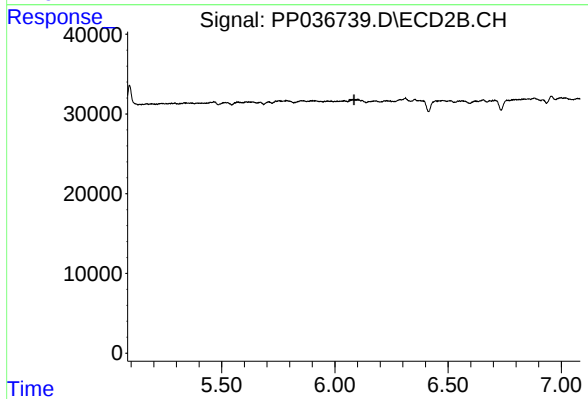

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

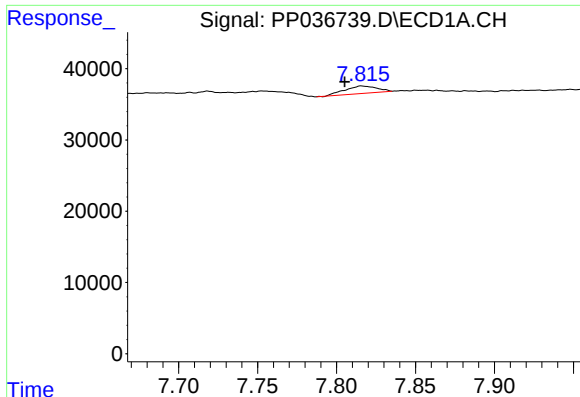

#28 AR-1254-3


R.T.: 7.816 min
Delta R.T.: 0.011 min
Response: 14710
Conc: 4.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
B3-6-8

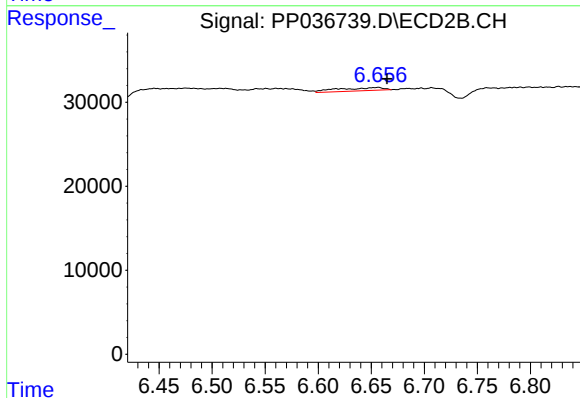


#28 AR-1254-3

R.T.: 6.657 min
Delta R.T.: -0.008 min
Response: 11427
Conc: 4.70 ng/ml

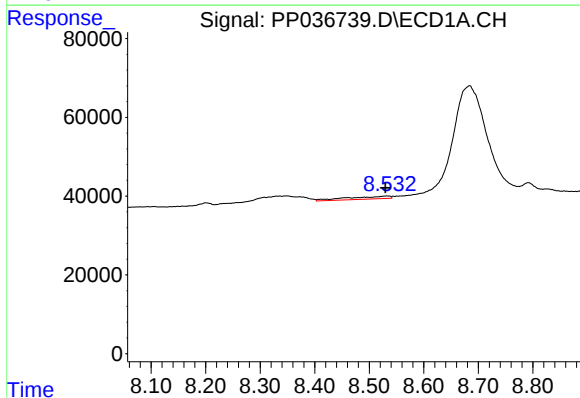


#30 AR-1254-5

R.T.: 8.533 min
Delta R.T.: 0.003 min
Response: 37972
Conc: 15.97 ng/ml

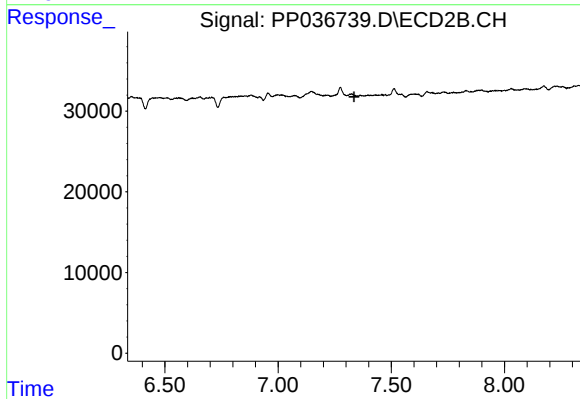

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.335 min
Response: 0
Conc: N.D.

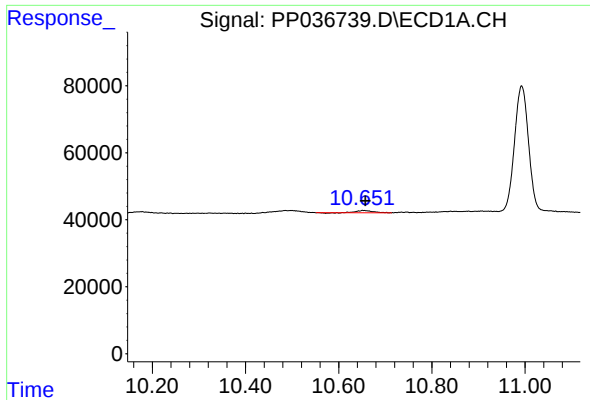

#45 AR-1268-5

R.T.: 10.651 min
Delta R.T.: -0.006 min
Response: 16311
Conc: 1.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
B3-6-8

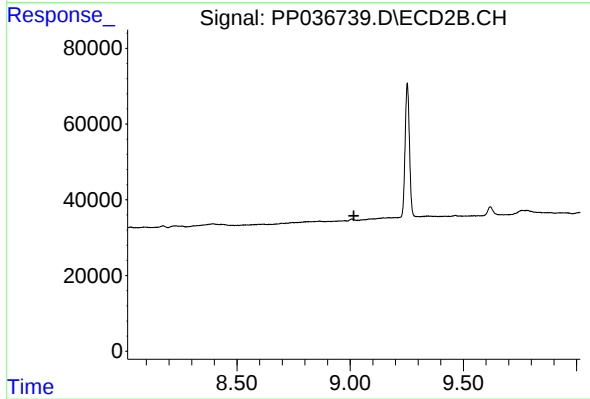

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.017 min
Response: 0
Conc: N.D.