

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036744.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 16:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:24:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.963	3.956	853374	579621	19.308	18.714
2)	SA Decachlor...	10.993	9.253	857800	532494	19.997	16.651
Target Compounds							
9)	L2 AR-1221-2	5.314	0.000	10233	0	23.747	N.D. #
15)	L3 AR-1232-5	6.570	0.000	21366	0	58.297	N.D. #
20)	L4 AR-1242-5	0.000	6.102f	0	19046	N.D.	23.344 #
22)	L5 AR-1248-2	6.570	0.000	21366	0	15.733	N.D. #
24)	L5 AR-1248-4	7.197f	0.000	22827	0	12.503	N.D. #
25)	L5 AR-1248-5	0.000	6.102f	0	19046	N.D.	16.057 #
26)	L6 AR-1254-1	7.197	6.102f	22827	19046	12.980	11.241
28)	L6 AR-1254-3	7.820	0.000	14075	0	4.752	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036744.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 16:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:24:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

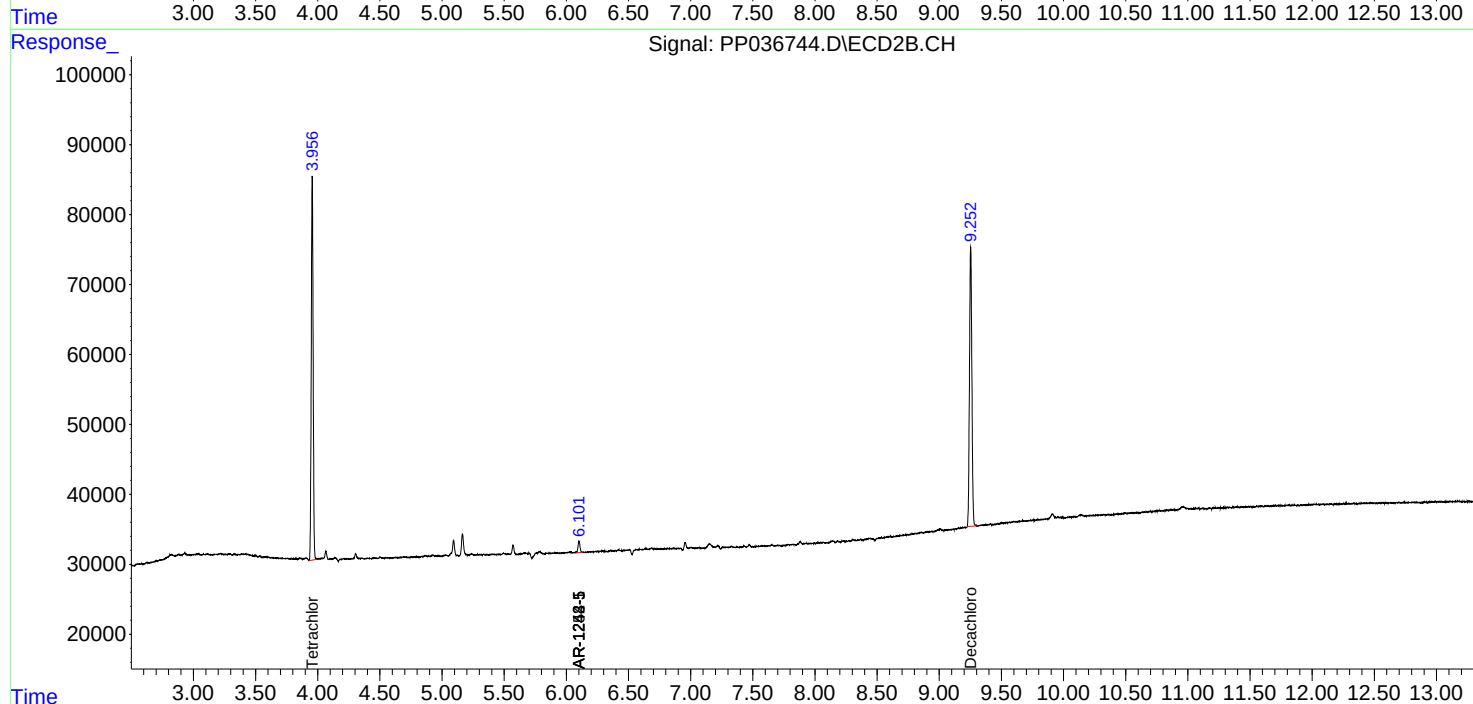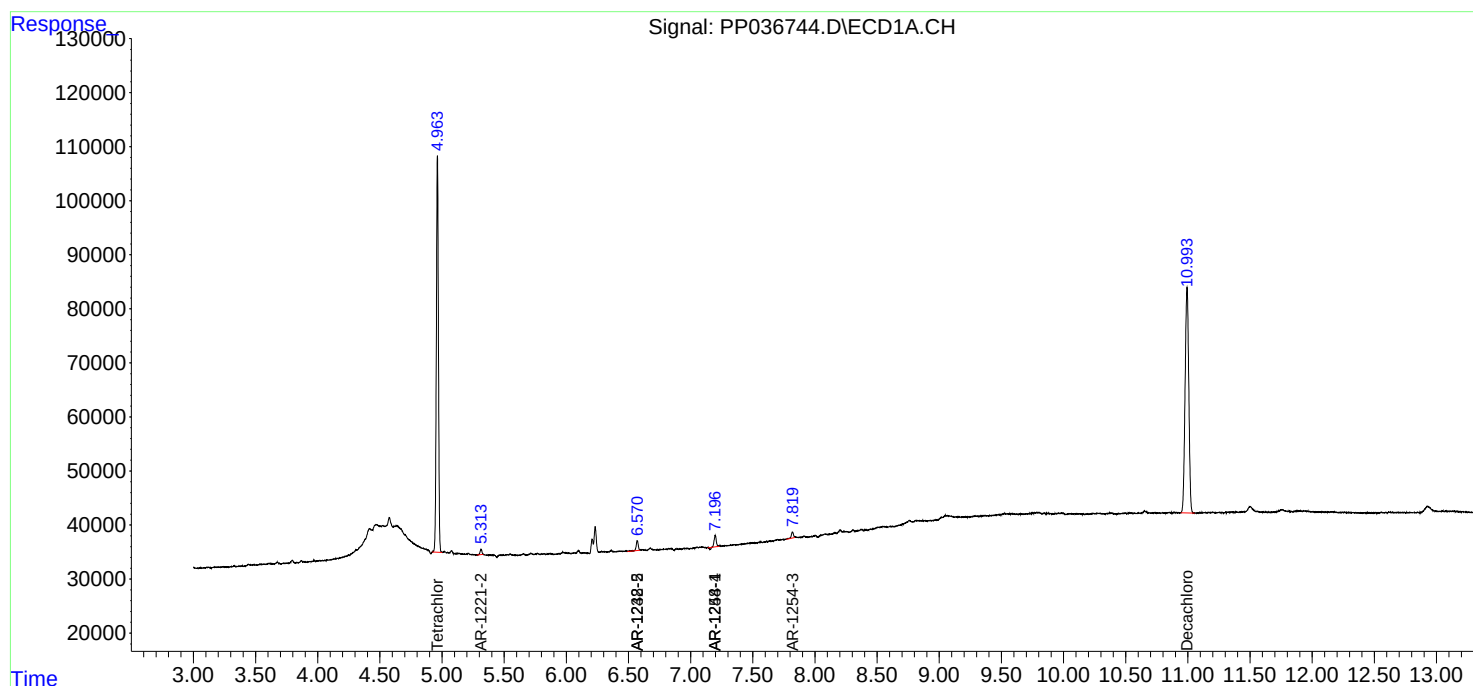


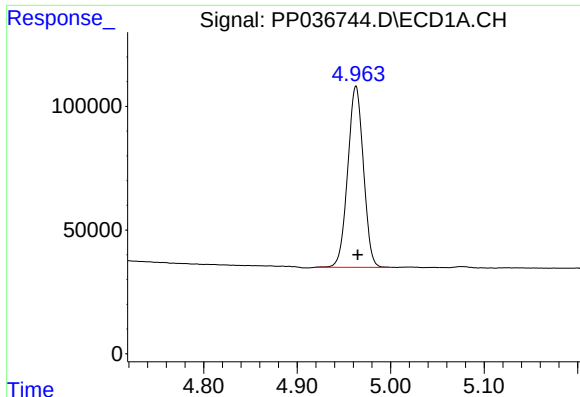

#1 Tetrachloro-m-xylene


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 853374
Conc: 19.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

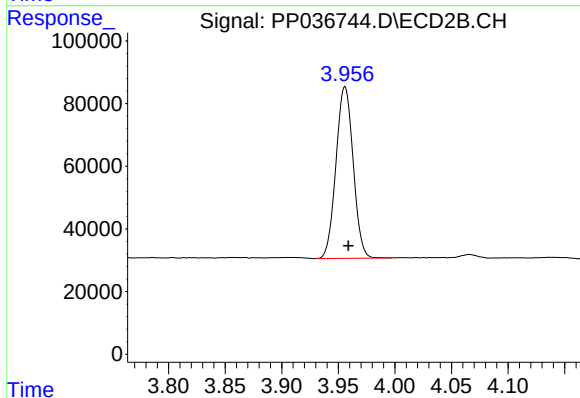


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.003 min
Response: 579621
Conc: 18.71 ng/ml

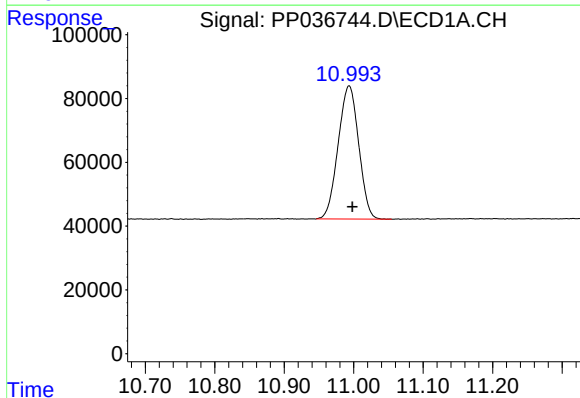


#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 857800
Conc: 20.00 ng/ml

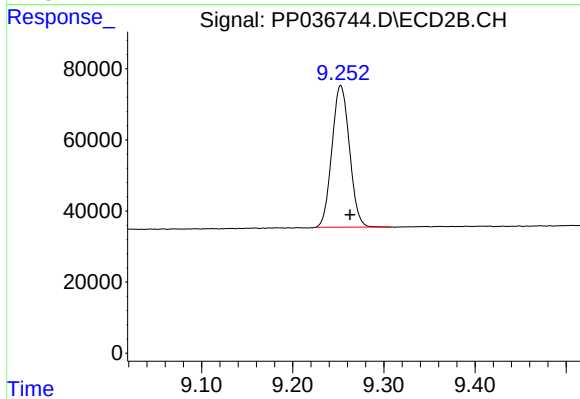

#2 Decachlorobiphenyl


R.T.: 9.253 min
Delta R.T.: -0.010 min
Response: 532494
Conc: 16.65 ng/ml

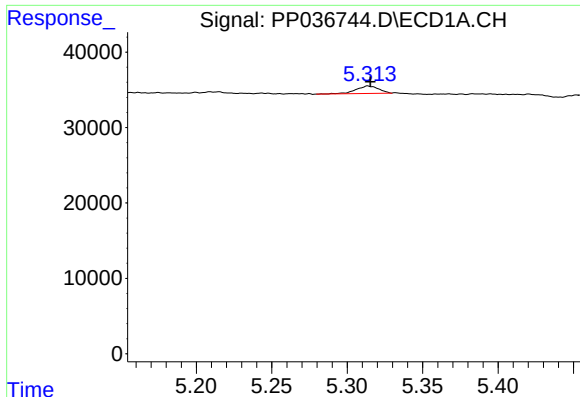

#9 AR-1221-2


R.T.: 5.314 min
Delta R.T.: -0.002 min
Response: 10233
Conc: 23.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

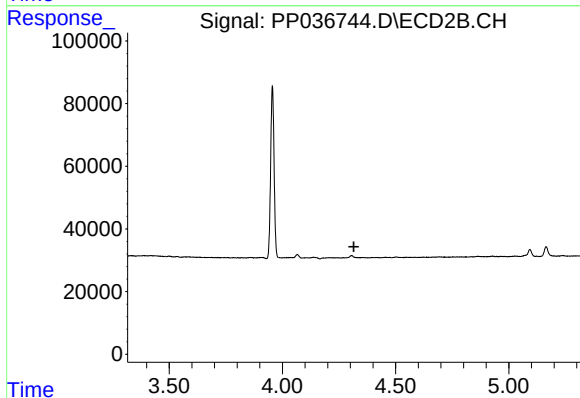


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

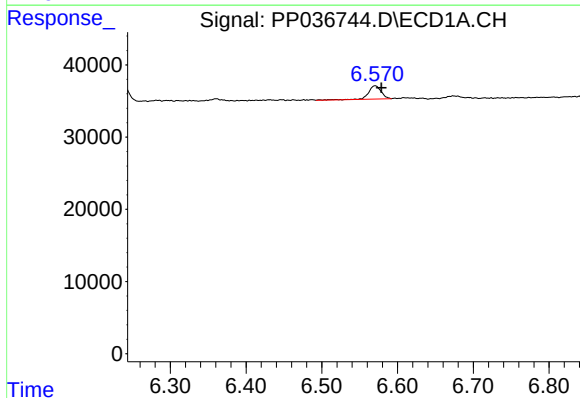


#15 AR-1232-5

R.T.: 6.570 min
Delta R.T.: -0.008 min
Response: 21366
Conc: 58.30 ng/ml

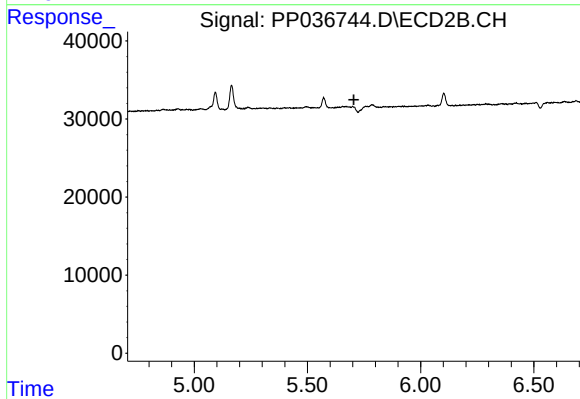

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

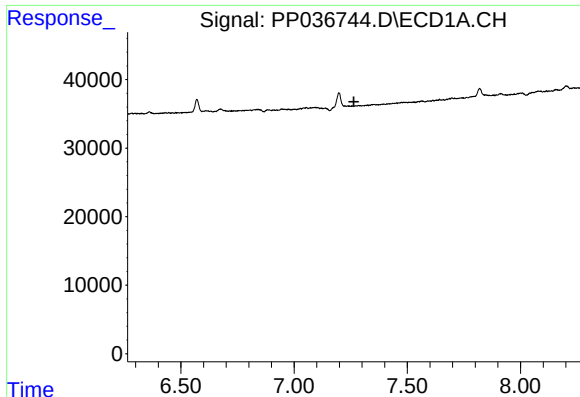

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

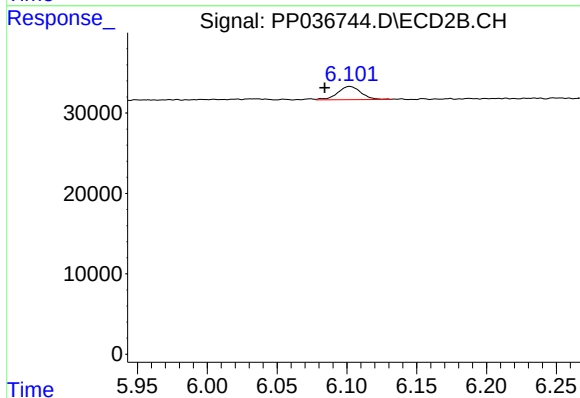


#20 AR-1242-5

R.T.: 6.102 min
Delta R.T.: 0.018 min
Response: 19046
Conc: 23.34 ng/ml

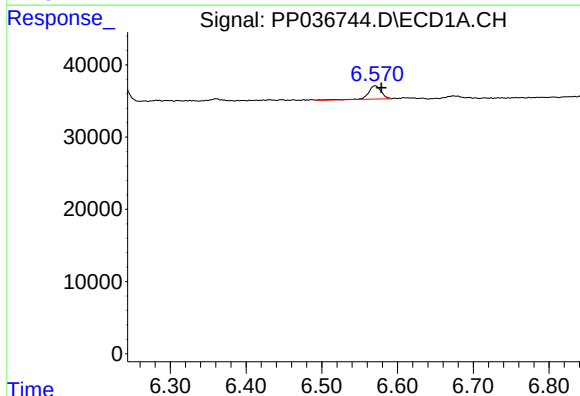


#22 AR-1248-2

R.T.: 6.570 min
Delta R.T.: -0.008 min
Response: 21366
Conc: 15.73 ng/ml

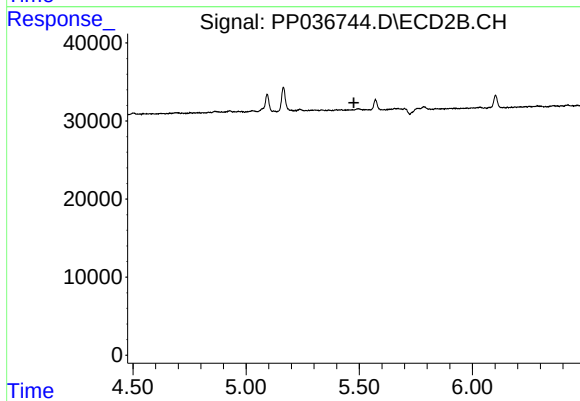

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.476 min
Response: 0
Conc: N.D.

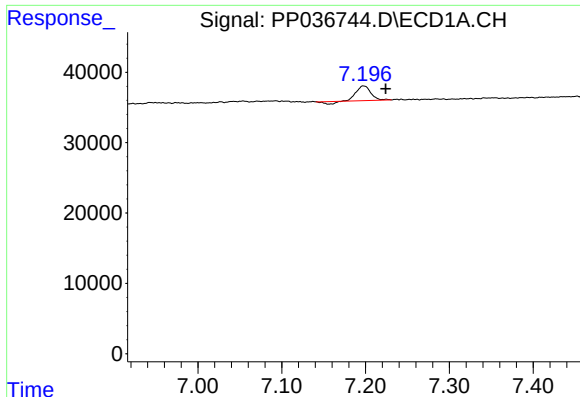

#24 AR-1248-4


R.T.: 7.197 min
Delta R.T.: -0.027 min
Response: 22827
Conc: 12.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

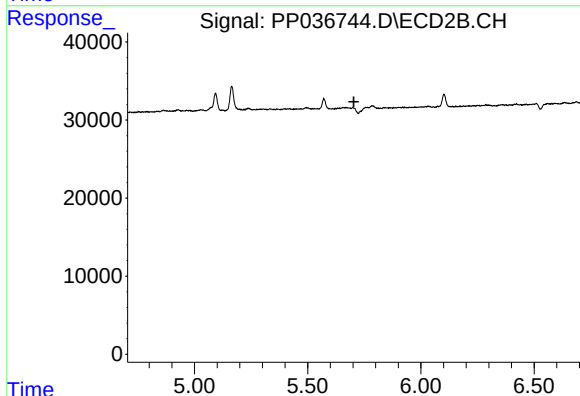


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

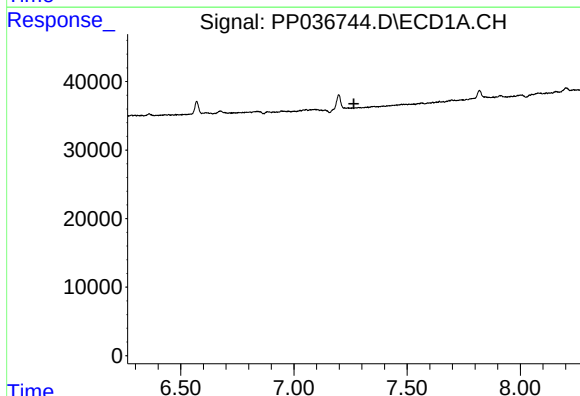


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

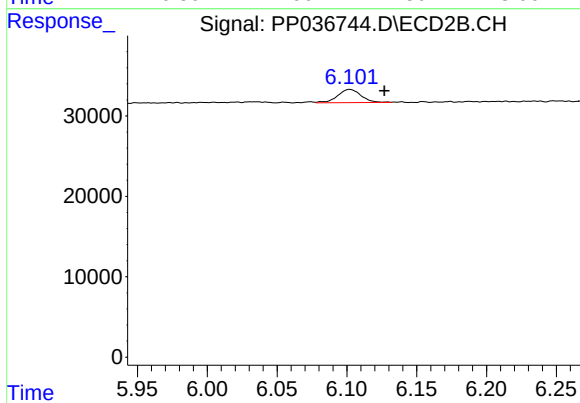

#25 AR-1248-5


R.T.: 6.102 min
Delta R.T.: -0.025 min
Response: 19046
Conc: 16.06 ng/ml

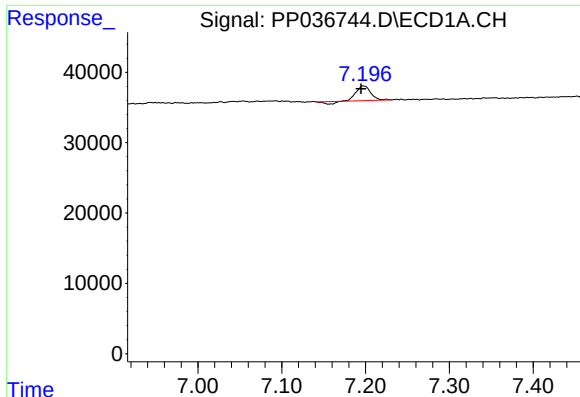

#26 AR-1254-1


R.T.: 7.197 min
Delta R.T.: 0.003 min
Response: 22827
Conc: 12.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

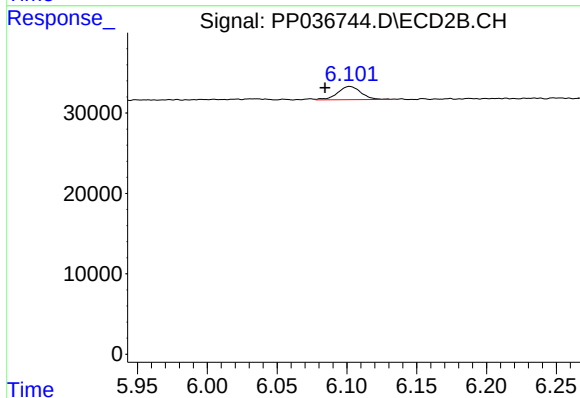


#26 AR-1254-1

R.T.: 6.102 min
Delta R.T.: 0.018 min
Response: 19046
Conc: 11.24 ng/ml

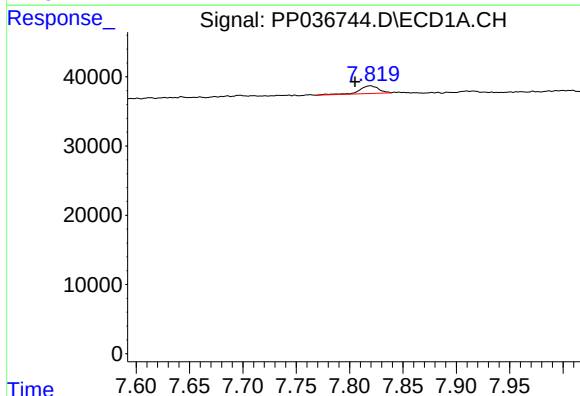

#28 AR-1254-3

R.T.: 7.820 min
Delta R.T.: 0.015 min
Response: 14075
Conc: 4.75 ng/ml

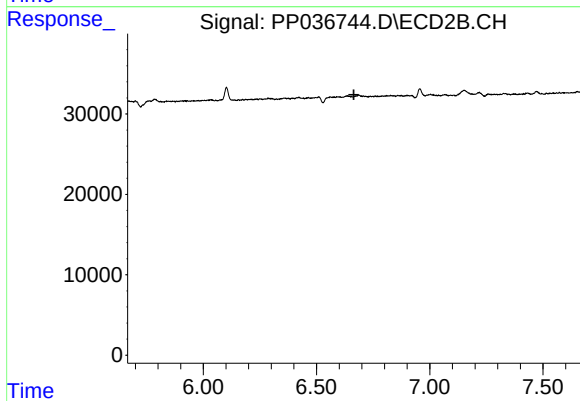

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.665 min
Response: 0
Conc: N.D.