

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036725.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 11:13
 Operator : DD\AJ
 Sample : M2789-23
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1ST-WALLS

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:20:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:18:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.955	790635	556739	17.888	17.975
2) SA Decachlor...	10.993	9.253	845536	536419	19.711	16.773
Target Compounds						
26) L6 AR-1254-1	7.192	6.078	25369	21171	14.425m	12.495
27) L6 AR-1254-2	7.422	6.238	42520	17488	15.715	11.758 #
28) L6 AR-1254-3	7.804	6.657	69306	31720	23.398	13.047m#
29) L6 AR-1254-4	8.099	6.898	57179	28965	26.010	18.718m#
30) L6 AR-1254-5	8.527	7.328	71014	100324	29.861m	46.656 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036725.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 11:13
Operator : DD\AJ
Sample : M2789-23
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
1ST-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:20:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:18:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

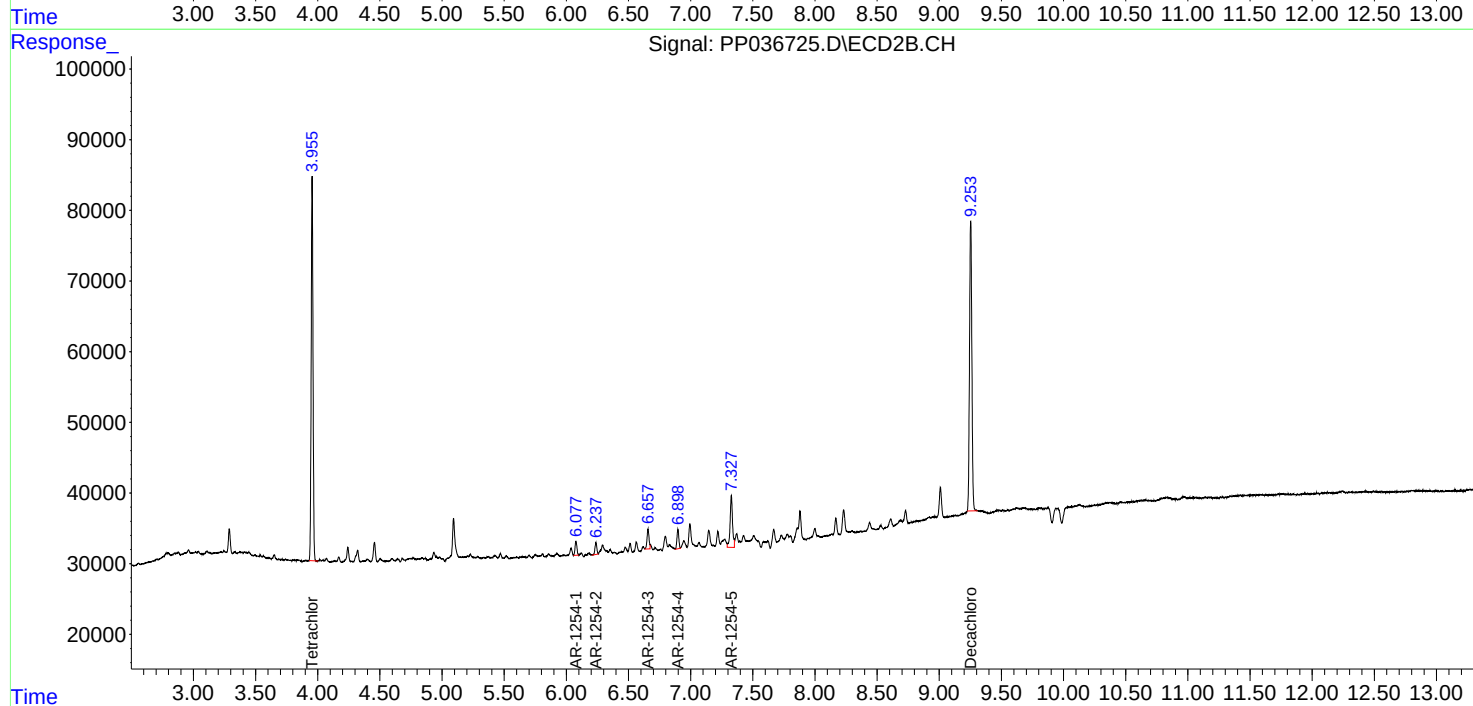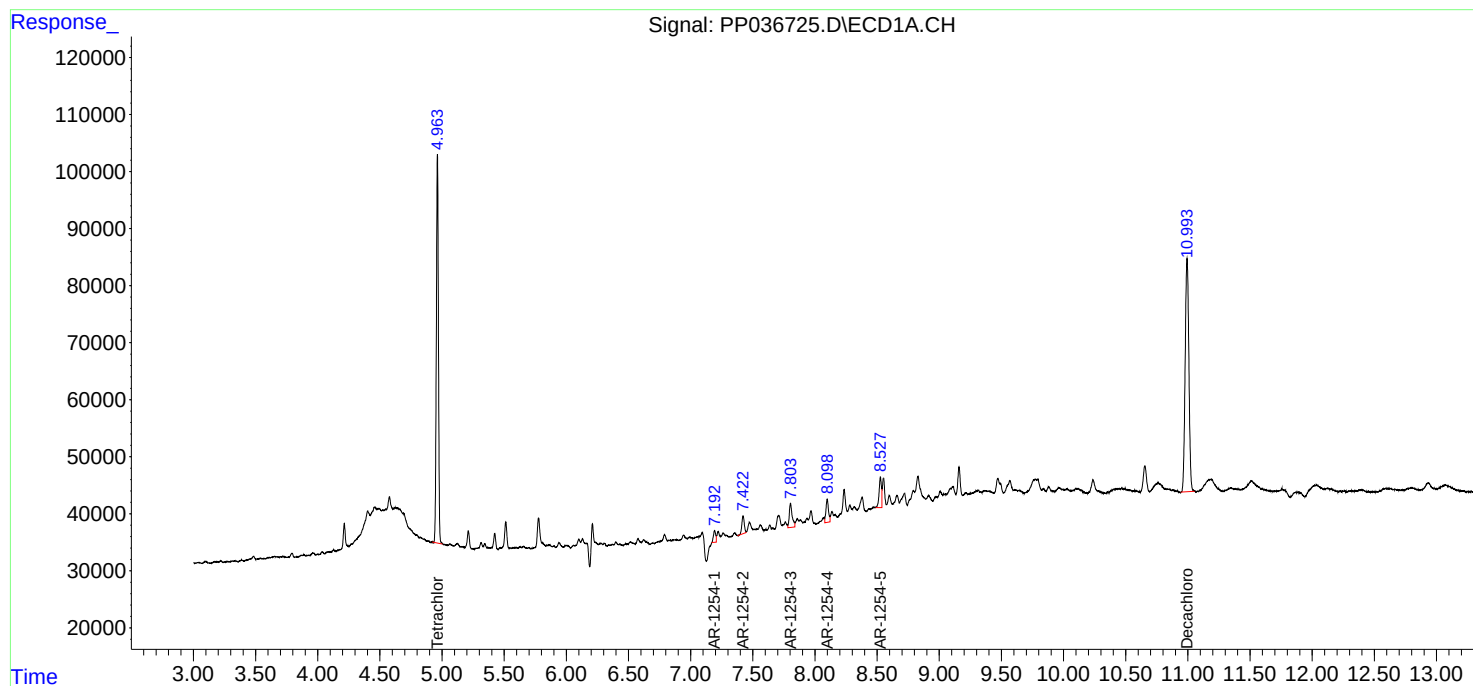

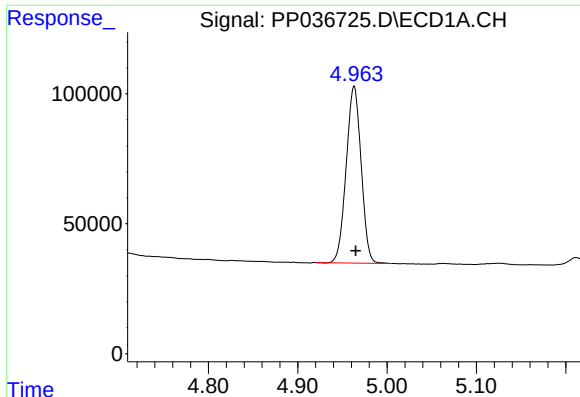


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 790635
Conc: 17.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:20:54 PM

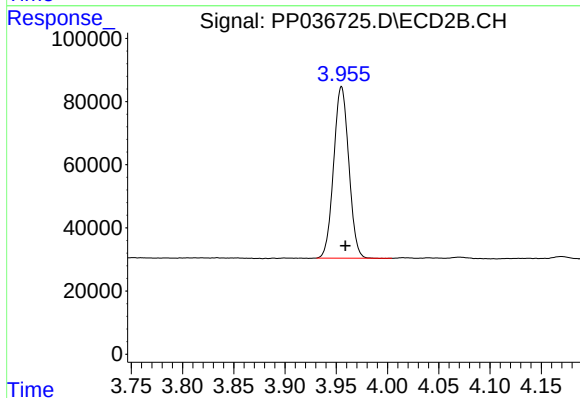


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 556739
Conc: 17.97 ng/ml

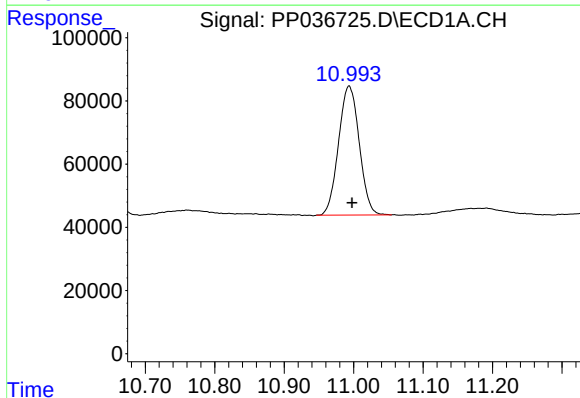


#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 845536
Conc: 19.71 ng/ml

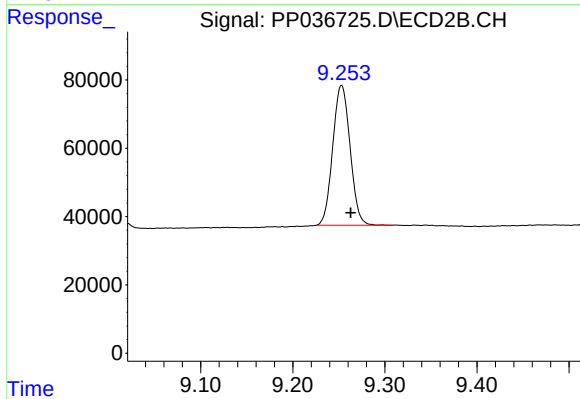

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.010 min
Response: 536419
Conc: 16.77 ng/ml

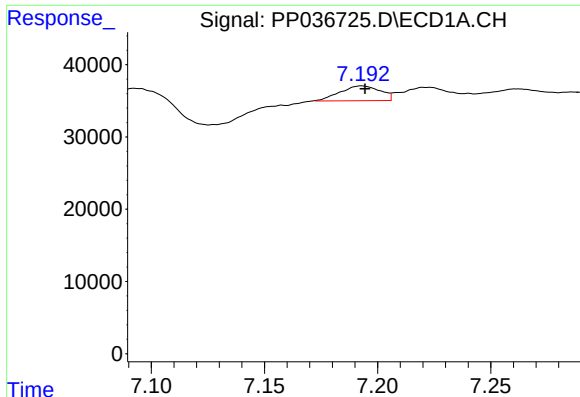


#26 AR-1254-1

R.T.: 7.192 min
Delta R.T.: -0.002 min
Response: 25369
Conc: 14.43 ng/ml m

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:20:54 PM

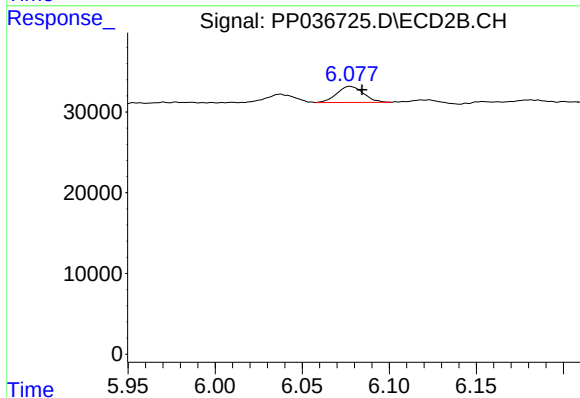


#26 AR-1254-1

R.T.: 6.078 min
Delta R.T.: -0.007 min
Response: 21171
Conc: 12.50 ng/ml

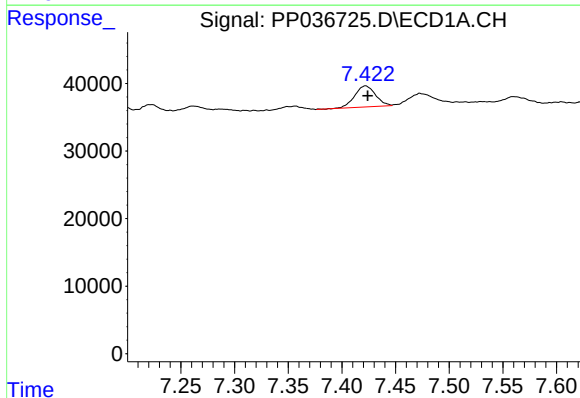


#27 AR-1254-2

R.T.: 7.422 min
Delta R.T.: -0.002 min
Response: 42520
Conc: 15.71 ng/ml

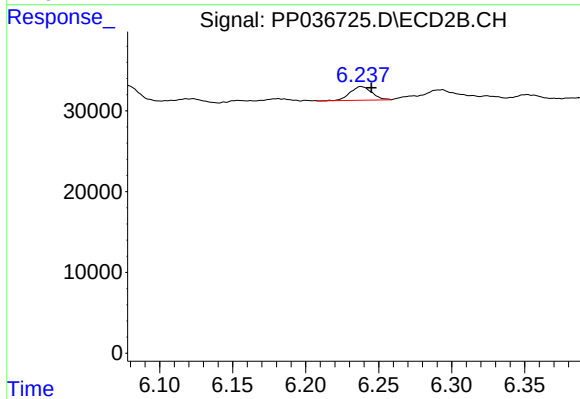

#27 AR-1254-2

R.T.: 6.238 min
Delta R.T.: -0.007 min
Response: 17488
Conc: 11.76 ng/ml

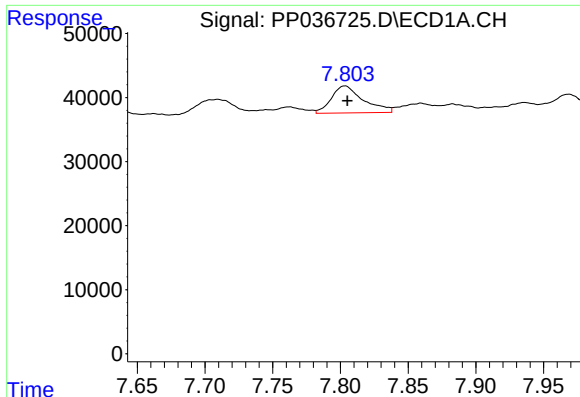


#28 AR-1254-3

R.T.: 7.804 min
Delta R.T.: -0.002 min
Response: 69306
Conc: 23.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:20:54 PM

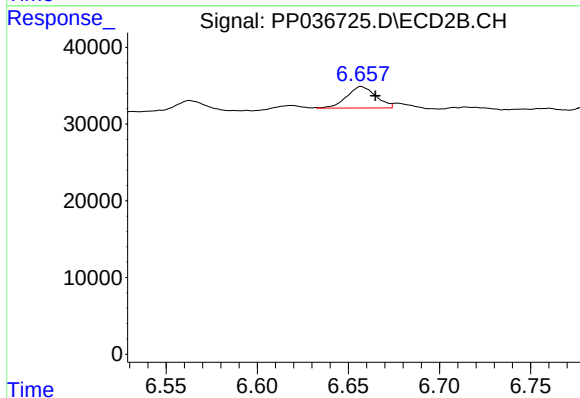


#28 AR-1254-3

R.T.: 6.657 min
Delta R.T.: -0.008 min
Response: 31720
Conc: 13.05 ng/ml m

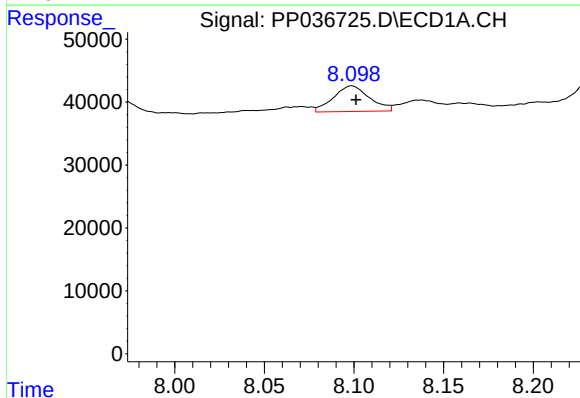


#29 AR-1254-4

R.T.: 8.099 min
Delta R.T.: -0.002 min
Response: 57179
Conc: 26.01 ng/ml

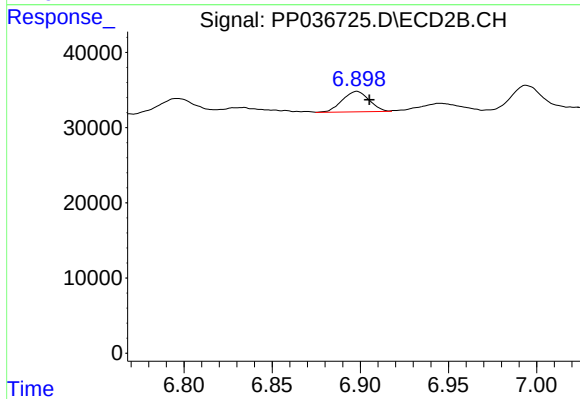

#29 AR-1254-4

R.T.: 6.898 min
Delta R.T.: -0.007 min
Response: 28965
Conc: 18.72 ng/ml m

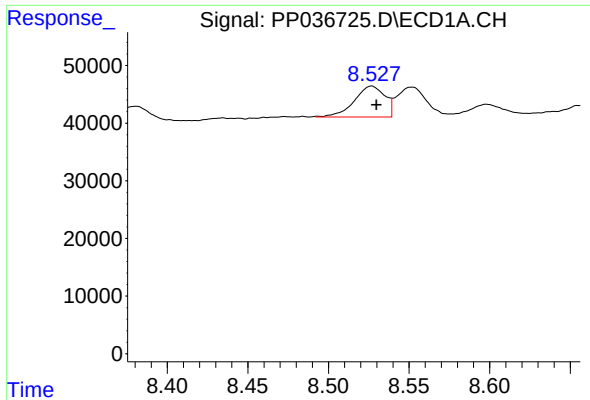


#30 AR-1254-5

R.T.: 8.527 min
Delta R.T.: -0.003 min
Response: 71014
Conc: 29.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
1ST-WALLS

Manual Integrations
APPROVED

Ankita
6/24/2021 1:20:54 PM

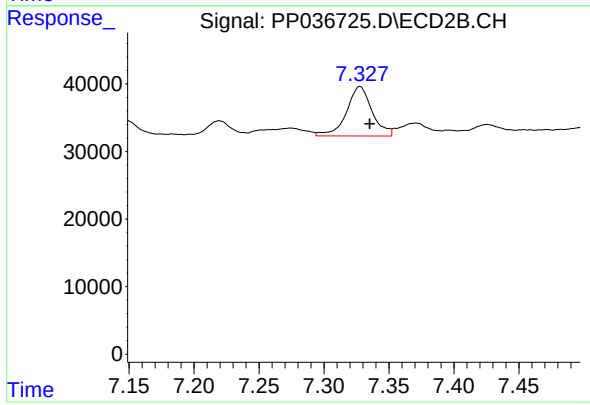

#30 AR-1254-5

R.T.: 7.328 min
Delta R.T.: -0.008 min
Response: 100324
Conc: 46.66 ng/ml