

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036736.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 14:22
 Operator : DD\AJ
 Sample : M2795-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B2-0-2

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:21:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:21:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.955	813724	584621	18.411	18.875
2) SA Decachlor...	10.992	9.252	886100	512414	20.656	16.023
Target Compounds						
26) L6 AR-1254-1	7.191	6.078	74493	70445	42.358	41.576
27) L6 AR-1254-2	7.421	6.239	131023	81096	48.424m	54.522
28) L6 AR-1254-3	7.804	6.656	139623	98133	47.137	40.365m
29) L6 AR-1254-4	8.098	6.897	73267	26718	33.328m	17.265 #
30) L6 AR-1254-5	8.526	7.327	141497	103127	59.499	47.960m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036736.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 14:22
Operator : DD\AJ
Sample : M2795-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
B2-0-2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:21:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

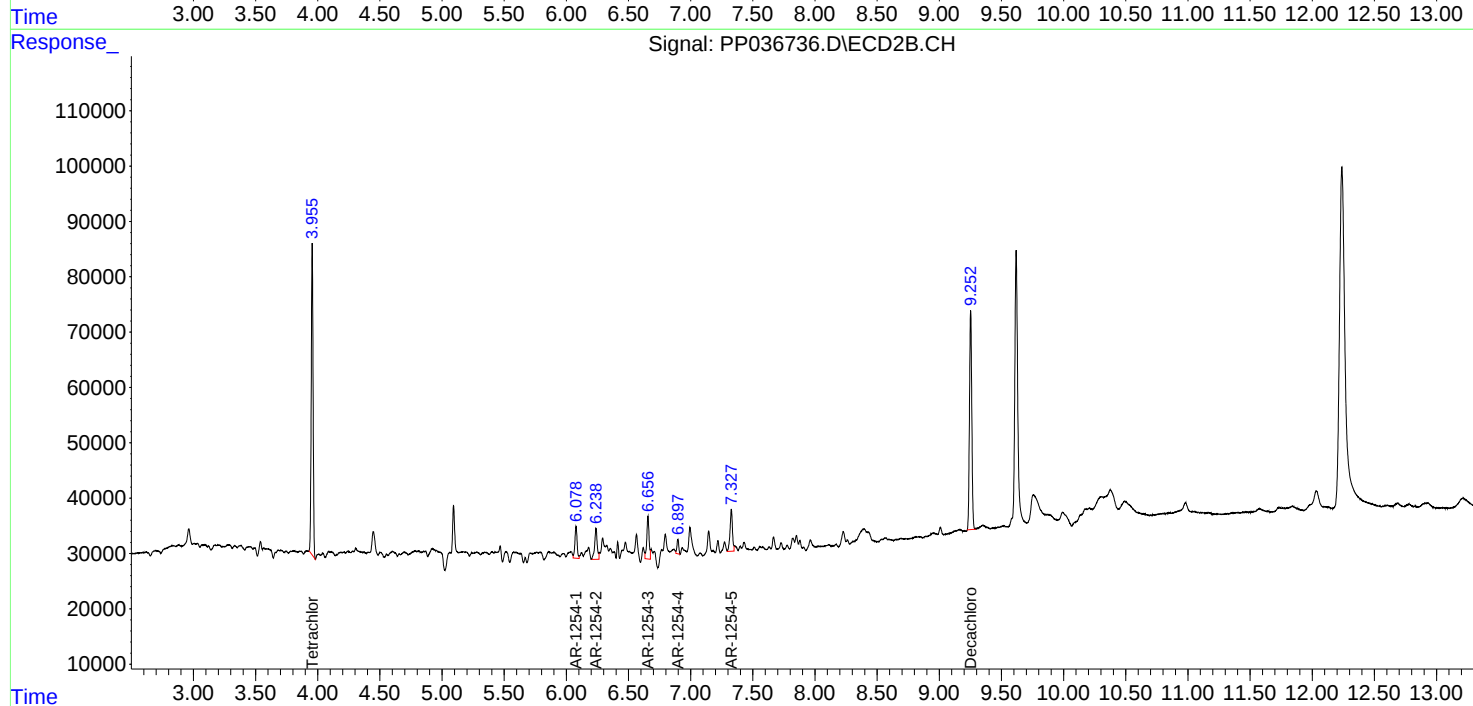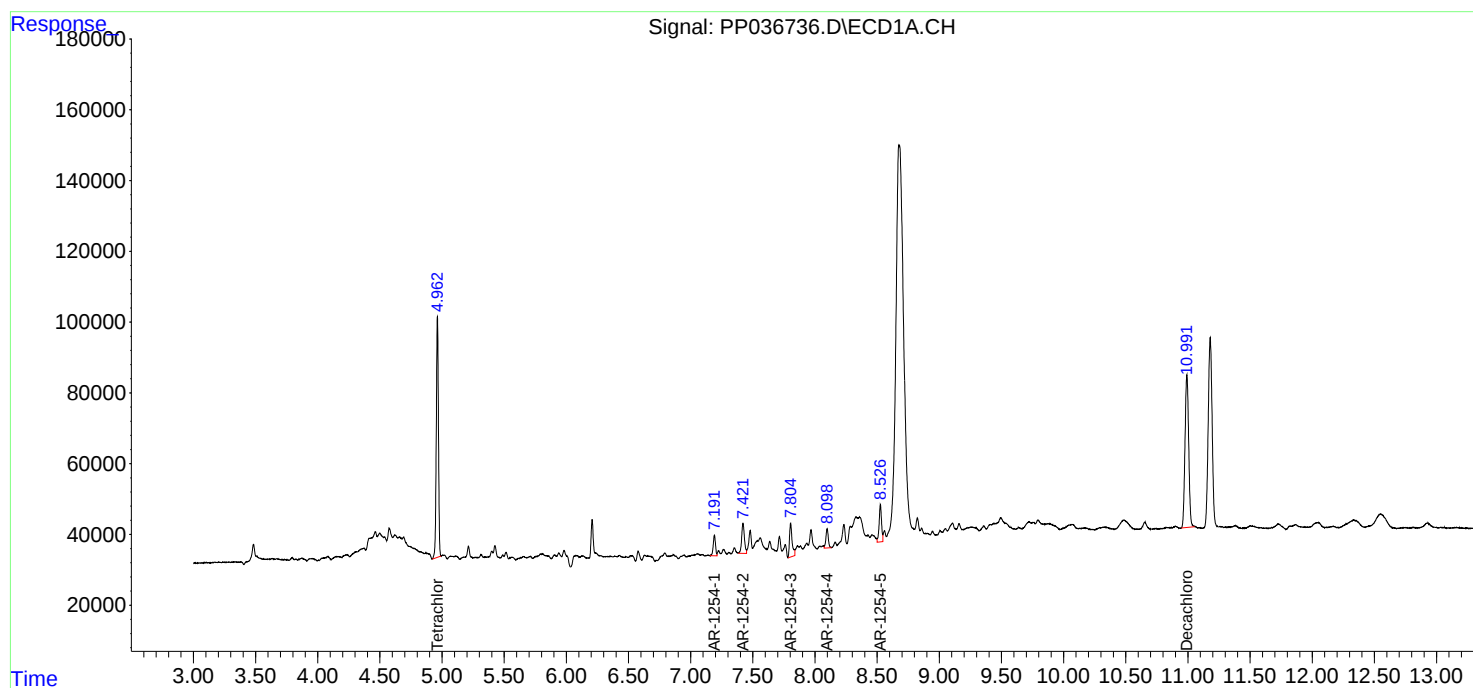

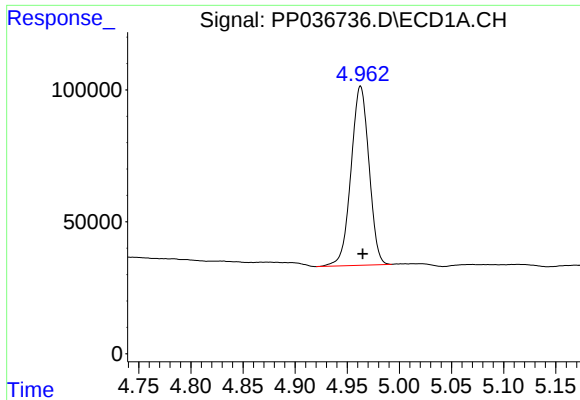


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 813724
Conc: 18.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
B2-0-2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:00 PM

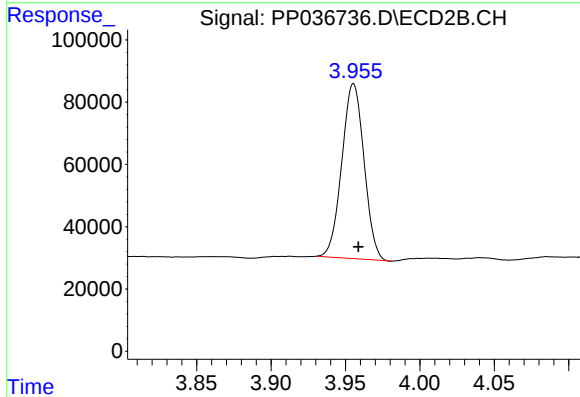


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.003 min
Response: 584621
Conc: 18.88 ng/ml

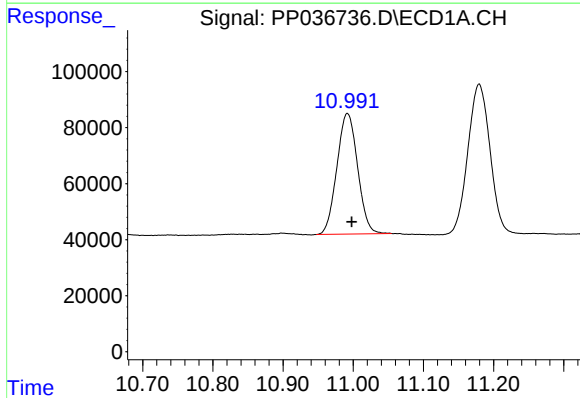


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.006 min
Response: 886100
Conc: 20.66 ng/ml

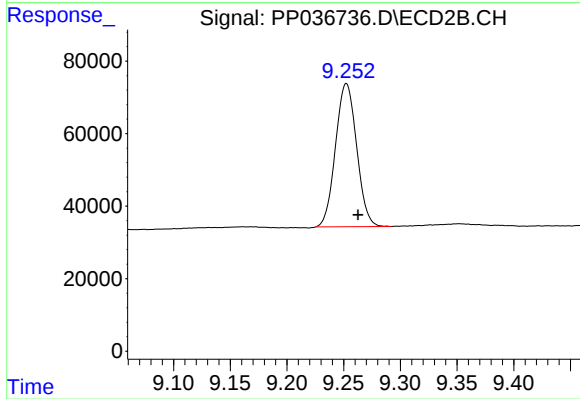

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.011 min
Response: 512414
Conc: 16.02 ng/ml

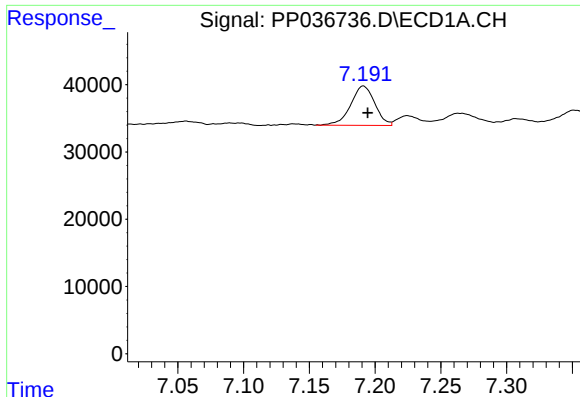


#26 AR-1254-1

R.T.: 7.191 min
Delta R.T.: -0.003 min
Response: 74493
Conc: 42.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
B2-0-2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:00 PM

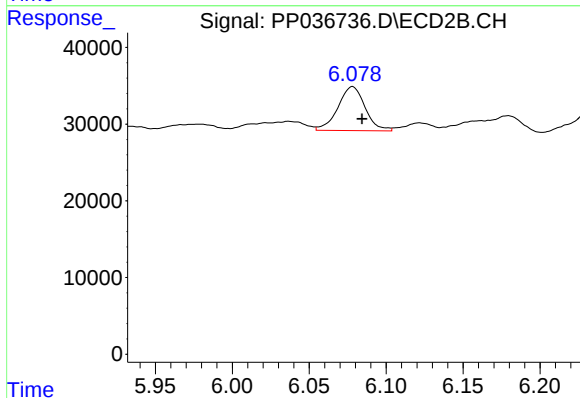


#26 AR-1254-1

R.T.: 6.078 min
Delta R.T.: -0.006 min
Response: 70445
Conc: 41.58 ng/ml

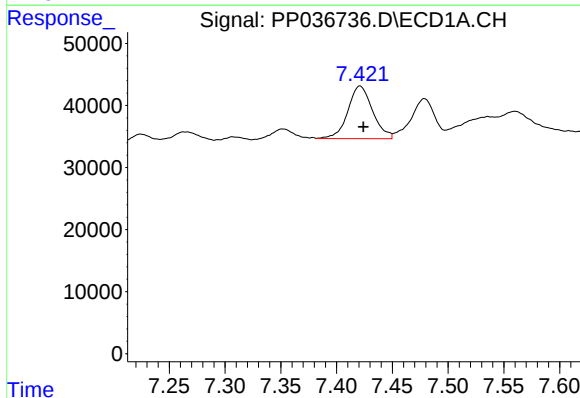


#27 AR-1254-2

R.T.: 7.421 min
Delta R.T.: -0.003 min
Response: 131023
Conc: 48.42 ng/ml m

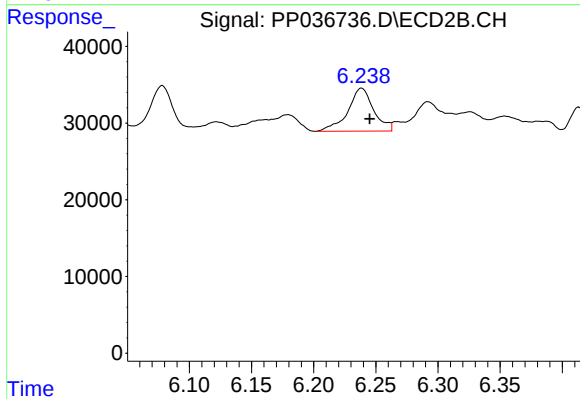

#27 AR-1254-2

R.T.: 6.239 min
Delta R.T.: -0.007 min
Response: 81096
Conc: 54.52 ng/ml

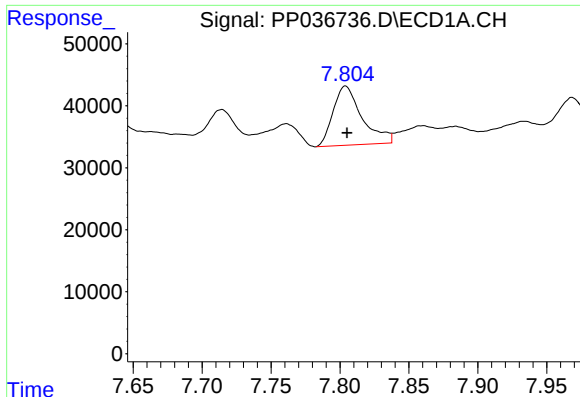


#28 AR-1254-3

R.T.: 7.804 min
Delta R.T.: -0.001 min
Response: 139623
Conc: 47.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
B2-0-2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:00 PM

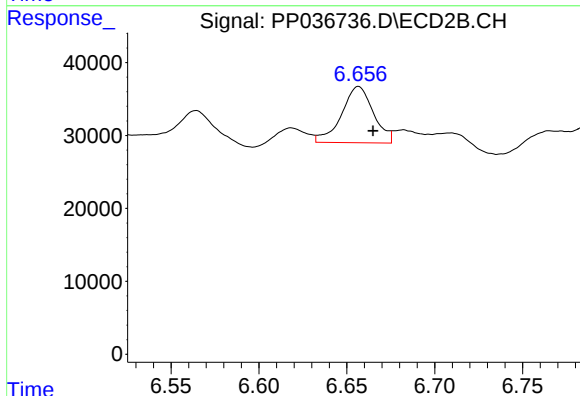


#28 AR-1254-3

R.T.: 6.656 min
Delta R.T.: -0.009 min
Response: 98133
Conc: 40.36 ng/ml m

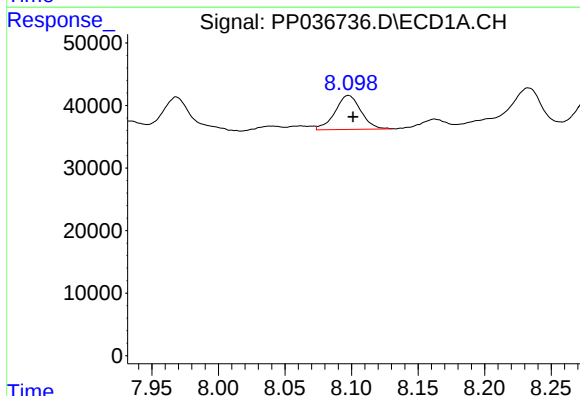


#29 AR-1254-4

R.T.: 8.098 min
Delta R.T.: -0.004 min
Response: 73267
Conc: 33.33 ng/ml m

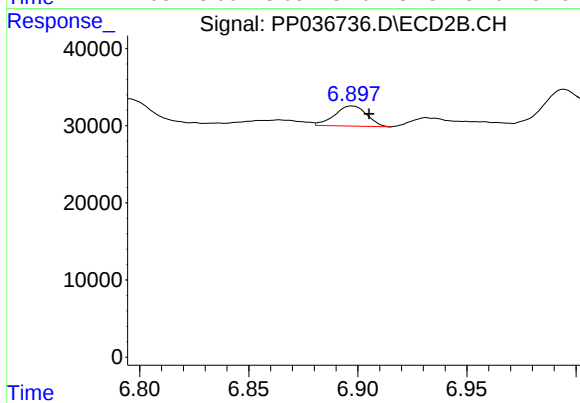

#29 AR-1254-4

R.T.: 6.897 min
Delta R.T.: -0.008 min
Response: 26718
Conc: 17.27 ng/ml

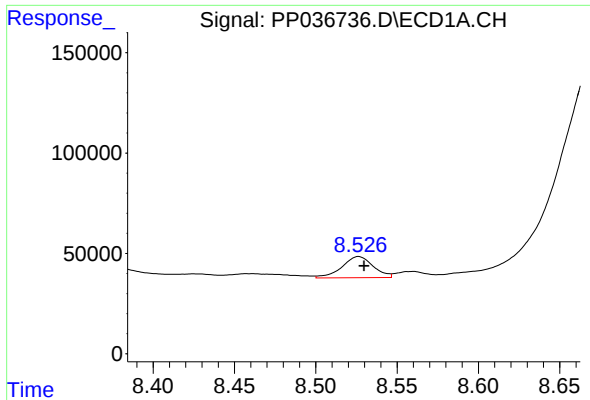


#30 AR-1254-5

R.T.: 8.526 min
Delta R.T.: -0.003 min
Response: 141497
Conc: 59.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
B2-0-2

Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:00 PM

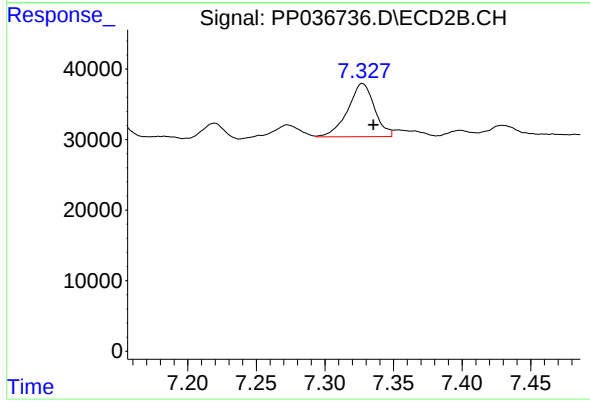

#30 AR-1254-5

R.T.: 7.327 min
Delta R.T.: -0.009 min
Response: 103127
Conc: 47.96 ng/ml m