

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036743.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 16:20
 Operator : DD\AJ
 Sample : AR1268CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268CCC500

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:21:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:24:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.955	2365188	1658571	53.513	53.548
2) SA Decachlor...	10.992	9.253	3644334	2387995	84.955	74.670
Target Compounds						
41) L9 AR-1268-1	9.470	8.168	2797236	2047768	466.244	439.757
42) L9 AR-1268-2	9.568	8.233	2678427	1914362	469.870	443.799
43) L9 AR-1268-3	9.795	8.442	2308064	1615716	480.077m	442.527
44) L9 AR-1268-4	10.236	8.729	1063287	692270	451.407m	435.192
45) L9 AR-1268-5	10.654	9.009	7458192	5186620	484.981	438.702m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 16:20
Operator : DD\AJ
Sample : AR1268CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:24:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

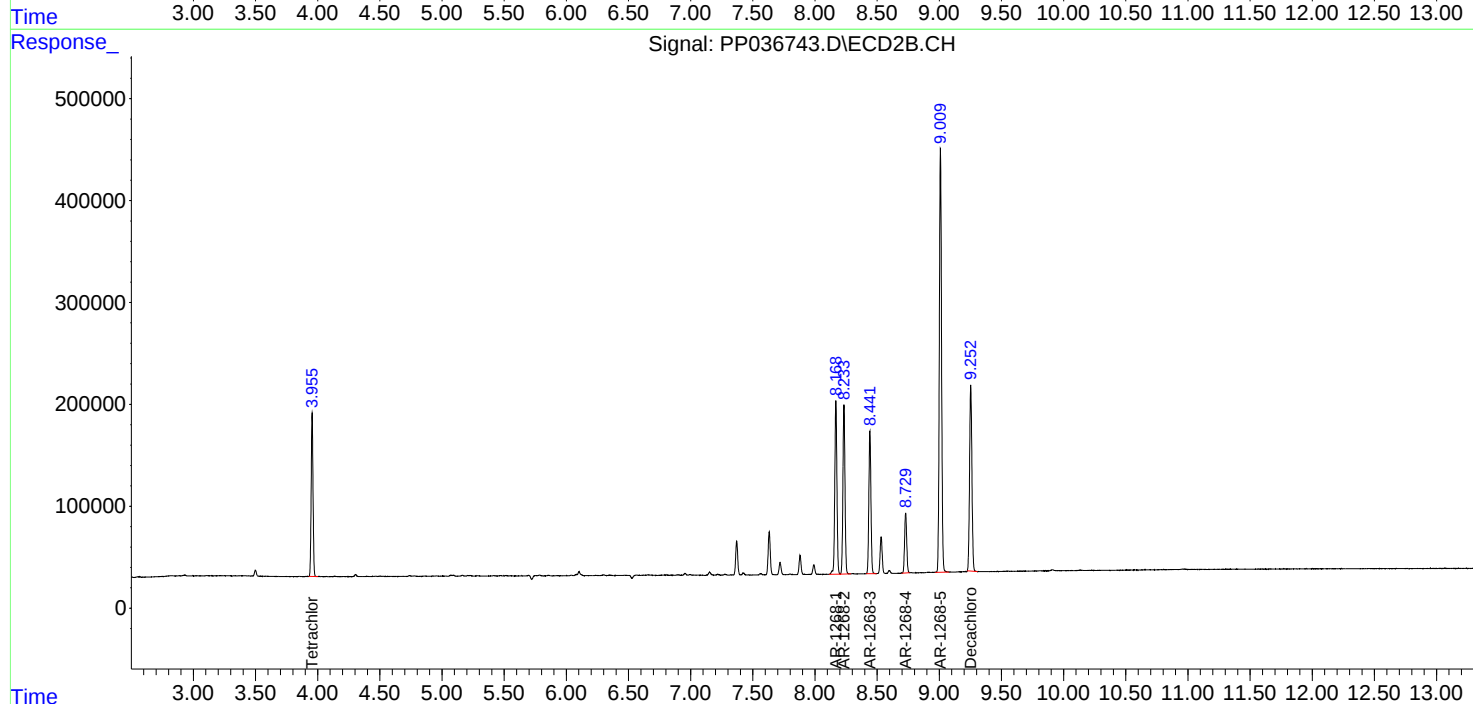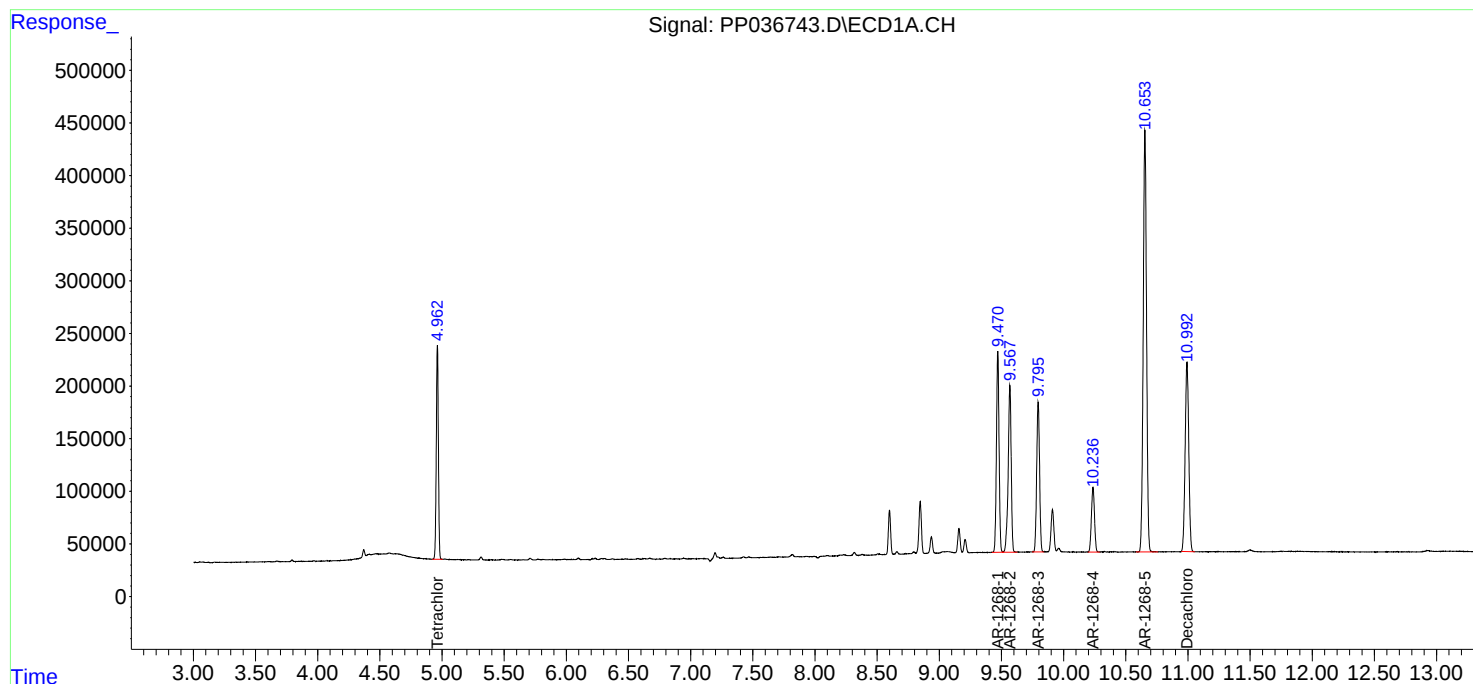

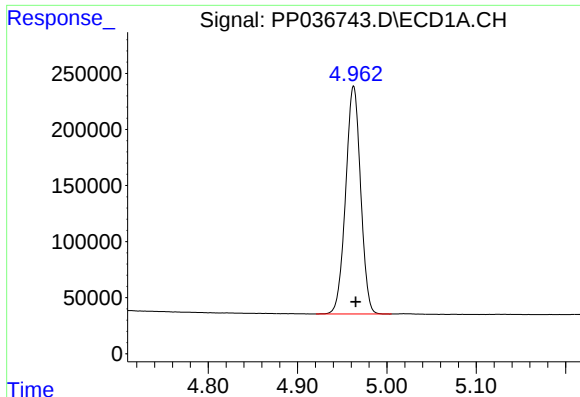


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 2365188
Conc: 53.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:02 PM

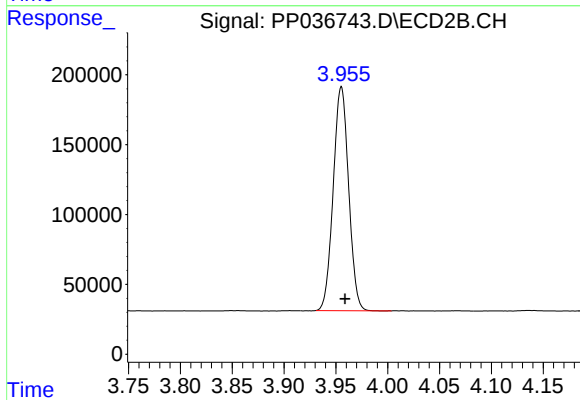


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 1658571
Conc: 53.55 ng/ml

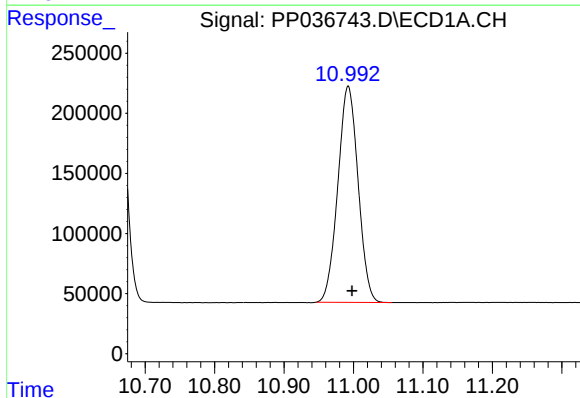


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.006 min
Response: 3644334
Conc: 84.95 ng/ml

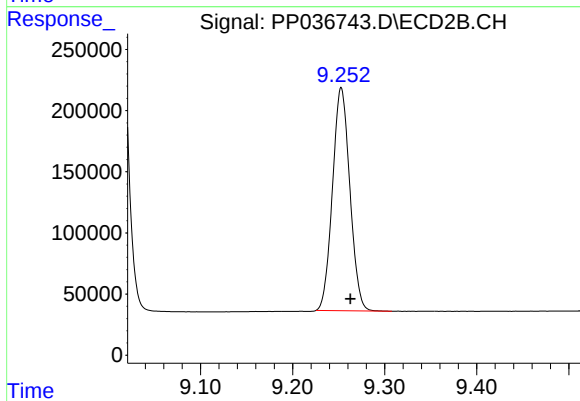

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.010 min
Response: 2387995
Conc: 74.67 ng/ml

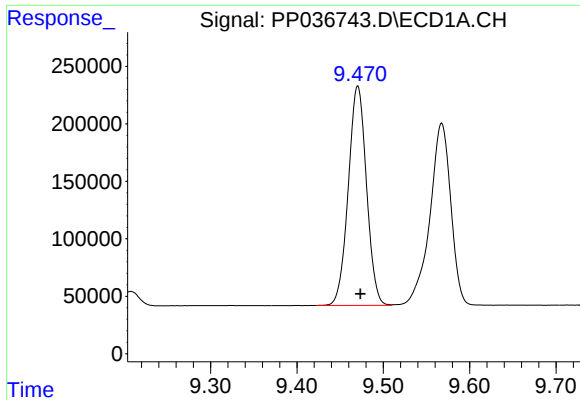


#41 AR-1268-1

R.T.: 9.470 min
Delta R.T.: -0.003 min
Response: 2797236
Conc: 466.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:02 PM

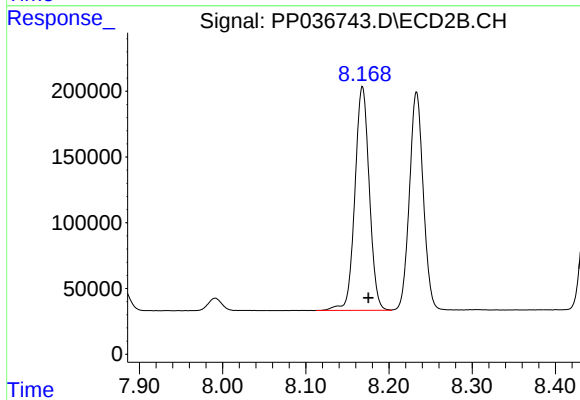


#41 AR-1268-1

R.T.: 8.168 min
Delta R.T.: -0.007 min
Response: 2047768
Conc: 439.76 ng/ml

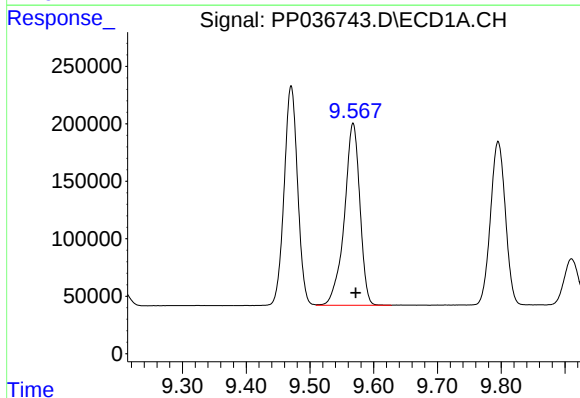


#42 AR-1268-2

R.T.: 9.568 min
Delta R.T.: -0.004 min
Response: 2678427
Conc: 469.87 ng/ml

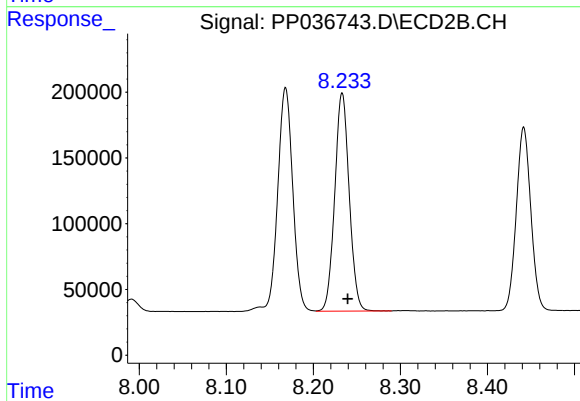

#42 AR-1268-2

R.T.: 8.233 min
Delta R.T.: -0.006 min
Response: 1914362
Conc: 443.80 ng/ml

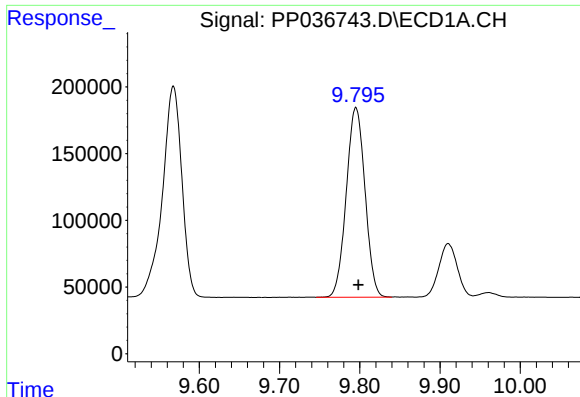


#43 AR-1268-3

R.T.: 9.795 min
Delta R.T.: -0.004 min
Response: 2308064
Conc: 480.08 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:02 PM

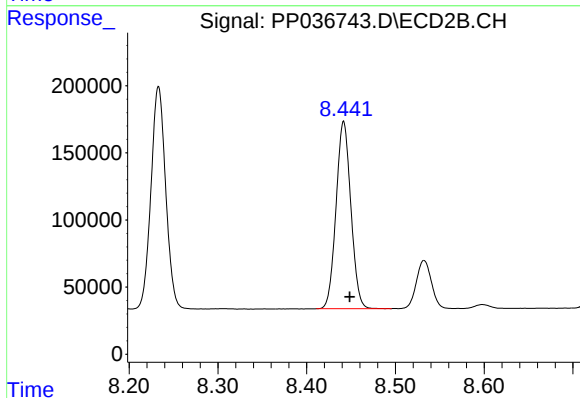


#43 AR-1268-3

R.T.: 8.442 min
Delta R.T.: -0.007 min
Response: 1615716
Conc: 442.53 ng/ml

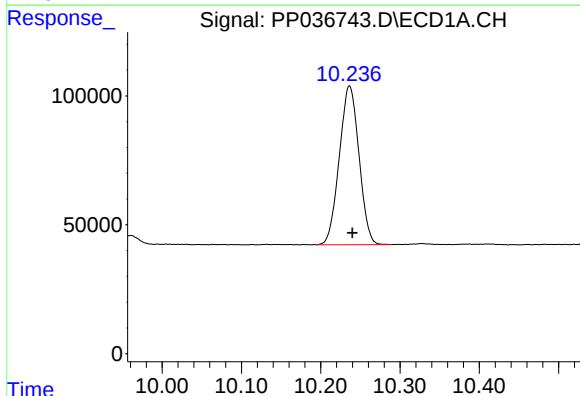


#44 AR-1268-4

R.T.: 10.236 min
Delta R.T.: -0.004 min
Response: 1063287
Conc: 451.41 ng/ml m

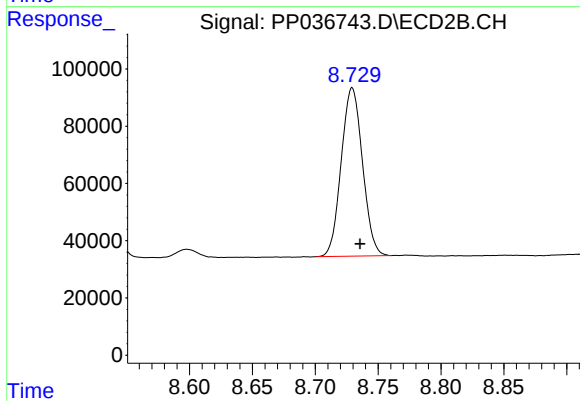

#44 AR-1268-4

R.T.: 8.729 min
Delta R.T.: -0.006 min
Response: 692270
Conc: 435.19 ng/ml

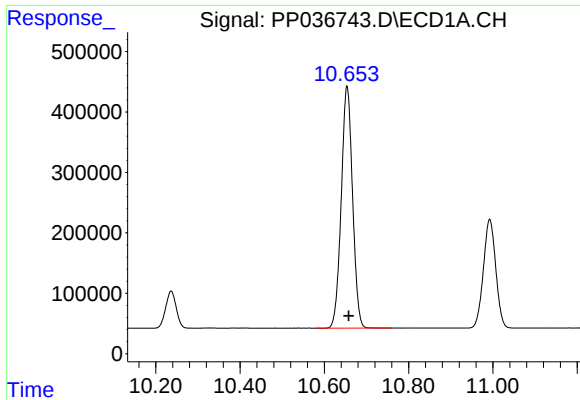


#45 AR-1268-5

R.T.: 10.654 min
Delta R.T.: -0.004 min
Response: 7458192
Conc: 484.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268CCC500

Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:02 PM

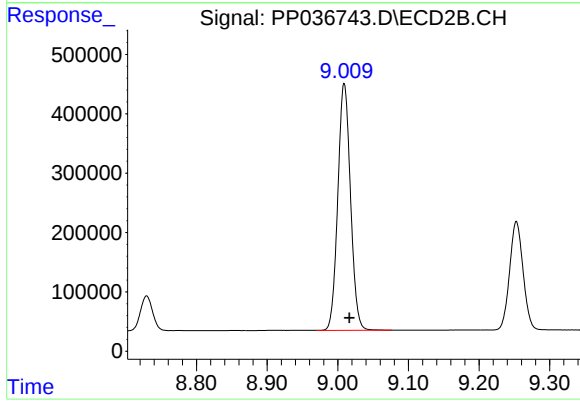

#45 AR-1268-5

R.T.: 9.009 min
Delta R.T.: -0.008 min
Response: 5186620
Conc: 438.70 ng/ml m