

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036750.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 18:18
 Operator : DD\AJ
 Sample : M2809-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JD310E-R2

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:21:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:25:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.956	364890	240299	8.256	7.758
2) SA Decachlor...	10.992	9.252	408285	239204	9.518	7.480
Target Compounds						
31) L7 AR-1260-1	7.969	6.796	18196	15509	8.384	9.633
32) L7 AR-1260-2	8.235	6.996	35693	35863	13.927	18.493 #
33) L7 AR-1260-3	8.599	7.148	23694	30253	11.820	16.635 #
34) L7 AR-1260-4	8.831	7.631	34354	20063	14.500	12.938m
35) L7 AR-1260-5	9.159	7.880	83018	65876	18.606	17.927

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036750.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 18:18
Operator : DD\AJ
Sample : M2809-04
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
JD310E-R2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:25:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

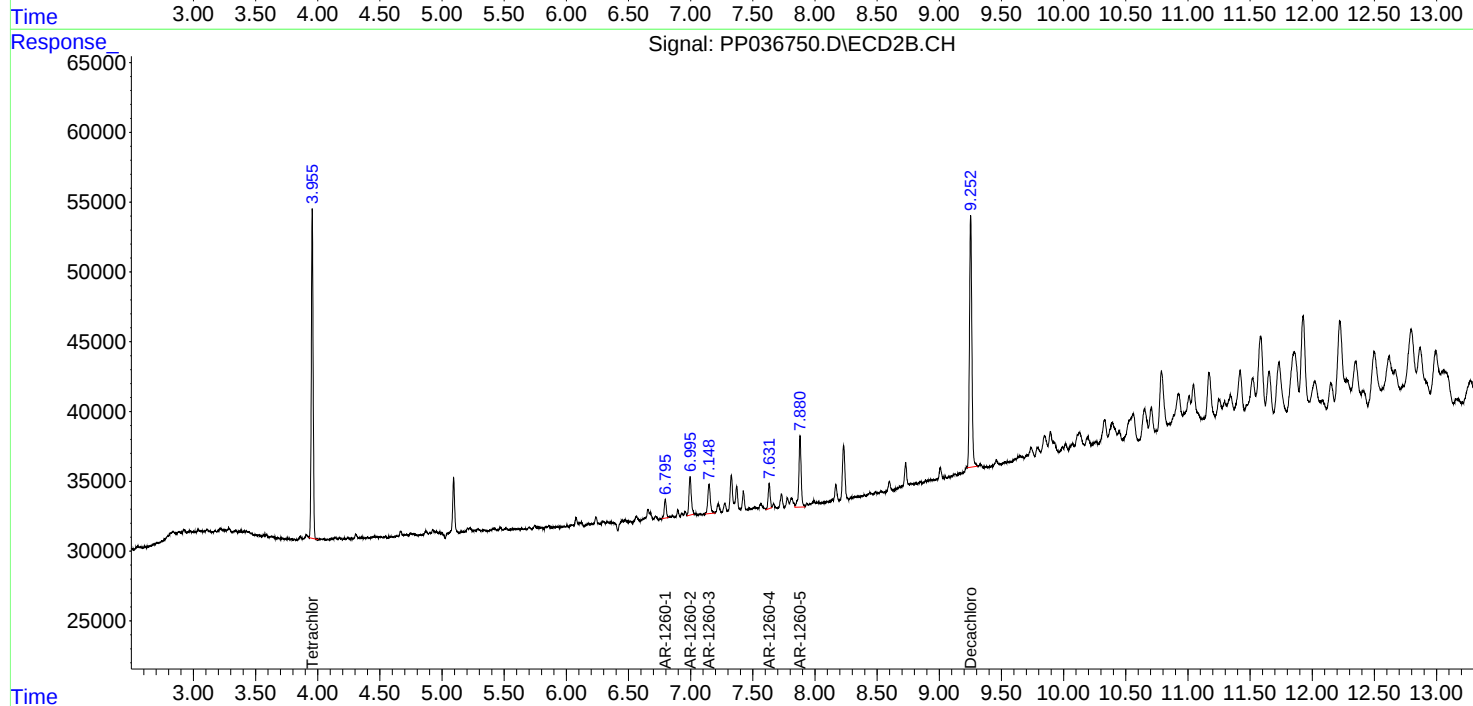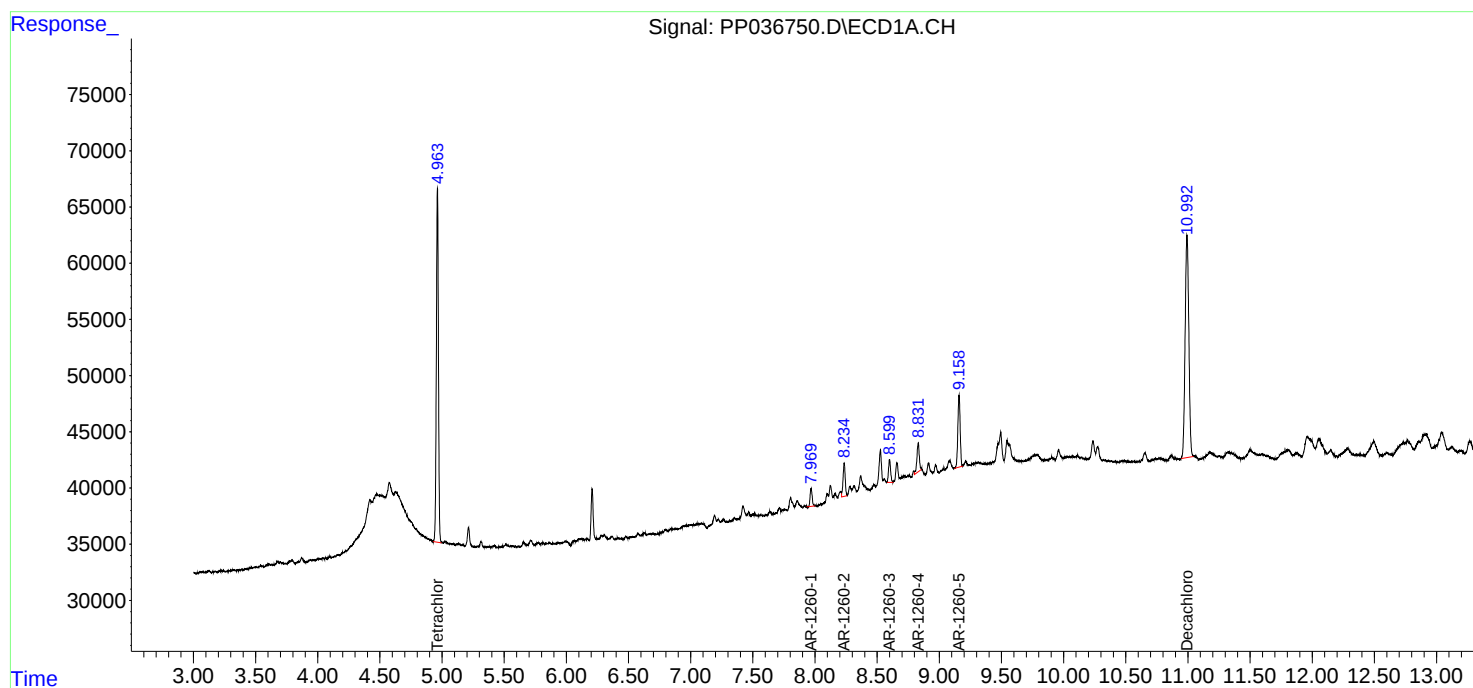

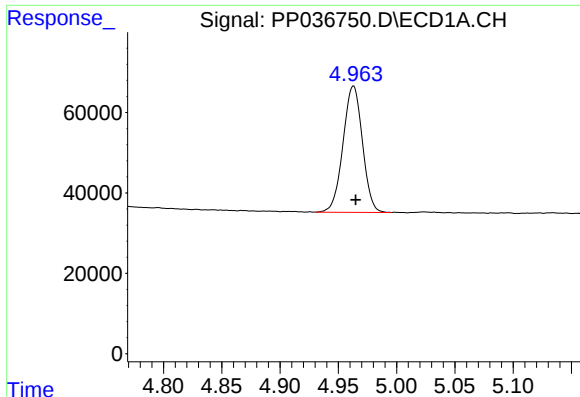


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 364890
Conc: 8.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
JD310E-R2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:09 PM

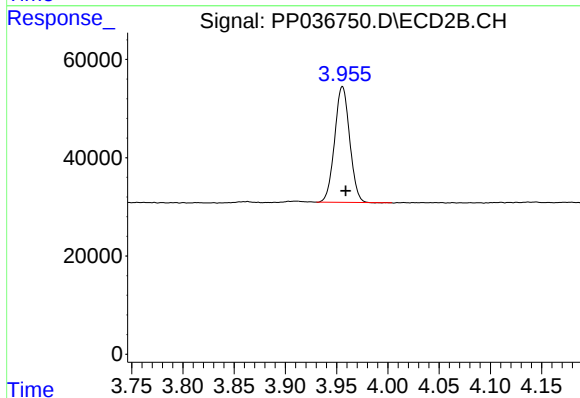


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.003 min
Response: 240299
Conc: 7.76 ng/ml

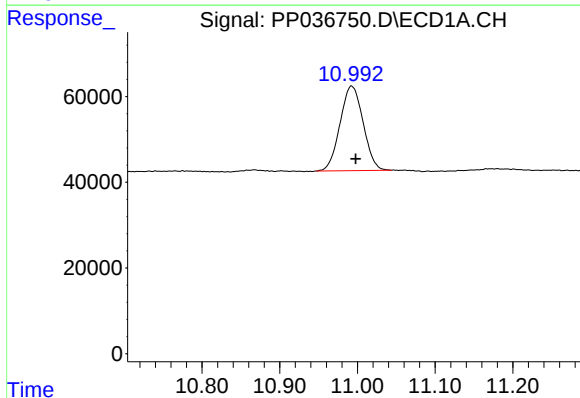


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.006 min
Response: 408285
Conc: 9.52 ng/ml

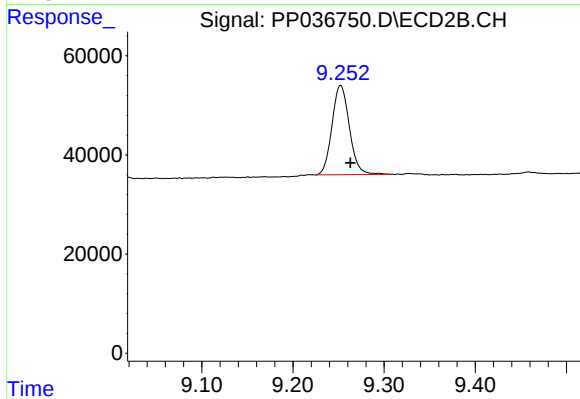

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.011 min
Response: 239204
Conc: 7.48 ng/ml

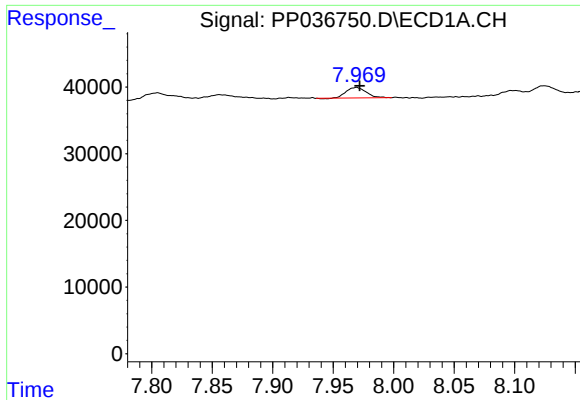


#31 AR-1260-1

R.T.: 7.969 min
Delta R.T.: -0.002 min
Response: 18196
Conc: 8.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
JD310E-R2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:09 PM

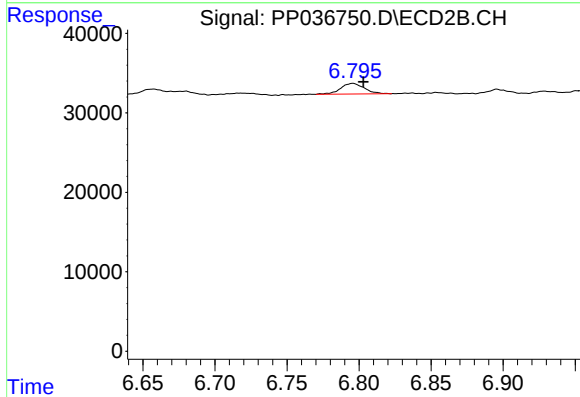


#31 AR-1260-1

R.T.: 6.796 min
Delta R.T.: -0.007 min
Response: 15509
Conc: 9.63 ng/ml

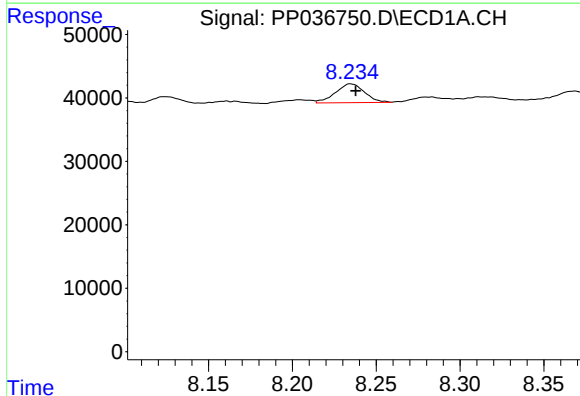


#32 AR-1260-2

R.T.: 8.235 min
Delta R.T.: -0.003 min
Response: 35693
Conc: 13.93 ng/ml

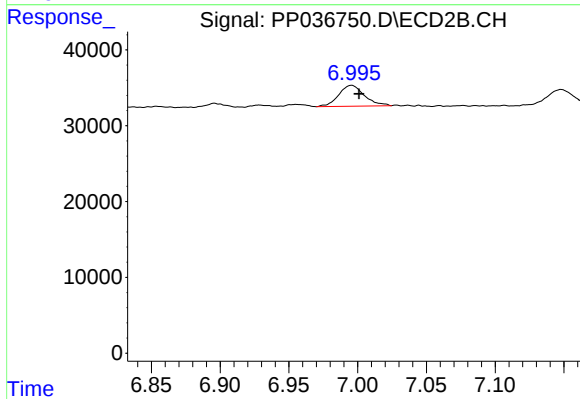

#32 AR-1260-2

R.T.: 6.996 min
Delta R.T.: -0.005 min
Response: 35863
Conc: 18.49 ng/ml

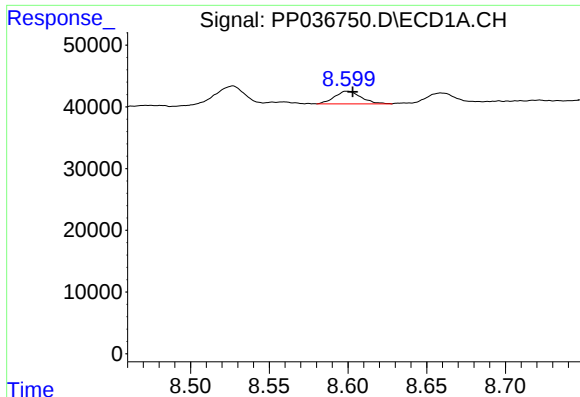


#33 AR-1260-3

R.T.: 8.599 min
Delta R.T.: -0.004 min
Response: 23694
Conc: 11.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
JD310E-R2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:09 PM

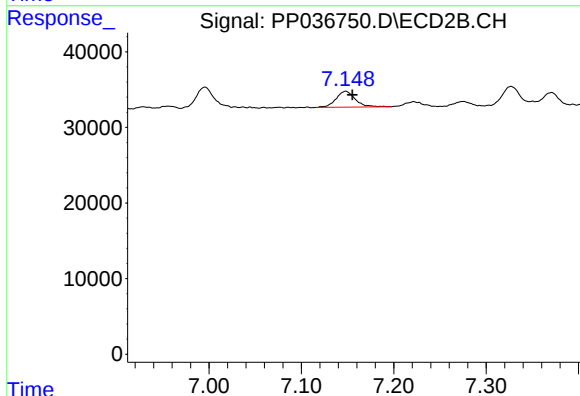


#33 AR-1260-3

R.T.: 7.148 min
Delta R.T.: -0.007 min
Response: 30253
Conc: 16.63 ng/ml

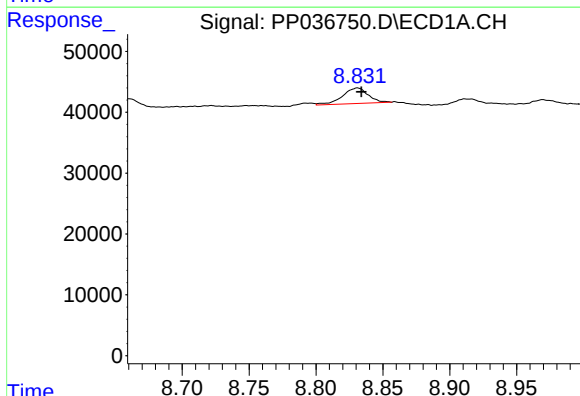


#34 AR-1260-4

R.T.: 8.831 min
Delta R.T.: -0.003 min
Response: 34354
Conc: 14.50 ng/ml

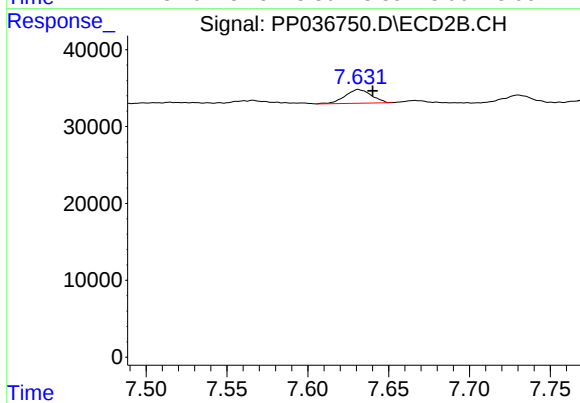

#34 AR-1260-4

R.T.: 7.631 min
Delta R.T.: -0.009 min
Response: 20063
Conc: 12.94 ng/ml m

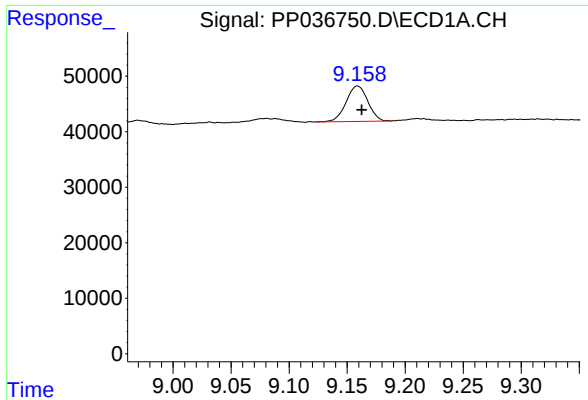


#35 AR-1260-5

R.T.: 9.159 min
Delta R.T.: -0.004 min
Response: 83018
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
JD310E-R2

Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:09 PM

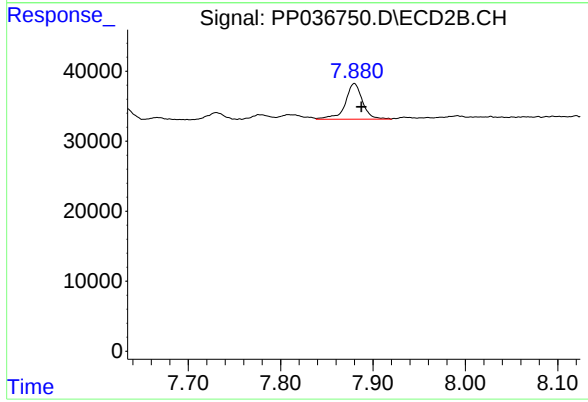

#35 AR-1260-5

R.T.: 7.880 min
Delta R.T.: -0.008 min
Response: 65876
Conc: 17.93 ng/ml