

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
 Data File : PP036752.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 18:52
 Operator : DD\AJ
 Sample : M2809-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 H151-I2

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:21:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:26:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.955	625615	420505	14.155	13.576
2) SA Decachlor...	10.993	9.252	674278	412401	15.718	12.895
Target Compounds						
31) L7 AR-1260-1	7.969	6.795	400522	279796	184.529	173.782
32) L7 AR-1260-2	8.234	6.994	574655	427769	224.216m	220.583
33) L7 AR-1260-3	8.600	7.148	548972	380936	273.872	209.456
34) L7 AR-1260-4	8.830	7.631	711104	475915	300.140	306.894
35) L7 AR-1260-5	9.159	7.880	1617916	1259621	362.606	342.777

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062321\
Data File : PP036752.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 18:52
Operator : DD\AJ
Sample : M2809-06
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
H151-I2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:26:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

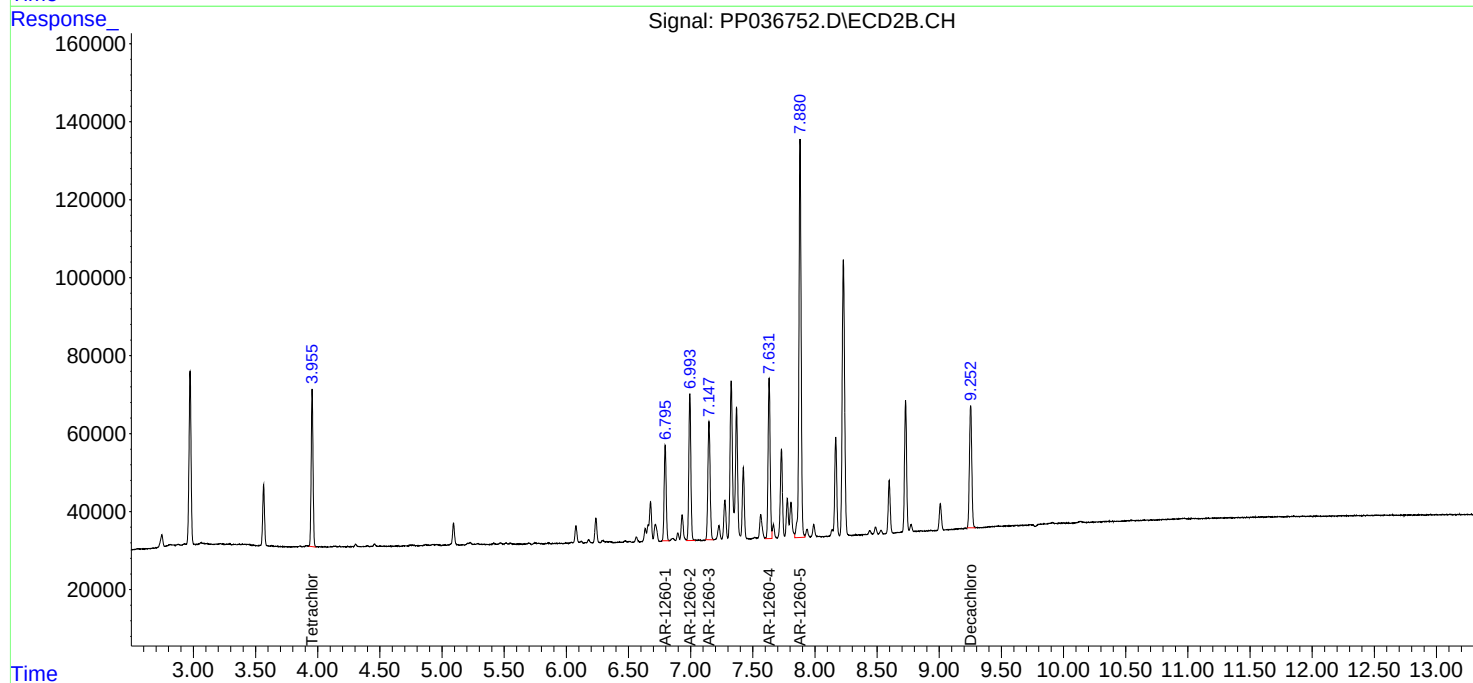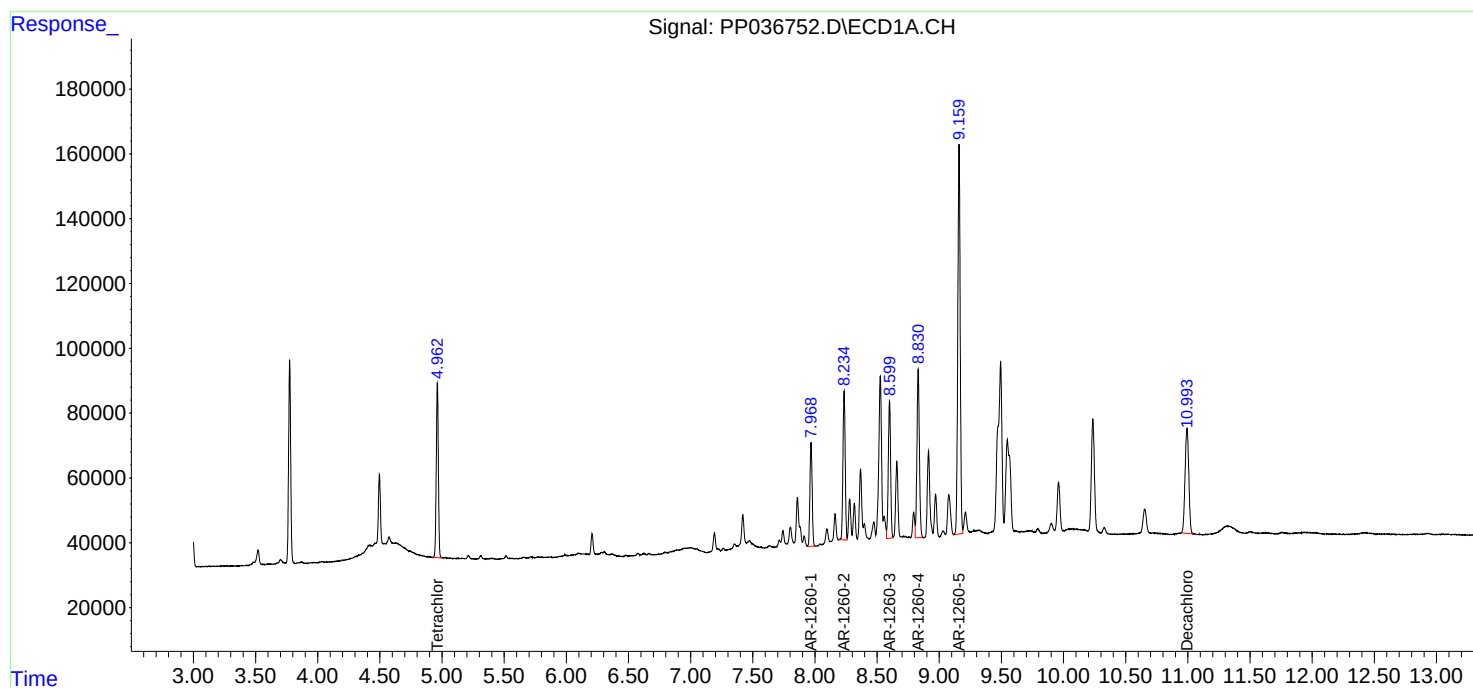

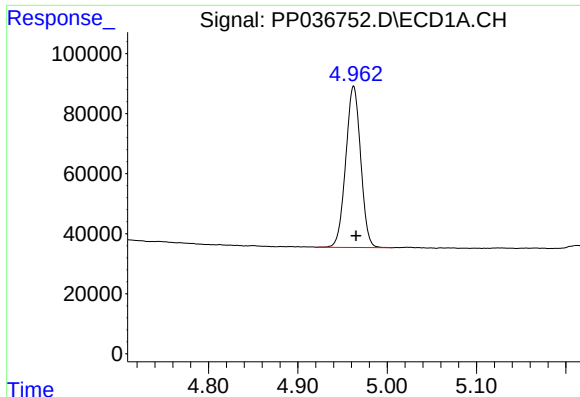


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 625615
Conc: 14.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
H151-I2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:11 PM

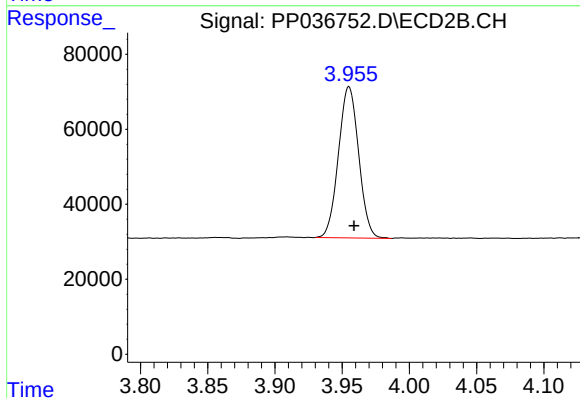


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 420505
Conc: 13.58 ng/ml

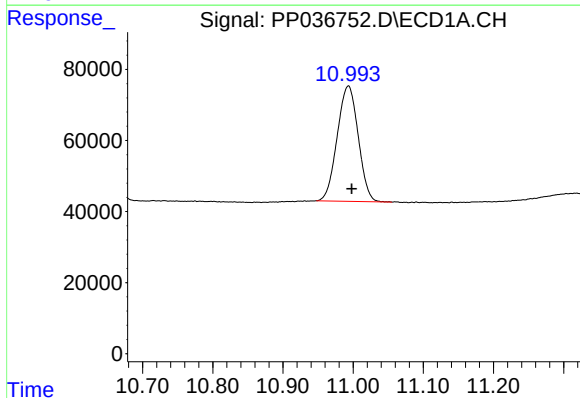


#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 674278
Conc: 15.72 ng/ml

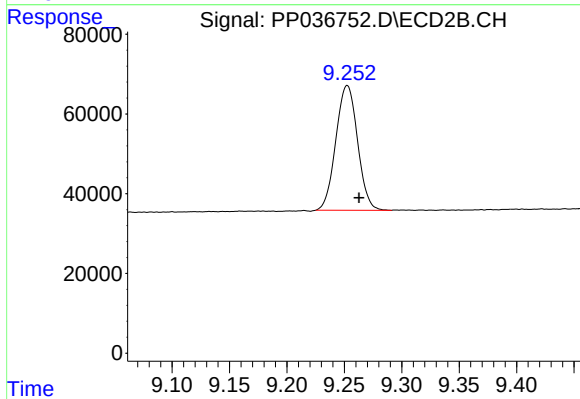

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.010 min
Response: 412401
Conc: 12.90 ng/ml

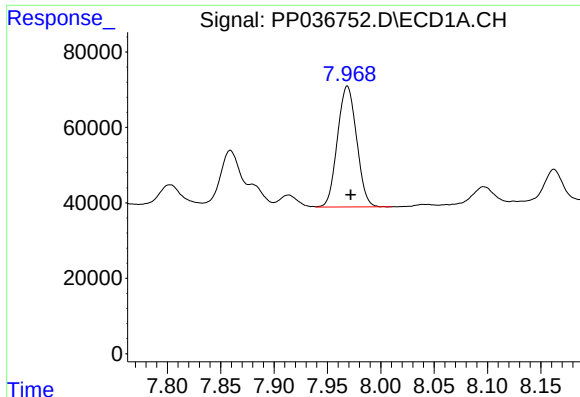


#31 AR-1260-1

R.T.: 7.969 min
Delta R.T.: -0.003 min
Response: 400522
Conc: 184.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
H151-I2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:11 PM

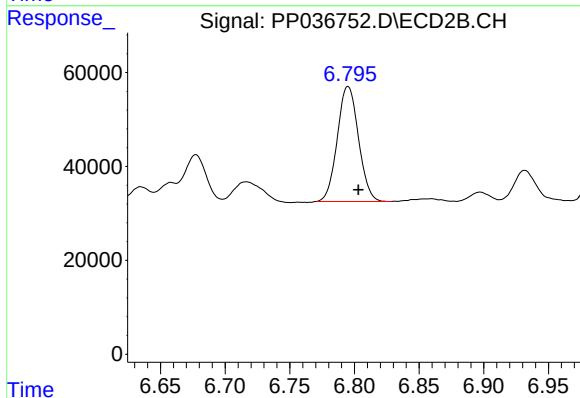


#31 AR-1260-1

R.T.: 6.795 min
Delta R.T.: -0.008 min
Response: 279796
Conc: 173.78 ng/ml

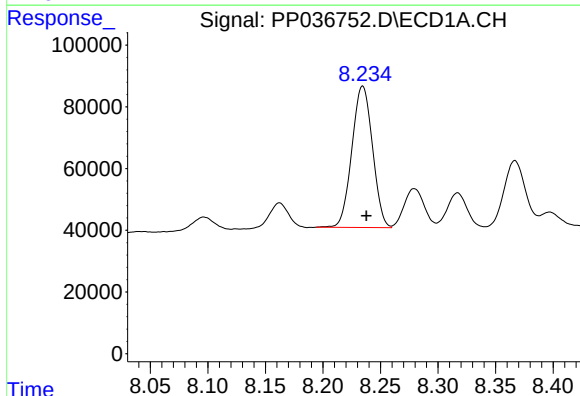


#32 AR-1260-2

R.T.: 8.234 min
Delta R.T.: -0.003 min
Response: 574655
Conc: 224.22 ng/ml m

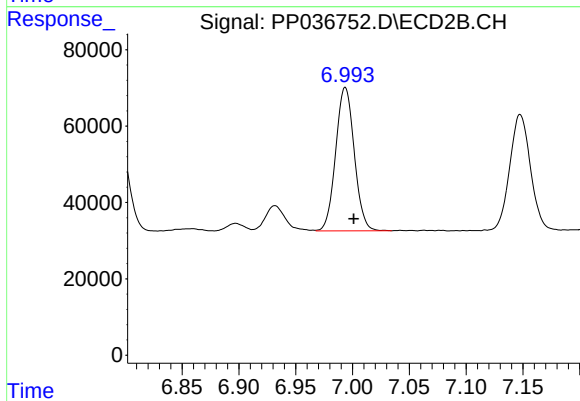

#32 AR-1260-2

R.T.: 6.994 min
Delta R.T.: -0.007 min
Response: 427769
Conc: 220.58 ng/ml

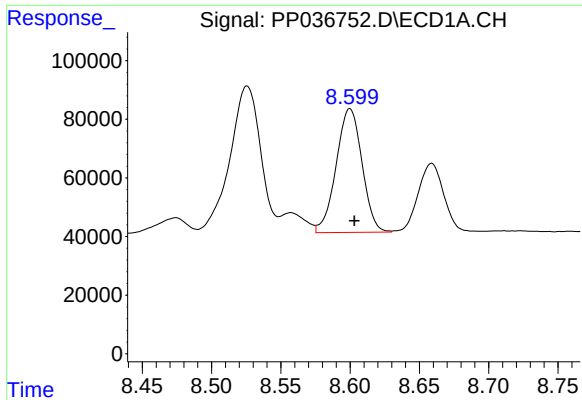


#33 AR-1260-3

R.T.: 8.600 min
Delta R.T.: -0.003 min
Response: 548972
Conc: 273.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
H151-I2


Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:11 PM

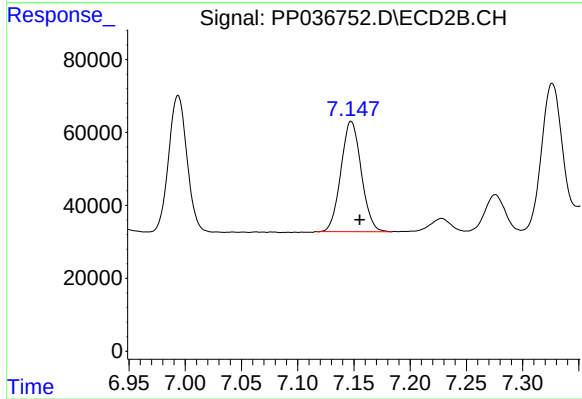


#33 AR-1260-3

R.T.: 7.148 min
Delta R.T.: -0.008 min
Response: 380936
Conc: 209.46 ng/ml

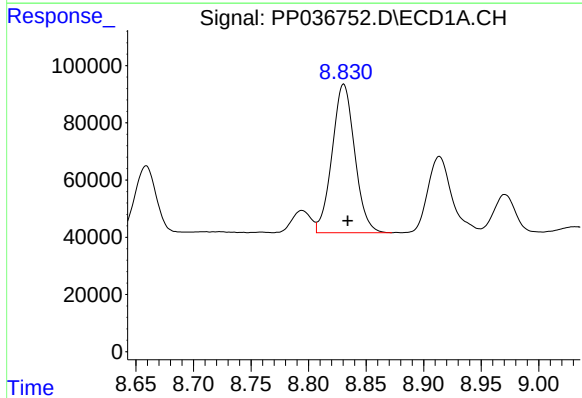


#34 AR-1260-4

R.T.: 8.830 min
Delta R.T.: -0.004 min
Response: 711104
Conc: 300.14 ng/ml

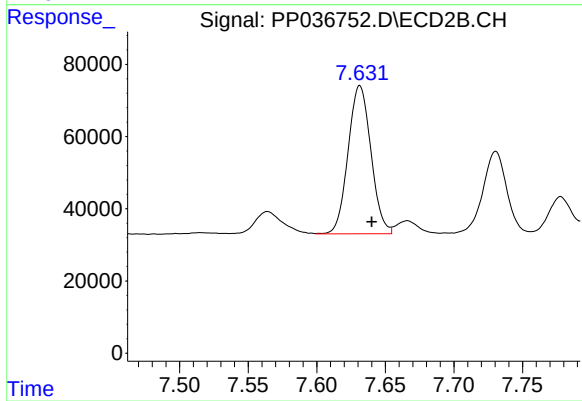

#34 AR-1260-4

R.T.: 7.631 min
Delta R.T.: -0.009 min
Response: 475915
Conc: 306.89 ng/ml

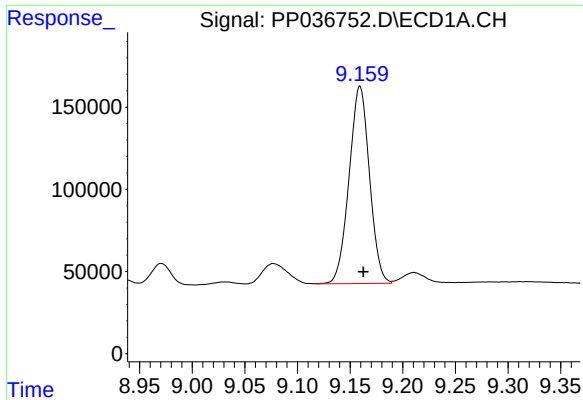


#35 AR-1260-5

R.T.: 9.159 min
Delta R.T.: -0.003 min
Response: 1617916
Conc: 362.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
H151-I2

Manual Integrations
APPROVED

Ankita
6/24/2021 1:21:11 PM

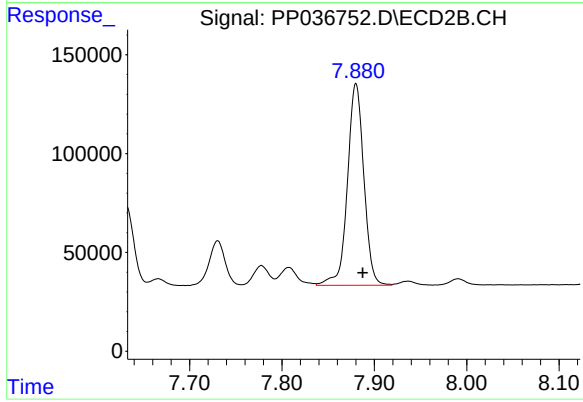

#35 AR-1260-5

R.T.: 7.880 min
Delta R.T.: -0.007 min
Response: 1259621
Conc: 342.78 ng/ml