

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062325\
 Data File : PP073182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2025 18:08
 Operator : YP\AJ
 Sample : Q2384-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-01-6202025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/24/2025
 Supervised By :mohammad ahmed 06/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:46:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.789	31131373	36400631	14.749m	20.202m#
2) SA Decachlor...	10.184	8.797	25336350	22559759	14.826	16.902

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062325\
Data File : PP073182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2025 18:08
Operator : YP\AJ
Sample : Q2384-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OK-01-6202025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2025
Supervised By :mohammad ahmed 06/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:46:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

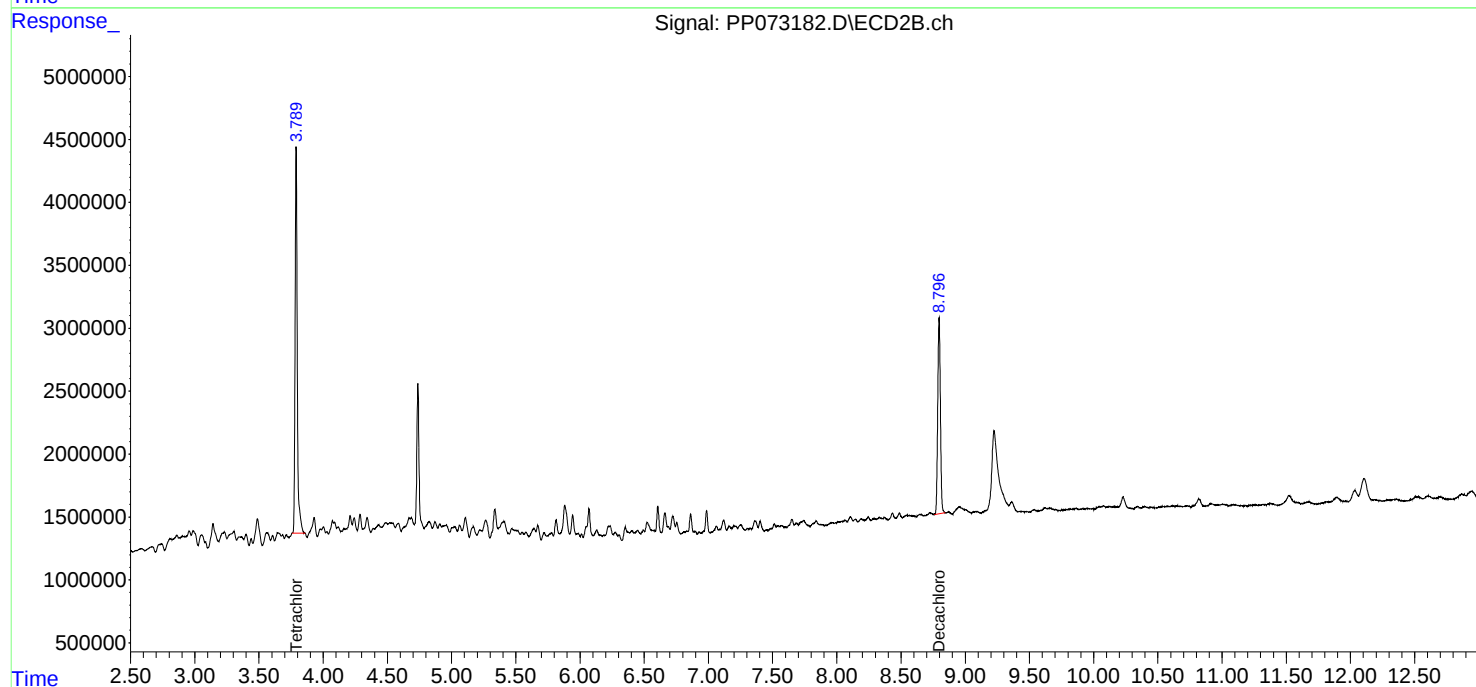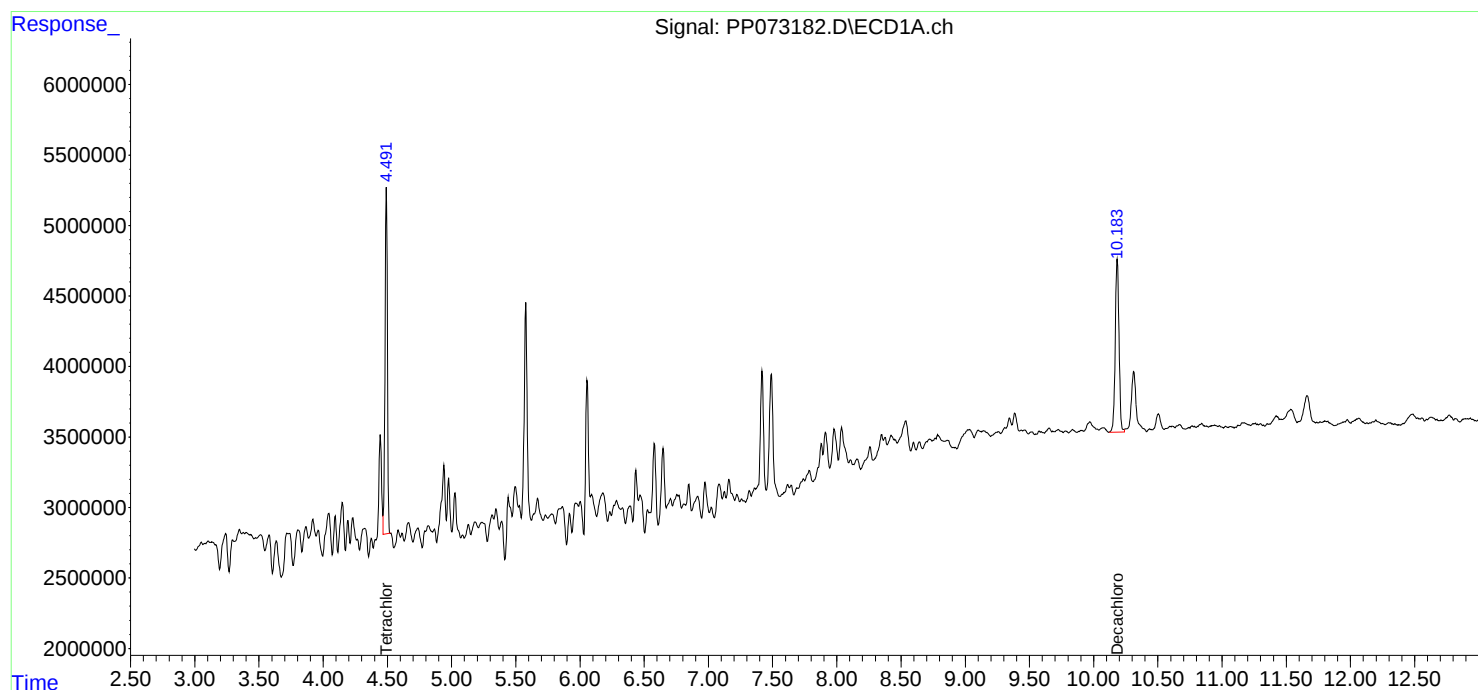

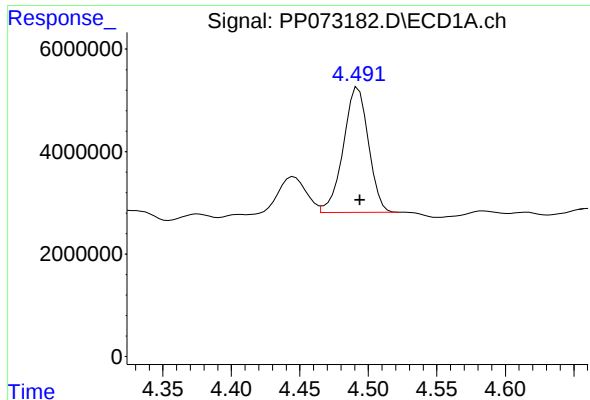


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: -0.003 min
Response: 31131373
Conc: 14.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-01-6202025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2025
Supervised By :mohammad ahmed 06/25/2025

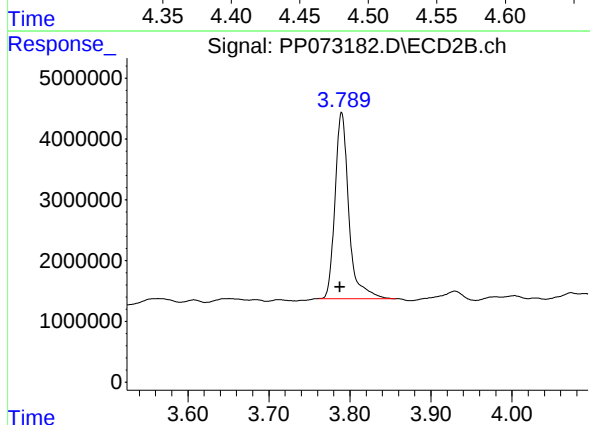


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.002 min
Response: 36400631
Conc: 20.20 ng/ml m

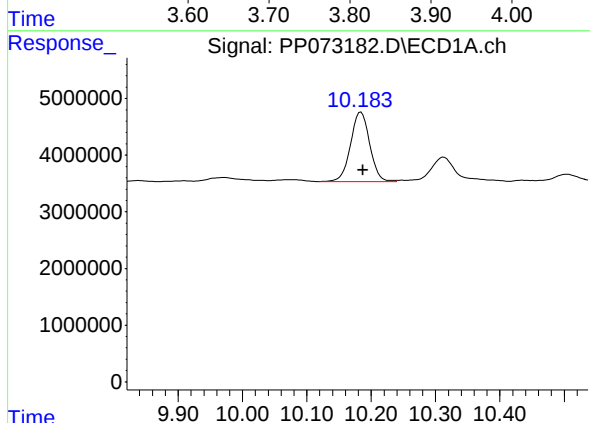

#2 Decachlorobiphenyl

R.T.: 10.184 min
Delta R.T.: -0.003 min
Response: 25336350
Conc: 14.83 ng/ml

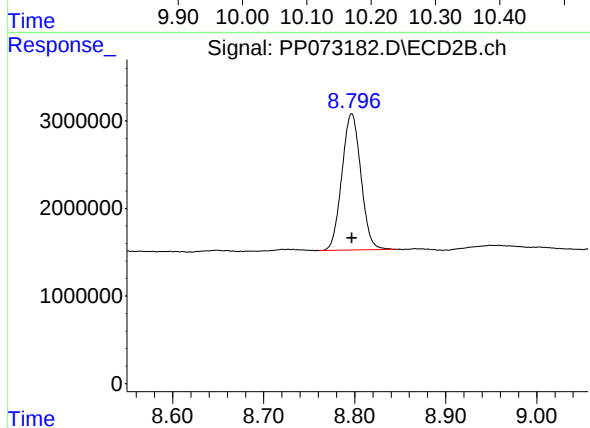

#2 Decachlorobiphenyl

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 22559759
Conc: 16.90 ng/ml