

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
 Data File : PP036780.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2021 17:47
 Operator : DD\AJ
 Sample : M2833-01MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-01-D8-C9-D8A-C9AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:52:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.961	3.953	924634	591225	20.920	19.088
2)	SA Decachlor...	10.990	9.250	922315	572329	21.500	17.896
Target Compounds							
3)	L1 AR-1016-1	6.281	5.205	790007	512514	466.398	434.755
4)	L1 AR-1016-2	6.305	5.226	1123463	713753	465.926	439.465
5)	L1 AR-1016-3	6.370	5.416	716729	390856	466.240	433.217
6)	L1 AR-1016-4	6.478	5.469	600846	297789	467.386	419.490
7)	L1 AR-1016-5	6.791	5.696	577018	387367	451.128	427.451
8)	L2 AR-1221-1	5.210	4.209	130955	51821	233.259	133.165 #
9)	L2 AR-1221-2	5.309	4.308	99589	66429	231.102	222.553
10)	L2 AR-1221-3	5.396	4.396	446593	285633	346.405	316.305
11)	L3 AR-1232-1	5.396	4.396	446593	285633	419.306	388.265
12)	L3 AR-1232-2	5.985	5.226	579018	713753	1052.806	1067.419
13)	L3 AR-1232-3	6.305	5.416	1123463	390856	1099.754	1077.404
14)	L3 AR-1232-4	6.478	5.513	600846	366651	1113.129	1170.876
15)	L3 AR-1232-5	6.575	5.696	462446	387367	1261.784	1087.520
16)	L4 AR-1242-1	6.281	5.205	790007	512514	616.066	575.799
17)	L4 AR-1242-2	6.305	5.226	1123463	713753	615.657	585.135
18)	L4 AR-1242-3	6.370	5.416	716729	390856	610.939	580.869
19)	L4 AR-1242-4	6.478	5.513	600846	366651	620.858	566.319
20)	L4 AR-1242-5	7.259	6.076	85212	308074	81.010	377.587 #
21)	L5 AR-1248-1	6.281	5.205	790007	512514	783.097	735.559
22)	L5 AR-1248-2	6.575	5.469	462446	297789	340.520	314.395
23)	L5 AR-1248-3	6.791	5.513	577018	366651	354.635	370.565
24)	L5 AR-1248-4	7.219	5.696	96830	387367	53.036	331.160 #
25)	L5 AR-1248-5	7.259	6.119	85212	49090	47.260	41.385
26)	L6 AR-1254-1	7.189	6.076	440235	308074	250.324	181.823 #
27)	L6 AR-1254-2	7.418	6.236	477987	290640	176.658	195.401
28)	L6 AR-1254-3	7.801	6.656	281216	153681	94.940	63.213 #
29)	L6 AR-1254-4	8.094	6.896	176579	62573	80.323	40.436 #
30)	L6 AR-1254-5	8.524	7.325	1521499	1047391	639.785	487.094
31)	L7 AR-1260-1	7.967	6.794	1030812	699695	474.918	434.582
32)	L7 AR-1260-2	8.232	6.992	1206800	859721	470.864	443.323
33)	L7 AR-1260-3	8.598	7.145	805982	811218	402.090	446.045
34)	L7 AR-1260-4	8.828	7.630	1029749	543164	434.633	350.260
35)	L7 AR-1260-5	9.157	7.879	1868397	1421801	418.743	386.911
36)	L8 AR-1262-1	8.598	7.325	805982	1047391	282.855	878.768 #
37)	L8 AR-1262-2	9.157	7.879	1868397	1421801	367.735	362.701
38)	L8 AR-1262-3	9.492f	8.166	1311975	280408	354.152	176.196 #
39)	L8 AR-1262-4	9.544f	8.227	759722	1043860	264.512	350.717 #
40)	L8 AR-1262-5	10.234	8.727	549871	336127	260.265	235.871
41)	L9 AR-1268-1	9.492f	8.166	1311975	280408	218.680	60.217 #
42)	L9 AR-1268-2	9.544f	8.227	759722	1043860	133.276	241.994 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
 Data File : PP036780.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2021 17:47
 Operator : DD\AJ
 Sample : M2833-01MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-01-D8-C9-D8A-C9AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:52:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.792	8.439	43954	24861	9.142	6.809 #
44) L9	AR-1268-4	10.234	8.727	549871	336127	233.442	211.305
45) L9	AR-1268-5	10.650	9.007	193370	110890	12.574	9.379 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
Data File : PP036780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2021 17:47
Operator : DD\AJ
Sample : M2833-01MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 02:52:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

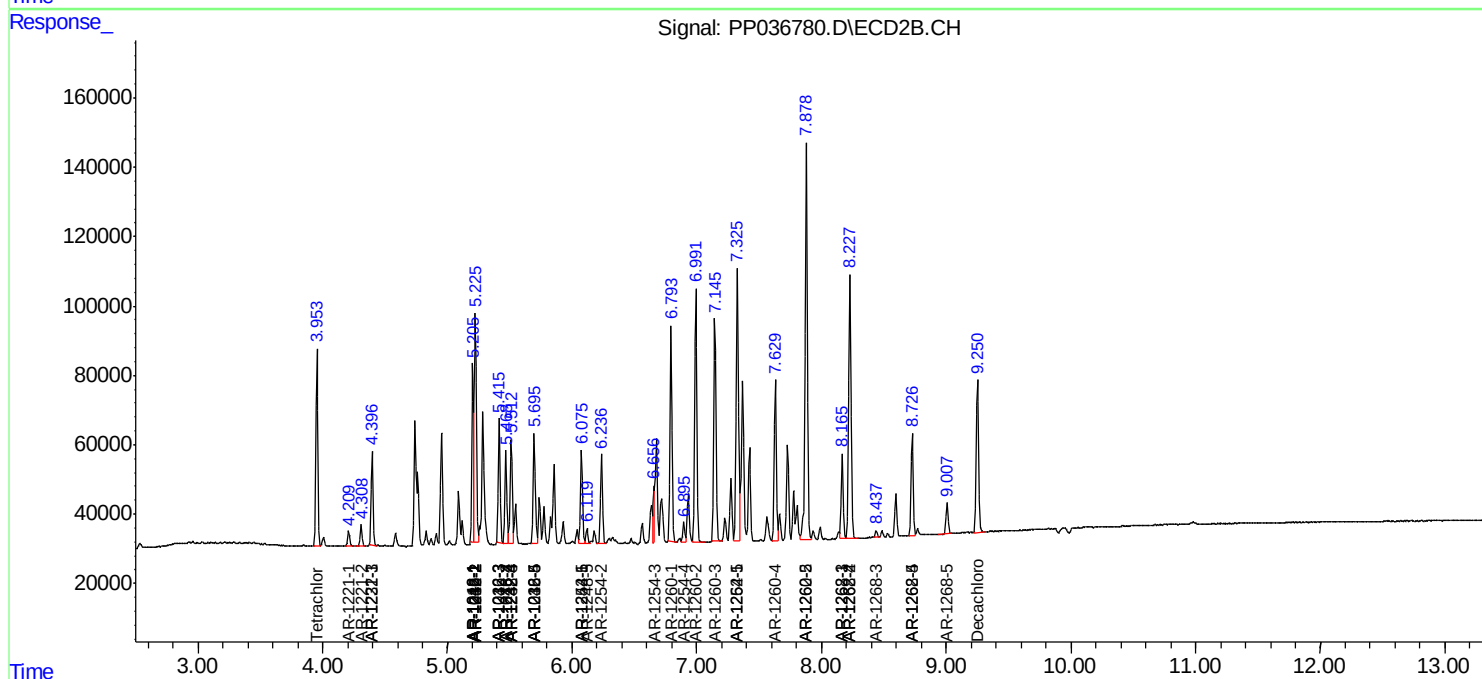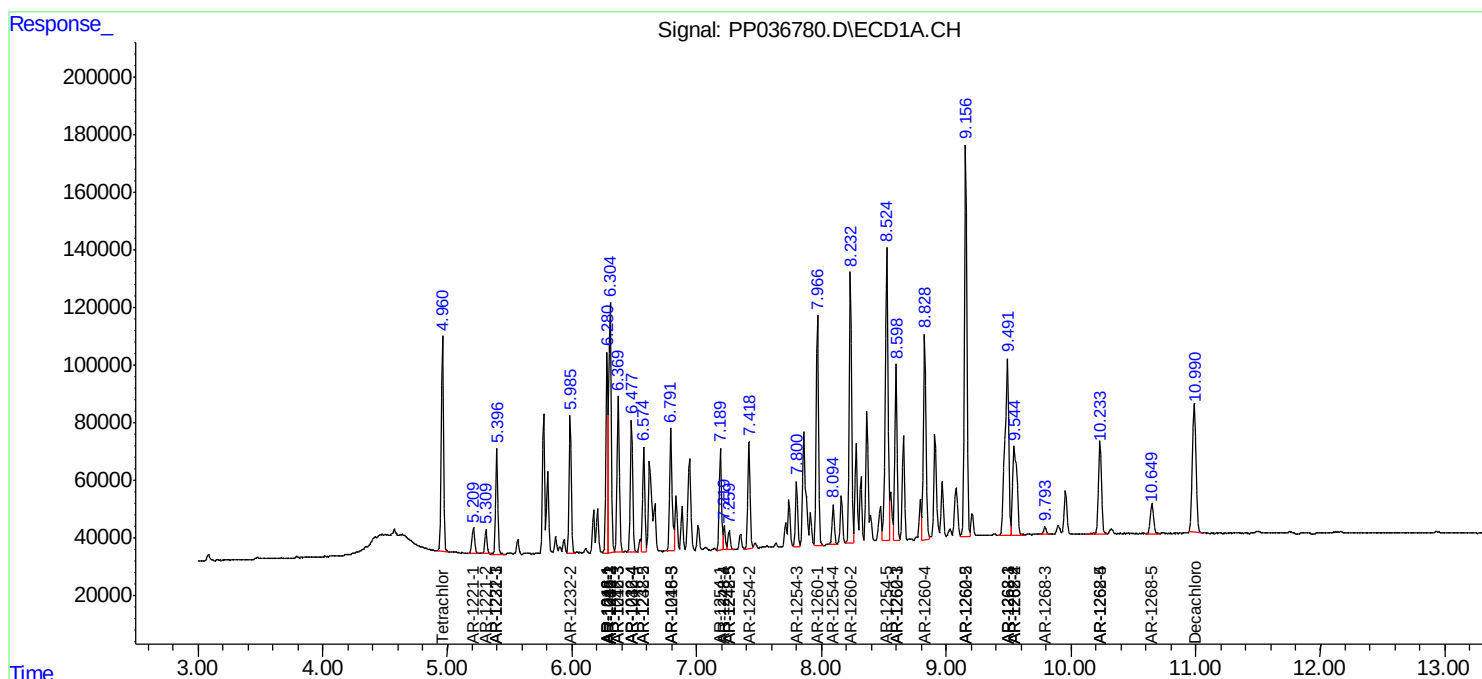




#1 Tetrachloro-m-xylene


R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 924634
Conc: 20.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

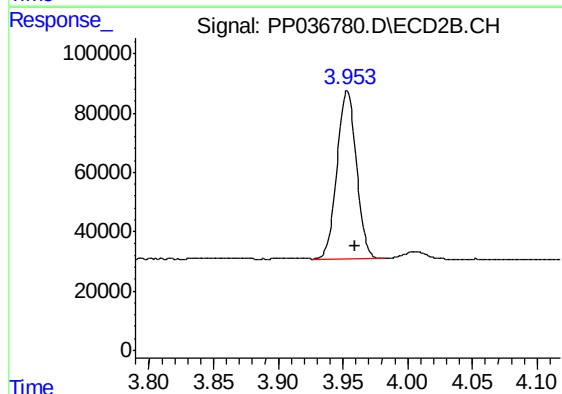


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.006 min
Response: 591225
Conc: 19.09 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.990 min
Delta R.T.: -0.008 min
Response: 922315
Conc: 21.50 ng/ml

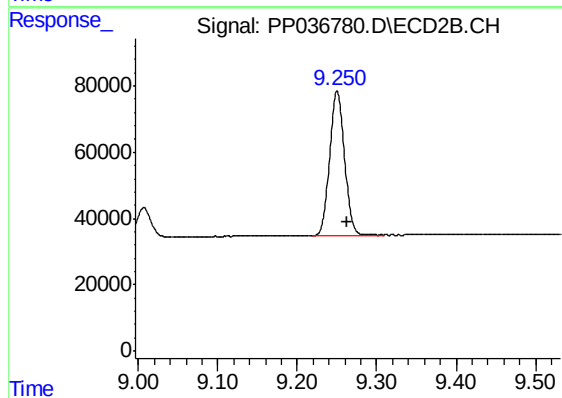

#2 Decachlorobiphenyl


R.T.: 9.250 min
Delta R.T.: -0.013 min
Response: 572329
Conc: 17.90 ng/ml

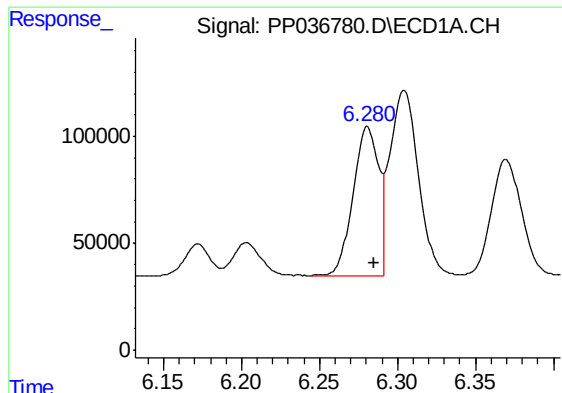

#3 AR-1016-1


R.T.: 6.281 min
Delta R.T.: -0.004 min
Response: 790007
Conc: 466.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

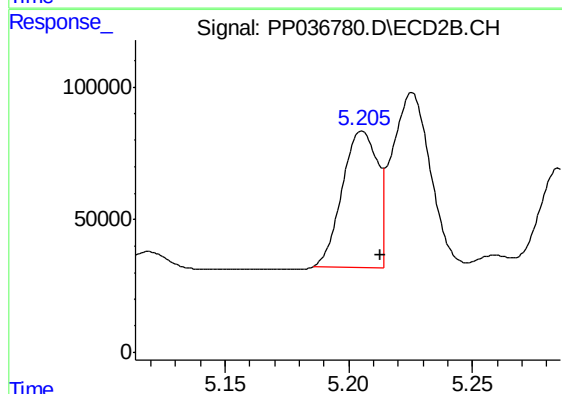


#3 AR-1016-1

R.T.: 5.205 min
Delta R.T.: -0.008 min
Response: 512514
Conc: 434.75 ng/ml

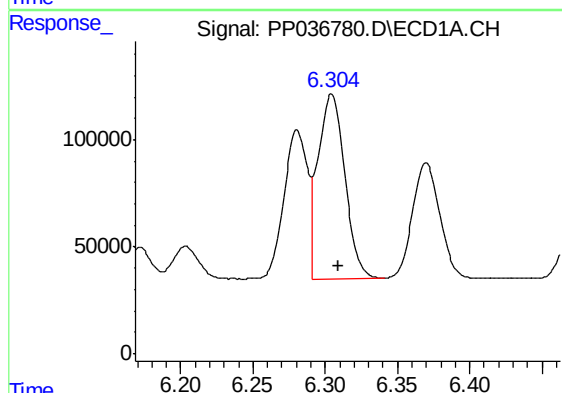


#4 AR-1016-2

R.T.: 6.305 min
Delta R.T.: -0.005 min
Response: 1123463
Conc: 465.93 ng/ml

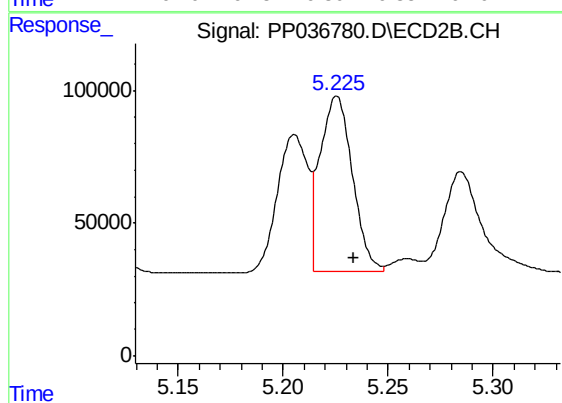

#4 AR-1016-2


R.T.: 5.226 min
Delta R.T.: -0.008 min
Response: 713753
Conc: 439.46 ng/ml

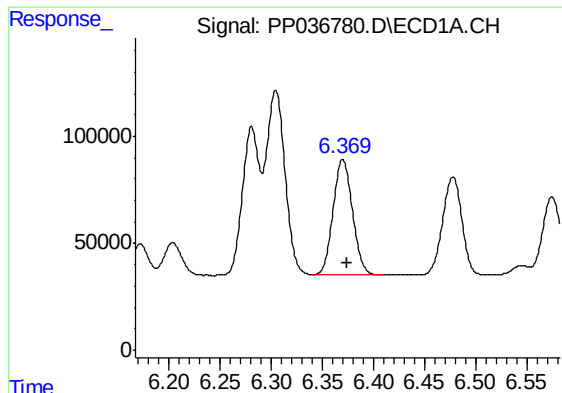

#5 AR-1016-3


R.T.: 6.370 min
Delta R.T.: -0.005 min
Response: 716729
Conc: 466.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

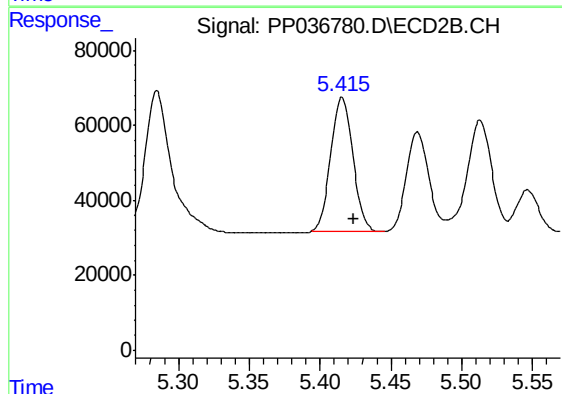


#5 AR-1016-3

R.T.: 5.416 min
Delta R.T.: -0.008 min
Response: 390856
Conc: 433.22 ng/ml




#6 AR-1016-4

R.T.: 6.478 min
Delta R.T.: -0.004 min
Response: 600846
Conc: 467.39 ng/ml

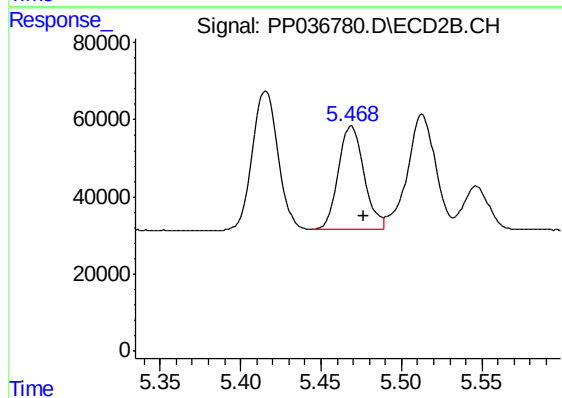

#6 AR-1016-4


R.T.: 5.469 min
Delta R.T.: -0.008 min
Response: 297789
Conc: 419.49 ng/ml



#7 AR-1016-5


R.T.: 6.791 min
Delta R.T.: -0.005 min
Response: 577018
Conc: 451.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

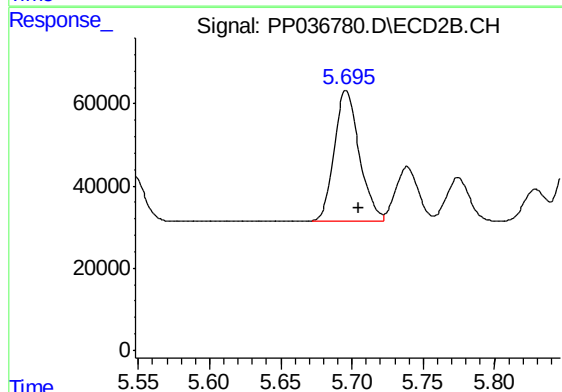


#7 AR-1016-5

R.T.: 5.696 min
Delta R.T.: -0.009 min
Response: 387367
Conc: 427.45 ng/ml




#8 AR-1221-1

R.T.: 5.210 min
Delta R.T.: -0.006 min
Response: 130955
Conc: 233.26 ng/ml

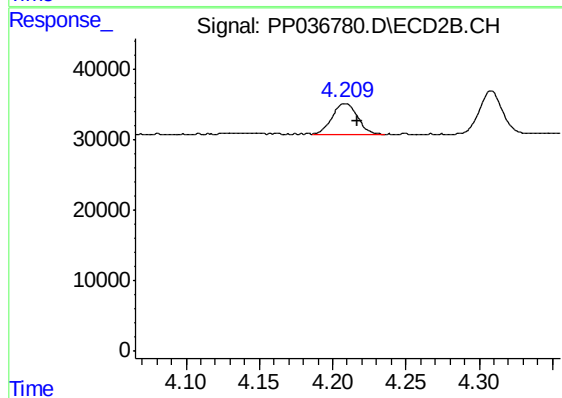

#8 AR-1221-1


R.T.: 4.209 min
Delta R.T.: -0.008 min
Response: 51821
Conc: 133.16 ng/ml



#9 AR-1221-2


R.T.: 5.309 min
Delta R.T.: -0.006 min
Response: 99589
Conc: 231.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

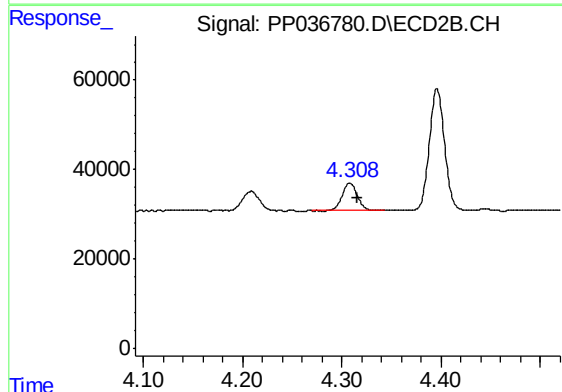


#9 AR-1221-2

R.T.: 4.308 min
Delta R.T.: -0.007 min
Response: 66429
Conc: 222.55 ng/ml

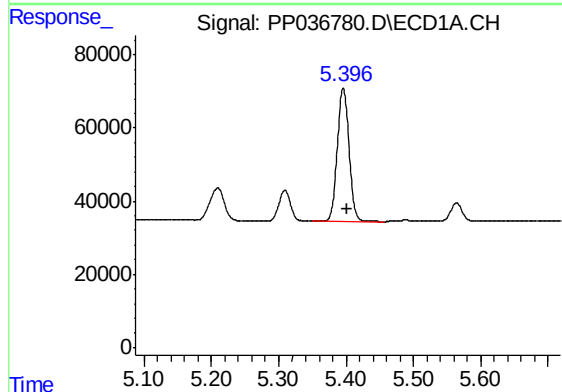


#10 AR-1221-3

R.T.: 5.396 min
Delta R.T.: -0.006 min
Response: 446593
Conc: 346.41 ng/ml

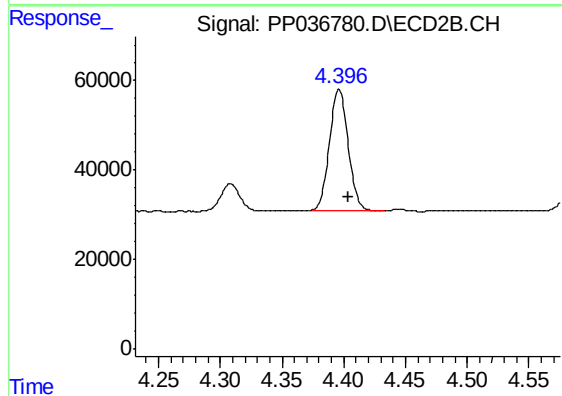

#10 AR-1221-3


R.T.: 4.396 min
Delta R.T.: -0.008 min
Response: 285633
Conc: 316.31 ng/ml



#11 AR-1232-1


R.T.: 5.396 min
Delta R.T.: -0.004 min
Response: 446593
Conc: 419.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

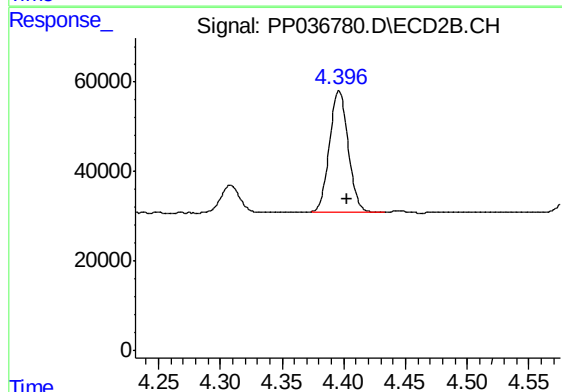


#11 AR-1232-1

R.T.: 4.396 min
Delta R.T.: -0.006 min
Response: 285633
Conc: 388.26 ng/ml

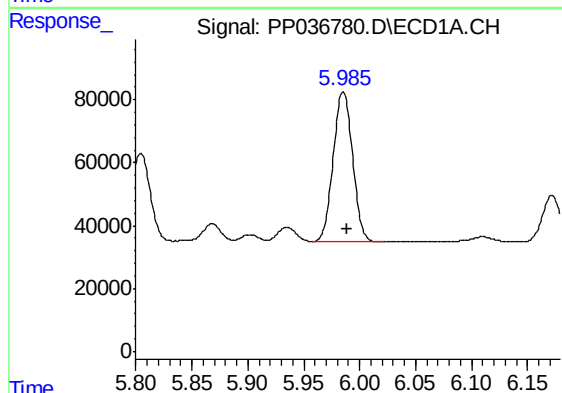


#12 AR-1232-2

R.T.: 5.985 min
Delta R.T.: -0.004 min
Response: 579018
Conc: 1052.81 ng/ml

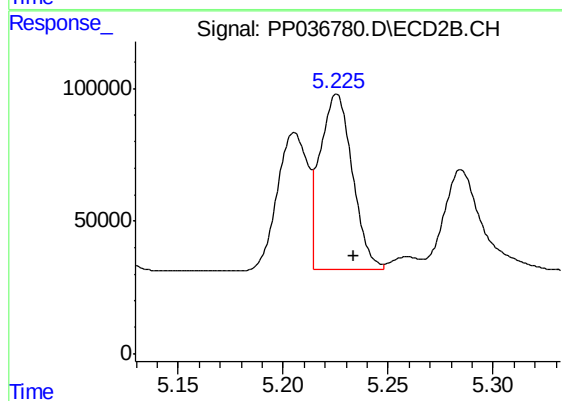

#12 AR-1232-2


R.T.: 5.226 min
Delta R.T.: -0.008 min
Response: 713753
Conc: 1067.42 ng/ml



#13 AR-1232-3


R.T.: 6.305 min
Delta R.T.: -0.004 min
Response: 1123463
Conc: 1099.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

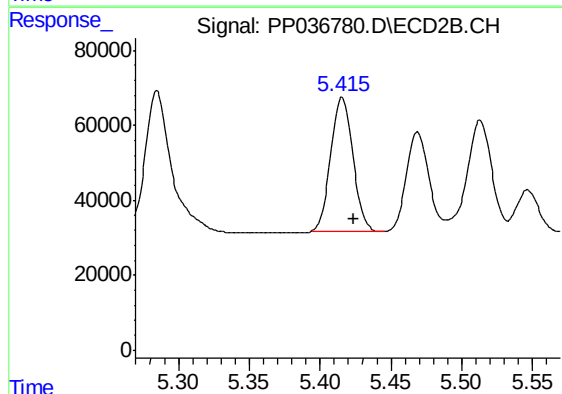


#13 AR-1232-3

R.T.: 5.416 min
Delta R.T.: -0.008 min
Response: 390856
Conc: 1077.40 ng/ml




#14 AR-1232-4

R.T.: 6.478 min
Delta R.T.: -0.004 min
Response: 600846
Conc: 1113.13 ng/ml

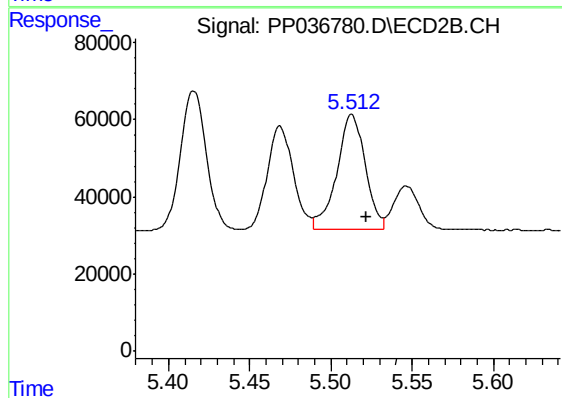

#14 AR-1232-4


R.T.: 5.513 min
Delta R.T.: -0.009 min
Response: 366651
Conc: 1170.88 ng/ml

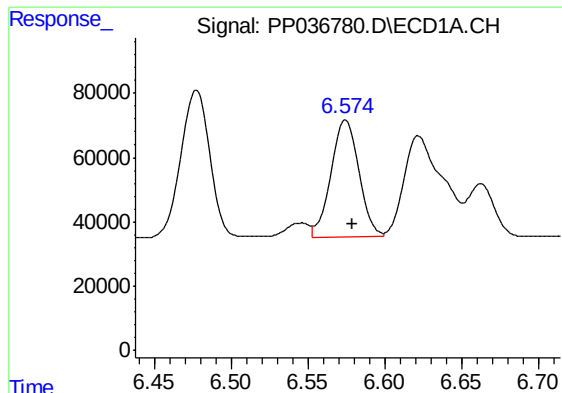

#15 AR-1232-5


R.T.: 6.575 min
Delta R.T.: -0.004 min
Response: 462446
Conc: 1261.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

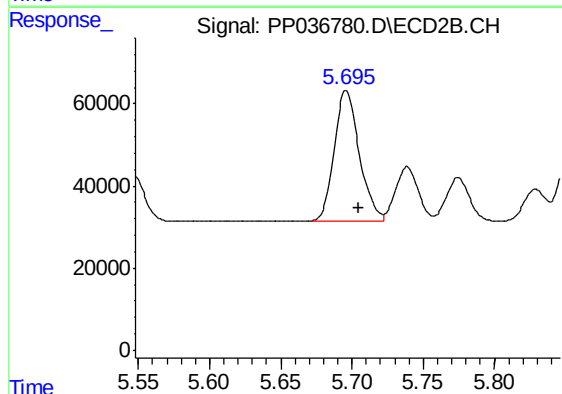


#15 AR-1232-5

R.T.: 5.696 min
Delta R.T.: -0.009 min
Response: 387367
Conc: 1087.52 ng/ml

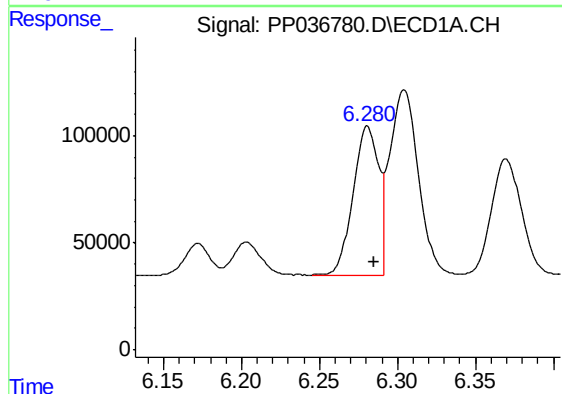


#16 AR-1242-1

R.T.: 6.281 min
Delta R.T.: -0.004 min
Response: 790007
Conc: 616.07 ng/ml

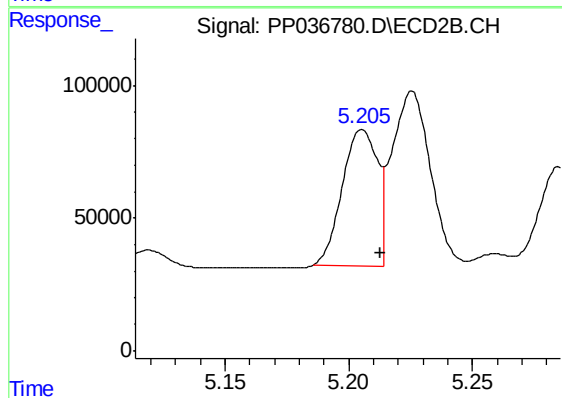

#16 AR-1242-1


R.T.: 5.205 min
Delta R.T.: -0.007 min
Response: 512514
Conc: 575.80 ng/ml



#17 AR-1242-2


R.T.: 6.305 min
Delta R.T.: -0.004 min
Response: 1123463
Conc: 615.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

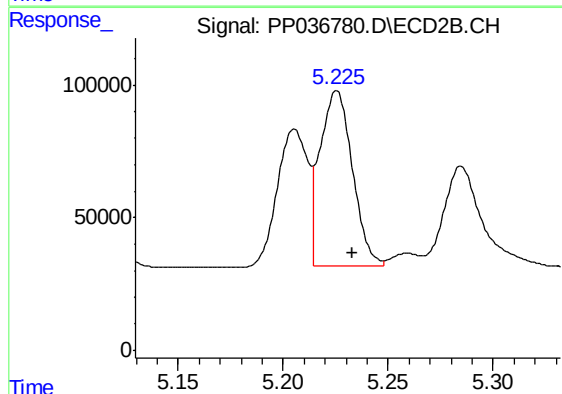


#17 AR-1242-2

R.T.: 5.226 min
Delta R.T.: -0.007 min
Response: 713753
Conc: 585.13 ng/ml




#18 AR-1242-3

R.T.: 6.370 min
Delta R.T.: -0.005 min
Response: 716729
Conc: 610.94 ng/ml

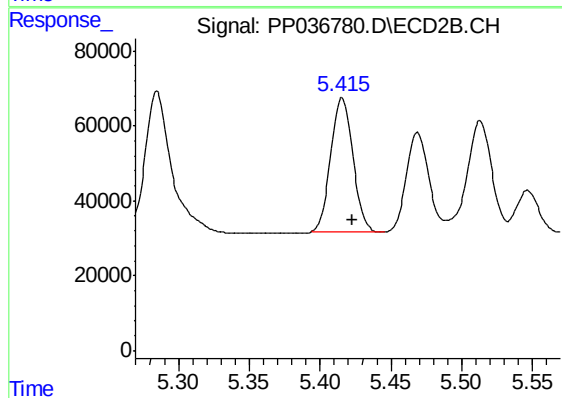

#18 AR-1242-3


R.T.: 5.416 min
Delta R.T.: -0.008 min
Response: 390856
Conc: 580.87 ng/ml



#19 AR-1242-4


R.T.: 6.478 min
Delta R.T.: -0.004 min
Response: 600846
Conc: 620.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

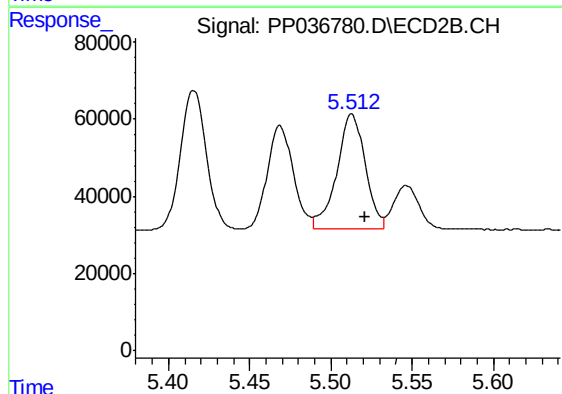


#19 AR-1242-4

R.T.: 5.513 min
Delta R.T.: -0.008 min
Response: 366651
Conc: 566.32 ng/ml




#20 AR-1242-5

R.T.: 7.259 min
Delta R.T.: -0.005 min
Response: 85212
Conc: 81.01 ng/ml

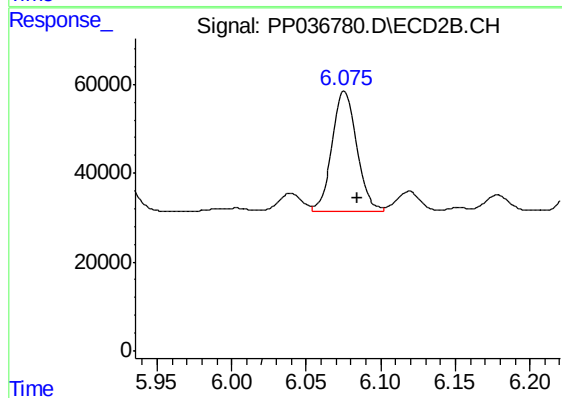

#20 AR-1242-5


R.T.: 6.076 min
Delta R.T.: -0.008 min
Response: 308074
Conc: 377.59 ng/ml

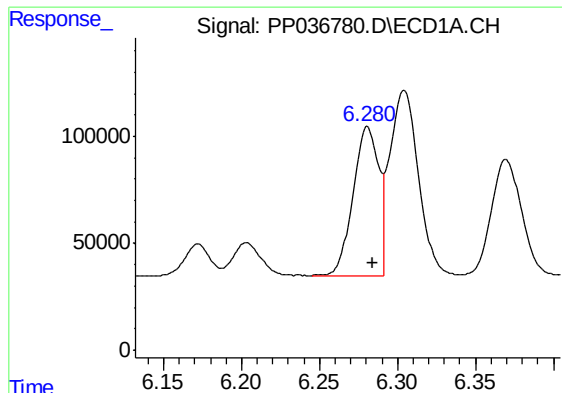

#21 AR-1248-1


R.T.: 6.281 min
Delta R.T.: -0.004 min
Response: 790007
Conc: 783.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

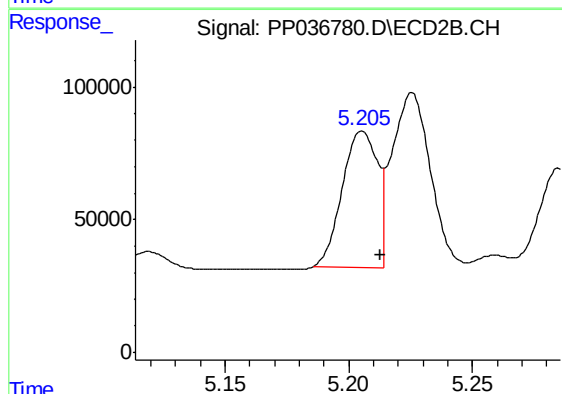


#21 AR-1248-1

R.T.: 5.205 min
Delta R.T.: -0.007 min
Response: 512514
Conc: 735.56 ng/ml

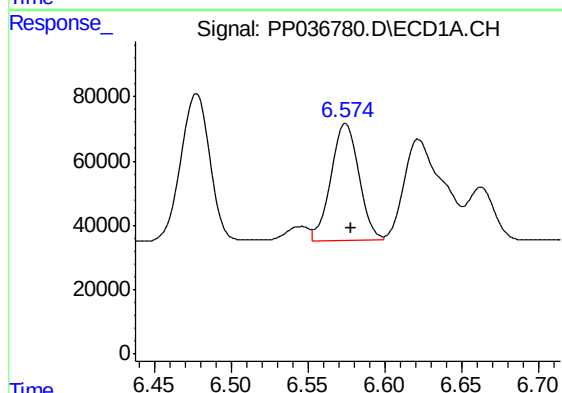


#22 AR-1248-2

R.T.: 6.575 min
Delta R.T.: -0.004 min
Response: 462446
Conc: 340.52 ng/ml

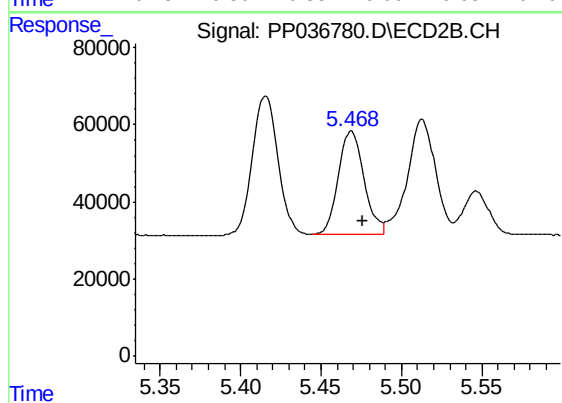

#22 AR-1248-2


R.T.: 5.469 min
Delta R.T.: -0.008 min
Response: 297789
Conc: 314.40 ng/ml

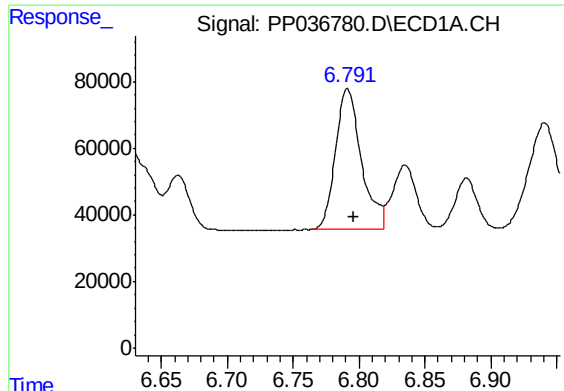

#23 AR-1248-3


R.T.: 6.791 min
Delta R.T.: -0.005 min
Response: 577018
Conc: 354.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

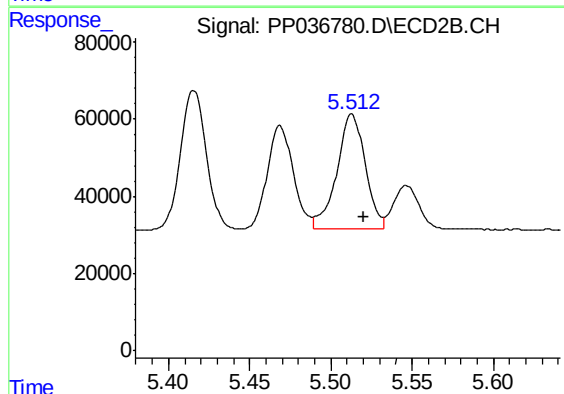


#23 AR-1248-3

R.T.: 5.513 min
Delta R.T.: -0.008 min
Response: 366651
Conc: 370.56 ng/ml

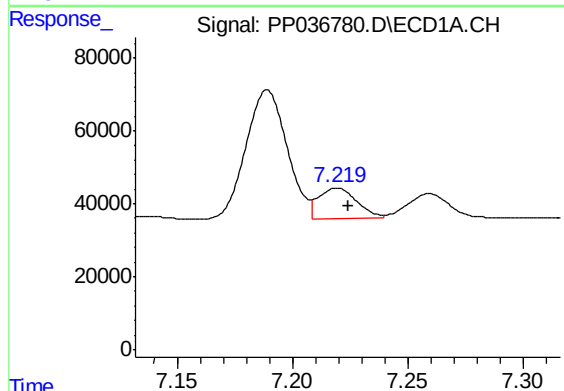


#24 AR-1248-4

R.T.: 7.219 min
Delta R.T.: -0.005 min
Response: 96830
Conc: 53.04 ng/ml

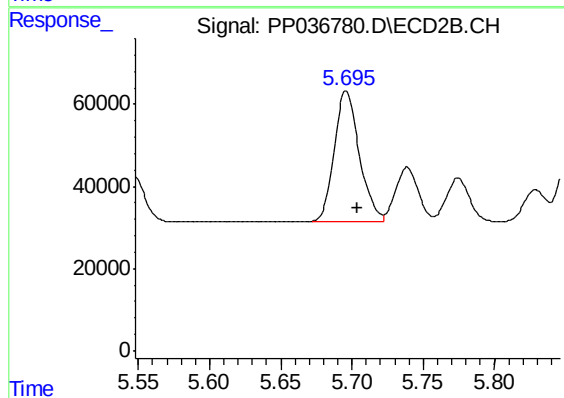

#24 AR-1248-4


R.T.: 5.696 min
Delta R.T.: -0.008 min
Response: 387367
Conc: 331.16 ng/ml

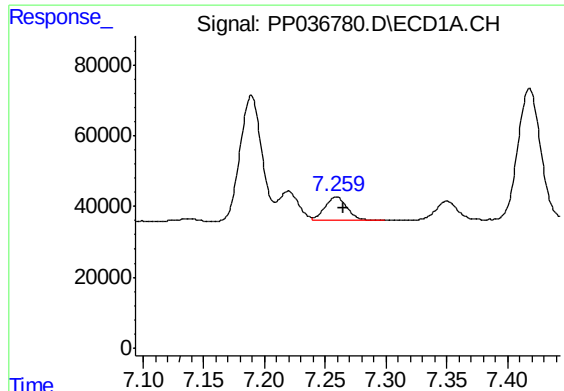

#25 AR-1248-5


R.T.: 7.259 min
Delta R.T.: -0.005 min
Response: 85212
Conc: 47.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

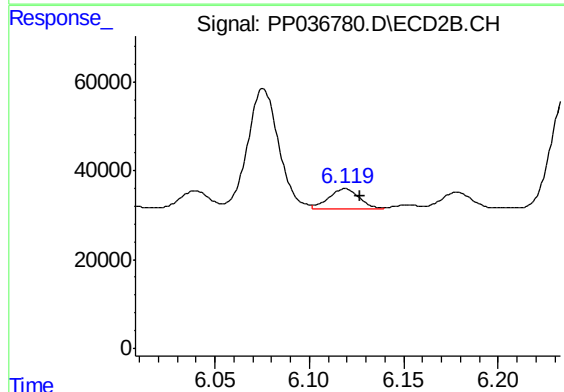


#25 AR-1248-5

R.T.: 6.119 min
Delta R.T.: -0.008 min
Response: 49090
Conc: 41.39 ng/ml

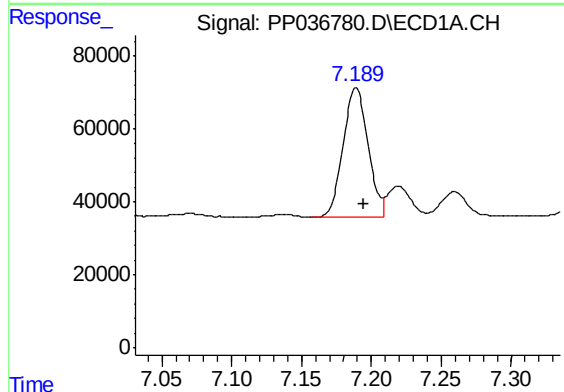


#26 AR-1254-1

R.T.: 7.189 min
Delta R.T.: -0.005 min
Response: 440235
Conc: 250.32 ng/ml

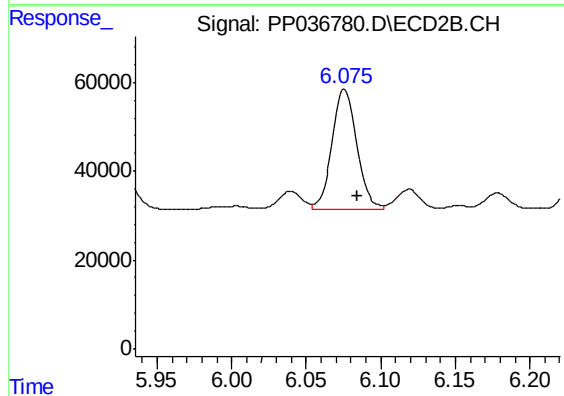

#26 AR-1254-1


R.T.: 6.076 min
Delta R.T.: -0.009 min
Response: 308074
Conc: 181.82 ng/ml



#27 AR-1254-2


R.T.: 7.418 min
Delta R.T.: -0.006 min
Response: 477987
Conc: 176.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

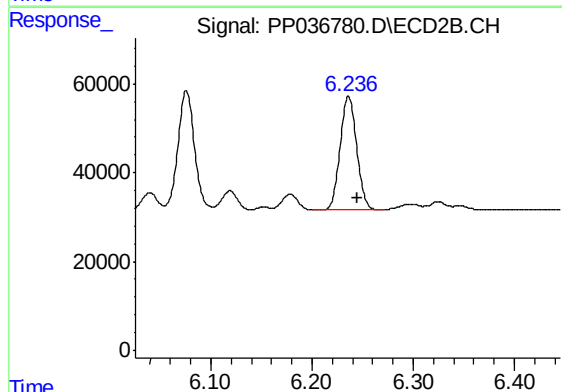


#27 AR-1254-2

R.T.: 6.236 min
Delta R.T.: -0.009 min
Response: 290640
Conc: 195.40 ng/ml




#28 AR-1254-3

R.T.: 7.801 min
Delta R.T.: -0.005 min
Response: 281216
Conc: 94.94 ng/ml

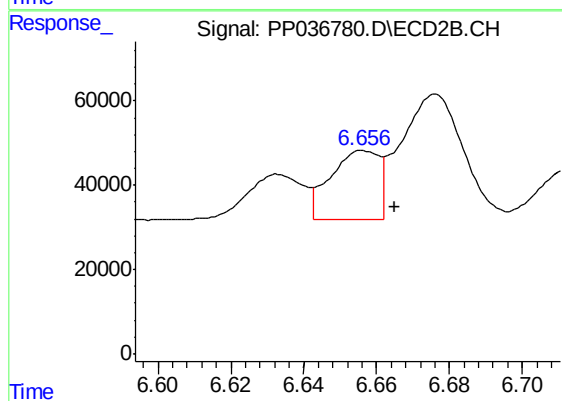

#28 AR-1254-3


R.T.: 6.656 min
Delta R.T.: -0.009 min
Response: 153681
Conc: 63.21 ng/ml

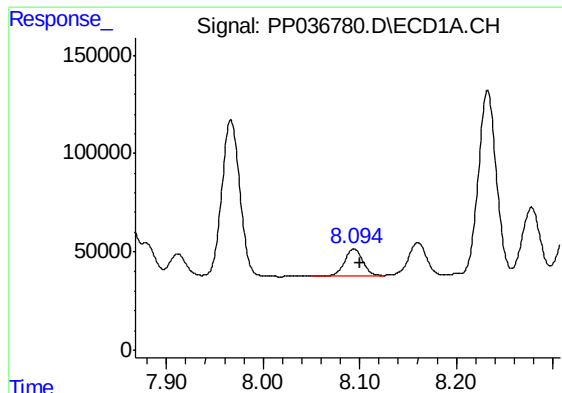

#29 AR-1254-4


R.T.: 8.094 min
Delta R.T.: -0.007 min
Response: 176579
Conc: 80.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

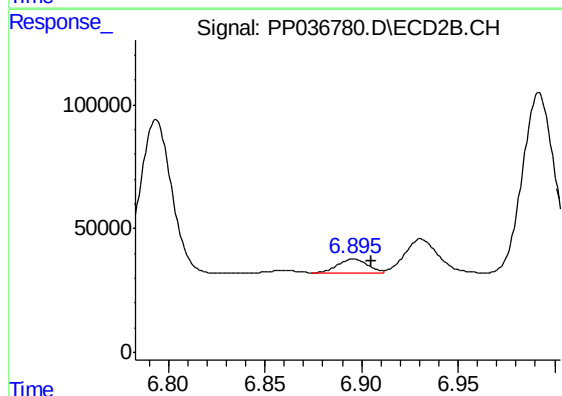


#29 AR-1254-4

R.T.: 6.896 min
Delta R.T.: -0.009 min
Response: 62573
Conc: 40.44 ng/ml

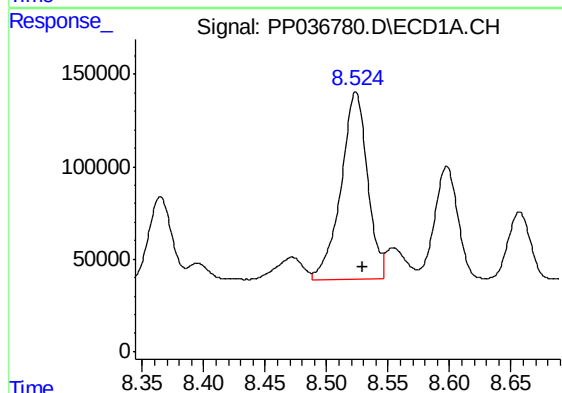


#30 AR-1254-5

R.T.: 8.524 min
Delta R.T.: -0.006 min
Response: 1521499
Conc: 639.79 ng/ml

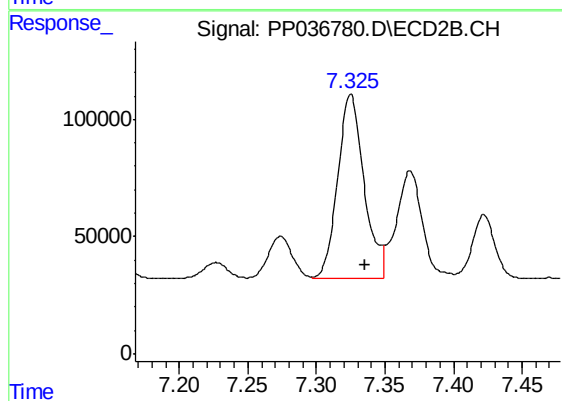

#30 AR-1254-5


R.T.: 7.325 min
Delta R.T.: -0.010 min
Response: 1047391
Conc: 487.09 ng/ml

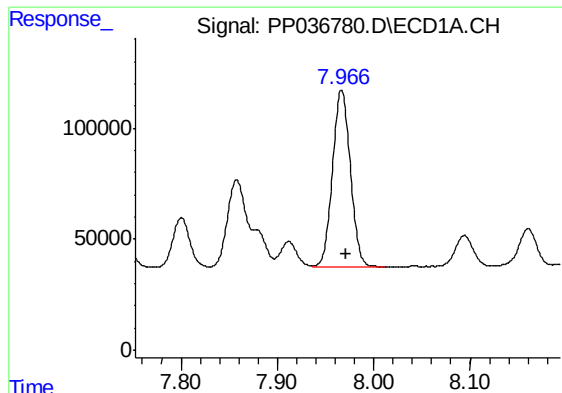

#31 AR-1260-1


R.T.: 7.967 min
Delta R.T.: -0.005 min
Response: 1030812
Conc: 474.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

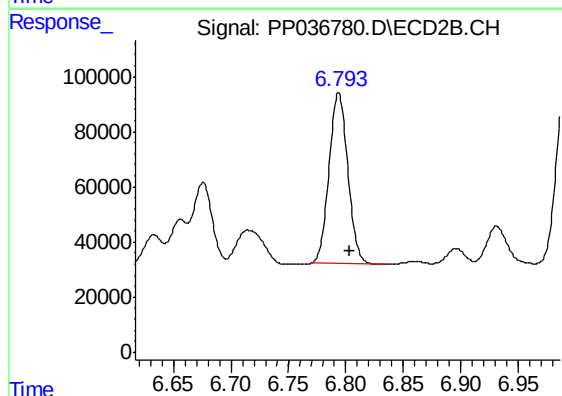


#31 AR-1260-1

R.T.: 6.794 min
Delta R.T.: -0.009 min
Response: 699695
Conc: 434.58 ng/ml

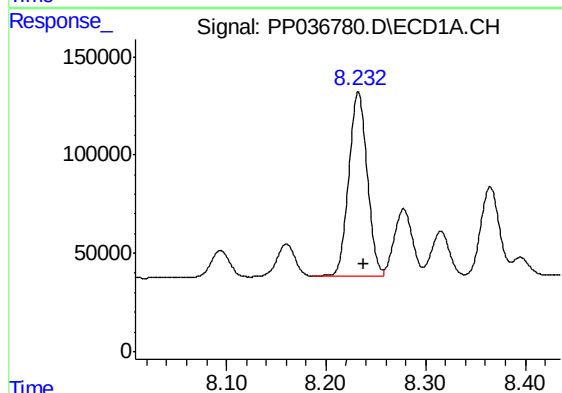


#32 AR-1260-2

R.T.: 8.232 min
Delta R.T.: -0.005 min
Response: 1206800
Conc: 470.86 ng/ml

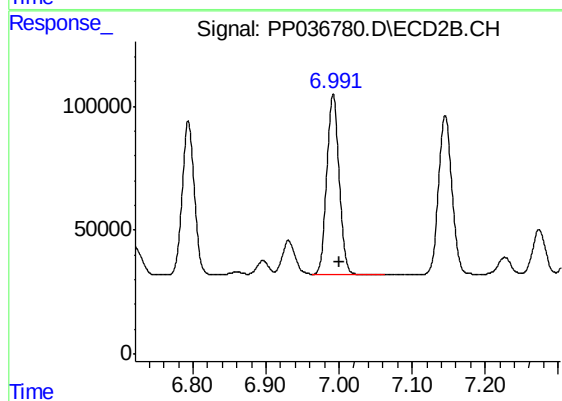

#32 AR-1260-2


R.T.: 6.992 min
Delta R.T.: -0.009 min
Response: 859721
Conc: 443.32 ng/ml



#33 AR-1260-3


R.T.: 8.598 min
Delta R.T.: -0.005 min
Response: 805982
Conc: 402.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

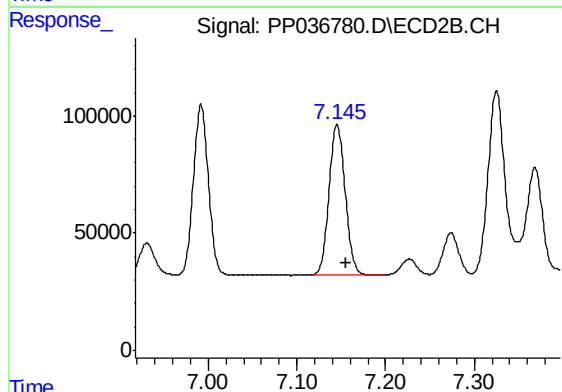


#33 AR-1260-3

R.T.: 7.145 min
Delta R.T.: -0.010 min
Response: 811218
Conc: 446.04 ng/ml

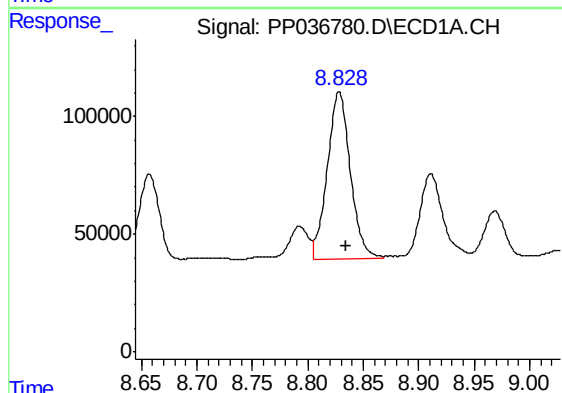


#34 AR-1260-4

R.T.: 8.828 min
Delta R.T.: -0.006 min
Response: 1029749
Conc: 434.63 ng/ml

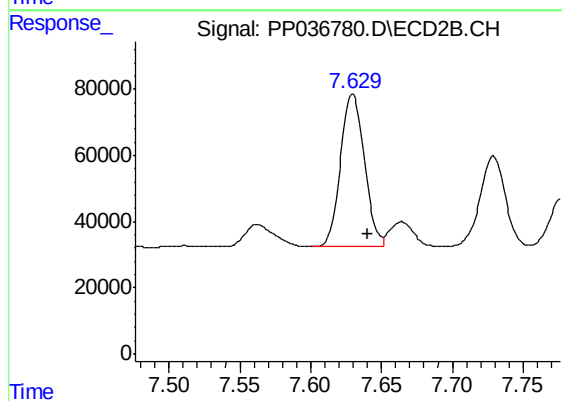

#34 AR-1260-4


R.T.: 7.630 min
Delta R.T.: -0.010 min
Response: 543164
Conc: 350.26 ng/ml

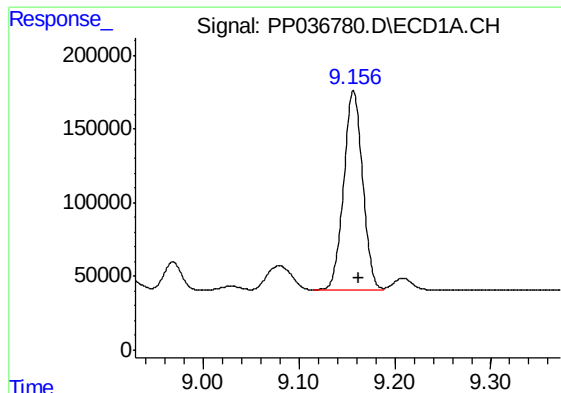

#35 AR-1260-5


R.T.: 9.157 min
Delta R.T.: -0.006 min
Response: 1868397
Conc: 418.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

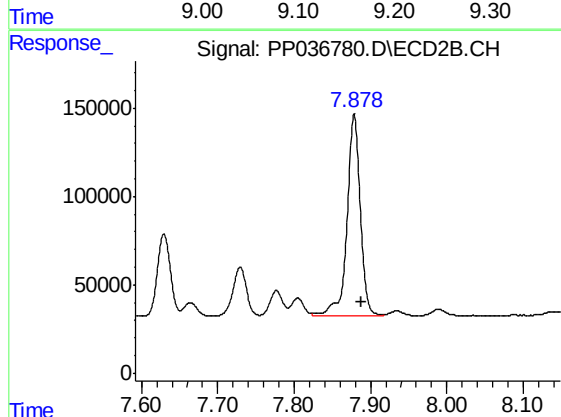


#35 AR-1260-5

R.T.: 7.879 min
Delta R.T.: -0.009 min
Response: 1421801
Conc: 386.91 ng/ml

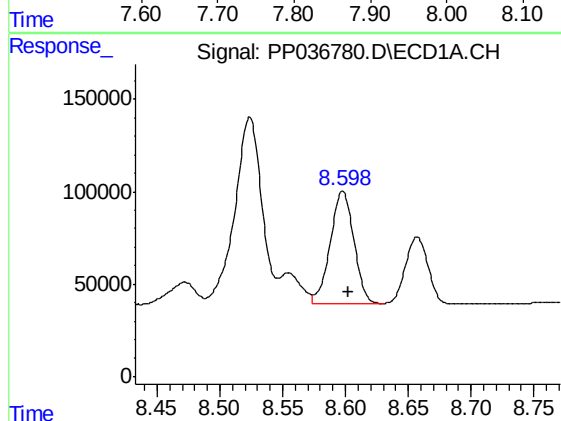


#36 AR-1262-1

R.T.: 8.598 min
Delta R.T.: -0.005 min
Response: 805982
Conc: 282.86 ng/ml

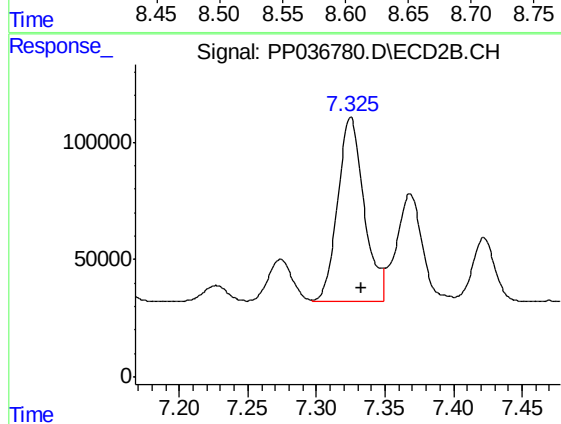

#36 AR-1262-1


R.T.: 7.325 min
Delta R.T.: -0.008 min
Response: 1047391
Conc: 878.77 ng/ml



#37 AR-1262-2


R.T.: 9.157 min
Delta R.T.: -0.005 min
Response: 1868397
Conc: 367.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

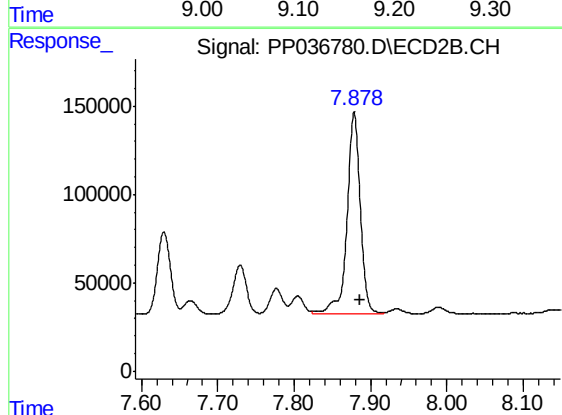


#37 AR-1262-2

R.T.: 7.879 min
Delta R.T.: -0.008 min
Response: 1421801
Conc: 362.70 ng/ml

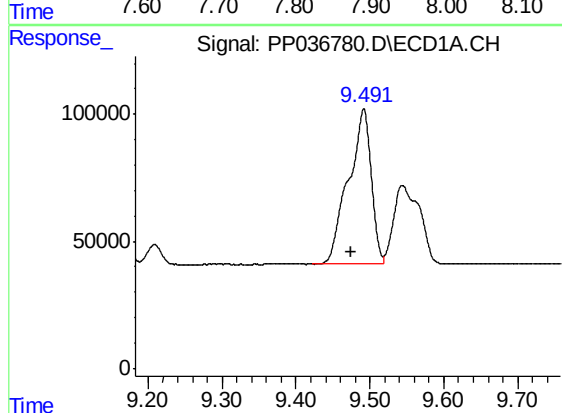


#38 AR-1262-3

R.T.: 9.492 min
Delta R.T.: 0.017 min
Response: 1311975
Conc: 354.15 ng/ml

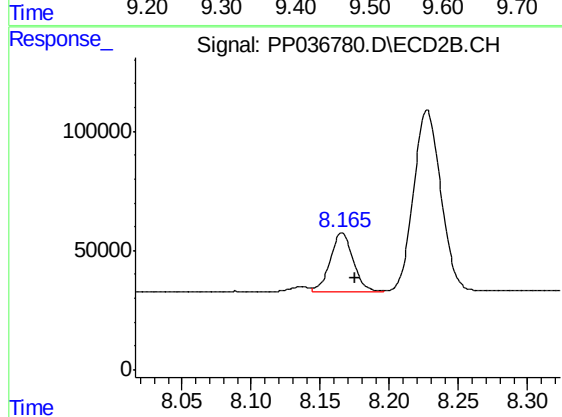

#38 AR-1262-3


R.T.: 8.166 min
Delta R.T.: -0.009 min
Response: 280408
Conc: 176.20 ng/ml

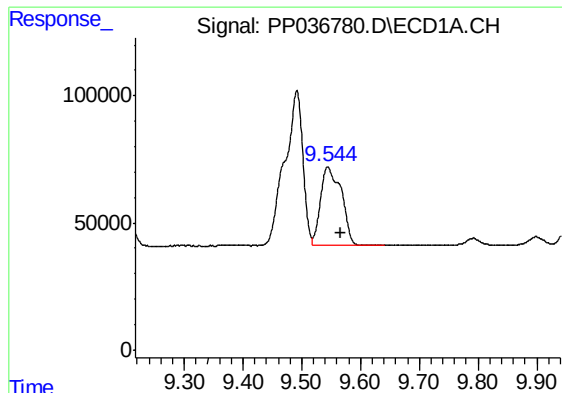

#39 AR-1262-4


R.T.: 9.544 min
Delta R.T.: -0.022 min
Response: 759722
Conc: 264.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

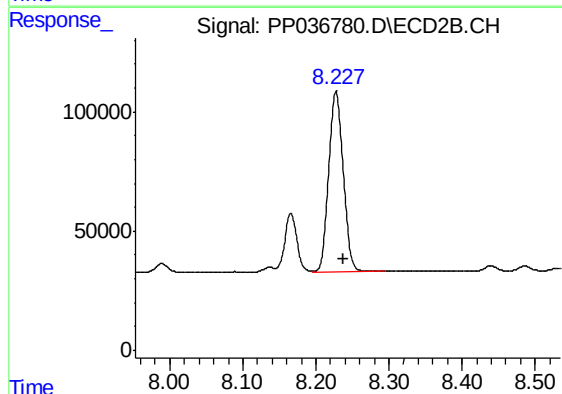


#39 AR-1262-4

R.T.: 8.227 min
Delta R.T.: -0.011 min
Response: 1043860
Conc: 350.72 ng/ml

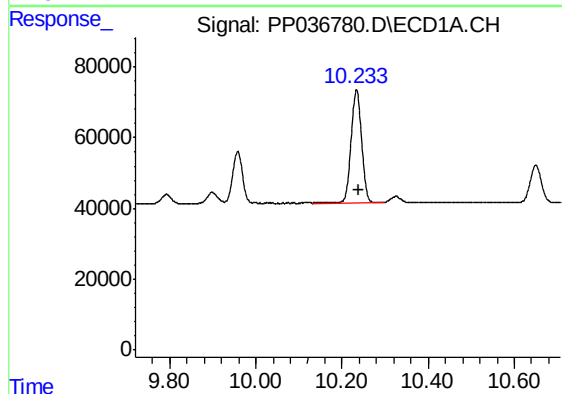


#40 AR-1262-5

R.T.: 10.234 min
Delta R.T.: -0.006 min
Response: 549871
Conc: 260.26 ng/ml

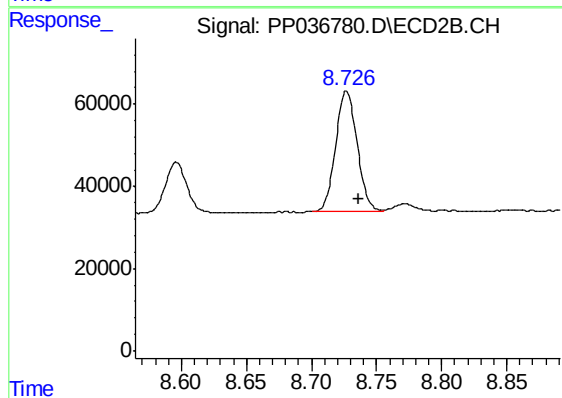

#40 AR-1262-5


R.T.: 8.727 min
Delta R.T.: -0.010 min
Response: 336127
Conc: 235.87 ng/ml



#41 AR-1268-1


R.T.: 9.492 min
Delta R.T.: 0.018 min
Response: 1311975
Conc: 218.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

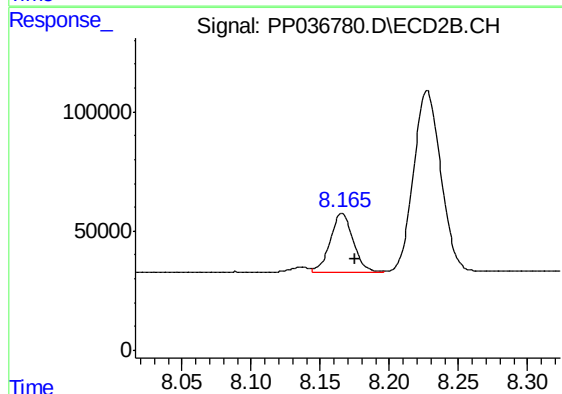


#41 AR-1268-1

R.T.: 8.166 min
Delta R.T.: -0.009 min
Response: 280408
Conc: 60.22 ng/ml




#42 AR-1268-2

R.T.: 9.544 min
Delta R.T.: -0.027 min
Response: 759722
Conc: 133.28 ng/ml

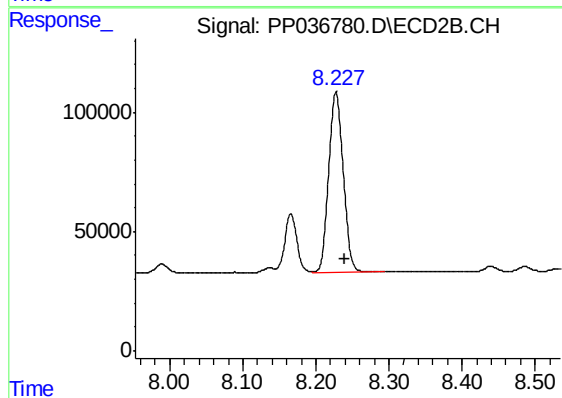

#42 AR-1268-2


R.T.: 8.227 min
Delta R.T.: -0.012 min
Response: 1043860
Conc: 241.99 ng/ml

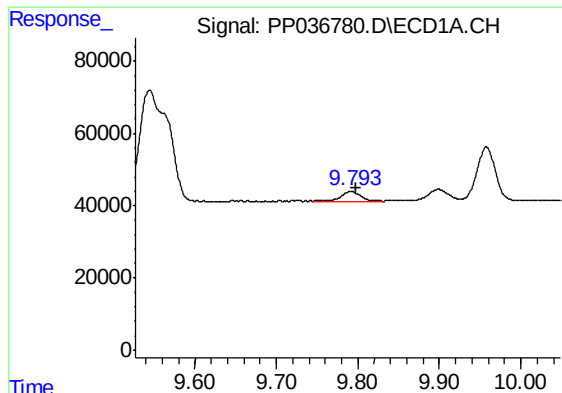

#43 AR-1268-3


R.T.: 9.792 min
Delta R.T.: -0.006 min
Response: 43954
Conc: 9.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

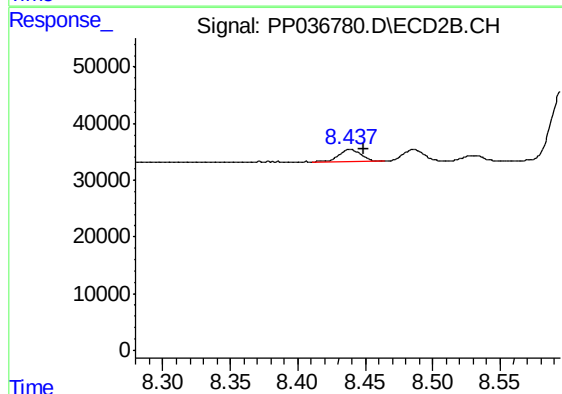


#43 AR-1268-3

R.T.: 8.439 min
Delta R.T.: -0.010 min
Response: 24861
Conc: 6.81 ng/ml

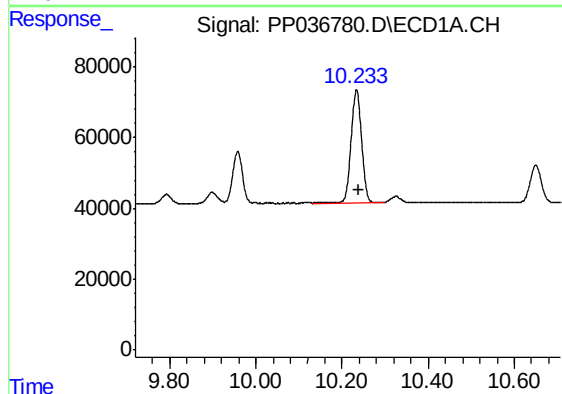


#44 AR-1268-4

R.T.: 10.234 min
Delta R.T.: -0.006 min
Response: 549871
Conc: 233.44 ng/ml

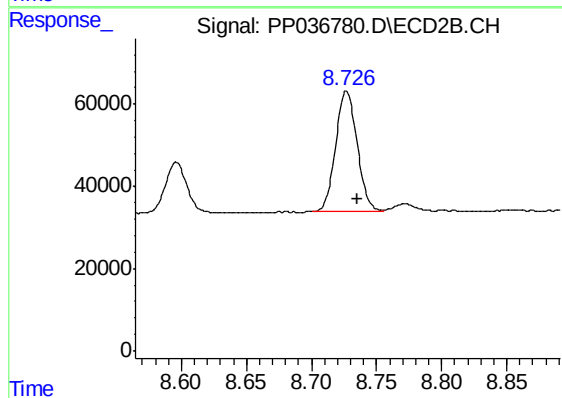

#44 AR-1268-4


R.T.: 8.727 min
Delta R.T.: -0.009 min
Response: 336127
Conc: 211.30 ng/ml

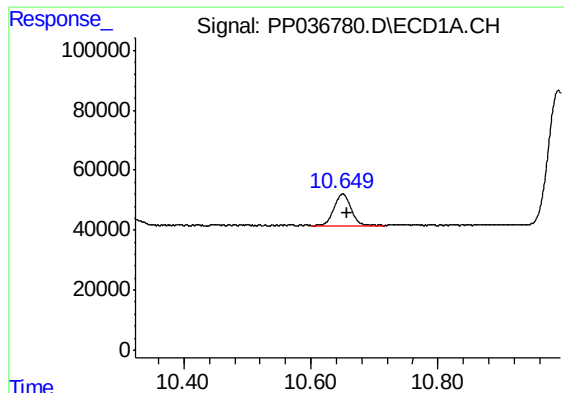

#45 AR-1268-5

R.T.: 10.650 min
Delta R.T.: -0.008 min
Response: 193370
Conc: 12.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-D8-C9-D8A-C9AMS

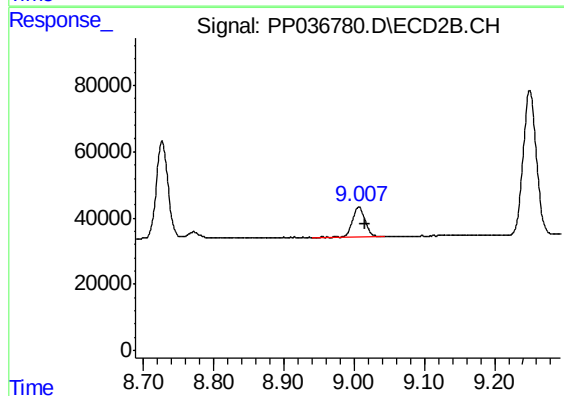

#45 AR-1268-5

R.T.: 9.007 min
Delta R.T.: -0.010 min
Response: 110890
Conc: 9.38 ng/ml