

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
 Data File : PP036782.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2021 18:21
 Operator : DD\AJ
 Sample : M2834-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-01-B8-C8-B8A-C8A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:54:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.961	3.953	865538	583804	19.583	18.849
2)	SA Decachlor...	10.990	9.250	898562	556279	20.947	17.394
Target Compounds							
8)	L2 AR-1221-1	5.211	0.000	32725	0	58.291	N.D. #
9)	L2 AR-1221-2	5.313	0.000	13092	0	30.381	N.D. #
24)	L5 AR-1248-4	7.195f	0.000	8899	0	4.874	N.D. #
26)	L6 AR-1254-1	7.195	0.000	8899	0	5.060	N.D. #
28)	L6 AR-1254-3	7.820	0.000	8549	0	2.886	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
Data File : PP036782.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2021 18:21
Operator : DD\AJ
Sample : M2834-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 02:54:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

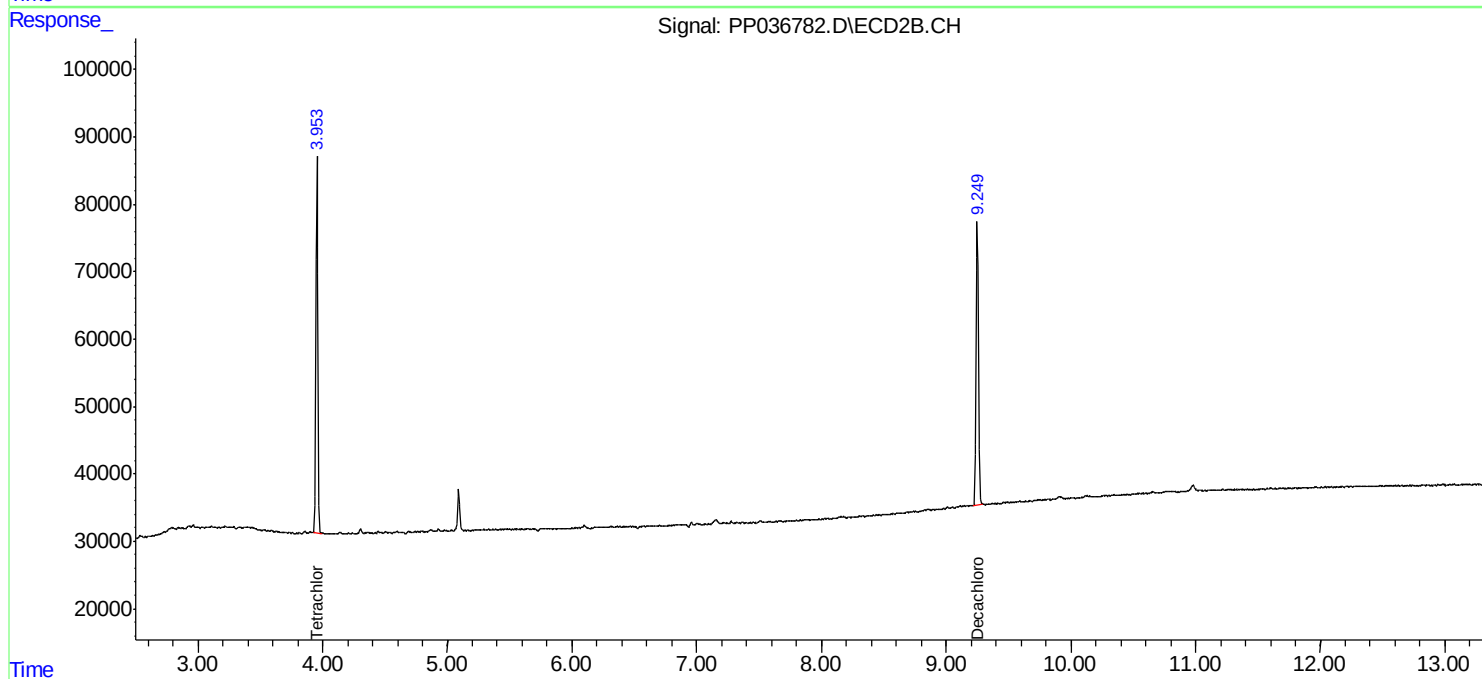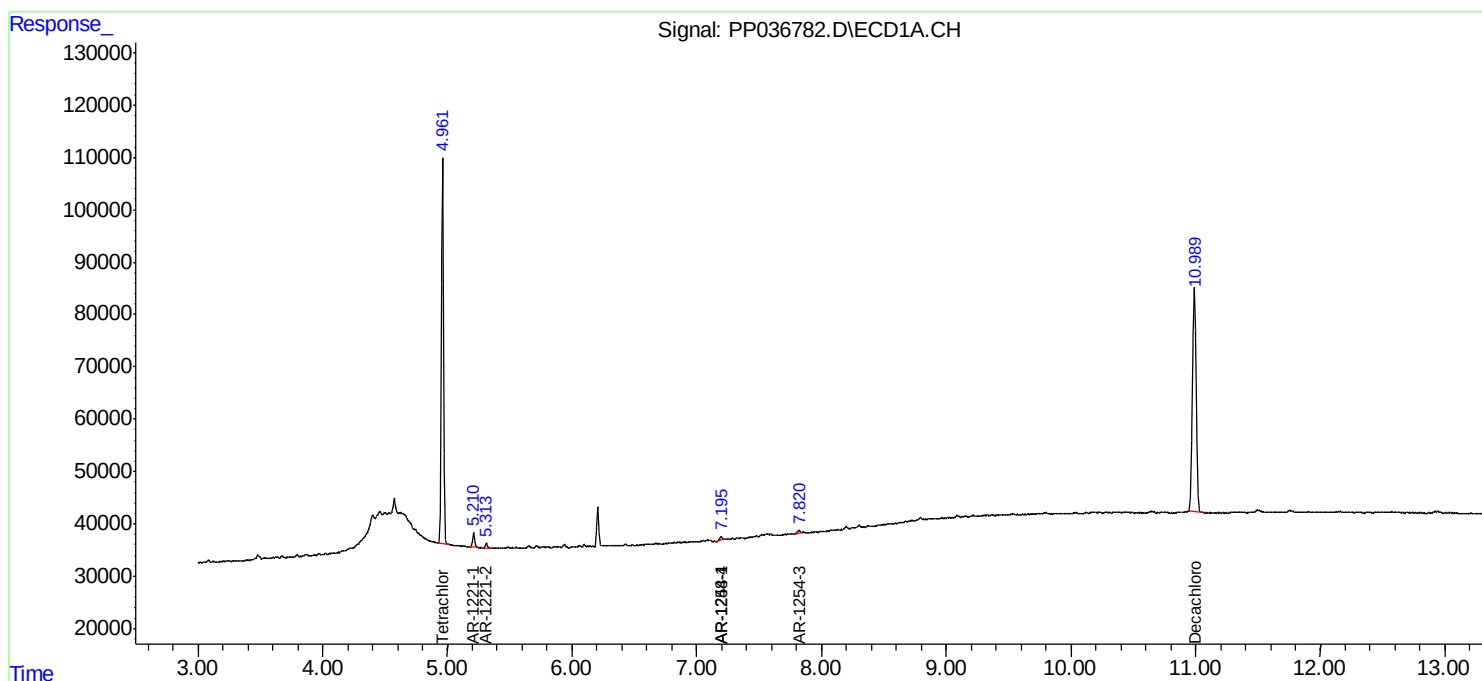


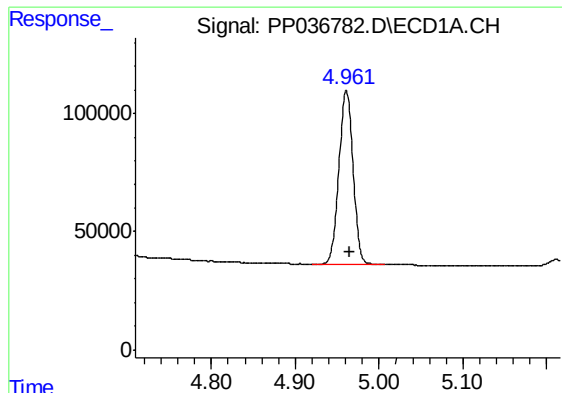

#1 Tetrachloro-m-xylene


R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 865538
Conc: 19.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A

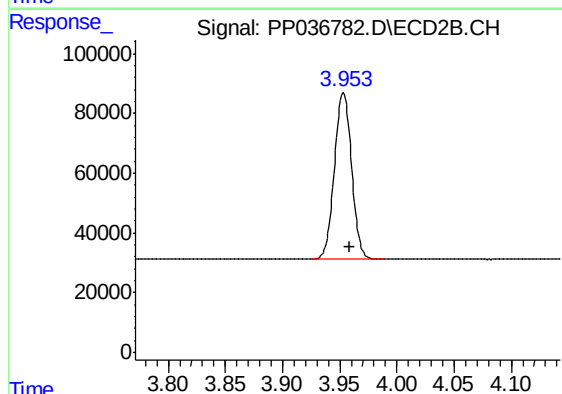


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.006 min
Response: 583804
Conc: 18.85 ng/ml

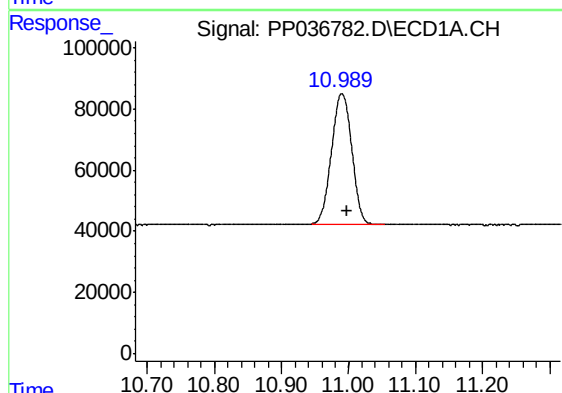


#2 Decachlorobiphenyl

R.T.: 10.990 min
Delta R.T.: -0.008 min
Response: 898562
Conc: 20.95 ng/ml

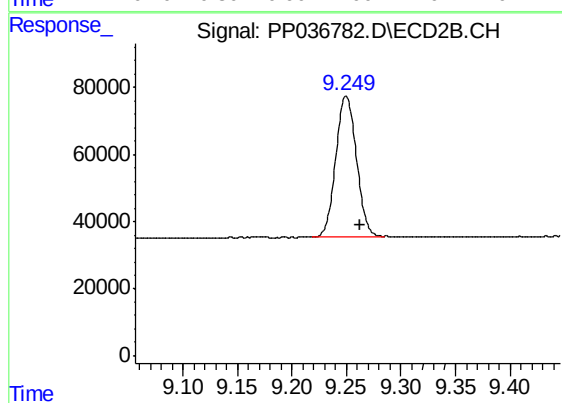

#2 Decachlorobiphenyl


R.T.: 9.250 min
Delta R.T.: -0.013 min
Response: 556279
Conc: 17.39 ng/ml

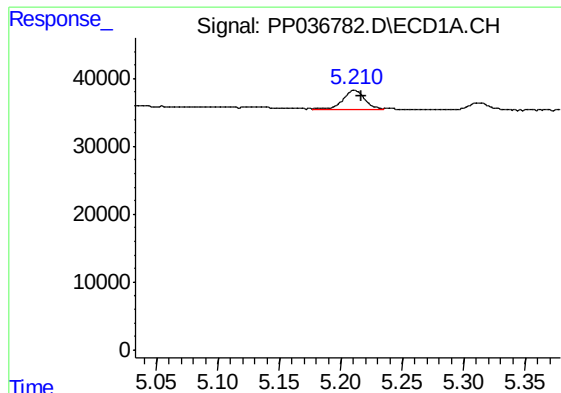

#8 AR-1221-1


R.T.: 5.211 min
Delta R.T.: -0.006 min
Response: 32725
Conc: 58.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A

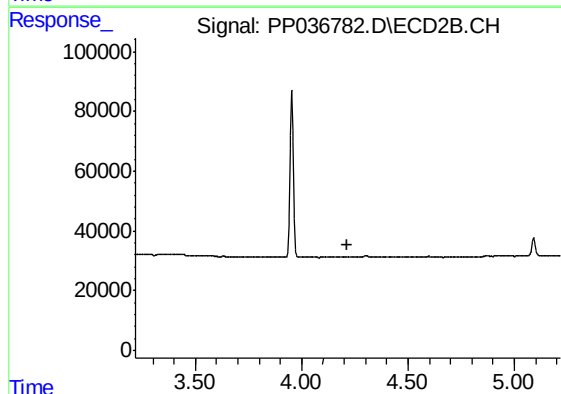


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

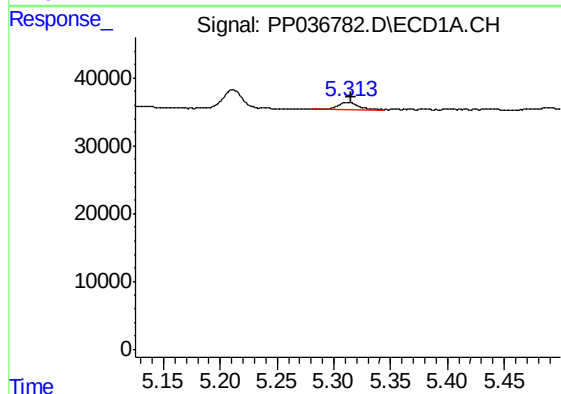


#9 AR-1221-2

R.T.: 5.313 min
Delta R.T.: -0.002 min
Response: 13092
Conc: 30.38 ng/ml

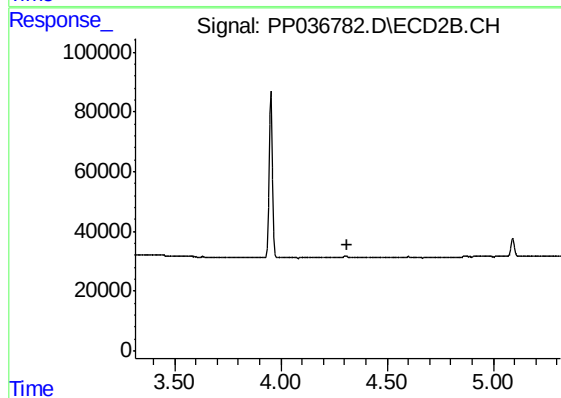

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

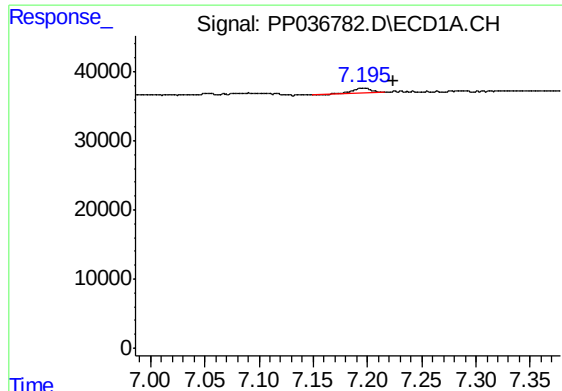

#24 AR-1248-4


R.T.: 7.195 min
Delta R.T.: -0.029 min
Response: 8899
Conc: 4.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A

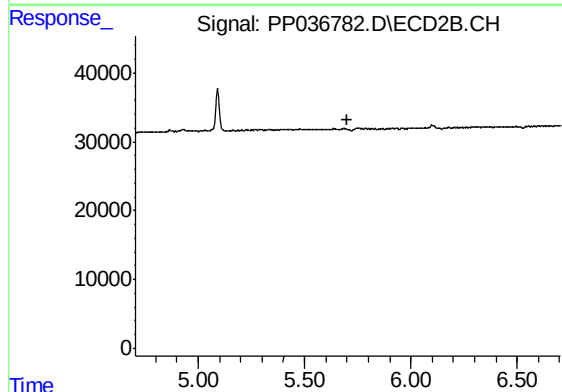


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

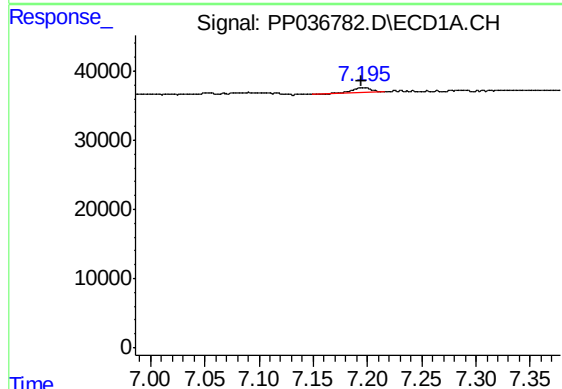


#26 AR-1254-1

R.T.: 7.195 min
Delta R.T.: 0.000 min
Response: 8899
Conc: 5.06 ng/ml

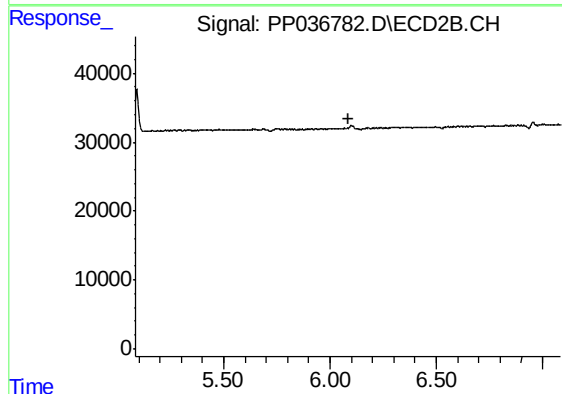

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

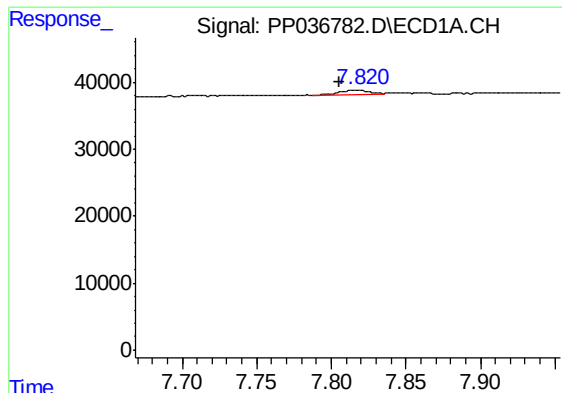

#28 AR-1254-3

R.T.: 7.820 min
Delta R.T.: 0.015 min
Response: 8549
Conc: 2.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B8-C8-B8A-C8A

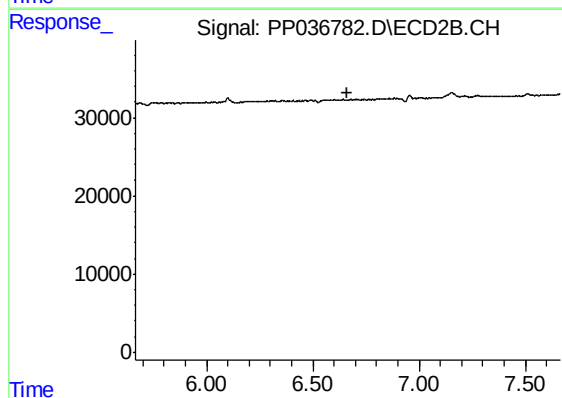

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.