

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
 Data File : PP036769.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2021 11:30
 Operator : DD\AJ
 Sample : M2809-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 H345-O1

Manual Integrations
 APPROVED

Ankita
 6/25/2021 1:27:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:47:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.961	3.954	728004	498555	16.471	16.096
2) SA Decachlor...	10.988	9.249	792506	508751	18.474	15.908
Target Compounds						
31) L7 AR-1260-1	7.966	6.793	273715	177320	126.107	110.134
32) L7 AR-1260-2	8.232	6.991	373066	247252	145.561	127.498
33) L7 AR-1260-3	8.596	7.145	273889	209730	136.638m	115.319
34) L7 AR-1260-4	8.827	7.629	316682	191349	133.664m	123.391
35) L7 AR-1260-5	9.156	7.877	640367	463933	143.518	126.249

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
Data File : PP036769.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2021 11:30
Operator : DD\AJ
Sample : M2809-11
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
H345-O1


Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 02:47:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

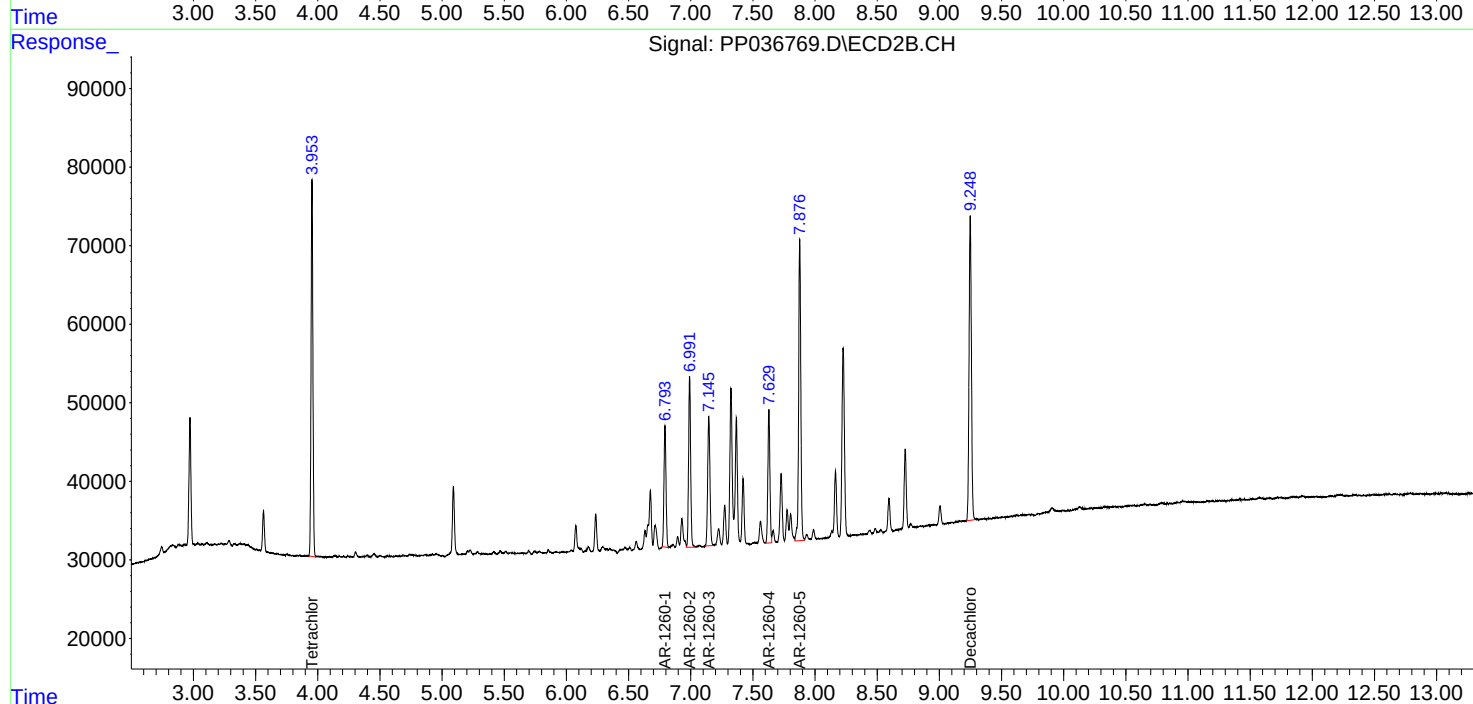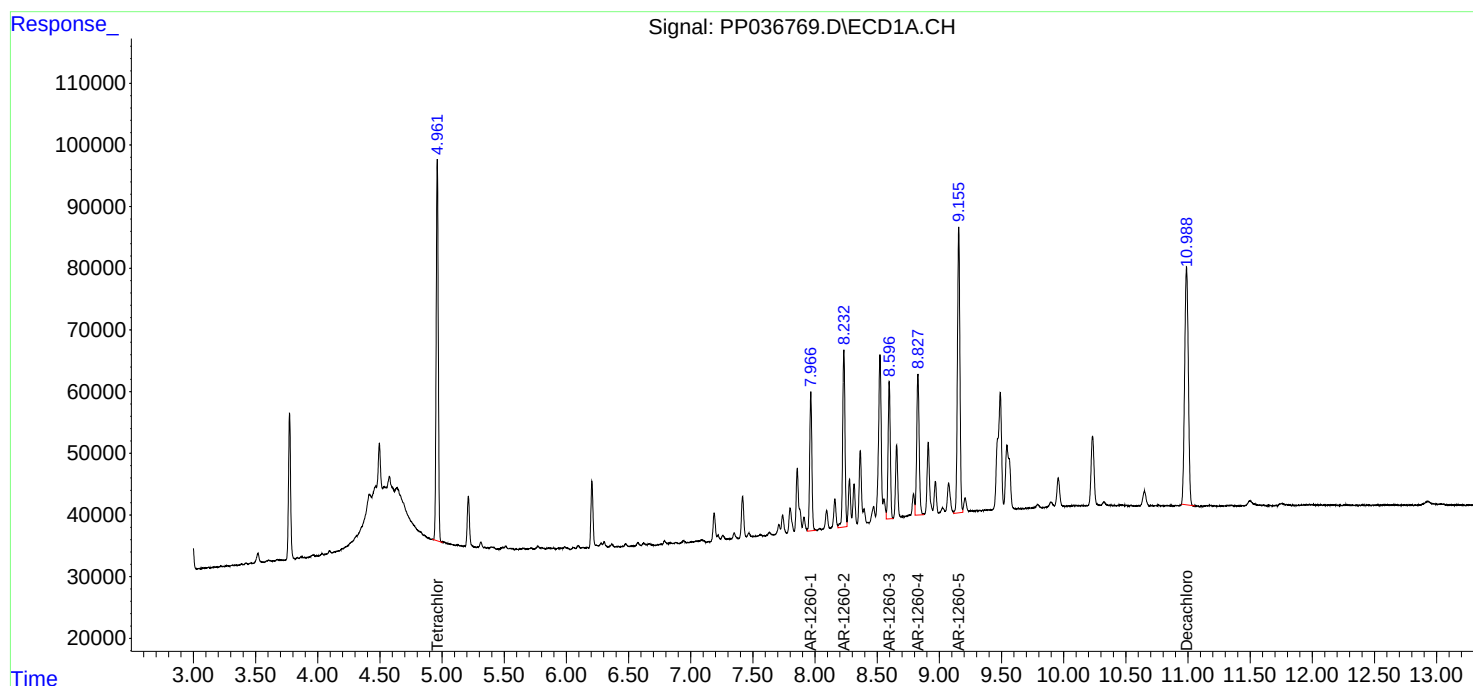

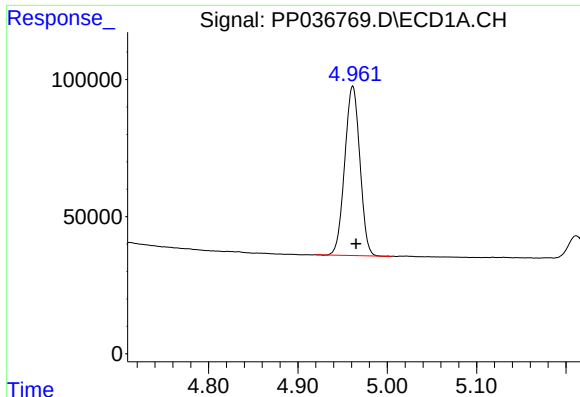


#1 Tetrachloro-m-xylene

R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 728004
Conc: 16.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
H345-O1


Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:52 PM

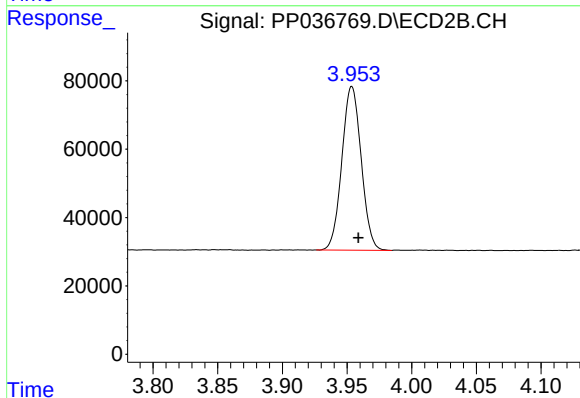


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 498555
Conc: 16.10 ng/ml

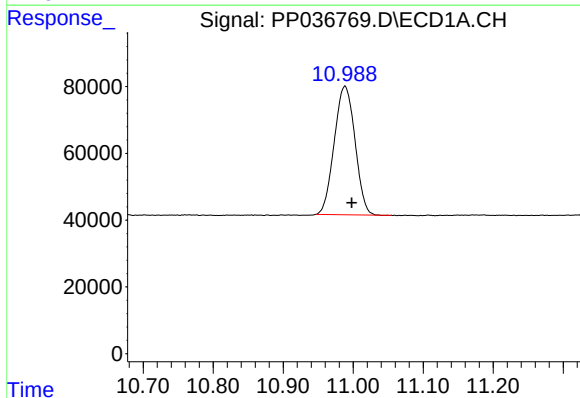


#2 Decachlorobiphenyl

R.T.: 10.988 min
Delta R.T.: -0.010 min
Response: 792506
Conc: 18.47 ng/ml

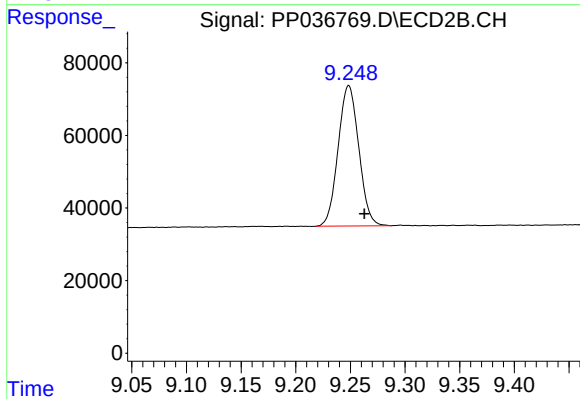

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.014 min
Response: 508751
Conc: 15.91 ng/ml

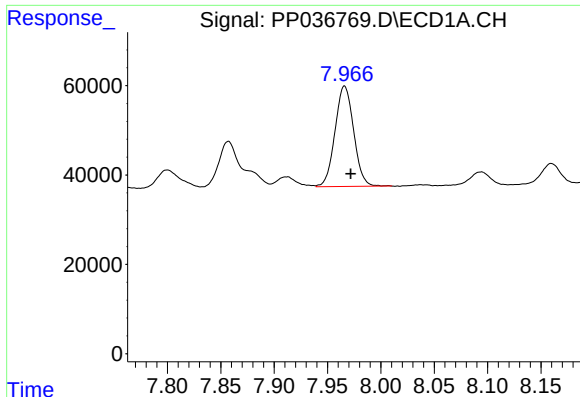


#31 AR-1260-1

R.T.: 7.966 min
Delta R.T.: -0.006 min
Response: 273715
Conc: 126.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
H345-O1

Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:52 PM

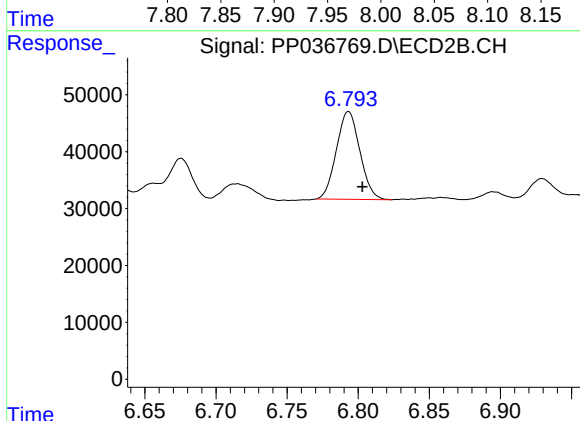

#31 AR-1260-1


R.T.: 6.793 min
Delta R.T.: -0.010 min
Response: 177320
Conc: 110.13 ng/ml

#32 AR-1260-2

R.T.: 8.232 min
Delta R.T.: -0.006 min
Response: 373066
Conc: 145.56 ng/ml

#32 AR-1260-2

R.T.: 6.991 min
Delta R.T.: -0.010 min
Response: 247252
Conc: 127.50 ng/ml

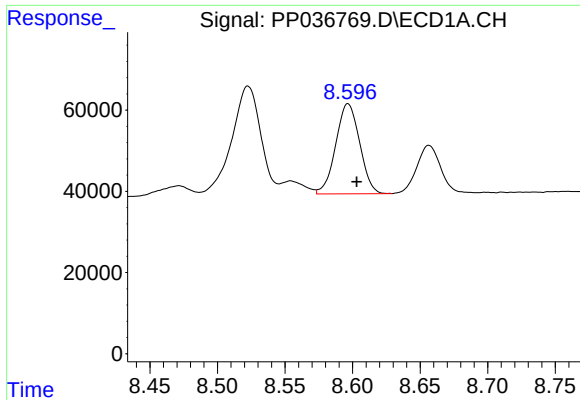


#33 AR-1260-3

R.T.: 8.596 min
Delta R.T.: -0.007 min
Response: 273889
Conc: 136.64 ng/ml m

Instrument :
ECD_P
ClientSampleId :
H345-O1


Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:52 PM

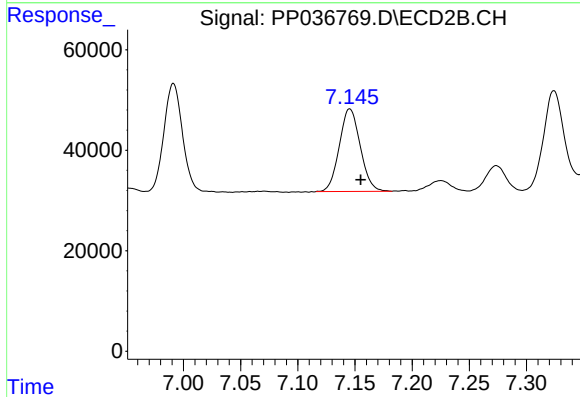


#33 AR-1260-3

R.T.: 7.145 min
Delta R.T.: -0.010 min
Response: 209730
Conc: 115.32 ng/ml

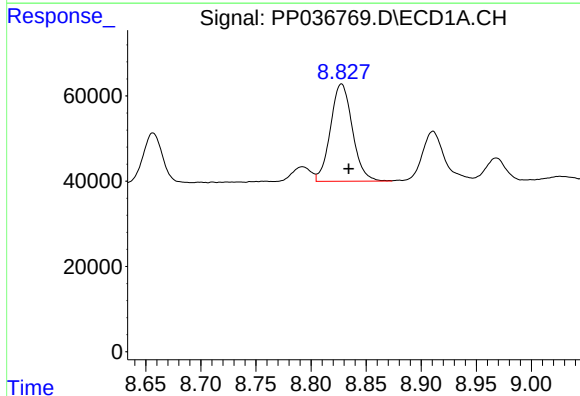


#34 AR-1260-4

R.T.: 8.827 min
Delta R.T.: -0.007 min
Response: 316682
Conc: 133.66 ng/ml m

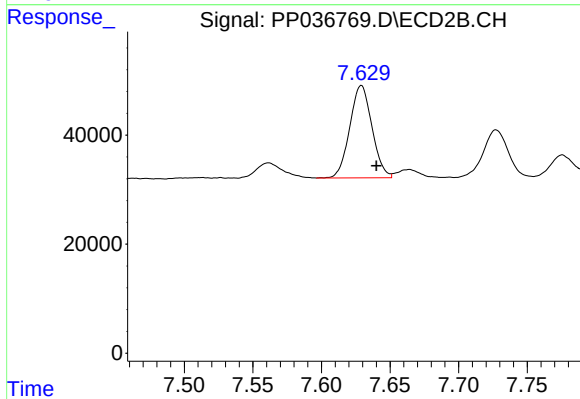

#34 AR-1260-4

R.T.: 7.629 min
Delta R.T.: -0.011 min
Response: 191349
Conc: 123.39 ng/ml

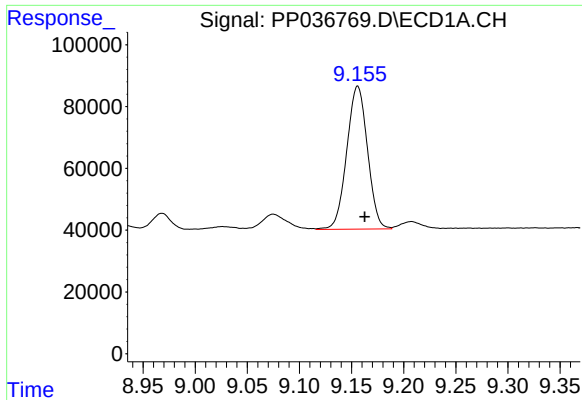


#35 AR-1260-5

R.T.: 9.156 min
Delta R.T.: -0.007 min
Response: 640367
Conc: 143.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
H345-O1

Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:52 PM

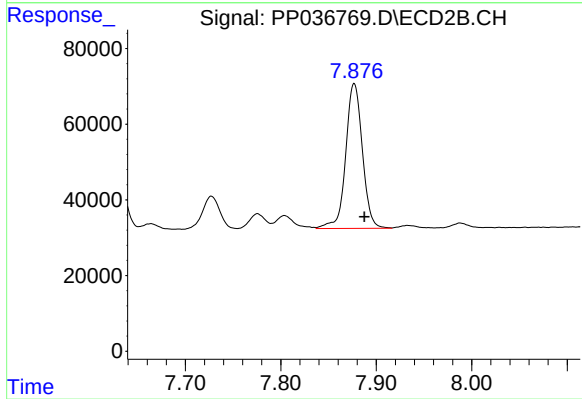

#35 AR-1260-5

R.T.: 7.877 min
Delta R.T.: -0.011 min
Response: 463933
Conc: 126.25 ng/ml