

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
 Data File : PP036776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2021 16:40
 Operator : DD\AJ
 Sample : M2819-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CL-02-062321

Manual Integrations
 APPROVED

Ankita
 6/25/2021 1:27:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:51:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.954	863387	574247	19.534	18.540
2) SA Decachlor...	10.987	9.249	902130	524891	21.030m	16.413

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062421\
Data File : PP036776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2021 16:40
Operator : DD\AJ
Sample : M2819-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CL-02-062321


Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 02:51:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

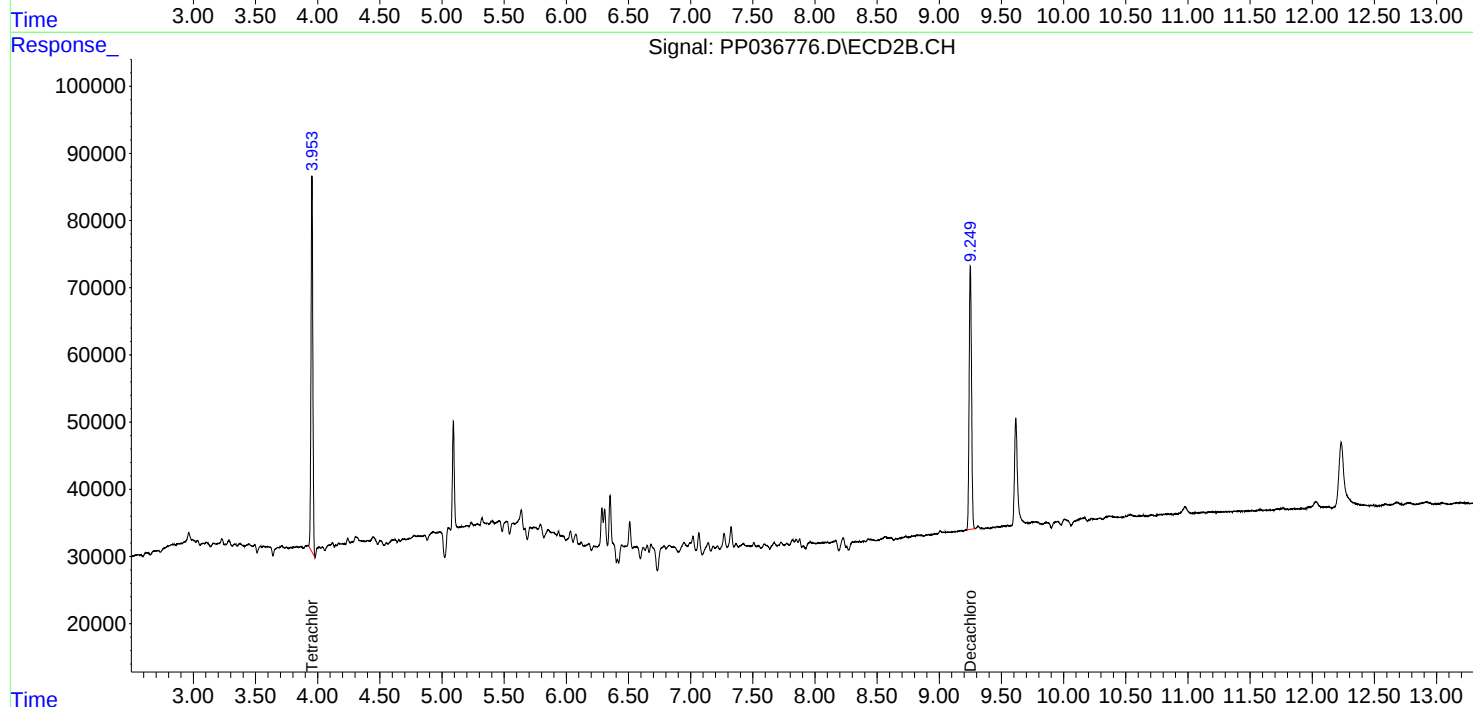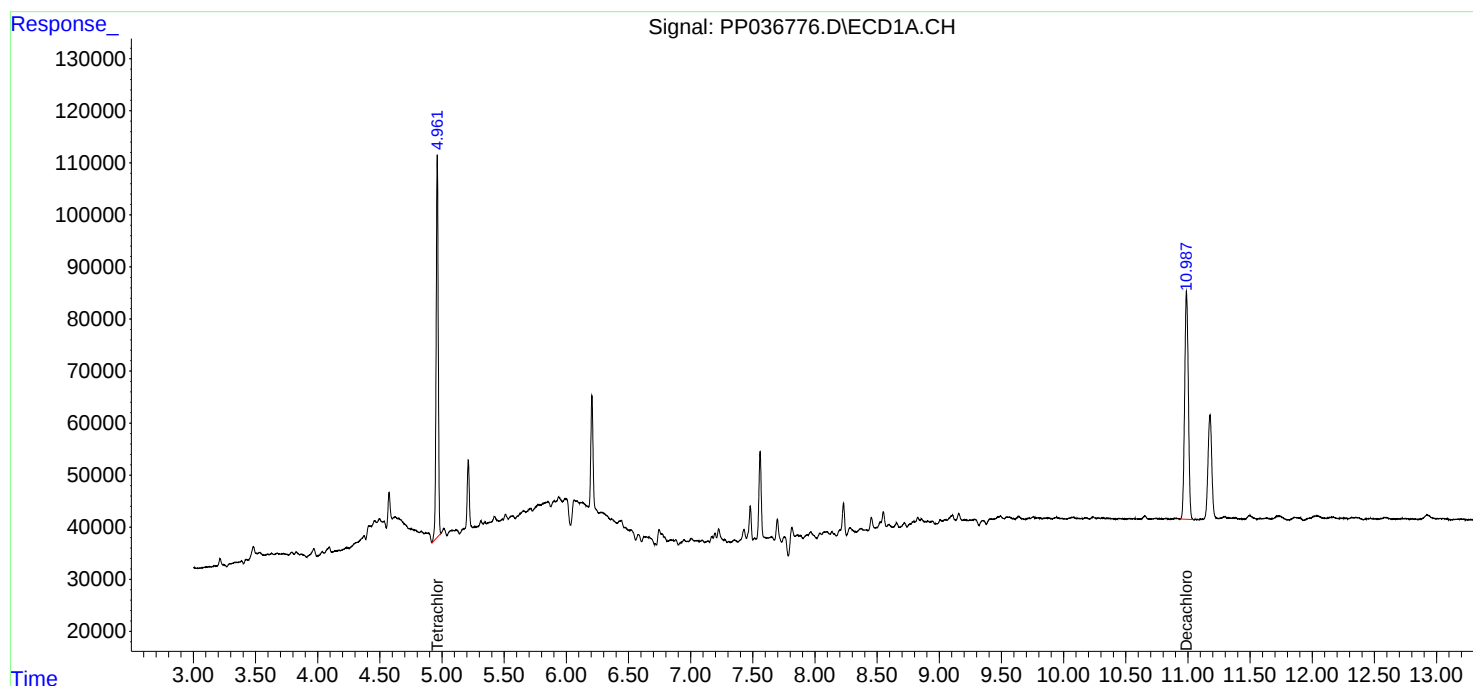

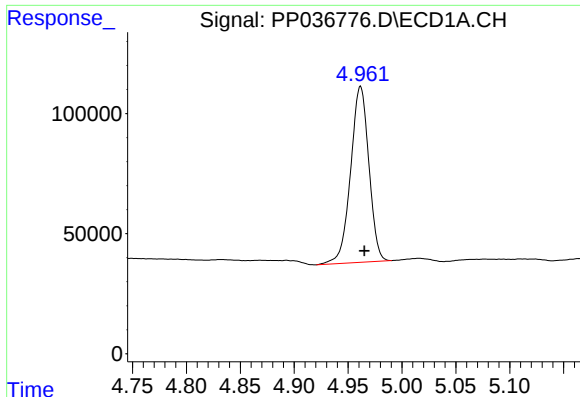


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 863387
Conc: 19.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-02-062321


Manual Integrations
APPROVED

Ankita
6/25/2021 1:27:55 PM

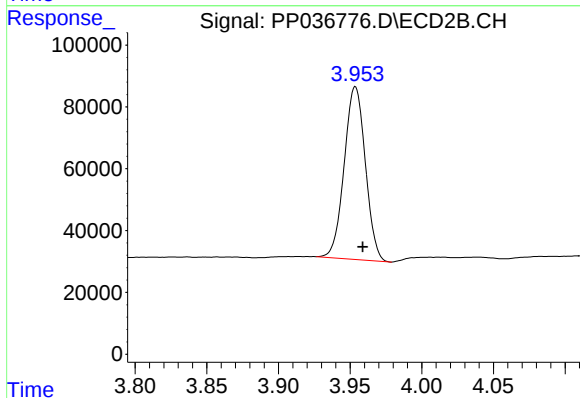


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 574247
Conc: 18.54 ng/ml

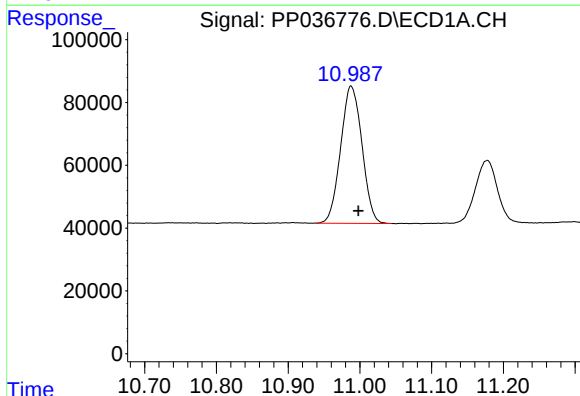

#2 Decachlorobiphenyl

R.T.: 10.987 min
Delta R.T.: -0.011 min
Response: 902130
Conc: 21.03 ng/ml m

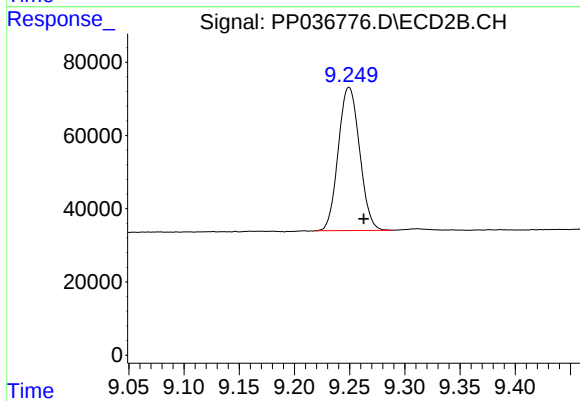

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.013 min
Response: 524891
Conc: 16.41 ng/ml