

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP062421\  
 Data File : PP036783.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 24 Jun 2021 18:38  
 Operator : DD\AJ  
 Sample : M2835-01  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 FK-PS-01-075

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 25 02:55:00 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP061721.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Jun 18 06:06:19 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|--------|--------|--------|--------|
| -----                       |        |       |        |        |        |        |
| System Monitoring Compounds |        |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.960  | 3.953 | 697518 | 469285 | 15.781 | 15.151 |
| 2) SA Decachlor...          | 10.990 | 9.250 | 492849 | 298234 | 11.489 | 9.325  |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP062421\  
Data File : PP036783.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 24 Jun 2021 18:38  
Operator : DD\AJ  
Sample : M2835-01  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
FK-PS-01-075

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 25 02:55:00 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP061721.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Jun 18 06:06:19 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

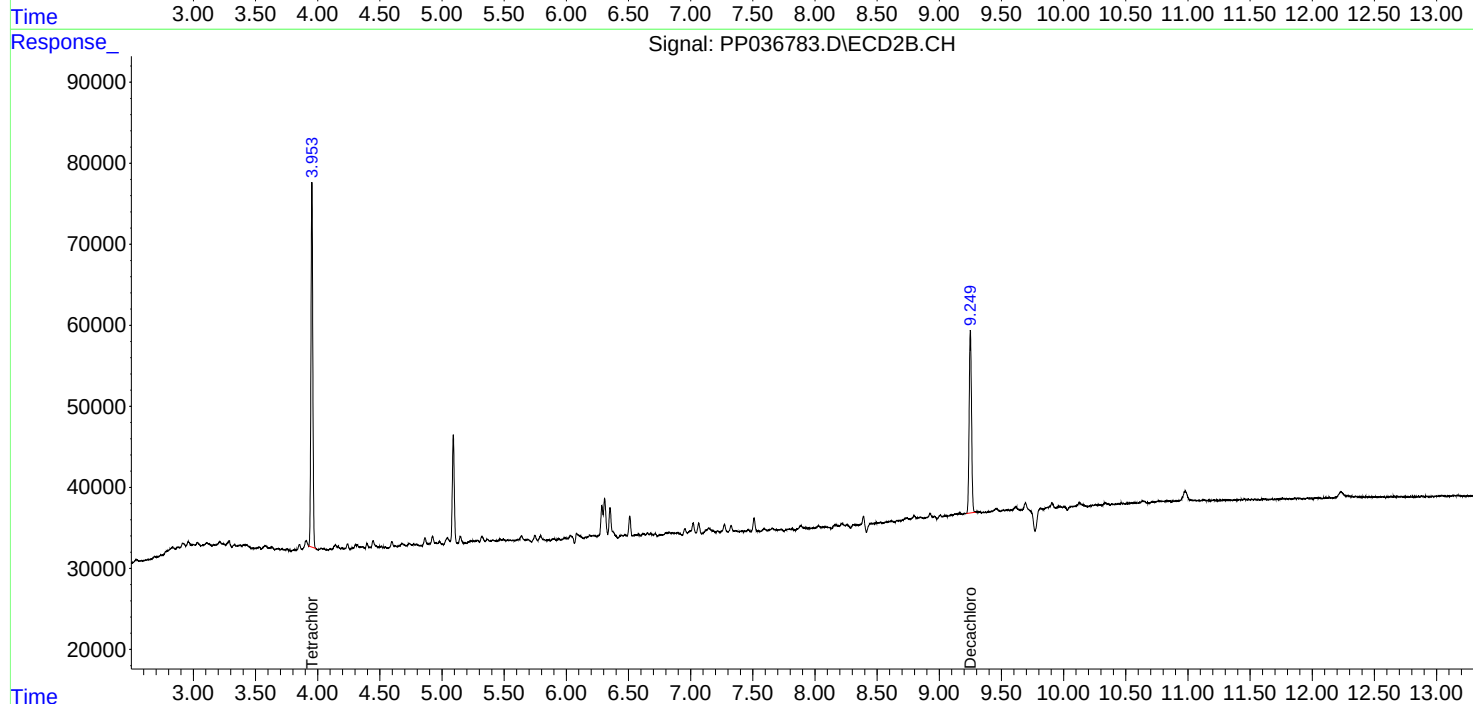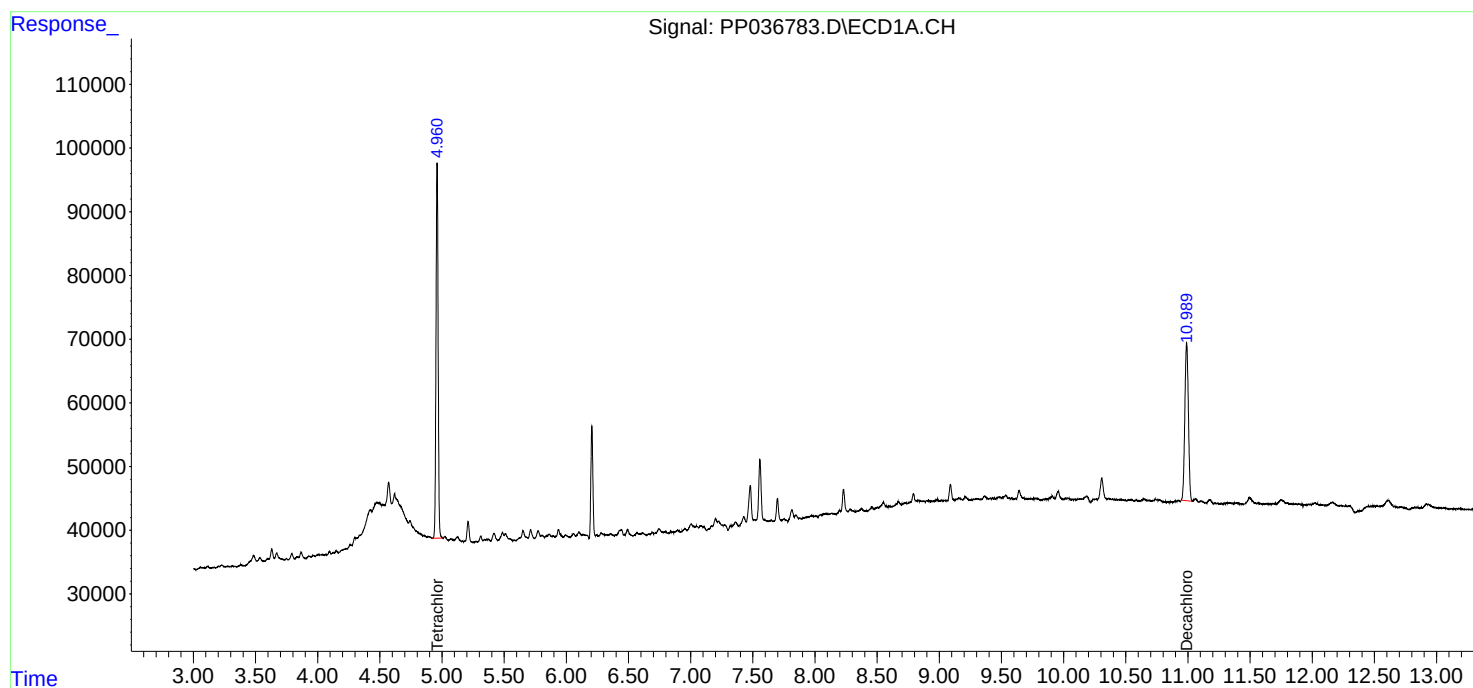


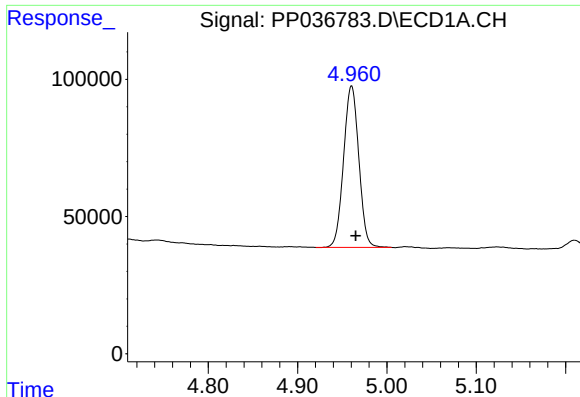

#1 Tetrachloro-m-xylene


R.T.: 4.960 min  
Delta R.T.: -0.005 min  
Response: 697518  
Conc: 15.78 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
FK-PS-01-075

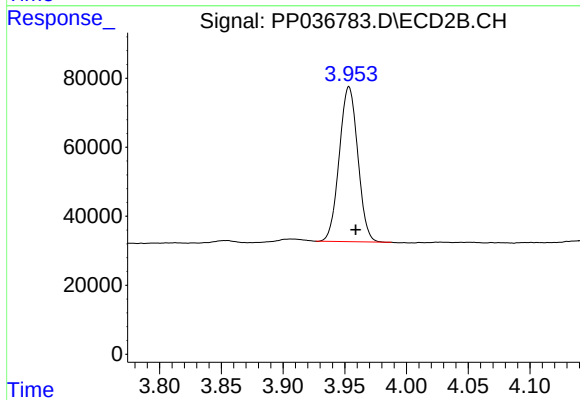


#1 Tetrachloro-m-xylene

R.T.: 3.953 min  
Delta R.T.: -0.005 min  
Response: 469285  
Conc: 15.15 ng/ml

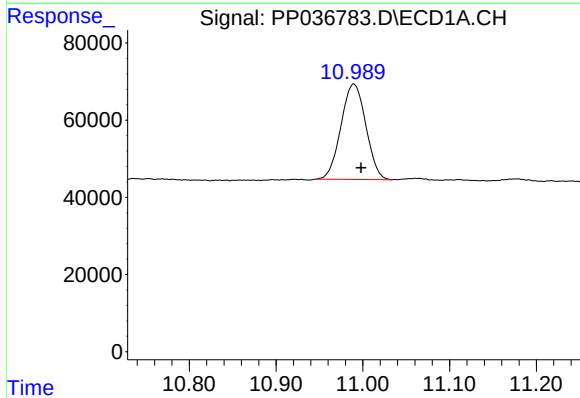

#2 Decachlorobiphenyl

R.T.: 10.990 min  
Delta R.T.: -0.008 min  
Response: 492849  
Conc: 11.49 ng/ml

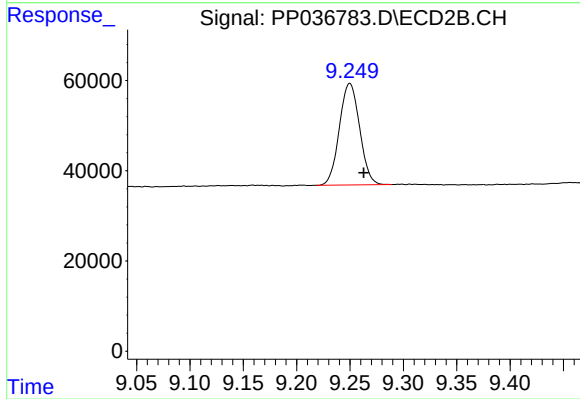

#2 Decachlorobiphenyl

R.T.: 9.250 min  
Delta R.T.: -0.013 min  
Response: 298234  
Conc: 9.33 ng/ml