

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062425\
 Data File : PP073214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2025 19:08
 Operator : YP\AJ
 Sample : PB168599BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB168599BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/25/2025
 Supervised By :mohammad ahmed 06/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 05:31:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.492	3.788	41352676	34424666	19.591	19.106
2) SA Decachlor...	10.181	8.794	32388548	28261816	18.953m	21.174

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062425\
Data File : PP073214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2025 19:08
Operator : YP\AJ
Sample : PB168599BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB168599BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/25/2025
Supervised By :mohammad ahmed 06/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 05:31:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

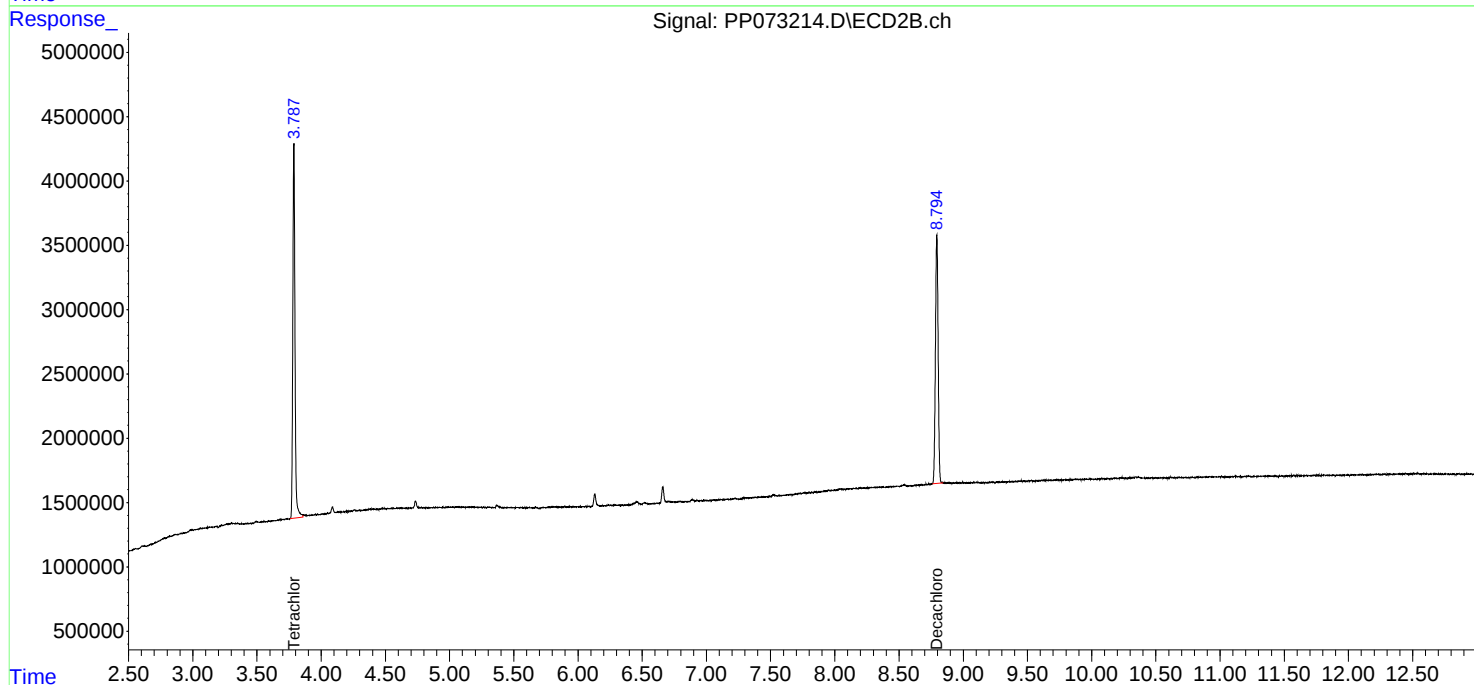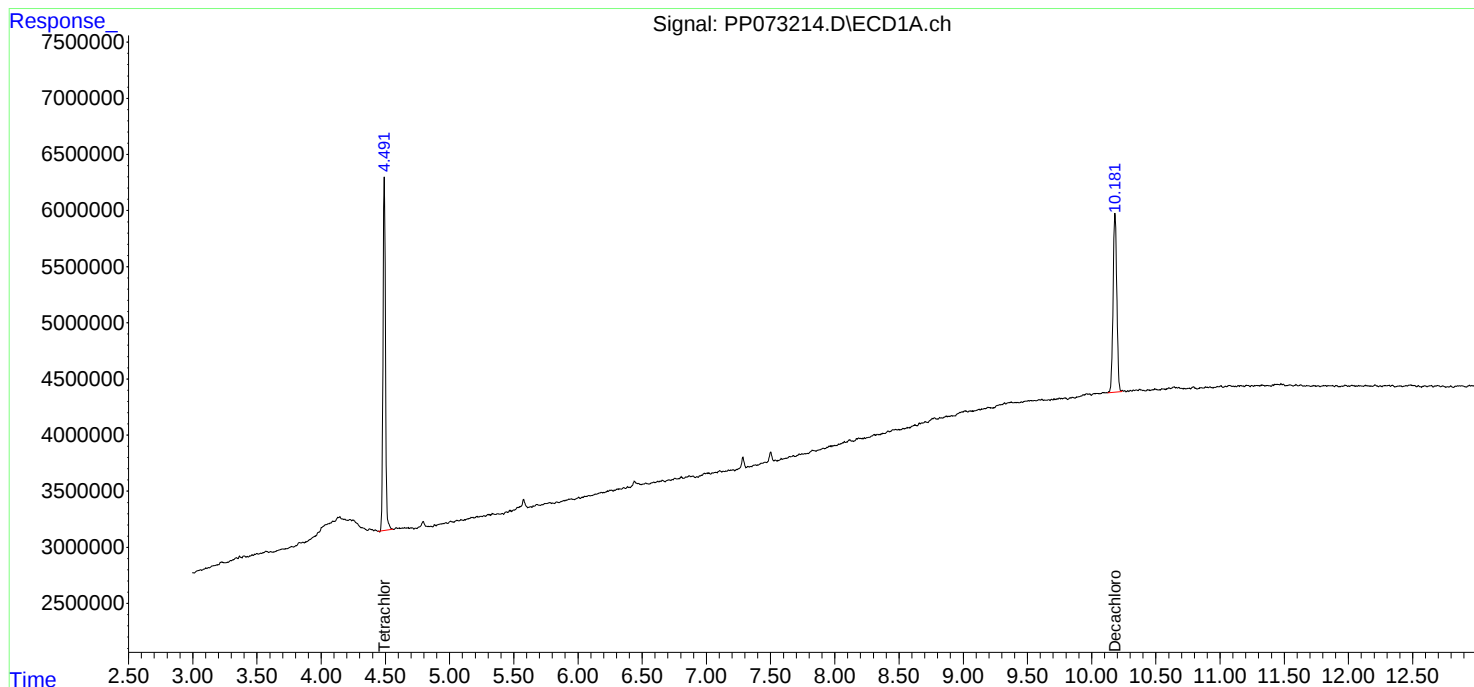

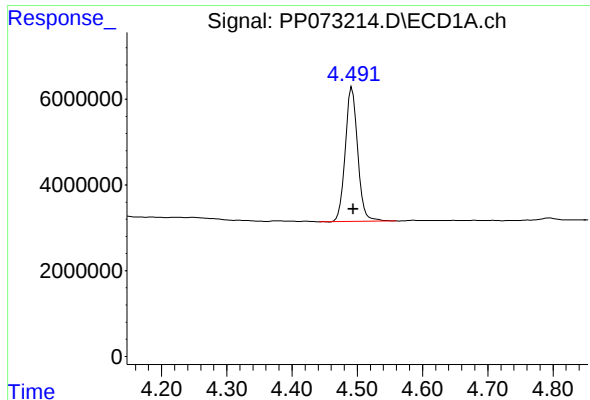


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: -0.002 min
Response: 41352676
Conc: 19.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB168599BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/25/2025
Supervised By :mohammad ahmed 06/26/2025

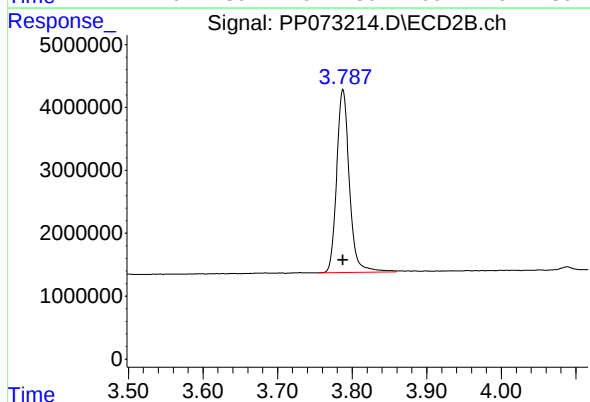


#1 Tetrachloro-m-xylene

R.T.: 3.788 min
Delta R.T.: 0.000 min
Response: 34424666
Conc: 19.11 ng/ml

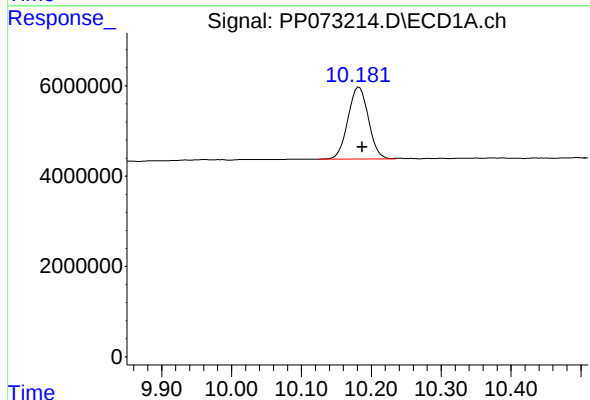

#2 Decachlorobiphenyl

R.T.: 10.181 min
Delta R.T.: -0.006 min
Response: 32388548
Conc: 18.95 ng/ml m

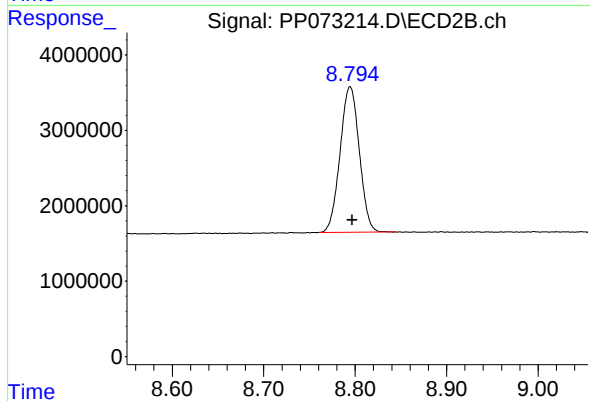

#2 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 28261816
Conc: 21.17 ng/ml