

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP062518\  
 Data File : PP026644.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 25 Jun 2018 18:05  
 Operator : UA/AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 26 06:53:26 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP062518.M  
 Quant Title : 8080.M  
 QLast Update : Tue Jun 26 06:52:58 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|----------|--------|--------|--------|
| -----                       |        |       |          |        |        |        |
| System Monitoring Compounds |        |       |          |        |        |        |
| Target Compounds            |        |       |          |        |        |        |
| 8) T DICHLORPROP            | 12.896 | 0.000 | 30030022 | 0      | 56.453 | N.D. # |
| 9) T 2,4-D                  | 13.268 | 0.000 | 35094155 | 0      | 51.057 | N.D. # |
| 15) T Picloram              | 16.937 | 0.000 | 3608698  | 0      | 0.793  | N.D. # |
| -----                       |        |       |          |        |        |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP062518\  
Data File : PP026644.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 25 Jun 2018 18:05  
Operator : UA/AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 26 06:53:26 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP062518.M  
Quant Title : 8080.M  
QLast Update : Tue Jun 26 06:52:58 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

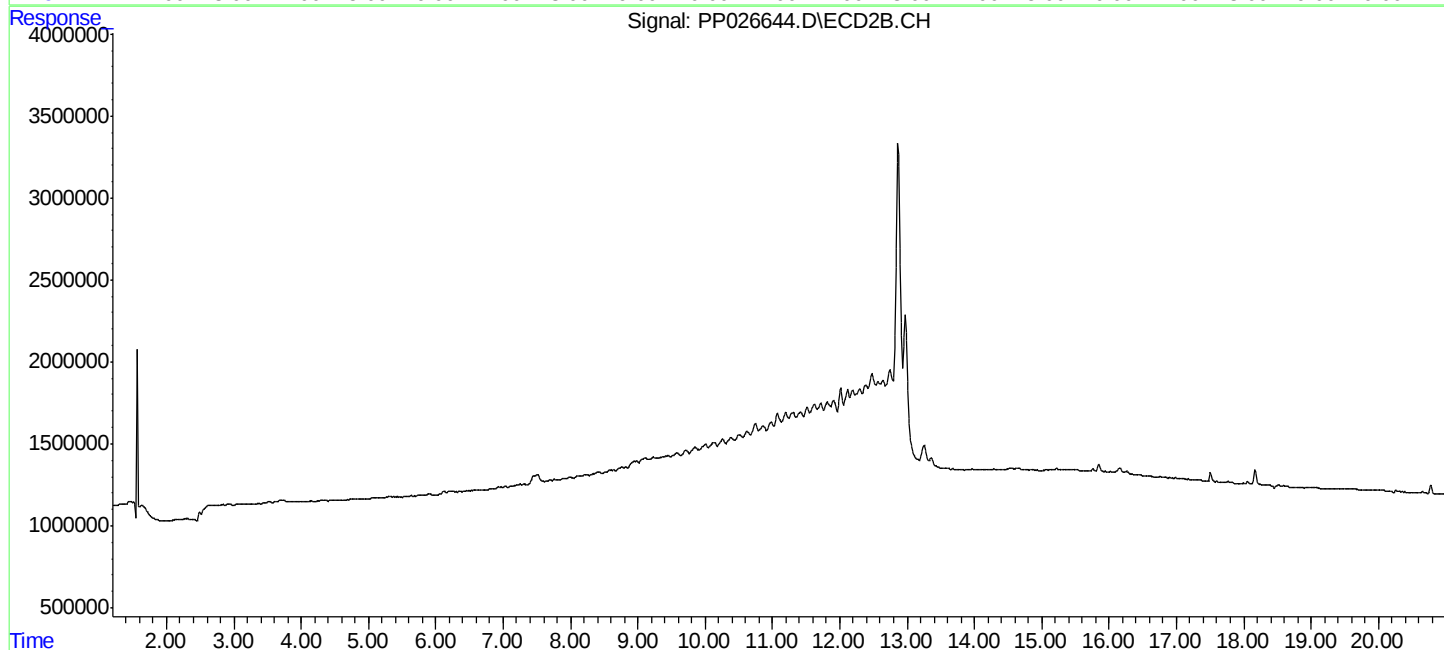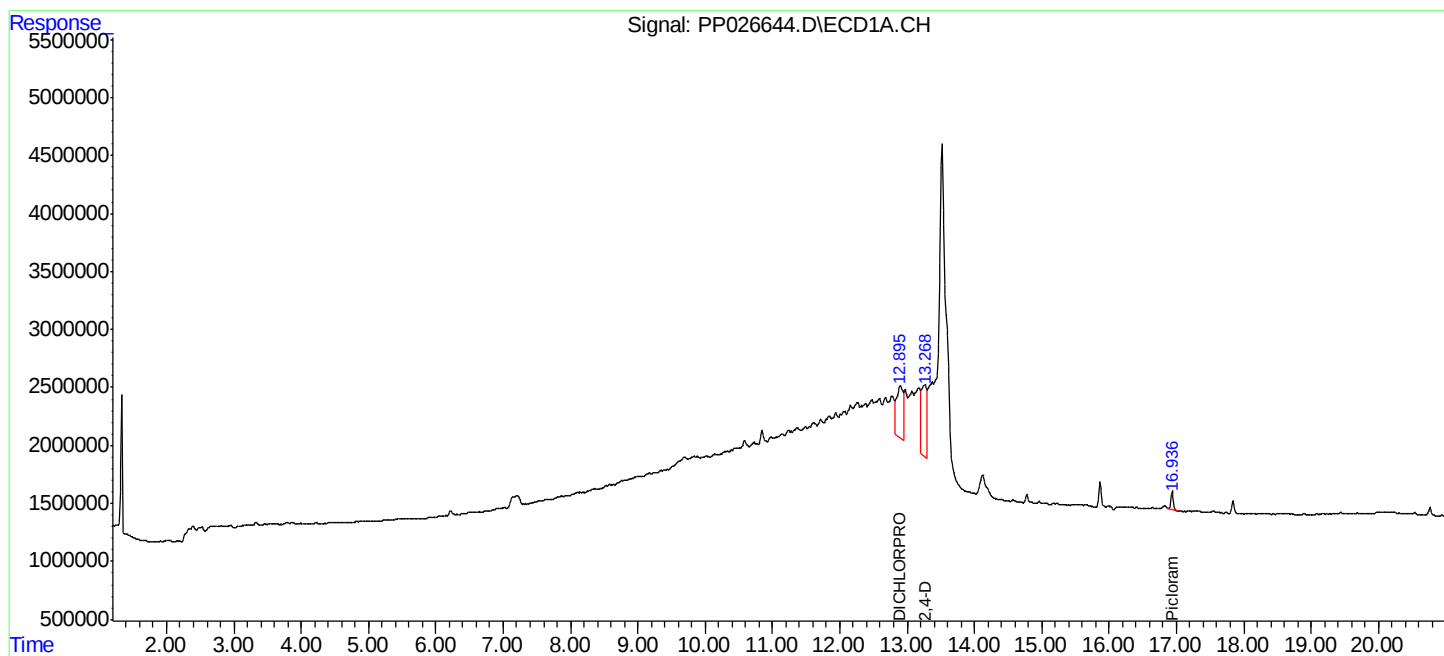


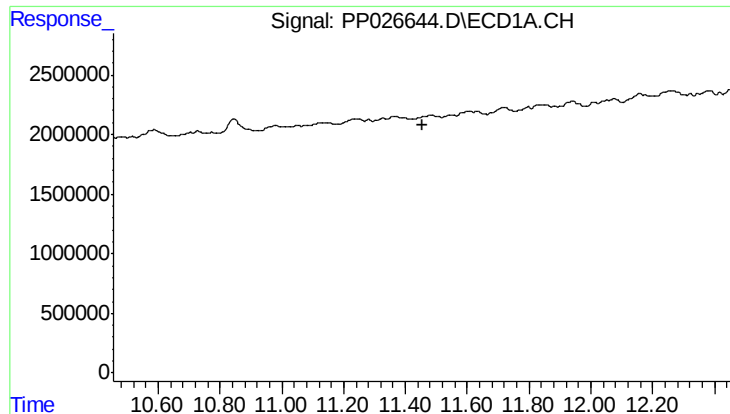

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T.: 11.454 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
HEXANE

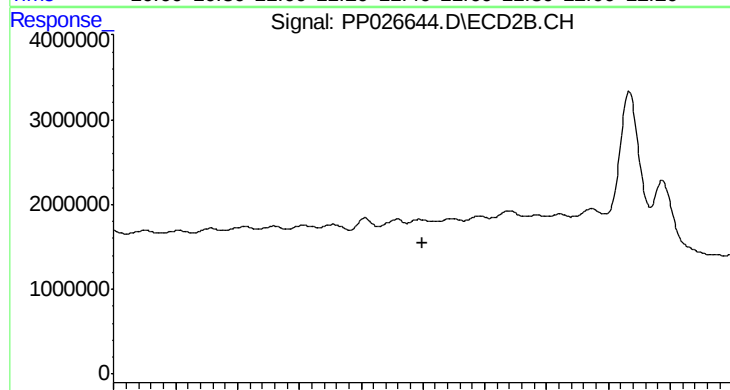


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T.: 12.198 min  
Response: 0  
Conc: N.D.

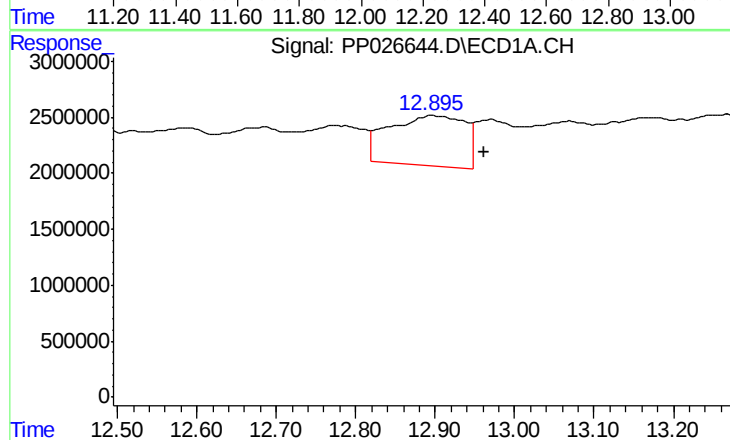


#8 DICHLORPROP

R.T.: 12.896 min  
Delta R.T.: -0.065 min  
Response: 30030022  
Conc: 56.45 ng/ml

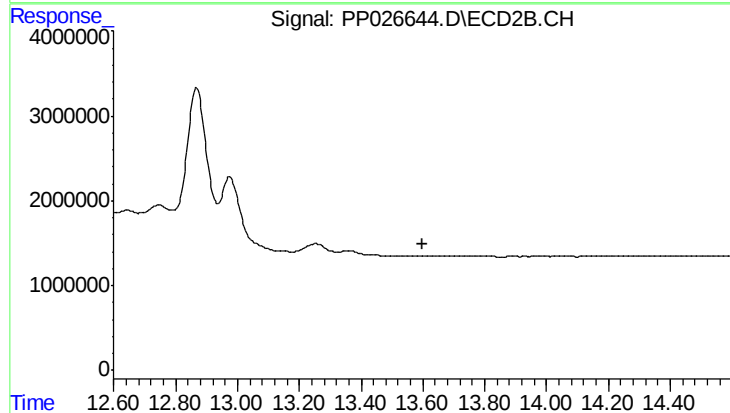

#8 DICHLORPROP


R.T.: 0.000 min  
Exp R.T.: 13.597 min  
Response: 0  
Conc: N.D.

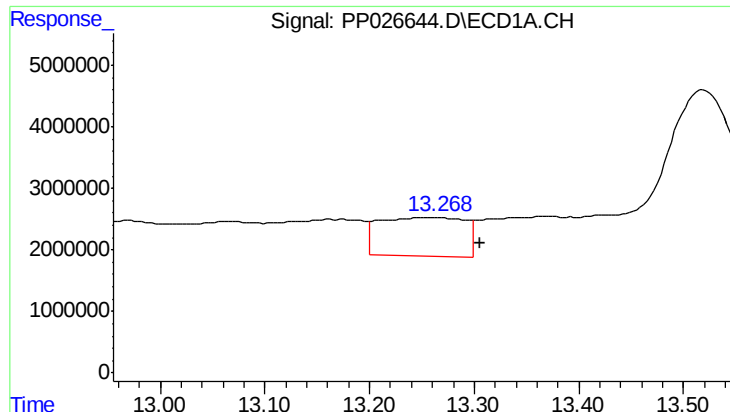

#9 2,4-D


R.T.: 13.268 min  
Delta R.T.: -0.038 min  
Response: 35094155  
Conc: 51.06 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
HEXANE

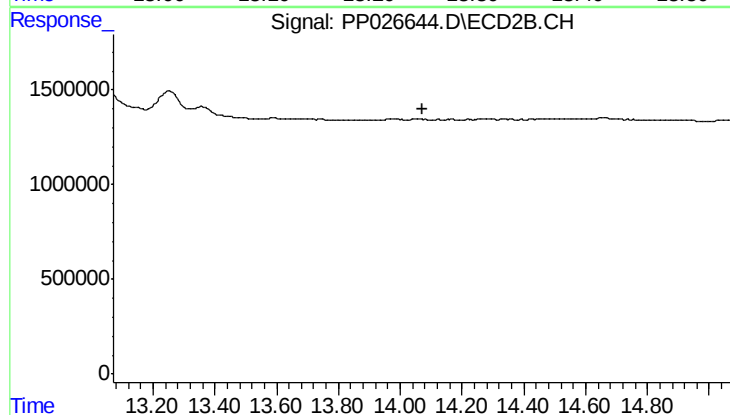


#9 2,4-D

R.T.: 0.000 min  
Exp R.T.: 14.071 min  
Response: 0  
Conc: N.D.

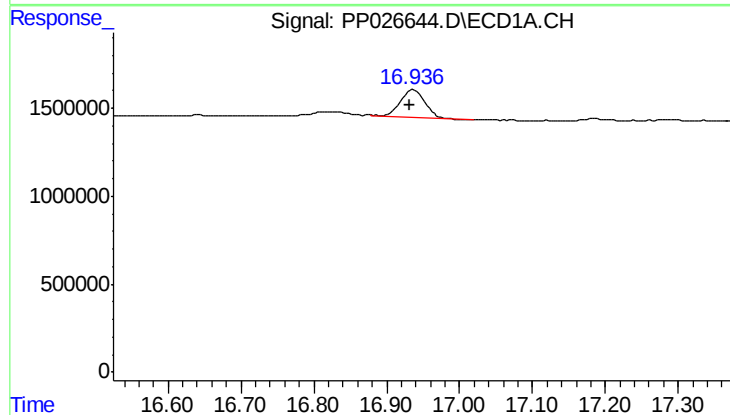

#15 Picloram

R.T.: 16.937 min  
Delta R.T.: 0.005 min  
Response: 3608698  
Conc: 0.79 ng/ml

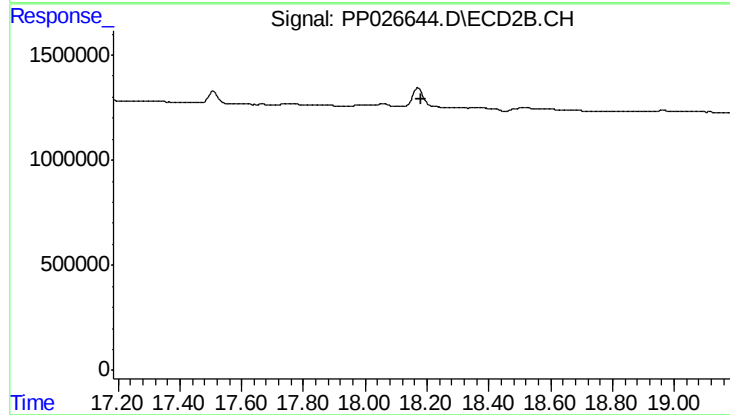

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 18.183 min  
Response: 0  
Conc: N.D.