

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
 Data File : PP036811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 20:00
 Operator : DD\AJ
 Sample : M2851-03DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-08DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 04:23:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.960	3.954	90352	60254	2.044	1.945
2) SA Decachlor...	10.984	9.249	99511	55735	2.320	1.743
Target Compounds						
8) L2 AR-1221-1	5.210	0.000	21508	0	38.310	N.D. #
28) L6 AR-1254-3	7.818	0.000	4838	0	1.633	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
Data File : PP036811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 20:00
Operator : DD\AJ
Sample : M2851-03DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 04:23:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

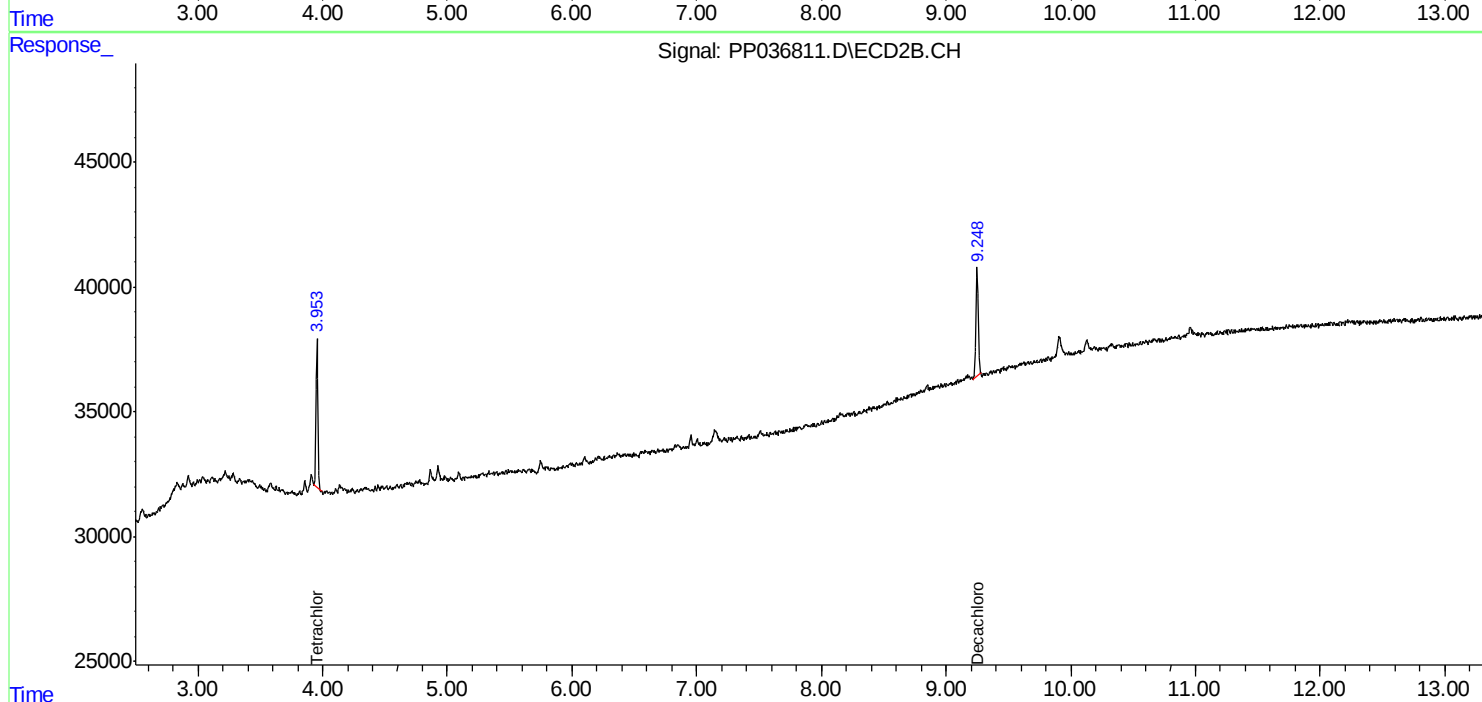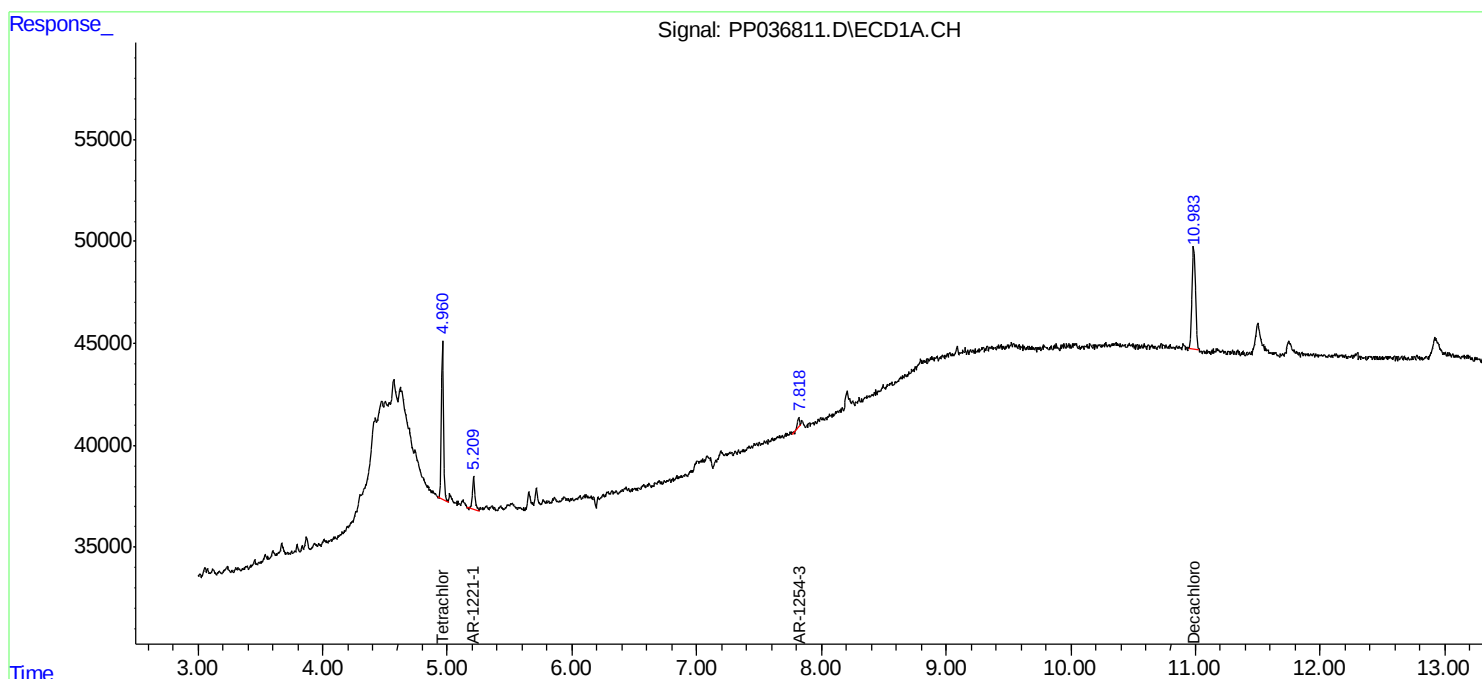


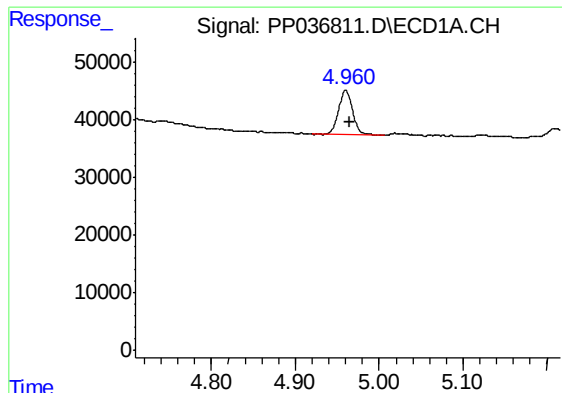

#1 Tetrachloro-m-xylene


R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 90352
Conc: 2.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08DL

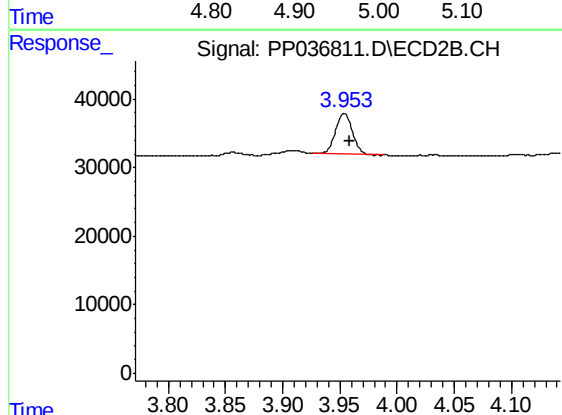


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 60254
Conc: 1.95 ng/ml

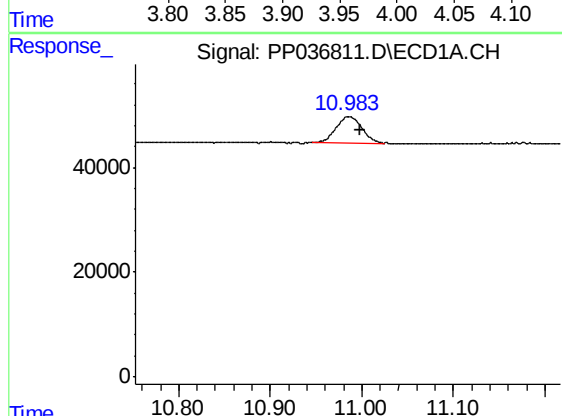


#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.014 min
Response: 99511
Conc: 2.32 ng/ml

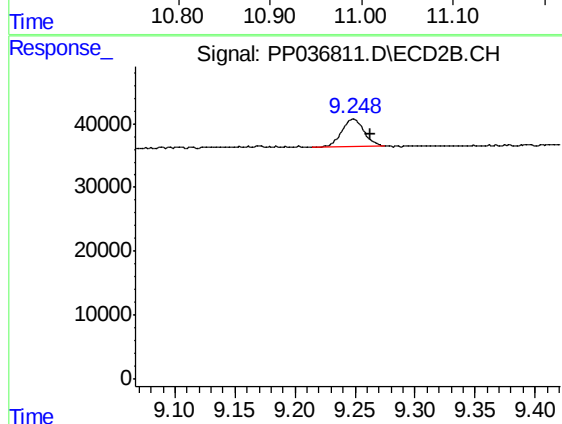

#2 Decachlorobiphenyl


R.T.: 9.249 min
Delta R.T.: -0.014 min
Response: 55735
Conc: 1.74 ng/ml

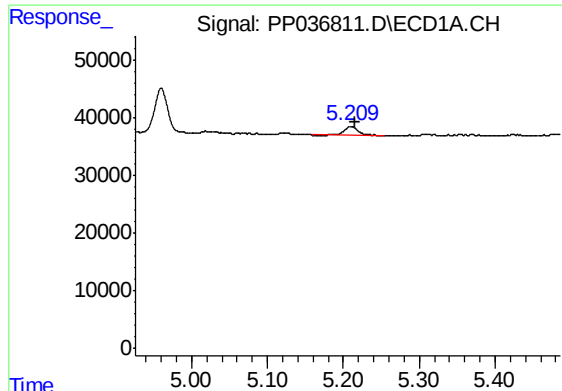

#8 AR-1221-1


R.T.: 5.210 min
Delta R.T.: -0.006 min
Response: 21508
Conc: 38.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08DL

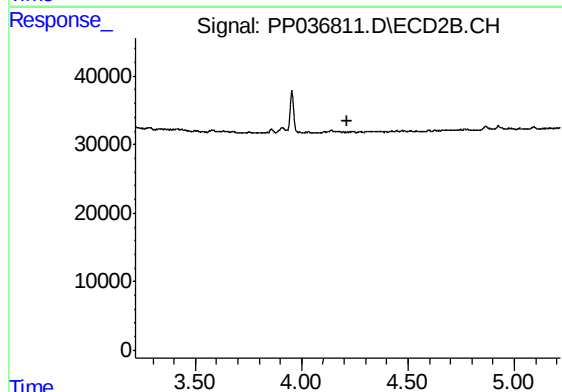


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

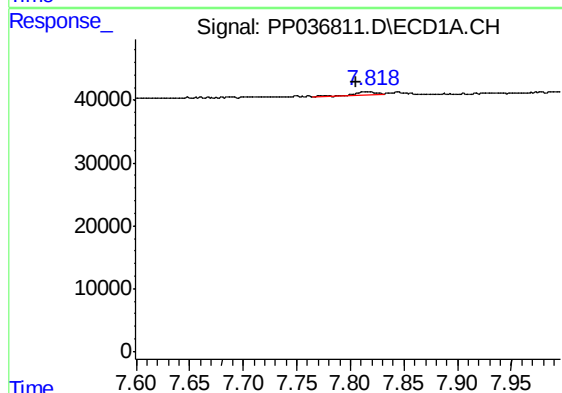

#28 AR-1254-3

R.T.: 7.818 min
Delta R.T.: 0.013 min
Response: 4838
Conc: 1.63 ng/ml

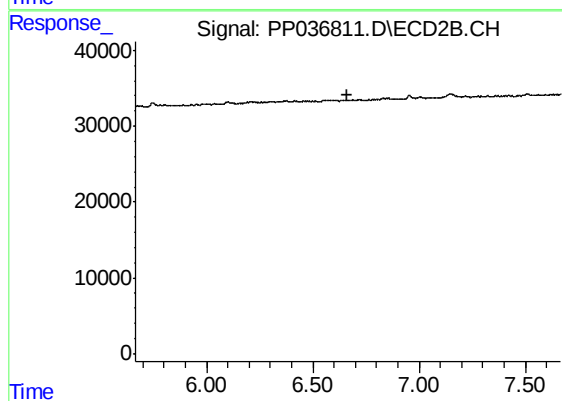

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.