

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
 Data File : PP036799.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 15:48
 Operator : DD\AJ
 Sample : M2829-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 15B-STOCKPILE-2A

Manual Integrations
 APPROVED

mohammad
 6/28/2021 9:33:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 04:16:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.954	735204	490193	16.634	15.826
2) SA Decachlor...	10.992	9.249	831747	500357	19.389	15.646m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
Data File : PP036799.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 15:48
Operator : DD\AJ
Sample : M2829-02
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
15B-STOCKPILE-2A


Manual Integrations
APPROVED

mohammad
6/28/2021 9:33:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 04:16:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

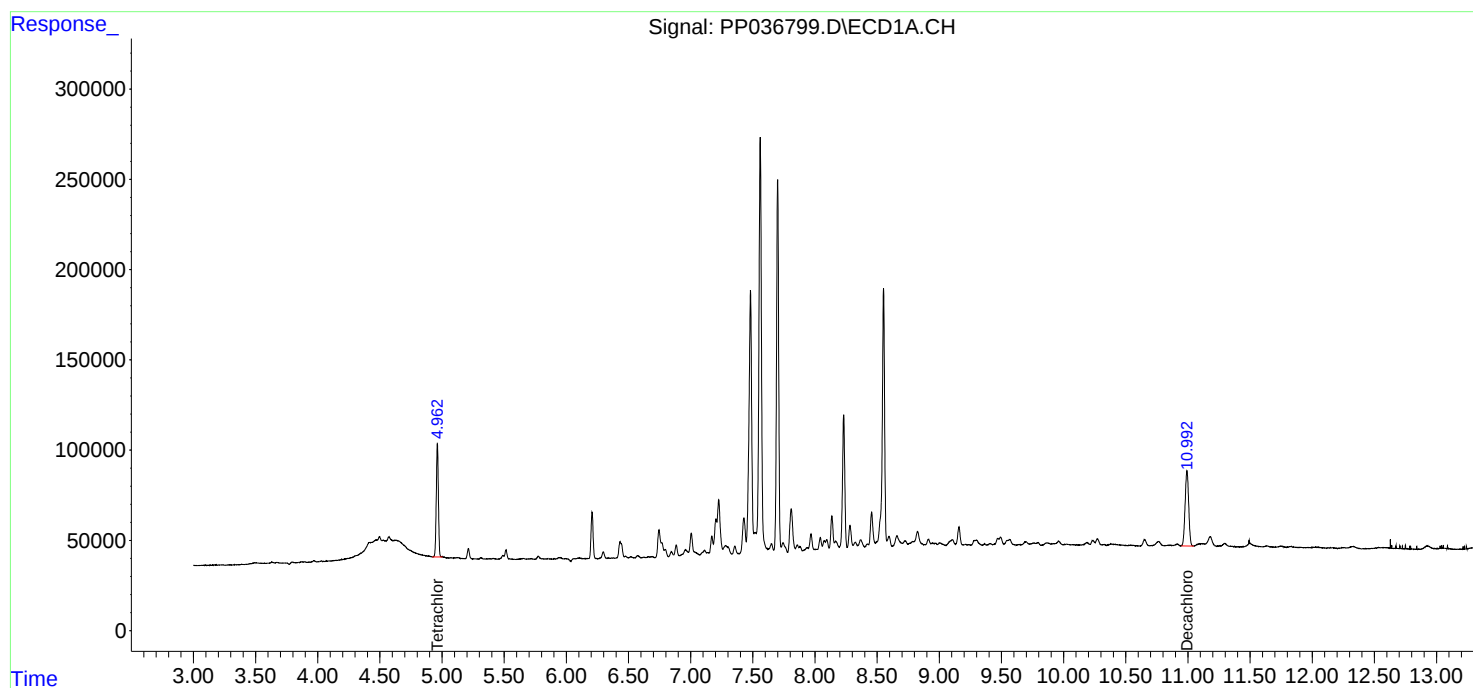

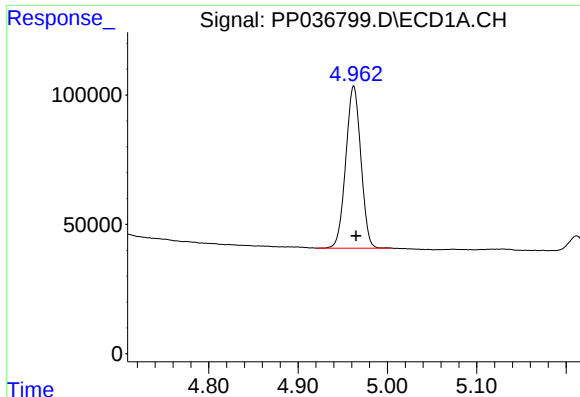


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 735204
Conc: 16.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
15B-STOCKPILE-2A


Manual Integrations
APPROVED

mohammad
6/28/2021 9:33:33 AM

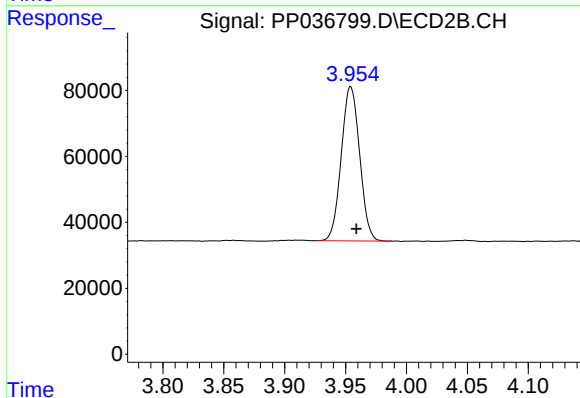


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 490193
Conc: 15.83 ng/ml

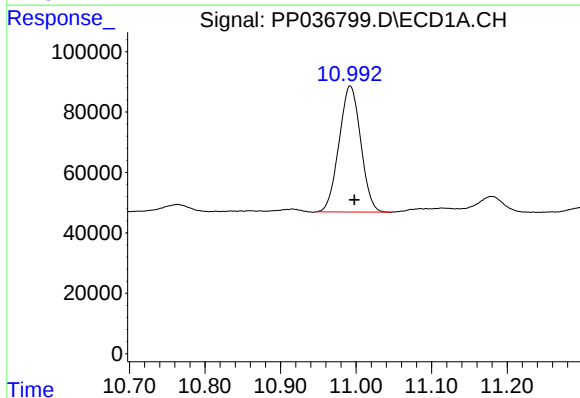

#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.006 min
Response: 831747
Conc: 19.39 ng/ml

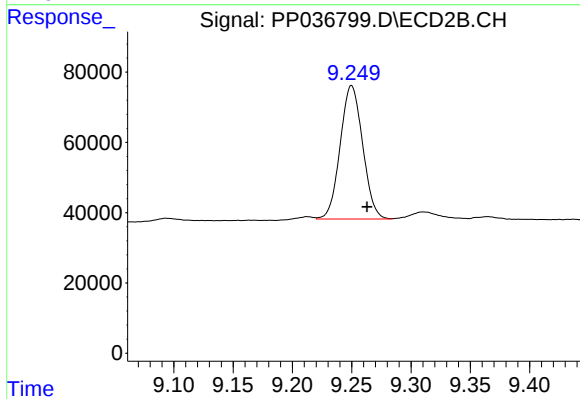

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.013 min
Response: 500357
Conc: 15.65 ng/ml m