

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
 Data File : PP036810.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 19:26
 Operator : DD\AJ
 Sample : M2851-01DL 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-07DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 04:23:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.960	3.953	91189	60896	2.063	1.966
2)	SA Decachlor...	10.988	9.249	98701	57399	2.301	1.795

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
Data File : PP036810.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 19:26
Operator : DD\AJ
Sample : M2851-01DL 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-07DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 04:23:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

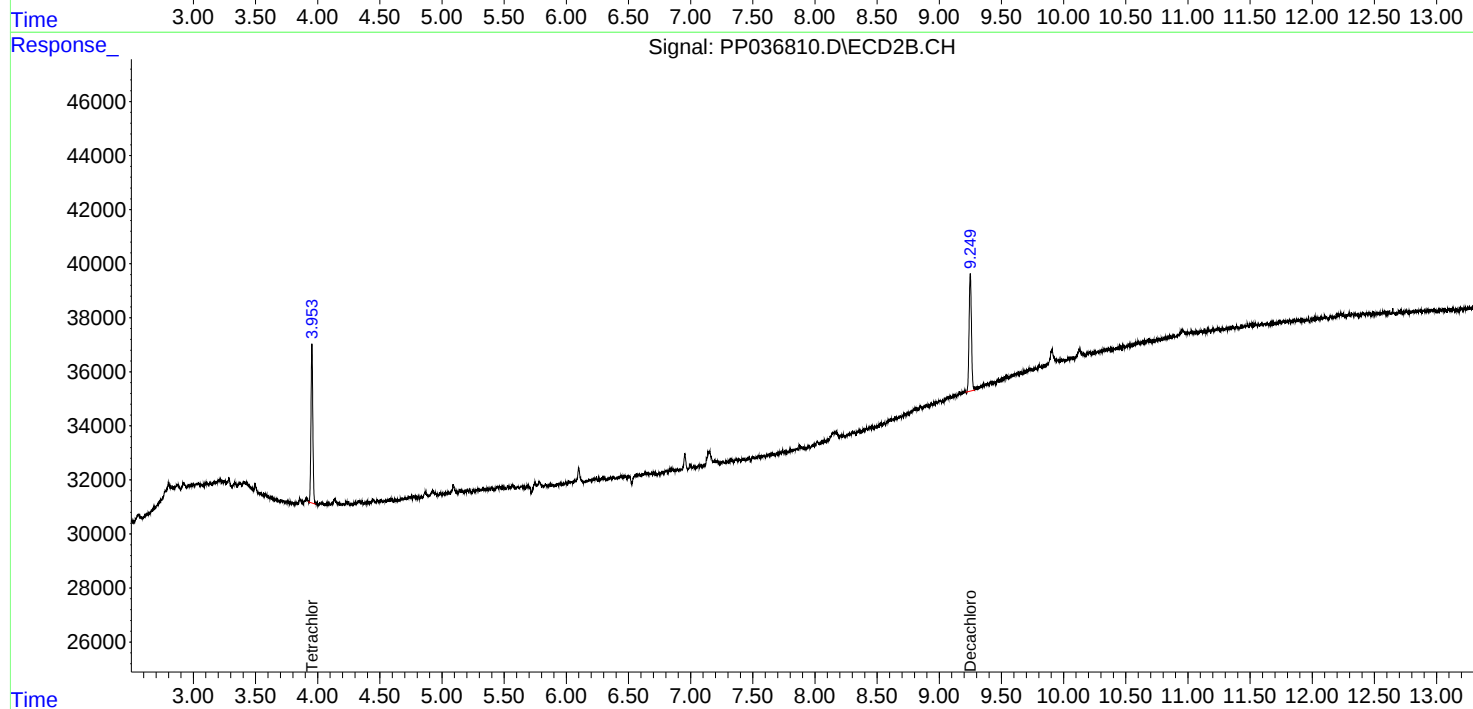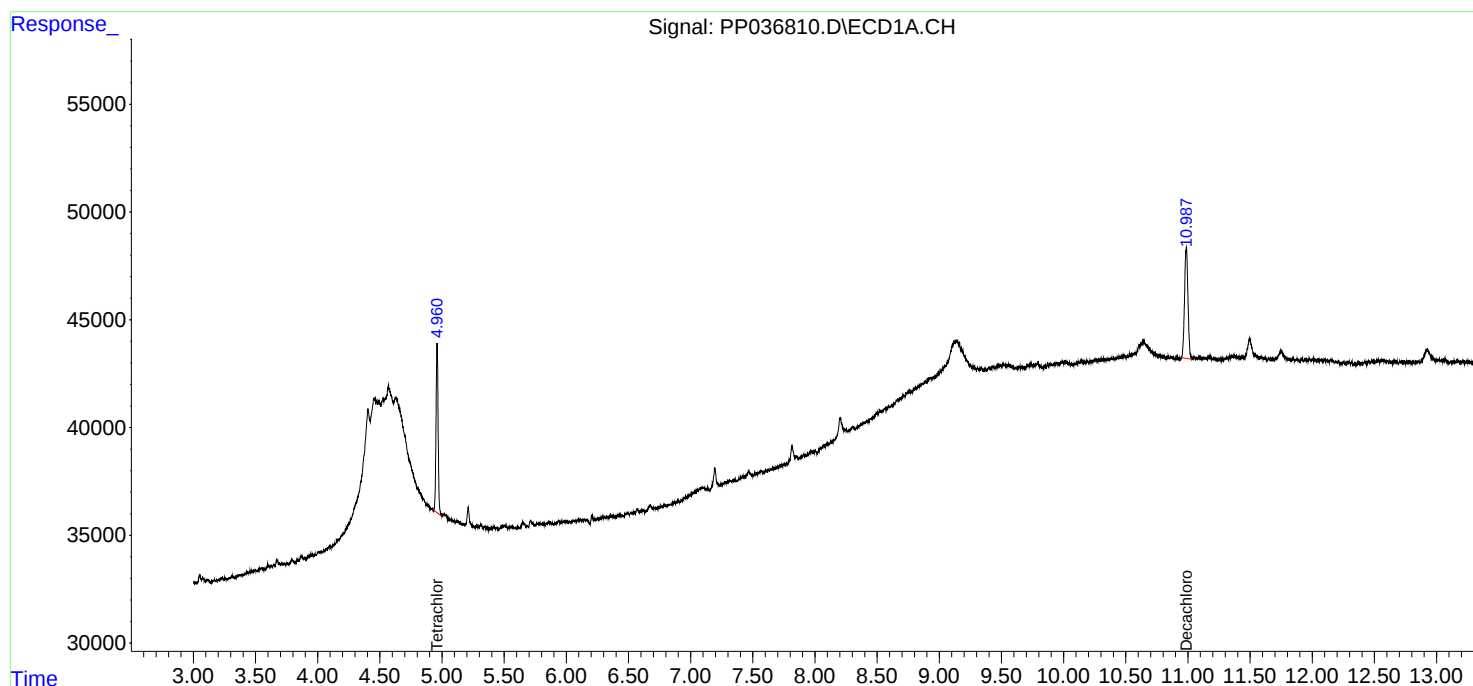


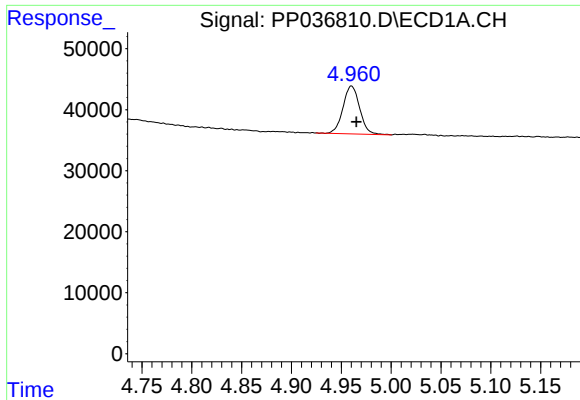

#1 Tetrachloro-m-xylene


R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 91189
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-07DL

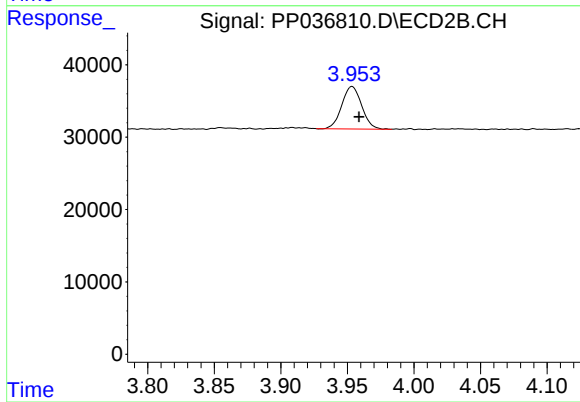


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.005 min
Response: 60896
Conc: 1.97 ng/ml

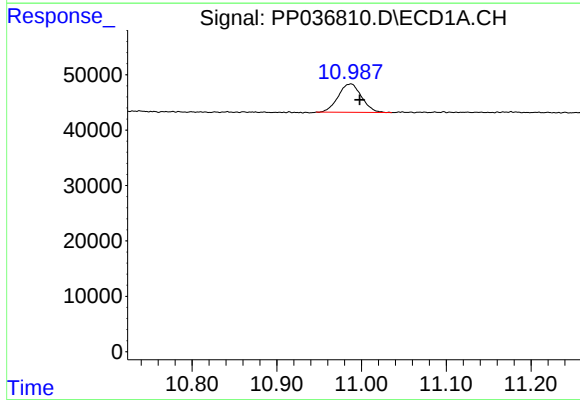

#2 Decachlorobiphenyl

R.T.: 10.988 min
Delta R.T.: -0.010 min
Response: 98701
Conc: 2.30 ng/ml

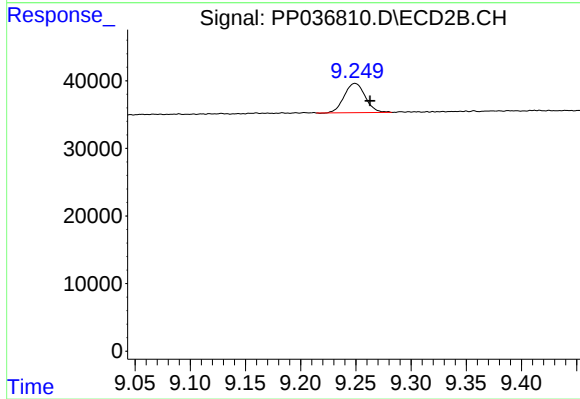

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.014 min
Response: 57399
Conc: 1.79 ng/ml