

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
 Data File : PP036811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 20:00
 Operator : DD\AJ
 Sample : M2851-03DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-08DL

Manual Integrations
 APPROVED

mohammad
 6/28/2021 9:33:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 04:23:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.960	3.953	90352	66174	2.044	2.136m
2) SA Decachlor...	10.984	9.248	99511	59063	2.320	1.847m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062521\
Data File : PP036811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 20:00
Operator : DD\AJ
Sample : M2851-03DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08DL


Manual Integrations
APPROVED

mohammad
6/28/2021 9:33:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 04:23:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

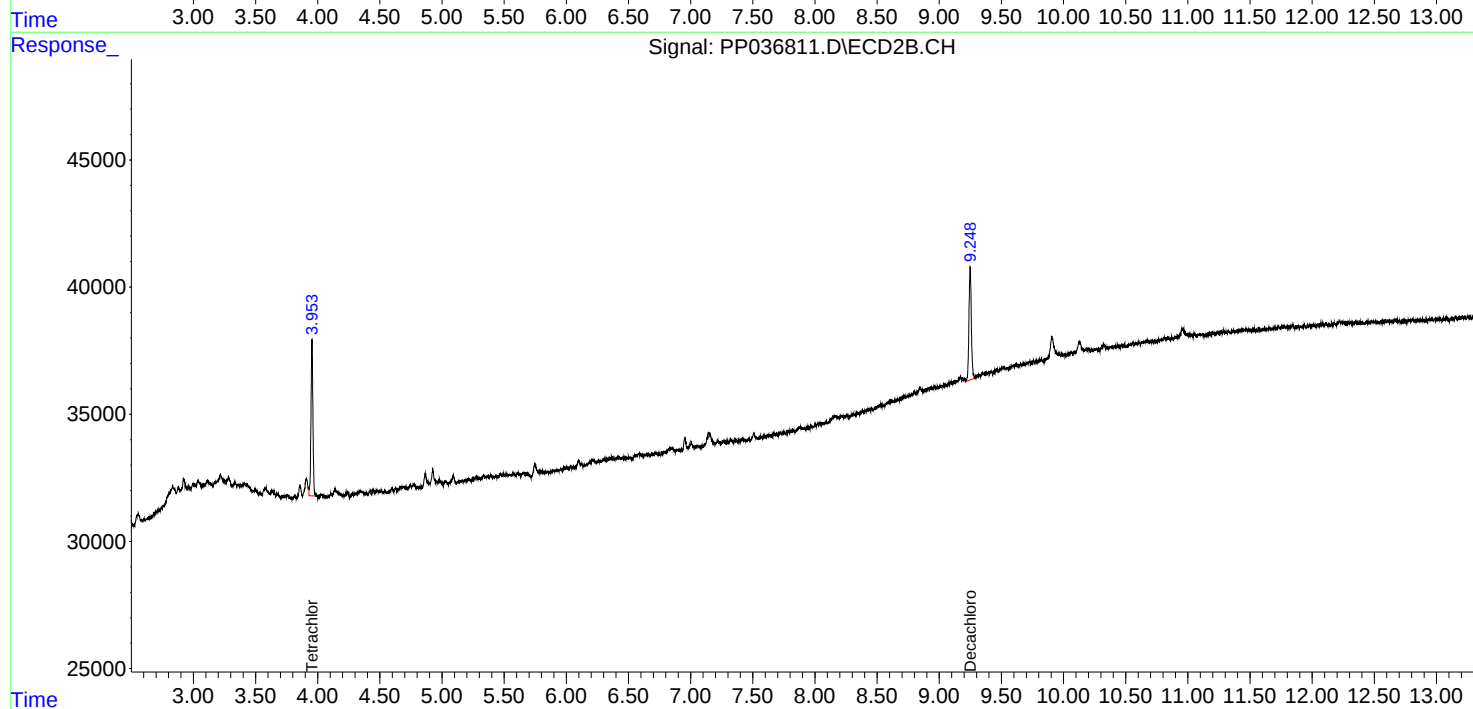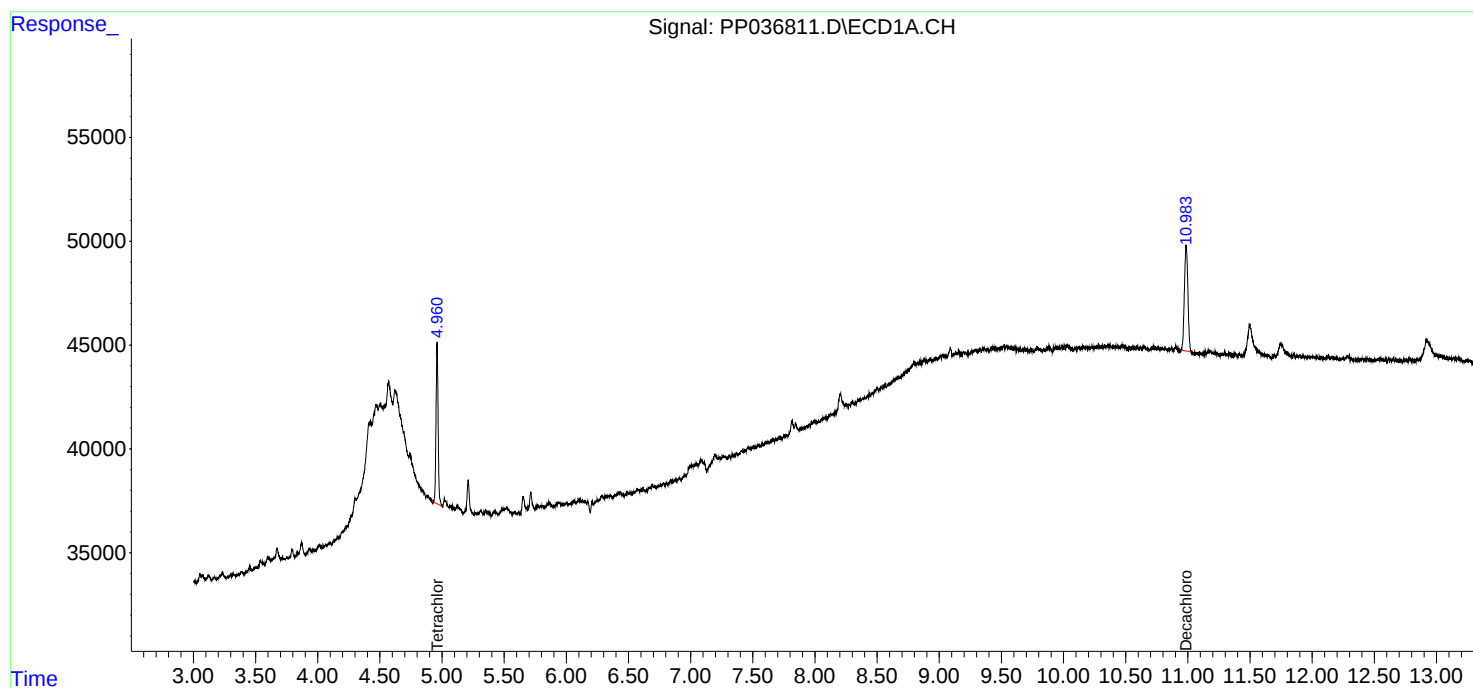

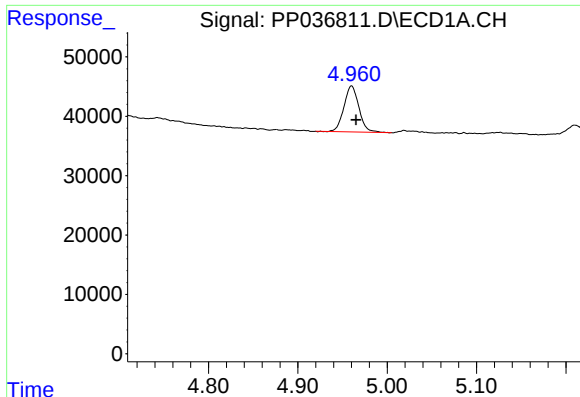


#1 Tetrachloro-m-xylene

R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 90352
Conc: 2.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08DL


Manual Integrations
APPROVED

mohammad
6/28/2021 9:33:40 AM

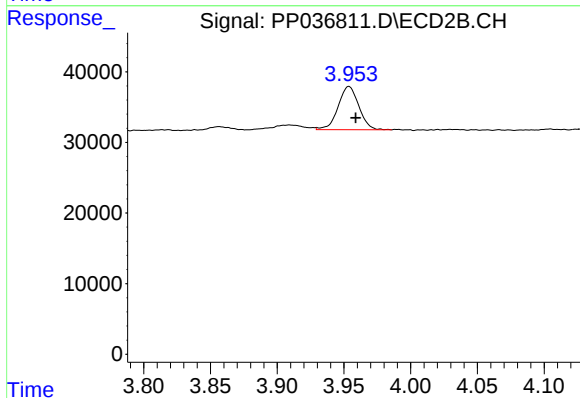


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.005 min
Response: 66174
Conc: 2.14 ng/ml m

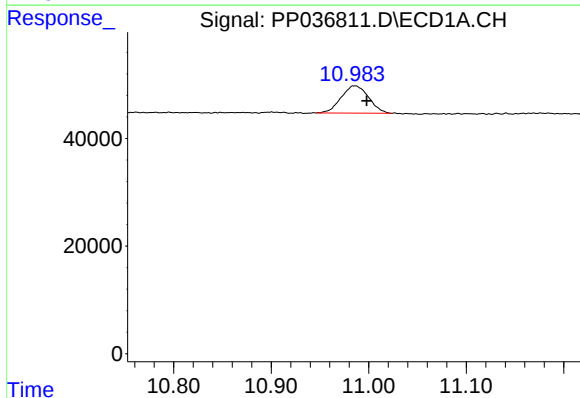

#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.014 min
Response: 99511
Conc: 2.32 ng/ml

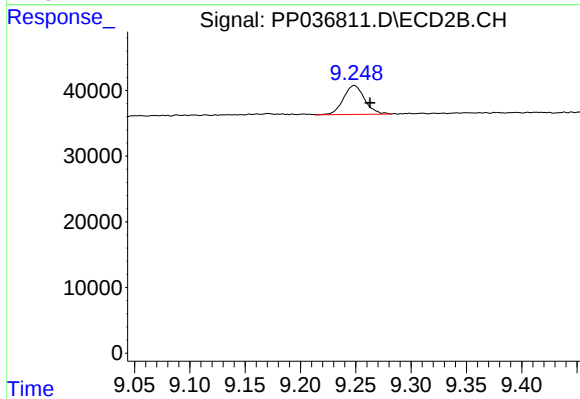

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.015 min
Response: 59063
Conc: 1.85 ng/ml m