

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062524\
 Data File : PP066018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2024 16:14
 Operator : YP\AJ
 Sample : P3048-02 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2308-0064-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 00:35:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 05:25:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.826	4.064	2163816	3690763	1.141	1.322
2) SA Decachlor...	10.845	9.247	3208193	1976158	1.631	1.341
Target Compounds						
27) L6 AR-1254-2	7.081	0.000	150194	0	1.271	N.D. #
28) L6 AR-1254-3	7.450	0.000	1044130	0	8.556	N.D. #
29) L6 AR-1254-4	7.764f	0.000	1101597	0	12.388	N.D. #
31) L7 AR-1260-1	7.609	0.000	726341	0	7.499	N.D. #
32) L7 AR-1260-2	7.872	0.000	733354	0	6.541	N.D. #
33) L7 AR-1260-3	8.218	0.000	236859	0	2.713	N.D. #
34) L7 AR-1260-4	8.478	0.000	180439	0	1.801	N.D. #
36) L8 AR-1262-1	8.304	0.000	1180617	0	22.035	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062524\
Data File : PP066018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2024 16:14
Operator : YP\AJ
Sample : P3048-02 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
Y2308-0064-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 00:35:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

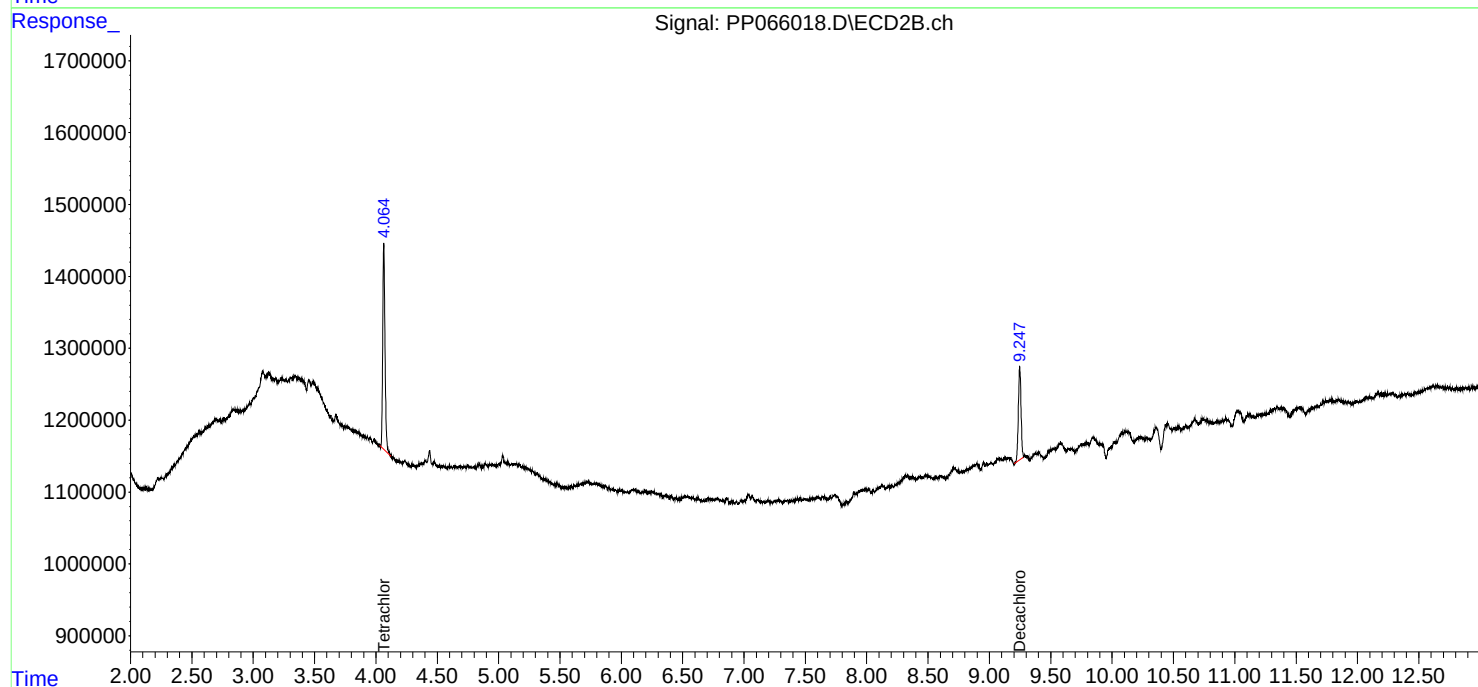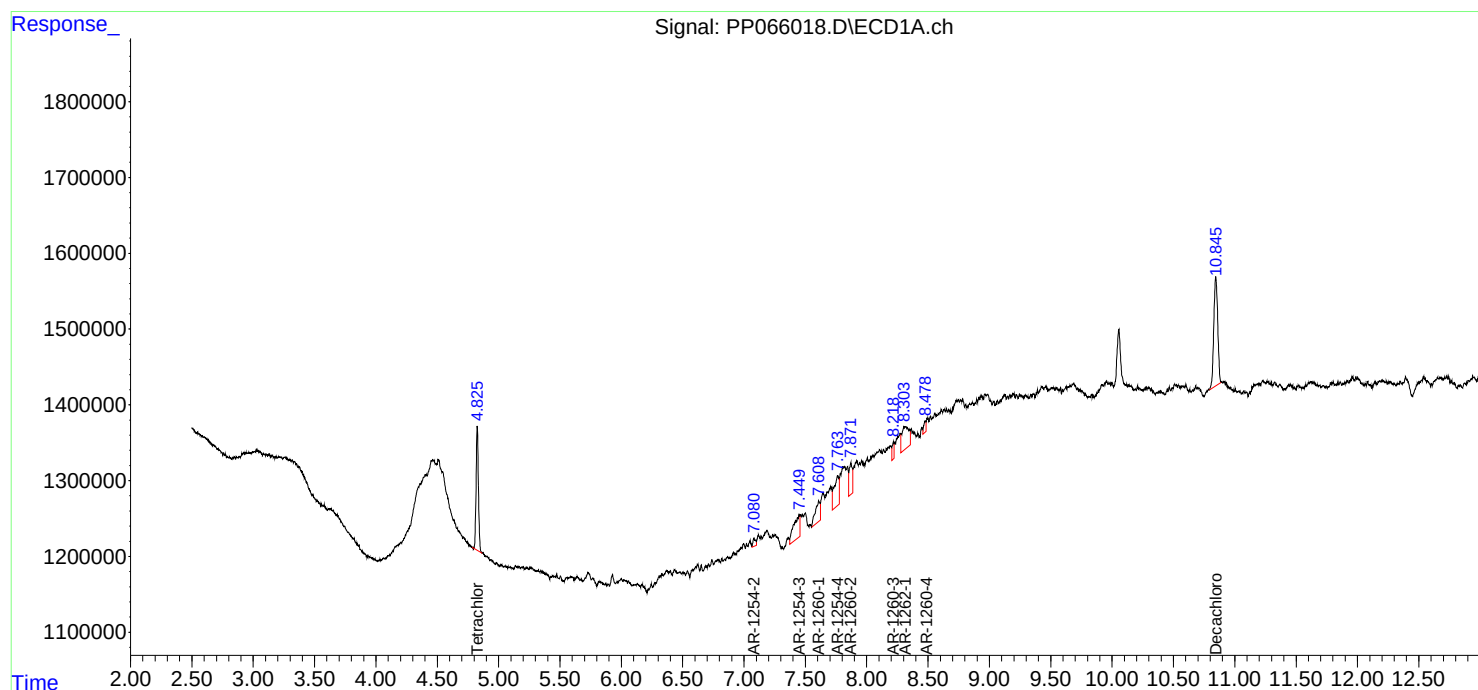


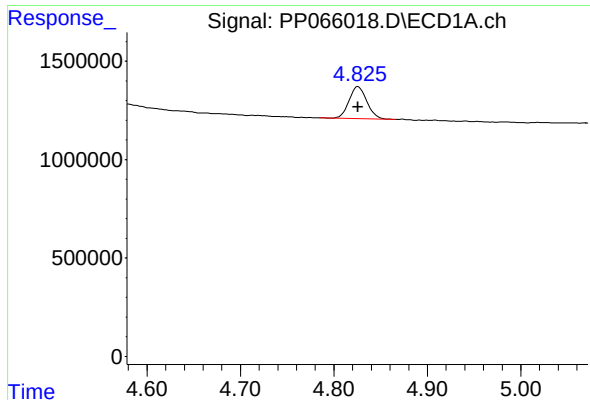

#1 Tetrachloro-m-xylene


R.T.: 4.826 min
Delta R.T.: 0.000 min
Response: 2163816
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0064-1-2

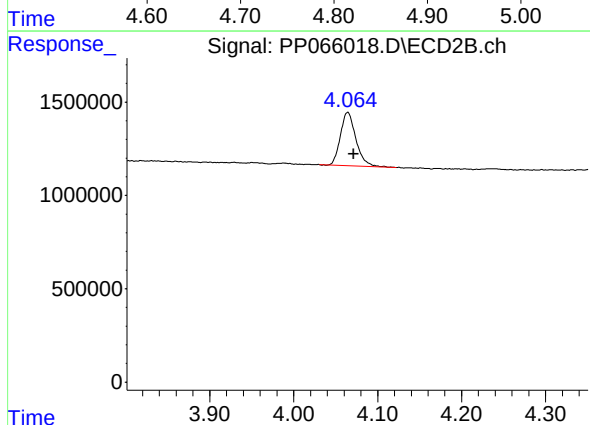


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: -0.007 min
Response: 3690763
Conc: 1.32 ng/ml

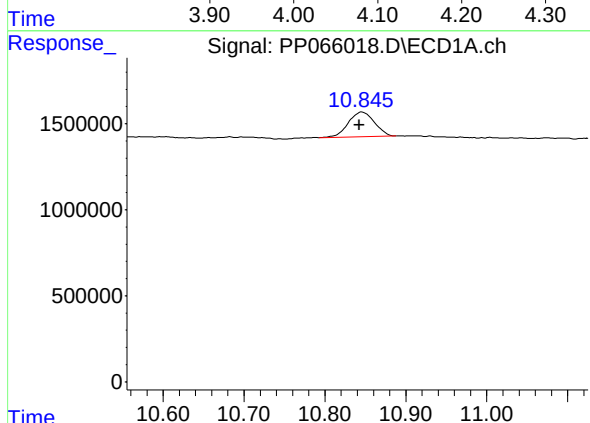


#2 Decachlorobiphenyl

R.T.: 10.845 min
Delta R.T.: 0.003 min
Response: 3208193
Conc: 1.63 ng/ml

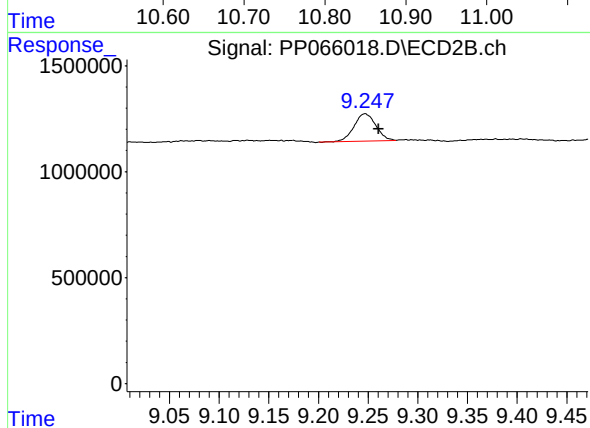

#2 Decachlorobiphenyl


R.T.: 9.247 min
Delta R.T.: -0.014 min
Response: 1976158
Conc: 1.34 ng/ml

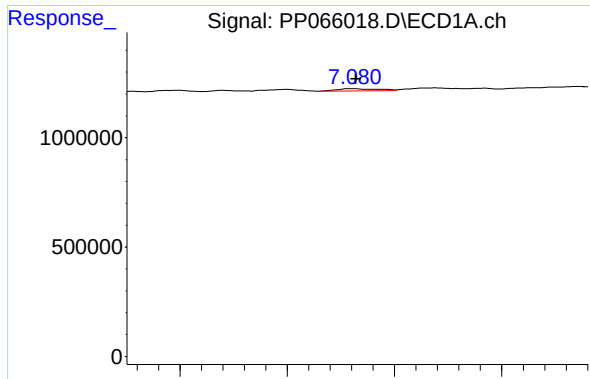

#27 AR-1254-2


R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 150194
Conc: 1.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0064-1-2

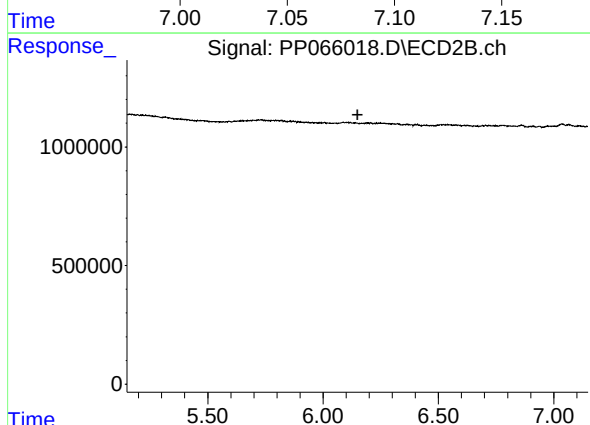


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.149 min
Response: 0
Conc: N.D.

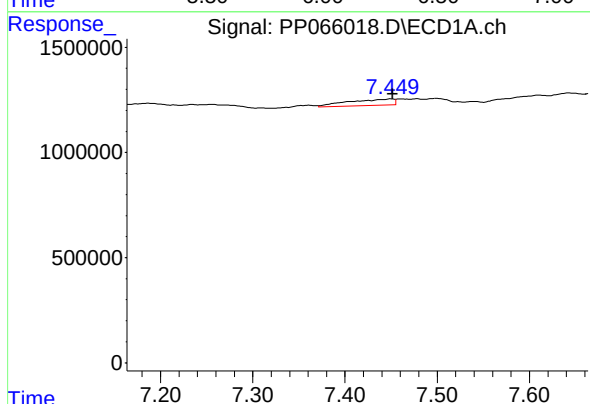


#28 AR-1254-3

R.T.: 7.450 min
Delta R.T.: -0.002 min
Response: 1044130
Conc: 8.56 ng/ml

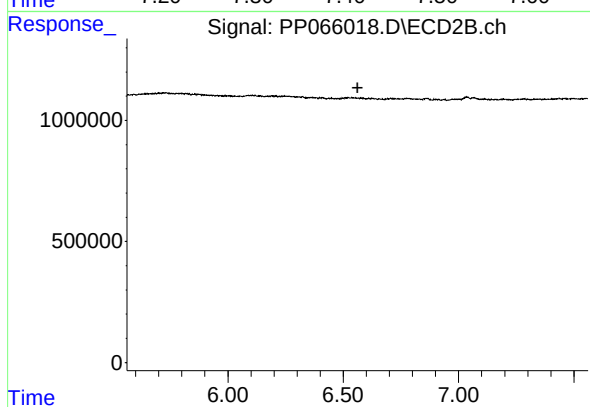

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.562 min
Response: 0
Conc: N.D.

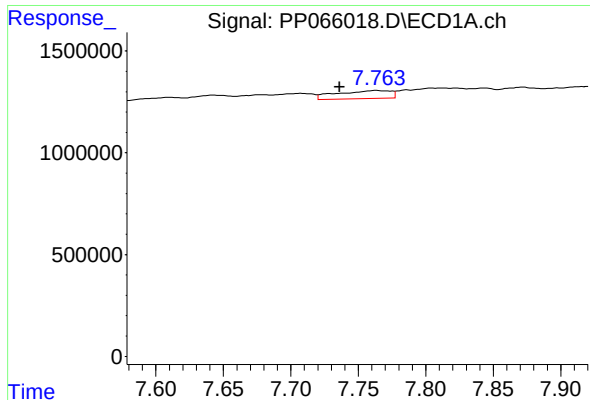

#29 AR-1254-4


R.T.: 7.764 min
Delta R.T.: 0.028 min
Response: 1101597
Conc: 12.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0064-1-2

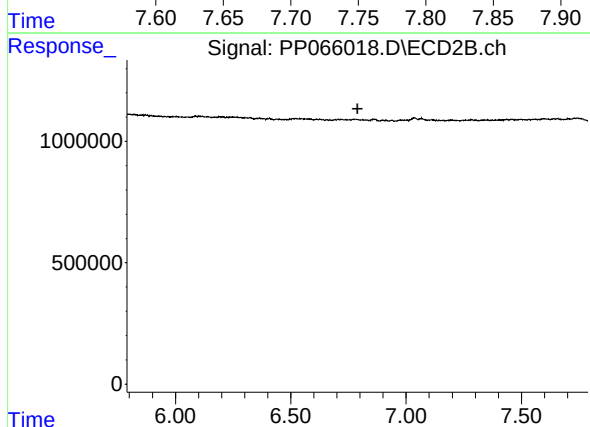


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 6.789 min
Response: 0
Conc: N.D.

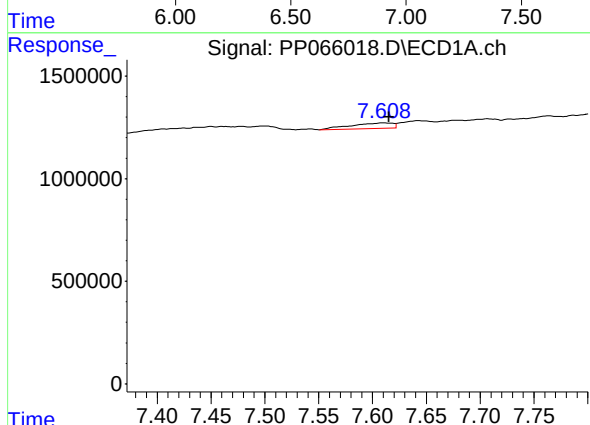


#31 AR-1260-1

R.T.: 7.609 min
Delta R.T.: -0.006 min
Response: 726341
Conc: 7.50 ng/ml

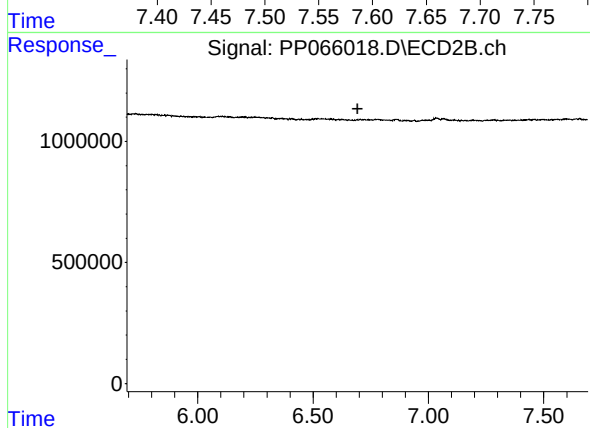

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

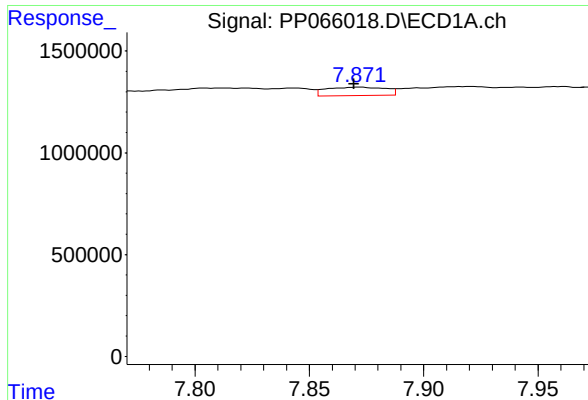

#32 AR-1260-2


R.T.: 7.872 min
Delta R.T.: 0.002 min
Response: 733354
Conc: 6.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0064-1-2

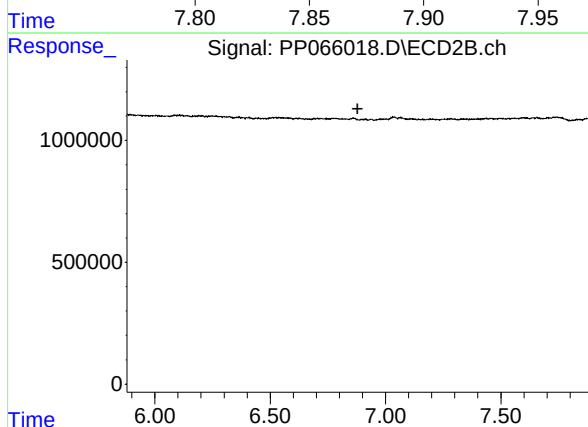


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.878 min
Response: 0
Conc: N.D.

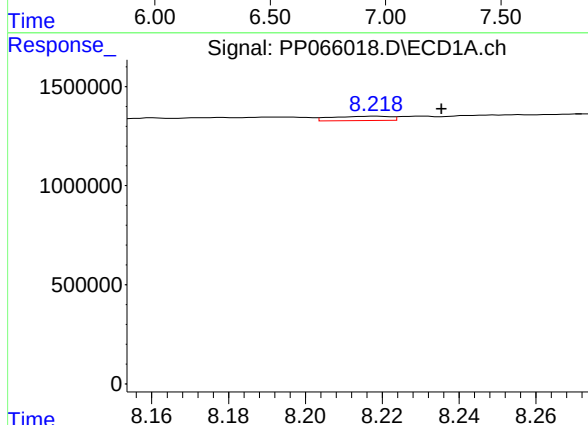


#33 AR-1260-3

R.T.: 8.218 min
Delta R.T.: -0.017 min
Response: 236859
Conc: 2.71 ng/ml

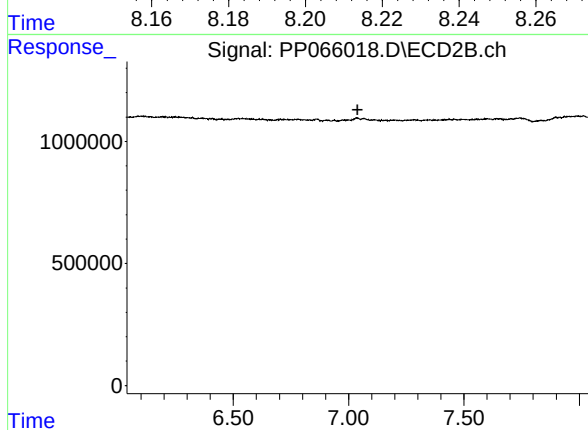

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.038 min
Response: 0
Conc: N.D.

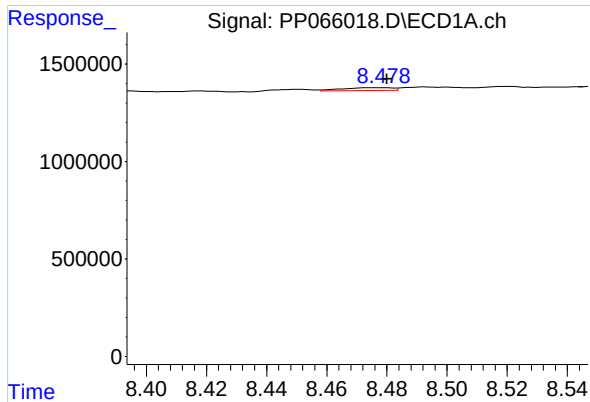

#34 AR-1260-4


R.T.: 8.478 min
Delta R.T.: -0.002 min
Response: 180439
Conc: 1.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0064-1-2

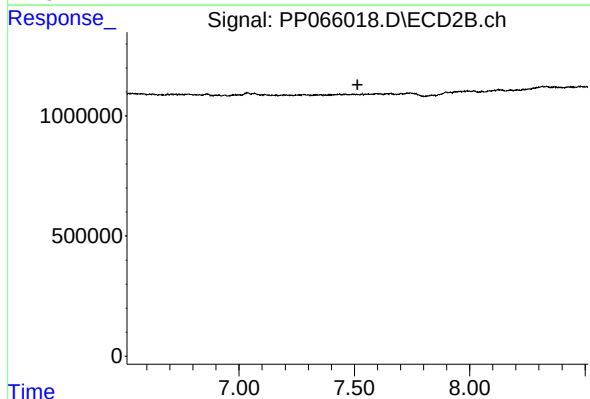


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.514 min
Response: 0
Conc: N.D.

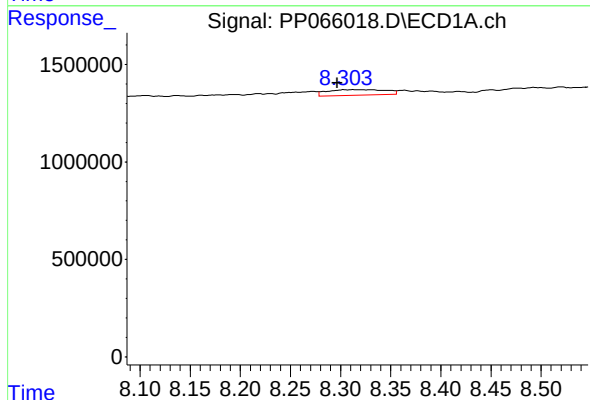

#36 AR-1262-1

R.T.: 8.304 min
Delta R.T.: 0.007 min
Response: 1180617
Conc: 22.04 ng/ml

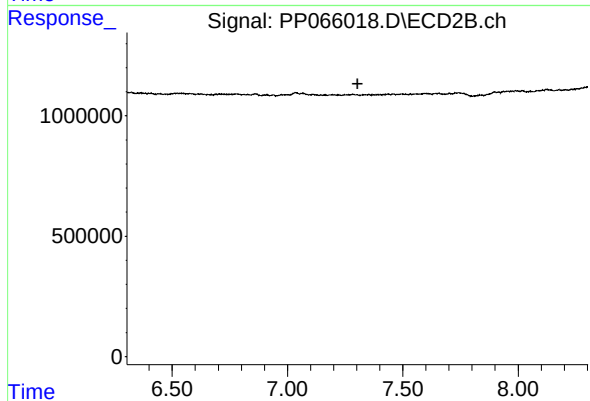

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.303 min
Response: 0
Conc: N.D.