

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062524\
 Data File : PP066029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2024 20:00
 Operator : YP\AJ
 Sample : P3048-07 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC288016-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2024
 Supervised By :Ankita Jodhani 06/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 00:49:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 05:25:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.826	4.065	2156039	3394590	1.137	1.216
2) SA Decachlor...	10.844	9.247	3449965	1933499	1.754	1.312m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062524\
Data File : PP066029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2024 20:00
Operator : YP\AJ
Sample : P3048-07 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC288016-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2024
Supervised By :Ankita Jodhani 06/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 00:49:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

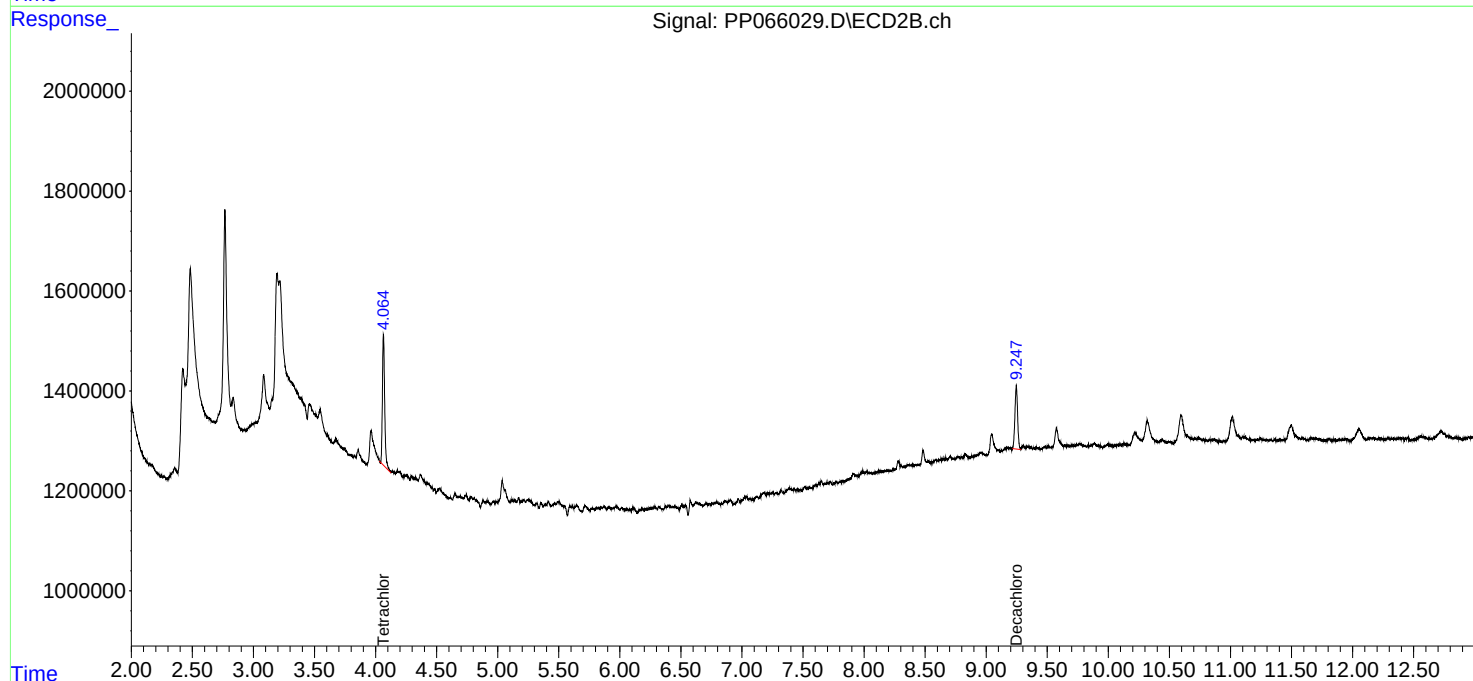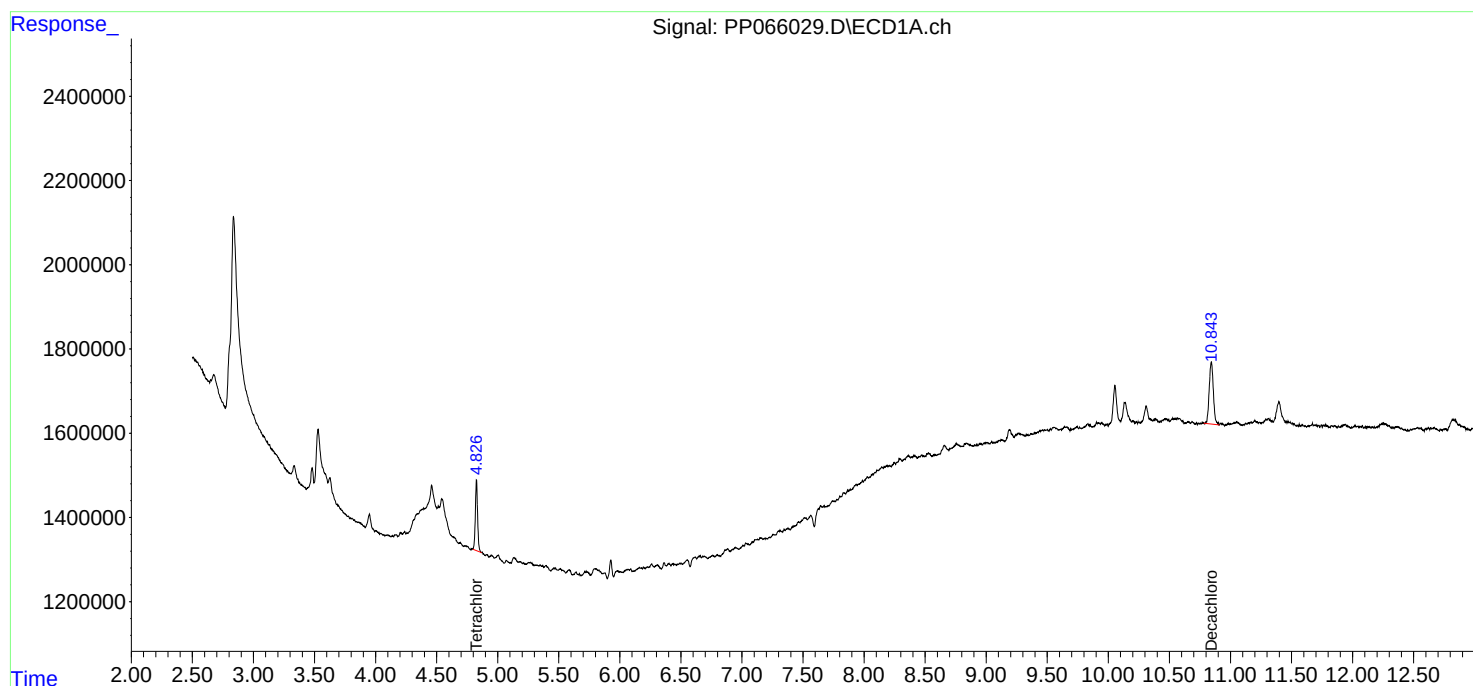

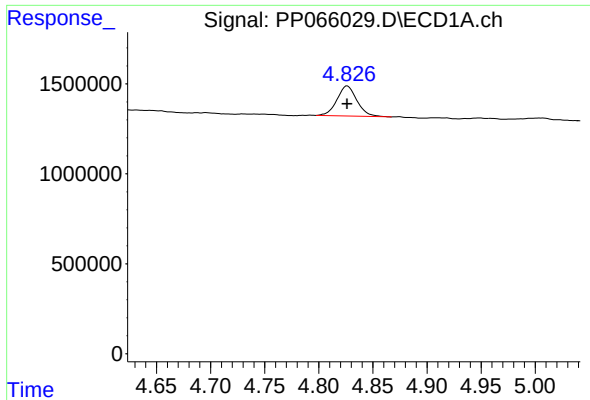


#1 Tetrachloro-m-xylene

R.T.: 4.826 min
Delta R.T.: 0.000 min
Response: 2156039
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC288016-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2024
Supervised By :Ankita Jodhani 06/26/2024

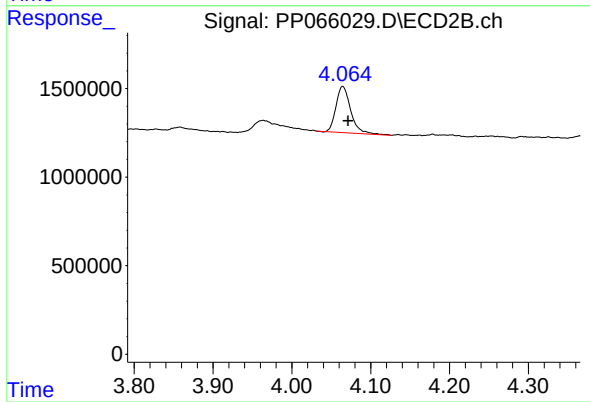


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.007 min
Response: 3394590
Conc: 1.22 ng/ml

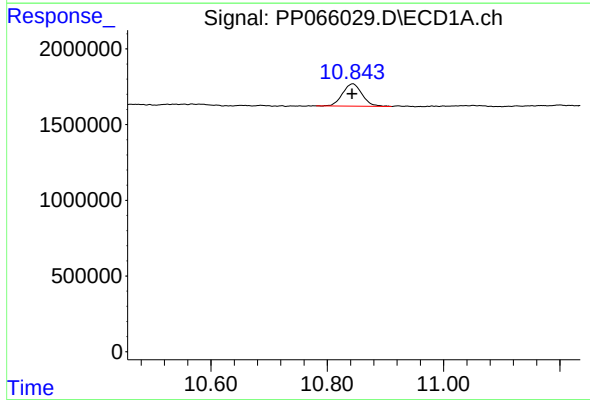

#2 Decachlorobiphenyl

R.T.: 10.844 min
Delta R.T.: 0.001 min
Response: 3449965
Conc: 1.75 ng/ml

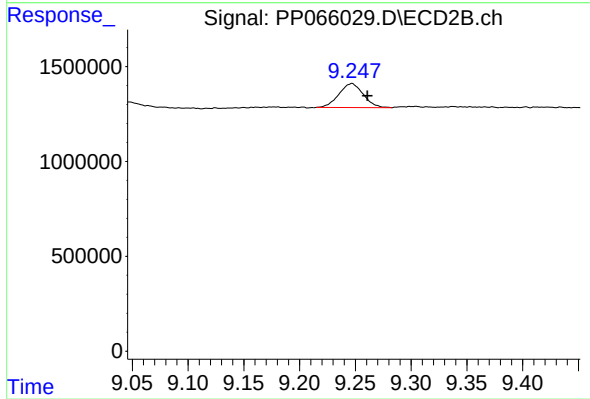

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: -0.014 min
Response: 1933499
Conc: 1.31 ng/ml m