

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062524\
 Data File : PP066030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2024 20:17
 Operator : YP\AJ
 Sample : P3048-08 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC288016-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2024
 Supervised By :Ankita Jodhani 06/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 00:50:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 05:25:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.826	4.065	2848636	4469227	1.502m	1.601
2) SA Decachlor...	10.845	9.248	3956852	2046600	2.012	1.389 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062524\
Data File : PP066030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2024 20:17
Operator : YP\AJ
Sample : P3048-08 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC288016-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2024
Supervised By :Ankita Jodhani 06/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 00:50:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

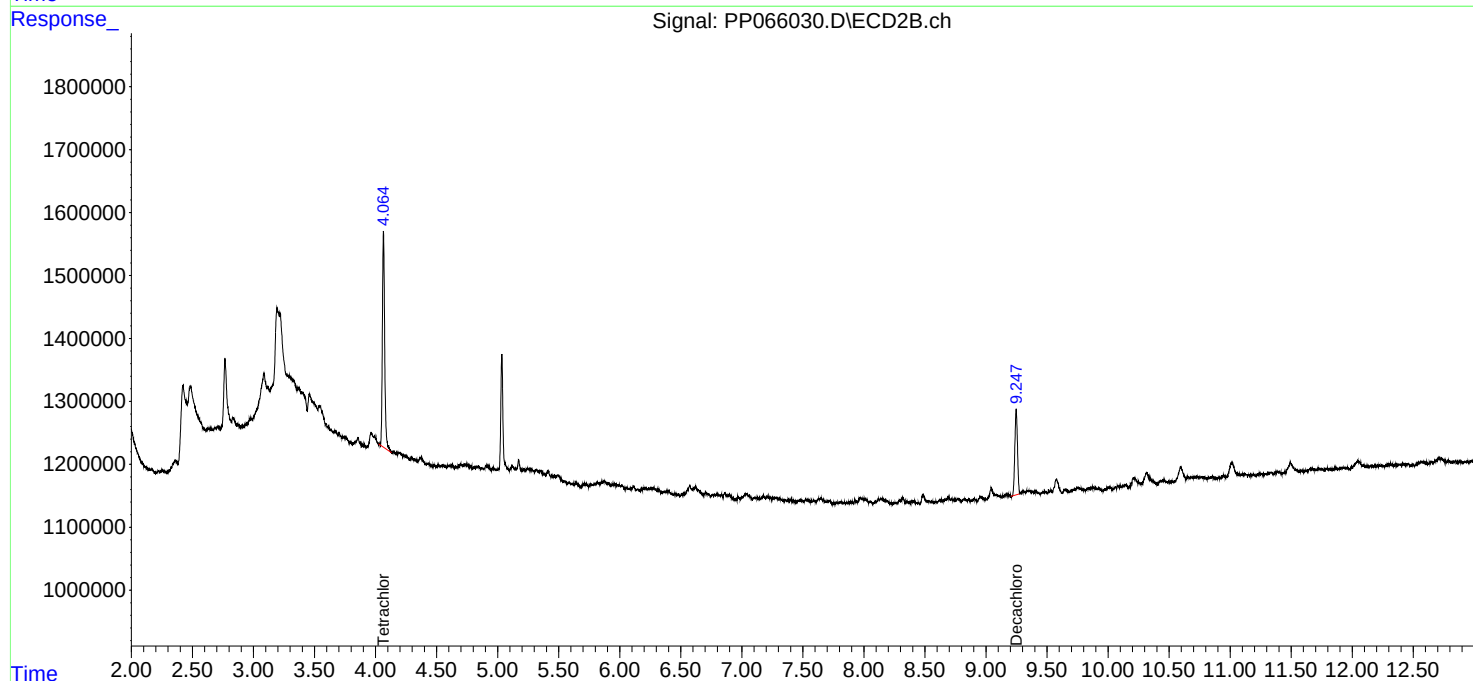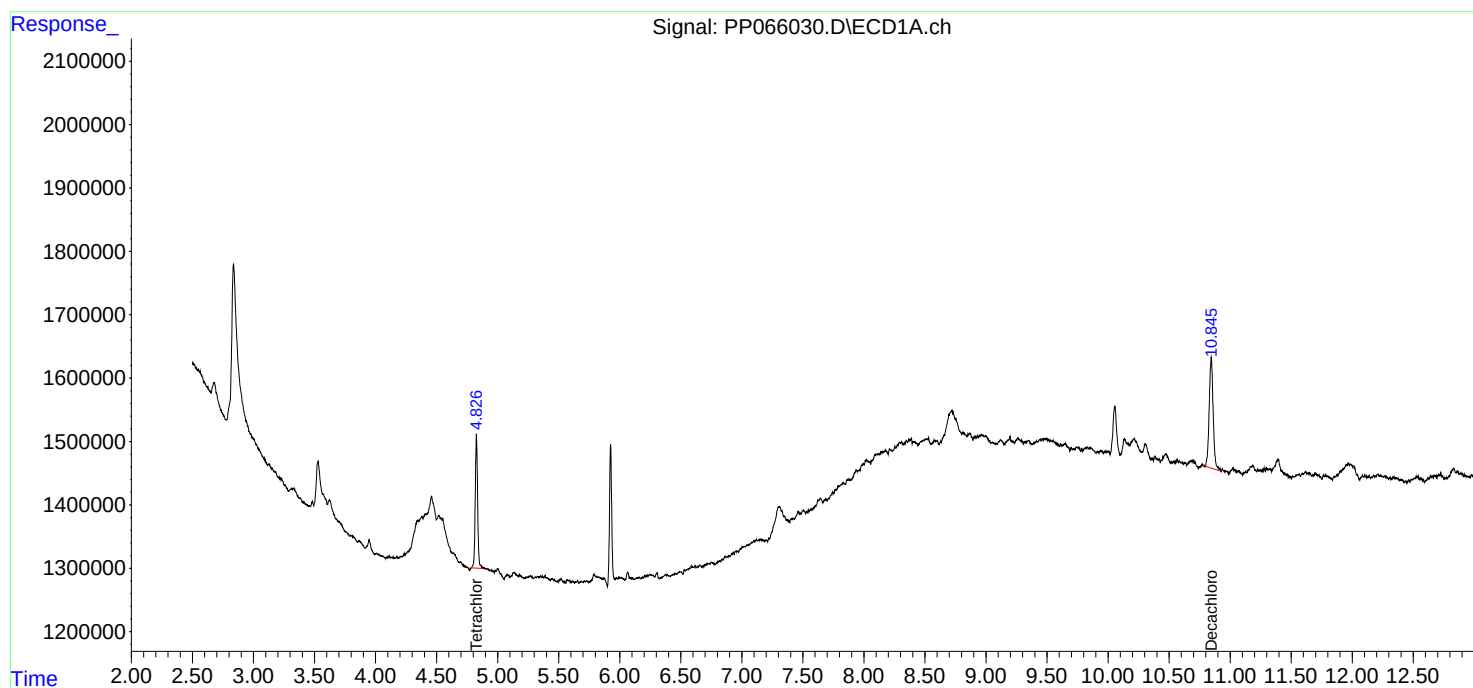

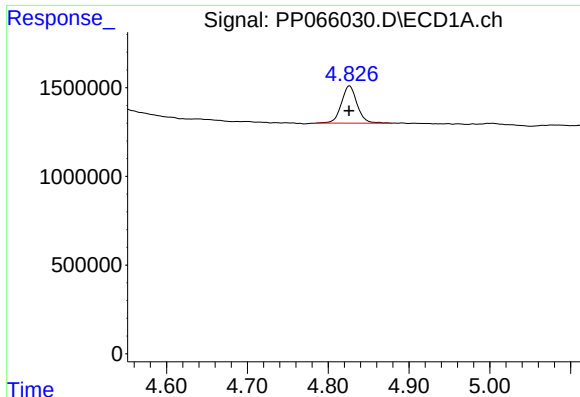


#1 Tetrachloro-m-xylene

R.T.: 4.826 min
Delta R.T.: 0.000 min
Response: 2848636
Conc: 1.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC288016-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2024
Supervised By :Ankita Jodhani 06/26/2024

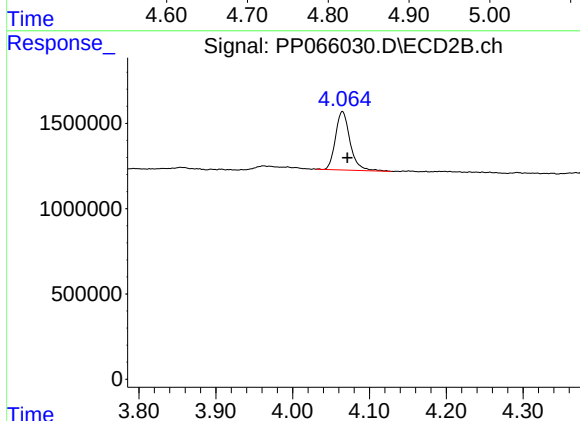


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.006 min
Response: 4469227
Conc: 1.60 ng/ml

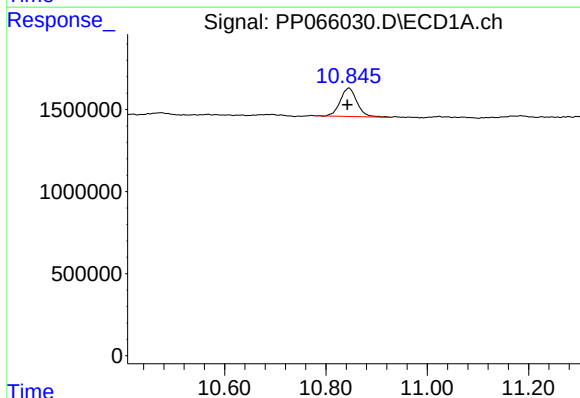

#2 Decachlorobiphenyl

R.T.: 10.845 min
Delta R.T.: 0.003 min
Response: 3956852
Conc: 2.01 ng/ml

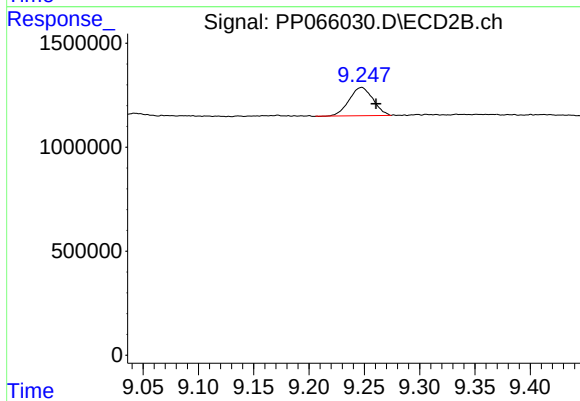

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.013 min
Response: 2046600
Conc: 1.39 ng/ml