

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062525\
 Data File : PP073235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2025 11:09
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 05:03:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30) L6 AR-1254-5	7.787	6.858	635.3E6	610.0E6	5560.384	4693.954



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062525\
Data File : PP073235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2025 11:09
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 05:03:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

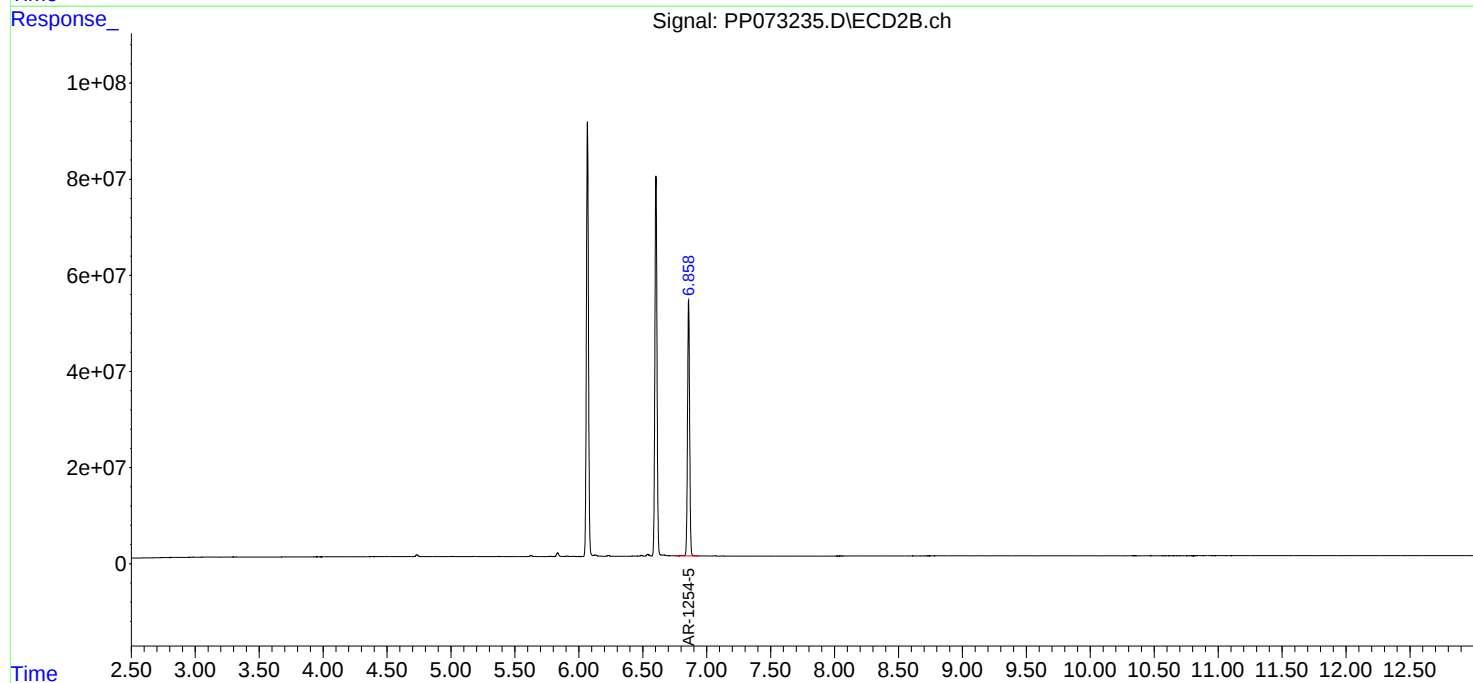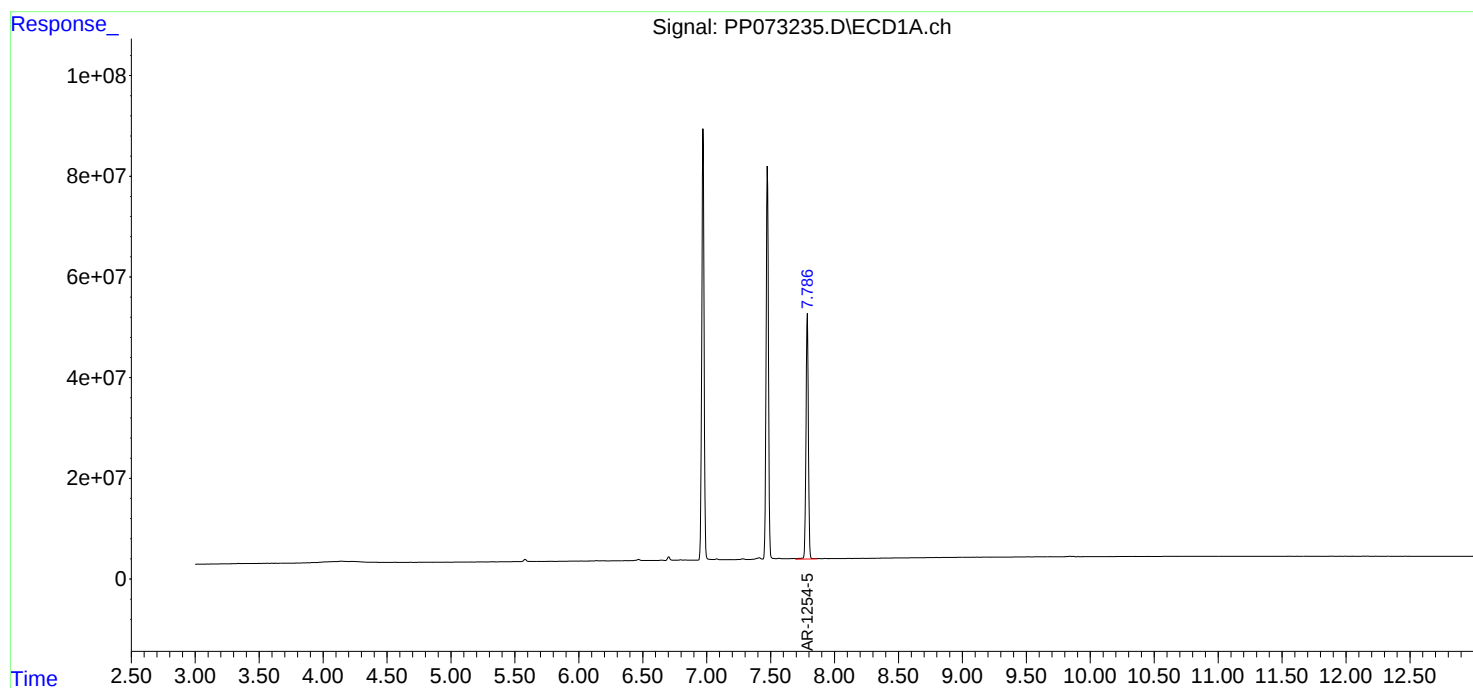


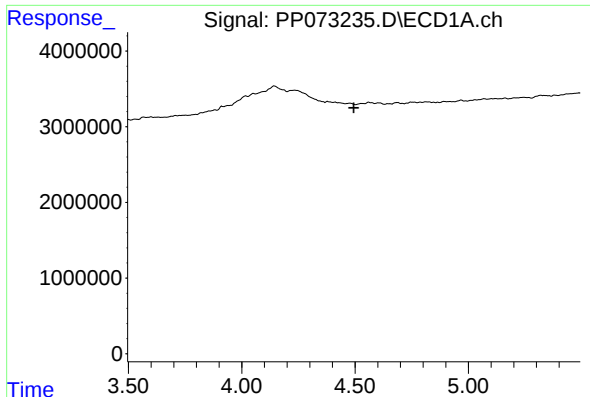

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

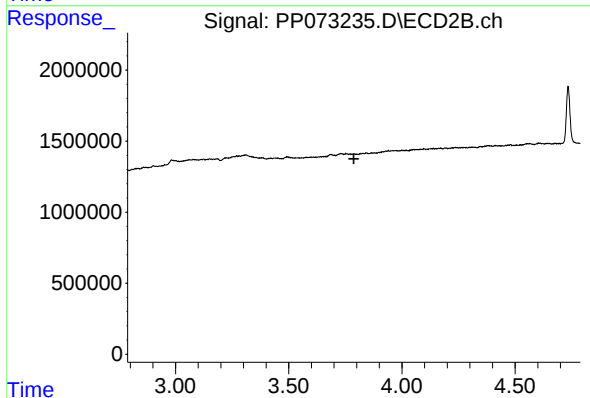


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.788 min
Response: 0
Conc: N.D.

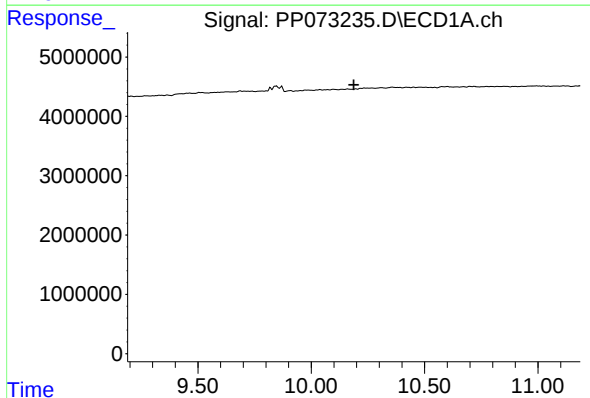


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.187 min
Response: 0
Conc: N.D.

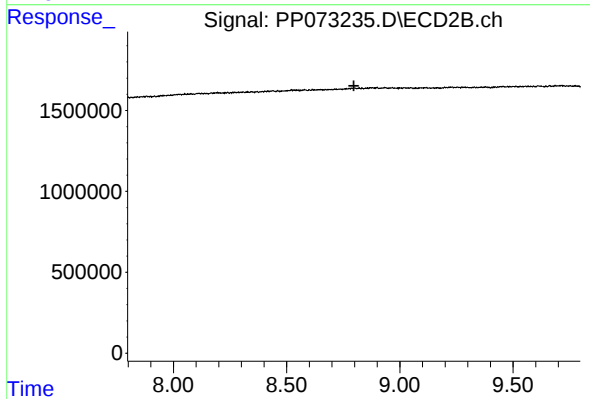

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.797 min
Response: 0
Conc: N.D.

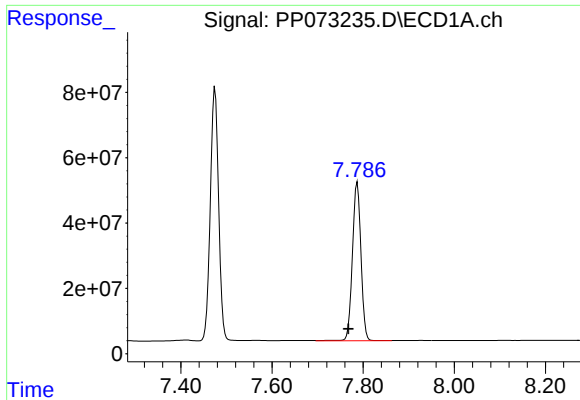

#30 AR-1254-5

R.T.: 7.787 min
Delta R.T.: 0.019 min
Response: 635309836
Conc: 5560.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

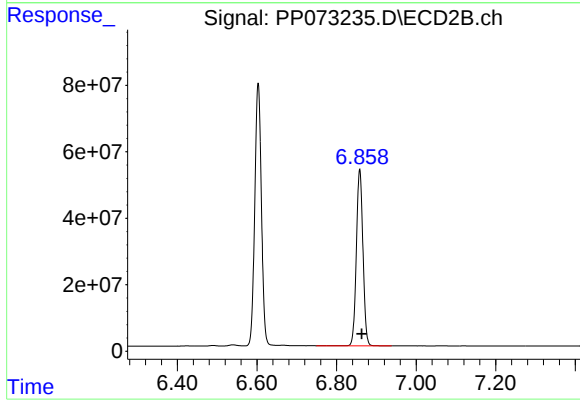

#30 AR-1254-5

R.T.: 6.858 min
Delta R.T.: -0.005 min
Response: 610038774
Conc: 4693.95 ng/ml