

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062525\
 Data File : PP073255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2025 18:43
 Operator : YP\AJ
 Sample : Q2412-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-05-062425

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2025
 Supervised By :mohammad ahmed 06/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:52:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.786	30735554	32318593	14.561m	17.937
2) SA Decachlor...	10.183	8.792	30450970	25599500	17.819	19.180

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062525\
Data File : PP073255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2025 18:43
Operator : YP\AJ
Sample : Q2412-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-05-062425


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2025
Supervised By :mohammad ahmed 06/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:52:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

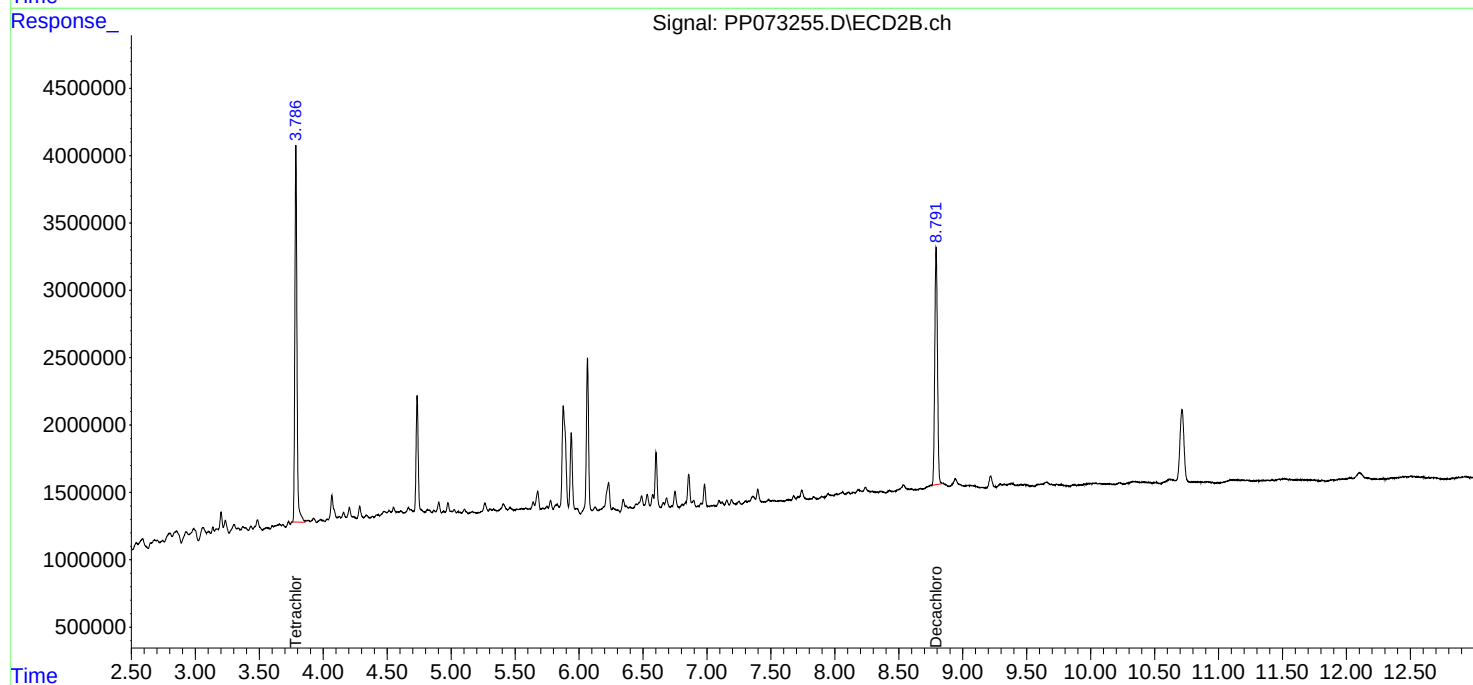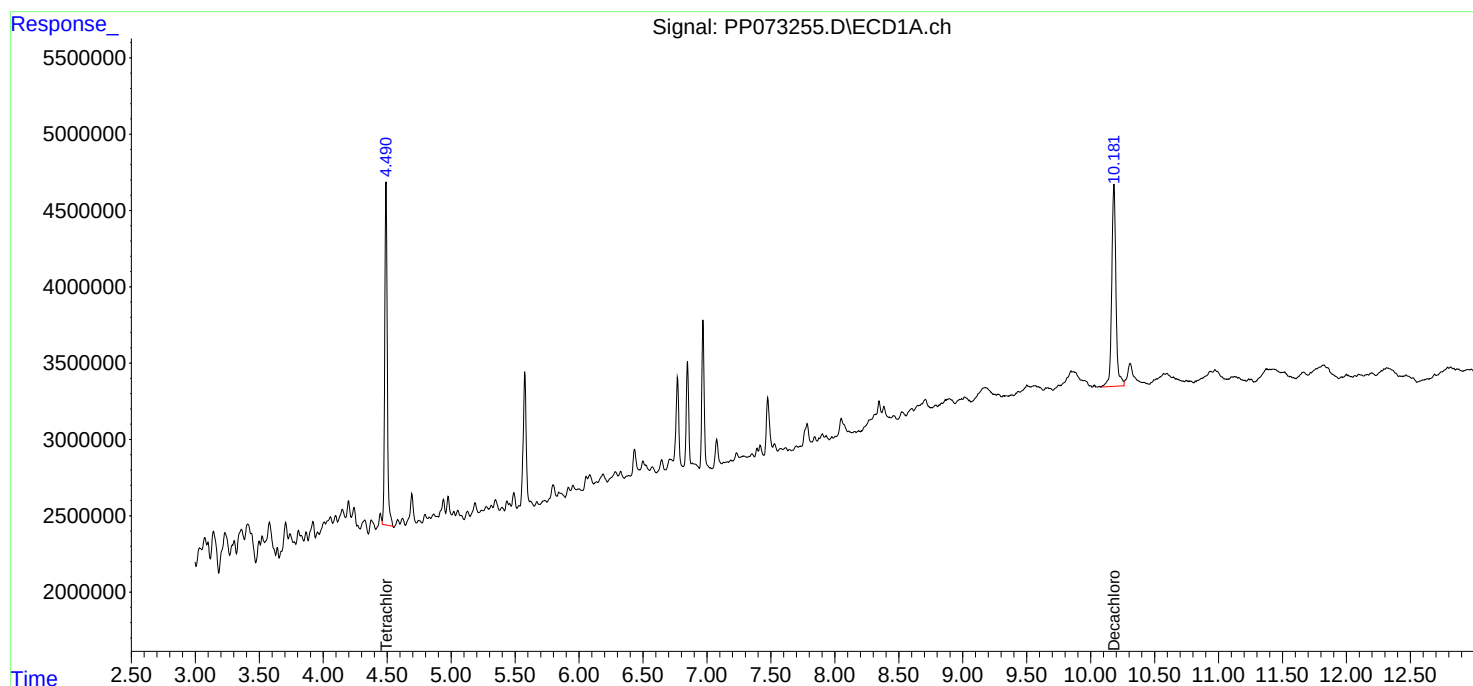

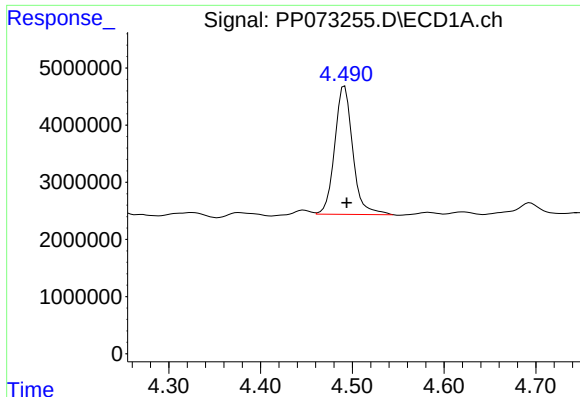


#1 Tetrachloro-m-xylene

R.T.: 4.490 min
Delta R.T.: -0.004 min
Response: 30735554
Conc: 14.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-05-062425


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2025
Supervised By :mohammad ahmed 06/27/2025

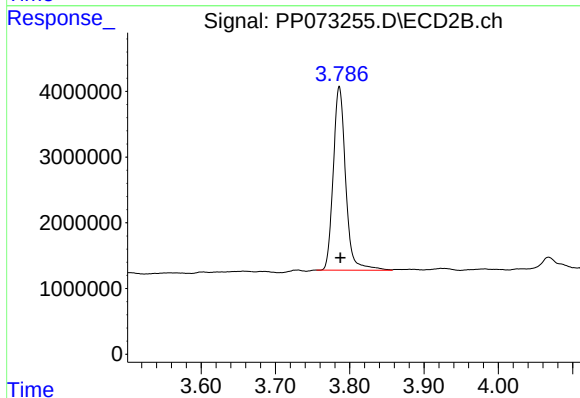


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: -0.002 min
Response: 32318593
Conc: 17.94 ng/ml

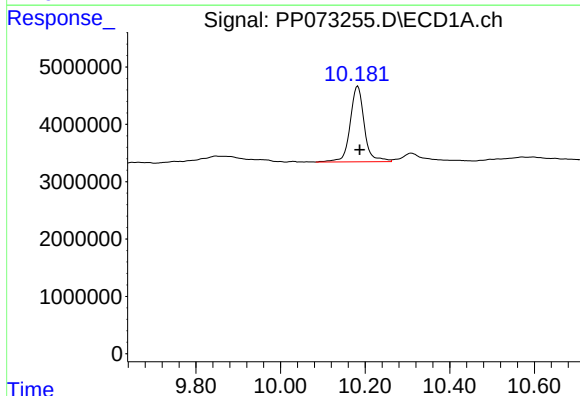

#2 Decachlorobiphenyl

R.T.: 10.183 min
Delta R.T.: -0.005 min
Response: 30450970
Conc: 17.82 ng/ml

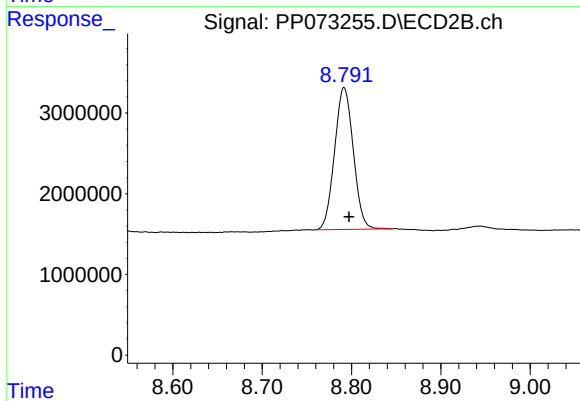

#2 Decachlorobiphenyl

R.T.: 8.792 min
Delta R.T.: -0.005 min
Response: 25599500
Conc: 19.18 ng/ml