

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD P\Data\PP062618\
 Data File : PP026653.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2018 9:40
 Operator : UA/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 03:31:05 2018
 Quant Method : Z:\bestpcbsrv\HPCHEM1\ECD_P\methods\PP062518.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 26 06:52:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.453	12.232	248.9E6	157.7E6	501.927	460.640
Target Compounds							
5) T	DICAMBA	0.000	12.521	0	3858107	N.D.	3.021 #
7) T	MCPA	0.000	13.033	0	71356141	N.D.	48.745 #
8) T	DICHLORPROP	12.895	0.000	9042396	0	16.999	N.D. #
12) T	2,4,5-T	0.000	15.893	0	4870249	N.D.	2.743 #
15) T	Picloram	16.934	18.215	14392861	8340257	3.163	2.992



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD P\Data\PP062618\
Data File : PP026653.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 9:40
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 03:31:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062518.M
Quant Title : 8080.M
QLast Update : Tue Jun 26 06:52:58 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

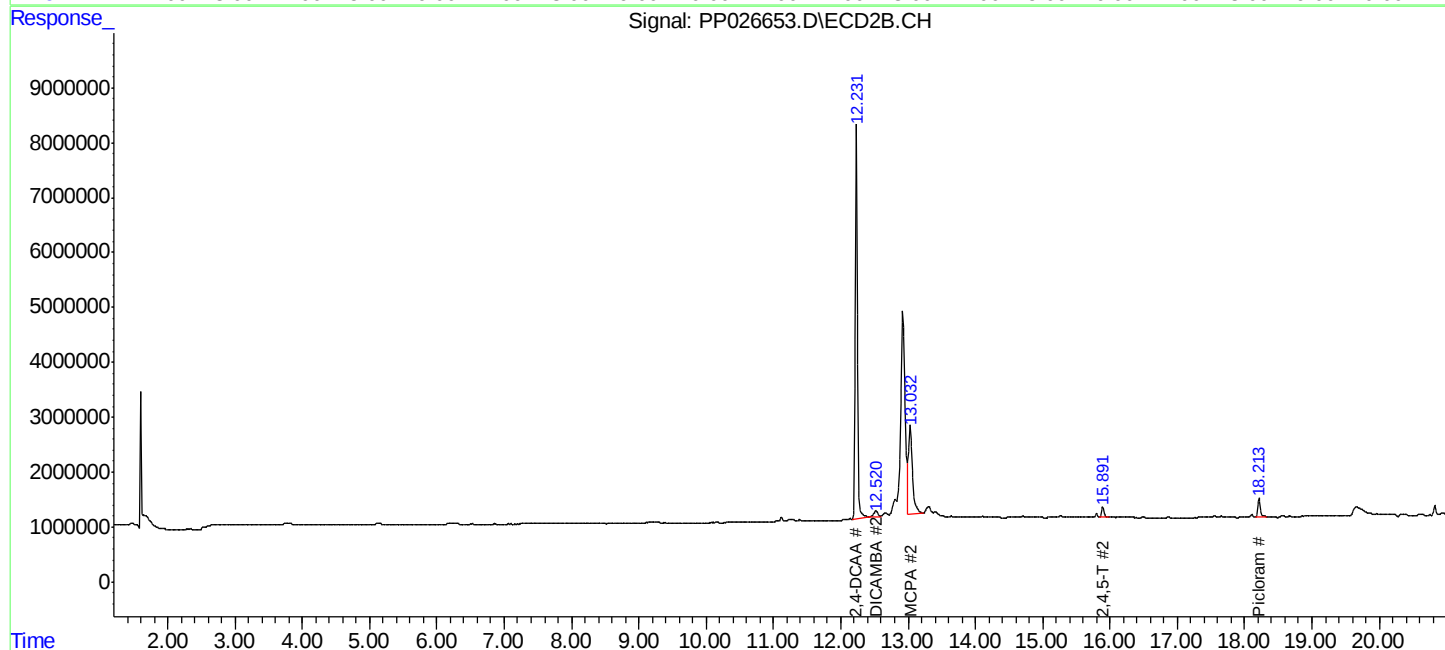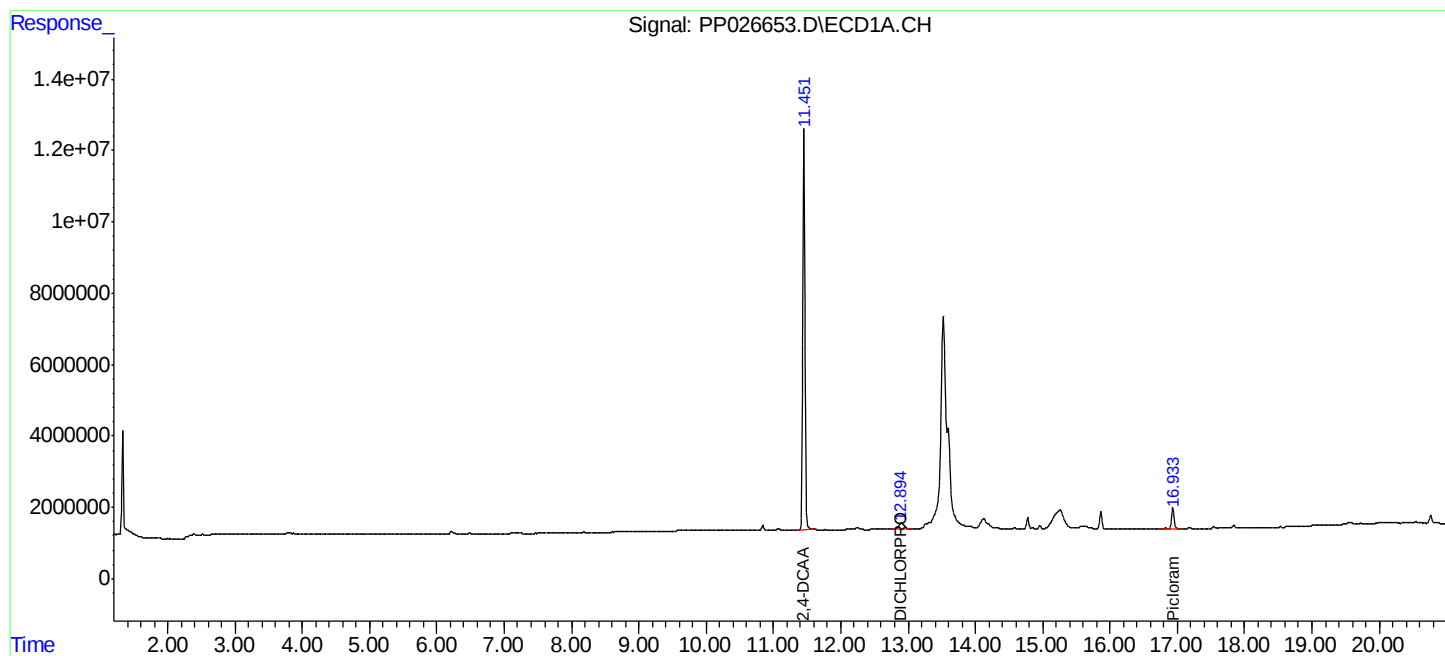


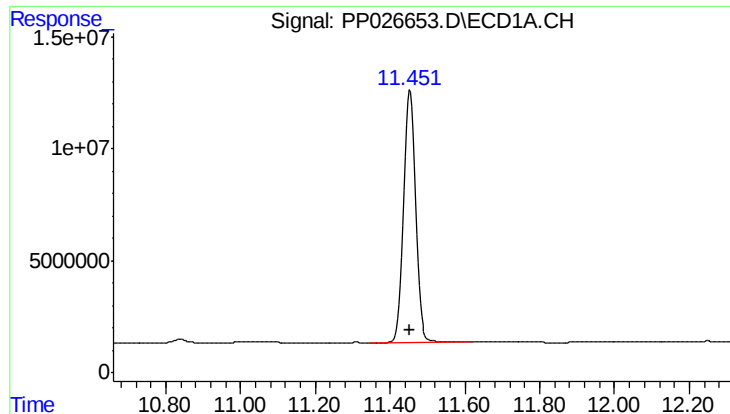

#4 2,4-DCAA


R.T.: 11.453 min
Delta R.T.: -0.001 min
Response: 248890365
Conc: 501.93 ng/ml

Instrument :
ECD_P
ClientSampleId :

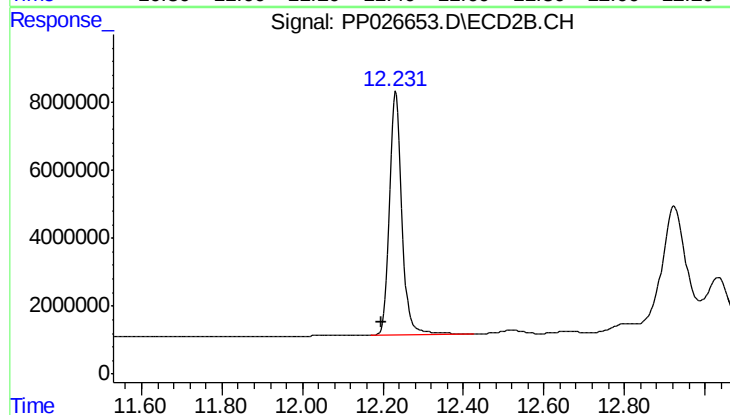


#4 2,4-DCAA

R.T.: 12.232 min
Delta R.T.: 0.034 min
Response: 157738552
Conc: 460.64 ng/ml

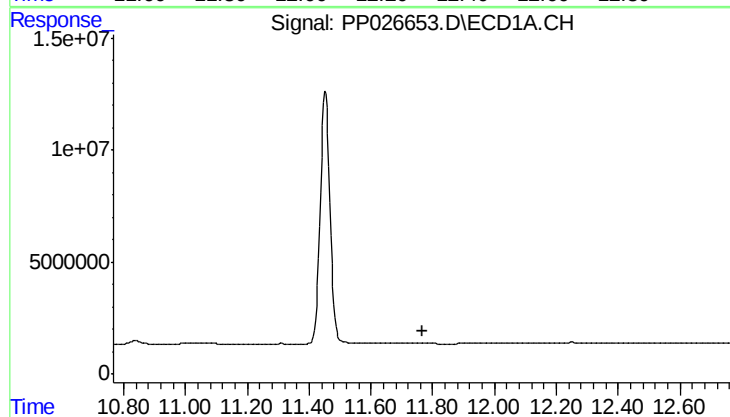


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.766 min
Response: 0
Conc: N.D.

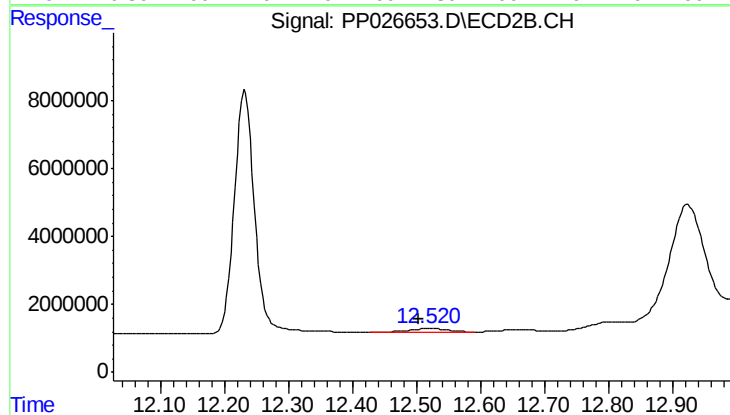

#5 DICAMBA


R.T.: 12.521 min
Delta R.T.: 0.018 min
Response: 3858107
Conc: 3.02 ng/ml

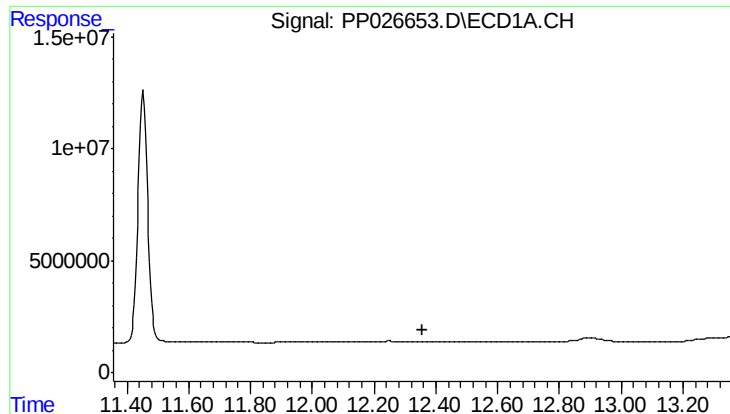

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.356 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

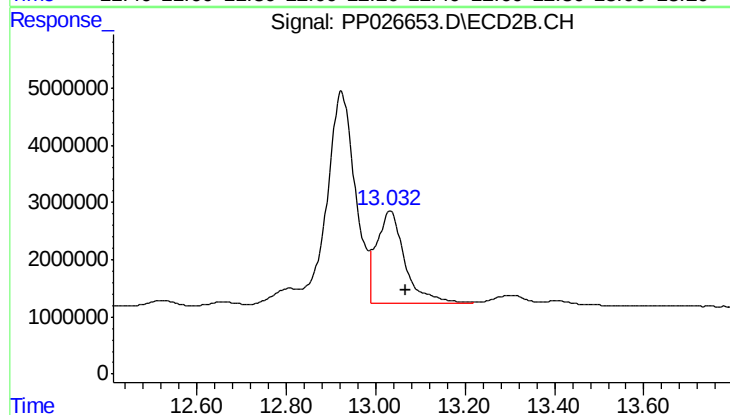


#7 MCPA

R.T.: 13.033 min
Delta R.T.: -0.035 min
Response: 71356141
Conc: 48.74 ug/ml

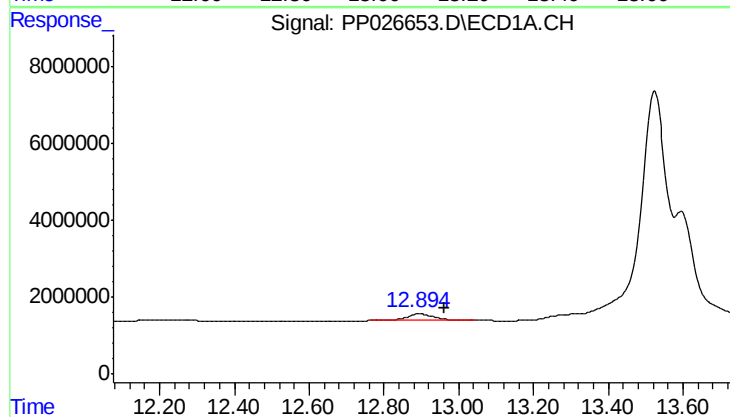


#8 DICHLORPROP

R.T.: 12.895 min
Delta R.T.: -0.066 min
Response: 9042396
Conc: 17.00 ng/ml

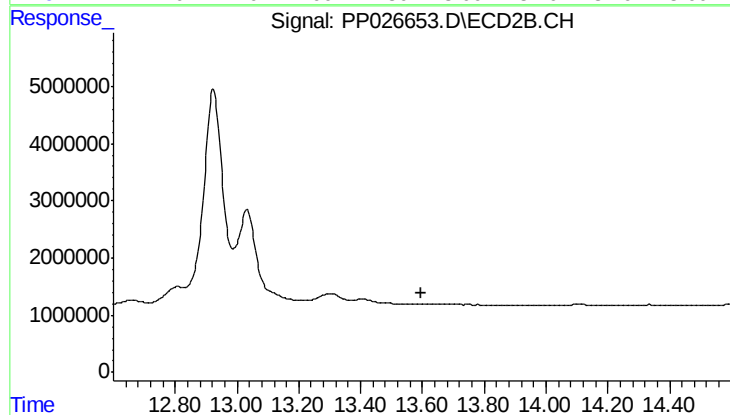

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.597 min
Response: 0
Conc: N.D.

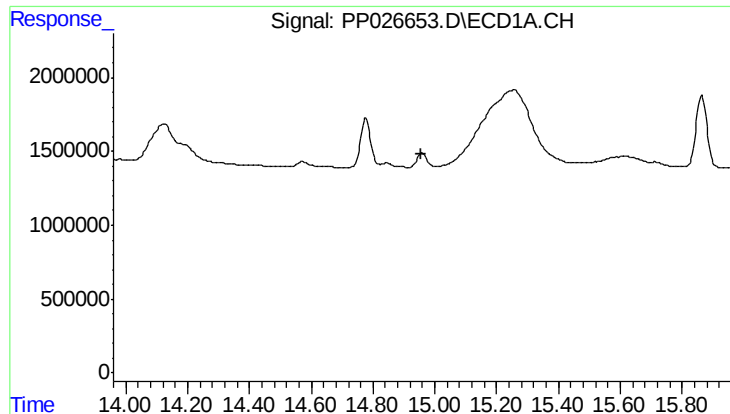

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

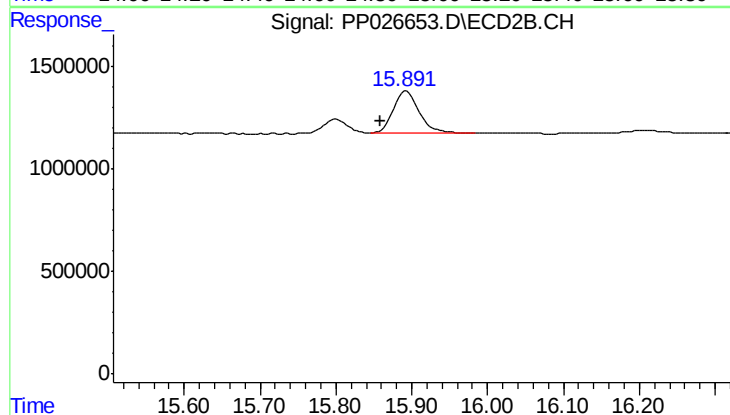


#12 2,4,5-T

R.T.: 15.893 min
Delta R.T.: 0.034 min
Response: 4870249
Conc: 2.74 ng/ml

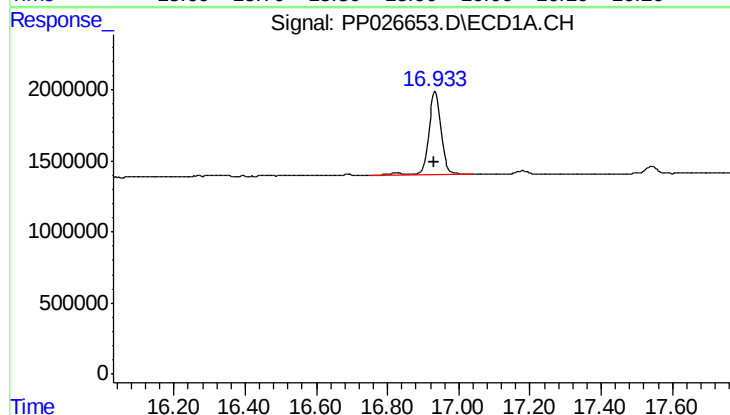

#15 Picloram

R.T.: 16.934 min
Delta R.T.: 0.002 min
Response: 14392861
Conc: 3.16 ng/ml

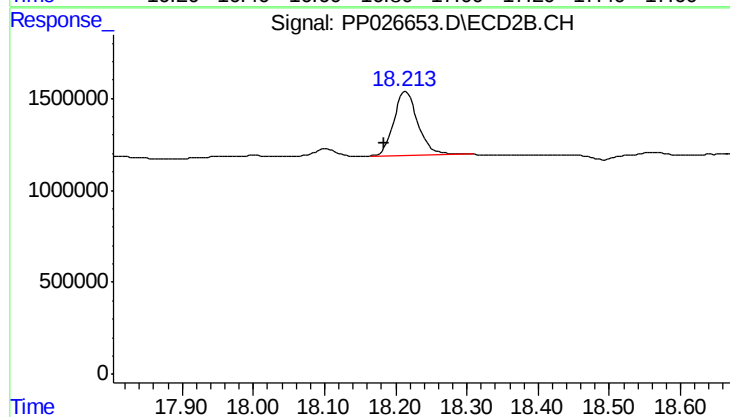

#15 Picloram

R.T.: 18.215 min
Delta R.T.: 0.031 min
Response: 8340257
Conc: 2.99 ng/ml