

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062725\
 Data File : PP073321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2025 10:51
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 11:20:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.466f	3.785	95906	97425	0.045	0.054
2)	SA Decachlor...	10.176	8.785	329031	204676	0.193	0.153
Target Compounds							
3)	L1 AR-1016-1	5.665	4.864	242534	566855	3.337	8.249 #
4)	L1 AR-1016-2	5.665	4.864	242534	566855	2.332	5.633 #
5)	L1 AR-1016-3	5.716	5.102f	172330	300952	2.637	5.500 #
6)	L1 AR-1016-4	5.833	5.102	196339	300952	3.755	6.755 #
7)	L1 AR-1016-5	6.132	5.307	805417	3467021	16.107	62.715 #
8)	L2 AR-1221-1	4.705	4.000	267981	111396	10.867	4.145 #
9)	L2 AR-1221-2	4.784	4.094	163044	267183	8.080	13.236 #
10)	L2 AR-1221-3	4.849	4.162	287700	257297	4.674	4.381
11)	L3 AR-1232-1	4.849	4.162	287700	257297	6.127	5.647
12)	L3 AR-1232-2	5.412	4.864	187108	566855	8.364	12.254 #
13)	L3 AR-1232-3	5.665	5.102f	242534	300952	4.700	12.255 #
14)	L3 AR-1232-4	5.833	5.127	196339	107486	7.607	4.970 #
15)	L3 AR-1232-5	5.919	5.307	609904	3467021	17.098	151.671 #
16)	L4 AR-1242-1	5.665	4.864	242534	566855	4.150	10.266 #
17)	L4 AR-1242-2	5.665	4.864	242534	566855	2.802	7.131 #
18)	L4 AR-1242-3	5.716	5.102f	172330	300952	3.270	6.950 #
19)	L4 AR-1242-4	5.833	5.127	196339	107486	4.466	2.590 #
20)	L4 AR-1242-5	6.542	5.651	1903498	1454495	38.408	27.659 #
21)	L5 AR-1248-1	5.665	4.864	242534	566855	5.099	13.004 #
22)	L5 AR-1248-2	5.919	5.102	609904	300952	10.417	5.136 #
23)	L5 AR-1248-3	6.132	5.127	805417	107486	12.344	1.775 #
24)	L5 AR-1248-4	6.542	5.307	1903498	3467021	22.377	49.513 #
25)	L5 AR-1248-5	6.542	5.685	1903498	9093279	22.744	128.017 #
26)	L6 AR-1254-1	6.482	5.685	7916358	9093279	94.048	82.930
27)	L6 AR-1254-2	6.695	5.829	9237471	9777748	73.664	103.418 #
28)	L6 AR-1254-3	7.062	6.228	23563609	4955407	179.586	33.585 #
29)	L6 AR-1254-4	7.320	6.454	1658470	554299	13.846	5.708 #
30)	L6 AR-1254-5	7.779	6.853	614.7E6	593.2E6	5380.062	4564.186
31)	L7 AR-1260-1	7.232	6.342	2657004	720324	30.120	7.604 #
32)	L7 AR-1260-2	7.467	6.513	996.6E6	16143797	7334.134	138.649 #
33)	L7 AR-1260-3	7.868	6.661	1712989	573773	15.006	5.509 #
34)	L7 AR-1260-4	8.065	7.114f	566719	284022	5.500	3.237 #
35)	L7 AR-1260-5	8.387	7.397	228325	72504	0.949	0.340 #
36)	L8 AR-1262-1	8.065	6.853f	566719	593.2E6	3.829	4105.951 #
37)	L8 AR-1262-2	8.387	7.114f	228325	284022	0.721	2.324 #
38)	L8 AR-1262-3	8.709	7.703	195977	5338629	0.916	47.369 #
39)	L8 AR-1262-4	8.796	7.703f	160032	5338629	1.015	29.116 #
40)	L8 AR-1262-5	9.441	8.234	190872	108119	1.706	1.249 #
41)	L9 AR-1268-1	8.709	7.703	195977	5338629	0.548	18.584 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062725\
 Data File : PP073321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2025 10:51
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 11:20:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.796	7.703f	160032	5338629	0.525	20.763 #
43) L9	AR-1268-3	9.027	7.953	352718	53906	1.328	0.250 #
44) L9	AR-1268-4	9.441	8.234	190872	108119	1.631	1.148 #
45) L9	AR-1268-5	9.827	8.530	187074	103678	0.253	0.179 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062725\
Data File : PP073321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2025 10:51
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 11:20:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

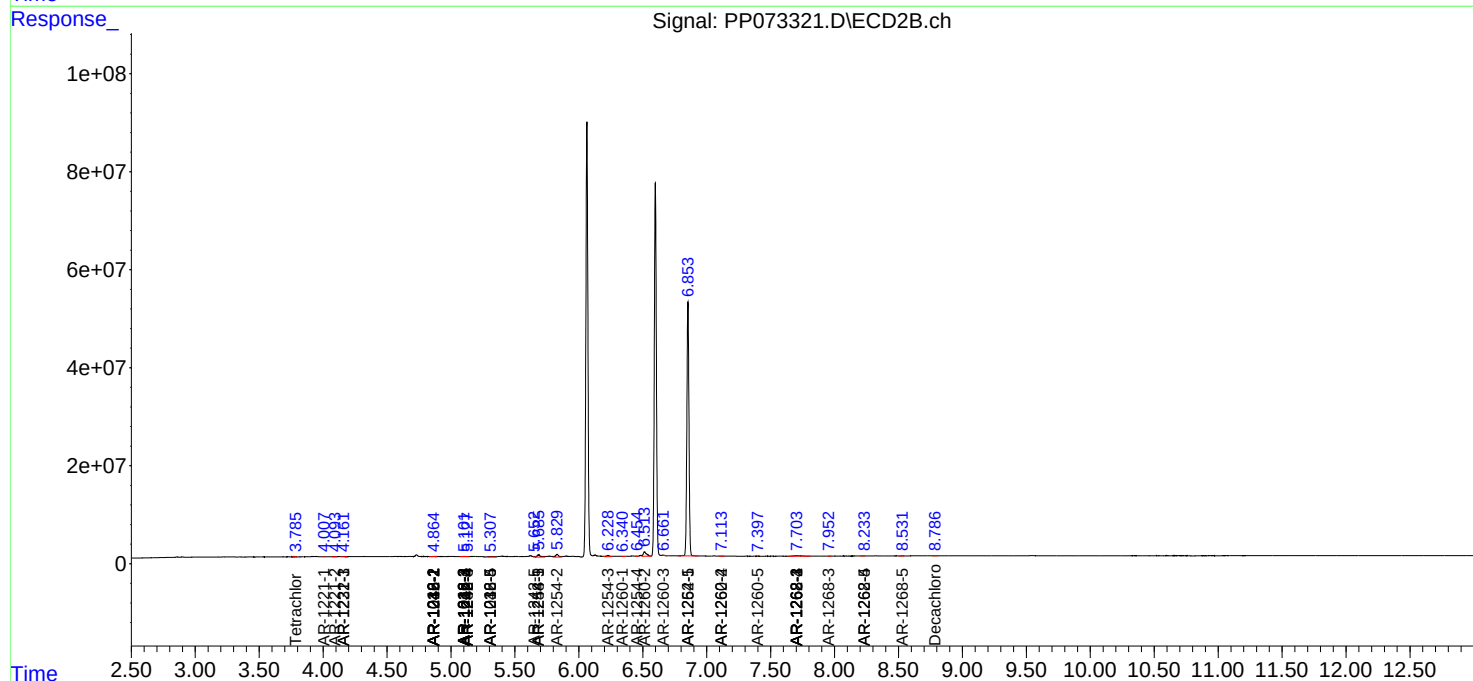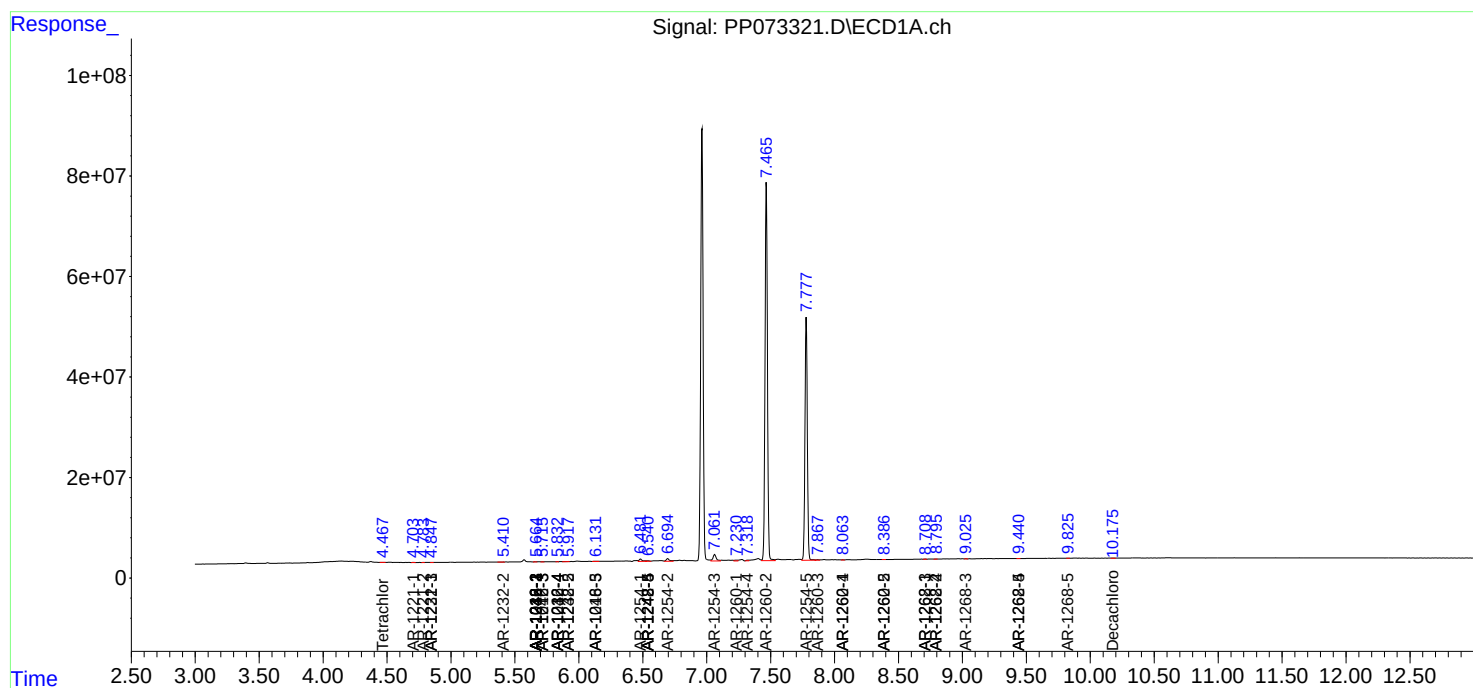


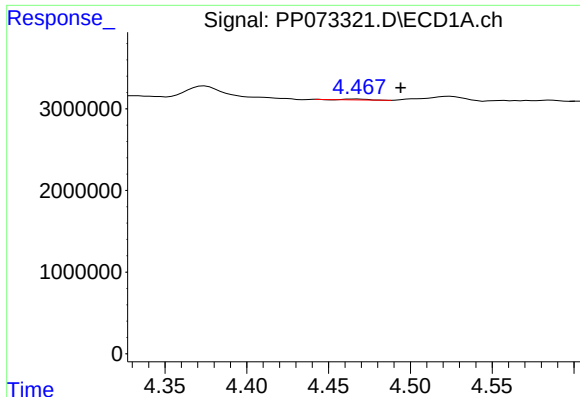

#1 Tetrachloro-m-xylene


R.T.: 4.466 min
Delta R.T.: -0.028 min
Response: 95906
Conc: 0.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

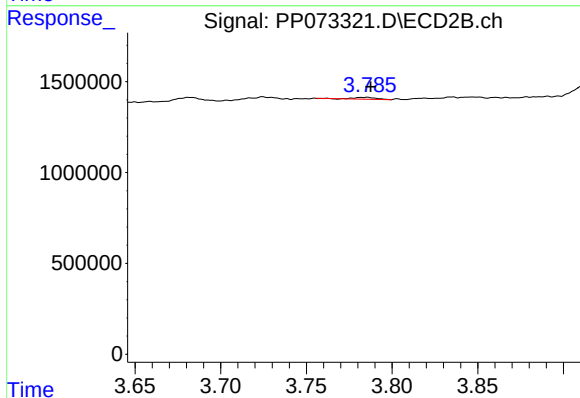


#1 Tetrachloro-m-xylene

R.T.: 3.785 min
Delta R.T.: -0.002 min
Response: 97425
Conc: 0.05 ng/ml

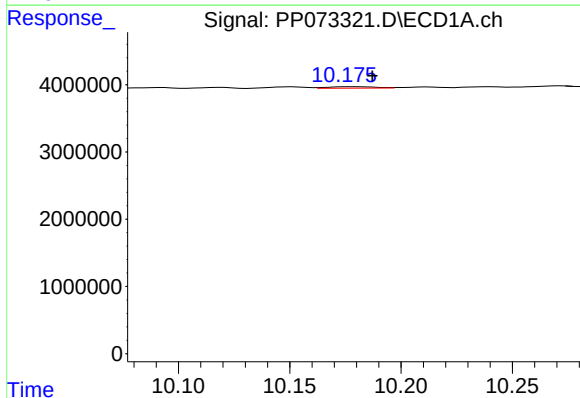


#2 Decachlorobiphenyl

R.T.: 10.176 min
Delta R.T.: -0.011 min
Response: 329031
Conc: 0.19 ng/ml

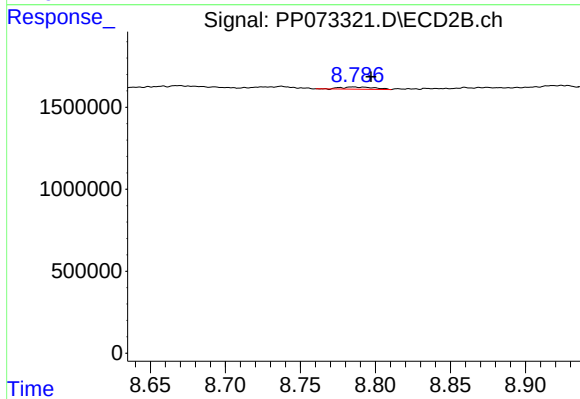

#2 Decachlorobiphenyl


R.T.: 8.785 min
Delta R.T.: -0.012 min
Response: 204676
Conc: 0.15 ng/ml

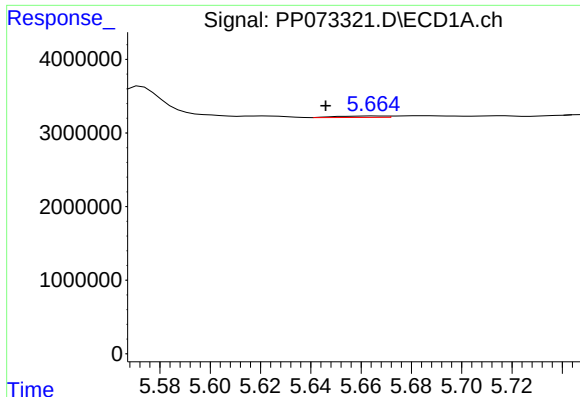

#3 AR-1016-1


R.T.: 5.665 min
Delta R.T.: 0.019 min
Response: 242534
Conc: 3.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

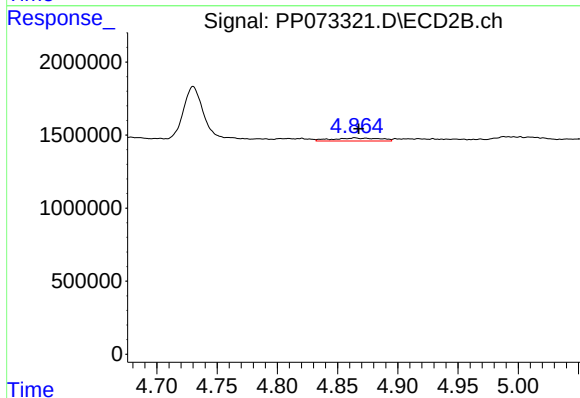


#3 AR-1016-1

R.T.: 4.864 min
Delta R.T.: -0.003 min
Response: 566855
Conc: 8.25 ng/ml

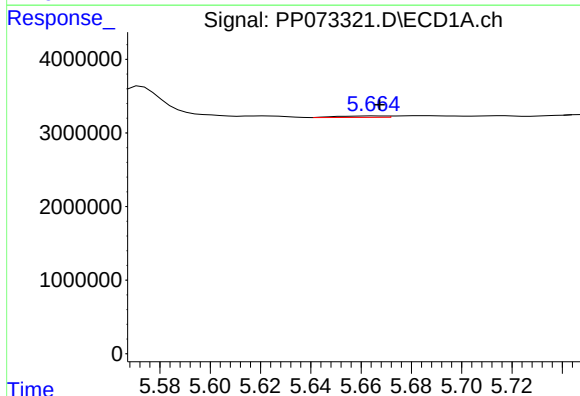


#4 AR-1016-2

R.T.: 5.665 min
Delta R.T.: -0.002 min
Response: 242534
Conc: 2.33 ng/ml

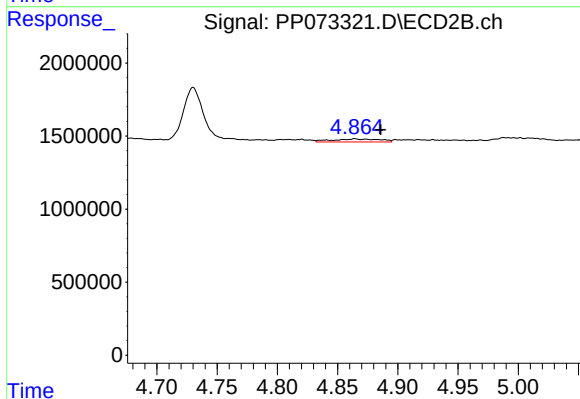

#4 AR-1016-2


R.T.: 4.864 min
Delta R.T.: -0.021 min
Response: 566855
Conc: 5.63 ng/ml

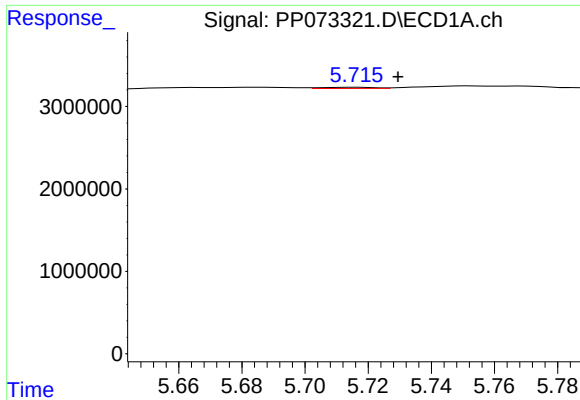

#5 AR-1016-3


R.T.: 5.716 min
Delta R.T.: -0.013 min
Response: 172330
Conc: 2.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

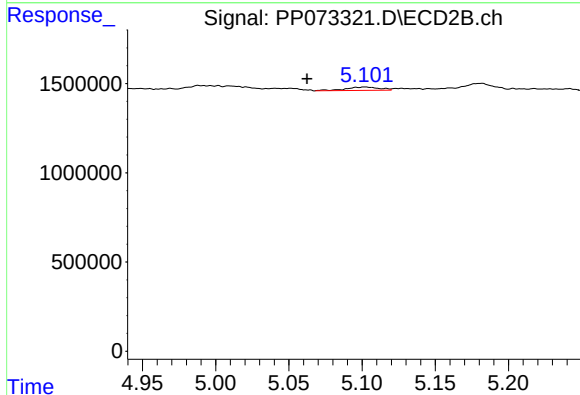


#5 AR-1016-3

R.T.: 5.102 min
Delta R.T.: 0.040 min
Response: 300952
Conc: 5.50 ng/ml

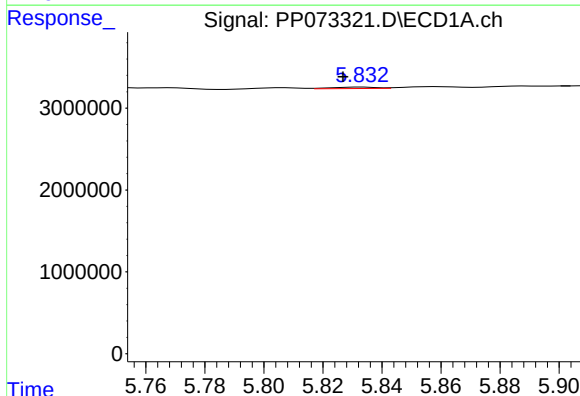


#6 AR-1016-4

R.T.: 5.833 min
Delta R.T.: 0.007 min
Response: 196339
Conc: 3.76 ng/ml

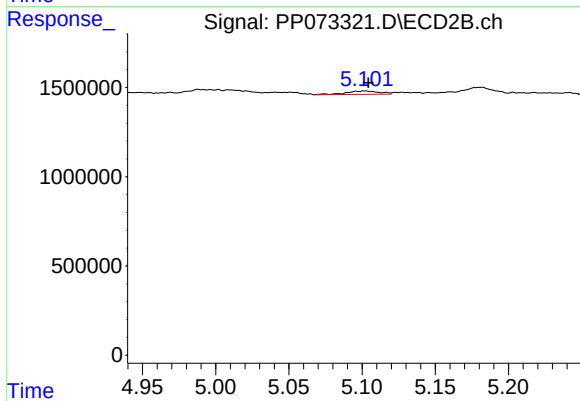

#6 AR-1016-4


R.T.: 5.102 min
Delta R.T.: -0.002 min
Response: 300952
Conc: 6.76 ng/ml

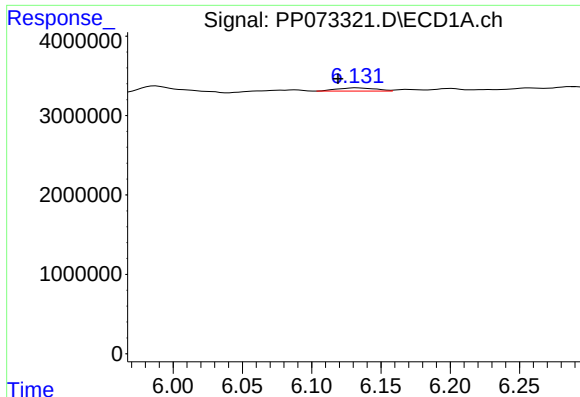

#7 AR-1016-5


R.T.: 6.132 min
Delta R.T.: 0.013 min
Response: 805417
Conc: 16.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

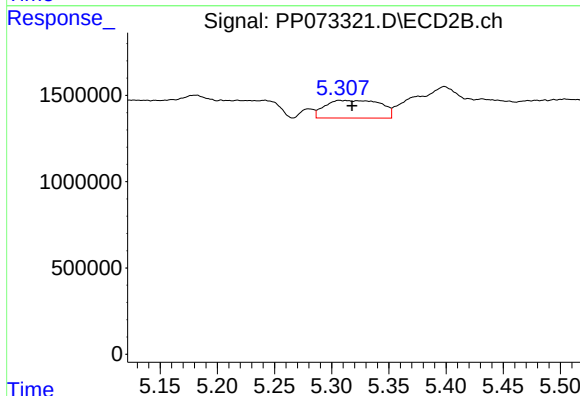


#7 AR-1016-5

R.T.: 5.307 min
Delta R.T.: -0.011 min
Response: 3467021
Conc: 62.71 ng/ml

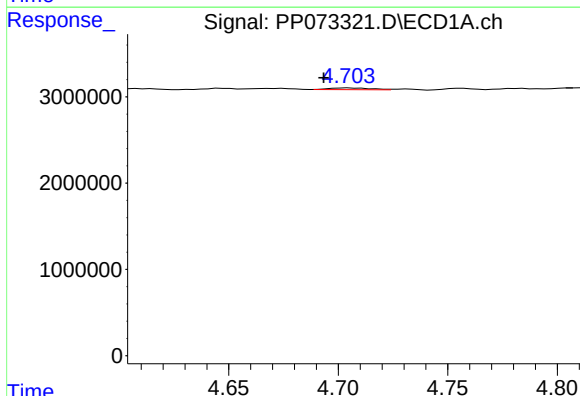


#8 AR-1221-1

R.T.: 4.705 min
Delta R.T.: 0.012 min
Response: 267981
Conc: 10.87 ng/ml

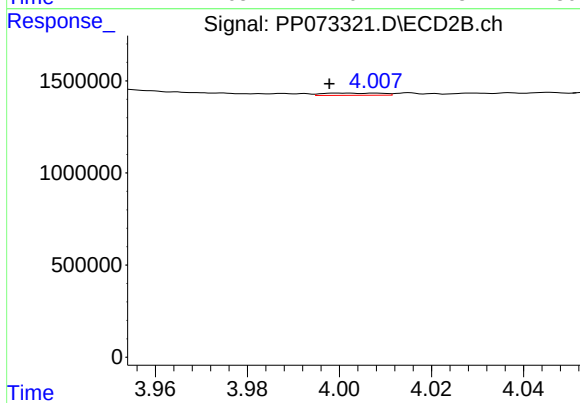

#8 AR-1221-1


R.T.: 4.000 min
Delta R.T.: 0.003 min
Response: 111396
Conc: 4.15 ng/ml

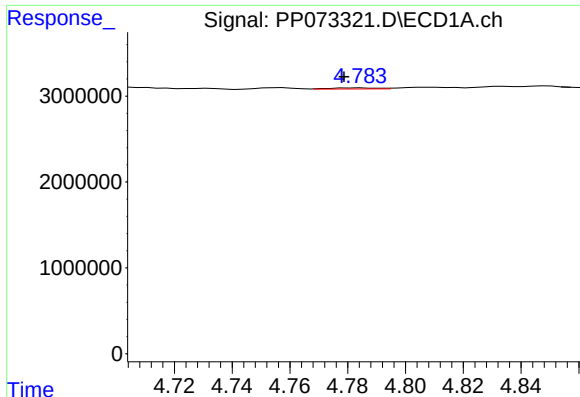

#9 AR-1221-2


R.T.: 4.784 min
Delta R.T.: 0.005 min
Response: 163044
Conc: 8.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

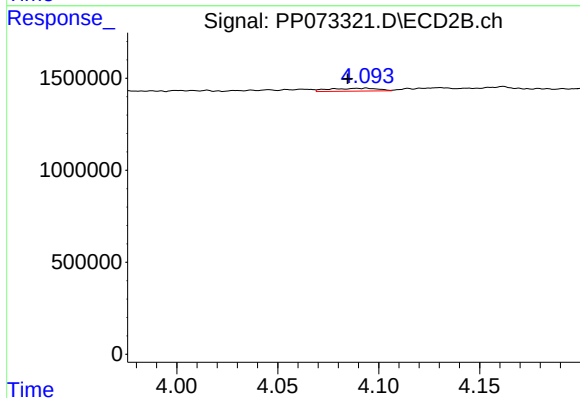


#9 AR-1221-2

R.T.: 4.094 min
Delta R.T.: 0.009 min
Response: 267183
Conc: 13.24 ng/ml

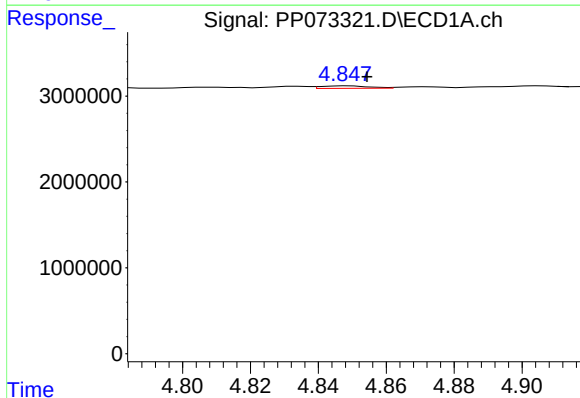


#10 AR-1221-3

R.T.: 4.849 min
Delta R.T.: -0.006 min
Response: 287700
Conc: 4.67 ng/ml

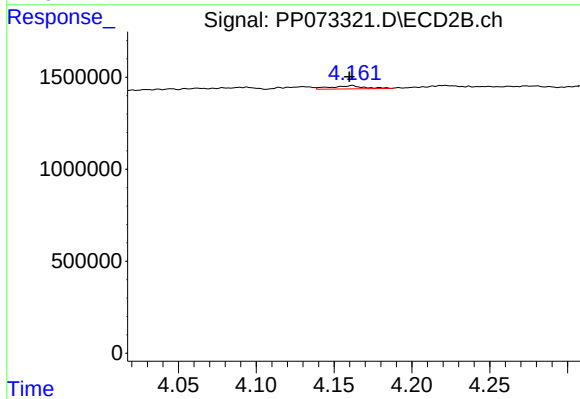

#10 AR-1221-3


R.T.: 4.162 min
Delta R.T.: 0.002 min
Response: 257297
Conc: 4.38 ng/ml

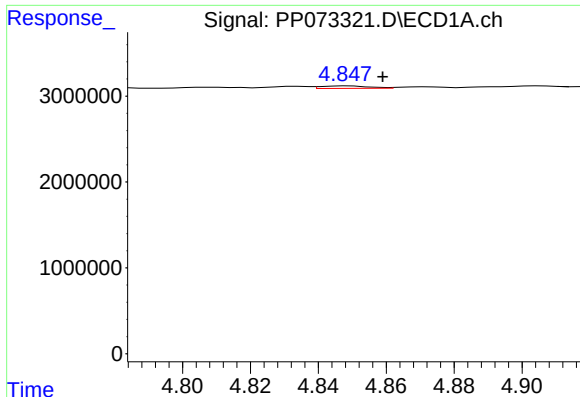

#11 AR-1232-1


R.T.: 4.849 min
Delta R.T.: -0.010 min
Response: 287700
Conc: 6.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

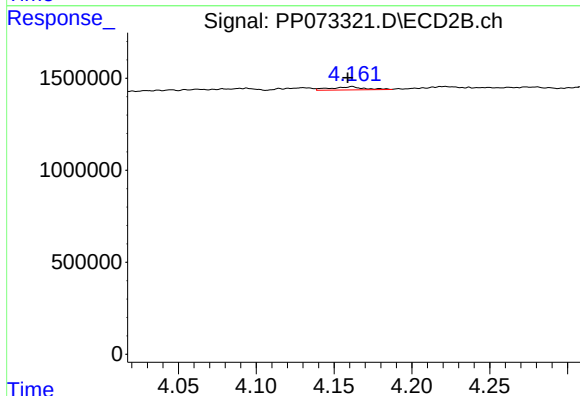


#11 AR-1232-1

R.T.: 4.162 min
Delta R.T.: 0.003 min
Response: 257297
Conc: 5.65 ng/ml

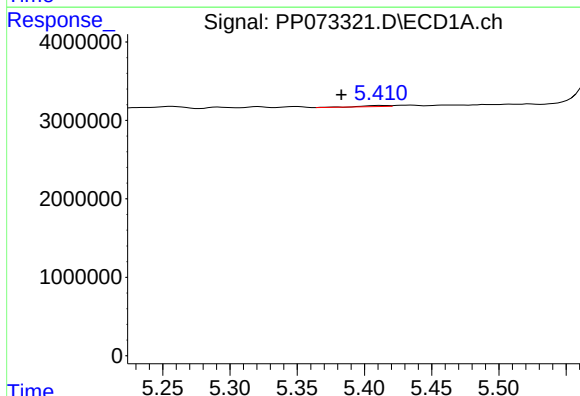


#12 AR-1232-2

R.T.: 5.412 min
Delta R.T.: 0.029 min
Response: 187108
Conc: 8.36 ng/ml

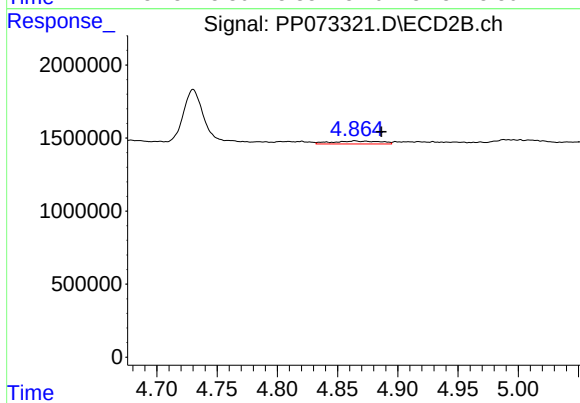

#12 AR-1232-2


R.T.: 4.864 min
Delta R.T.: -0.022 min
Response: 566855
Conc: 12.25 ng/ml

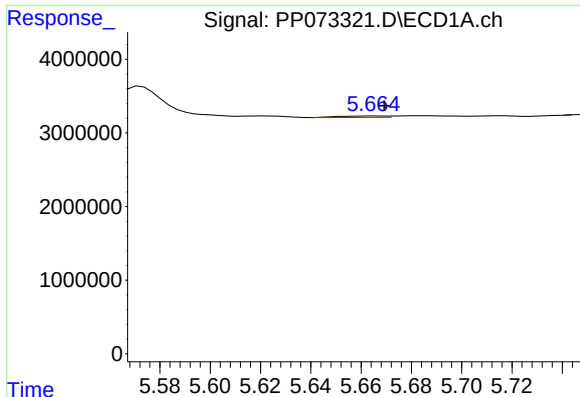

#13 AR-1232-3


R.T.: 5.665 min
Delta R.T.: -0.004 min
Response: 242534
Conc: 4.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

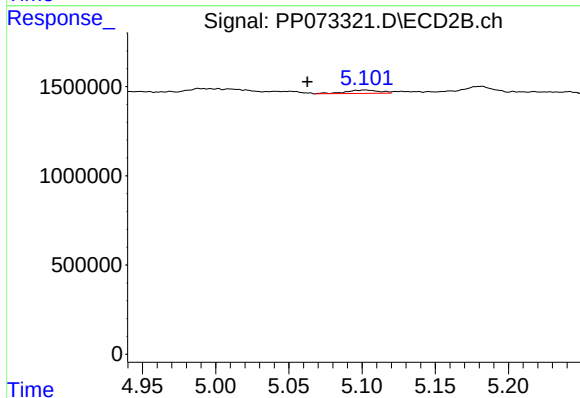


#13 AR-1232-3

R.T.: 5.102 min
Delta R.T.: 0.039 min
Response: 300952
Conc: 12.25 ng/ml

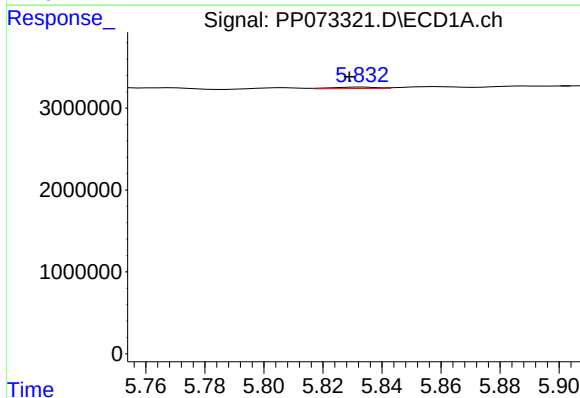


#14 AR-1232-4

R.T.: 5.833 min
Delta R.T.: 0.004 min
Response: 196339
Conc: 7.61 ng/ml

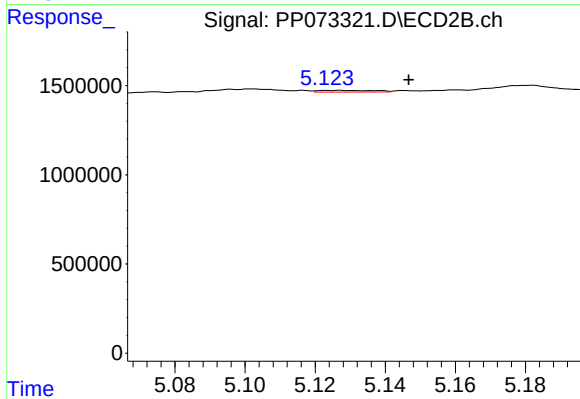

#14 AR-1232-4


R.T.: 5.127 min
Delta R.T.: -0.020 min
Response: 107486
Conc: 4.97 ng/ml

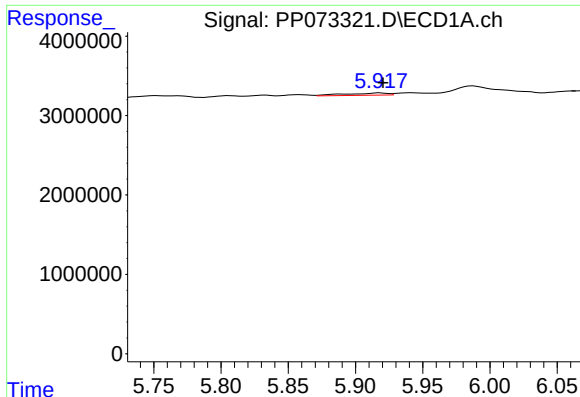

#15 AR-1232-5


R.T.: 5.919 min
Delta R.T.: -0.002 min
Response: 609904
Conc: 17.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

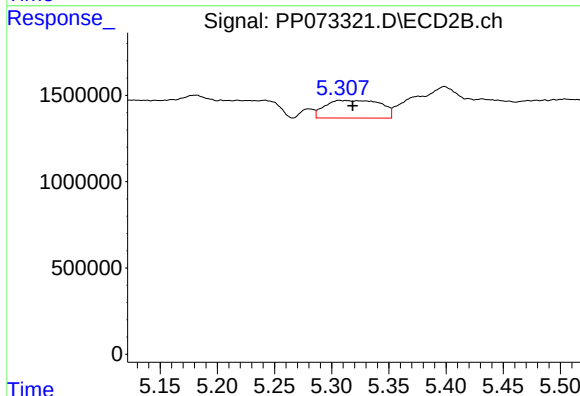


#15 AR-1232-5

R.T.: 5.307 min
Delta R.T.: -0.011 min
Response: 3467021
Conc: 151.67 ng/ml

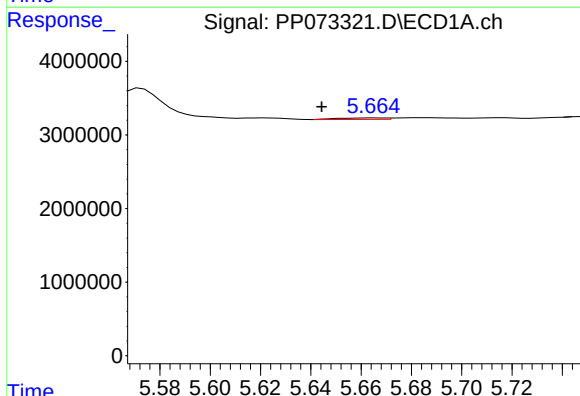


#16 AR-1242-1

R.T.: 5.665 min
Delta R.T.: 0.021 min
Response: 242534
Conc: 4.15 ng/ml

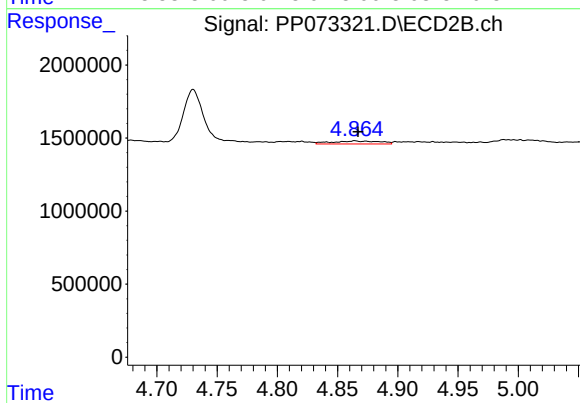

#16 AR-1242-1


R.T.: 4.864 min
Delta R.T.: -0.003 min
Response: 566855
Conc: 10.27 ng/ml

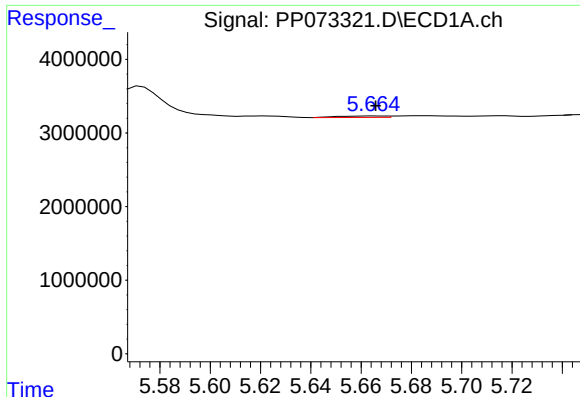

#17 AR-1242-2


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 242534
Conc: 2.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

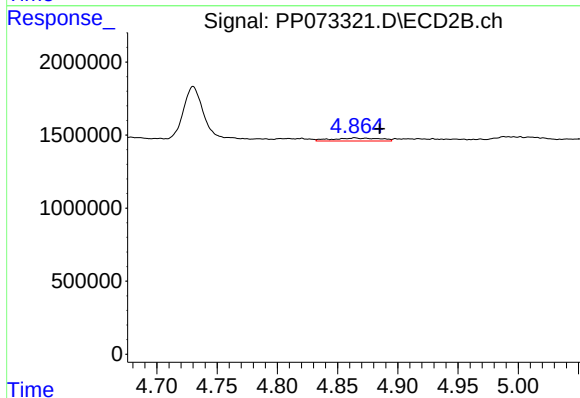


#17 AR-1242-2

R.T.: 4.864 min
Delta R.T.: -0.021 min
Response: 566855
Conc: 7.13 ng/ml

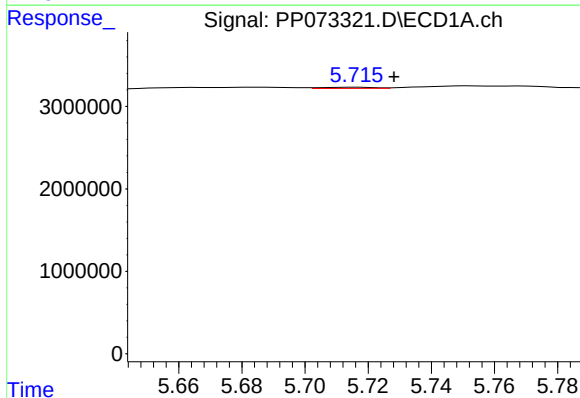


#18 AR-1242-3

R.T.: 5.716 min
Delta R.T.: -0.012 min
Response: 172330
Conc: 3.27 ng/ml

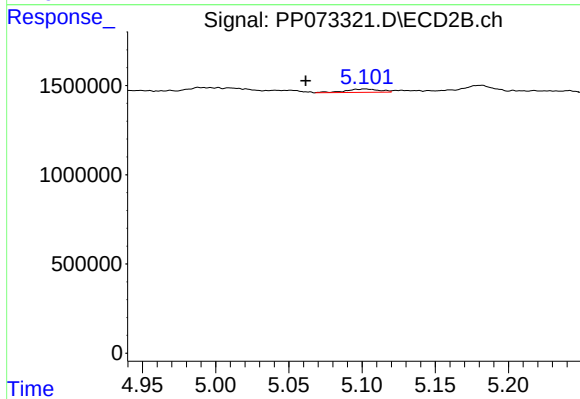

#18 AR-1242-3


R.T.: 5.102 min
Delta R.T.: 0.040 min
Response: 300952
Conc: 6.95 ng/ml

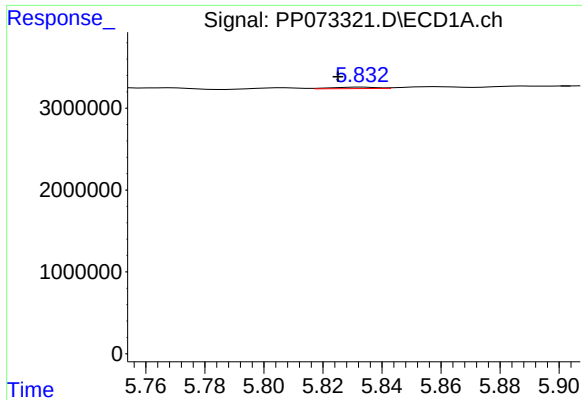

#19 AR-1242-4


R.T.: 5.833 min
Delta R.T.: 0.008 min
Response: 196339
Conc: 4.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

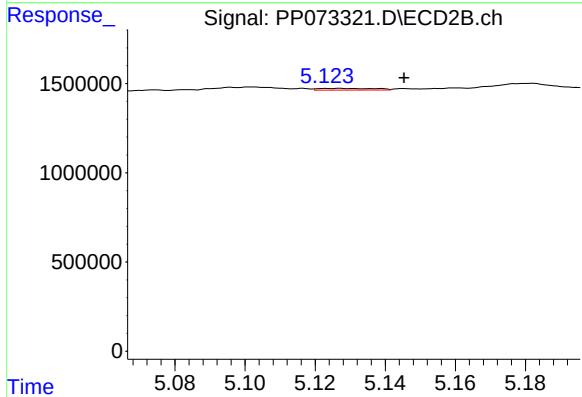


#19 AR-1242-4

R.T.: 5.127 min
Delta R.T.: -0.018 min
Response: 107486
Conc: 2.59 ng/ml

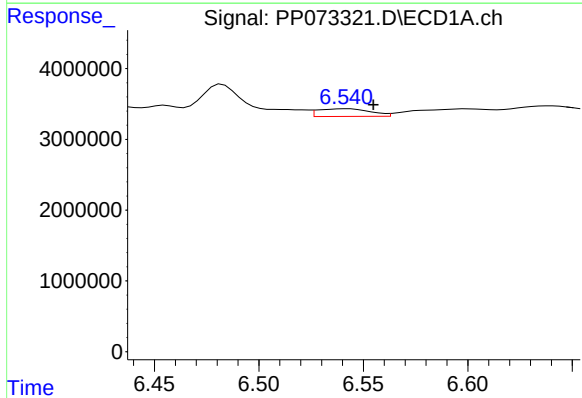


#20 AR-1242-5

R.T.: 6.542 min
Delta R.T.: -0.013 min
Response: 1903498
Conc: 38.41 ng/ml

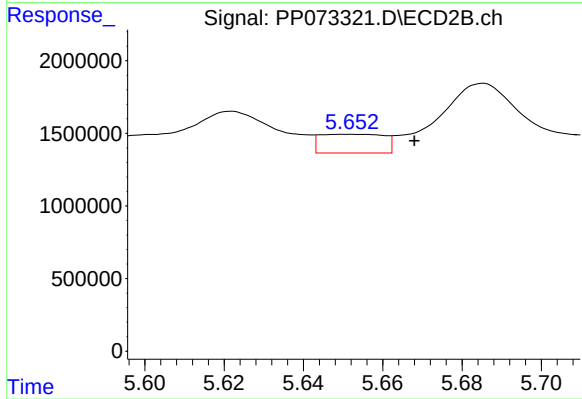

#20 AR-1242-5


R.T.: 5.651 min
Delta R.T.: -0.017 min
Response: 1454495
Conc: 27.66 ng/ml

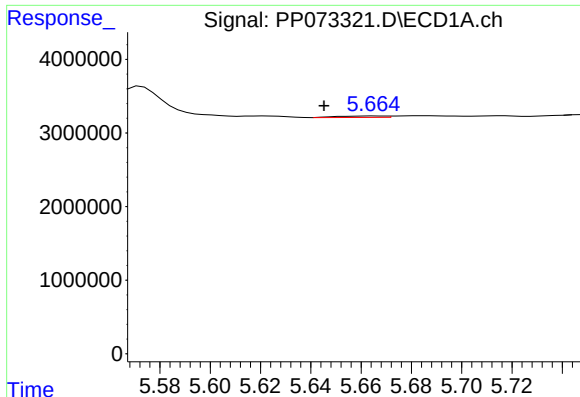

#21 AR-1248-1


R.T.: 5.665 min
Delta R.T.: 0.020 min
Response: 242534
Conc: 5.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

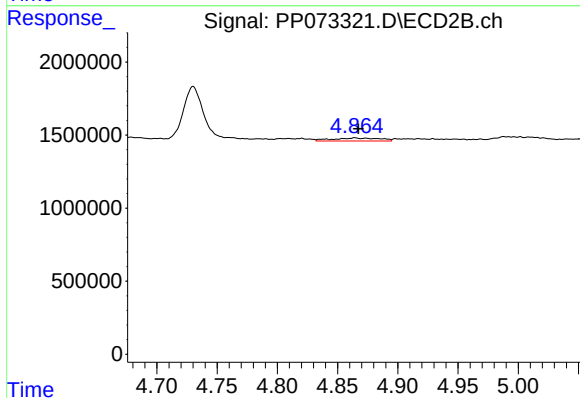


#21 AR-1248-1

R.T.: 4.864 min
Delta R.T.: -0.003 min
Response: 566855
Conc: 13.00 ng/ml

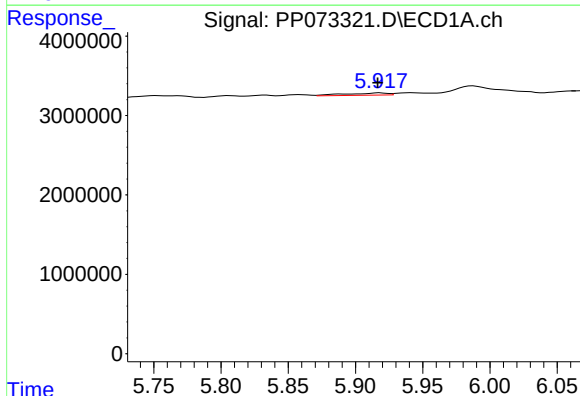


#22 AR-1248-2

R.T.: 5.919 min
Delta R.T.: 0.002 min
Response: 609904
Conc: 10.42 ng/ml

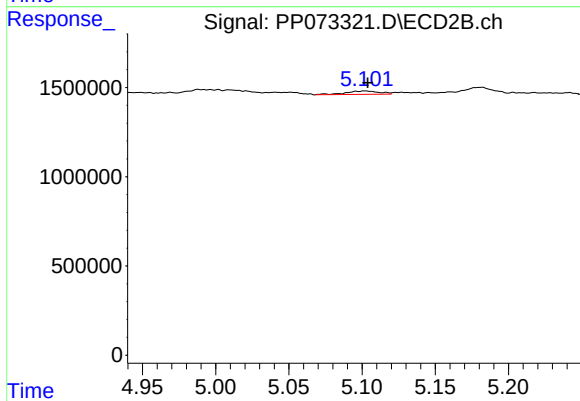

#22 AR-1248-2


R.T.: 5.102 min
Delta R.T.: -0.002 min
Response: 300952
Conc: 5.14 ng/ml

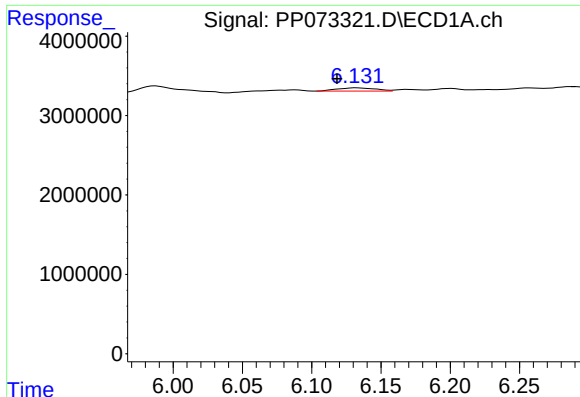

#23 AR-1248-3


R.T.: 6.132 min
Delta R.T.: 0.014 min
Response: 805417
Conc: 12.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

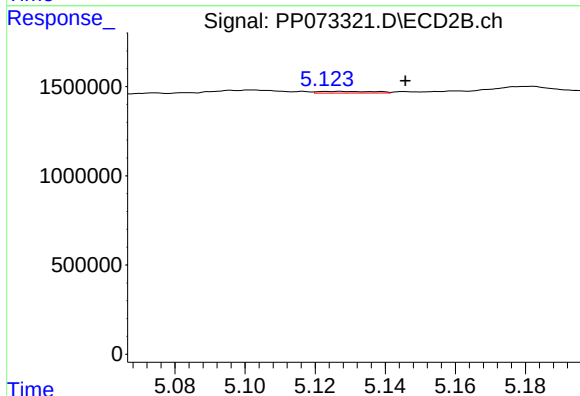


#23 AR-1248-3

R.T.: 5.127 min
Delta R.T.: -0.019 min
Response: 107486
Conc: 1.78 ng/ml

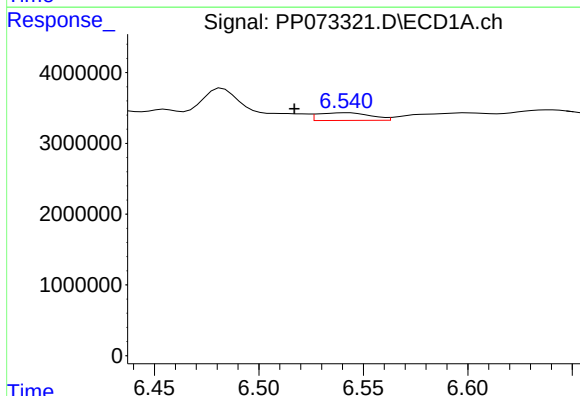


#24 AR-1248-4

R.T.: 6.542 min
Delta R.T.: 0.025 min
Response: 1903498
Conc: 22.38 ng/ml

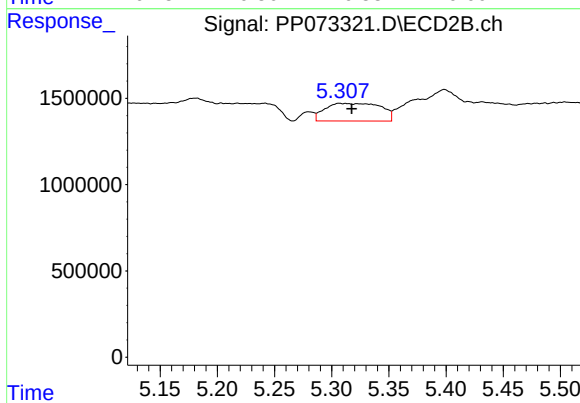

#24 AR-1248-4


R.T.: 5.307 min
Delta R.T.: -0.011 min
Response: 3467021
Conc: 49.51 ng/ml

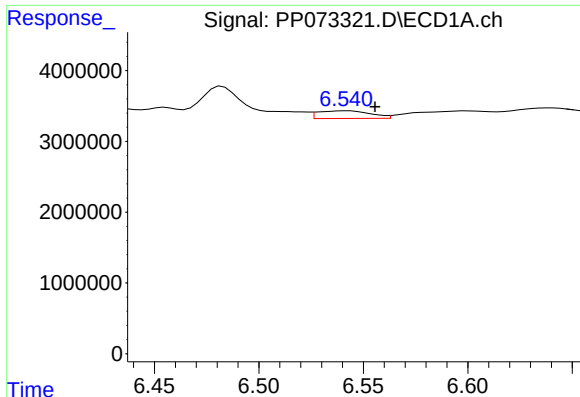

#25 AR-1248-5


R.T.: 6.542 min
Delta R.T.: -0.013 min
Response: 1903498
Conc: 22.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

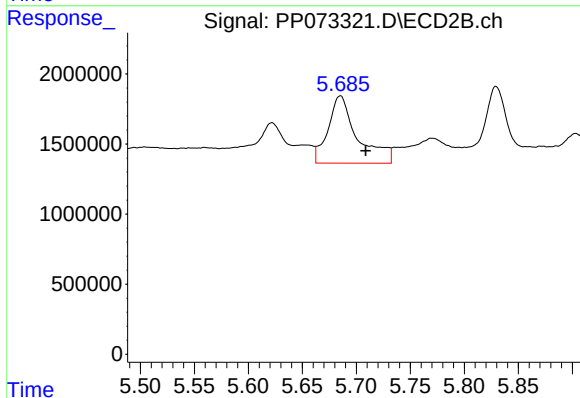


#25 AR-1248-5

R.T.: 5.685 min
Delta R.T.: -0.024 min
Response: 9093279
Conc: 128.02 ng/ml

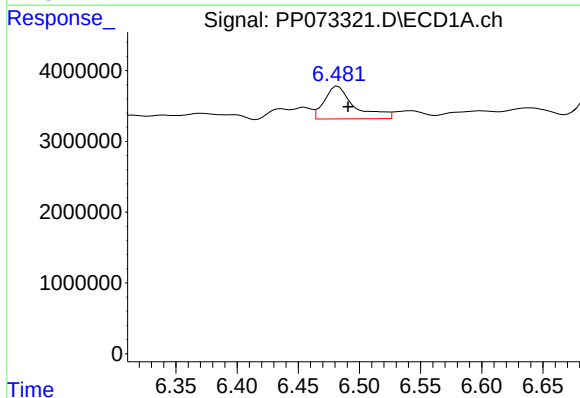


#26 AR-1254-1

R.T.: 6.482 min
Delta R.T.: -0.008 min
Response: 7916358
Conc: 94.05 ng/ml

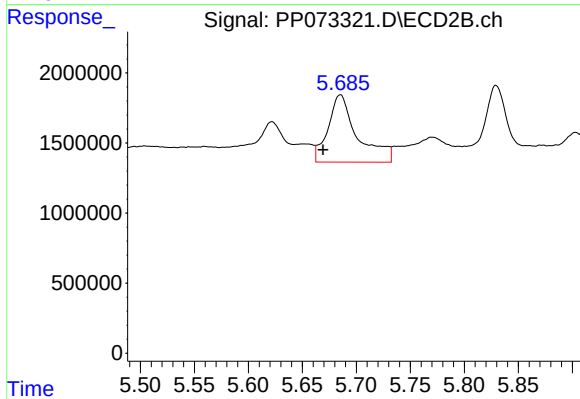

#26 AR-1254-1


R.T.: 5.685 min
Delta R.T.: 0.016 min
Response: 9093279
Conc: 82.93 ng/ml

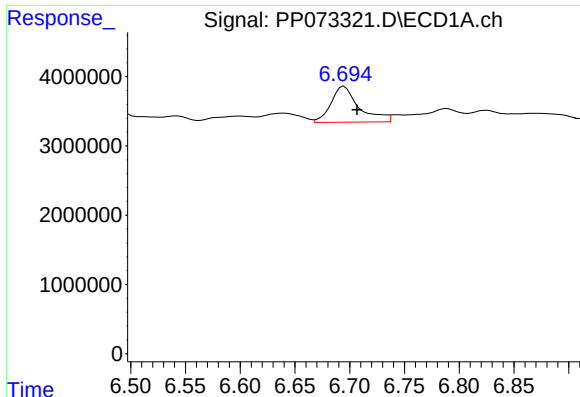

#27 AR-1254-2


R.T.: 6.695 min
Delta R.T.: -0.012 min
Response: 9237471
Conc: 73.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

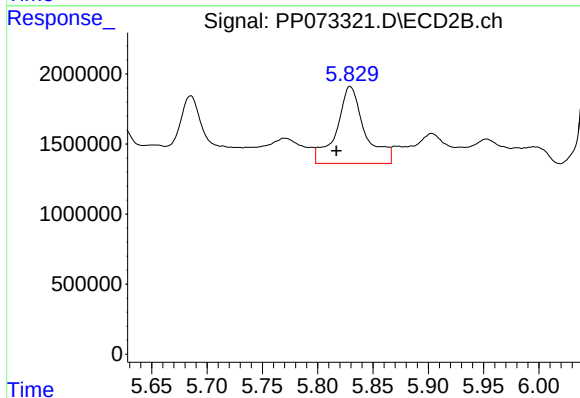


#27 AR-1254-2

R.T.: 5.829 min
Delta R.T.: 0.013 min
Response: 9777748
Conc: 103.42 ng/ml

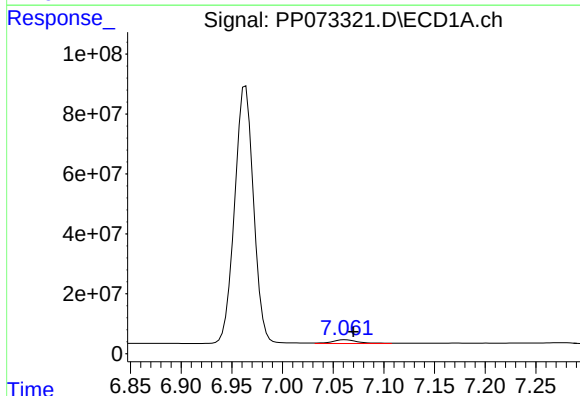


#28 AR-1254-3

R.T.: 7.062 min
Delta R.T.: -0.008 min
Response: 23563609
Conc: 179.59 ng/ml

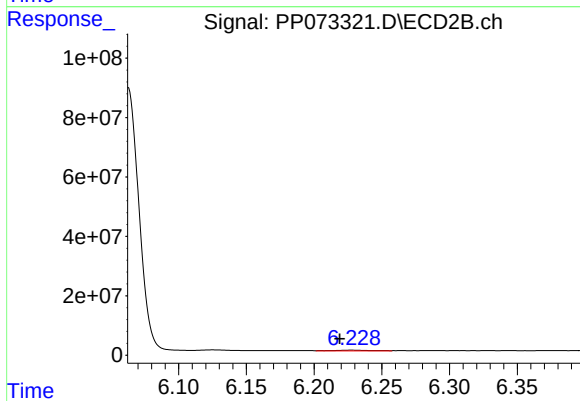

#28 AR-1254-3


R.T.: 6.228 min
Delta R.T.: 0.009 min
Response: 4955407
Conc: 33.59 ng/ml

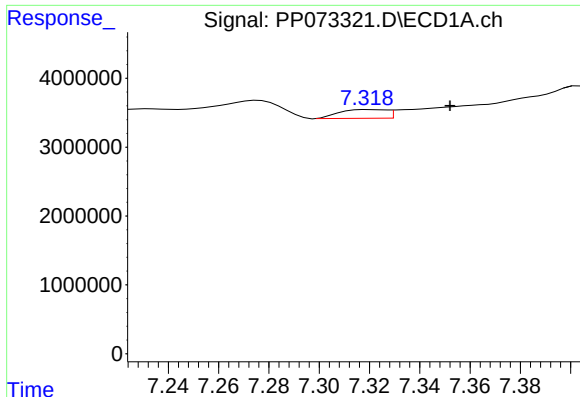

#29 AR-1254-4


R.T.: 7.320 min
Delta R.T.: -0.032 min
Response: 1658470
Conc: 13.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

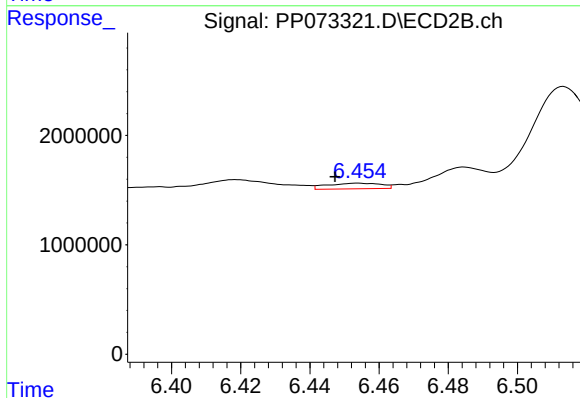


#29 AR-1254-4

R.T.: 6.454 min
Delta R.T.: 0.007 min
Response: 554299
Conc: 5.71 ng/ml

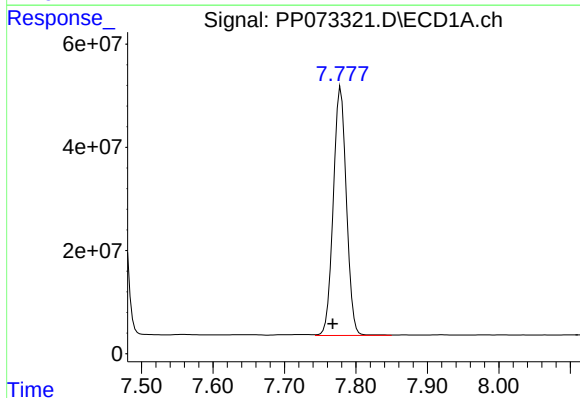


#30 AR-1254-5

R.T.: 7.779 min
Delta R.T.: 0.011 min
Response: 614706824
Conc: 5380.06 ng/ml

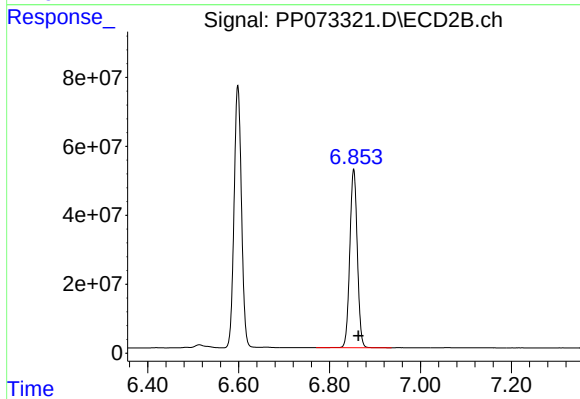

#30 AR-1254-5


R.T.: 6.853 min
Delta R.T.: -0.010 min
Response: 593173824
Conc: 4564.19 ng/ml

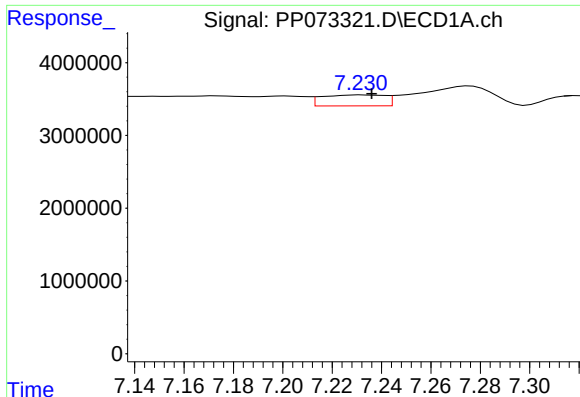

#31 AR-1260-1


R.T.: 7.232 min
Delta R.T.: -0.004 min
Response: 2657004
Conc: 30.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

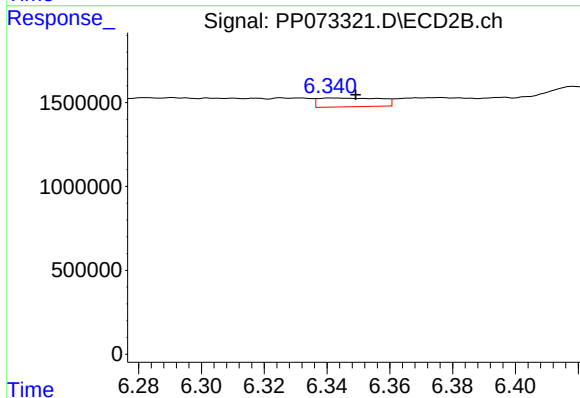


#31 AR-1260-1

R.T.: 6.342 min
Delta R.T.: -0.008 min
Response: 720324
Conc: 7.60 ng/ml

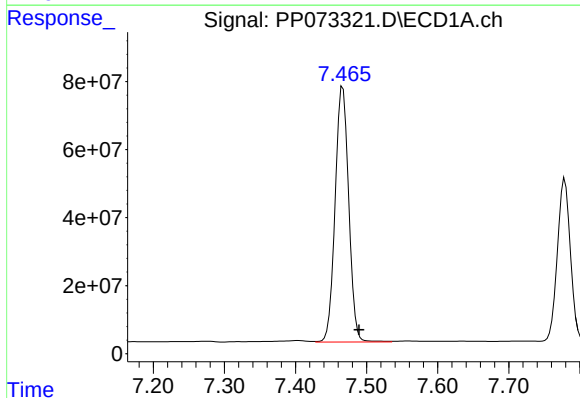


#32 AR-1260-2

R.T.: 7.467 min
Delta R.T.: -0.023 min
Response: 996589432
Conc: 7334.13 ng/ml

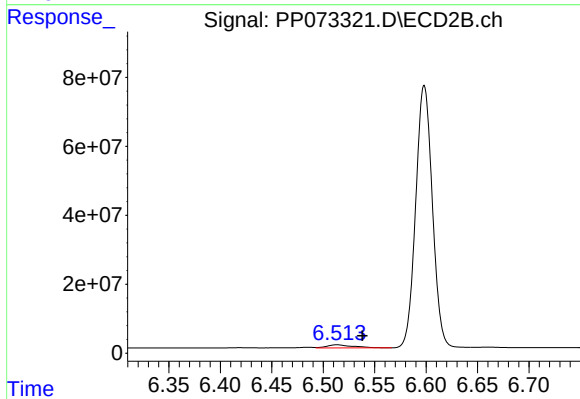

#32 AR-1260-2


R.T.: 6.513 min
Delta R.T.: -0.025 min
Response: 16143797
Conc: 138.65 ng/ml

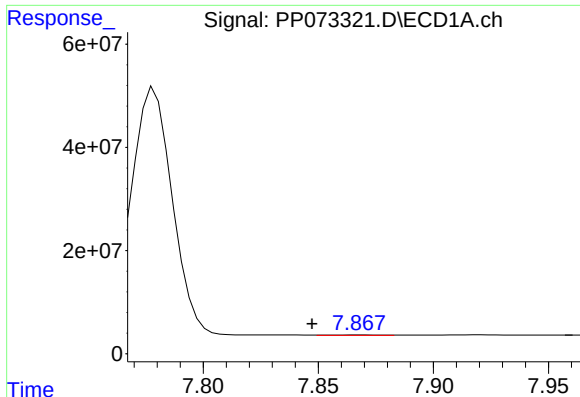

#33 AR-1260-3


R.T.: 7.868 min
Delta R.T.: 0.020 min
Response: 1712989
Conc: 15.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

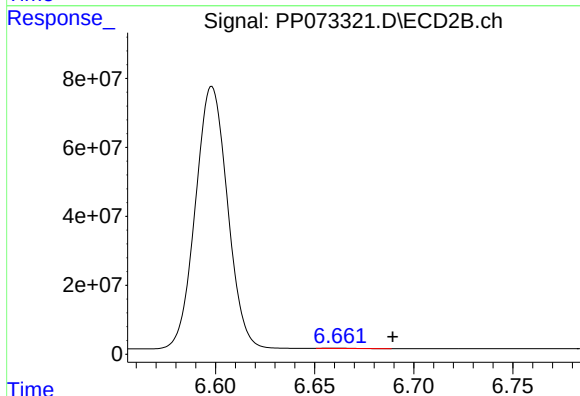


#33 AR-1260-3

R.T.: 6.661 min
Delta R.T.: -0.028 min
Response: 573773
Conc: 5.51 ng/ml

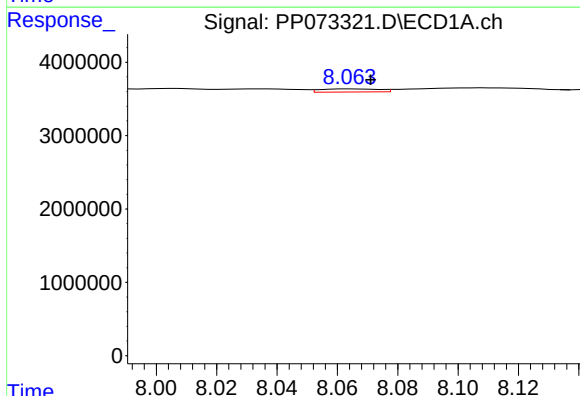


#34 AR-1260-4

R.T.: 8.065 min
Delta R.T.: -0.006 min
Response: 566719
Conc: 5.50 ng/ml

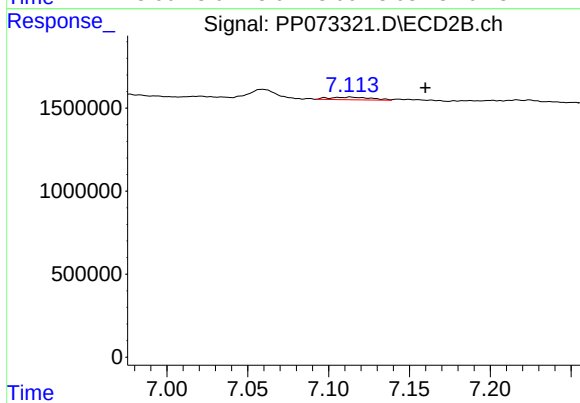

#34 AR-1260-4


R.T.: 7.114 min
Delta R.T.: -0.046 min
Response: 284022
Conc: 3.24 ng/ml

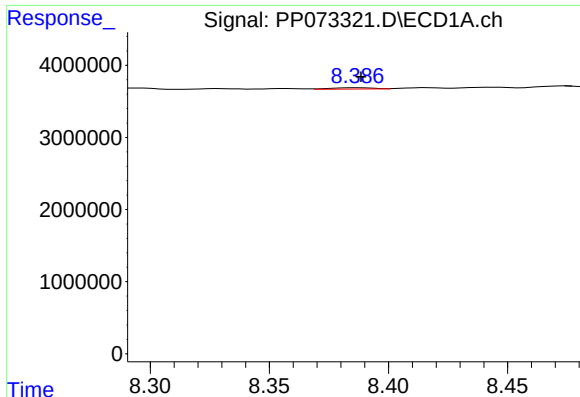

#35 AR-1260-5


R.T.: 8.387 min
Delta R.T.: -0.001 min
Response: 228325
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

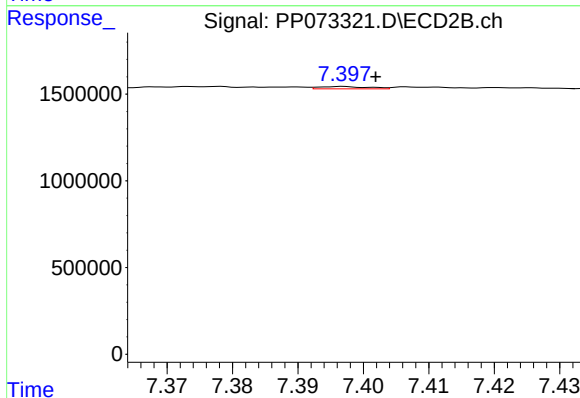


#35 AR-1260-5

R.T.: 7.397 min
Delta R.T.: -0.005 min
Response: 72504
Conc: 0.34 ng/ml

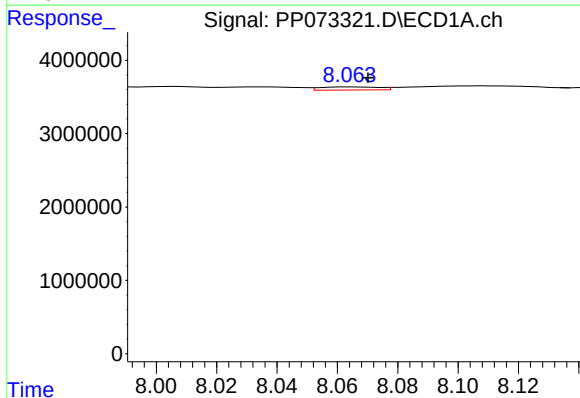


#36 AR-1262-1

R.T.: 8.065 min
Delta R.T.: -0.006 min
Response: 566719
Conc: 3.83 ng/ml

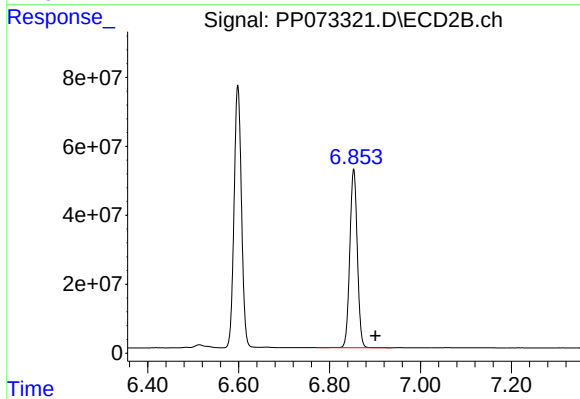

#36 AR-1262-1


R.T.: 6.853 min
Delta R.T.: -0.048 min
Response: 593173824
Conc: 4105.95 ng/ml

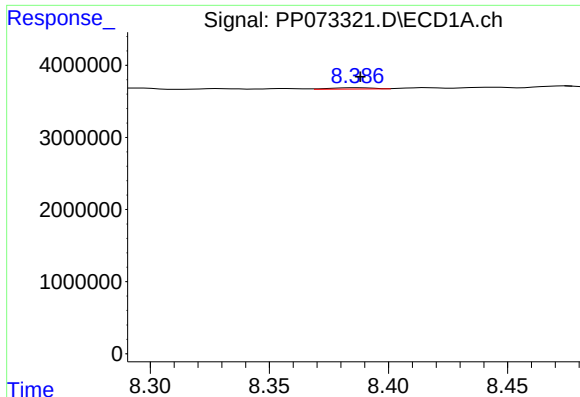

#37 AR-1262-2


R.T.: 8.387 min
Delta R.T.: -0.001 min
Response: 228325
Conc: 0.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

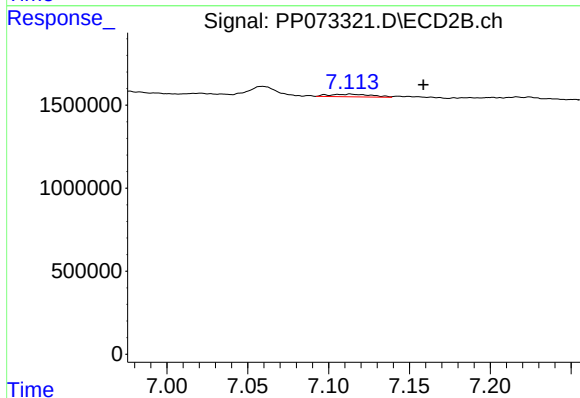


#37 AR-1262-2

R.T.: 7.114 min
Delta R.T.: -0.045 min
Response: 284022
Conc: 2.32 ng/ml

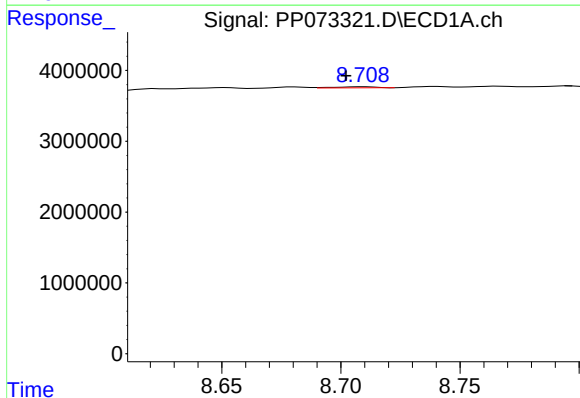


#38 AR-1262-3

R.T.: 8.709 min
Delta R.T.: 0.007 min
Response: 195977
Conc: 0.92 ng/ml

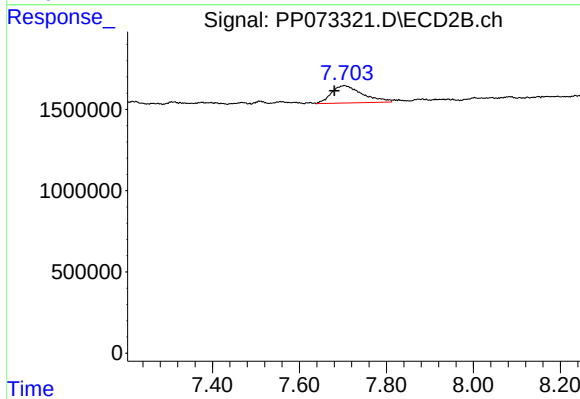

#38 AR-1262-3


R.T.: 7.703 min
Delta R.T.: 0.022 min
Response: 5338629
Conc: 47.37 ng/ml

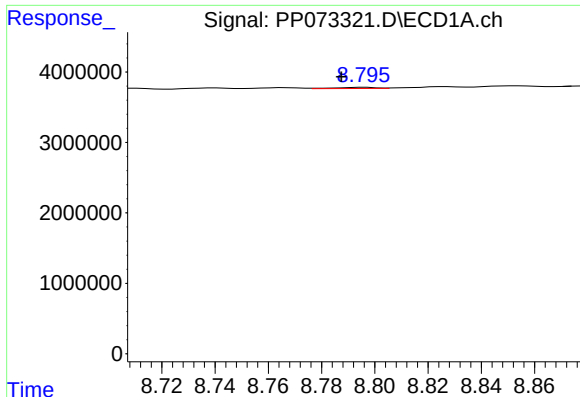

#39 AR-1262-4


R.T.: 8.796 min
Delta R.T.: 0.008 min
Response: 160032
Conc: 1.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

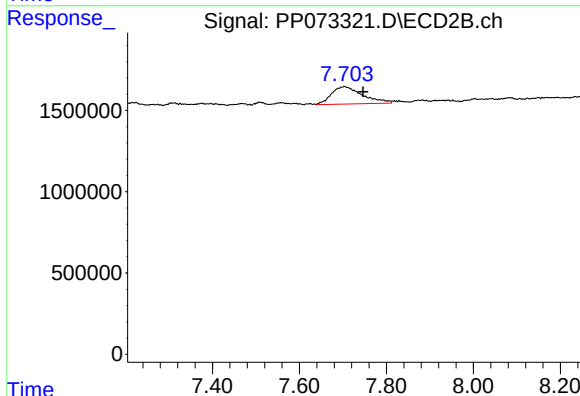


#39 AR-1262-4

R.T.: 7.703 min
Delta R.T.: -0.043 min
Response: 5338629
Conc: 29.12 ng/ml

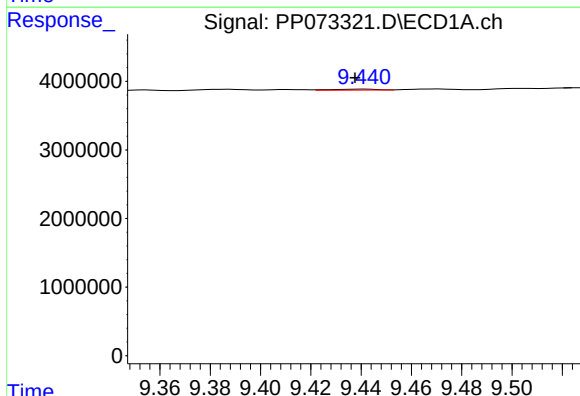


#40 AR-1262-5

R.T.: 9.441 min
Delta R.T.: 0.004 min
Response: 190872
Conc: 1.71 ng/ml

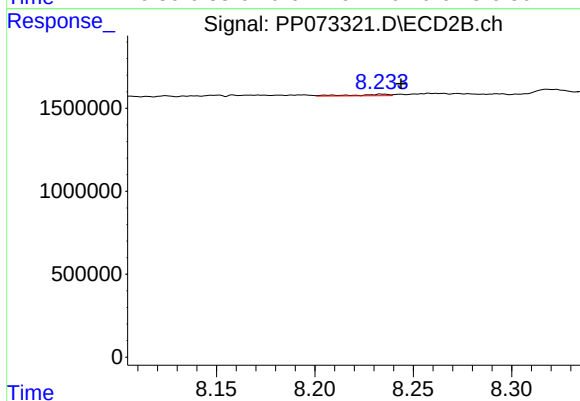

#40 AR-1262-5


R.T.: 8.234 min
Delta R.T.: -0.010 min
Response: 108119
Conc: 1.25 ng/ml

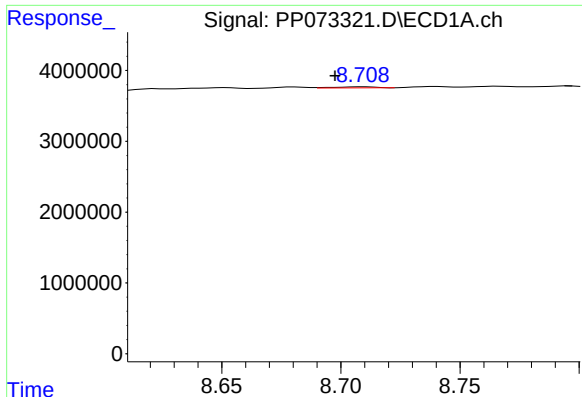

#41 AR-1268-1


R.T.: 8.709 min
Delta R.T.: 0.012 min
Response: 195977
Conc: 0.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

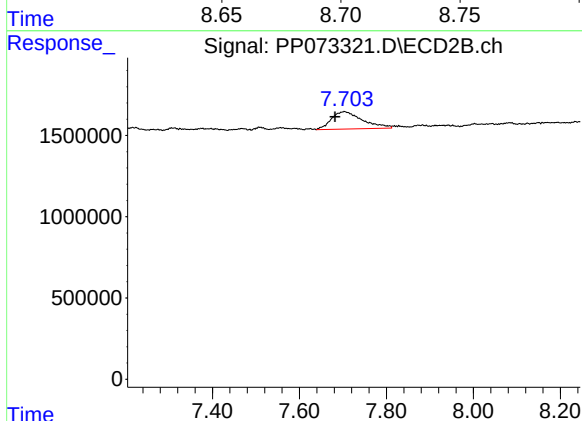


#41 AR-1268-1

R.T.: 7.703 min
Delta R.T.: 0.021 min
Response: 5338629
Conc: 18.58 ng/ml

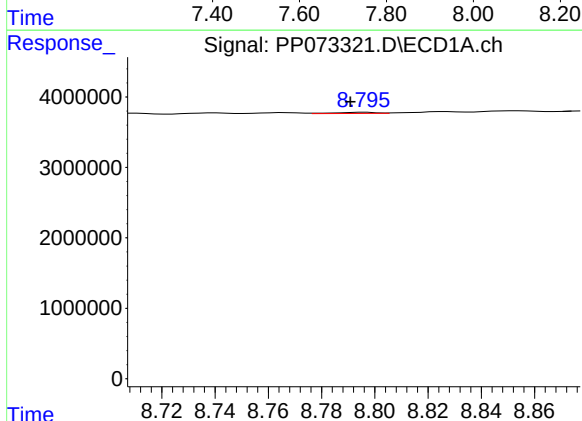


#42 AR-1268-2

R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 160032
Conc: 0.52 ng/ml

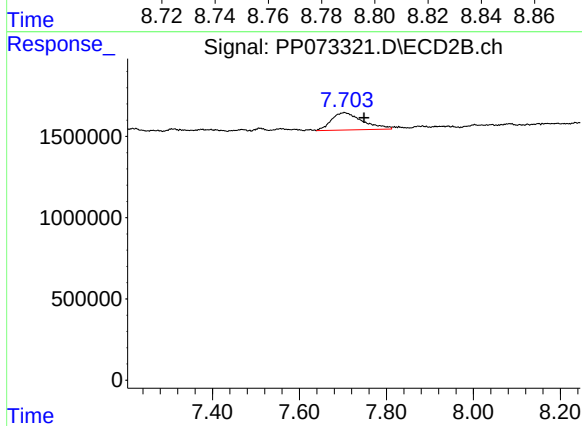

#42 AR-1268-2


R.T.: 7.703 min
Delta R.T.: -0.045 min
Response: 5338629
Conc: 20.76 ng/ml

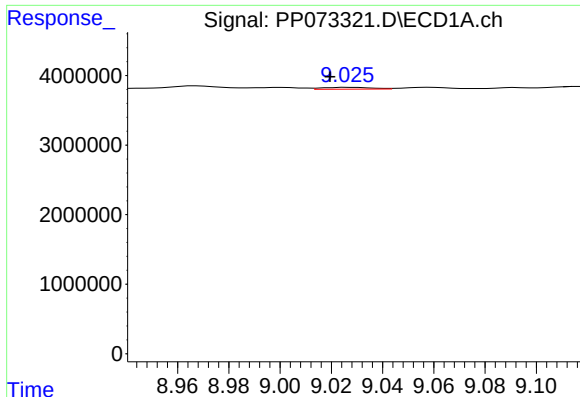

#43 AR-1268-3


R.T.: 9.027 min
Delta R.T.: 0.007 min
Response: 352718
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

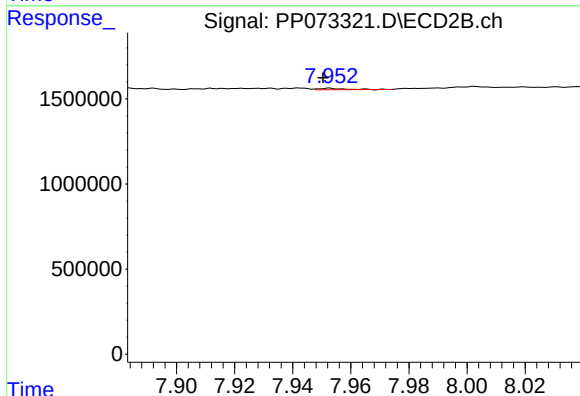


#43 AR-1268-3

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 53906
Conc: 0.25 ng/ml

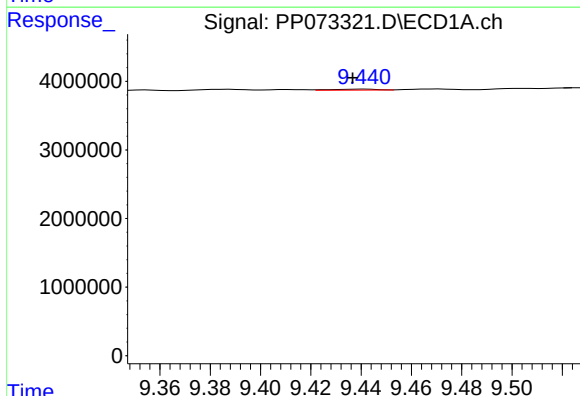


#44 AR-1268-4

R.T.: 9.441 min
Delta R.T.: 0.005 min
Response: 190872
Conc: 1.63 ng/ml

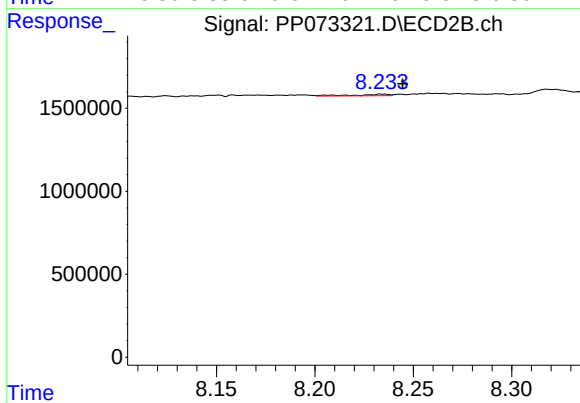

#44 AR-1268-4


R.T.: 8.234 min
Delta R.T.: -0.010 min
Response: 108119
Conc: 1.15 ng/ml

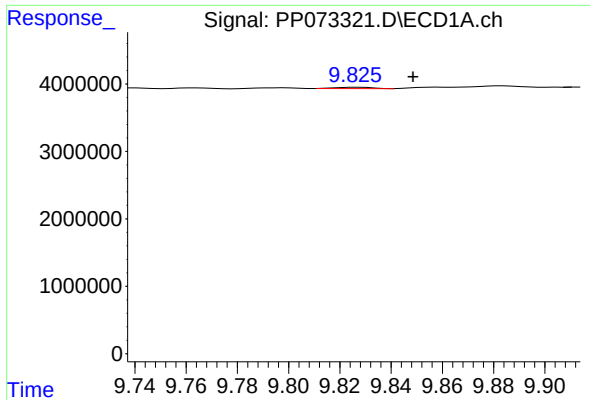

#45 AR-1268-5

R.T.: 9.827 min
Delta R.T.: -0.022 min
Response: 187074
Conc: 0.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

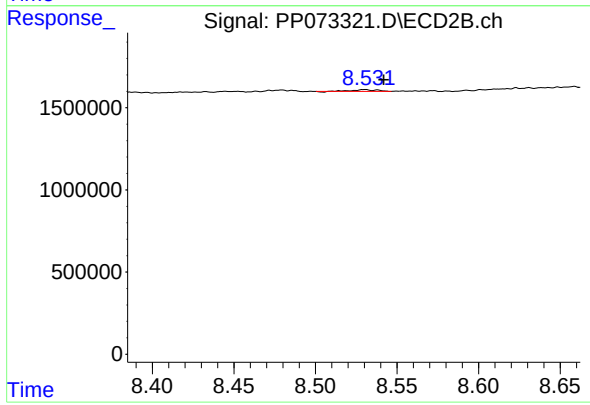

#45 AR-1268-5

R.T.: 8.530 min
Delta R.T.: -0.012 min
Response: 103678
Conc: 0.18 ng/ml