

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
 Data File : PP036818.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2021 10:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:54:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.955	869164	589547	19.665	19.034
2)	SA Decachlor...	10.995	9.251	912135	577900	21.263	18.070
Target Compounds							
9)	L2 AR-1221-2	5.317	0.000	11854	0	27.509	N.D. #
15)	L3 AR-1232-5	6.573	0.000	18960	0	51.731	N.D. #
22)	L5 AR-1248-2	6.573	0.000	18960	0	13.961	N.D. #
28)	L6 AR-1254-3	7.820	0.000	4723	0	1.595	N.D. #
34)	L7 AR-1260-4	8.835	0.000	49243	0	20.784	N.D. #
35)	L7 AR-1260-5	9.155	0.000	8057	0	1.806	N.D. #
37)	L8 AR-1262-2	9.155	0.000	8057	0	1.586	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
Data File : PP036818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2021 10:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:54:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

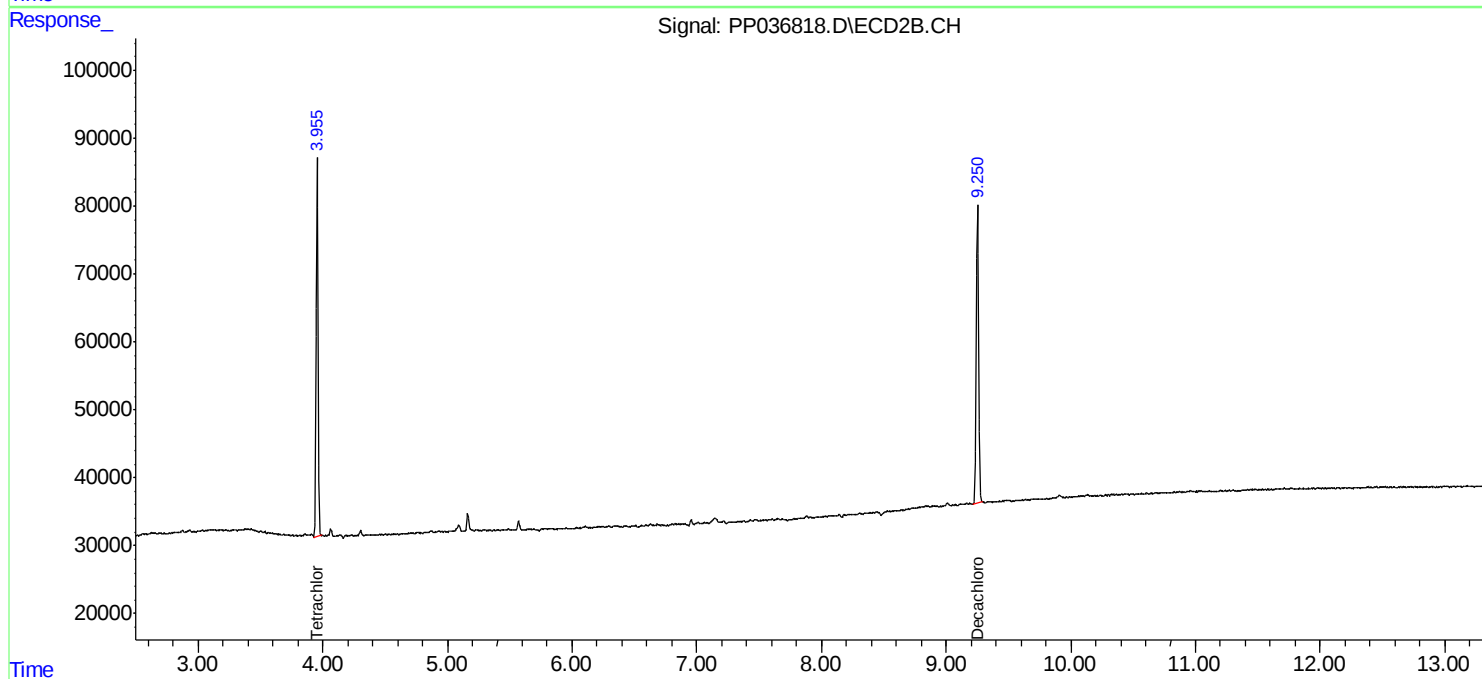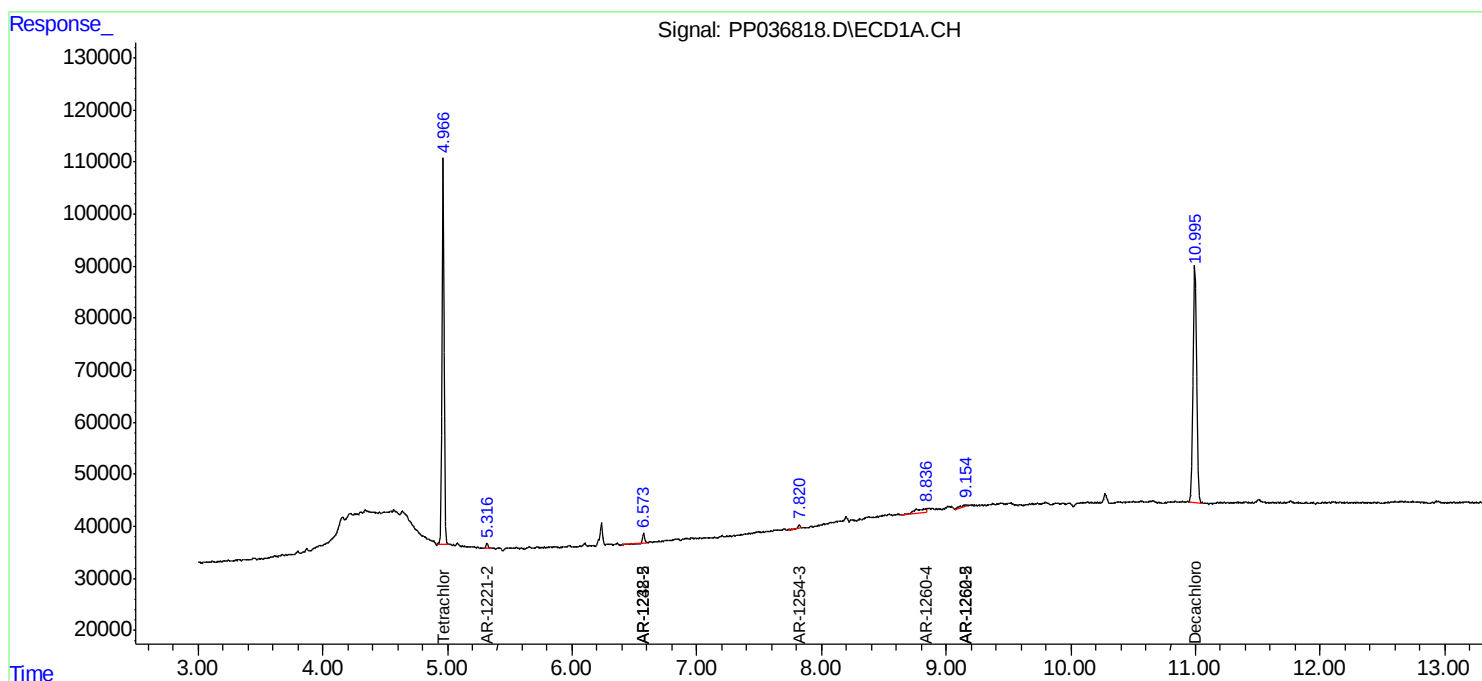


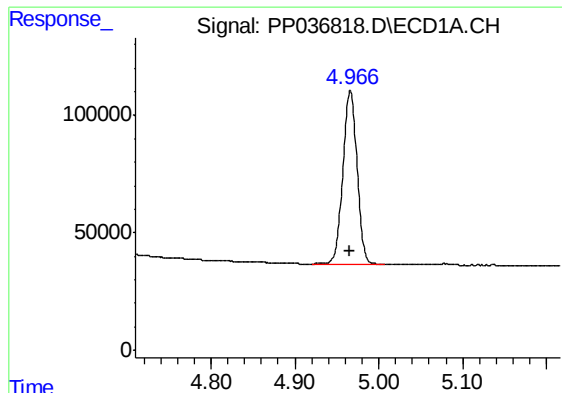

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.001 min
Response: 869164
Conc: 19.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

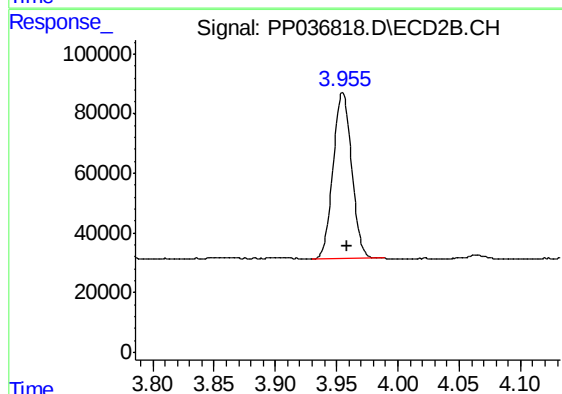


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 589547
Conc: 19.03 ng/ml

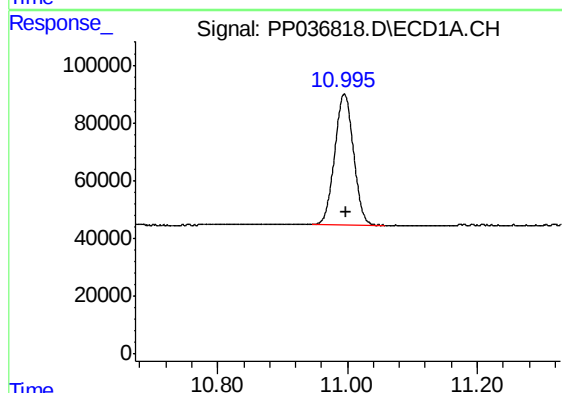


#2 Decachlorobiphenyl

R.T.: 10.995 min
Delta R.T.: -0.003 min
Response: 912135
Conc: 21.26 ng/ml

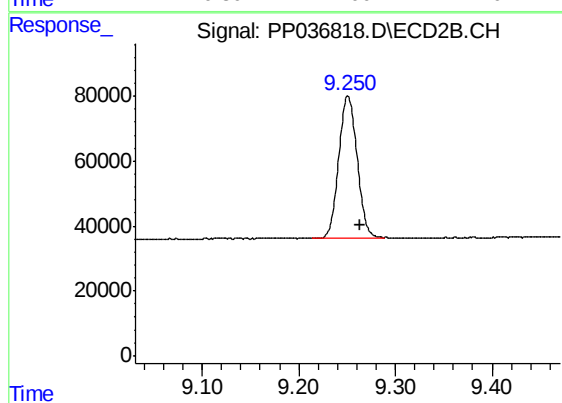

#2 Decachlorobiphenyl


R.T.: 9.251 min
Delta R.T.: -0.012 min
Response: 577900
Conc: 18.07 ng/ml

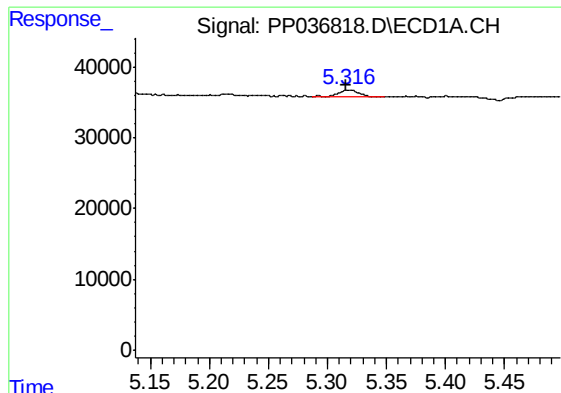

#9 AR-1221-2


R.T.: 5.317 min
Delta R.T.: 0.002 min
Response: 11854
Conc: 27.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

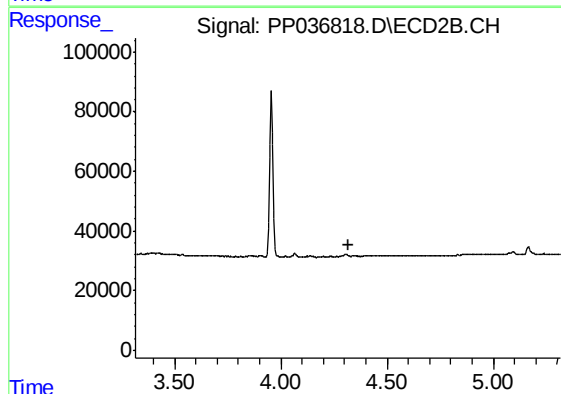


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

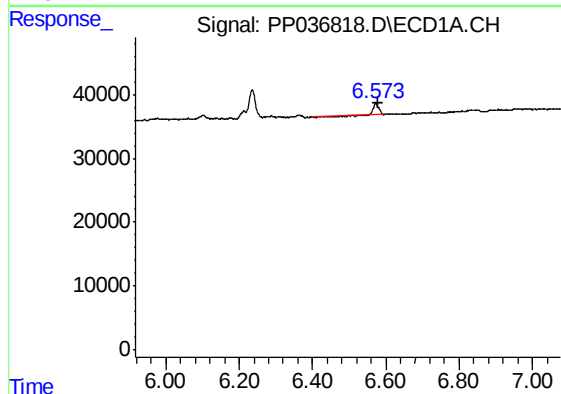


#15 AR-1232-5

R.T.: 6.573 min
Delta R.T.: -0.006 min
Response: 18960
Conc: 51.73 ng/ml

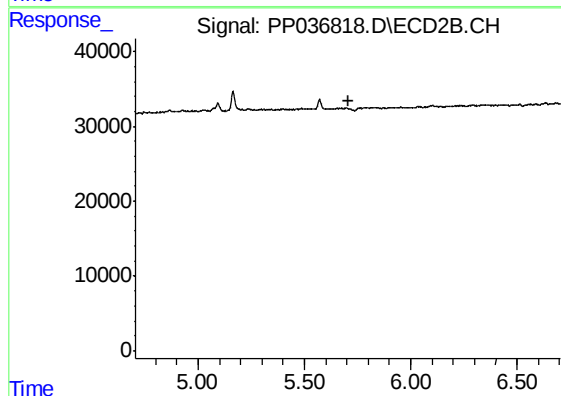

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

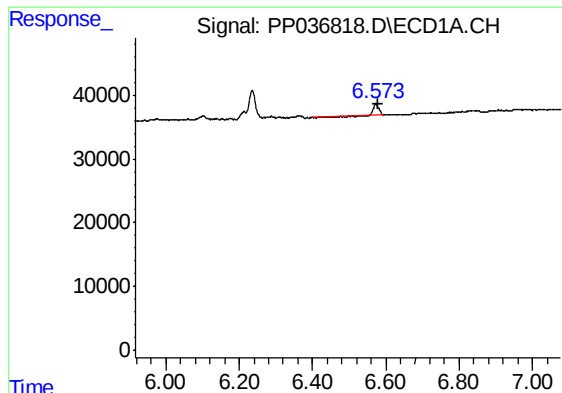

#22 AR-1248-2


R.T.: 6.573 min
Delta R.T.: -0.005 min
Response: 18960
Conc: 13.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

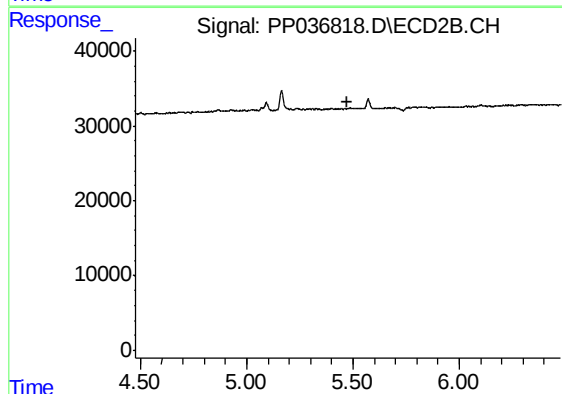


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

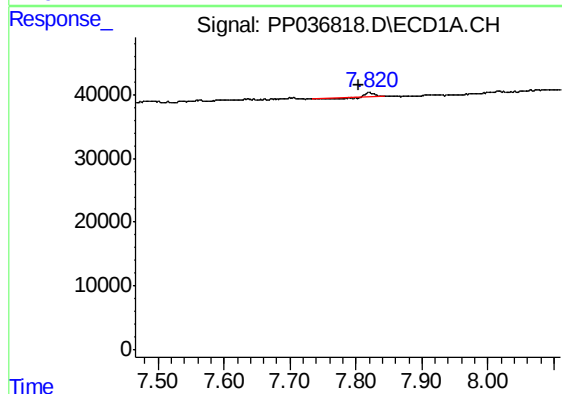


#28 AR-1254-3

R.T.: 7.820 min
Delta R.T.: 0.015 min
Response: 4723
Conc: 1.59 ng/ml

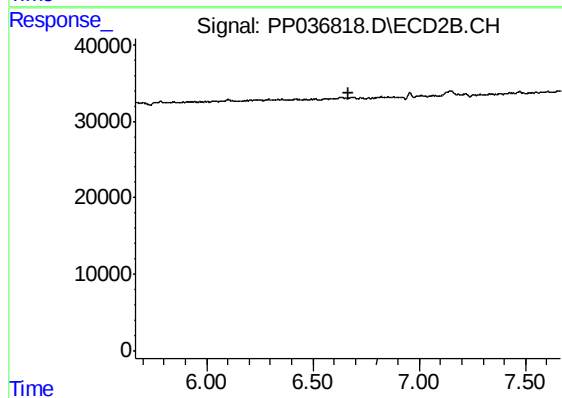

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

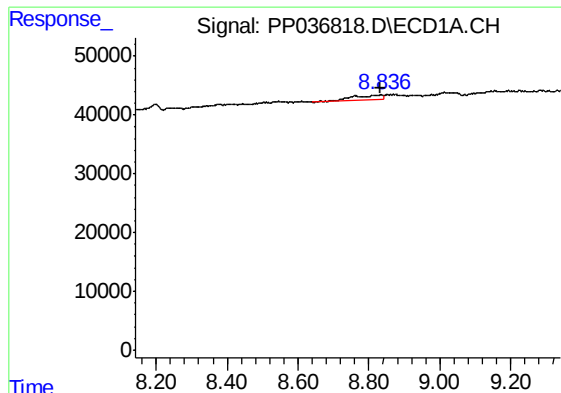

#34 AR-1260-4


R.T.: 8.835 min
Delta R.T.: 0.001 min
Response: 49243
Conc: 20.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

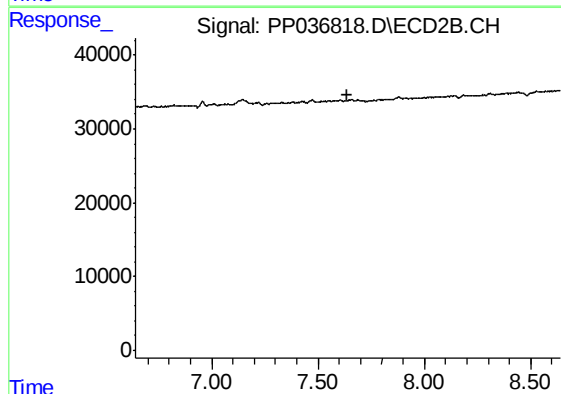


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.640 min
Response: 0
Conc: N.D.

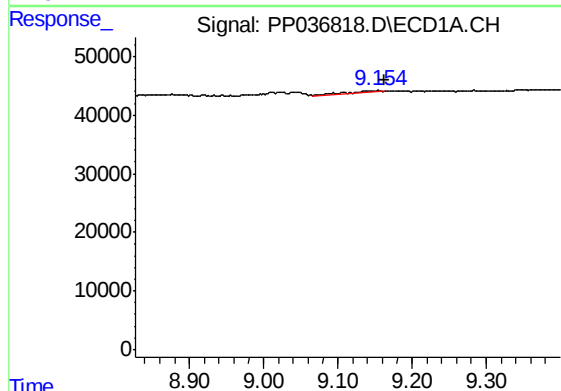


#35 AR-1260-5

R.T.: 9.155 min
Delta R.T.: -0.008 min
Response: 8057
Conc: 1.81 ng/ml

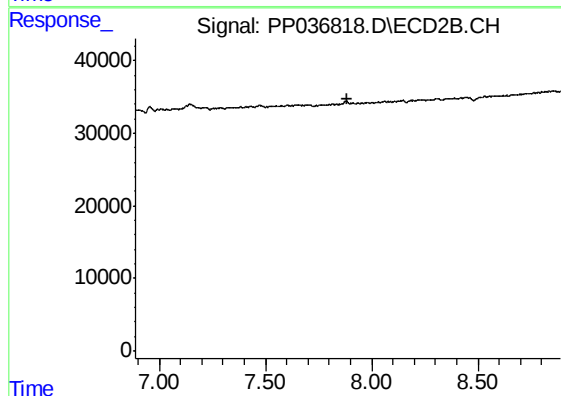

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.888 min
Response: 0
Conc: N.D.

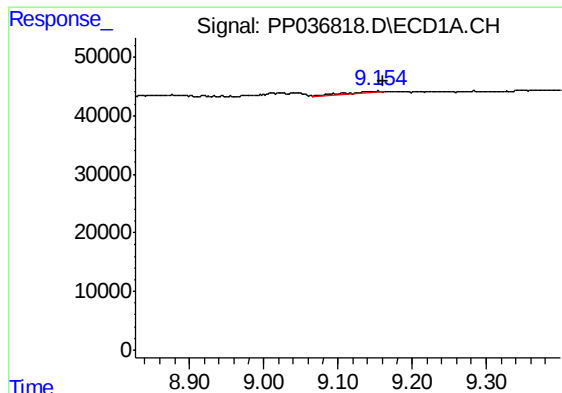

#37 AR-1262-2

R.T.: 9.155 min
Delta R.T.: -0.007 min
Response: 8057
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

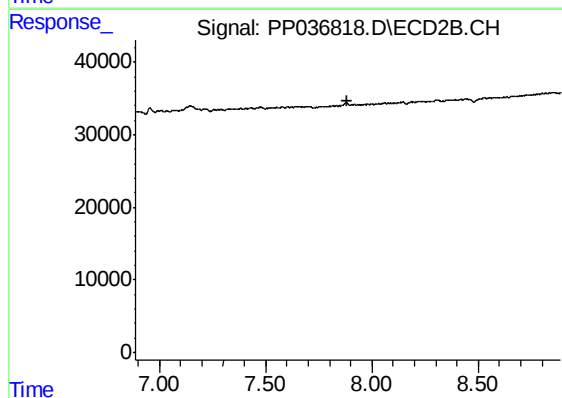

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.887 min
Response: 0
Conc: N.D.