

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
 Data File : PP036824.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2021 11:49
 Operator : DD\AJ
 Sample : M2856-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-06-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:56:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.957	906997	605362	20.521	19.545
2)	SA Decachlor...	10.992	9.250	936711	589295	21.836	18.427
Target Compounds							
8)	L2 AR-1221-1	5.213	0.000	23324	0	41.545	N.D. #
9)	L2 AR-1221-2	5.314	4.305	13001	8143	30.168	27.280
24)	L5 AR-1248-4	7.200f	0.000	10237	0	5.607	N.D. #
26)	L6 AR-1254-1	7.200	0.000	10237	0	5.821	N.D. #
28)	L6 AR-1254-3	7.820	0.000	14268	0	4.817	N.D. #
32)	L7 AR-1260-2	8.230	0.000	8360	0	3.262	N.D. #
35)	L7 AR-1260-5	0.000	7.896	0	19714	N.D.	5.365 #
37)	L8 AR-1262-2	0.000	7.896	0	19714	N.D.	5.029 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
Data File : PP036824.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2021 11:49
Operator : DD\AJ
Sample : M2856-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:56:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

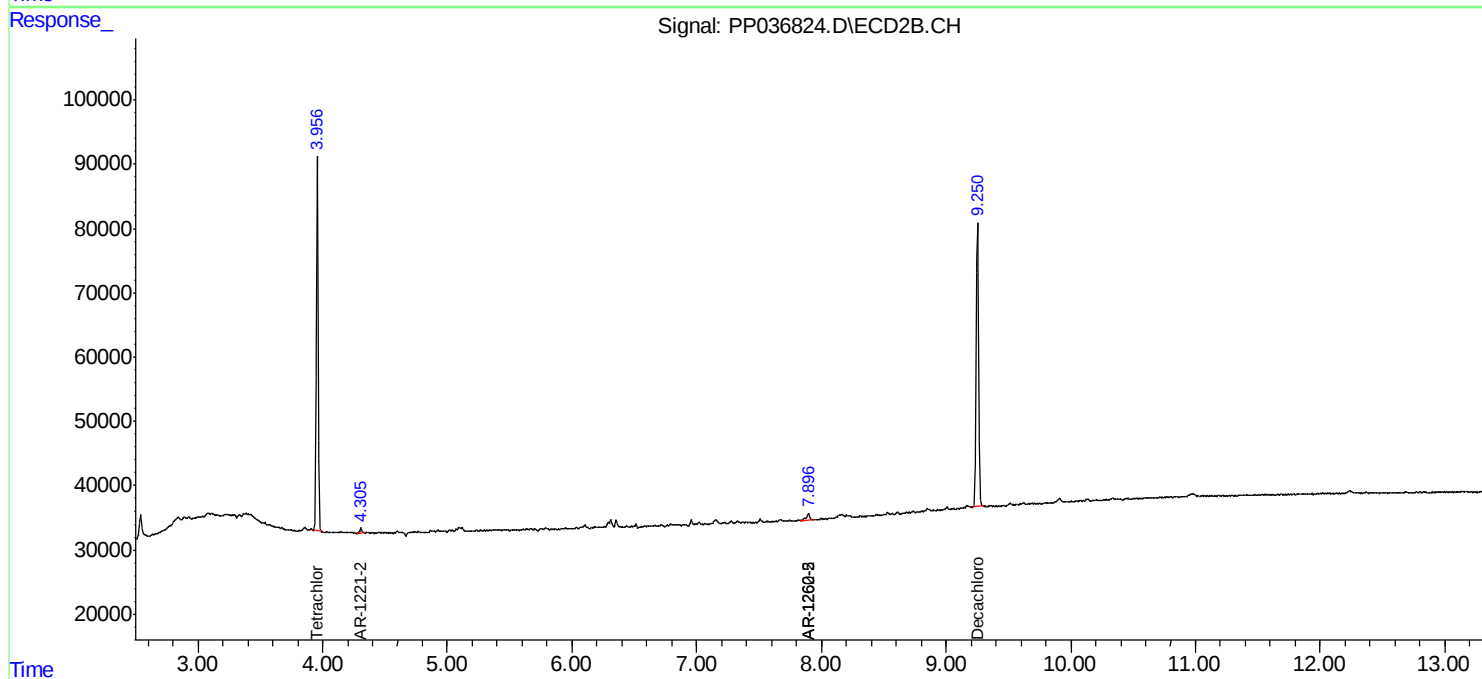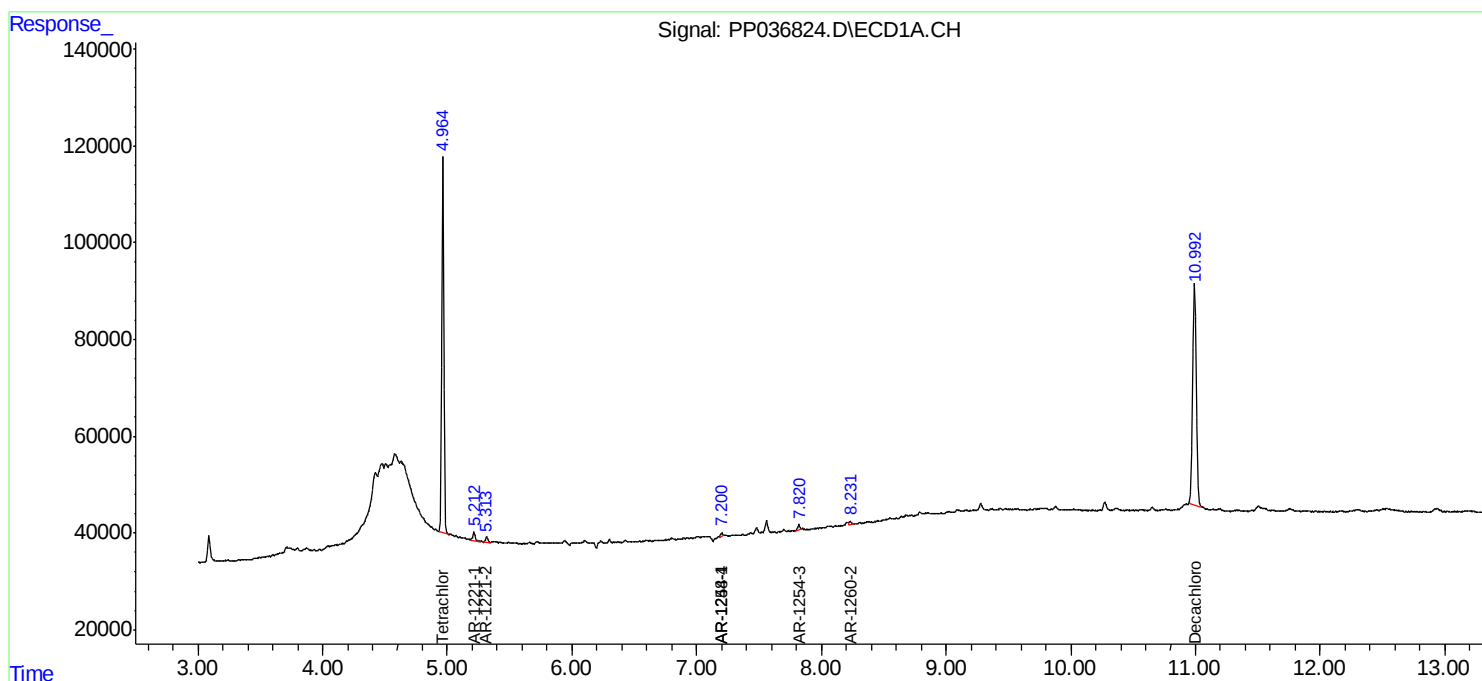


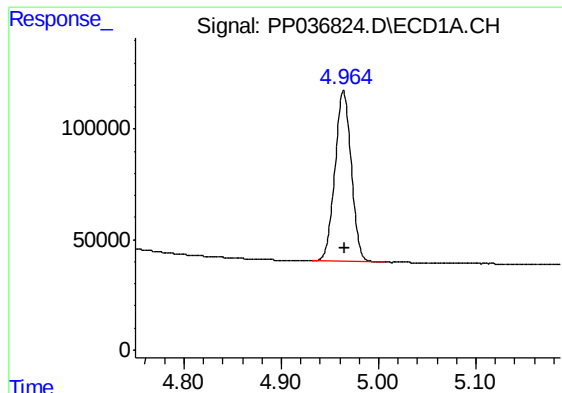

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 906997
Conc: 20.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

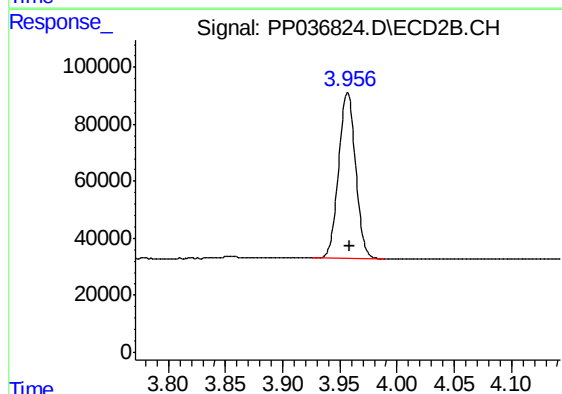


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.002 min
Response: 605362
Conc: 19.54 ng/ml

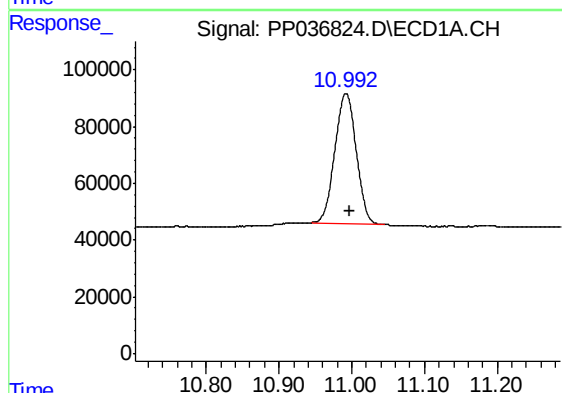


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.006 min
Response: 936711
Conc: 21.84 ng/ml

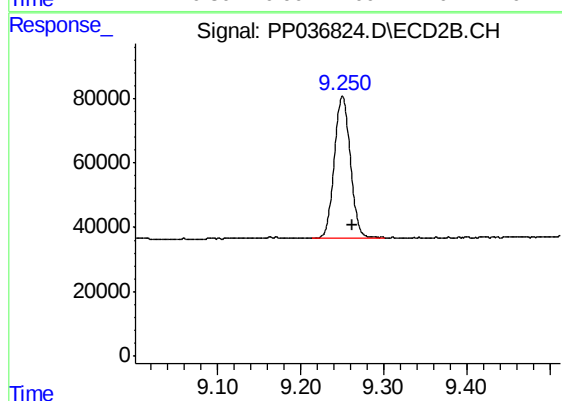

#2 Decachlorobiphenyl


R.T.: 9.250 min
Delta R.T.: -0.012 min
Response: 589295
Conc: 18.43 ng/ml

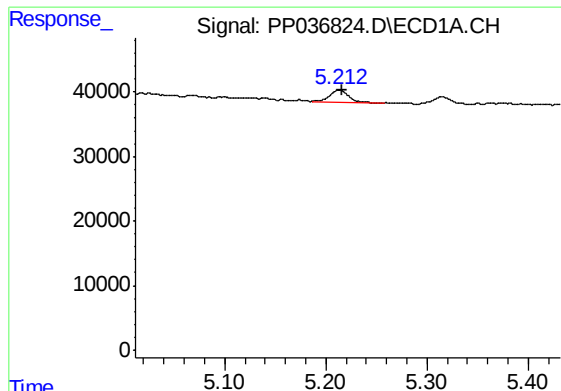

#8 AR-1221-1


R.T.: 5.213 min
Delta R.T.: -0.003 min
Response: 23324
Conc: 41.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

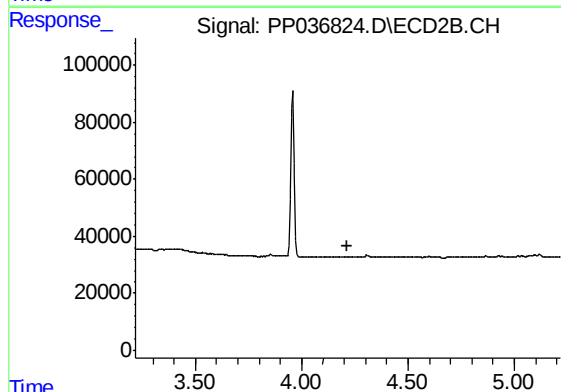


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

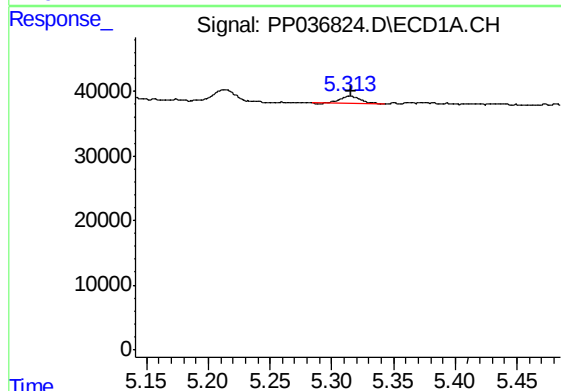


#9 AR-1221-2

R.T.: 5.314 min
Delta R.T.: -0.002 min
Response: 13001
Conc: 30.17 ng/ml

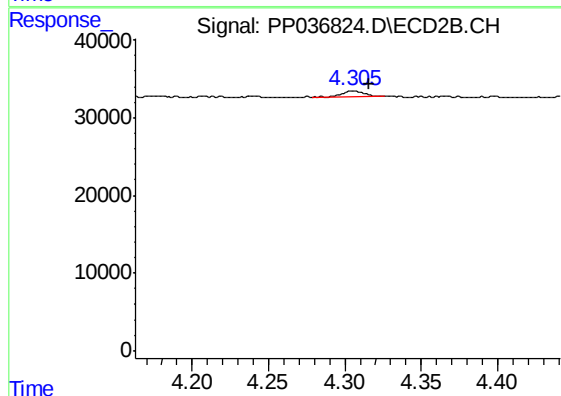

#9 AR-1221-2


R.T.: 4.305 min
Delta R.T.: -0.010 min
Response: 8143
Conc: 27.28 ng/ml

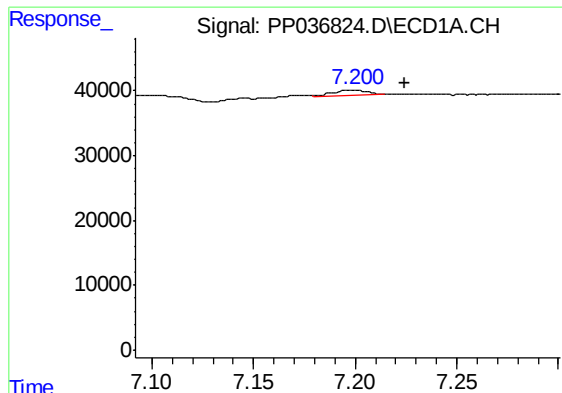

#24 AR-1248-4


R.T.: 7.200 min
Delta R.T.: -0.024 min
Response: 10237
Conc: 5.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

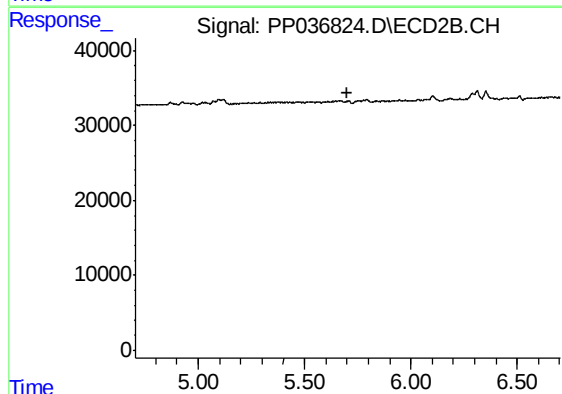


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

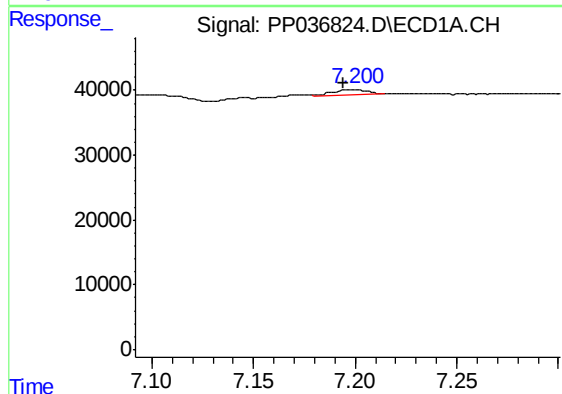


#26 AR-1254-1

R.T.: 7.200 min
Delta R.T.: 0.006 min
Response: 10237
Conc: 5.82 ng/ml

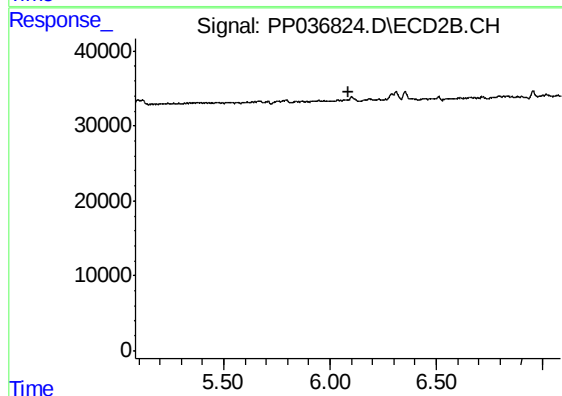

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

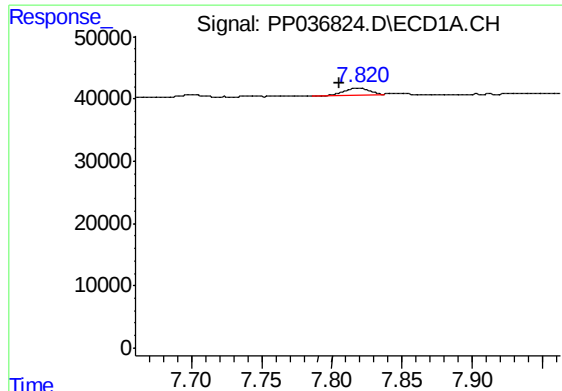

#28 AR-1254-3


R.T.: 7.820 min
Delta R.T.: 0.015 min
Response: 14268
Conc: 4.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

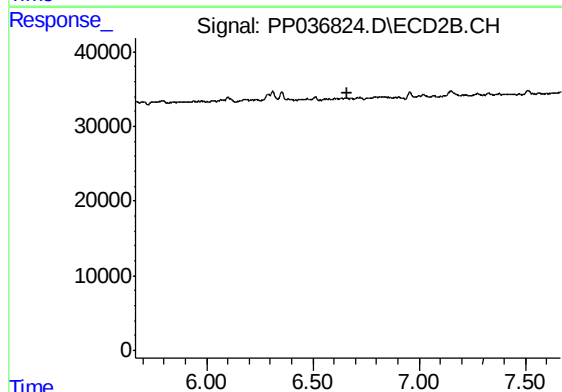


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

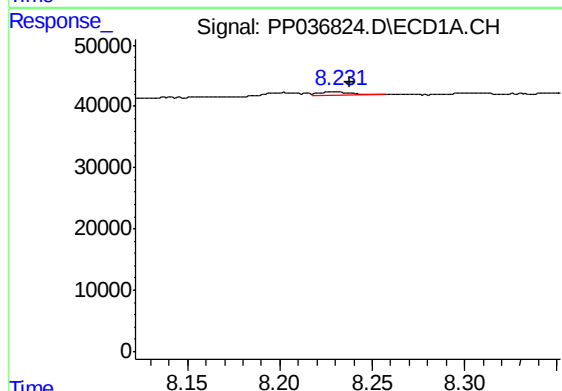


#32 AR-1260-2

R.T.: 8.230 min
Delta R.T.: -0.007 min
Response: 8360
Conc: 3.26 ng/ml

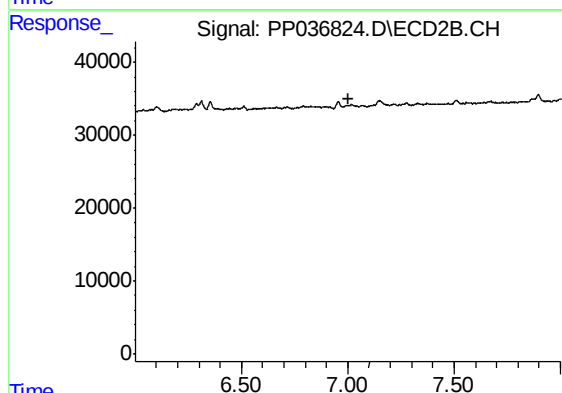

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.001 min
Response: 0
Conc: N.D.

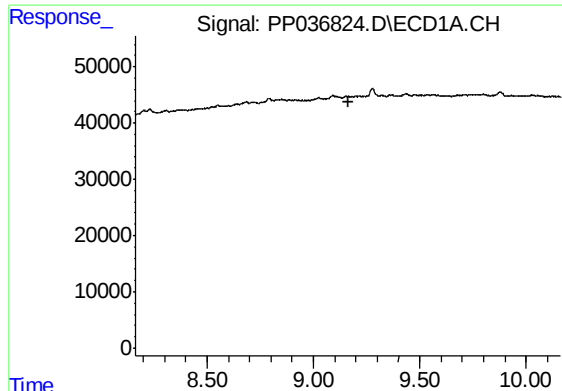

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 9.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

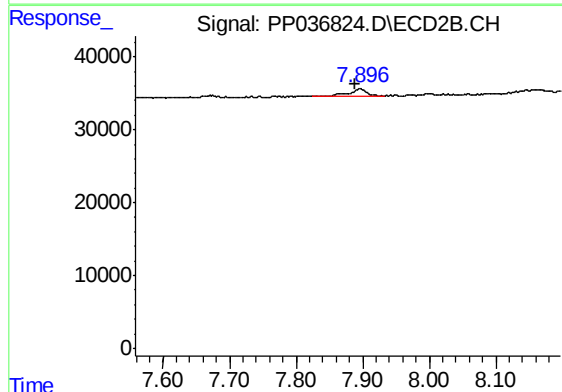


#35 AR-1260-5

R.T.: 7.896 min
Delta R.T.: 0.008 min
Response: 19714
Conc: 5.36 ng/ml

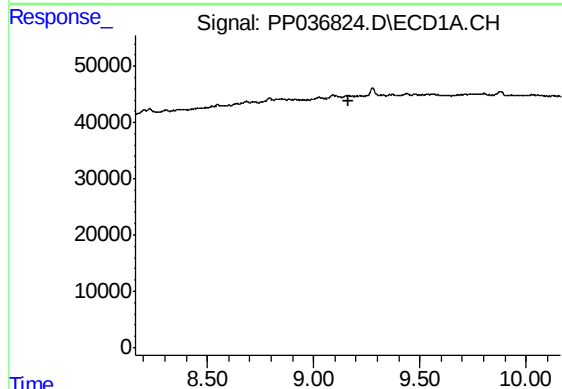

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.162 min
Response: 0
Conc: N.D.

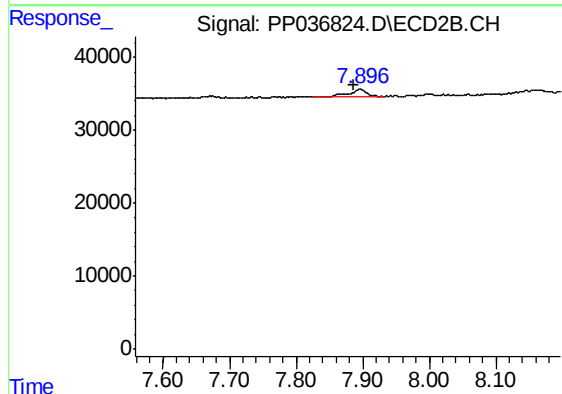

#37 AR-1262-2

R.T.: 7.896 min
Delta R.T.: 0.009 min
Response: 19714
Conc: 5.03 ng/ml