

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
 Data File : PP036830.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2021 13:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:58:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.956	878434	576982	19.875	18.628
2)	SA Decachlor...	10.993	9.252	949754	586754	22.140	18.347
Target Compounds							
9)	L2 AR-1221-2	5.315	4.305	11314	7631	26.254	25.565
15)	L3 AR-1232-5	6.572	0.000	21326	0	58.188	N.D. #
20)	L4 AR-1242-5	0.000	6.102f	0	21189	N.D.	25.970 #
22)	L5 AR-1248-2	6.572	0.000	21326	0	15.703	N.D. #
24)	L5 AR-1248-4	7.233	0.000	2020	0	1.106	N.D. #
25)	L5 AR-1248-5	0.000	6.102f	0	21189	N.D.	17.863 #
26)	L6 AR-1254-1	7.198	6.102f	44223	21189	25.146	12.505 #
28)	L6 AR-1254-3	7.819	0.000	14757	0	4.982	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
Data File : PP036830.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2021 13:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:58:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

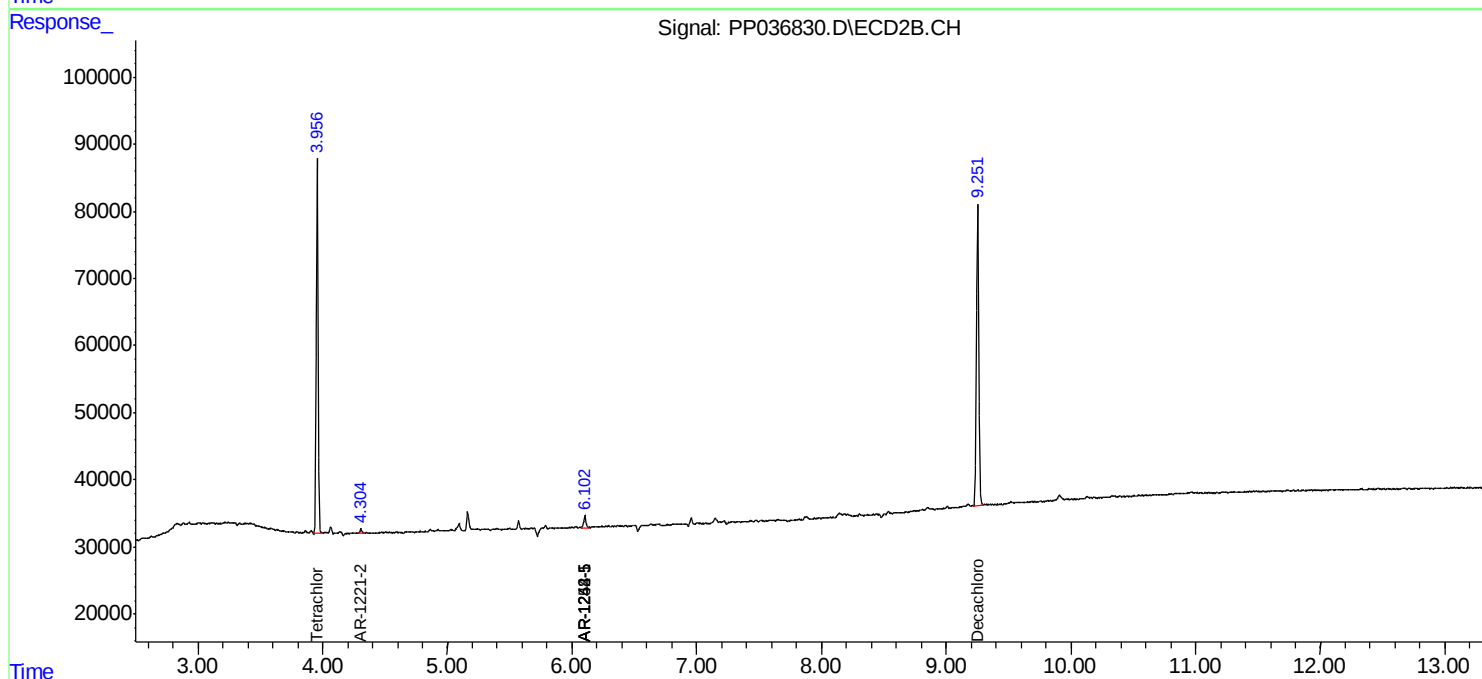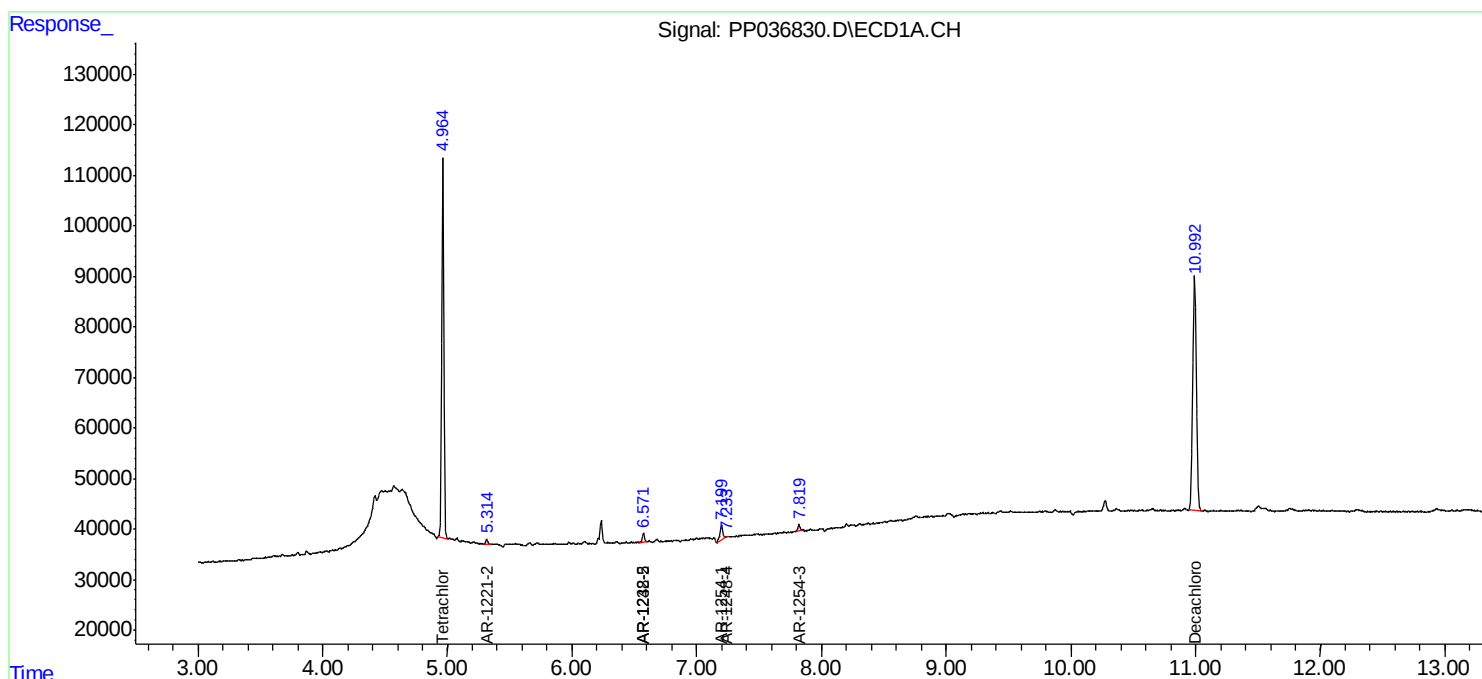


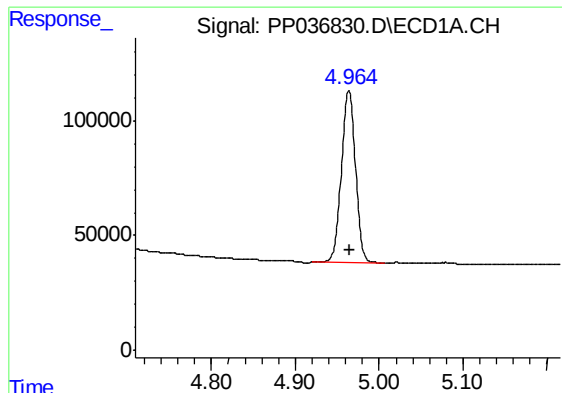

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 878434
Conc: 19.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

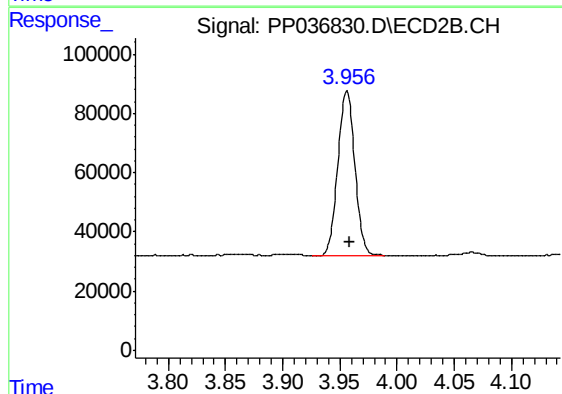


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.003 min
Response: 576982
Conc: 18.63 ng/ml

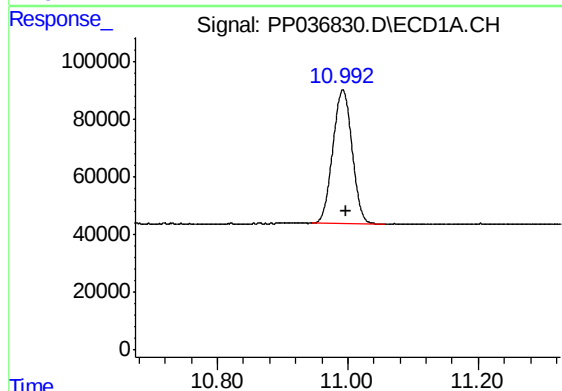


#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 949754
Conc: 22.14 ng/ml

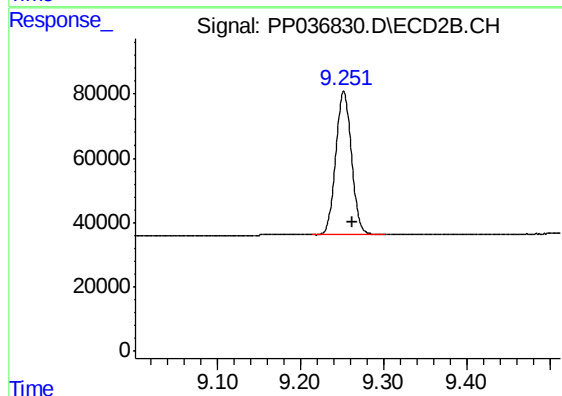

#2 Decachlorobiphenyl


R.T.: 9.252 min
Delta R.T.: -0.011 min
Response: 586754
Conc: 18.35 ng/ml

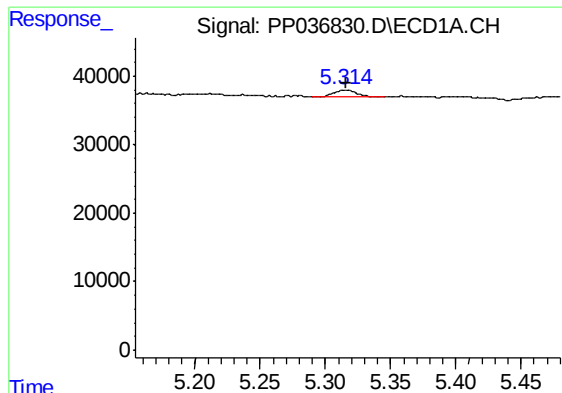

#9 AR-1221-2


R.T.: 5.315 min
Delta R.T.: 0.000 min
Response: 11314
Conc: 26.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

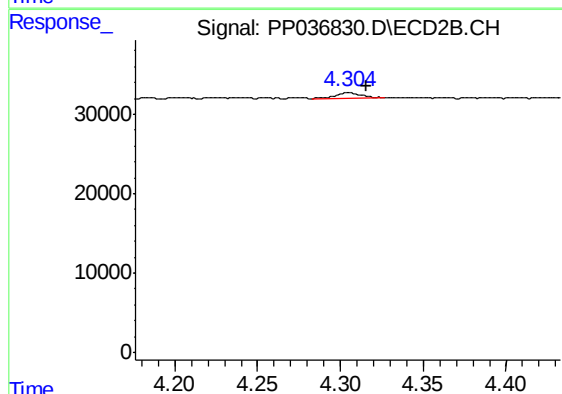


#9 AR-1221-2

R.T.: 4.305 min
Delta R.T.: -0.011 min
Response: 7631
Conc: 25.56 ng/ml

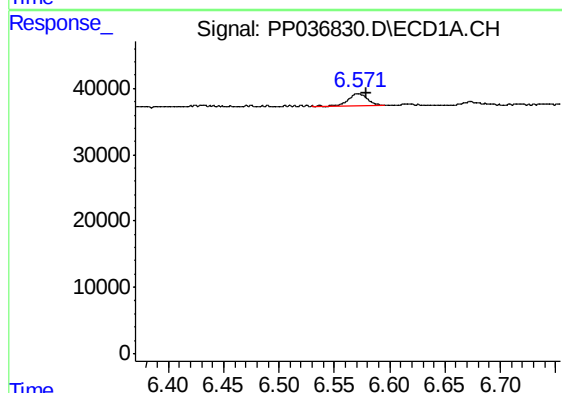


#15 AR-1232-5

R.T.: 6.572 min
Delta R.T.: -0.007 min
Response: 21326
Conc: 58.19 ng/ml

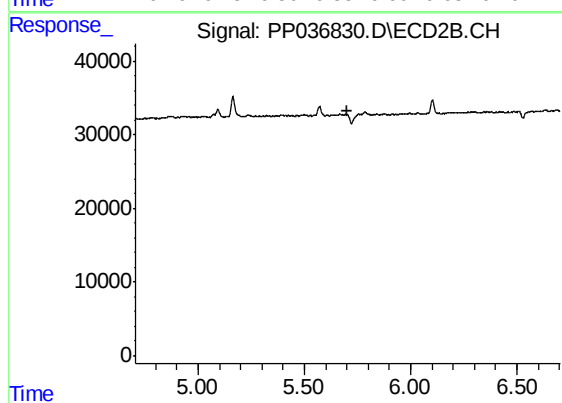

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

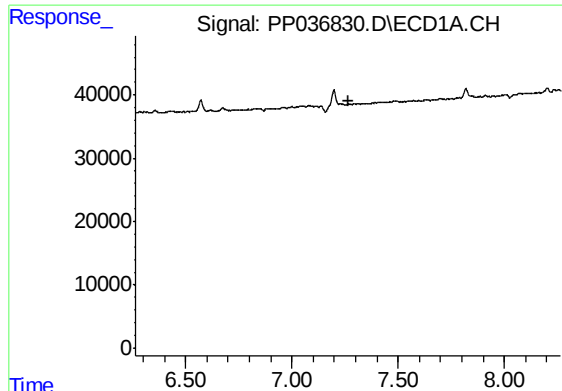

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

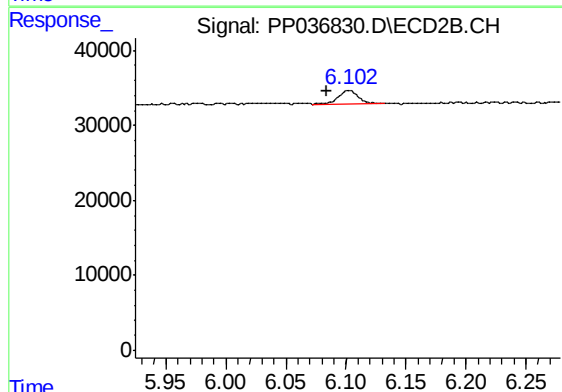


#20 AR-1242-5

R.T.: 6.102 min
Delta R.T.: 0.018 min
Response: 21189
Conc: 25.97 ng/ml

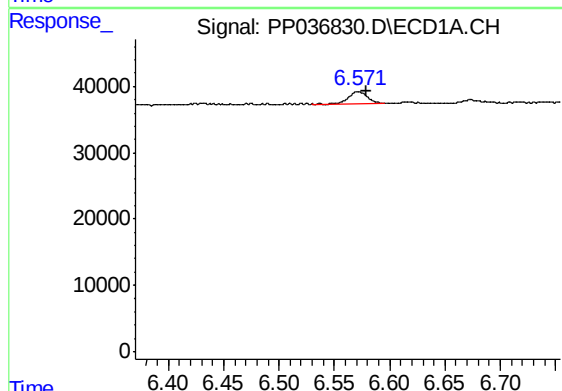


#22 AR-1248-2

R.T.: 6.572 min
Delta R.T.: -0.007 min
Response: 21326
Conc: 15.70 ng/ml

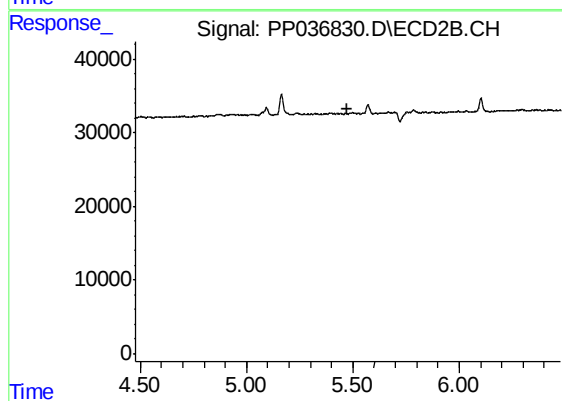

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

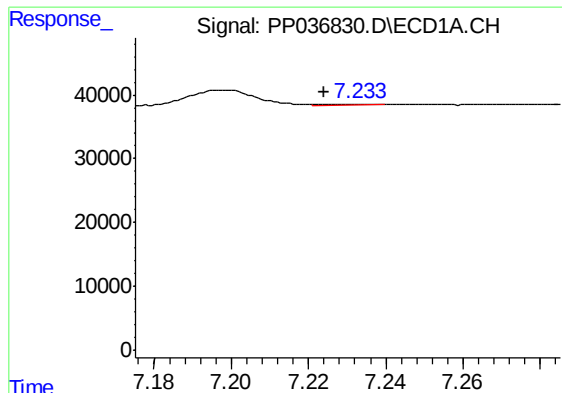

#24 AR-1248-4


R.T.: 7.233 min
Delta R.T.: 0.009 min
Response: 2020
Conc: 1.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

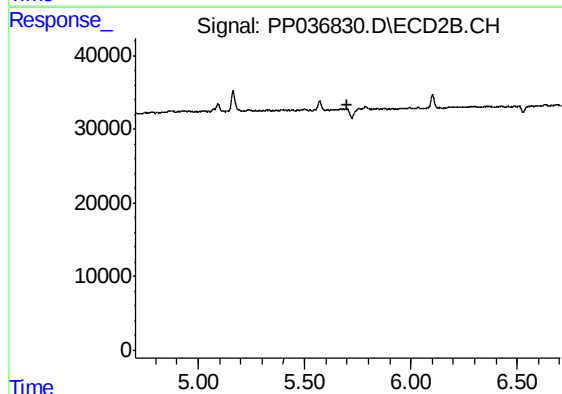


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

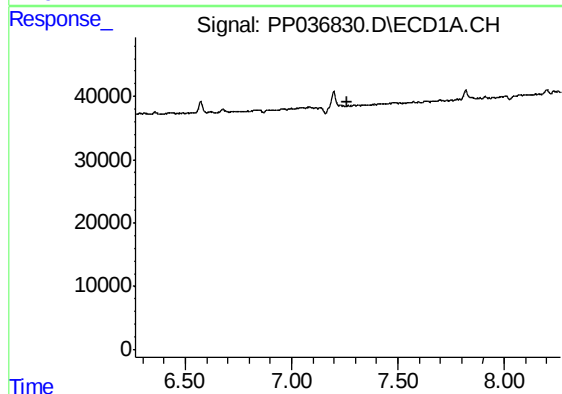


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

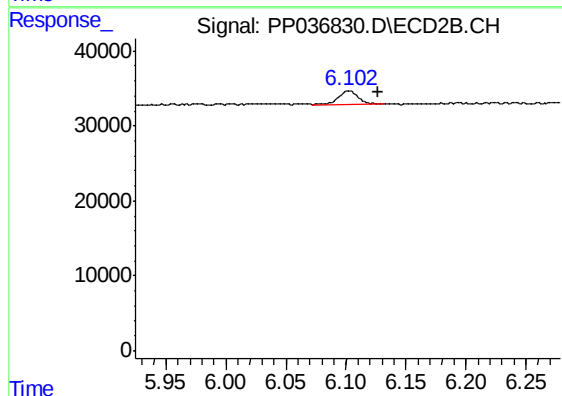

#25 AR-1248-5


R.T.: 6.102 min
Delta R.T.: -0.025 min
Response: 21189
Conc: 17.86 ng/ml

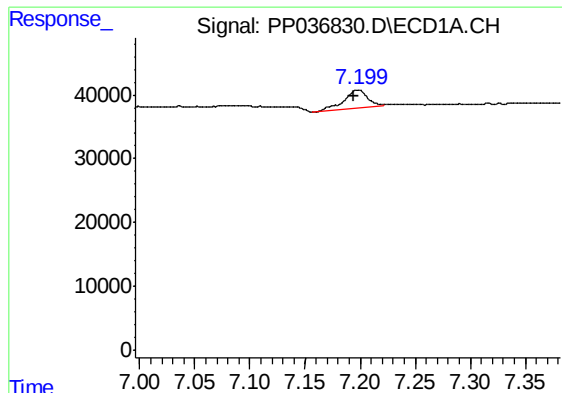

#26 AR-1254-1


R.T.: 7.198 min
Delta R.T.: 0.004 min
Response: 44223
Conc: 25.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

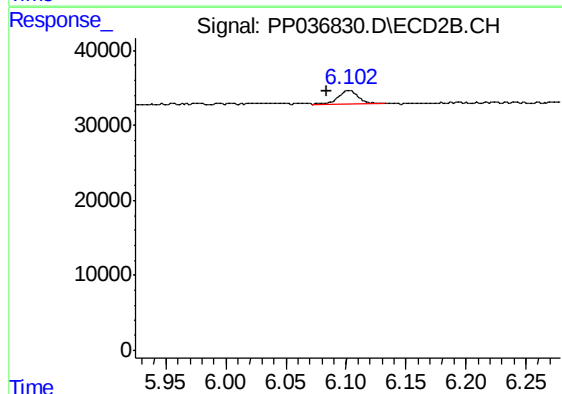


#26 AR-1254-1

R.T.: 6.102 min
Delta R.T.: 0.018 min
Response: 21189
Conc: 12.51 ng/ml

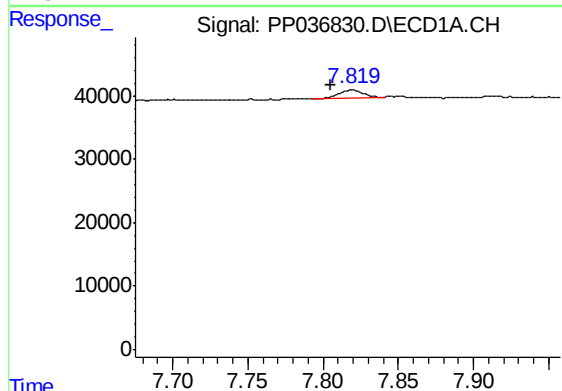

#28 AR-1254-3

R.T.: 7.819 min
Delta R.T.: 0.014 min
Response: 14757
Conc: 4.98 ng/ml

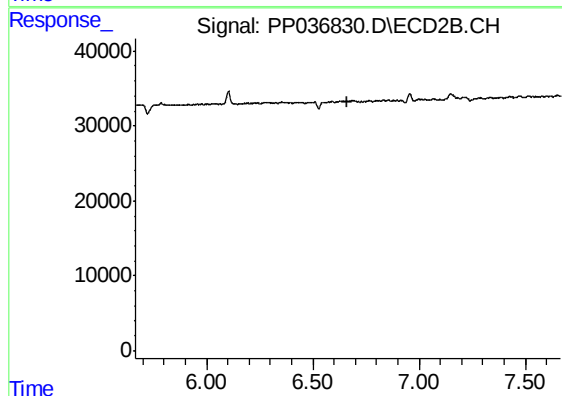

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.