

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
 Data File : PP036820.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2021 10:41
 Operator : DD\AJ
 Sample : M2856-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-02-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:54:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.963	3.955	902124	615849	20.411	19.883
2)	SA Decachlor...	10.991	9.250	895430	563820	20.874	17.630

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
Data File : PP036820.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2021 10:41
Operator : DD\AJ
Sample : M2856-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-02-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:54:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

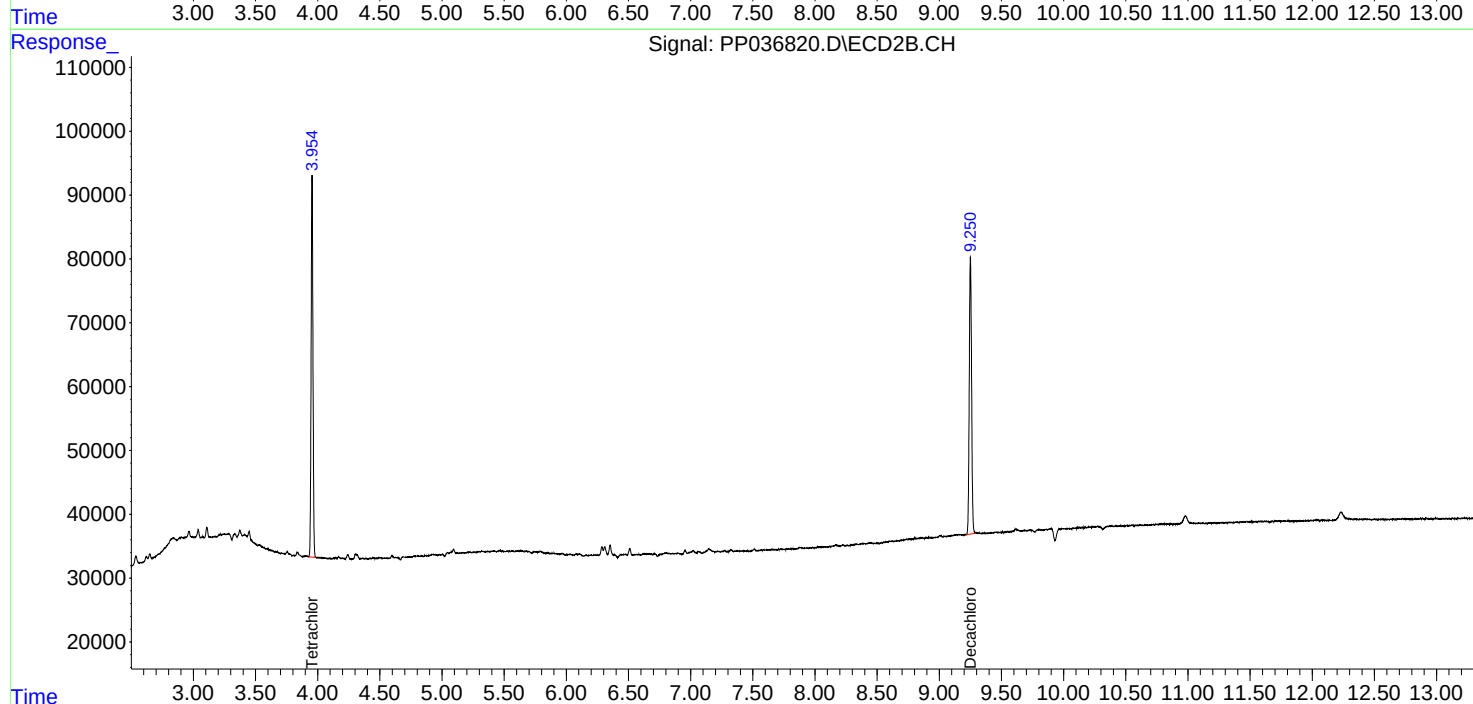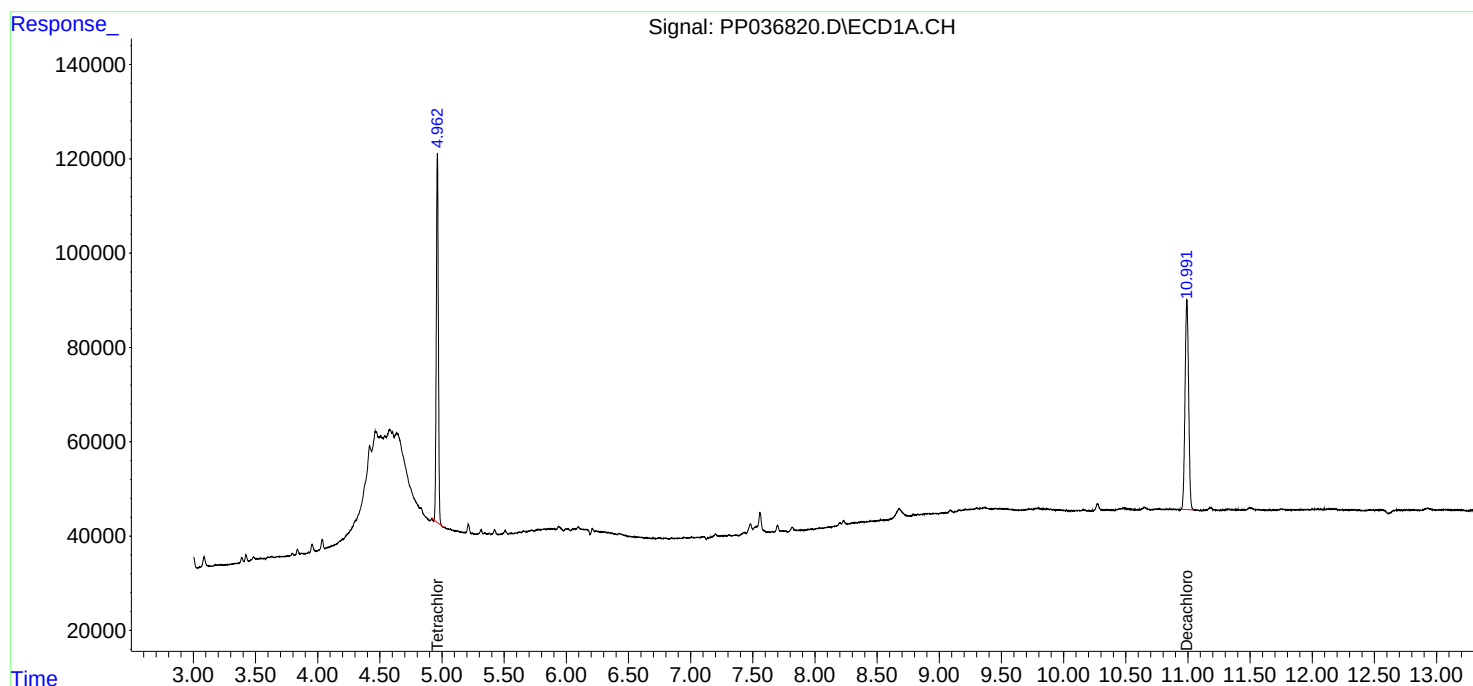


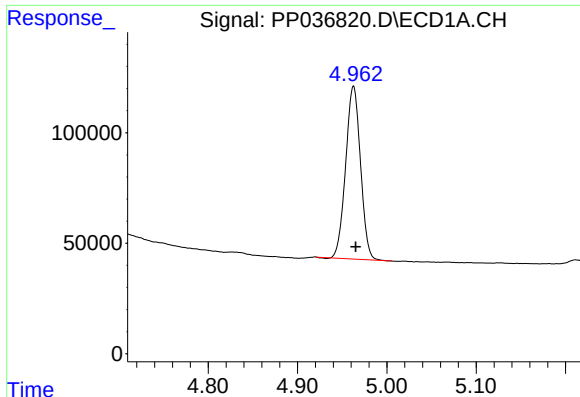

#1 Tetrachloro-m-xylene


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 902124
Conc: 20.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-02-COMP

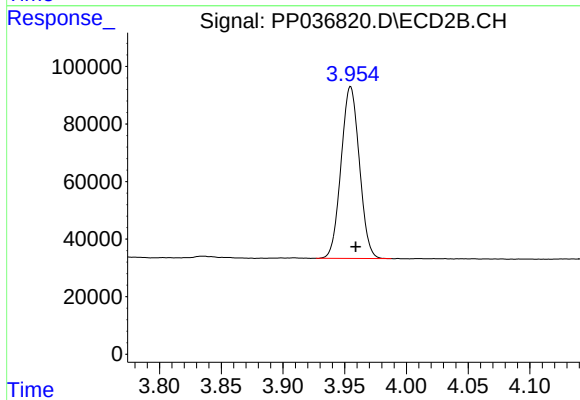


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 615849
Conc: 19.88 ng/ml

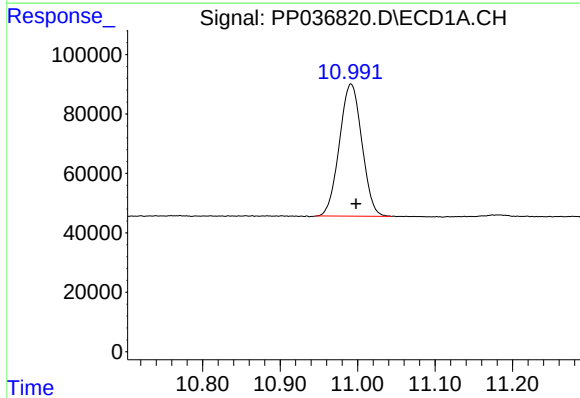

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.007 min
Response: 895430
Conc: 20.87 ng/ml

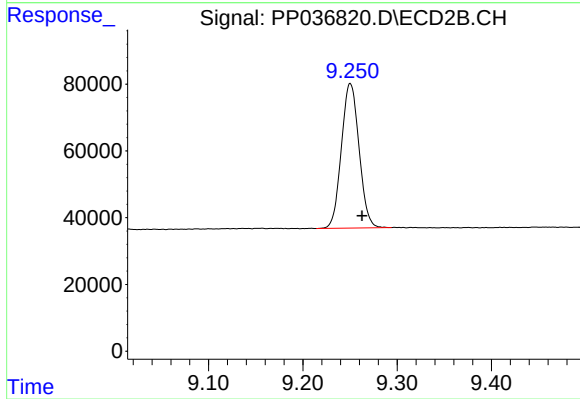

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.013 min
Response: 563820
Conc: 17.63 ng/ml