

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
 Data File : PP036831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2021 13:48
 Operator : DD\AJ
 Sample : M2866-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 124055

Manual Integrations
 APPROVED

mohammad
 6/29/2021 1:34:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:59:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.955	869289	575958	19.668	18.595
2) SA Decachlor...	10.991	9.249	943096	593482	21.985m	18.558m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062821\
Data File : PP036831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2021 13:48
Operator : DD\AJ
Sample : M2866-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
124055


Manual Integrations
APPROVED

mohammad
6/29/2021 1:34:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:59:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

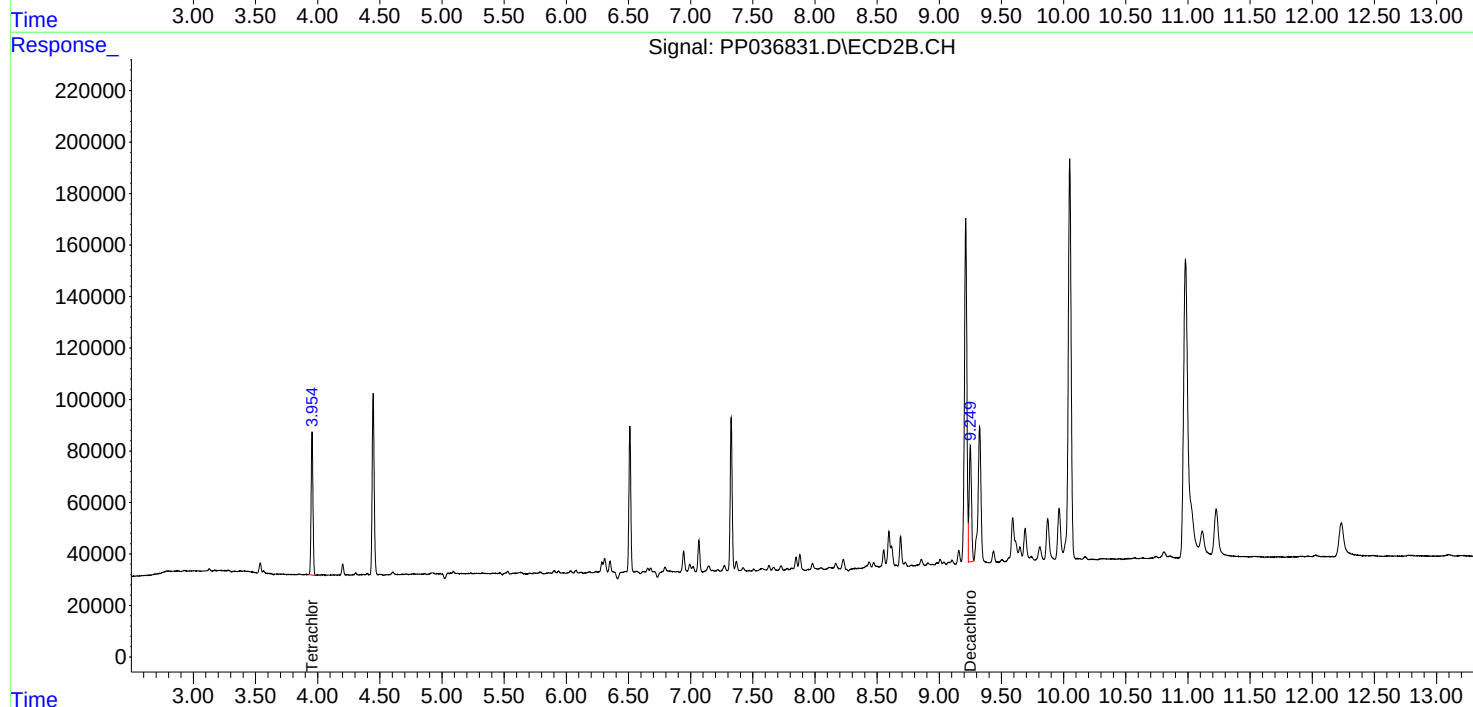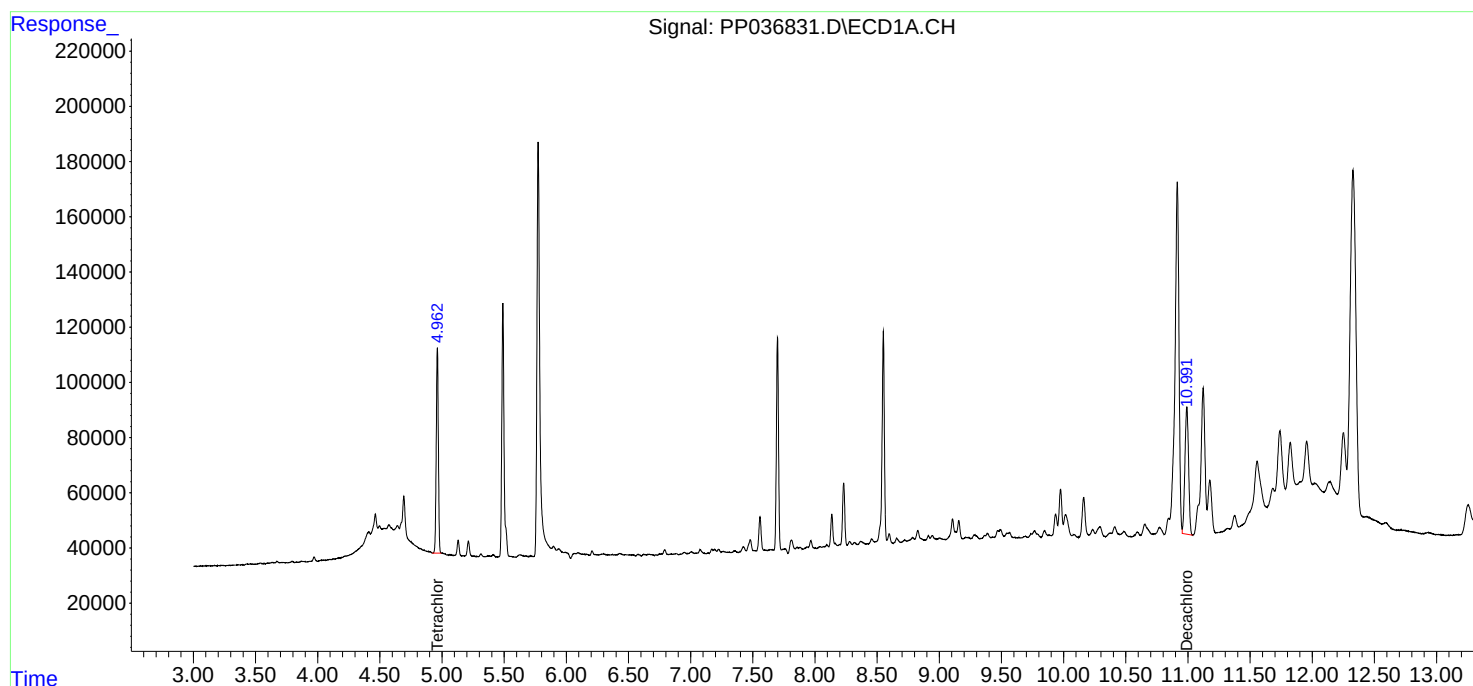

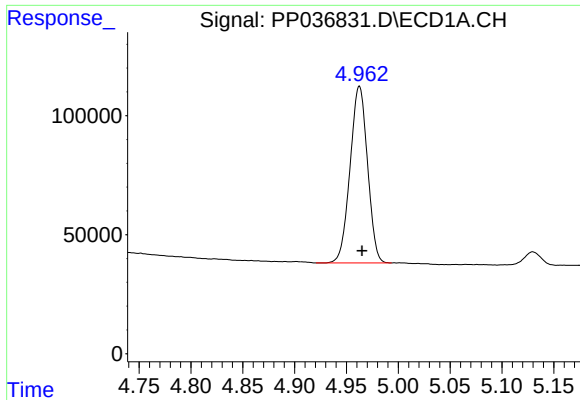


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 869289
Conc: 19.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
124055


Manual Integrations
APPROVED

mohammad
6/29/2021 1:34:20 PM

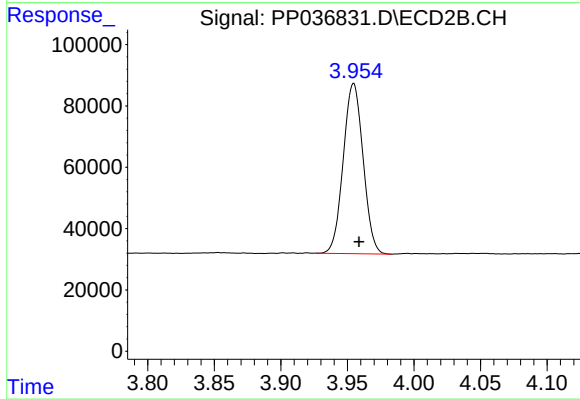


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 575958
Conc: 18.60 ng/ml

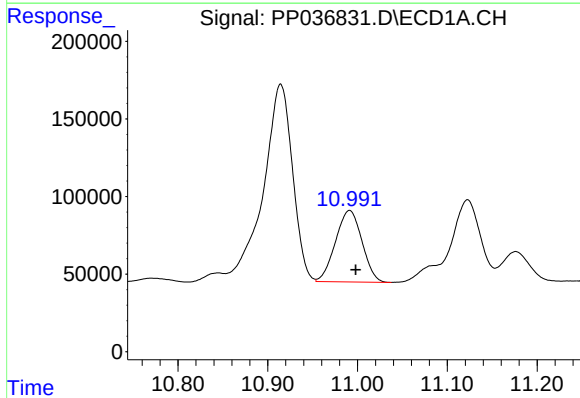

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.007 min
Response: 943096
Conc: 21.98 ng/ml m

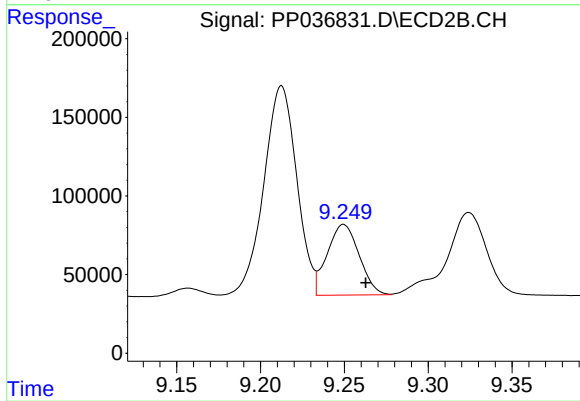

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.014 min
Response: 593482
Conc: 18.56 ng/ml m