

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062921\
 Data File : PP036875.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jun 2021 17:31
 Operator : DD\AJ
 Sample : M2886-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20426

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 01:37:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.961	3.954	542622	340545	12.277	10.995
2) SA Decachlor...	10.992	9.249	613618	350635	14.304	10.964
Target Compounds						
8) L2 AR-1221-1	5.211	0.000	25296	0	45.057	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062921\
Data File : PP036875.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jun 2021 17:31
Operator : DD\AJ
Sample : M2886-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20426

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 01:37:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

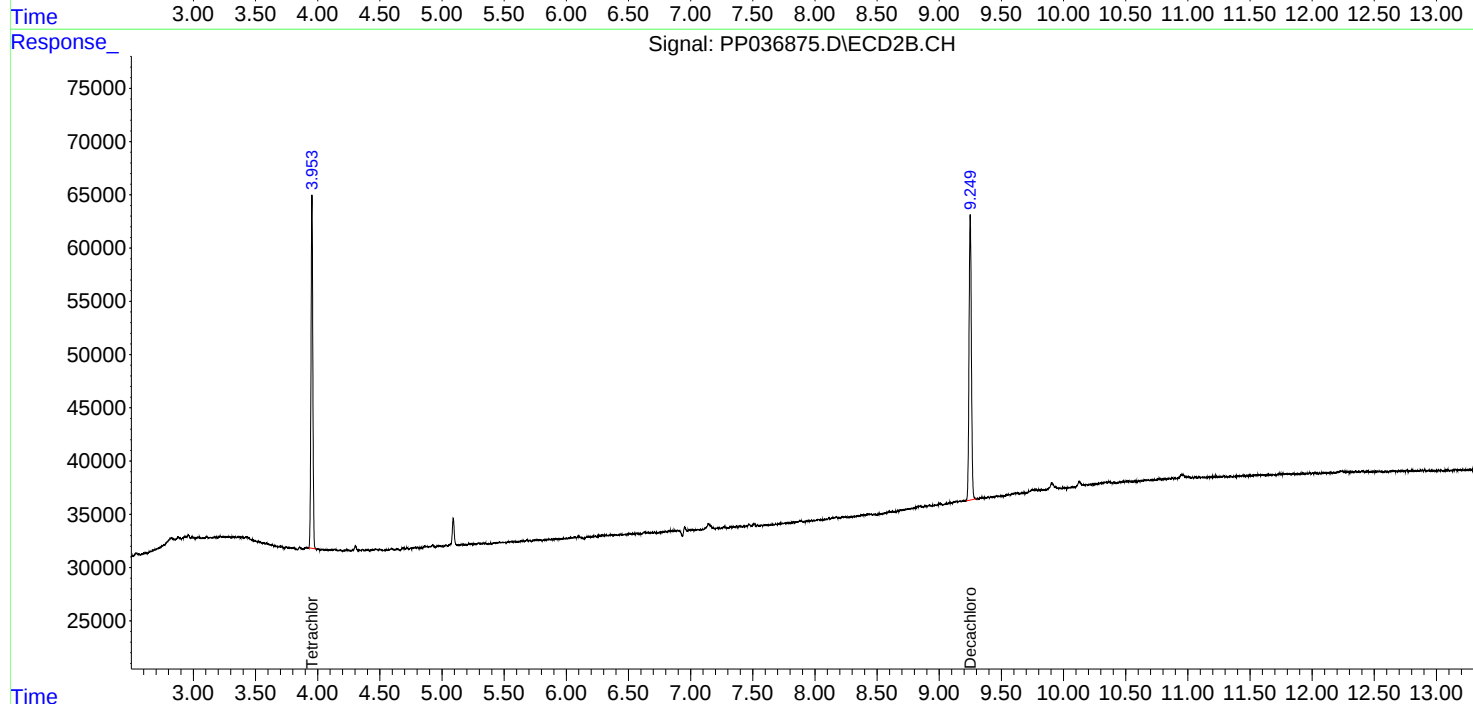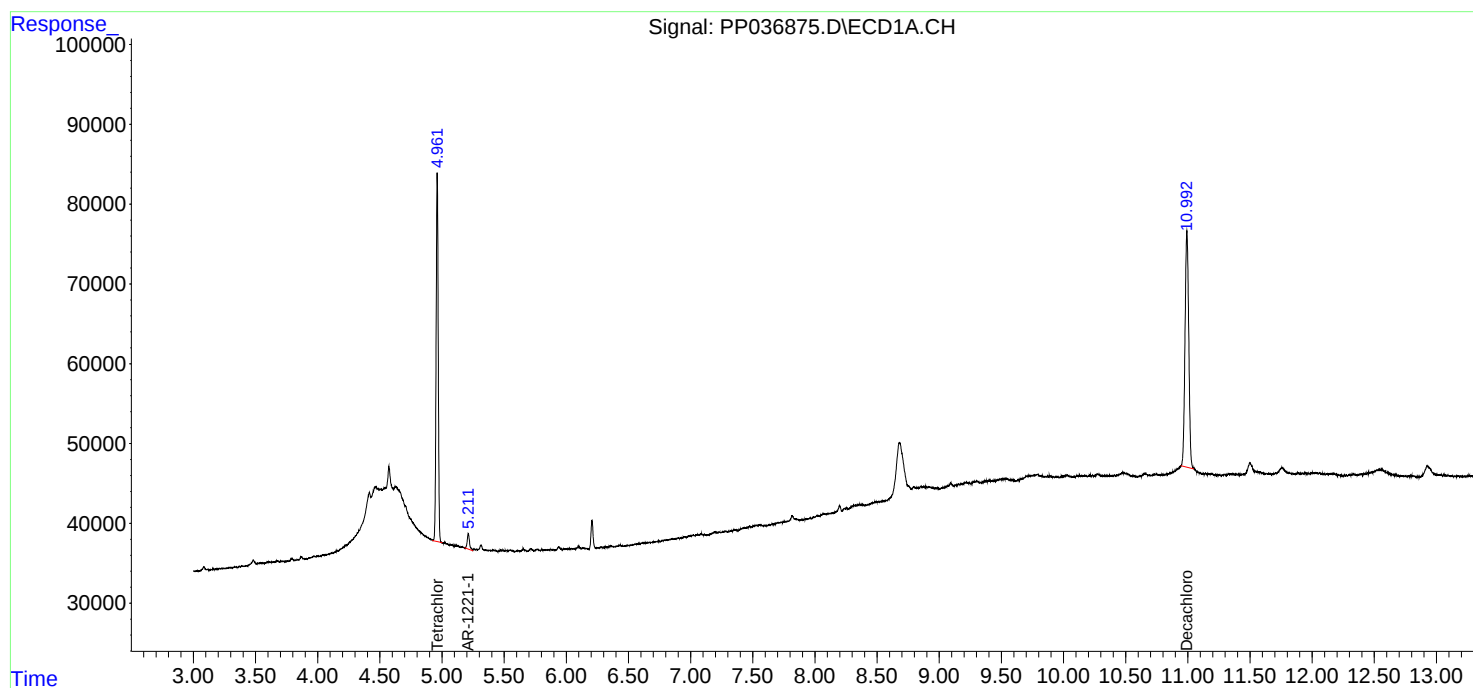


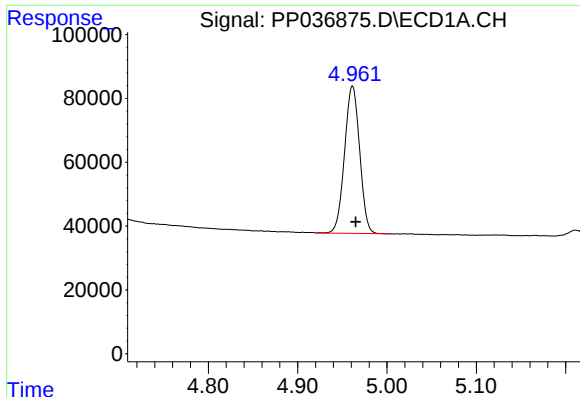

#1 Tetrachloro-m-xylene


R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 542622
Conc: 12.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
20426

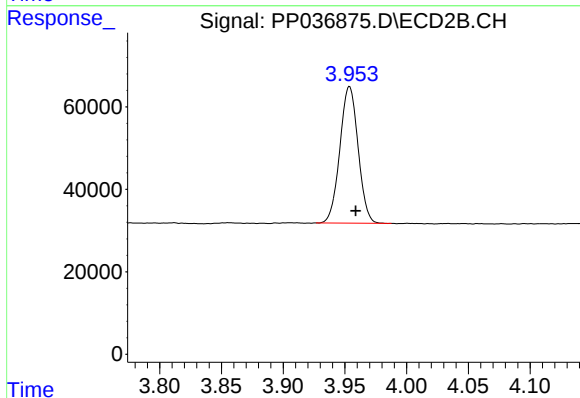


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 340545
Conc: 10.99 ng/ml

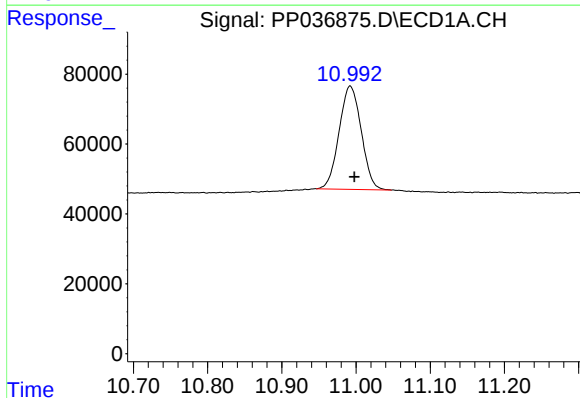


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.006 min
Response: 613618
Conc: 14.30 ng/ml

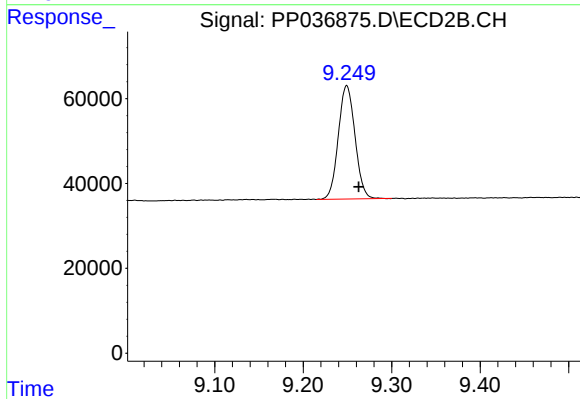

#2 Decachlorobiphenyl


R.T.: 9.249 min
Delta R.T.: -0.014 min
Response: 350635
Conc: 10.96 ng/ml

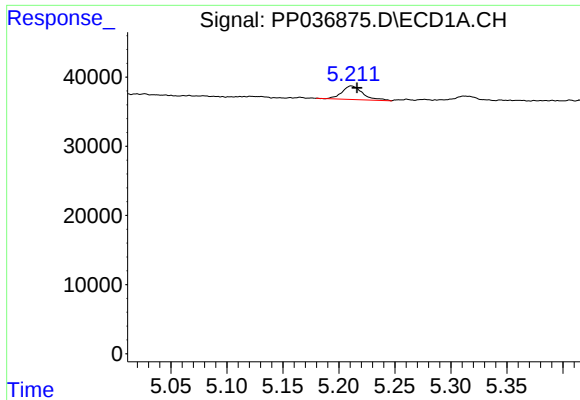

#8 AR-1221-1

R.T.: 5.211 min
Delta R.T.: -0.005 min
Response: 25296
Conc: 45.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
20426

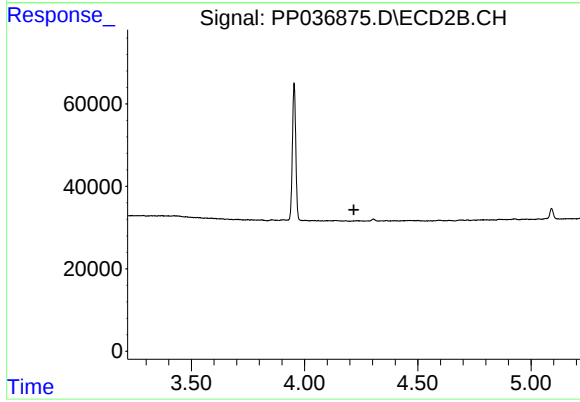

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.