

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062921\
 Data File : PP036869.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jun 2021 15:50
 Operator : DD\AJ
 Sample : M2882-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SPILL-COMP-31277-AUD-1077

Manual Integrations
 APPROVED

mohammad
 6/30/2021 2:05:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 08:13:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.954	808994	531277	18.304	17.153
2) SA Decachlor...	10.992	9.252	895353	487224	20.872	15.235 #
Target Compounds						
31) L7 AR-1260-1	7.970	6.796	62000	36120	28.565	22.434
32) L7 AR-1260-2	8.234	6.995	103589	55125	40.418	28.426 #
33) L7 AR-1260-3	8.589	7.146	25900	61584	12.921	33.861 #
34) L7 AR-1260-4	8.822	7.666f	75610	121030	31.913m	78.046 #
35) L7 AR-1260-5	9.158	7.881	26544	21288	5.949m	5.793

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062921\
Data File : PP036869.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jun 2021 15:50
Operator : DD\AJ
Sample : M2882-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SPILL-COMP-31277-AUD-1077


Manual Integrations
APPROVED

mohammad
6/30/2021 2:05:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 08:13:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

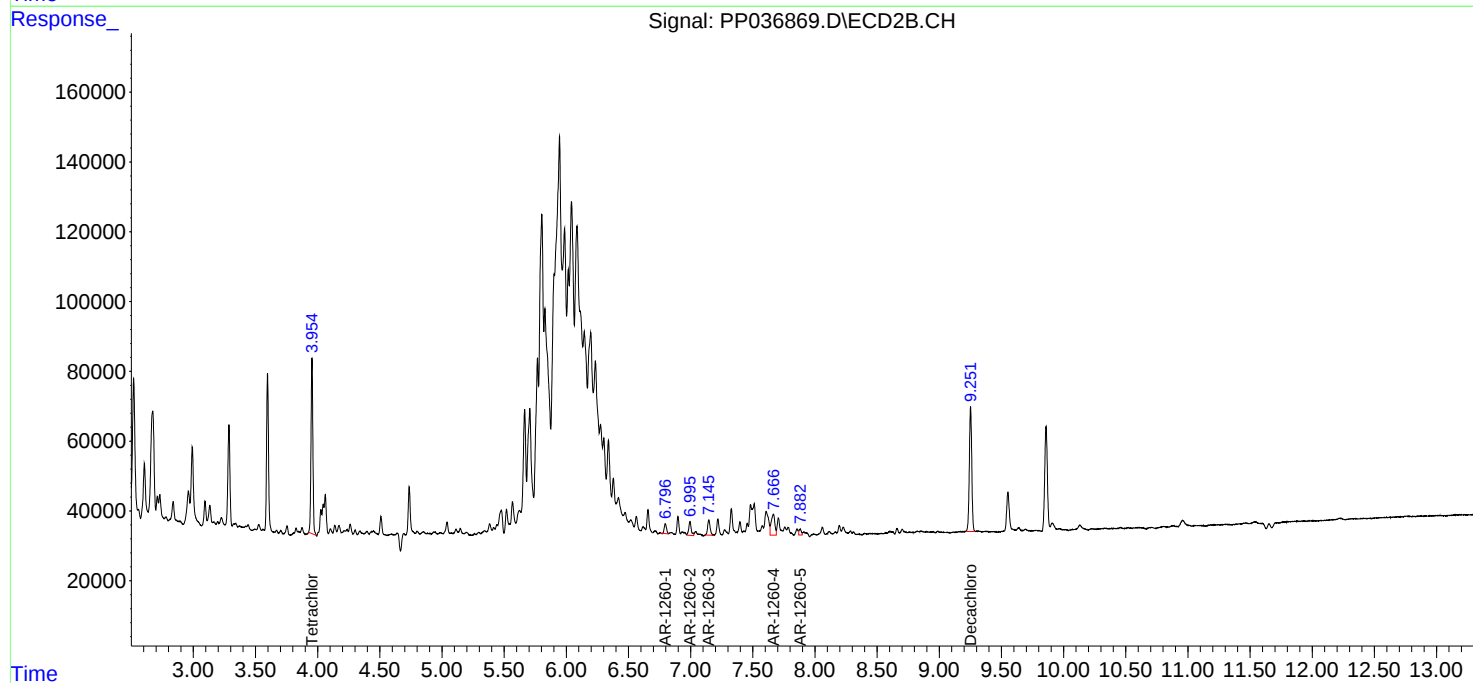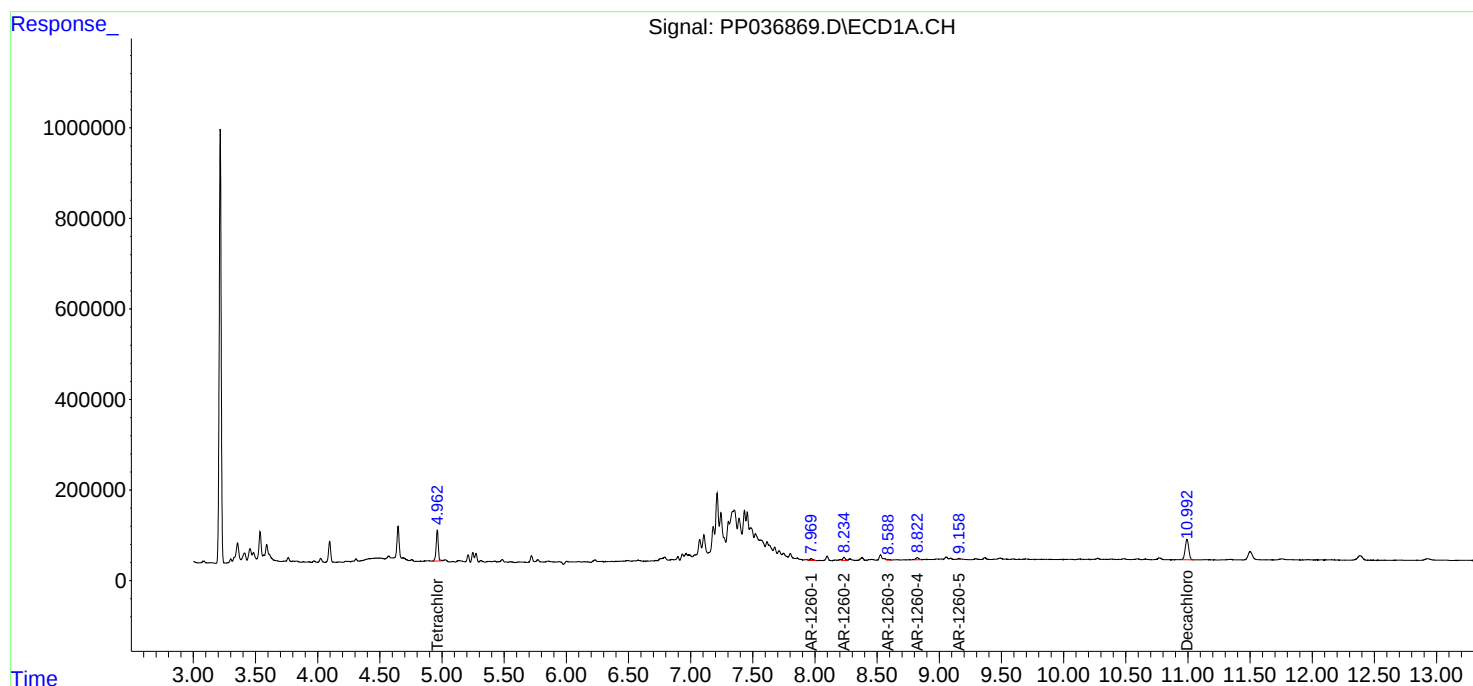

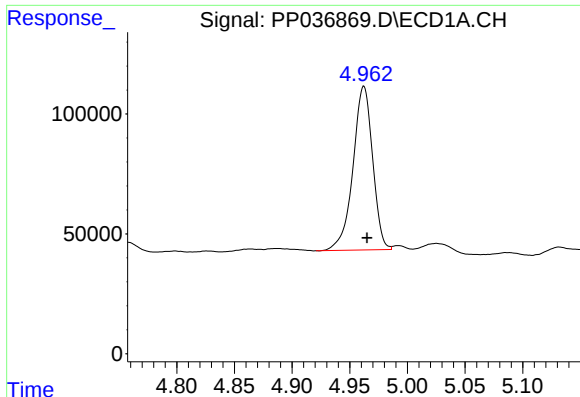


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 808994
Conc: 18.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
SPILL-COMP-31277-AUD-1077


Manual Integrations
APPROVED

mohammad
6/30/2021 2:05:43 PM

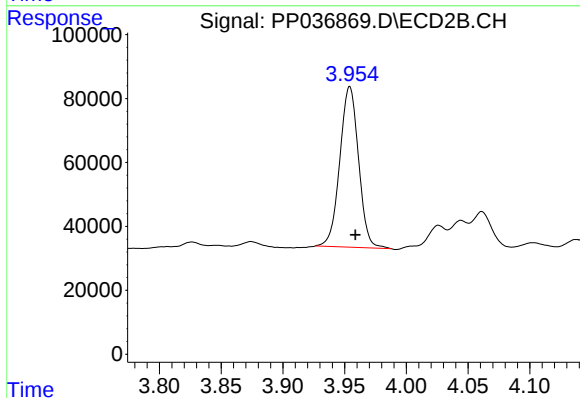


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 531277
Conc: 17.15 ng/ml

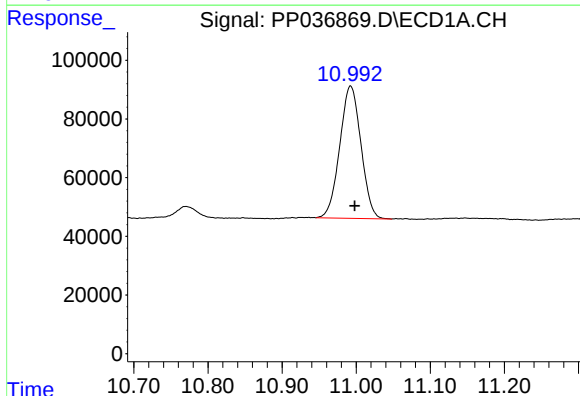


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.005 min
Response: 895353
Conc: 20.87 ng/ml

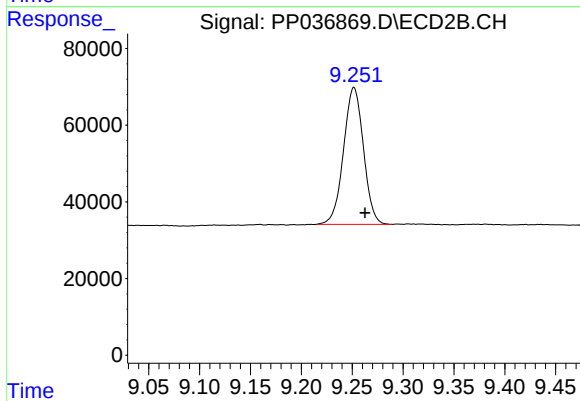

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.011 min
Response: 487224
Conc: 15.24 ng/ml

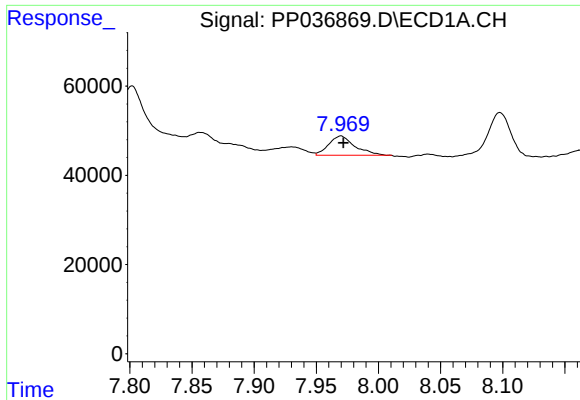


#31 AR-1260-1

R.T.: 7.970 min
Delta R.T.: -0.002 min
Response: 62000
Conc: 28.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
SPILL-COMP-31277-AUD-1077


Manual Integrations
APPROVED

mohammad
6/30/2021 2:05:43 PM

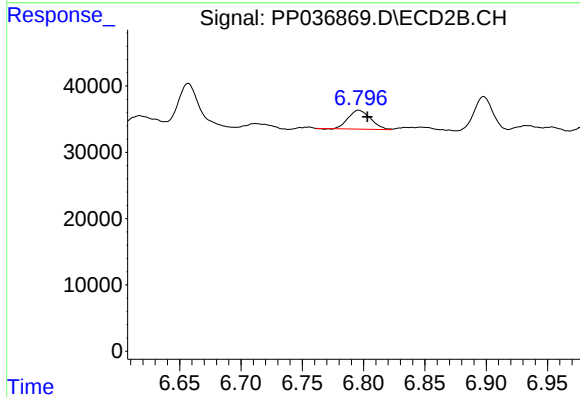


#31 AR-1260-1

R.T.: 6.796 min
Delta R.T.: -0.007 min
Response: 36120
Conc: 22.43 ng/ml

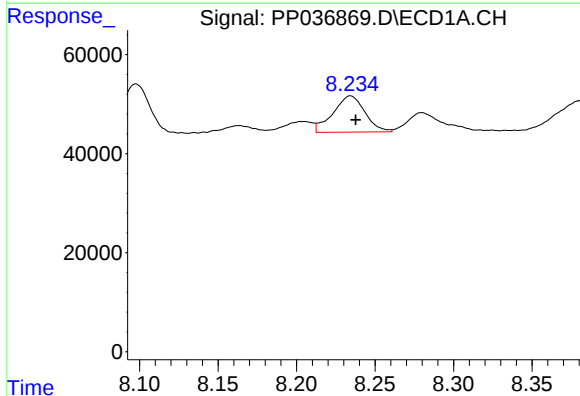


#32 AR-1260-2

R.T.: 8.234 min
Delta R.T.: -0.003 min
Response: 103589
Conc: 40.42 ng/ml

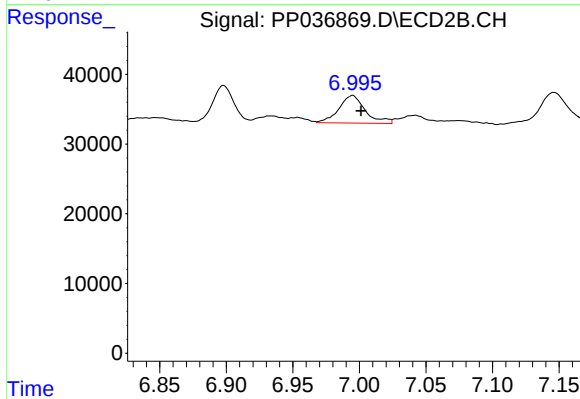

#32 AR-1260-2

R.T.: 6.995 min
Delta R.T.: -0.006 min
Response: 55125
Conc: 28.43 ng/ml

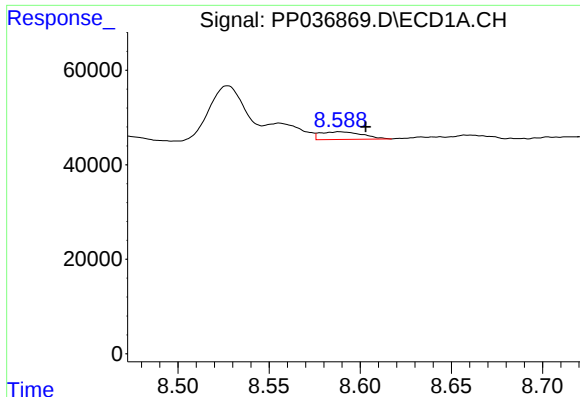


#33 AR-1260-3

R.T.: 8.589 min
Delta R.T.: -0.014 min
Response: 25900
Conc: 12.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
SPILL-COMP-31277-AUD-1077


Manual Integrations
APPROVED

mohammad
6/30/2021 2:05:43 PM

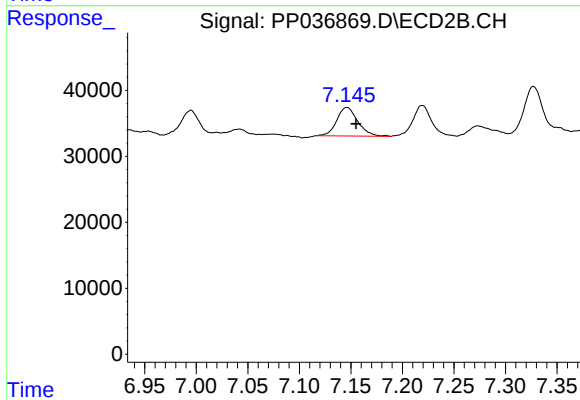


#33 AR-1260-3

R.T.: 7.146 min
Delta R.T.: -0.009 min
Response: 61584
Conc: 33.86 ng/ml

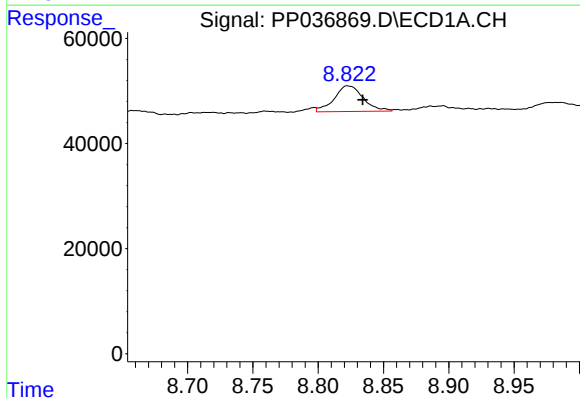


#34 AR-1260-4

R.T.: 8.822 min
Delta R.T.: -0.012 min
Response: 75610
Conc: 31.91 ng/ml m

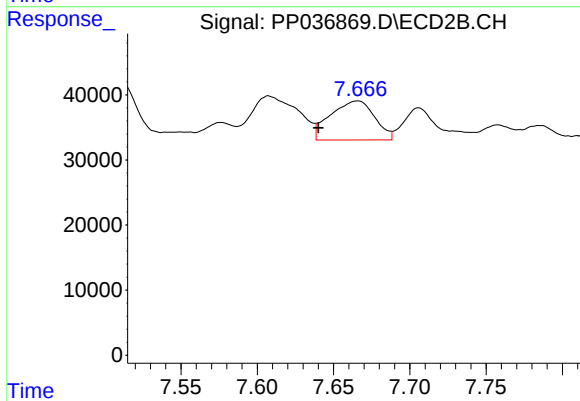

#34 AR-1260-4

R.T.: 7.666 min
Delta R.T.: 0.026 min
Response: 121030
Conc: 78.05 ng/ml

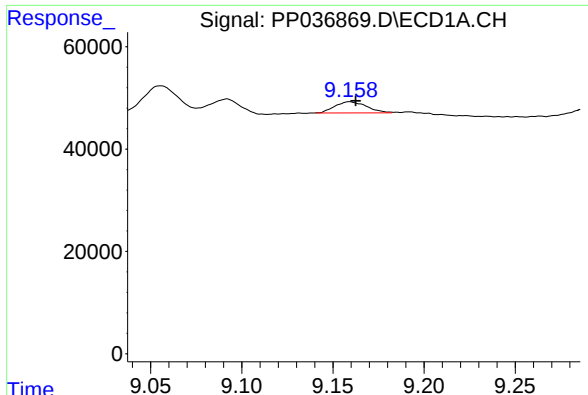


#35 AR-1260-5

R.T.: 9.158 min
Delta R.T.: -0.004 min
Response: 26544
Conc: 5.95 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SPILL-COMP-31277-AUD-1077

Manual Integrations
APPROVED

mohammad
6/30/2021 2:05:43 PM

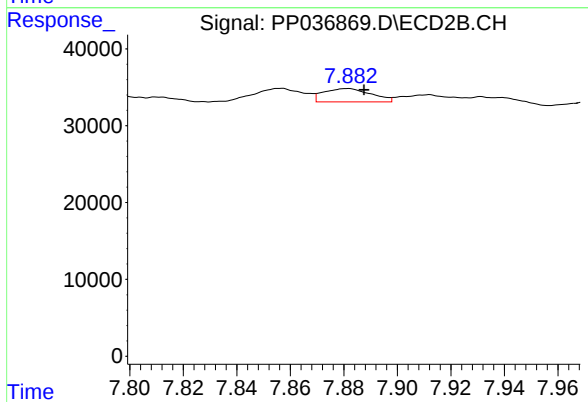

#35 AR-1260-5

R.T.: 7.881 min
Delta R.T.: -0.006 min
Response: 21288
Conc: 5.79 ng/ml