

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062921\
 Data File : PP036895.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2021 00:02
 Operator : DD\AJ
 Sample : M2881-06 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC123047LOK-END-1-2

Manual Integrations
 APPROVED

mohammad
 6/30/2021 2:06:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 01:44:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.954	87720	94611	1.985m	3.055m#
2) SA Decachlor...	10.993	9.252	113205	55046	2.639	1.721 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062921\
Data File : PP036895.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2021 00:02
Operator : DD\AJ
Sample : M2881-06 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC123047LOK-END-1-2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:06:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 01:44:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

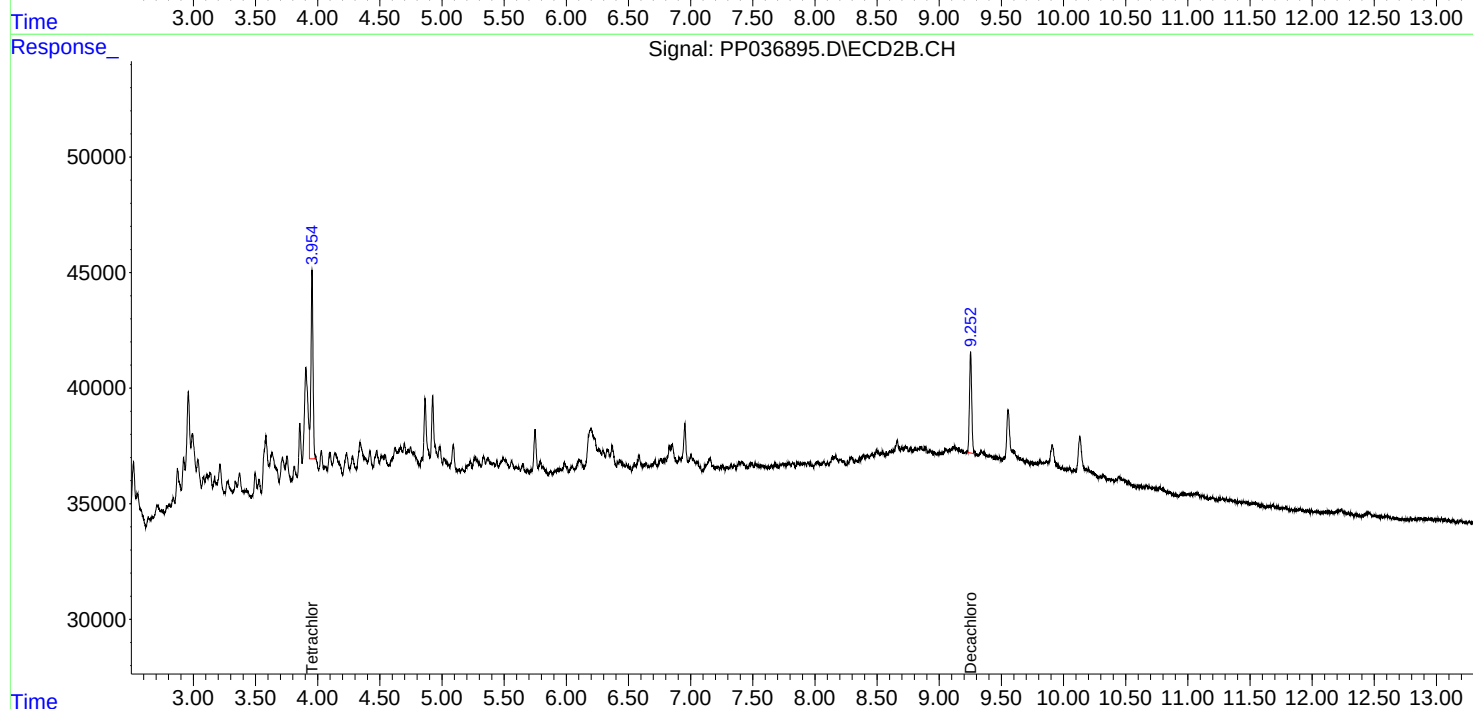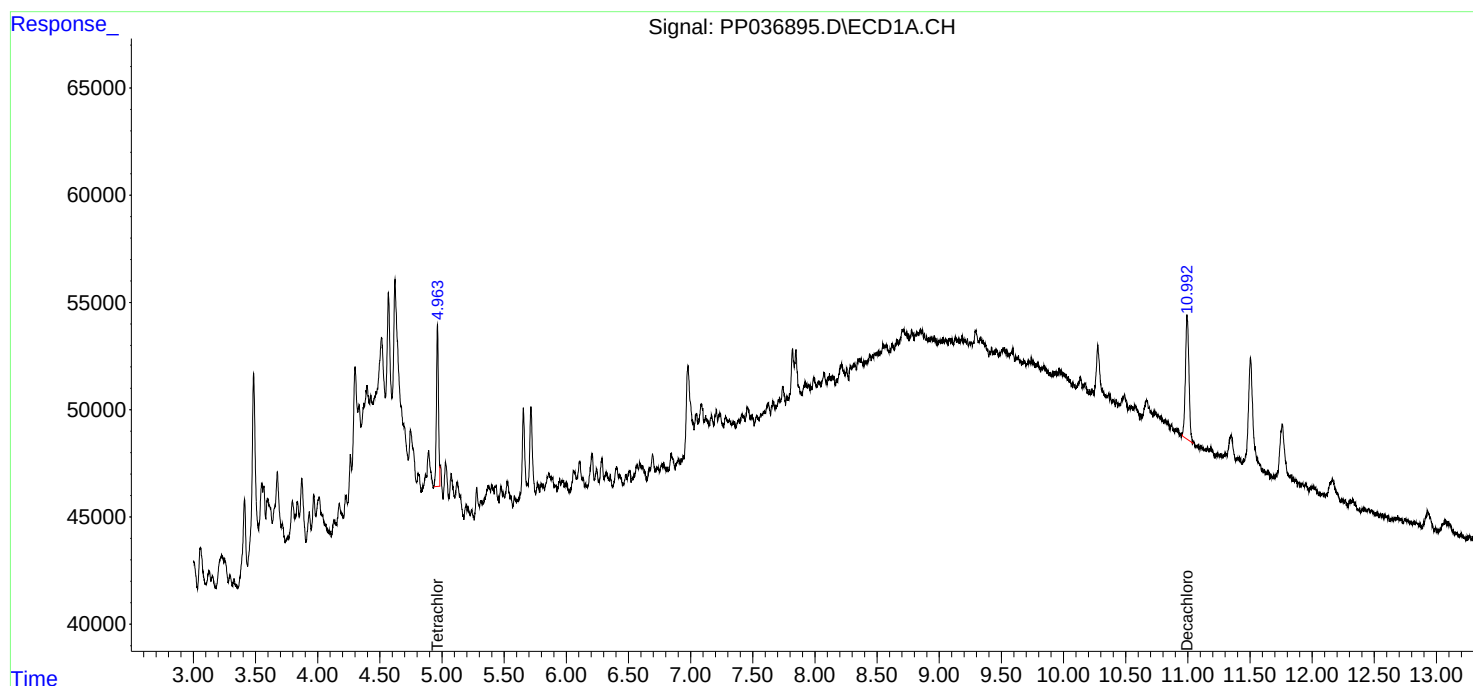

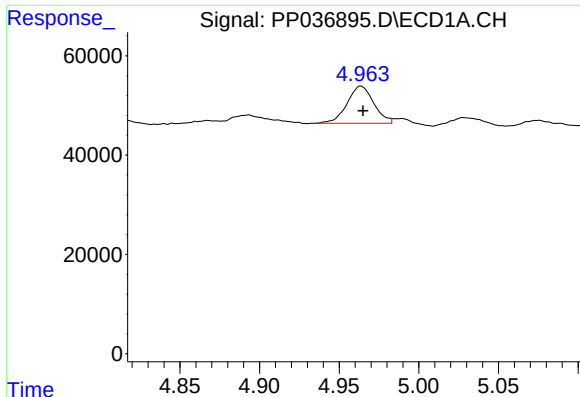


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 87720
Conc: 1.98 ng/ml m

Instrument :
ECD_P
ClientSampleId :
BC123047LOK-END-1-2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:06:00 PM

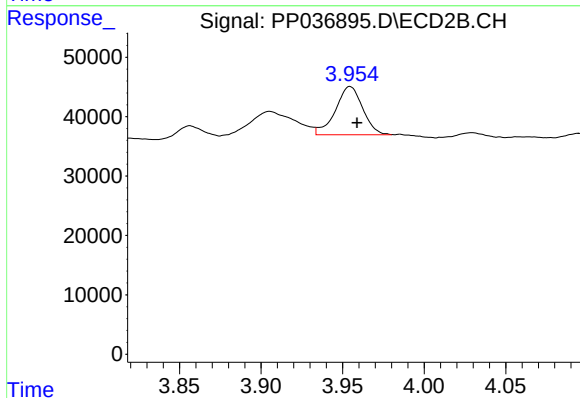


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.005 min
Response: 94611
Conc: 3.05 ng/ml m

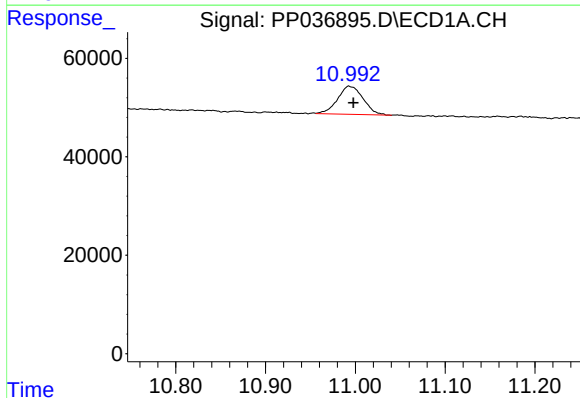

#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 113205
Conc: 2.64 ng/ml

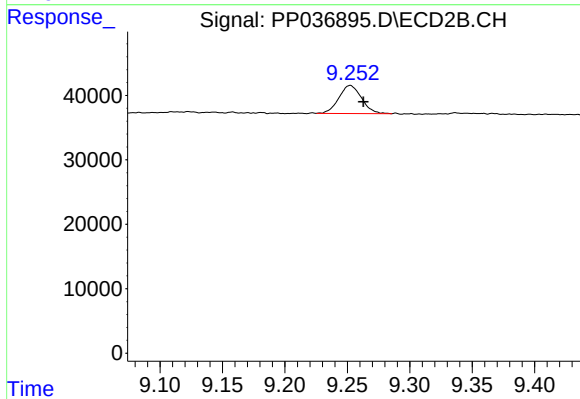

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.010 min
Response: 55046
Conc: 1.72 ng/ml