

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 17:23
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 18:51:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.593	27656380	51004365	19.455	19.919
2) SA Decachlor...	10.090	8.566	26469174	23969397	21.579	21.264
Target Compounds						
26) L6 AR-1254-1	6.381	5.466	2117718	3538876	31.416	24.105
27) L6 AR-1254-2	6.597	5.612	2353060	3303180	25.089	26.477
28) L6 AR-1254-3	6.967	6.014	2915081	4704950	28.729	26.130
29) L6 AR-1254-4	7.254	6.243	1849464	2805959	24.651	25.936
30) L6 AR-1254-5	7.674	6.659	1966944	3753858	23.314	25.864



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 17:23
Operator : YP\AJ
Sample : N3214-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 18:51:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

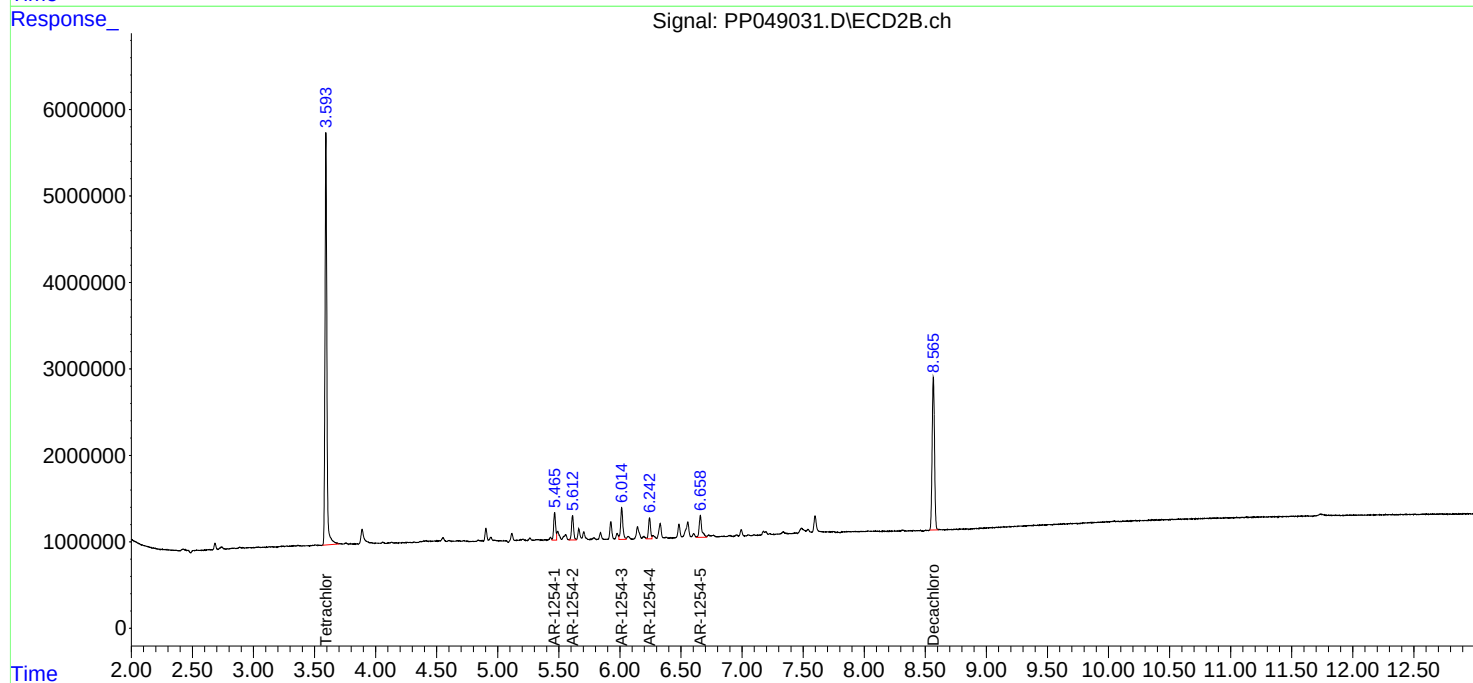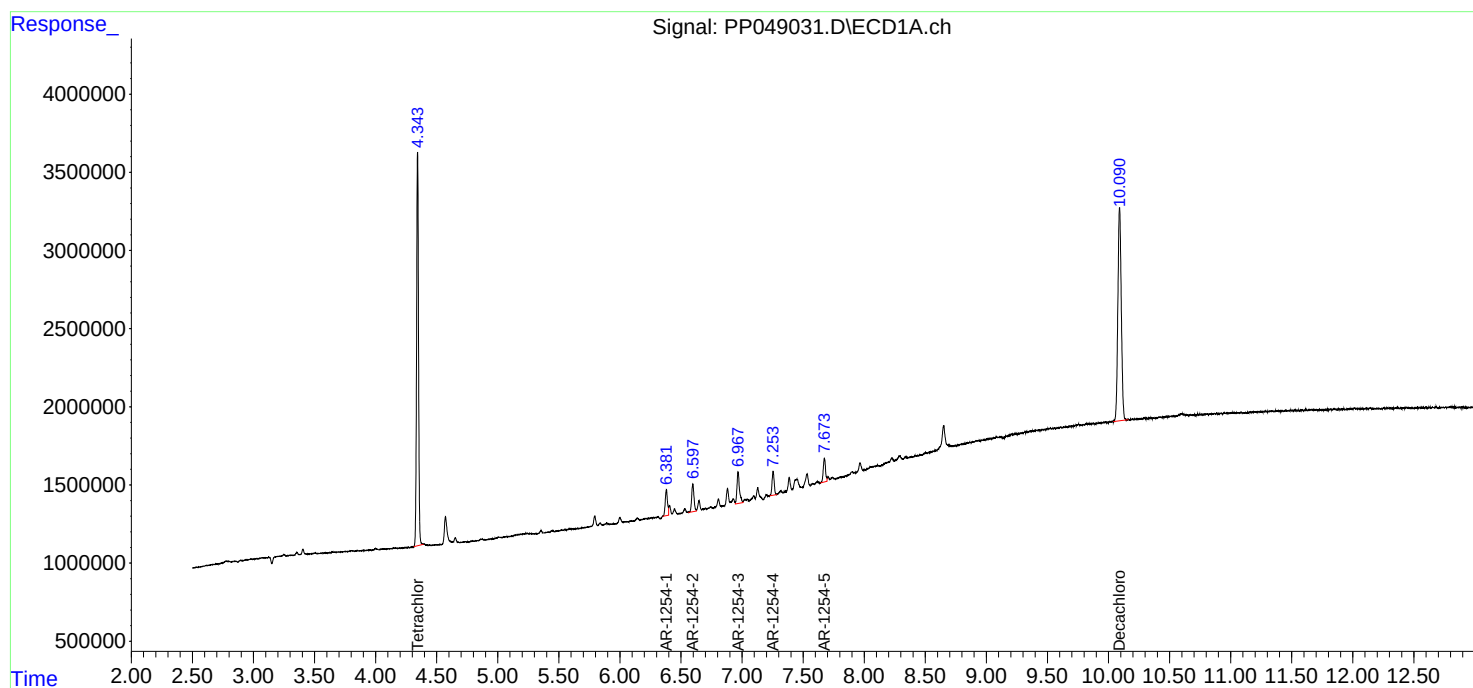


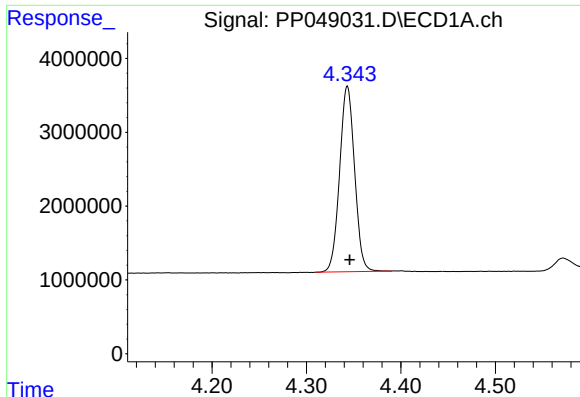

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.003 min
Response: 27656380
Conc: 19.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

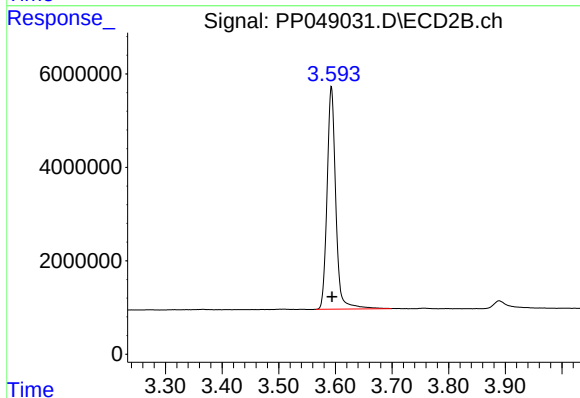


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: -0.001 min
Response: 51004365
Conc: 19.92 ng/ml

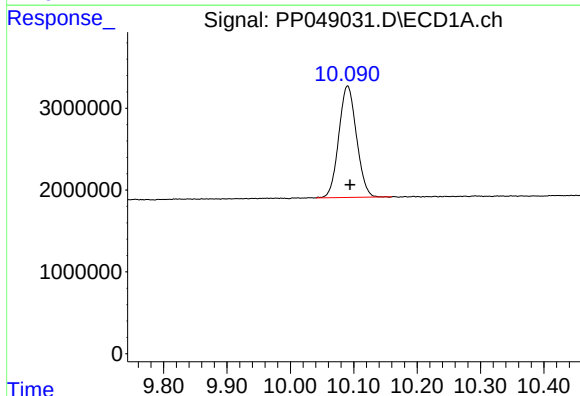


#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: -0.004 min
Response: 26469174
Conc: 21.58 ng/ml

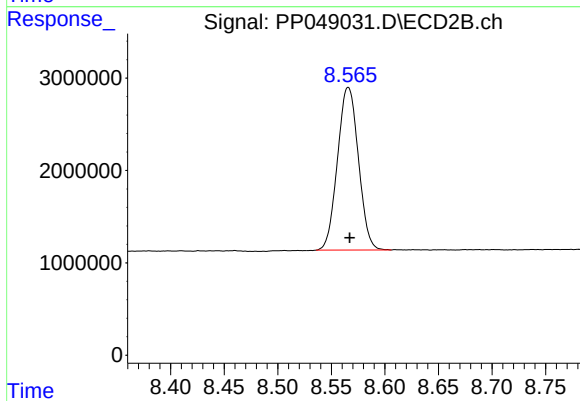

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.002 min
Response: 23969397
Conc: 21.26 ng/ml

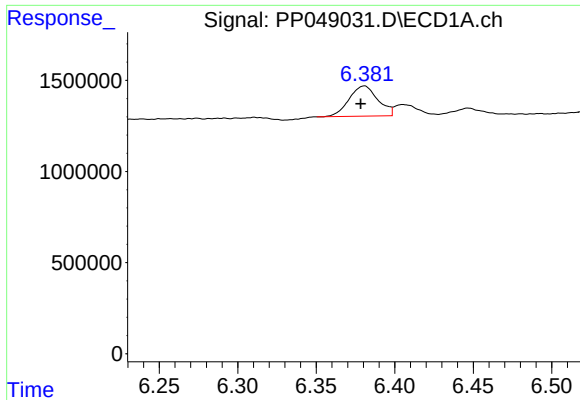

#26 AR-1254-1


R.T.: 6.381 min
Delta R.T.: 0.002 min
Response: 2117718
Conc: 31.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

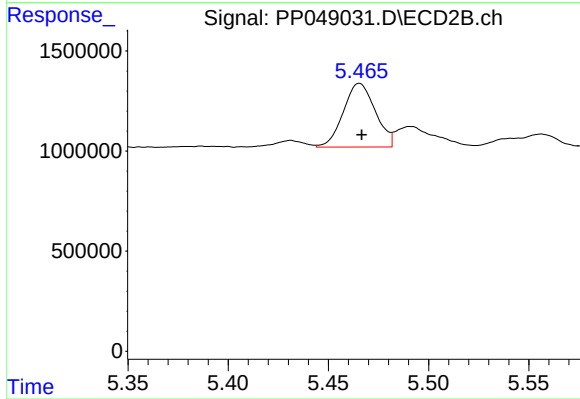


#26 AR-1254-1

R.T.: 5.466 min
Delta R.T.: -0.001 min
Response: 3538876
Conc: 24.11 ng/ml

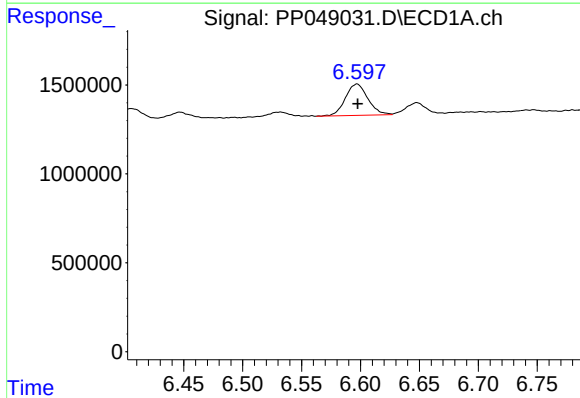


#27 AR-1254-2

R.T.: 6.597 min
Delta R.T.: 0.000 min
Response: 2353060
Conc: 25.09 ng/ml

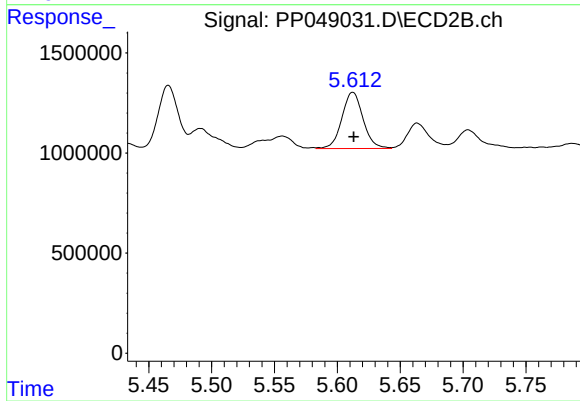

#27 AR-1254-2


R.T.: 5.612 min
Delta R.T.: 0.000 min
Response: 3303180
Conc: 26.48 ng/ml

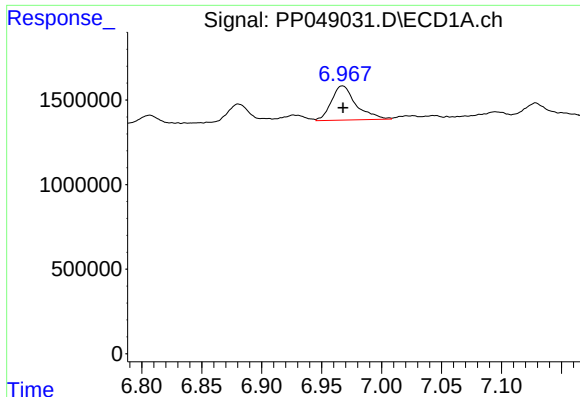

#28 AR-1254-3


R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 2915081
Conc: 28.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

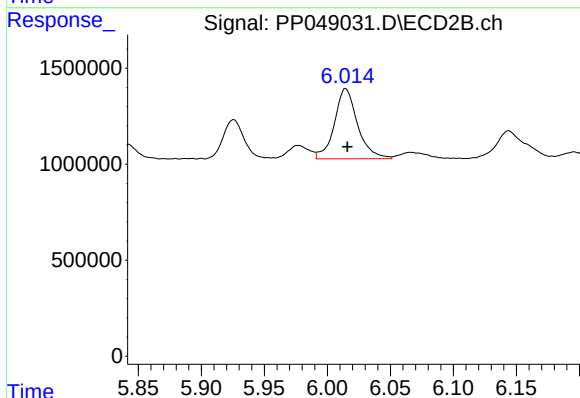


#28 AR-1254-3

R.T.: 6.014 min
Delta R.T.: -0.002 min
Response: 4704950
Conc: 26.13 ng/ml

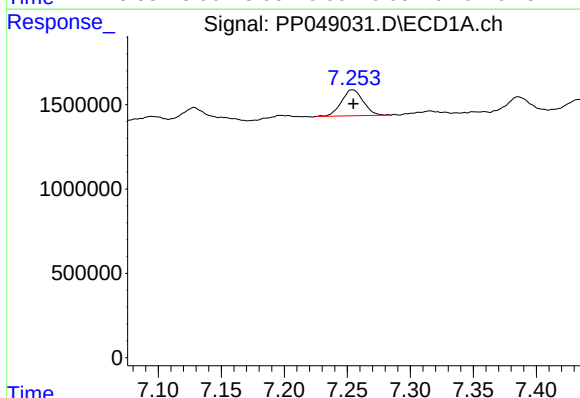


#29 AR-1254-4

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 1849464
Conc: 24.65 ng/ml

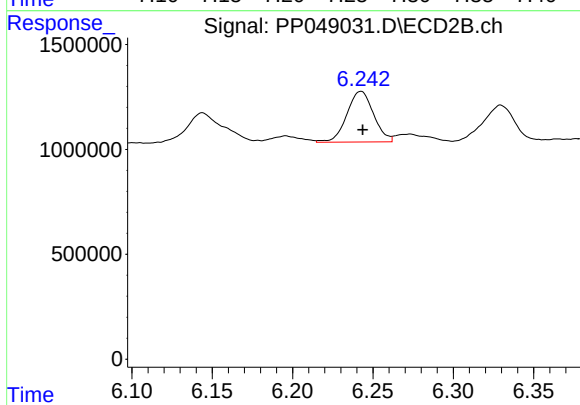

#29 AR-1254-4


R.T.: 6.243 min
Delta R.T.: 0.000 min
Response: 2805959
Conc: 25.94 ng/ml

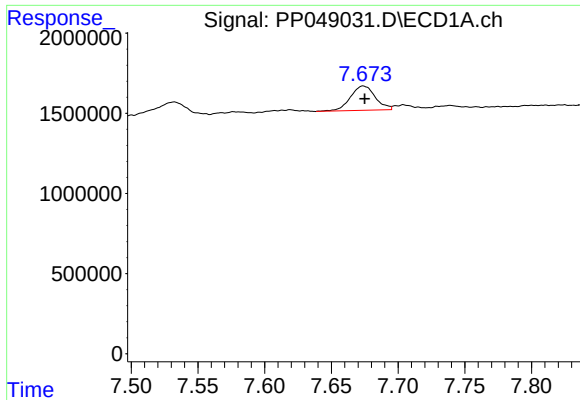

#30 AR-1254-5

R.T.: 7.674 min
Delta R.T.: -0.001 min
Response: 1966944
Conc: 23.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

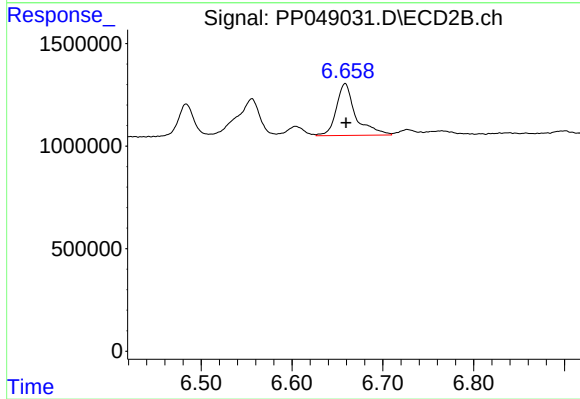

#30 AR-1254-5

R.T.: 6.659 min
Delta R.T.: 0.000 min
Response: 3753858
Conc: 25.86 ng/ml