

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 17:40
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 18:51:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.593	27474977	49771144	19.327	19.437
2) SA Decachlor...	10.093	8.566	26463576	23636809	21.575	20.969
Target Compounds						
36) L8 AR-1262-1	7.745	6.696	2418382	3750625	25.801	28.195
37) L8 AR-1262-2	8.292	6.955	4444360	3111124	25.971	27.454
38) L8 AR-1262-3	8.599	7.479	1821191	3188953	24.337	39.139 #
39) L8 AR-1262-4	8.690	7.542	1129780	4149097	24.070	28.464
40) L8 AR-1262-5	9.351	8.034	1784241	1536803	29.511	25.479



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 17:40
Operator : YP\AJ
Sample : N3214-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 18:51:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

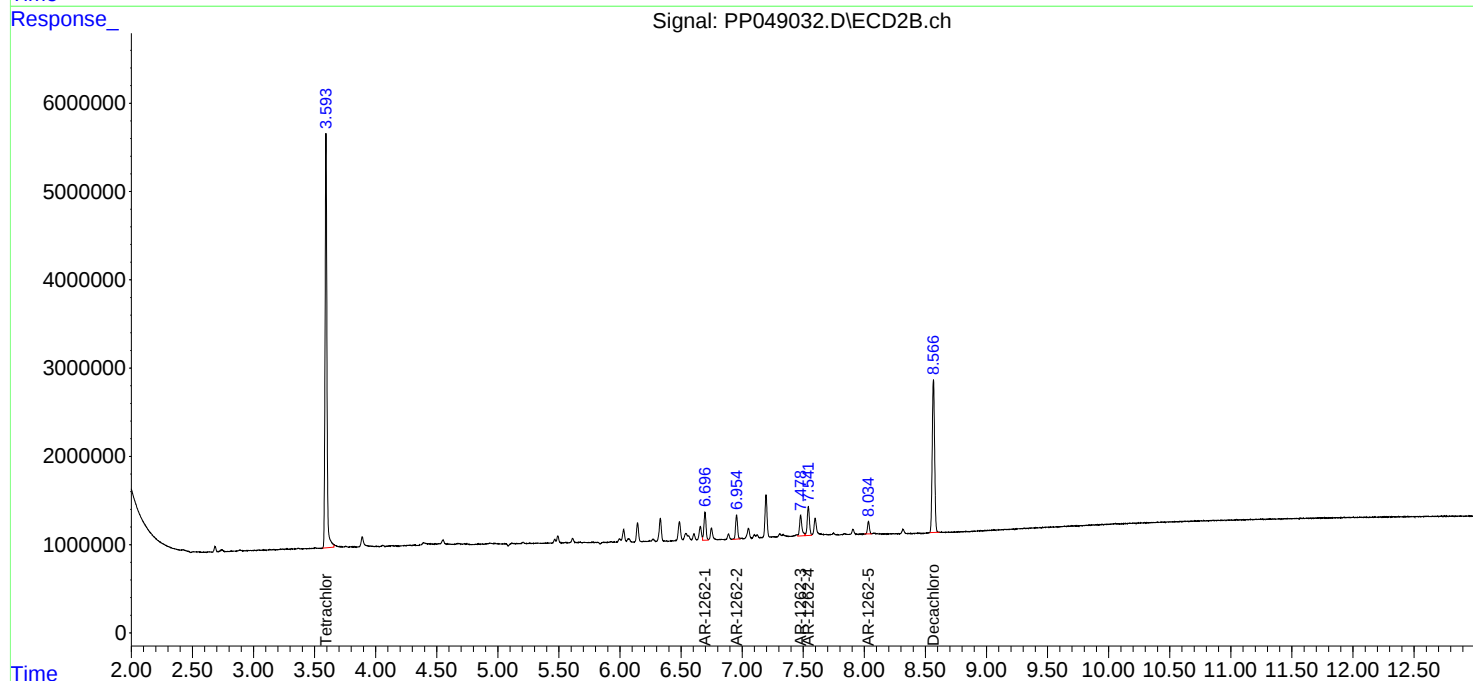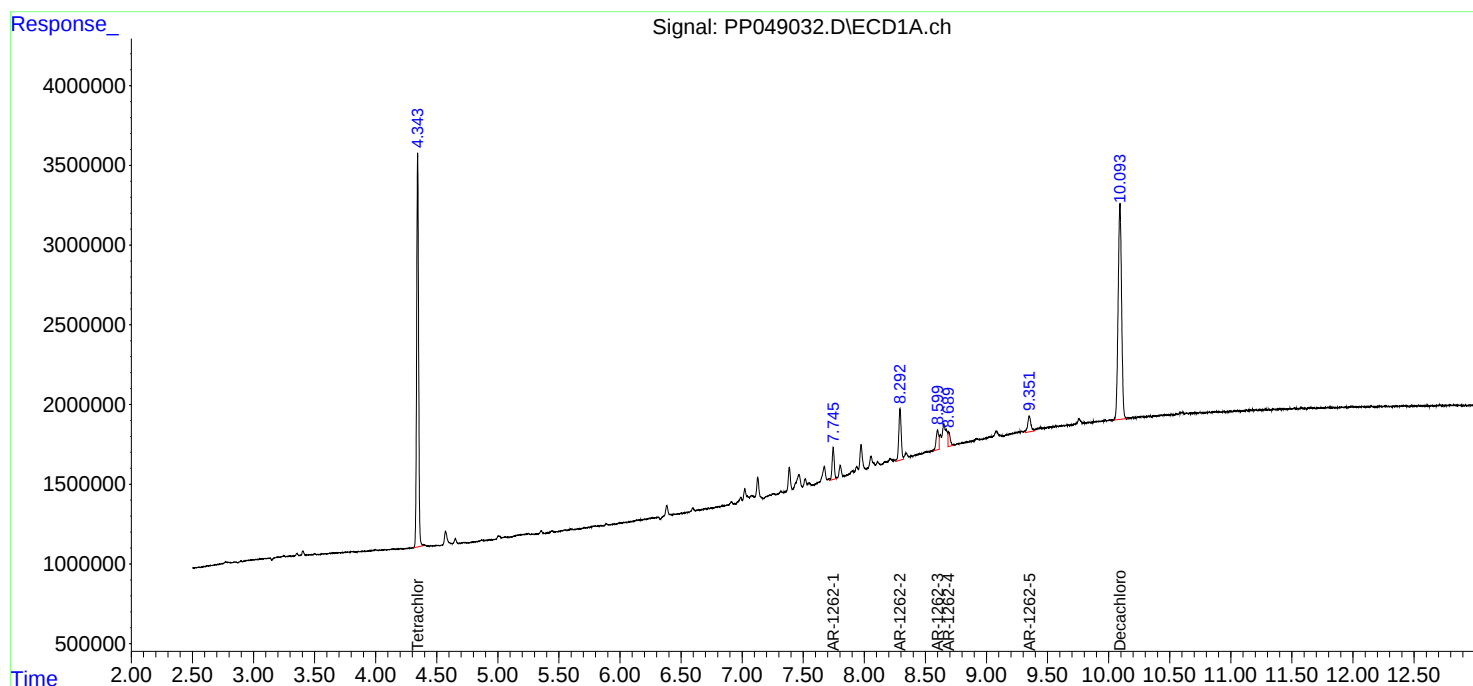


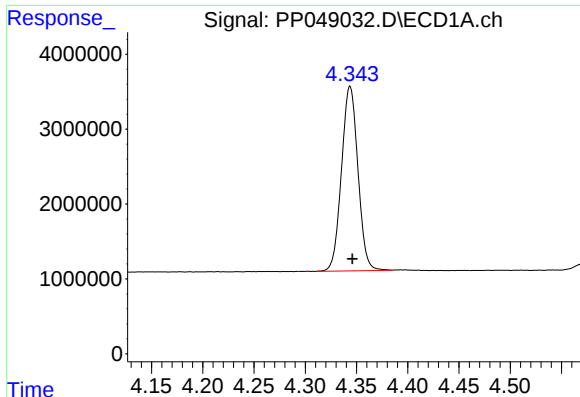

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 27474977
Conc: 19.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

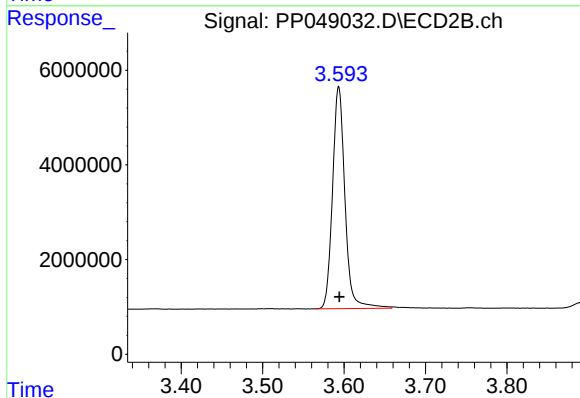


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 49771144
Conc: 19.44 ng/ml

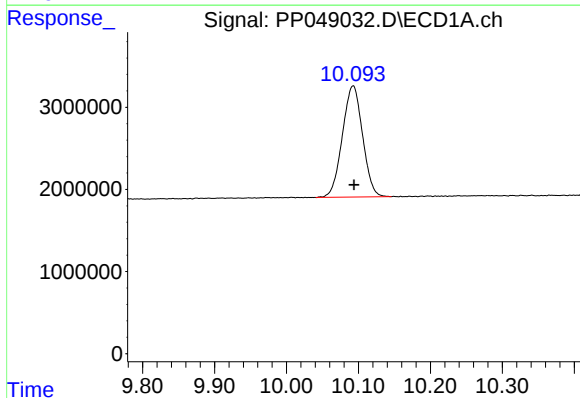


#2 Decachlorobiphenyl

R.T.: 10.093 min
Delta R.T.: -0.002 min
Response: 26463576
Conc: 21.57 ng/ml

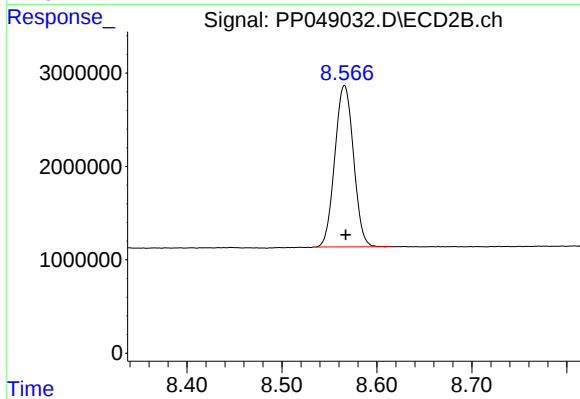

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.001 min
Response: 23636809
Conc: 20.97 ng/ml

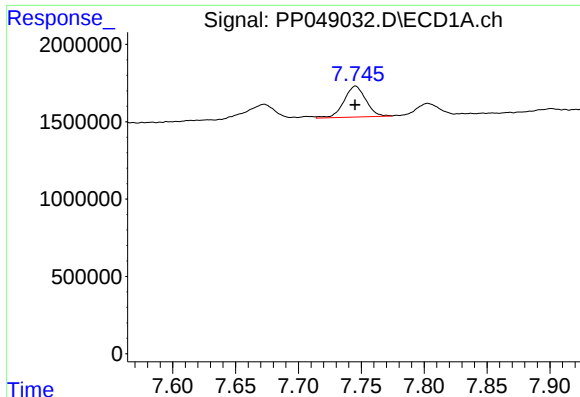

#36 AR-1262-1


R.T.: 7.745 min
Delta R.T.: 0.000 min
Response: 2418382
Conc: 25.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

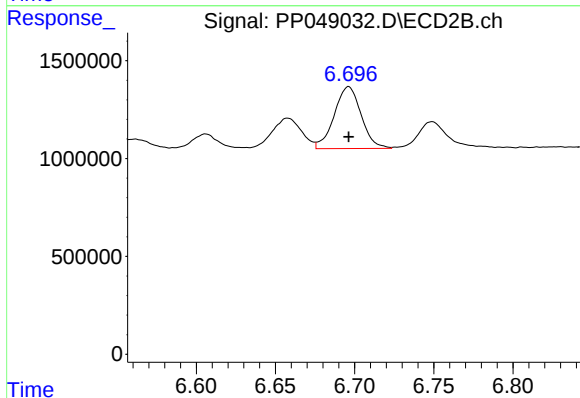


#36 AR-1262-1

R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 3750625
Conc: 28.20 ng/ml

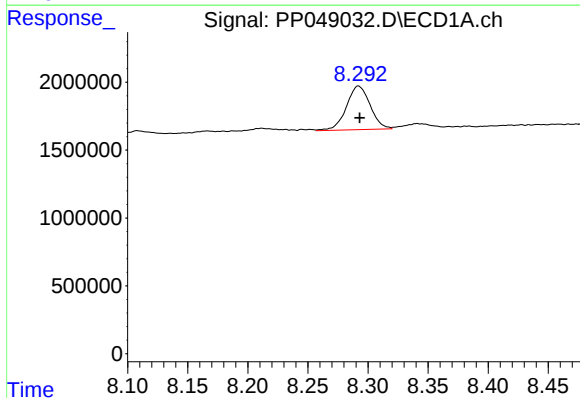


#37 AR-1262-2

R.T.: 8.292 min
Delta R.T.: -0.001 min
Response: 4444360
Conc: 25.97 ng/ml

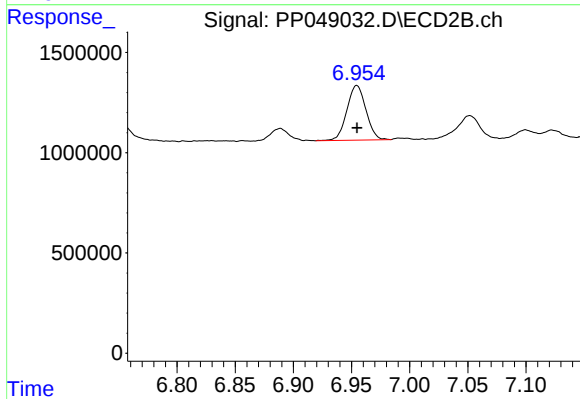

#37 AR-1262-2


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 3111124
Conc: 27.45 ng/ml

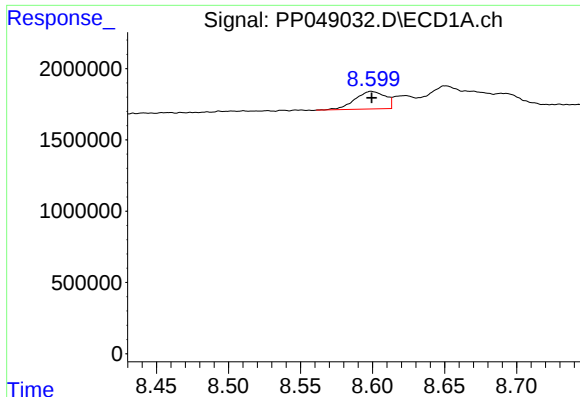

#38 AR-1262-3


R.T.: 8.599 min
Delta R.T.: 0.000 min
Response: 1821191
Conc: 24.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

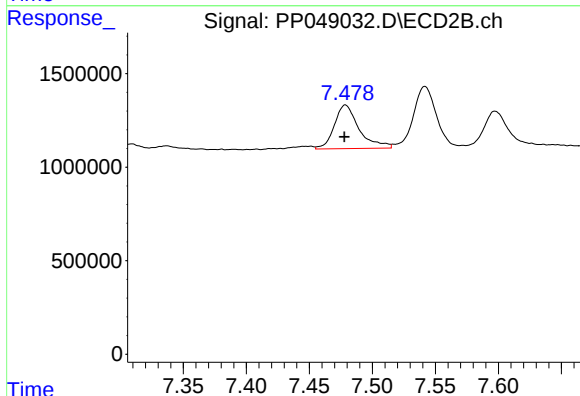


#38 AR-1262-3

R.T.: 7.479 min
Delta R.T.: 0.000 min
Response: 3188953
Conc: 39.14 ng/ml

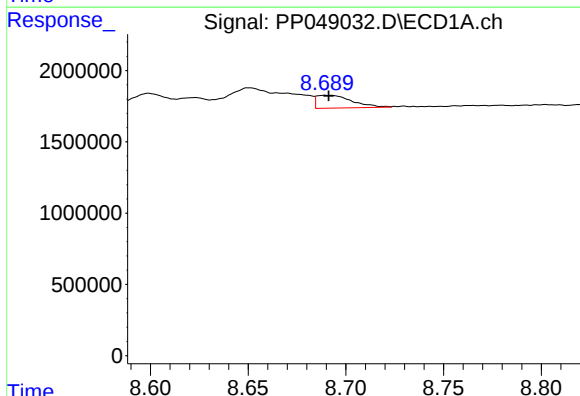


#39 AR-1262-4

R.T.: 8.690 min
Delta R.T.: -0.002 min
Response: 1129780
Conc: 24.07 ng/ml

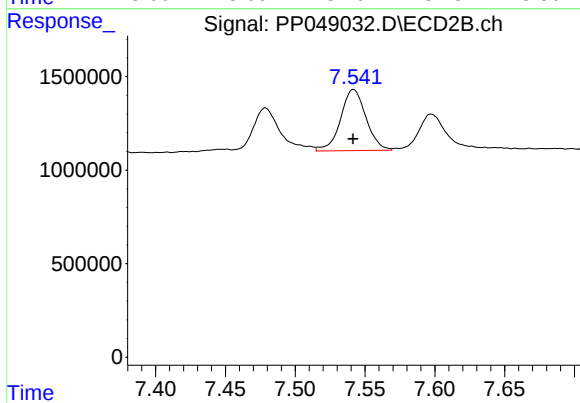

#39 AR-1262-4


R.T.: 7.542 min
Delta R.T.: 0.000 min
Response: 4149097
Conc: 28.46 ng/ml

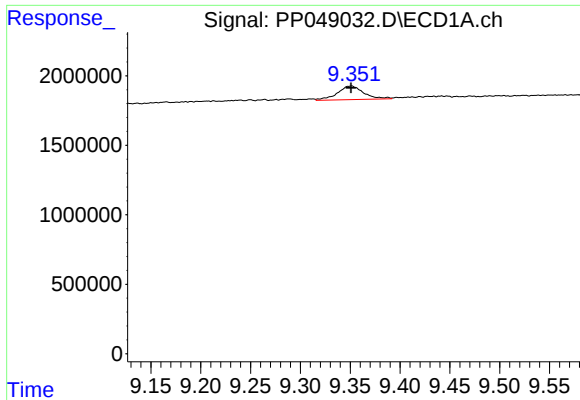

#40 AR-1262-5

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 1784241
Conc: 29.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

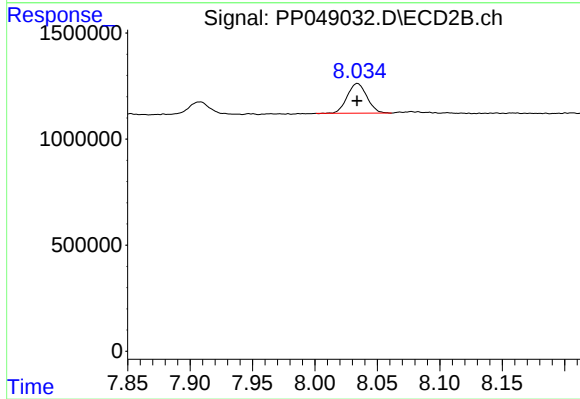

#40 AR-1262-5

R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 1536803
Conc: 25.48 ng/ml